

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
 Data File : PS003954.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2019 04:57
 Operator : EI\SJ
 Sample : K2182-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 S8B(2-10)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 06:52:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.275	10.779	320.0E6	290.7E6	733.475	592.448
Target Compounds							
1) T	Dalapon	2.799	2.296	50210299	122.5E6	67.348	167.875 #
2) T	3,5-DICHL...	0.000	8.945	0	5498739	N.D.	8.621
3) T	4-Nitroph...	0.000	9.950	0	12490255	N.D.	55.015
5) T	DICAMBA	0.000	11.020	0	5592572	N.D.	3.007
6) T	MCPD	0.000	11.263	0	436807	N.D.	<MDL
7) T	MCPA	12.206	0.000	112.6E6	0	53.369	N.D. #
9) T	2,4-D	0.000	12.638	0	2748933	N.D.	5.168
10) T	Pentachlo...	0.000	13.184	0	1056213	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.791	0	2672464	N.D.	1.009
12) T	2,4,5-T	0.000	14.371	0	326918	N.D.	<MDL
13) T	2,4-DB	0.000	15.007	0	1917639	N.D.	6.458
15) T	Picloram	16.768	16.639	11870007	4122043	3.494	1.300 #
16) T	DCPA	0.000	16.639	0	4122043	N.D.	1.220



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
Data File : PS003954.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2019 04:57
Operator : EI\SJ
Sample : K2182-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
S8B(2-10)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 06:52:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

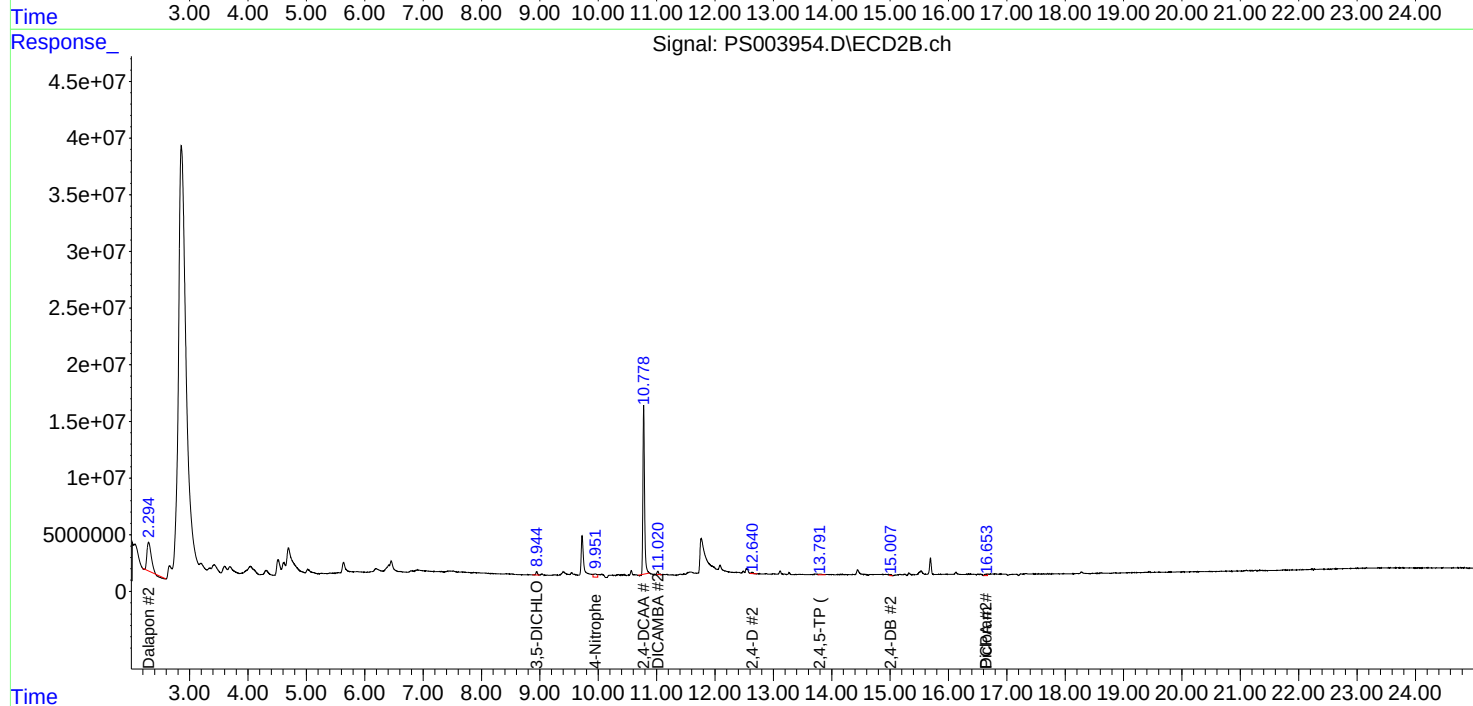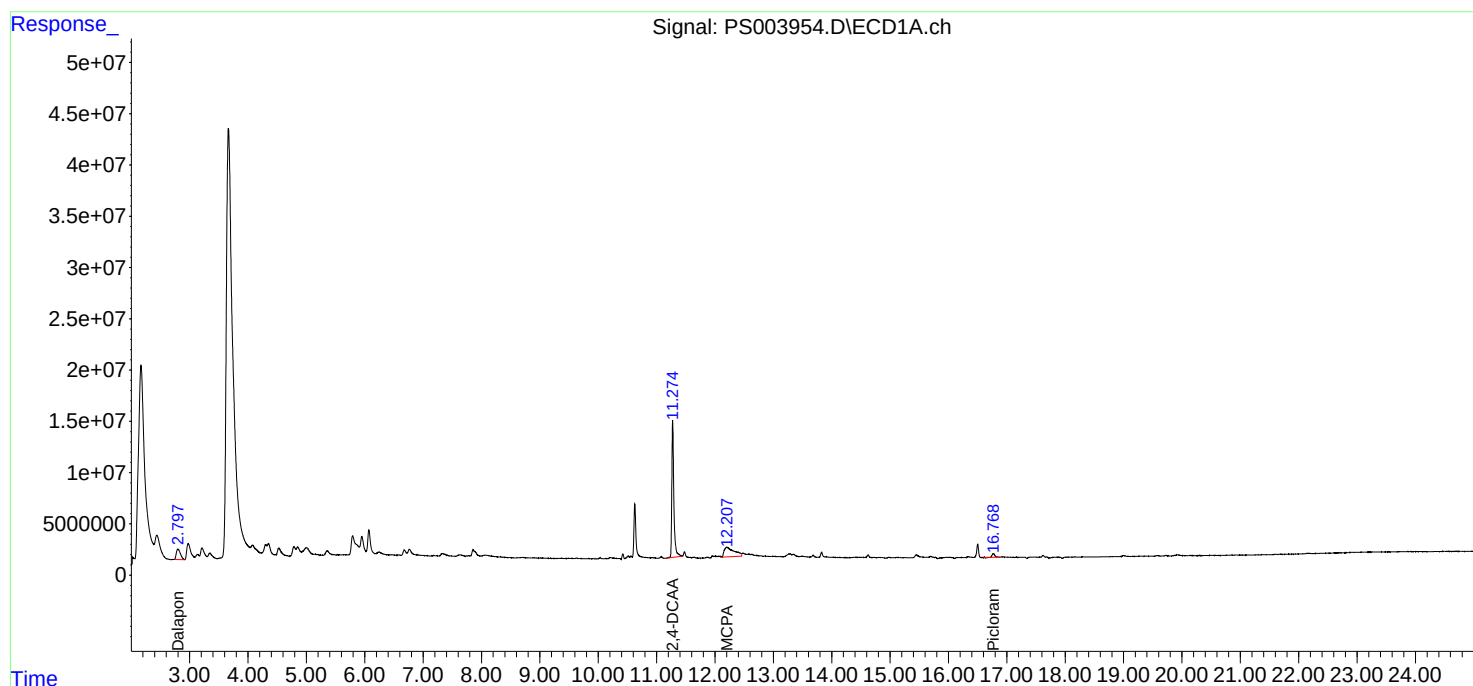


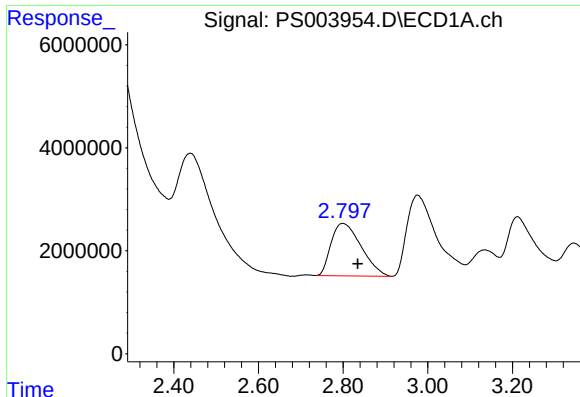

#1 Dalapon


R.T.: 2.799 min
Delta R.T.: -0.036 min
Response: 50210299
Conc: 67.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
S8B(2-10)COMP

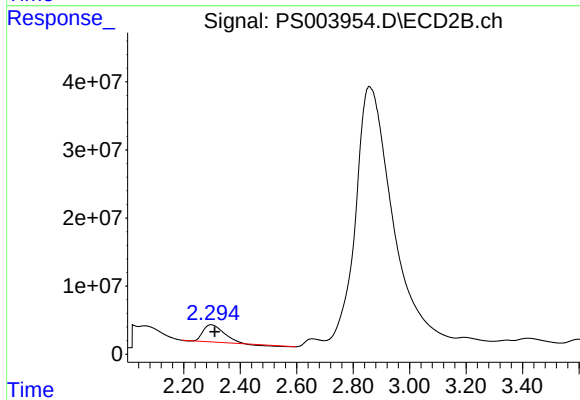


#1 Dalapon

R.T.: 2.296 min
Delta R.T.: -0.014 min
Response: 122486175
Conc: 167.87 ng/ml

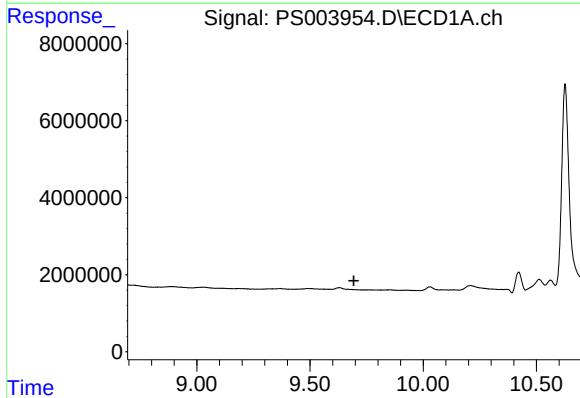


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

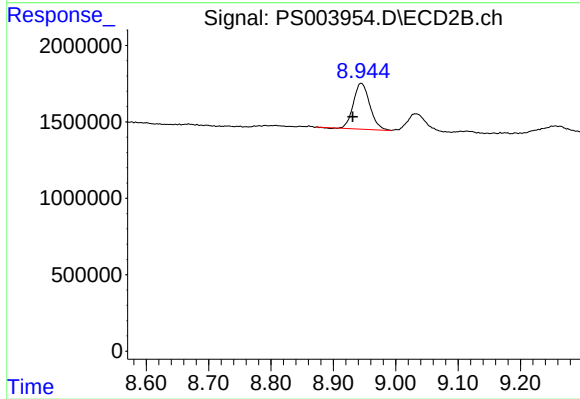

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.945 min
Delta R.T.: 0.014 min
Response: 5498739
Conc: 8.62 ng/ml

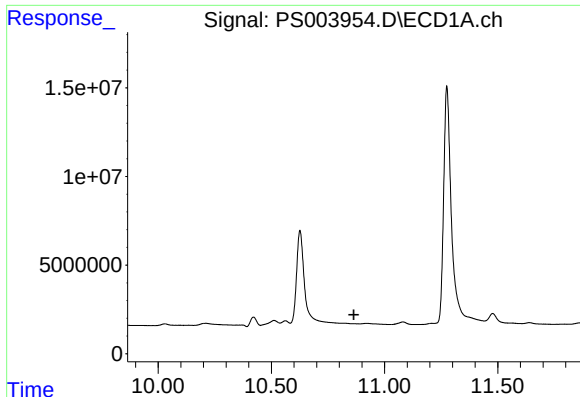

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S8B(2-10)COMP

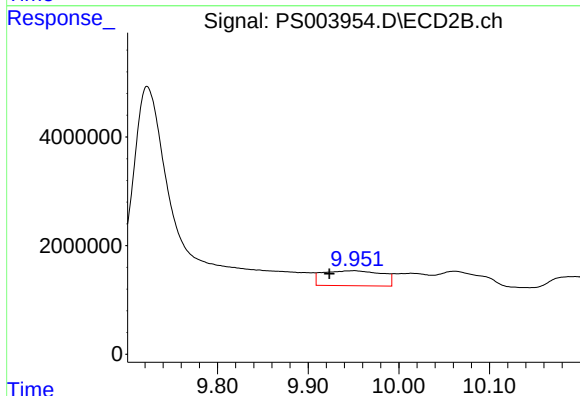


#3 4-Nitrophenol

R.T.: 9.950 min
Delta R.T.: 0.027 min
Response: 12490255
Conc: 55.01 ng/ml

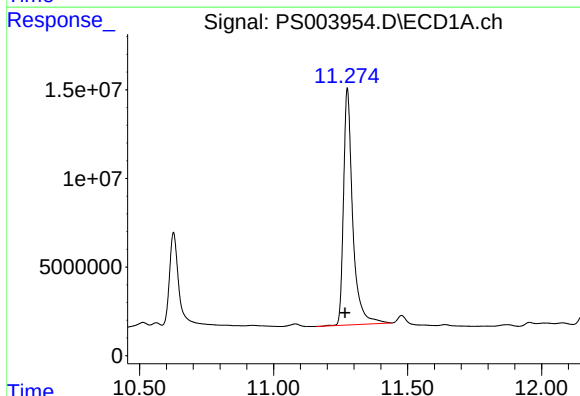


#4 2,4-DCAA

R.T.: 11.275 min
Delta R.T.: 0.008 min
Response: 319950985
Conc: 733.48 ng/ml

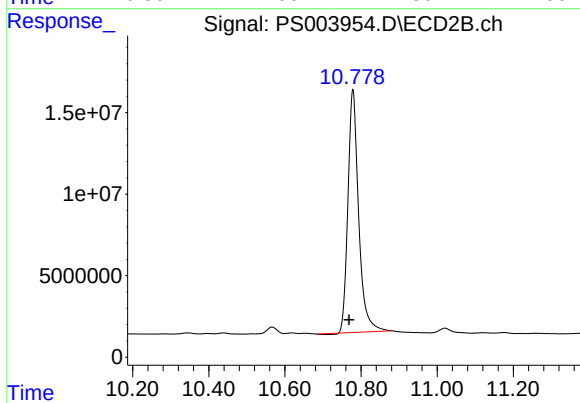

#4 2,4-DCAA


R.T.: 10.779 min
Delta R.T.: 0.010 min
Response: 290689763
Conc: 592.45 ng/ml

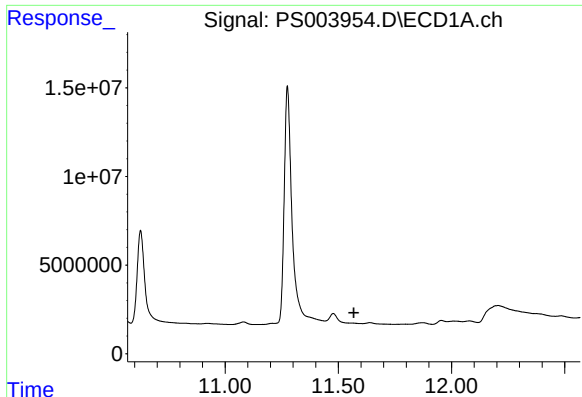

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S8B(2-10)COMP

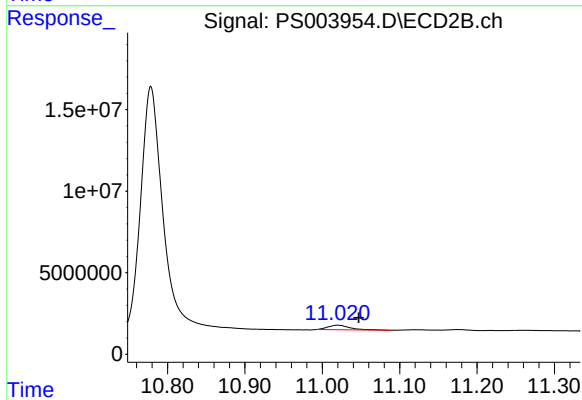


#5 DICAMBA

R.T.: 11.020 min
Delta R.T.: -0.027 min
Response: 5592572
Conc: 3.01 ng/ml

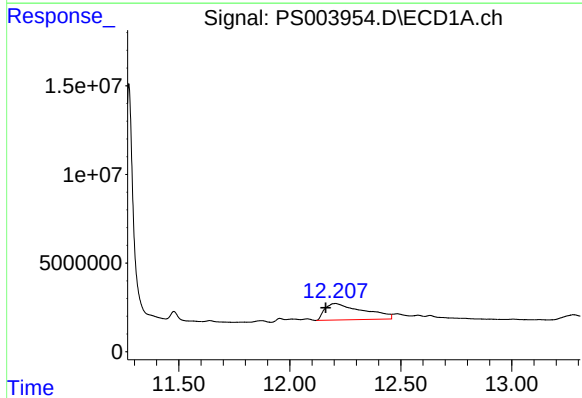


#7 MCPA

R.T.: 12.206 min
Delta R.T.: 0.044 min
Response: 112597823
Conc: 53.37 ug/ml

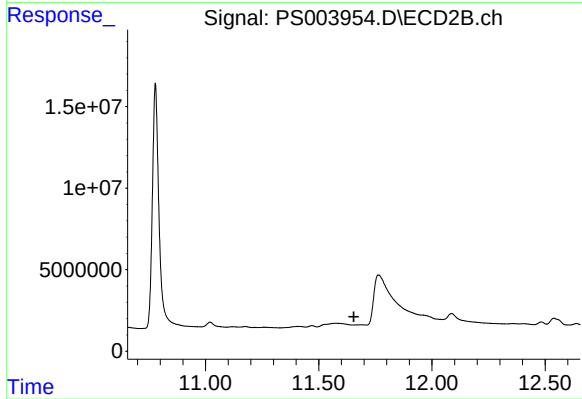

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.655 min
Response: 0
Conc: N.D.

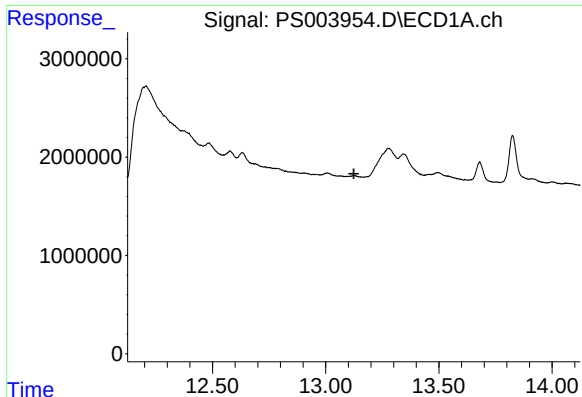

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S8B(2-10)COMP

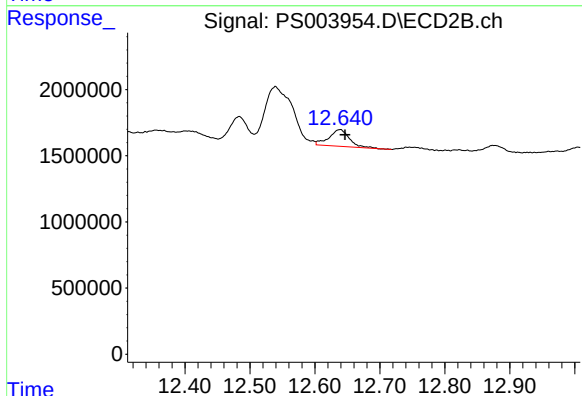


#9 2,4-D

R.T.: 12.638 min
Delta R.T.: -0.008 min
Response: 2748933
Conc: 5.17 ng/ml

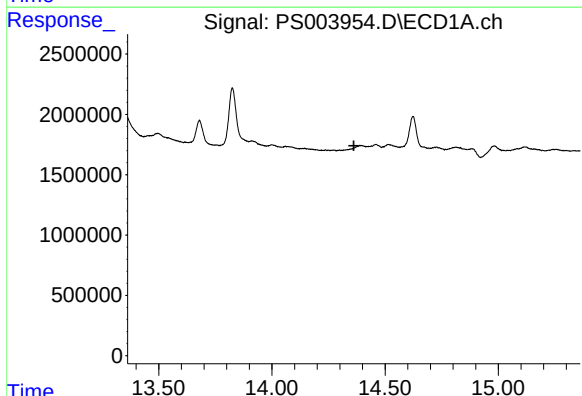


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

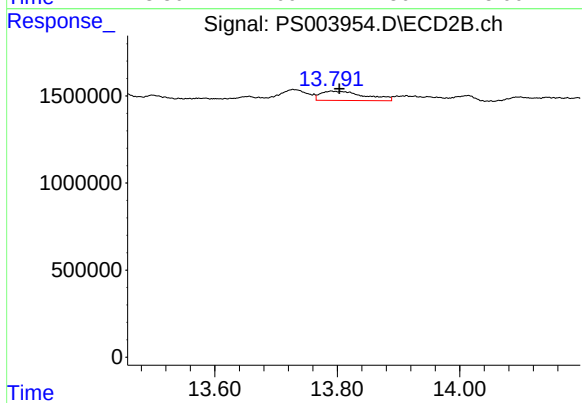

#11 2,4,5-TP (SILVEX)


R.T.: 13.791 min
Delta R.T.: -0.013 min
Response: 2672464
Conc: 1.01 ng/ml

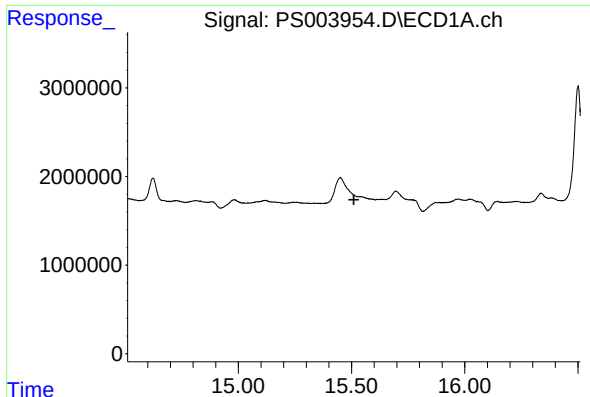

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S8B(2-10)COMP

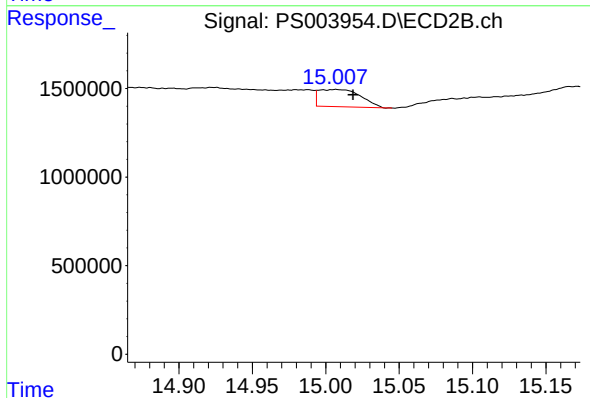


#13 2,4-DB

R.T.: 15.007 min
Delta R.T.: -0.011 min
Response: 1917639
Conc: 6.46 ng/ml

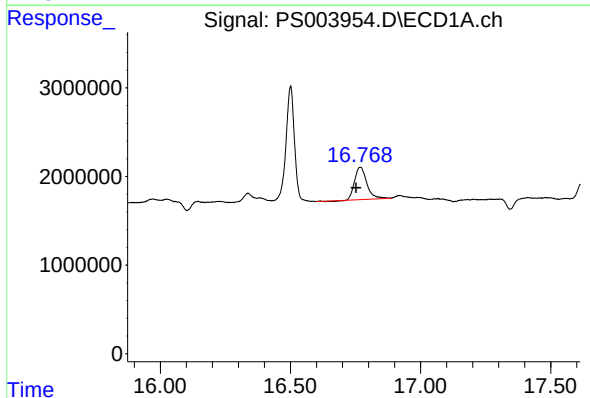


#15 Picloram

R.T.: 16.768 min
Delta R.T.: 0.017 min
Response: 11870007
Conc: 3.49 ng/ml

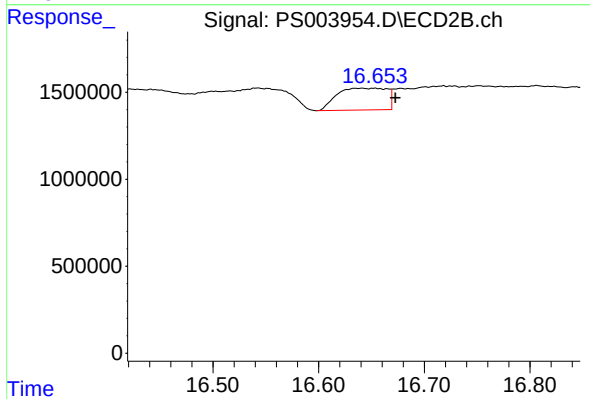

#15 Picloram


R.T.: 16.639 min
Delta R.T.: -0.034 min
Response: 4122043
Conc: 1.30 ng/ml

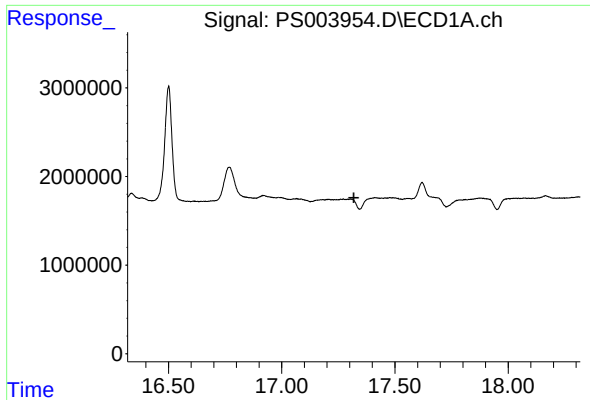

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S8B(2-10)COMP

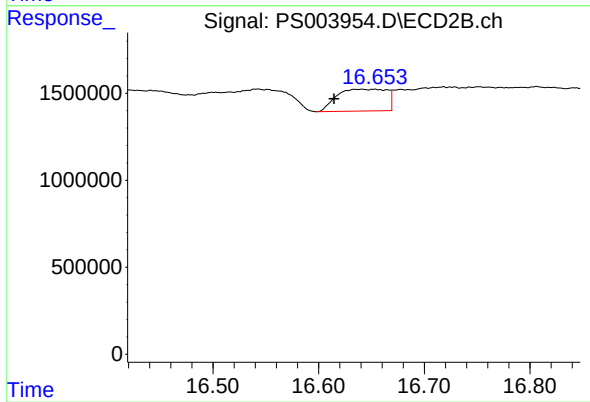

#16 DCPA

R.T.: 16.639 min
Delta R.T.: 0.024 min
Response: 4122043
Conc: 1.22 ng/ml