

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
 Data File : PS003956.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2019 05:59
 Operator : EI\SJ
 Sample : K2186-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 S7C(12-20)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 06:53:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.280	10.783	289.6E6	264.1E6	663.860	538.326
Target Compounds							
1) T	Dalapon	2.805	2.301	44977380	130.0E6	60.329	178.190 #
2) T	3,5-DICHL...	0.000	8.949	0	3950370	N.D.	6.193
3) T	4-Nitroph...	0.000	9.955	0	12119305	N.D.	53.381
5) T	DICAMBA	0.000	11.024	0	5323658	N.D.	2.863
6) T	MCPD	0.000	11.263	0	377045	N.D.	<MDL
7) T	MCPA	12.225	11.689	83573985	447014	39.613	<MDL #
9) T	2,4-D	0.000	12.642	0	2442803	N.D.	4.593
10) T	Pentachlo...	0.000	13.191	0	1001960	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.793	0	1088515	N.D.	<MDL
12) T	2,4,5-T	0.000	14.381	0	274328	N.D.	<MDL
14) T	DINOSEB	0.000	15.508	0	4834944	N.D.	2.520
15) T	Picloram	16.777	16.638	5762054	2384749	1.696	<MDL #
16) T	DCPA	0.000	16.638	0	2384749	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
Data File : PS003956.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2019 05:59
Operator : EI\SJ
Sample : K2186-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
S7C(12-20)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 06:53:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

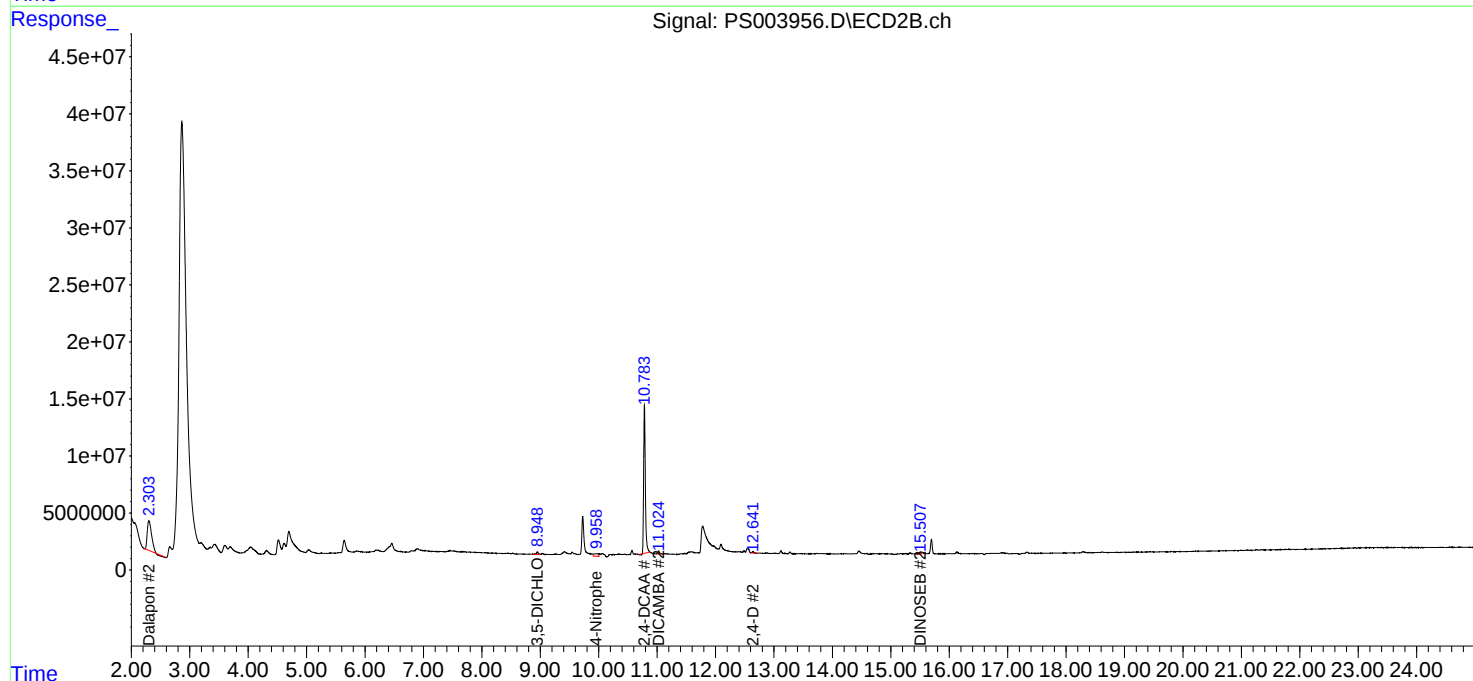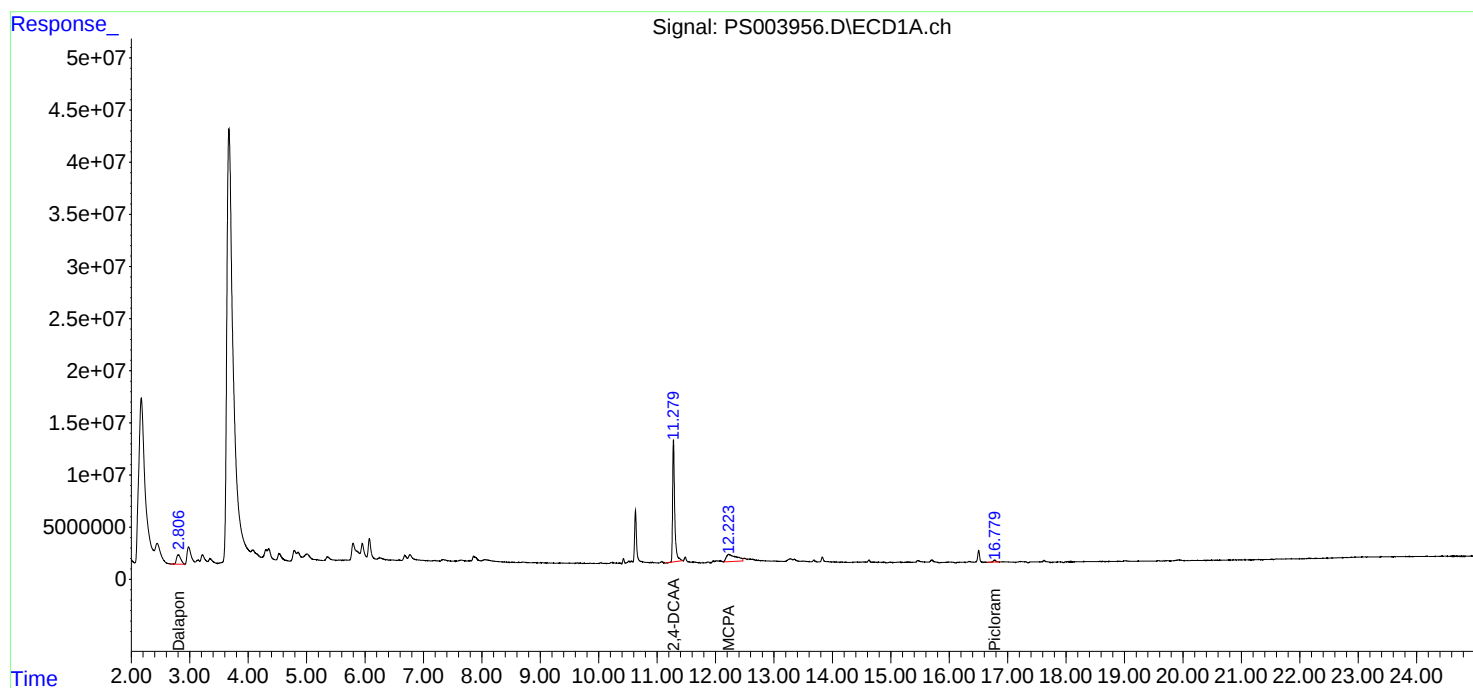


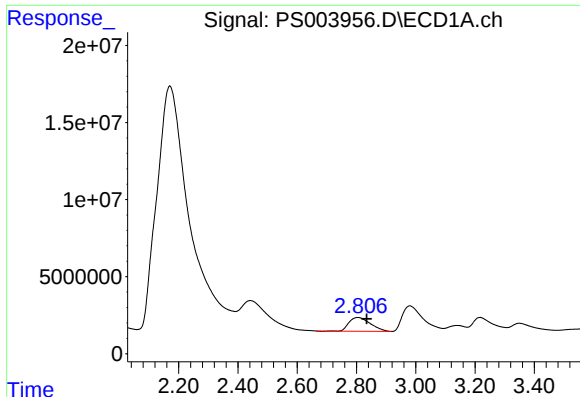

#1 Dalapon


R.T.: 2.805 min
Delta R.T.: -0.030 min
Response: 44977380
Conc: 60.33 ng/ml

Instrument :
ECD_S
ClientSampleId :
S7C(12-20)COMP

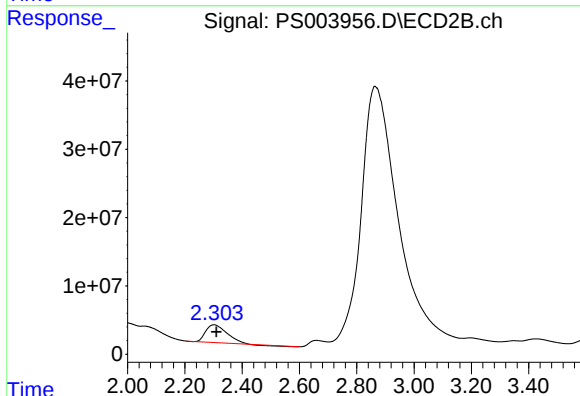


#1 Dalapon

R.T.: 2.301 min
Delta R.T.: -0.009 min
Response: 130012085
Conc: 178.19 ng/ml

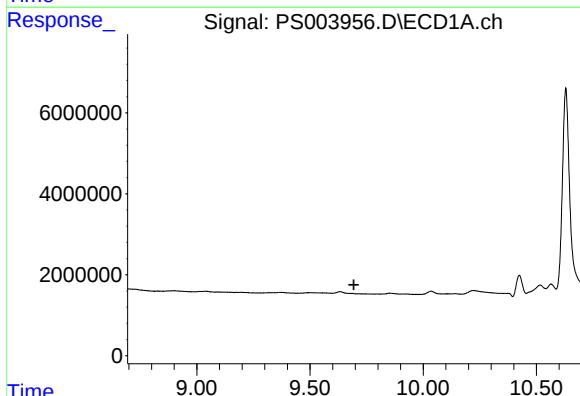


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

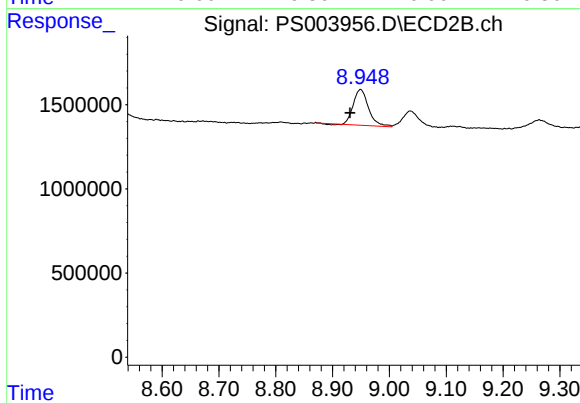

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.949 min
Delta R.T.: 0.018 min
Response: 3950370
Conc: 6.19 ng/ml

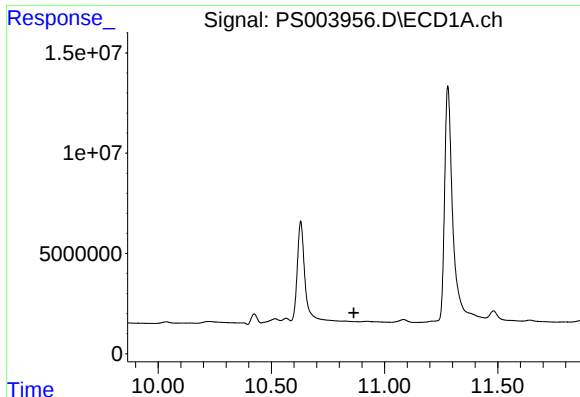

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S7C(12-20)COMP

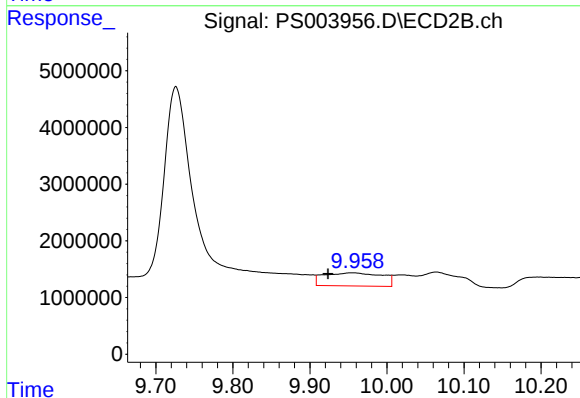


#3 4-Nitrophenol

R.T.: 9.955 min
Delta R.T.: 0.031 min
Response: 12119305
Conc: 53.38 ng/ml

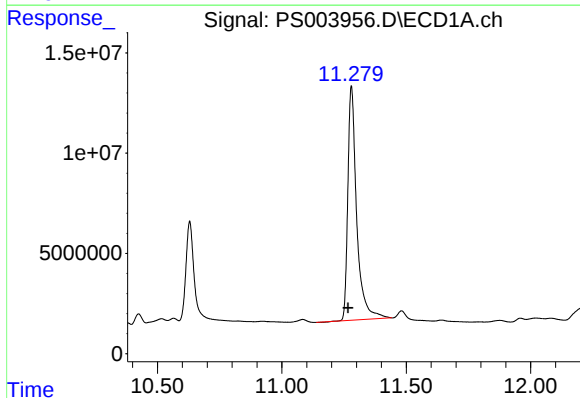


#4 2,4-DCAA

R.T.: 11.280 min
Delta R.T.: 0.013 min
Response: 289583810
Conc: 663.86 ng/ml

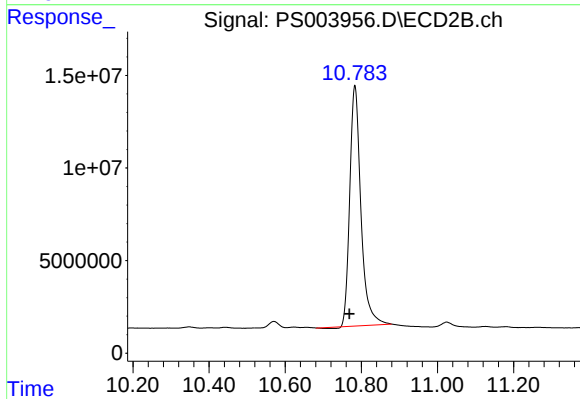

#4 2,4-DCAA


R.T.: 10.783 min
Delta R.T.: 0.014 min
Response: 264133956
Conc: 538.33 ng/ml

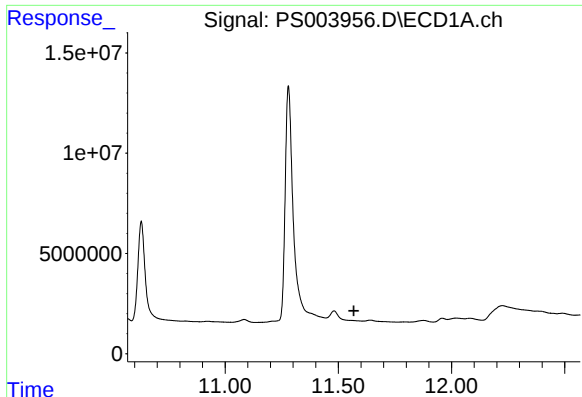

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S7C(12-20)COMP

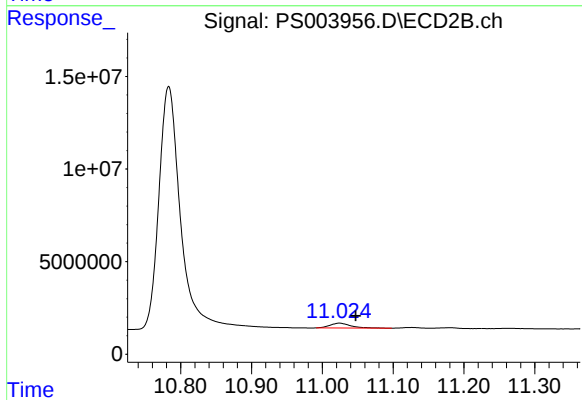


#5 DICAMBA

R.T.: 11.024 min
Delta R.T.: -0.023 min
Response: 5323658
Conc: 2.86 ng/ml

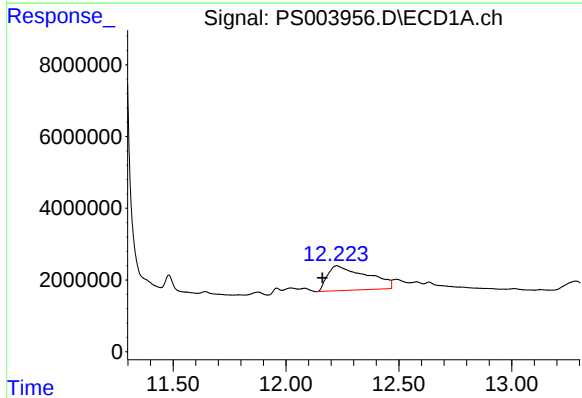


#7 MCPA

R.T.: 12.225 min
Delta R.T.: 0.063 min
Response: 83573985
Conc: 39.61 ug/ml

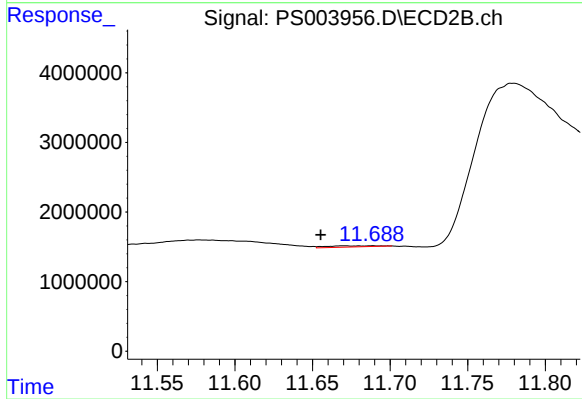

#7 MCPA


R.T.: 11.689 min
Delta R.T.: 0.034 min
Response: 447014
Conc: N.D.

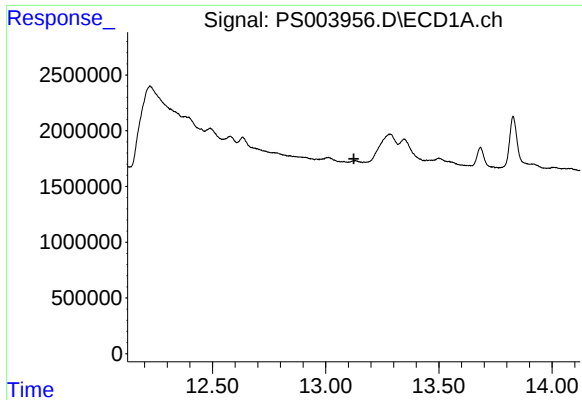

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S7C(12-20)COMP

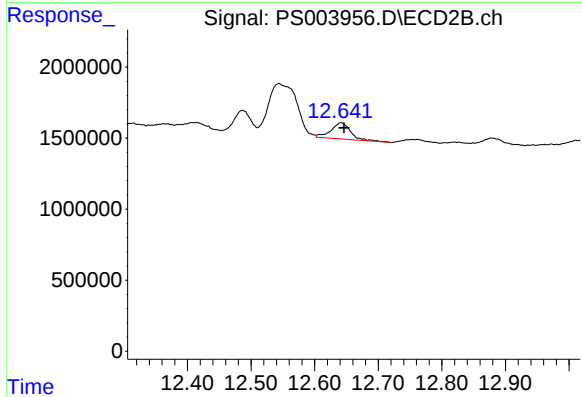


#9 2,4-D

R.T.: 12.642 min
Delta R.T.: -0.005 min
Response: 2442803
Conc: 4.59 ng/ml

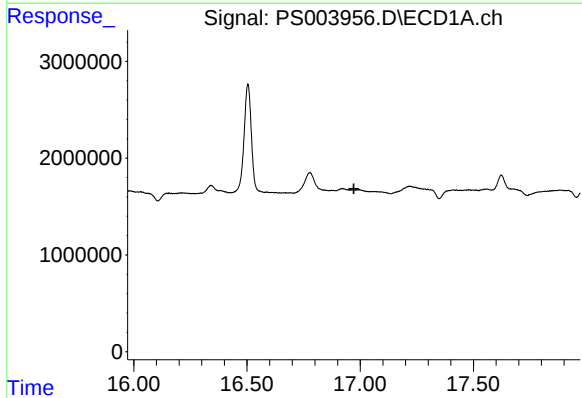


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

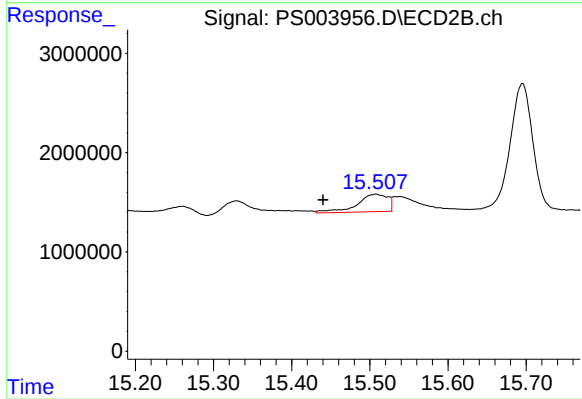

#14 DINOSEB


R.T.: 15.508 min
Delta R.T.: 0.068 min
Response: 4834944
Conc: 2.52 ng/ml

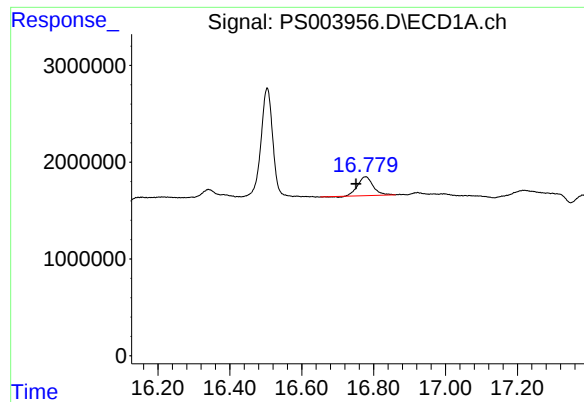

#15 Picloram

R.T.: 16.777 min
Delta R.T.: 0.026 min
Response: 5762054
Conc: 1.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
S7C(12-20)COMP

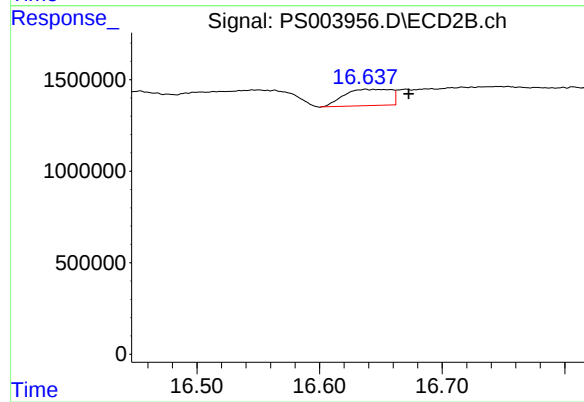

#15 Picloram

R.T.: 16.638 min
Delta R.T.: -0.034 min
Response: 2384749
Conc: N.D.