

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
 Data File : PS003958.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2019 07:01
 Operator : EI\SJ
 Sample : K2186-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 08:23:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.262	10.765	323.7E6	284.3E6	741.982	579.464
Target Compounds							
1) T	Dalapon	2.785	2.283	53867940	124.9E6	72.254	171.248 #
2) T	3,5-DICHL...	0.000	8.931	0	11598036	N.D.	18.183
3) T	4-Nitroph...	0.000	9.915	0	15026266	N.D.	66.185
5) T	DICAMBA	11.624	11.105	23209067	-1861053	11.313	N.D. #
7) T	MCPA	12.194	11.679	81654552	597601	38.703	<MDL #
9) T	2,4-D	13.118	12.624	3708127	4850699	7.626	9.119
10) T	Pentachlo...	0.000	13.171	0	1391521	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.778	0	4093353	N.D.	1.546
12) T	2,4,5-T	0.000	14.361	0	1554079	N.D.	<MDL
14) T	DINOSEB	0.000	15.489	0	5456591	N.D.	2.844
15) T	Picloram	16.750	16.622	6831094	3221997	2.011	1.016 #
16) T	DCPA	0.000	16.622	0	3221997	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
Data File : PS003958.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2019 07:01
Operator : EI\SJ
Sample : K2186-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 08:23:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

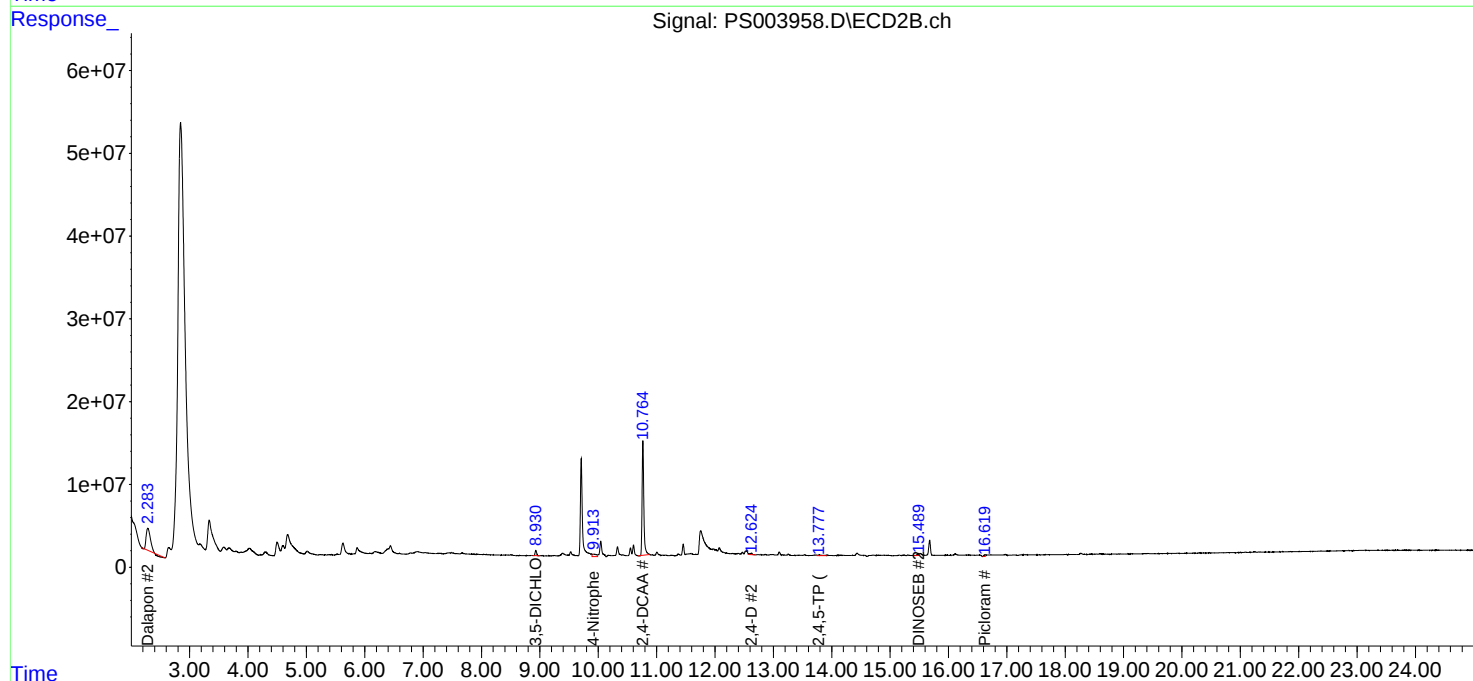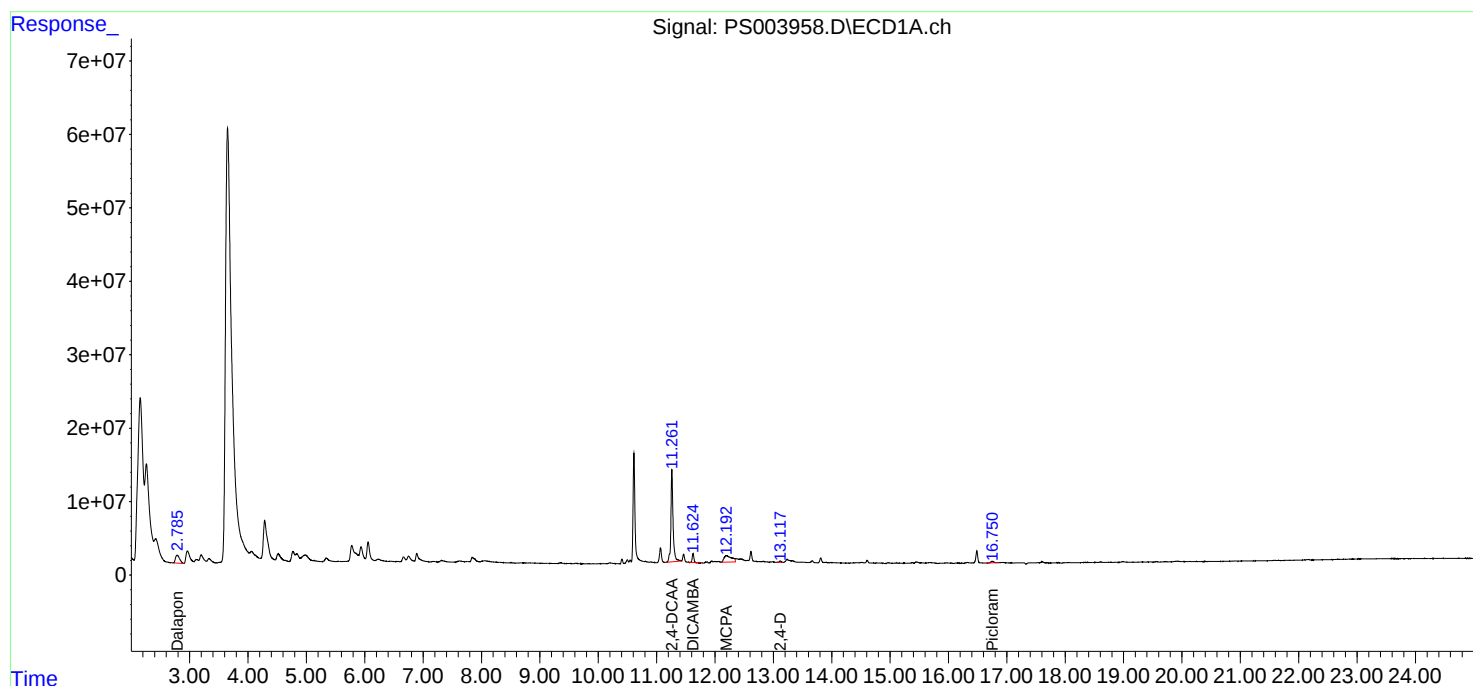


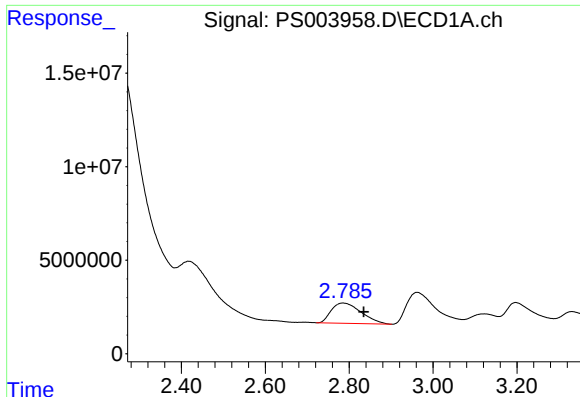

#1 Dalapon


R.T.: 2.785 min
Delta R.T.: -0.050 min
Response: 53867940
Conc: 72.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

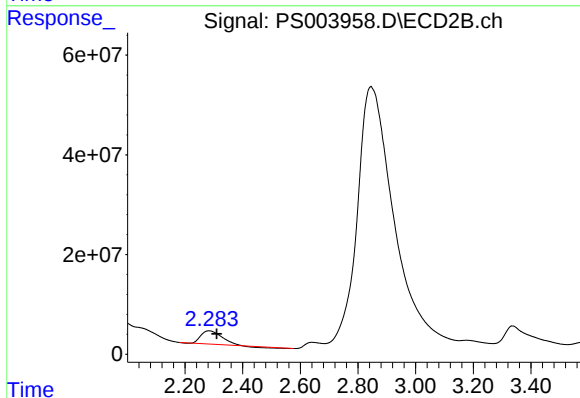


#1 Dalapon

R.T.: 2.283 min
Delta R.T.: -0.028 min
Response: 124947702
Conc: 171.25 ng/ml

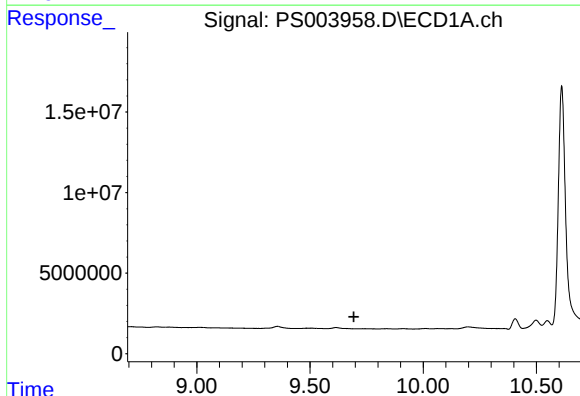


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

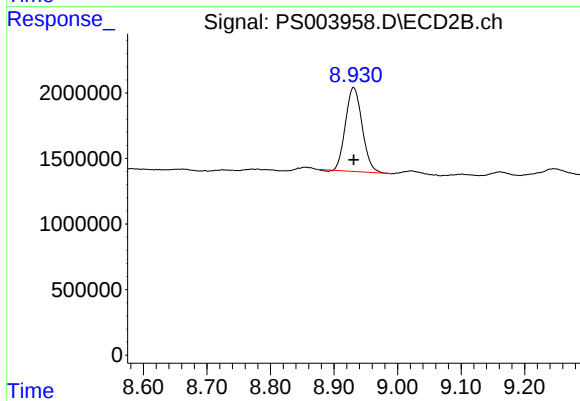

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.931 min
Delta R.T.: 0.000 min
Response: 11598036
Conc: 18.18 ng/ml

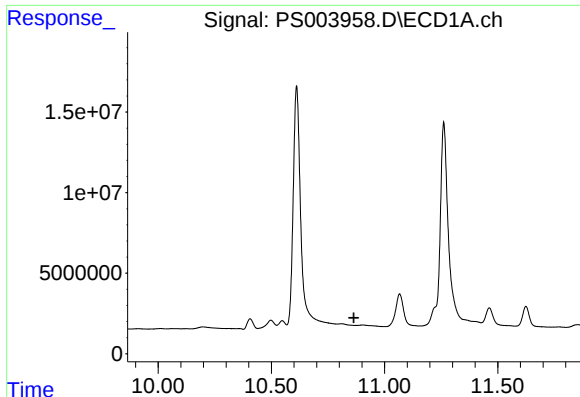

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

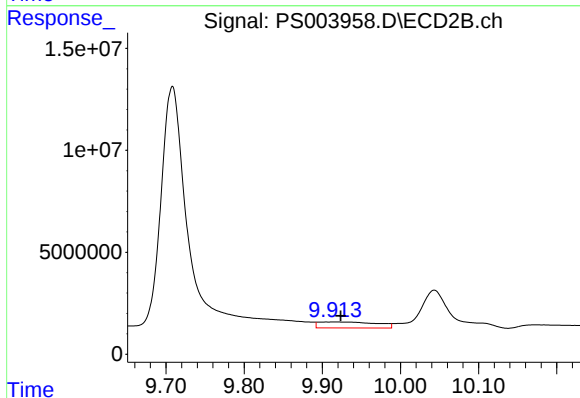


#3 4-Nitrophenol

R.T.: 9.915 min
Delta R.T.: -0.008 min
Response: 15026266
Conc: 66.18 ng/ml

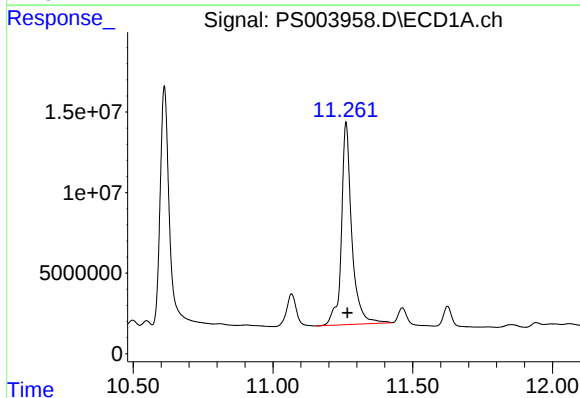


#4 2,4-DCAA

R.T.: 11.262 min
Delta R.T.: -0.005 min
Response: 323661539
Conc: 741.98 ng/ml

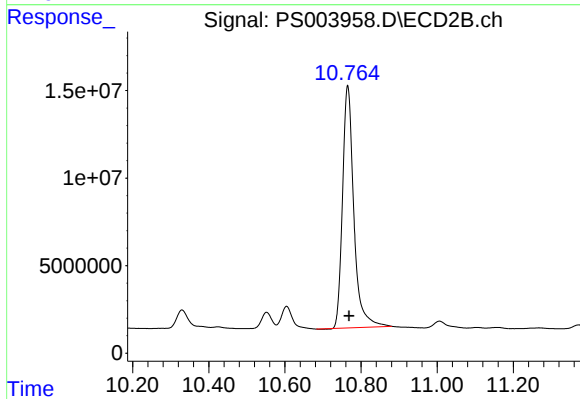

#4 2,4-DCAA


R.T.: 10.765 min
Delta R.T.: -0.004 min
Response: 284318779
Conc: 579.46 ng/ml

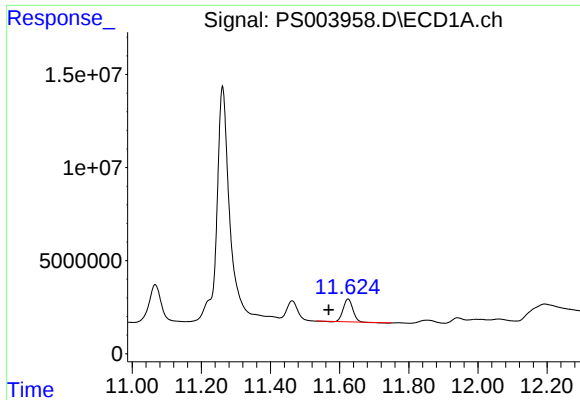

#5 DICAMBA


R.T.: 11.624 min
Delta R.T.: 0.056 min
Response: 23209067
Conc: 11.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

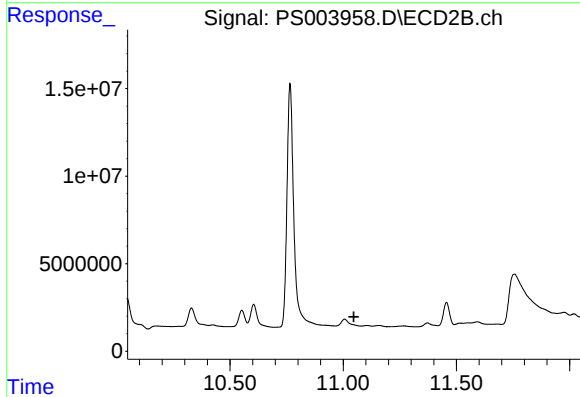


#5 DICAMBA

R.T.: 11.105 min
Delta R.T.: 0.058 min
Response: -1861053
Conc: N.D.

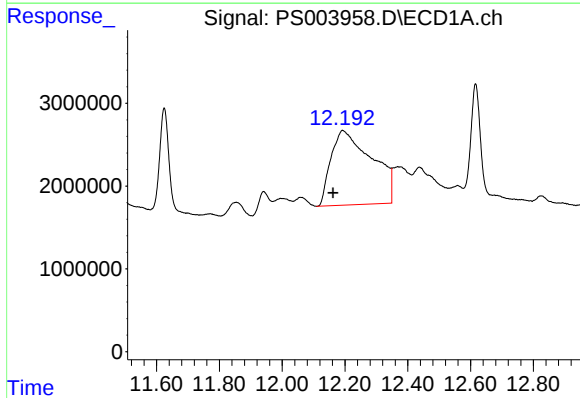


#7 MCPA

R.T.: 12.194 min
Delta R.T.: 0.032 min
Response: 81654552
Conc: 38.70 ug/ml

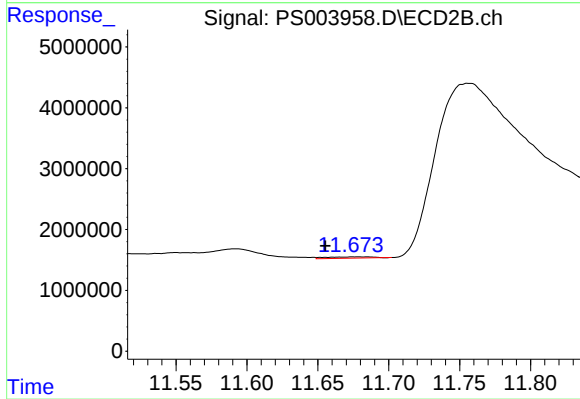

#7 MCPA


R.T.: 11.679 min
Delta R.T.: 0.024 min
Response: 597601
Conc: N.D.

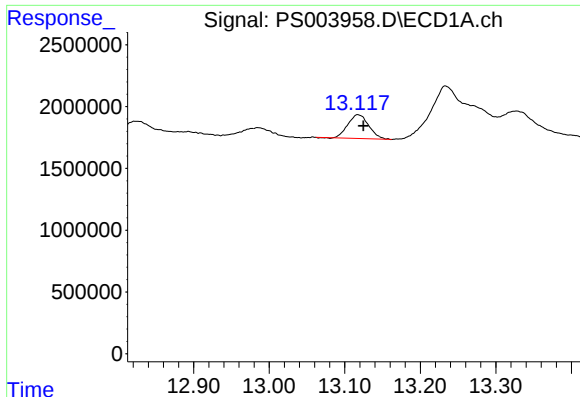

#9 2,4-D


R.T.: 13.118 min
Delta R.T.: -0.007 min
Response: 3708127
Conc: 7.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

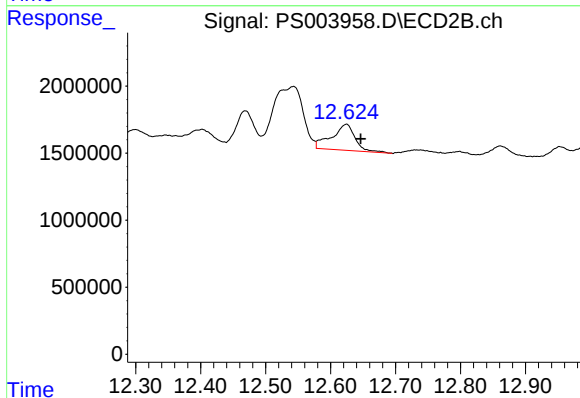


#9 2,4-D

R.T.: 12.624 min
Delta R.T.: -0.022 min
Response: 4850699
Conc: 9.12 ng/ml

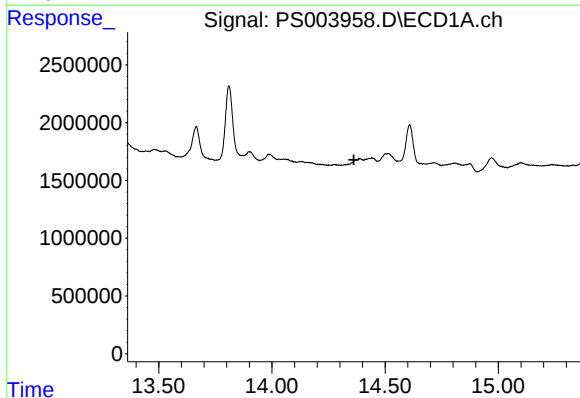


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.362 min
Response: 0
Conc: N.D.

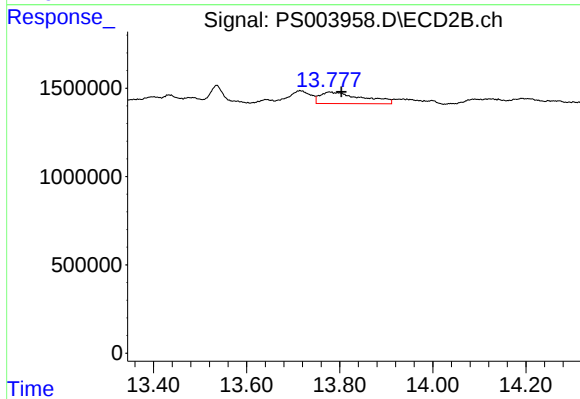

#11 2,4,5-TP (SILVEX)


R.T.: 13.778 min
Delta R.T.: -0.025 min
Response: 4093353
Conc: 1.55 ng/ml

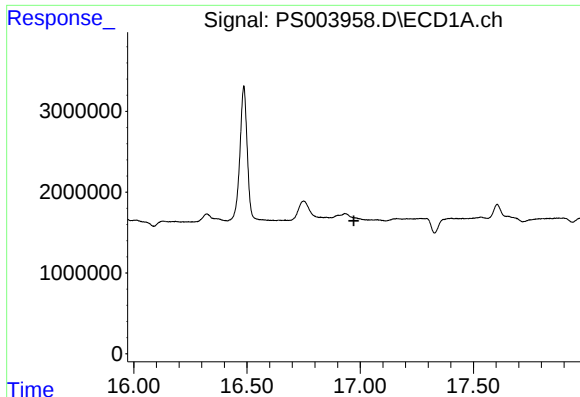

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

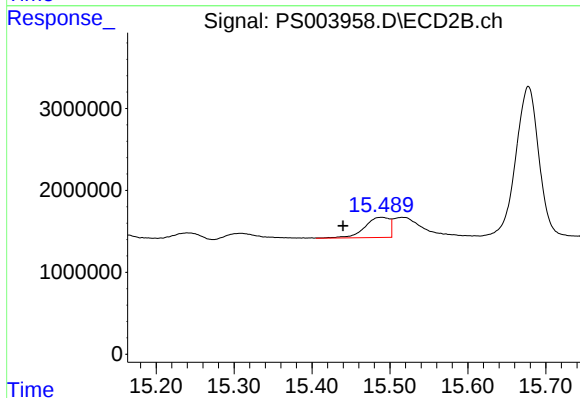


#14 DINOSEB

R.T.: 15.489 min
Delta R.T.: 0.049 min
Response: 5456591
Conc: 2.84 ng/ml

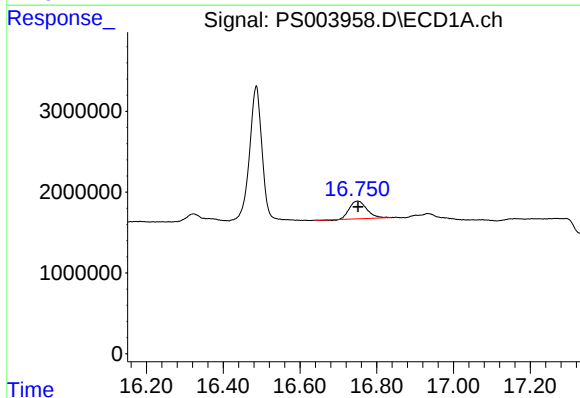

#15 Picloram

R.T.: 16.750 min
Delta R.T.: -0.002 min
Response: 6831094
Conc: 2.01 ng/ml

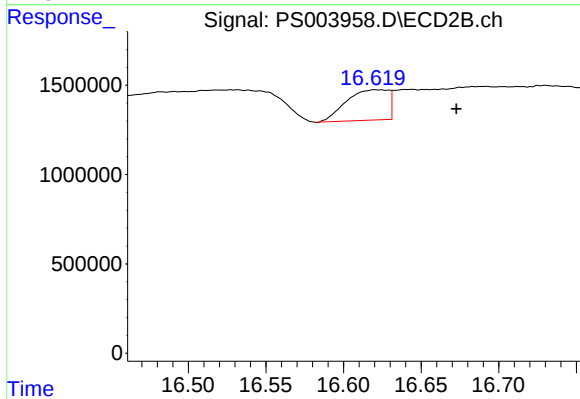

#15 Picloram

R.T.: 16.622 min
Delta R.T.: -0.050 min
Response: 3221997
Conc: 1.02 ng/ml