

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
 Data File : PS003959.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2019 07:33
 Operator : EI\SJ
 Sample : K2186-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 08:24:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.277	10.780	324.3E6	298.0E6	743.546	607.363
Target Compounds							
1) T	Dalapon	2.802	2.293	7077217	6016979	9.493	8.247
2) T	3,5-DICHL...	0.000	8.947	0	1445821	N.D.	2.267
3) T	4-Nitroph...	0.000	9.948	0	12702514	N.D.	55.950
5) T	DICAMBA	0.000	11.022	0	4778522	N.D.	2.569
6) T	MCPD	0.000	11.266	0	106554	N.D.	<MDL
7) T	MCPA	12.227	0.000	99302733	0	47.068	N.D. #
9) T	2,4-D	0.000	12.637	0	906251	N.D.	1.704
10) T	Pentachlo...	0.000	13.188	0	1205623	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.820	0	1342467	N.D.	<MDL
12) T	2,4,5-T	0.000	14.377	0	776659	N.D.	<MDL
13) T	2,4-DB	0.000	15.014	0	861231	N.D.	2.900
14) T	DINOSEB	0.000	15.507	0	13321135	N.D.	6.943
15) T	Picloram	16.774	0.000	7140690	0	2.102	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040319\
Data File : PS003959.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2019 07:33
Operator : EI\SJ
Sample : K2186-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 08:24:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

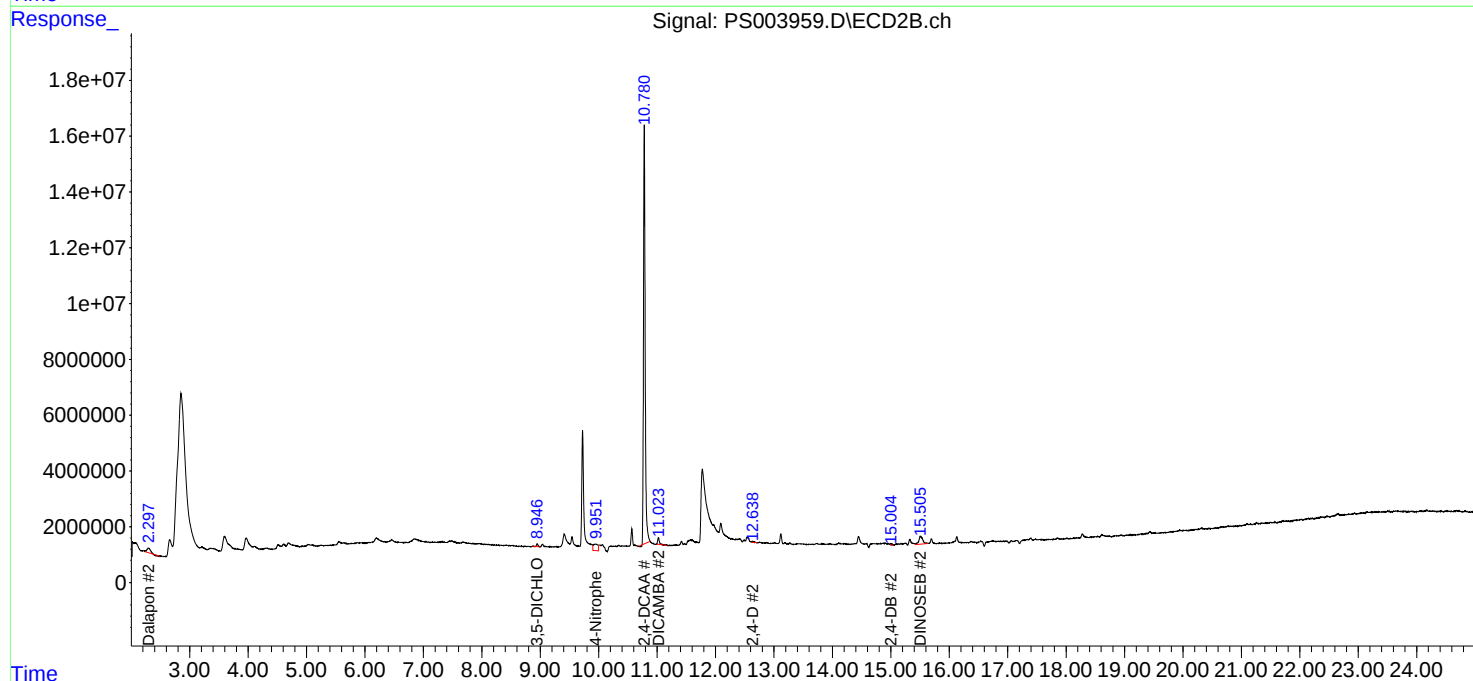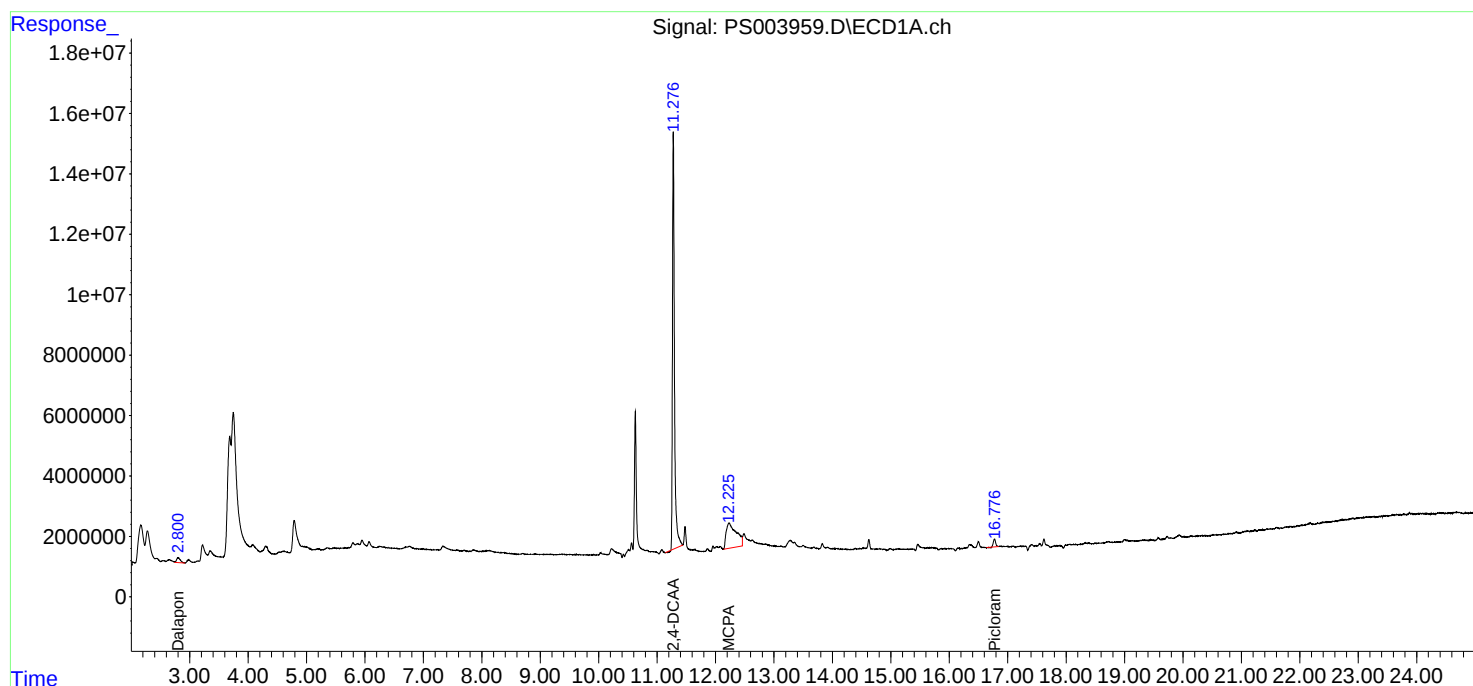


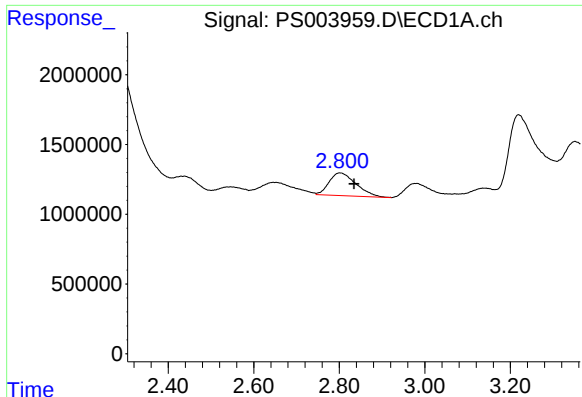

#1 Dalapon


R.T.: 2.802 min
Delta R.T.: -0.033 min
Response: 7077217
Conc: 9.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

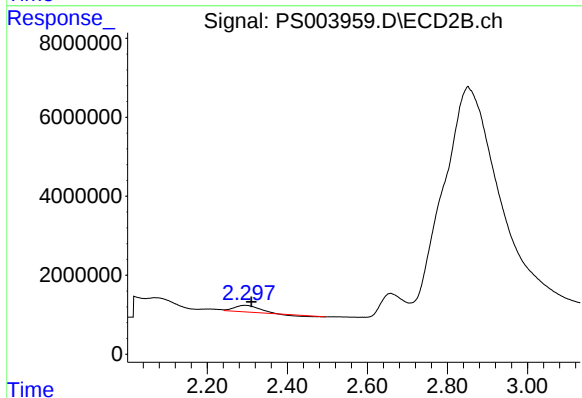


#1 Dalapon

R.T.: 2.293 min
Delta R.T.: -0.017 min
Response: 6016979
Conc: 8.25 ng/ml

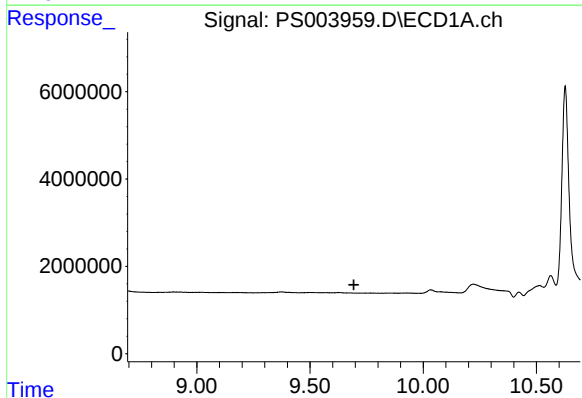


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

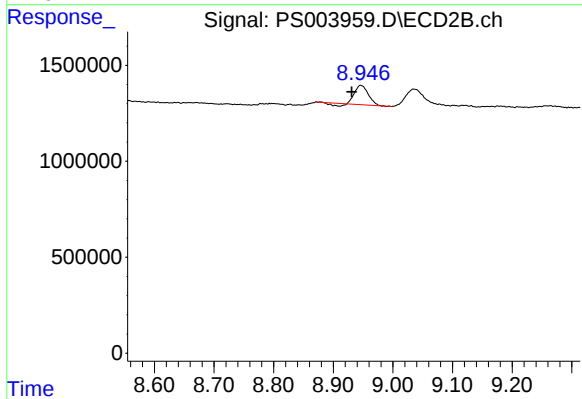

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.947 min
Delta R.T.: 0.016 min
Response: 1445821
Conc: 2.27 ng/ml

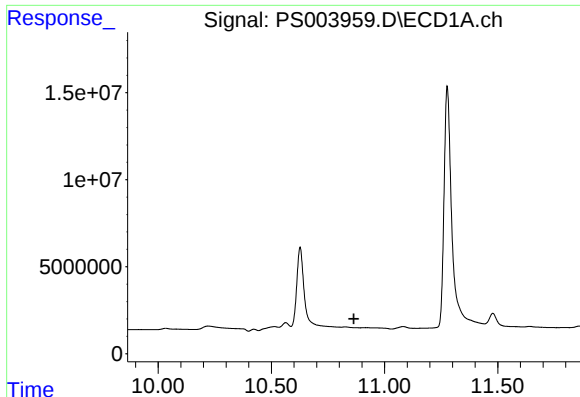

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

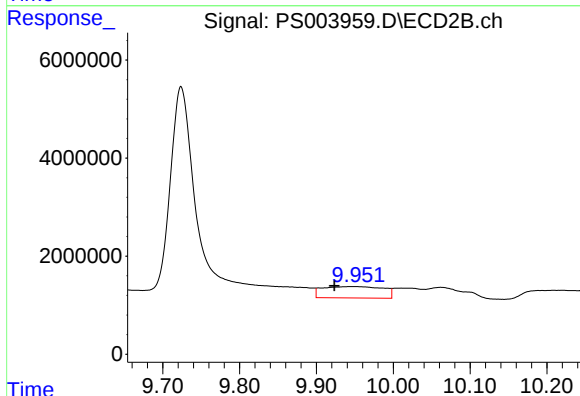


#3 4-Nitrophenol

R.T.: 9.948 min
Delta R.T.: 0.025 min
Response: 12702514
Conc: 55.95 ng/ml

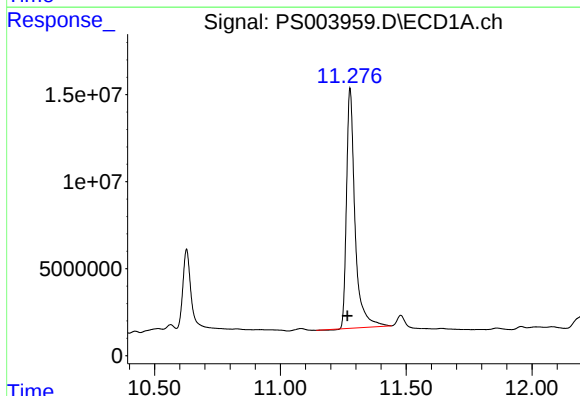


#4 2,4-DCAA

R.T.: 11.277 min
Delta R.T.: 0.010 min
Response: 324343896
Conc: 743.55 ng/ml

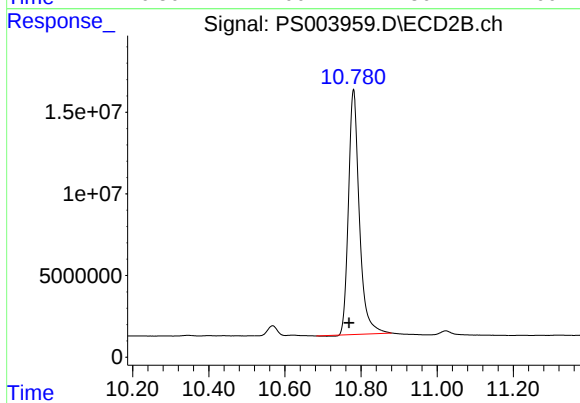

#4 2,4-DCAA


R.T.: 10.780 min
Delta R.T.: 0.012 min
Response: 298007627
Conc: 607.36 ng/ml

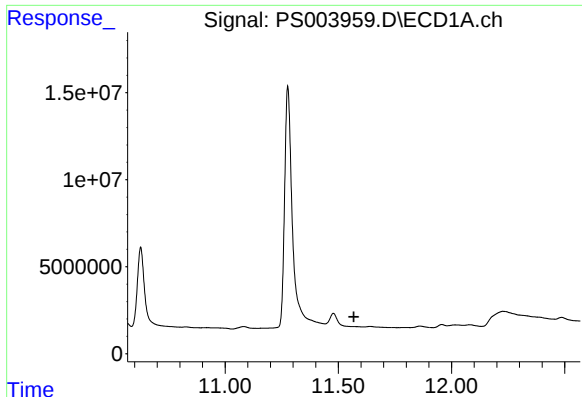

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

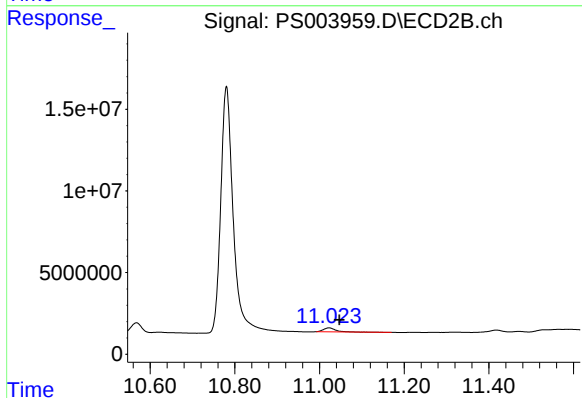


#5 DICAMBA

R.T.: 11.022 min
Delta R.T.: -0.025 min
Response: 4778522
Conc: 2.57 ng/ml

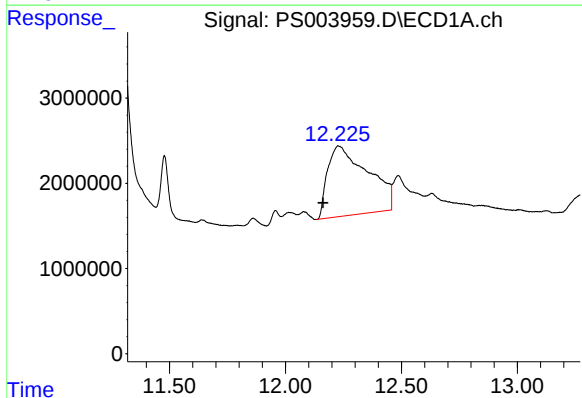


#7 MCPA

R.T.: 12.227 min
Delta R.T.: 0.065 min
Response: 99302733
Conc: 47.07 ug/ml

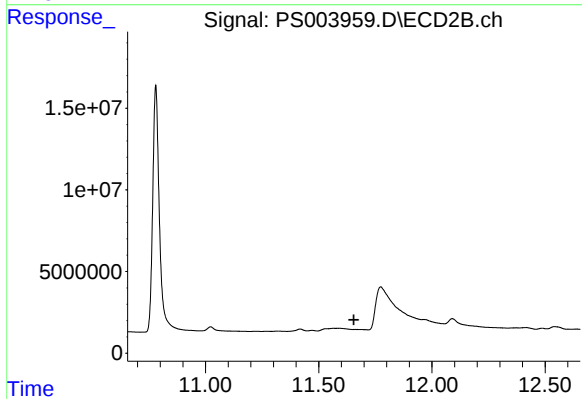

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.655 min
Response: 0
Conc: N.D.

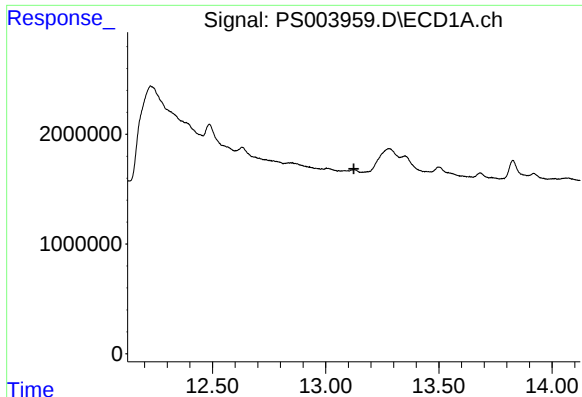

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

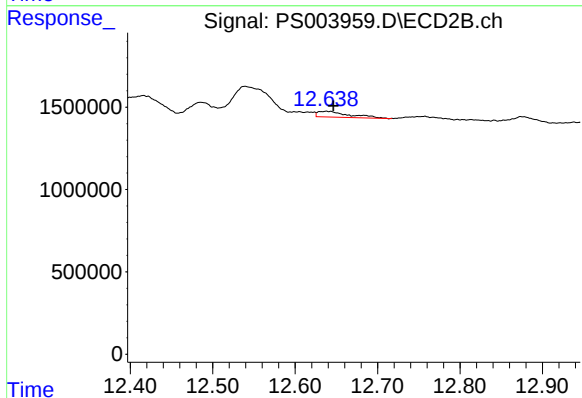


#9 2,4-D

R.T.: 12.637 min
Delta R.T.: -0.009 min
Response: 906251
Conc: 1.70 ng/ml

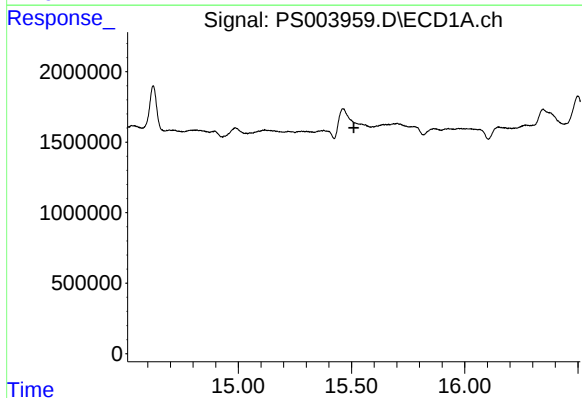


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

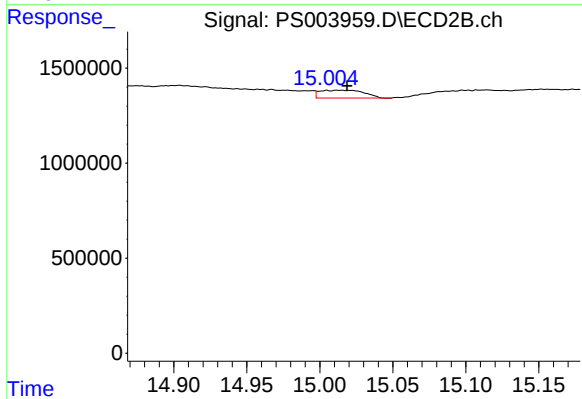

#13 2,4-DB


R.T.: 15.014 min
Delta R.T.: -0.005 min
Response: 861231
Conc: 2.90 ng/ml

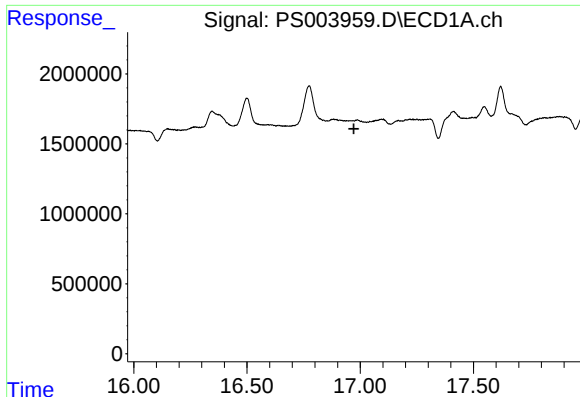

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

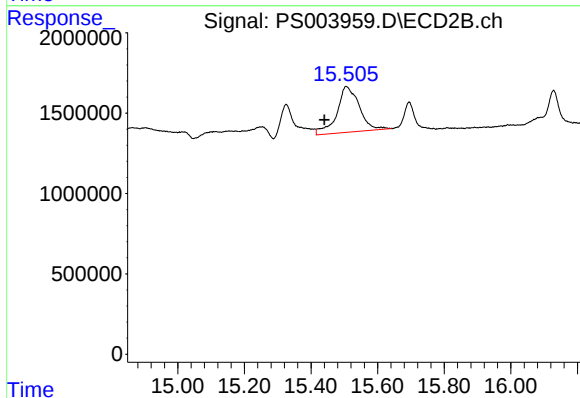


#14 DINOSEB

R.T.: 15.507 min
Delta R.T.: 0.067 min
Response: 13321135
Conc: 6.94 ng/ml

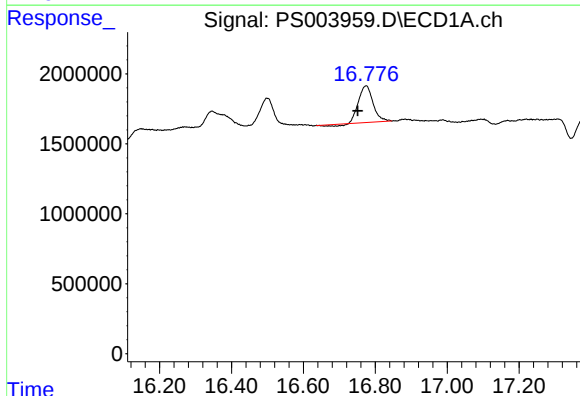

#15 Picloram

R.T.: 16.774 min
Delta R.T.: 0.023 min
Response: 7140690
Conc: 2.10 ng/ml

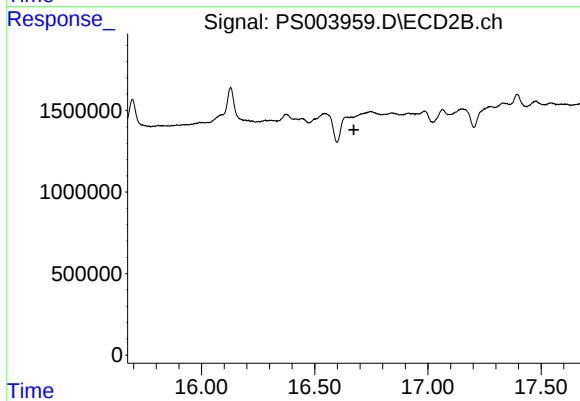

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.673 min
Response: 0
Conc: N.D.