

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
 Data File : PS003947.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2019 09:52
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 13:11:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.302	10.739	221.3E6	133033	507.319	<MDL #
Target Compounds							
1) T	Dalapon	0.000	2.256	0	88182	N.D.	<MDL
3) T	4-Nitroph...	0.000	9.943	0	57173	N.D.	<MDL
6) T	MCP	0.000	11.295	0	144611	N.D.	<MDL
7) T	MCPA	0.000	11.686	0	349409	N.D.	<MDL
8) T	DICHLORPROP	0.000	12.149	0	7334766	N.D.	15.756
9) T	2,4-D	0.000	12.623	0	714366	N.D.	1.343
10) T	Pentachlo...	0.000	13.215	0	1940215	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.861	0	1686524	N.D.	<MDL
12) T	2,4,5-T	0.000	14.322	0	48911	N.D.	<MDL
14) T	DINOSEB	0.000	15.492	0	683212	N.D.	<MDL
15) T	Picloram	0.000	16.654	0	4175432	N.D.	1.317
16) T	DCPA	0.000	16.654	0	4175432	N.D.	1.235



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
Data File : PS003947.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2019 09:52
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 13:11:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

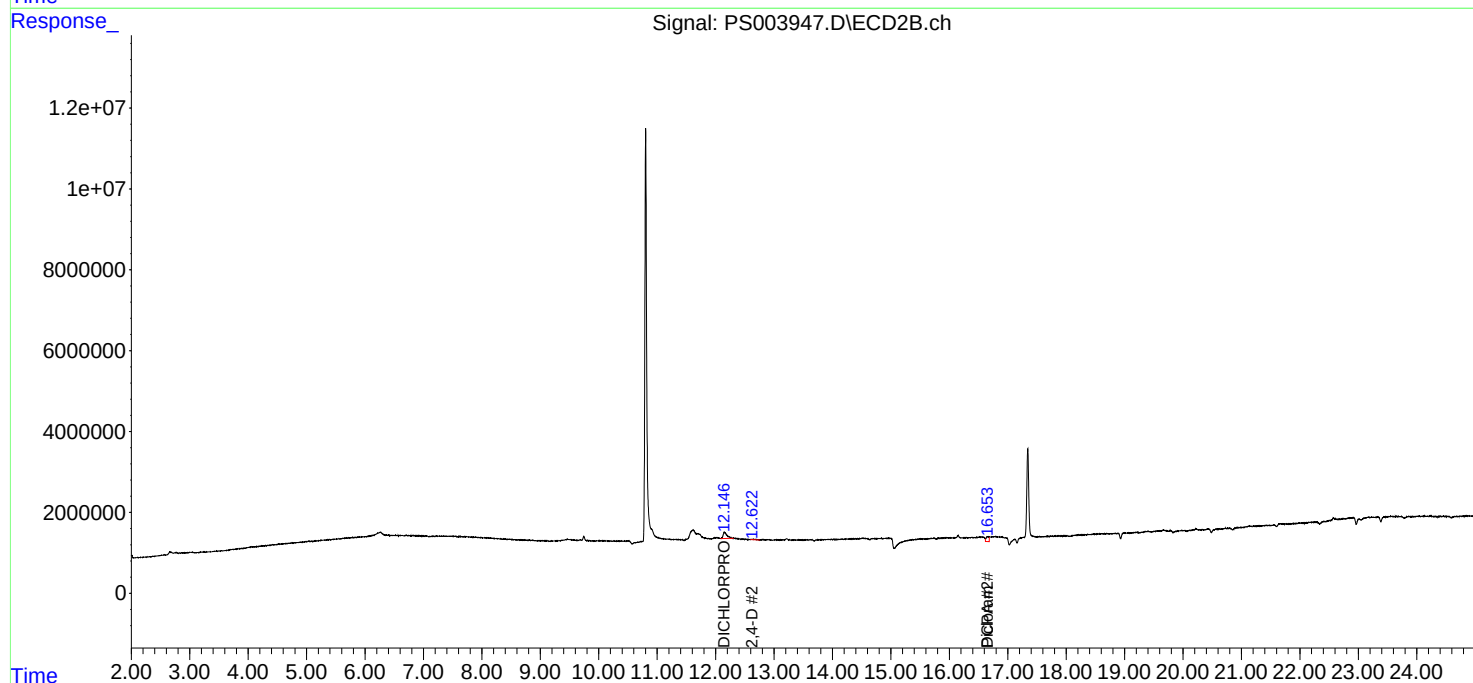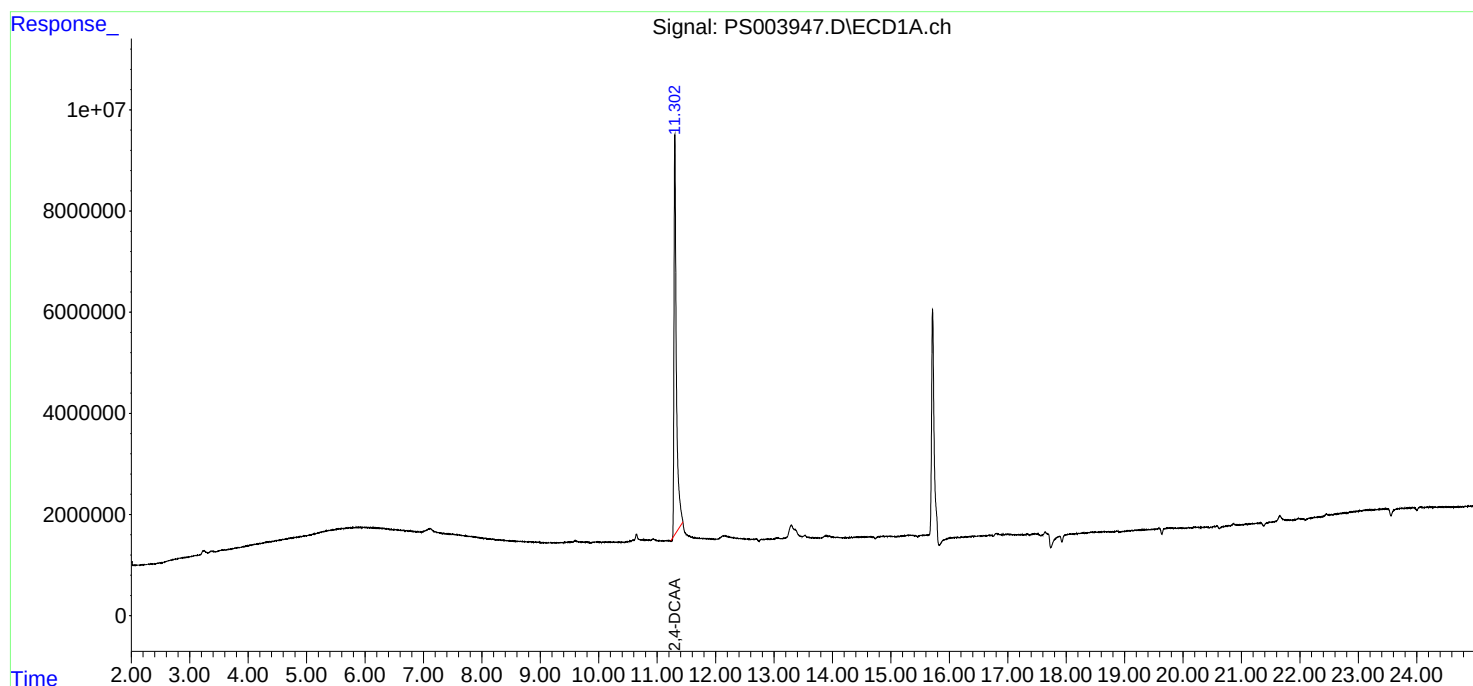


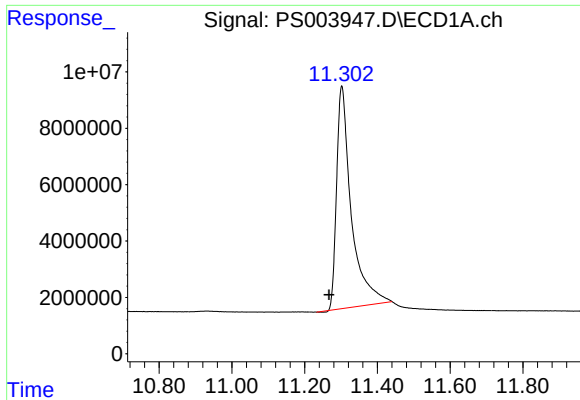

#4 2,4-DCAA


R.T.: 11.302 min
Delta R.T.: 0.036 min
Response: 221298894
Conc: 507.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

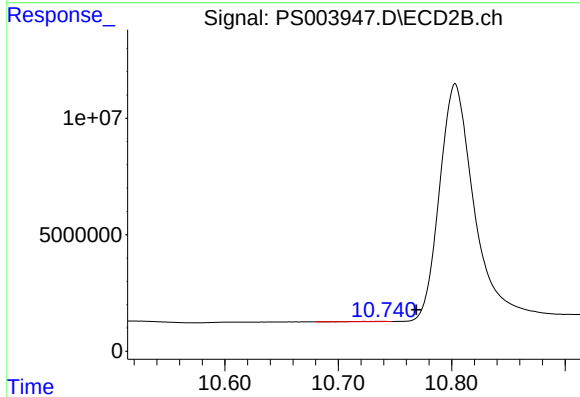


#4 2,4-DCAA

R.T.: 10.739 min
Delta R.T.: -0.030 min
Response: 133033
Conc: N.D.

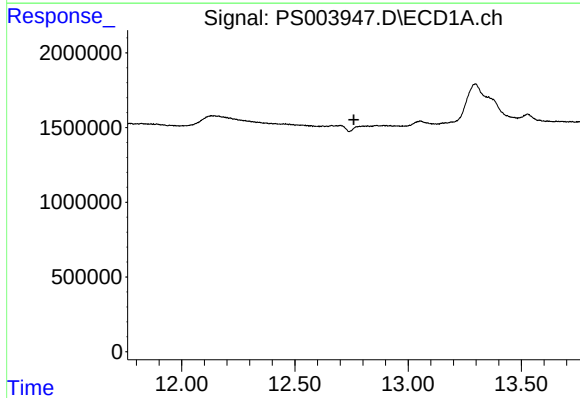


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.760 min
Response: 0
Conc: N.D.

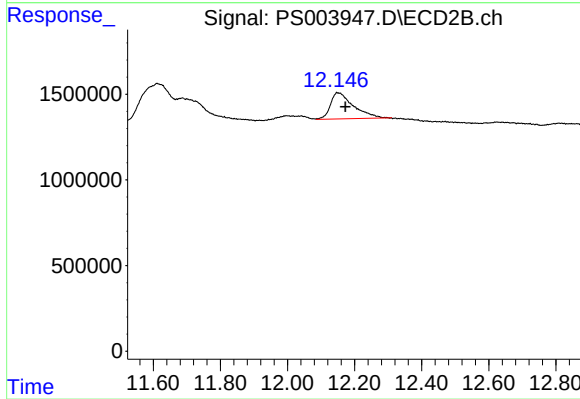

#8 DICHLORPROP


R.T.: 12.149 min
Delta R.T.: -0.024 min
Response: 7334766
Conc: 15.76 ng/ml

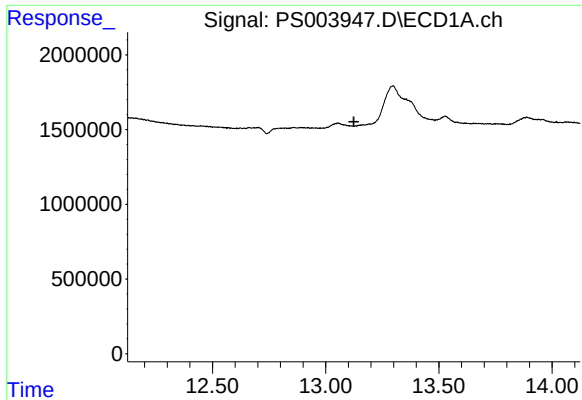

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

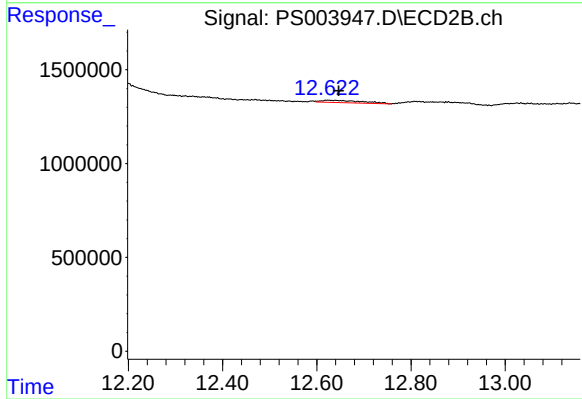


#9 2,4-D

R.T.: 12.623 min
Delta R.T.: -0.023 min
Response: 714366
Conc: 1.34 ng/ml

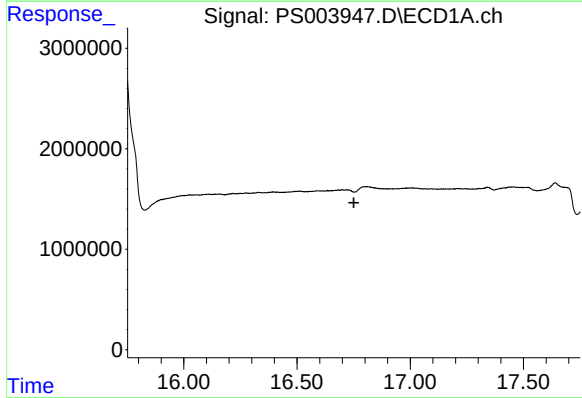


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.752 min
Response: 0
Conc: N.D.

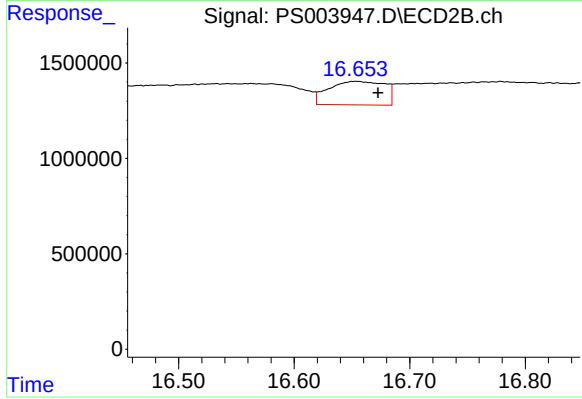

#15 Picloram


R.T.: 16.654 min
Delta R.T.: -0.019 min
Response: 4175432
Conc: 1.32 ng/ml

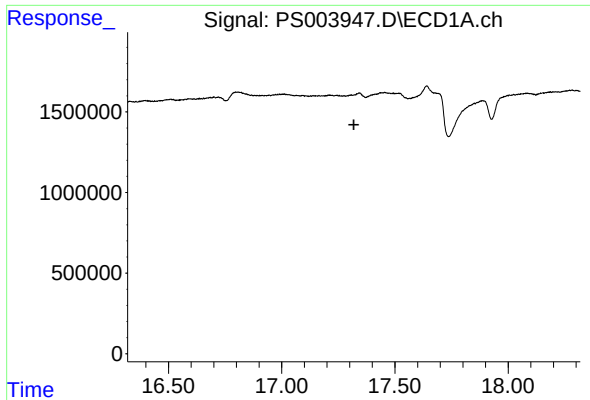

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

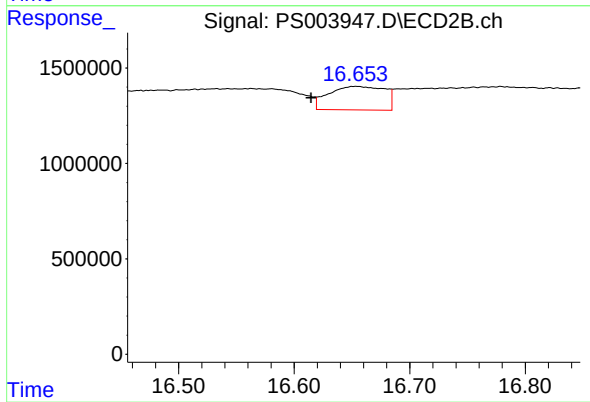

#16 DCPA

R.T.: 16.654 min
Delta R.T.: 0.039 min
Response: 4175432
Conc: 1.24 ng/ml