

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
 Data File : PS003948.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2019 10:25
 Operator : EI\SJ
 Sample : HTSDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 13:11:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.277	10.777	354.1E6	385.2E6	811.687	785.147
Target Compounds							
1) T	Dalapon	2.845	2.319	542.3E6	504.8E6	727.443	691.827
2) T	3,5-DICHL...	9.705	8.939	507.7E6	464.9E6	738.641	728.868
3) T	4-Nitroph...	10.883	9.933	164.6E6	163.8E6	759.694	721.636
5) T	DICAMBA	11.577	11.055	1543.8E6	1385.7E6	752.544	745.086
6) T	MCPD	11.919	11.287	105.7E6	89485937	76.005	75.790
7) T	MCPA	12.169	11.663	162.2E6	134.0E6	76.865	75.156
8) T	DICHLORPROP	12.770	12.181	360.3E6	341.6E6	737.564	733.741
9) T	2,4-D	13.138	12.656	359.4E6	389.8E6	739.149	732.756
10) T	Pentachlo...	13.491	13.183	5885.7E6	5217.8E6	764.050	753.976
11) T	2,4,5-TP ...	14.371	13.811	2195.3E6	1990.4E6	765.267	751.547
12) T	2,4,5-T	14.774	14.375	2220.1E6	1691.5E6	781.631	778.099
13) T	2,4-DB	15.521	15.026	253.4E6	193.8E6	840.370	652.555
14) T	DINOSEB	16.978	15.446	1834.4E6	1427.8E6	767.076	744.128
15) T	Picloram	16.763	16.680	2713.5E6	2531.4E6	798.768	798.232
16) T	DCPA	17.325	16.620	2769.2E6	2558.4E6	769.023	756.924



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
Data File : PS003948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2019 10:25
Operator : EI\SJ
Sample : HTSDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 13:11:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

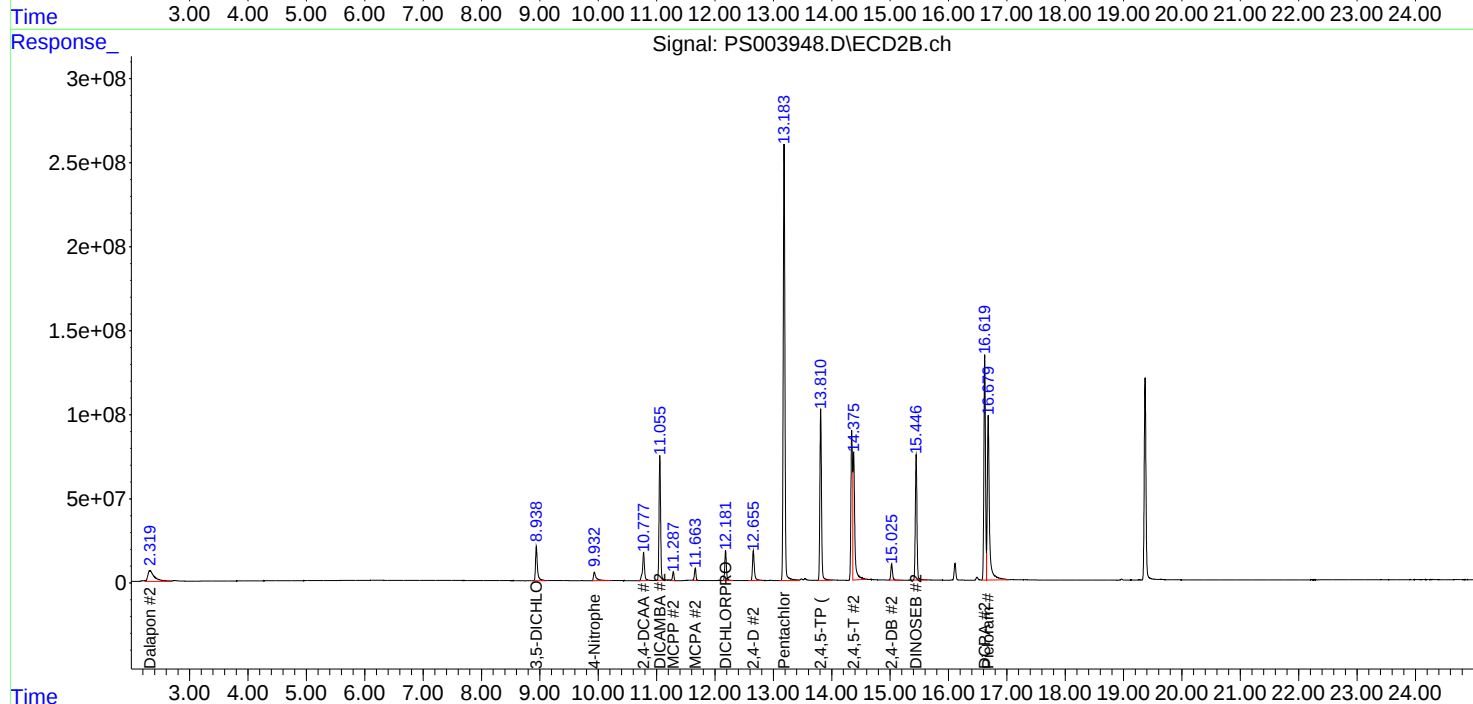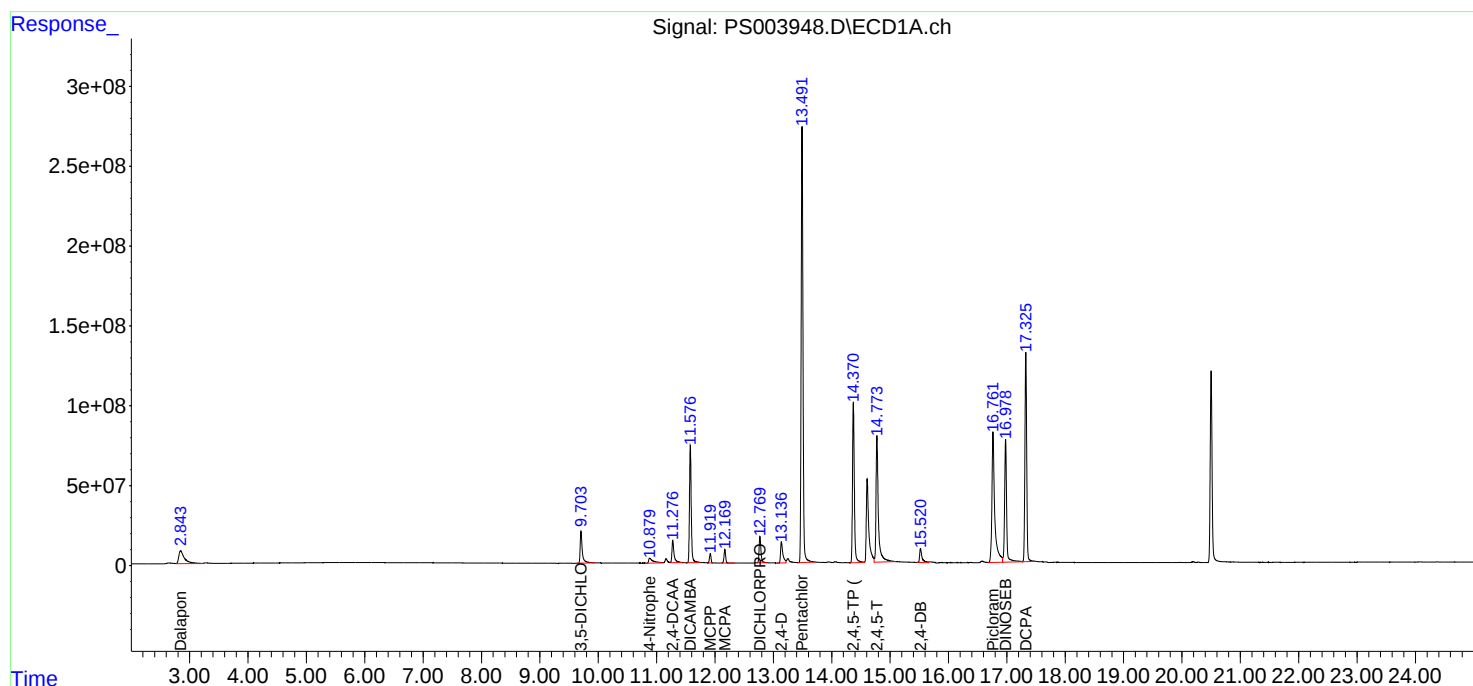


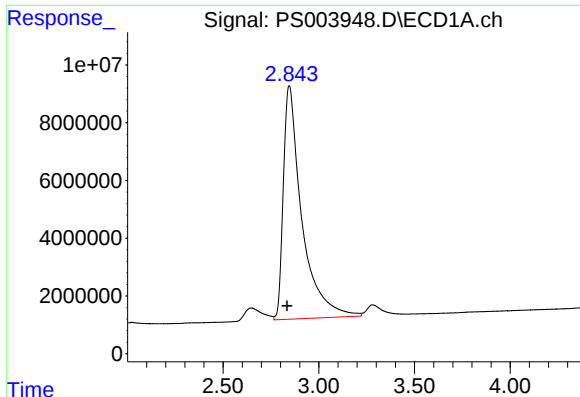

#1 Dalapon


R.T.: 2.845 min
Delta R.T.: 0.010 min
Response: 542332962
Conc: 727.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

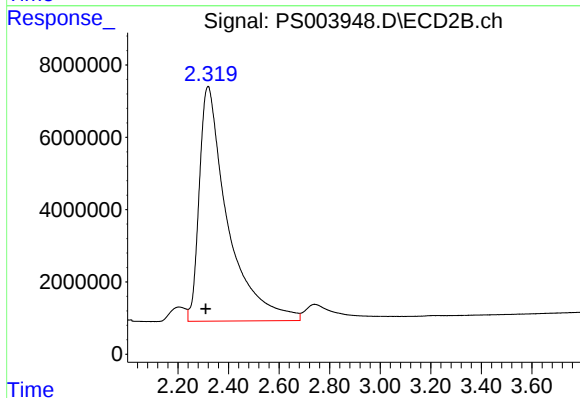


#1 Dalapon

R.T.: 2.319 min
Delta R.T.: 0.009 min
Response: 504776562
Conc: 691.83 ng/ml

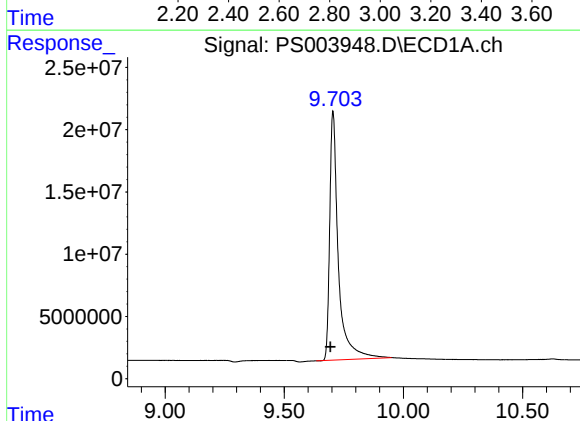


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.705 min
Delta R.T.: 0.011 min
Response: 507713930
Conc: 738.64 ng/ml

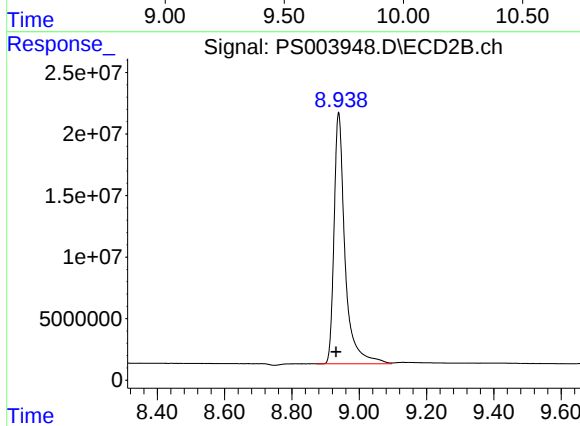

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.939 min
Delta R.T.: 0.008 min
Response: 464913670
Conc: 728.87 ng/ml

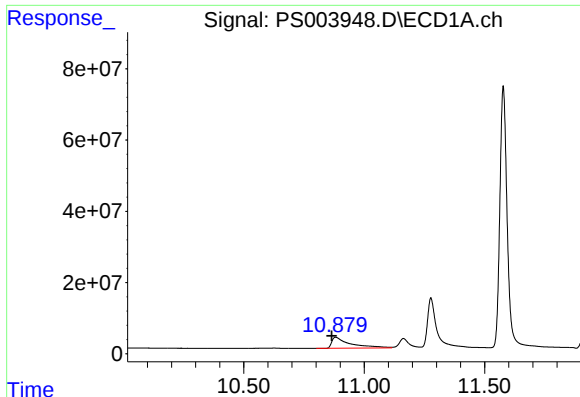

#3 4-Nitrophenol


R.T.: 10.883 min
Delta R.T.: 0.018 min
Response: 164595411
Conc: 759.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

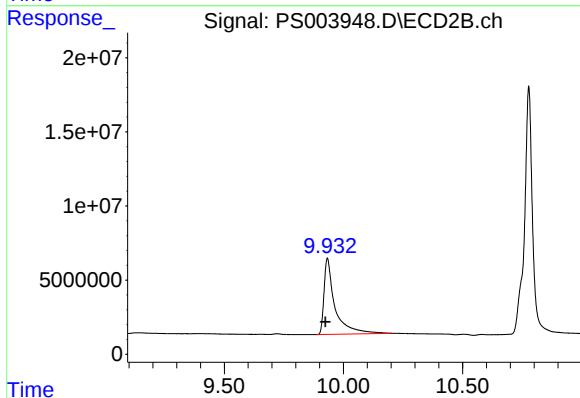


#3 4-Nitrophenol

R.T.: 9.933 min
Delta R.T.: 0.009 min
Response: 163836471
Conc: 721.64 ng/ml

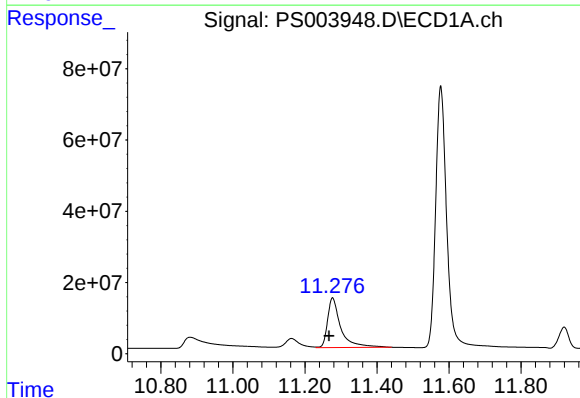


#4 2,4-DCAA

R.T.: 11.277 min
Delta R.T.: 0.010 min
Response: 354067814
Conc: 811.69 ng/ml

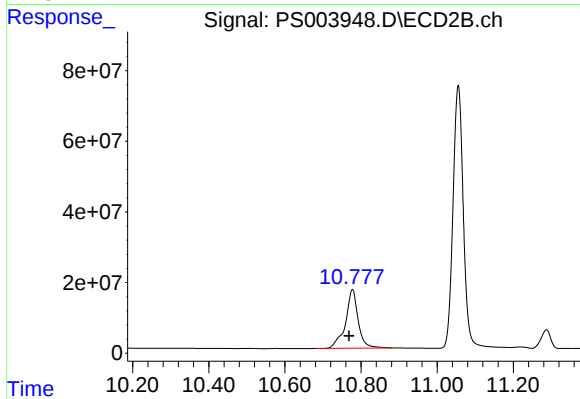

#4 2,4-DCAA


R.T.: 10.777 min
Delta R.T.: 0.009 min
Response: 385239151
Conc: 785.15 ng/ml

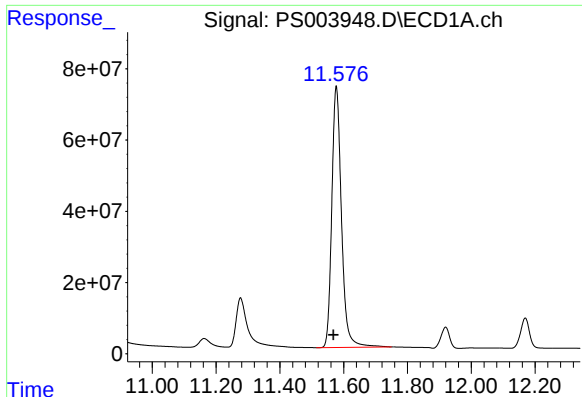

#5 DICAMBA


R.T.: 11.577 min
Delta R.T.: 0.009 min
Response: 1543809420
Conc: 752.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

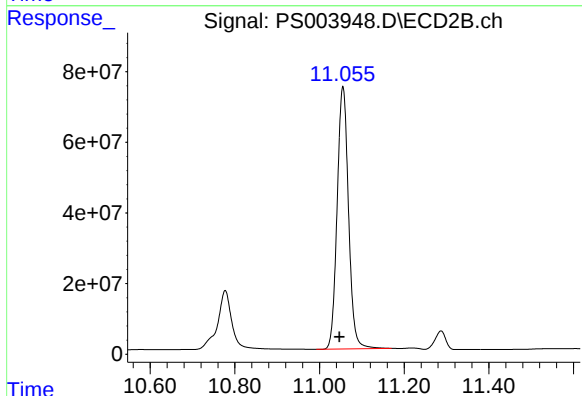


#5 DICAMBA

R.T.: 11.055 min
Delta R.T.: 0.008 min
Response: 1385676780
Conc: 745.09 ng/ml

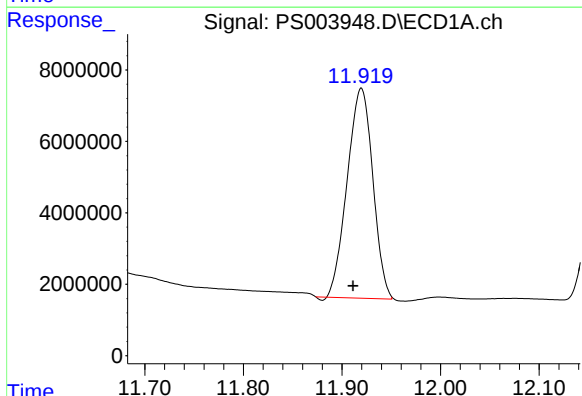


#6 MCP

R.T.: 11.919 min
Delta R.T.: 0.008 min
Response: 105725607
Conc: 76.01 ug/ml

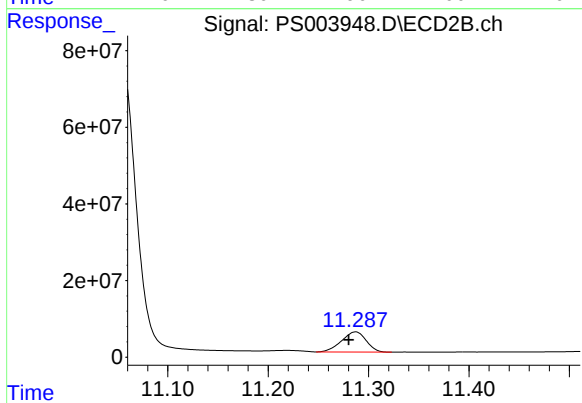

#6 MCP


R.T.: 11.287 min
Delta R.T.: 0.007 min
Response: 89485937
Conc: 75.79 ug/ml

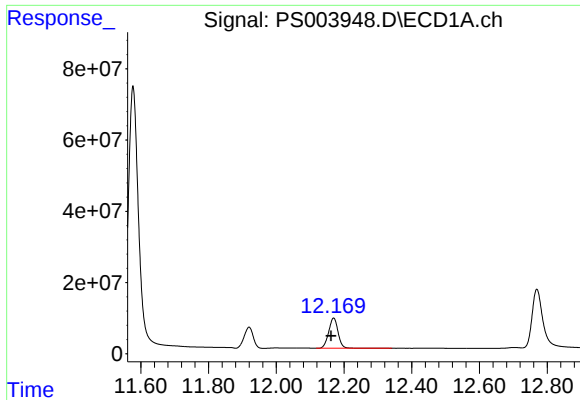

#7 MCPA


R.T.: 12.169 min
Delta R.T.: 0.007 min
Response: 162167933
Conc: 76.86 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

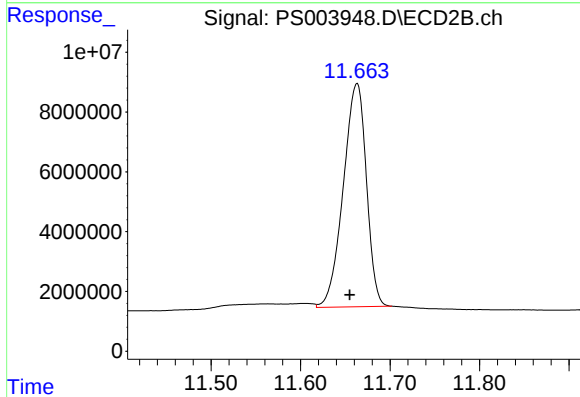


#7 MCPA

R.T.: 11.663 min
Delta R.T.: 0.007 min
Response: 134028183
Conc: 75.16 ug/ml

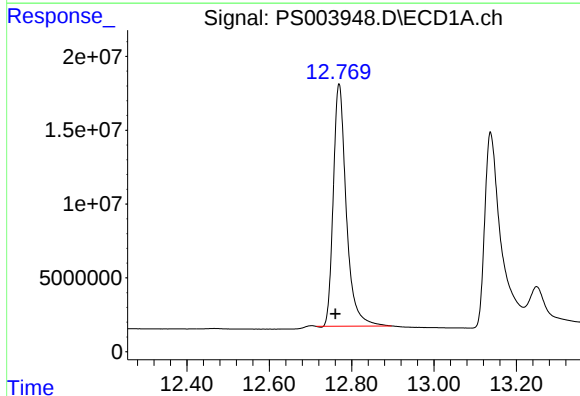


#8 DICHLORPROP

R.T.: 12.770 min
Delta R.T.: 0.010 min
Response: 360255105
Conc: 737.56 ng/ml

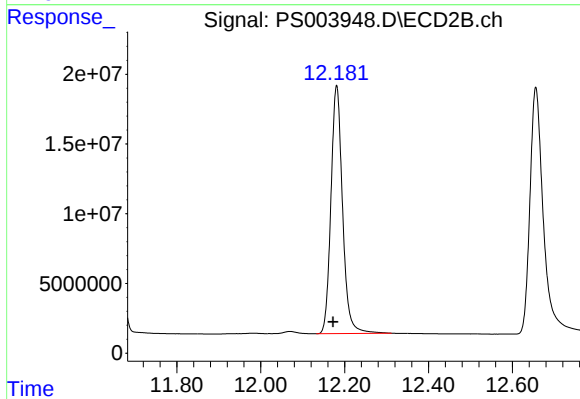

#8 DICHLORPROP


R.T.: 12.181 min
Delta R.T.: 0.008 min
Response: 341581074
Conc: 733.74 ng/ml

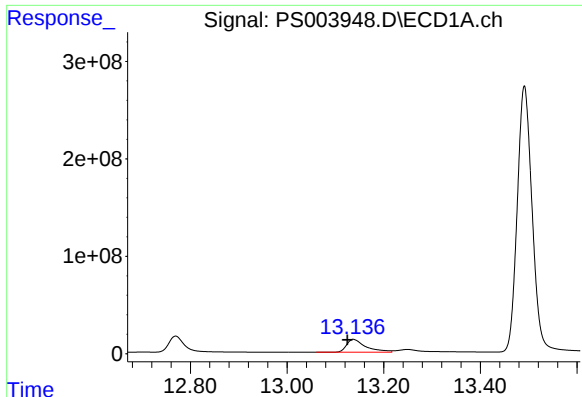

#9 2,4-D


R.T.: 13.138 min
Delta R.T.: 0.014 min
Response: 359429219
Conc: 739.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

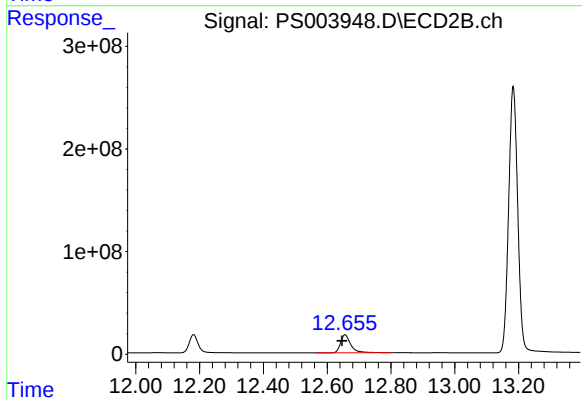


#9 2,4-D

R.T.: 12.656 min
Delta R.T.: 0.009 min
Response: 389757194
Conc: 732.76 ng/ml

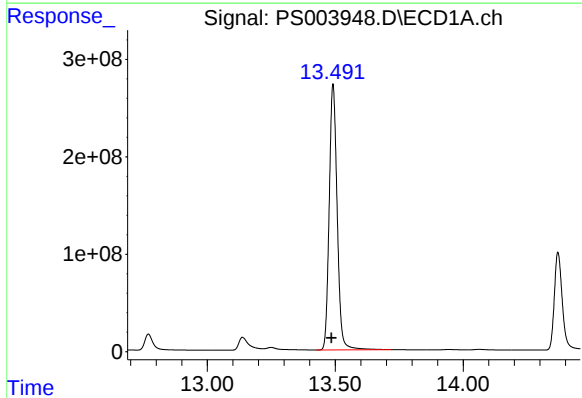


#10 Pentachlorophenol

R.T.: 13.491 min
Delta R.T.: 0.007 min
Response: 5885747727
Conc: 764.05 ng/ml

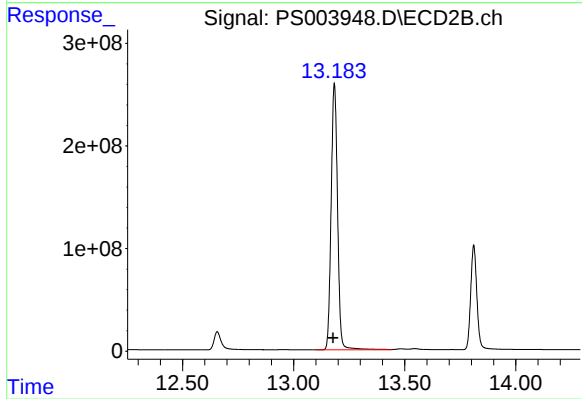

#10 Pentachlorophenol


R.T.: 13.183 min
Delta R.T.: 0.007 min
Response: 5217799381
Conc: 753.98 ng/ml

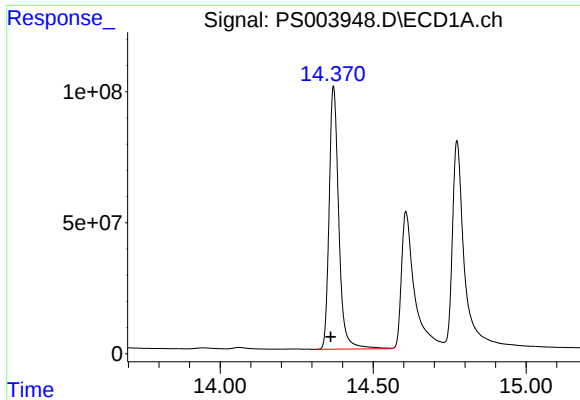

#11 2,4,5-TP (SILVEX)


R.T.: 14.371 min
Delta R.T.: 0.009 min
Response: 2195278166
Conc: 765.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

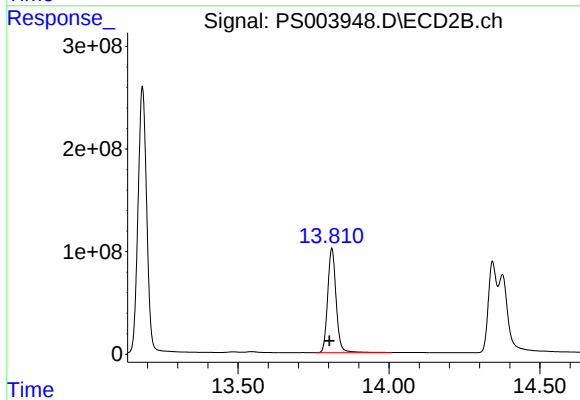


#11 2,4,5-TP (SILVEX)

R.T.: 13.811 min
Delta R.T.: 0.007 min
Response: 1990392975
Conc: 751.55 ng/ml

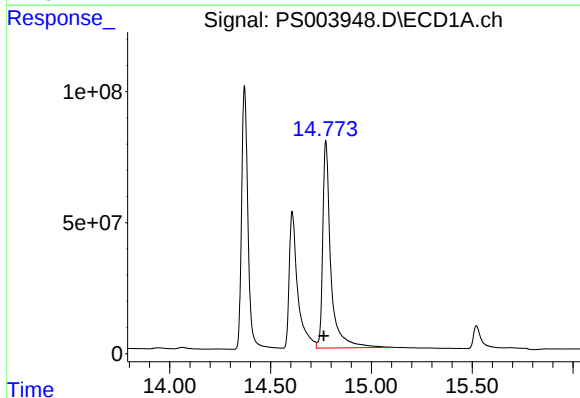


#12 2,4,5-T

R.T.: 14.774 min
Delta R.T.: 0.011 min
Response: 2220127577
Conc: 781.63 ng/ml

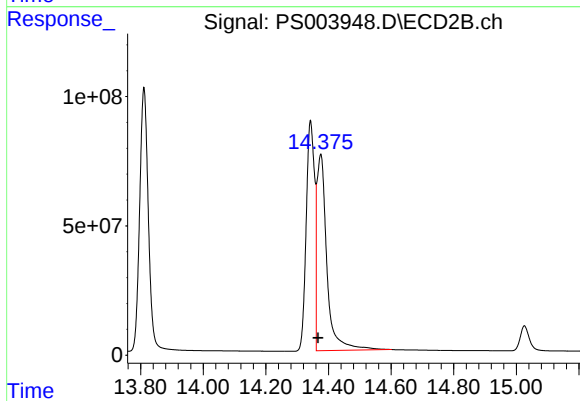

#12 2,4,5-T


R.T.: 14.375 min
Delta R.T.: 0.008 min
Response: 1691492598
Conc: 778.10 ng/ml

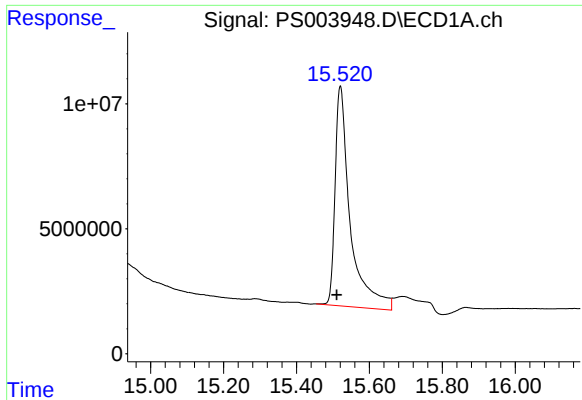

#13 2,4-DB


R.T.: 15.521 min
Delta R.T.: 0.011 min
Response: 253373457
Conc: 840.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

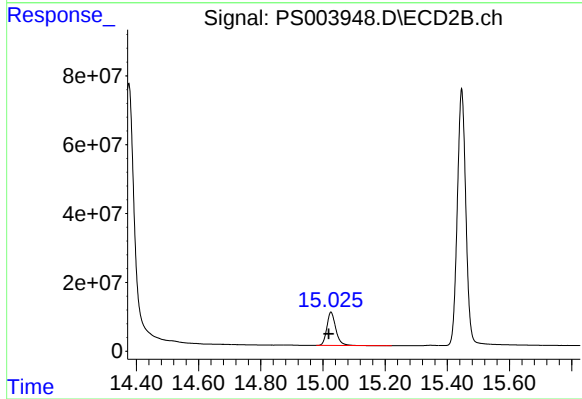


#13 2,4-DB

R.T.: 15.026 min
Delta R.T.: 0.007 min
Response: 193776312
Conc: 652.56 ng/ml

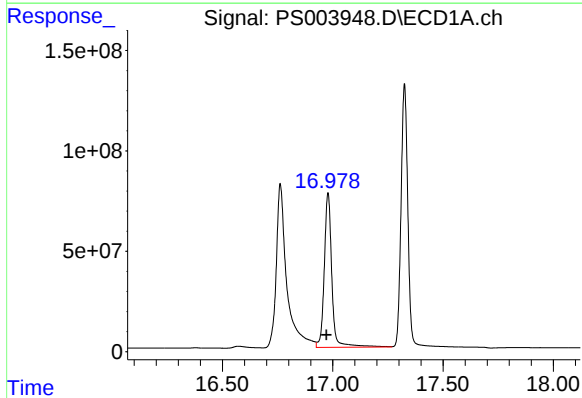


#14 DINOSEB

R.T.: 16.978 min
Delta R.T.: 0.006 min
Response: 1834372875
Conc: 767.08 ng/ml

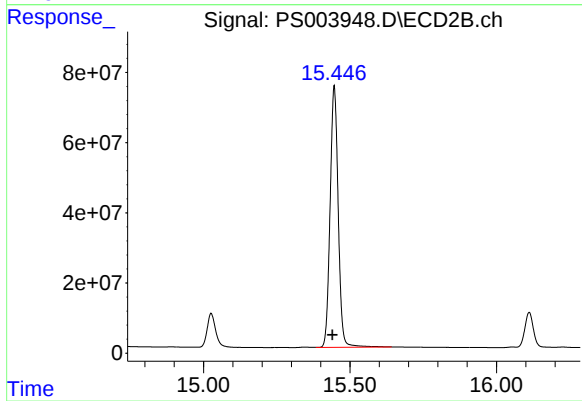

#14 DINOSEB


R.T.: 15.446 min
Delta R.T.: 0.006 min
Response: 1427765886
Conc: 744.13 ng/ml

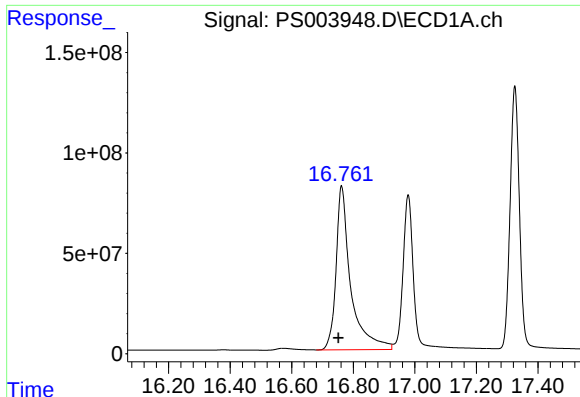

#15 Picloram


R.T.: 16.763 min
Delta R.T.: 0.011 min
Response: 2713463342
Conc: 798.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

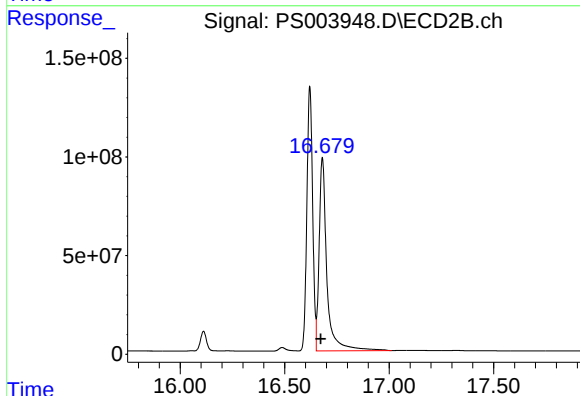


#15 Picloram

R.T.: 16.680 min
Delta R.T.: 0.007 min
Response: 2531370953
Conc: 798.23 ng/ml

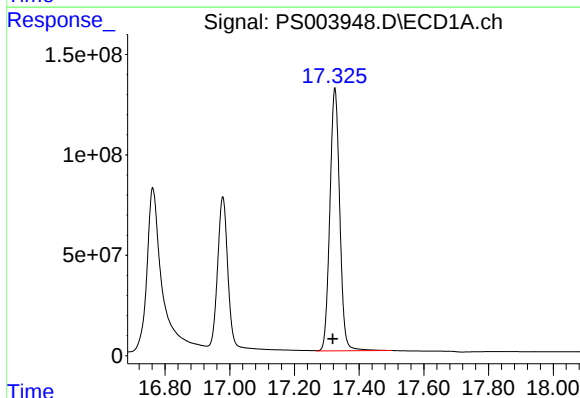

#16 DCPA

R.T.: 17.325 min
Delta R.T.: 0.006 min
Response: 2769176587
Conc: 769.02 ng/ml

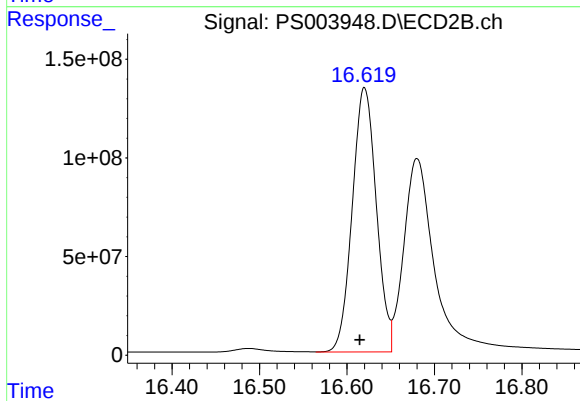

#16 DCPA

R.T.: 16.620 min
Delta R.T.: 0.006 min
Response: 2558428526
Conc: 756.92 ng/ml