

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
 Data File : PS003953.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2019 13:12
 Operator : EI\SJ
 Sample : K2182-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 S8A-S8B(12-16)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 14:11:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.274	10.776	305.5E6	270.0E6	700.320	550.327
Target Compounds							
1) T	Dalapon	2.804	2.307	54369106	106.4E6	72.926	145.894 #
2) T	3,5-DICHL...	0.000	8.943	0	10162308	N.D.	15.932
3) T	4-Nitroph...	0.000	9.940	0	14505264	N.D.	63.890
5) T	DICAMBA	0.000	11.016	0	5493644	N.D.	2.954
7) T	MCPA	12.130	11.669	330.5E6	233178	156.629	<MDL #
9) T	2,4-D	0.000	12.635	0	2043366	N.D.	3.842
10) T	Pentachlo...	0.000	13.178	0	704711	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.783	0	3009701	N.D.	1.136
12) T	2,4,5-T	0.000	14.359	0	2632946	N.D.	1.211
13) T	2,4-DB	0.000	14.979	0	8422764	N.D.	28.364
15) T	Picloram	16.758	16.641	10797208	10708962	3.178	3.377
16) T	DCPA	0.000	16.641	0	10708962	N.D.	3.168



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
Data File : PS003953.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2019 13:12
Operator : EI\SJ
Sample : K2182-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
S8A-S8B(12-16)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 14:11:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

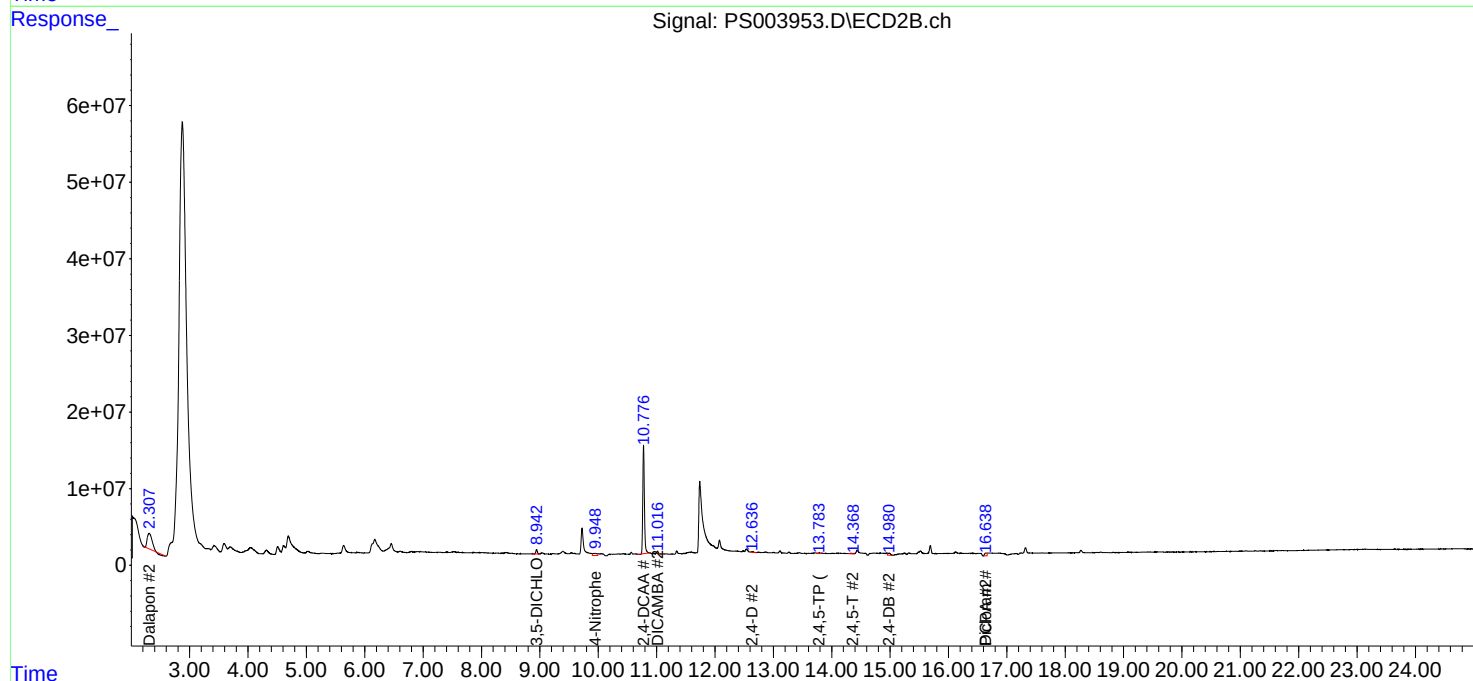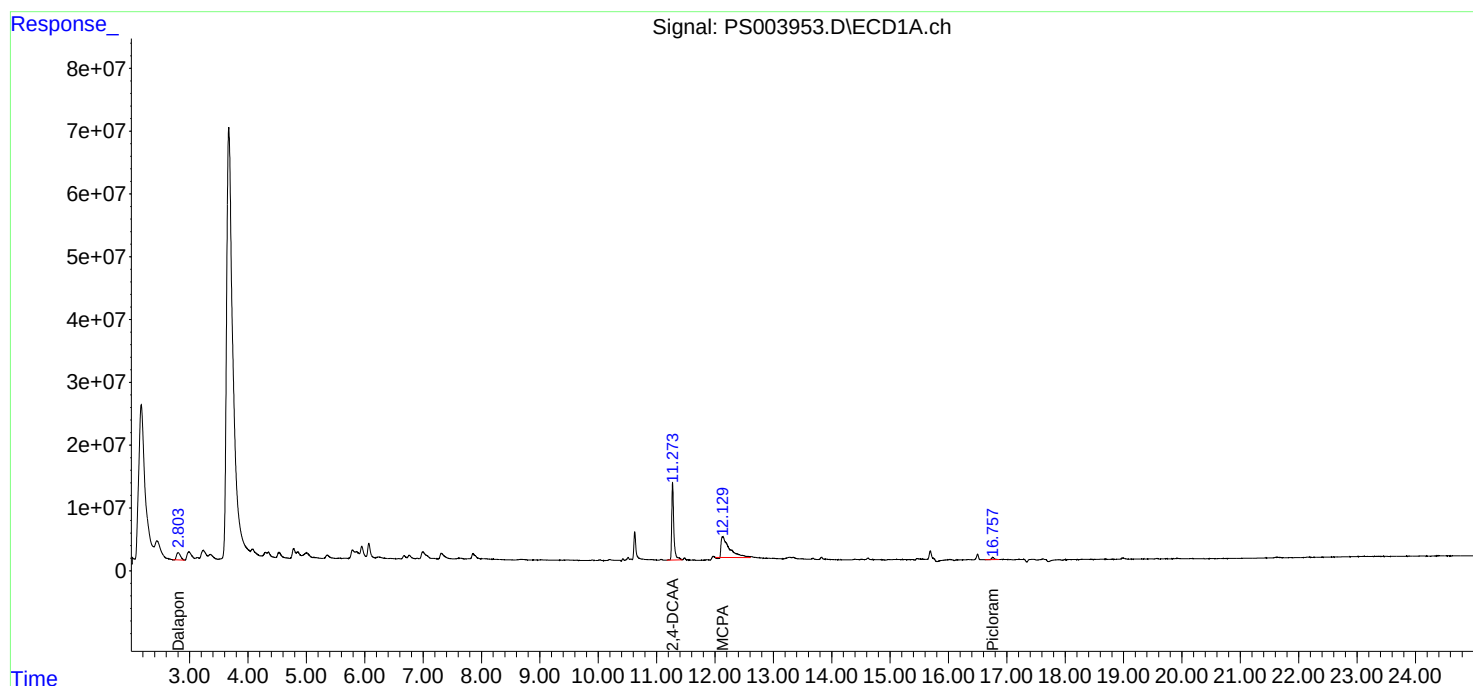


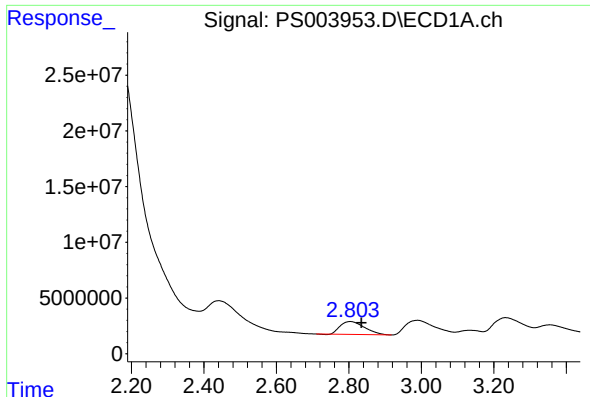

#1 Dalapon


R.T.: 2.804 min
Delta R.T.: -0.031 min
Response: 54369106
Conc: 72.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
S8A-S8B(12-16)COMP

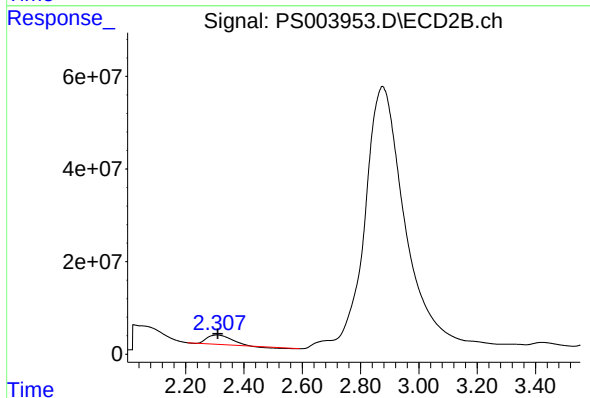


#1 Dalapon

R.T.: 2.307 min
Delta R.T.: -0.004 min
Response: 106448069
Conc: 145.89 ng/ml

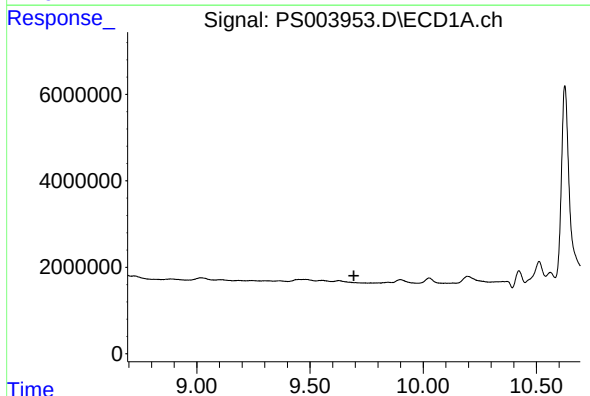


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

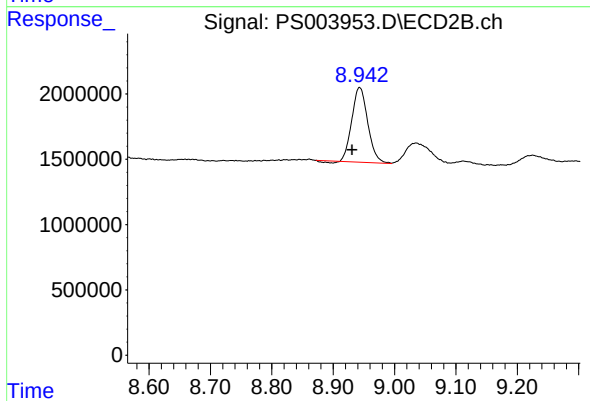

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.943 min
Delta R.T.: 0.012 min
Response: 10162308
Conc: 15.93 ng/ml

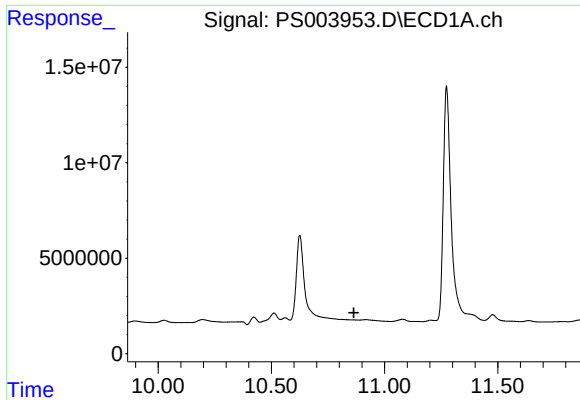

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S8A-S8B(12-16)COMP

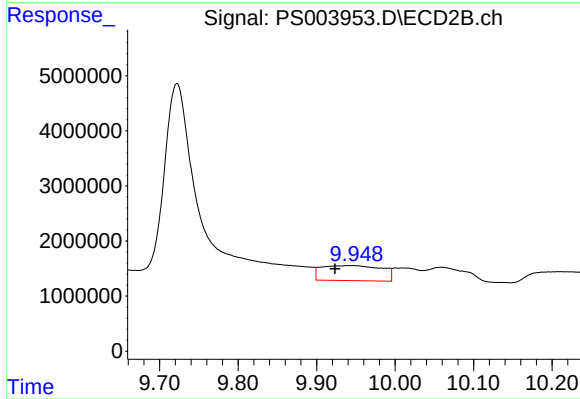


#3 4-Nitrophenol

R.T.: 9.940 min
Delta R.T.: 0.017 min
Response: 14505264
Conc: 63.89 ng/ml

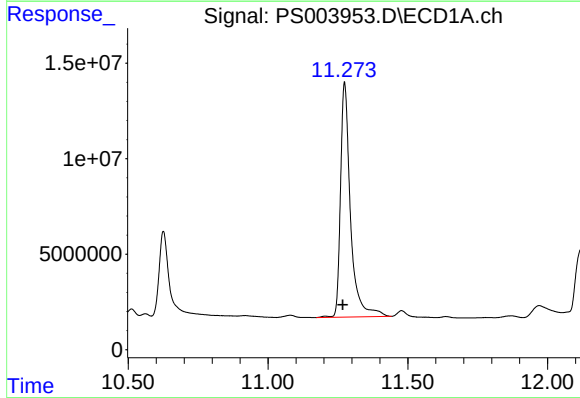


#4 2,4-DCAA

R.T.: 11.274 min
Delta R.T.: 0.007 min
Response: 305488314
Conc: 700.32 ng/ml

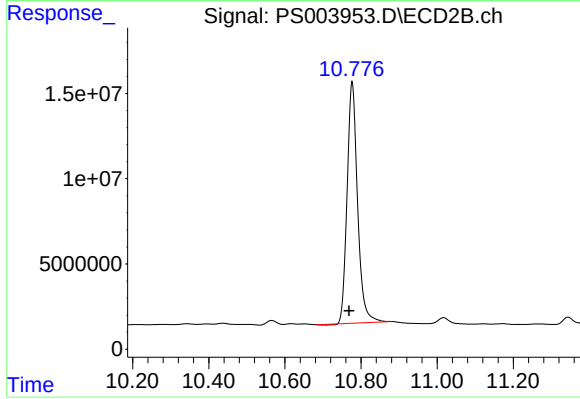

#4 2,4-DCAA


R.T.: 10.776 min
Delta R.T.: 0.008 min
Response: 270022640
Conc: 550.33 ng/ml

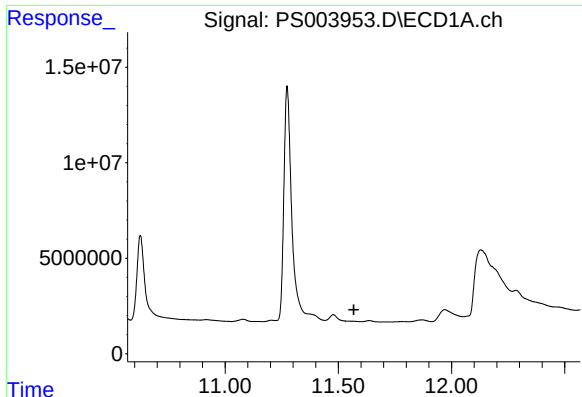

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S8A-S8B(12-16)COMP

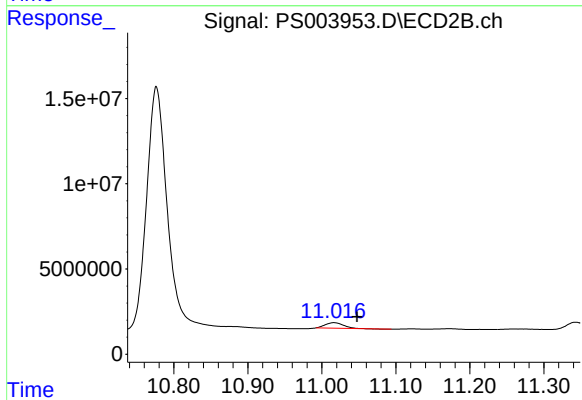


#5 DICAMBA

R.T.: 11.016 min
Delta R.T.: -0.031 min
Response: 5493644
Conc: 2.95 ng/ml

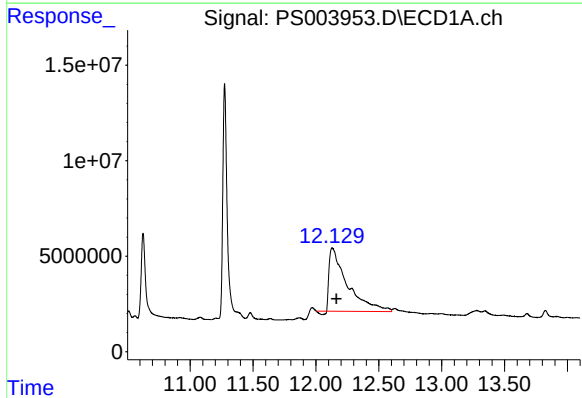


#7 MCPA

R.T.: 12.130 min
Delta R.T.: -0.031 min
Response: 330454048
Conc: 156.63 ug/ml

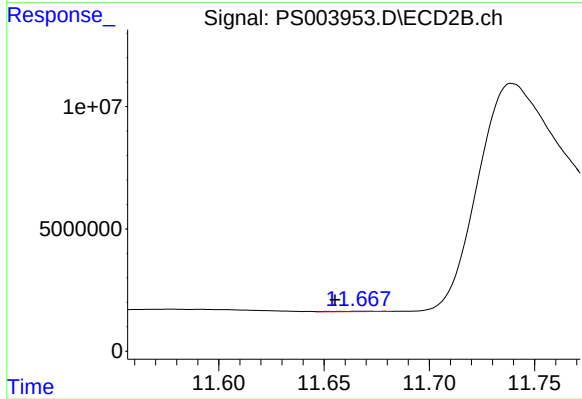

#7 MCPA


R.T.: 11.669 min
Delta R.T.: 0.014 min
Response: 233178
Conc: N.D.

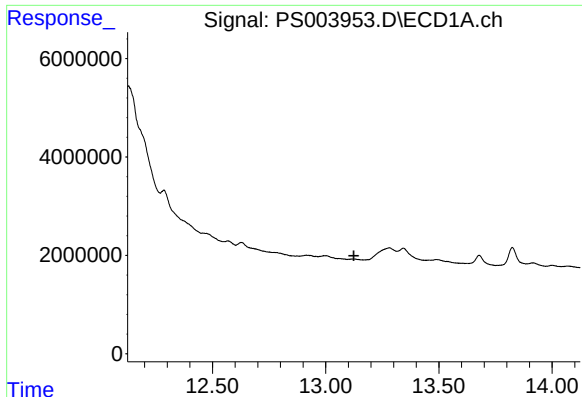

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S8A-S8B(12-16)COMP

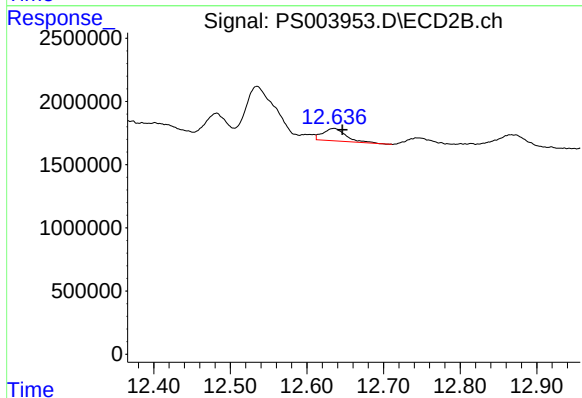


#9 2,4-D

R.T.: 12.635 min
Delta R.T.: -0.012 min
Response: 2043366
Conc: 3.84 ng/ml

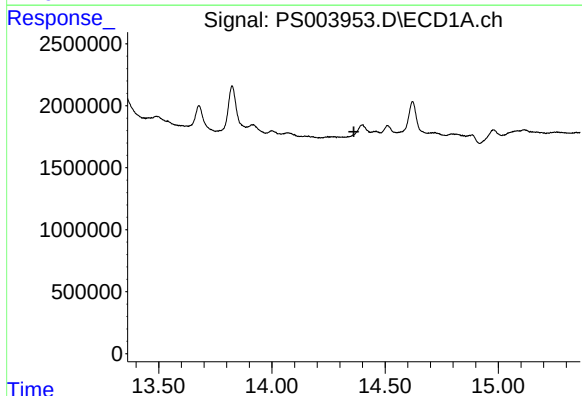


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

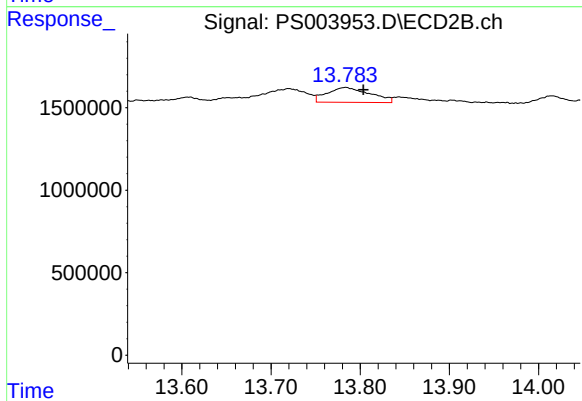

#11 2,4,5-TP (SILVEX)


R.T.: 13.783 min
Delta R.T.: -0.020 min
Response: 3009701
Conc: 1.14 ng/ml

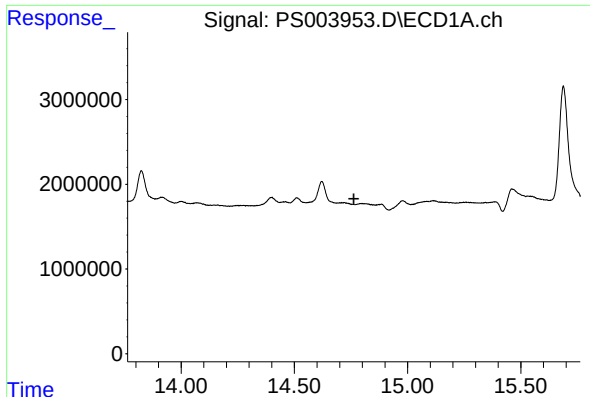

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.763 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S8A-S8B(12-16)COMP

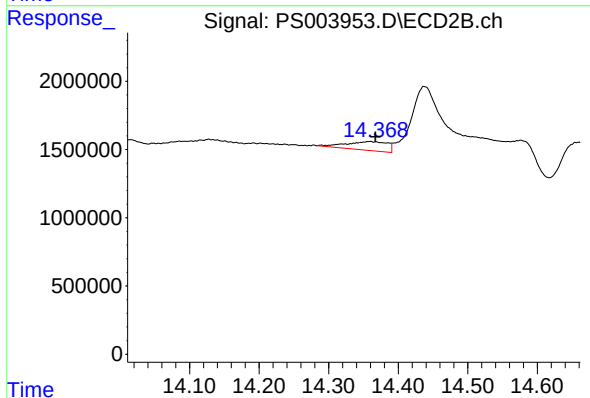


#12 2,4,5-T

R.T.: 14.359 min
Delta R.T.: -0.008 min
Response: 2632946
Conc: 1.21 ng/ml

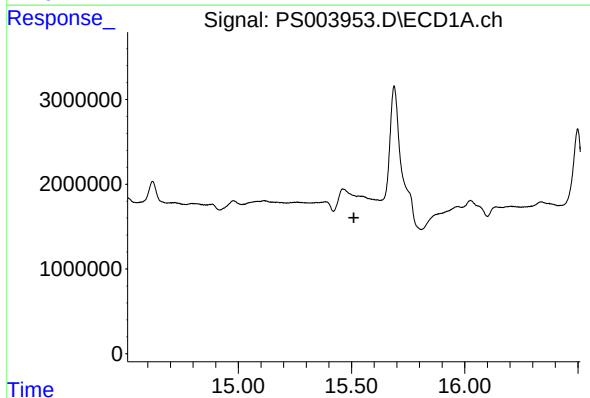


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 15.510 min
Response: 0
Conc: N.D.

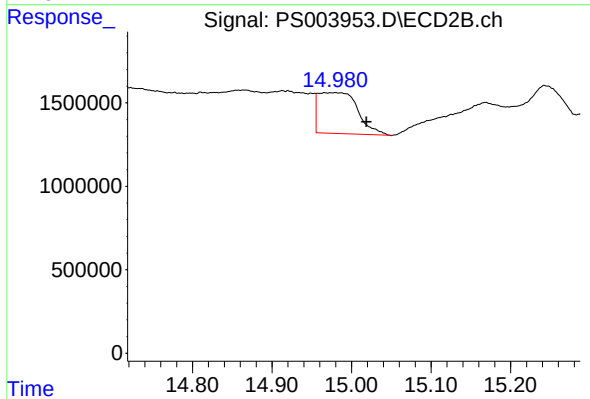

#13 2,4-DB


R.T.: 14.979 min
Delta R.T.: -0.040 min
Response: 8422764
Conc: 28.36 ng/ml

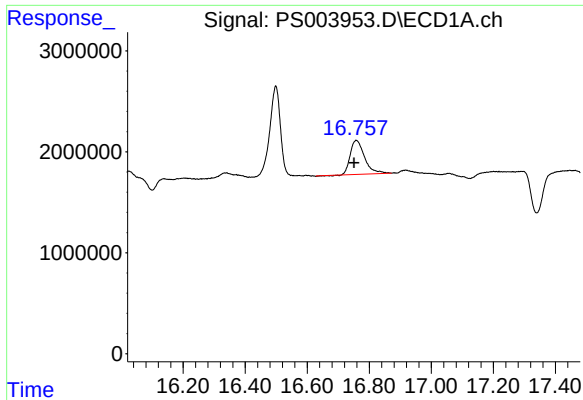

#15 Picloram


R.T.: 16.758 min
Delta R.T.: 0.007 min
Response: 10797208
Conc: 3.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
S8A-S8B(12-16)COMP

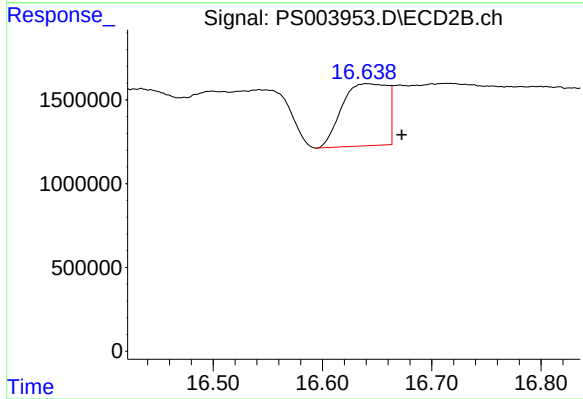


#15 Picloram

R.T.: 16.641 min
Delta R.T.: -0.032 min
Response: 10708962
Conc: 3.38 ng/ml

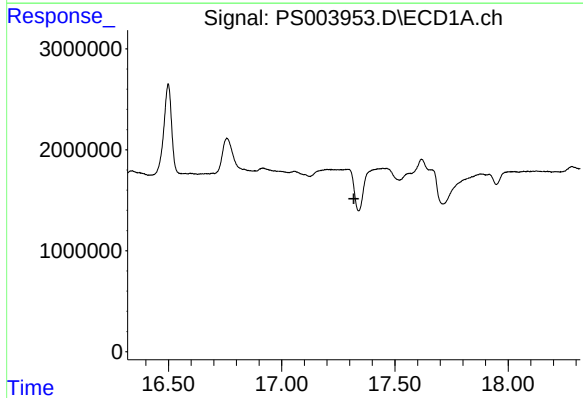

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.319 min
Response: 0
Conc: N.D.

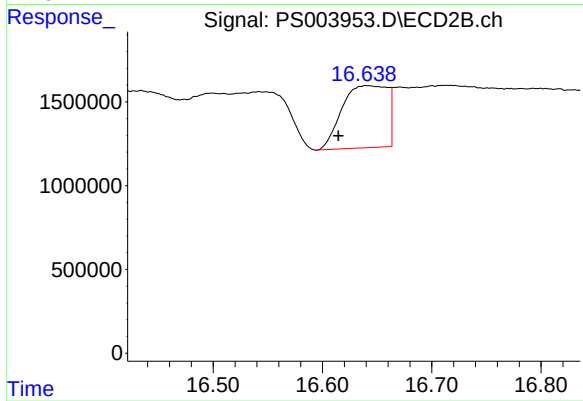

#16 DCPA

R.T.: 16.641 min
Delta R.T.: 0.027 min
Response: 10708962
Conc: 3.17 ng/ml