

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
 Data File : PS003955.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2019 14:14
 Operator : EI\SJ
 Sample : K2182-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 S7C(2-10)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 14:41:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.292	10.794	324.9E6	285.1E6	744.774	581.137
Target Compounds							
1) T	Dalapon	2.822	2.326	56263143	119.2E6	75.467	163.309 #
2) T	3,5-DICHL...	0.000	8.961	0	7415888	N.D.	11.626
3) T	4-Nitroph...	0.000	9.940	0	17321918	N.D.	76.296
5) T	DICAMBA	0.000	11.035	0	6592653	N.D.	3.545
6) T	MCPD	0.000	11.277	0	593233	N.D.	<MDL
7) T	MCPA	12.172	11.589	222.6E6	8810062	105.496	4.940 #
9) T	2,4-D	0.000	12.652	0	2054674	N.D.	3.863
10) T	Pentachlo...	0.000	13.200	0	686179	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.802	0	3518274	N.D.	1.328
12) T	2,4,5-T	0.000	14.366	0	6188022	N.D.	2.847
13) T	2,4-DB	0.000	14.994	0	8968460	N.D.	30.202
15) T	Picloram	16.759	16.653	77385679	13130151	22.780	4.140 #
16) T	DCPA	0.000	16.653	0	13130151	N.D.	3.885



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
Data File : PS003955.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2019 14:14
Operator : EI\SJ
Sample : K2182-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
S7C(2-10)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 14:41:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

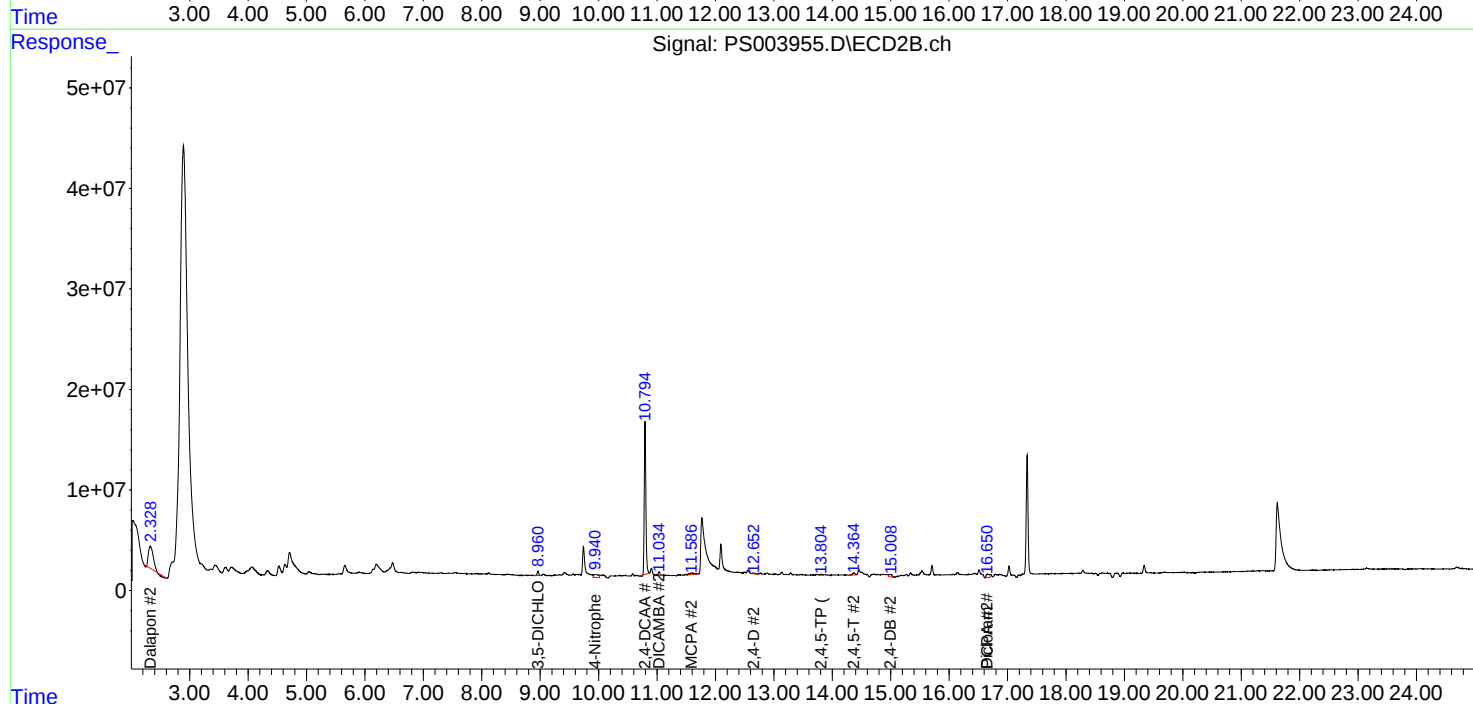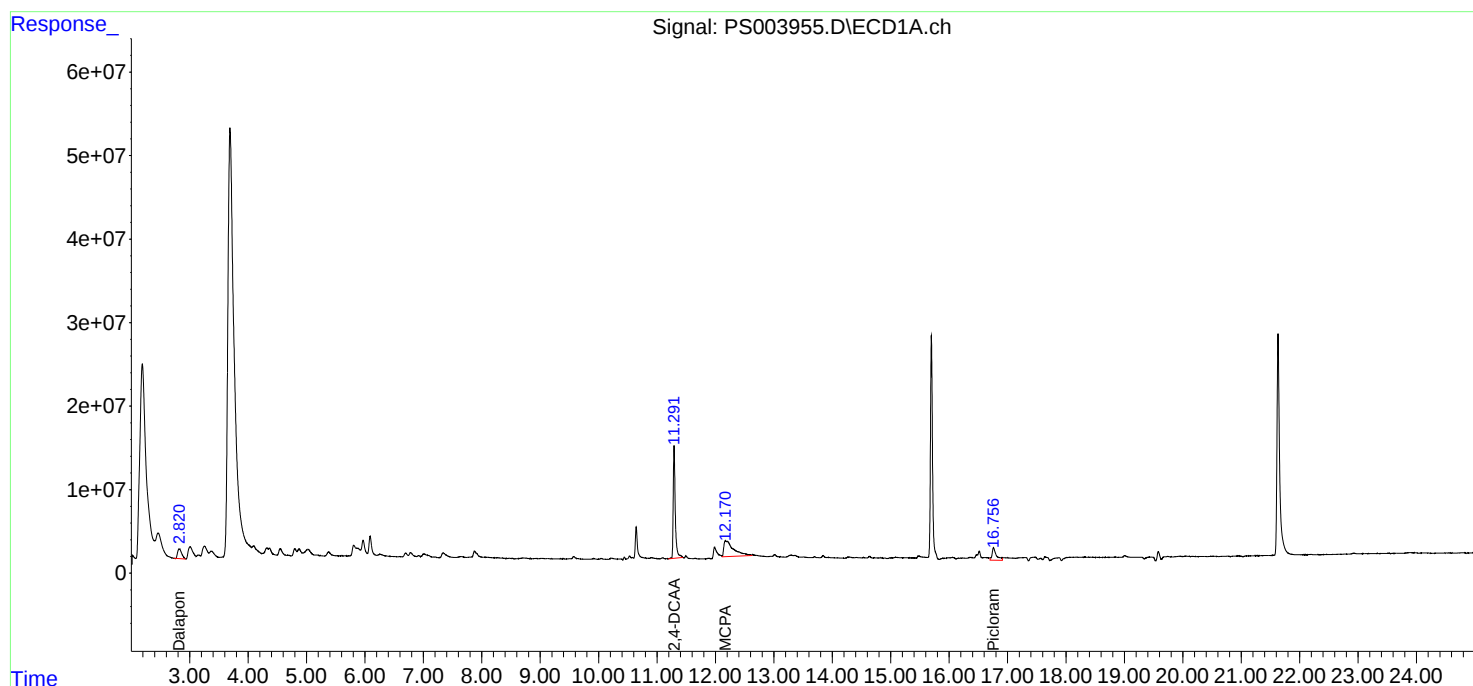


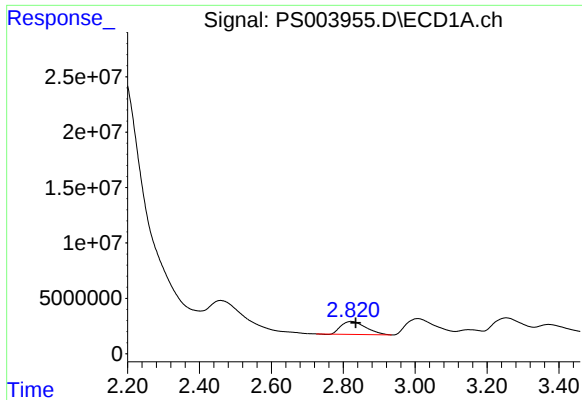

#1 Dalapon


R.T.: 2.822 min
Delta R.T.: -0.013 min
Response: 56263143
Conc: 75.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
S7C(2-10)COMP

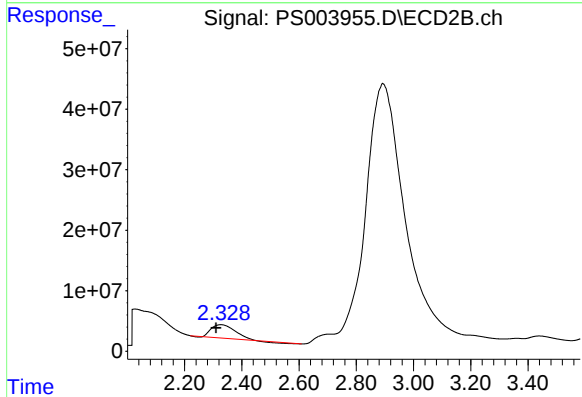


#1 Dalapon

R.T.: 2.326 min
Delta R.T.: 0.016 min
Response: 119154774
Conc: 163.31 ng/ml

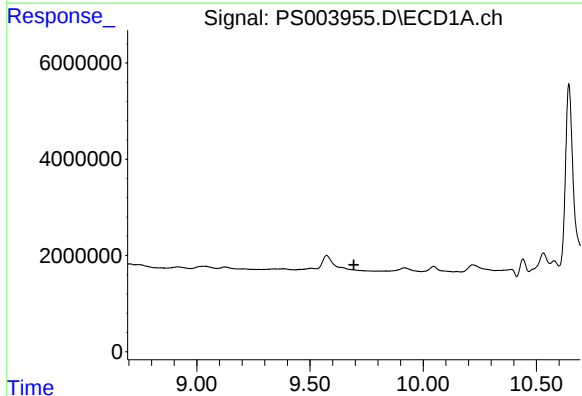


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

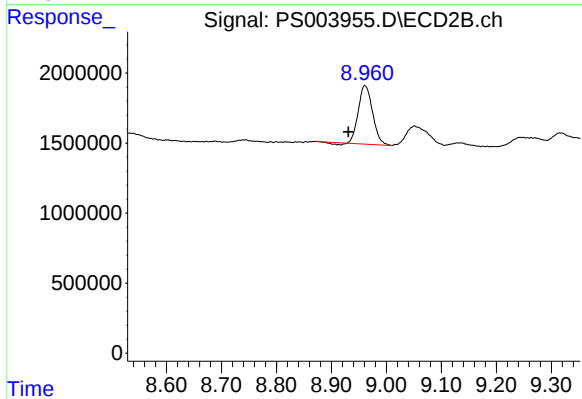

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.961 min
Delta R.T.: 0.030 min
Response: 7415888
Conc: 11.63 ng/ml

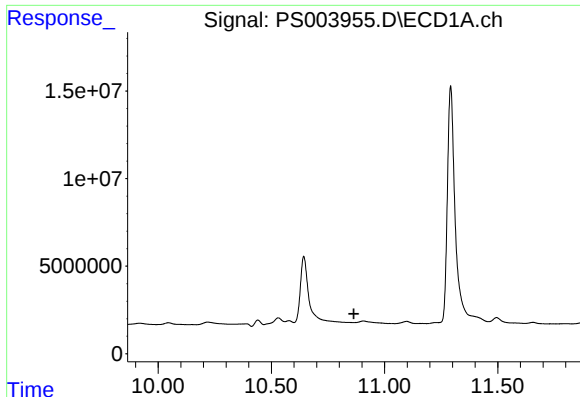

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S7C(2-10)COMP

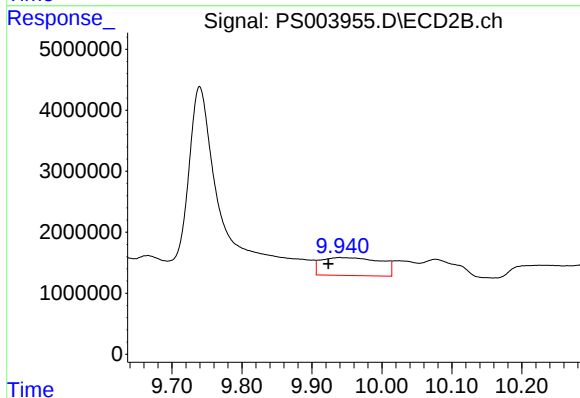


#3 4-Nitrophenol

R.T.: 9.940 min
Delta R.T.: 0.016 min
Response: 17321918
Conc: 76.30 ng/ml

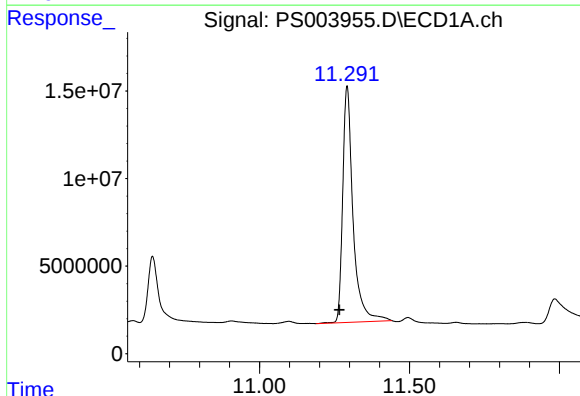


#4 2,4-DCAA

R.T.: 11.292 min
Delta R.T.: 0.025 min
Response: 324879466
Conc: 744.77 ng/ml

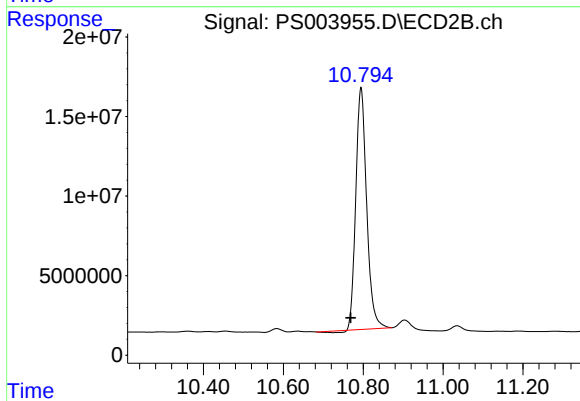

#4 2,4-DCAA


R.T.: 10.794 min
Delta R.T.: 0.026 min
Response: 285139527
Conc: 581.14 ng/ml

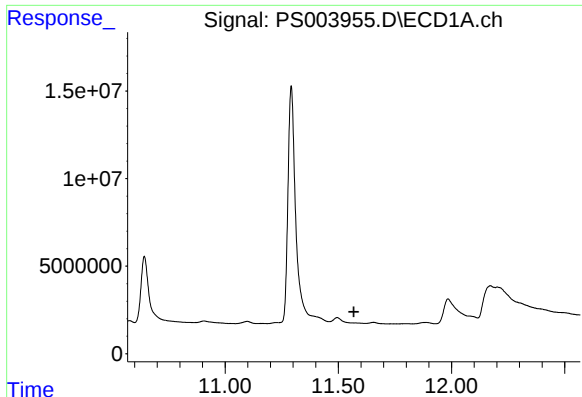

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S7C(2-10)COMP

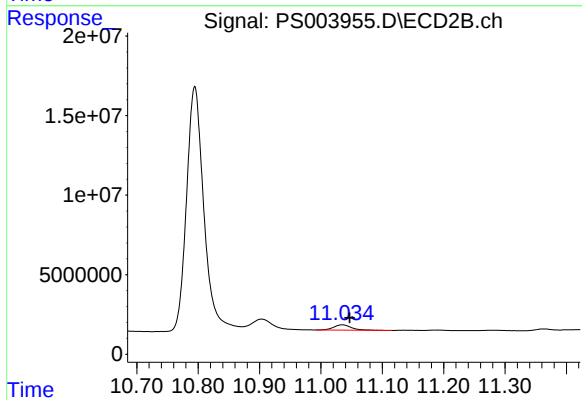


#5 DICAMBA

R.T.: 11.035 min
Delta R.T.: -0.013 min
Response: 6592653
Conc: 3.54 ng/ml

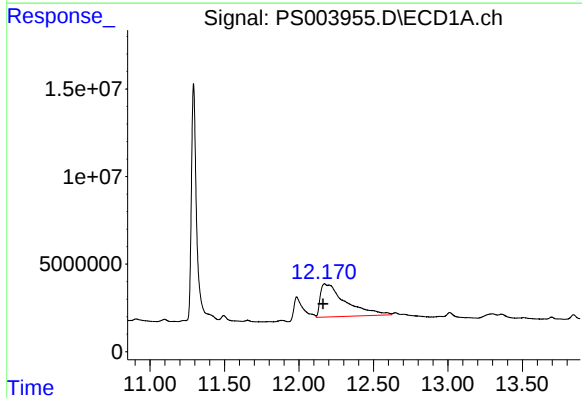


#7 MCPA

R.T.: 12.172 min
Delta R.T.: 0.010 min
Response: 222574341
Conc: 105.50 ug/ml

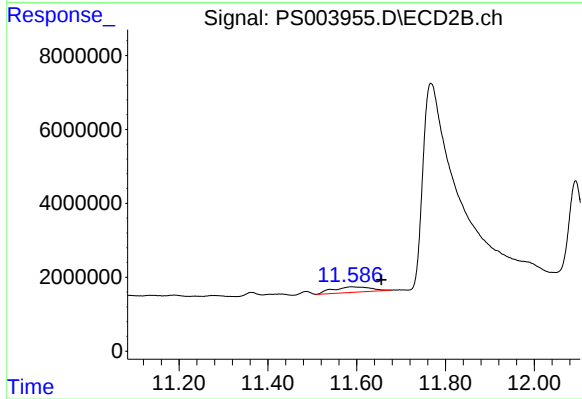

#7 MCPA


R.T.: 11.589 min
Delta R.T.: -0.066 min
Response: 8810062
Conc: 4.94 ug/ml

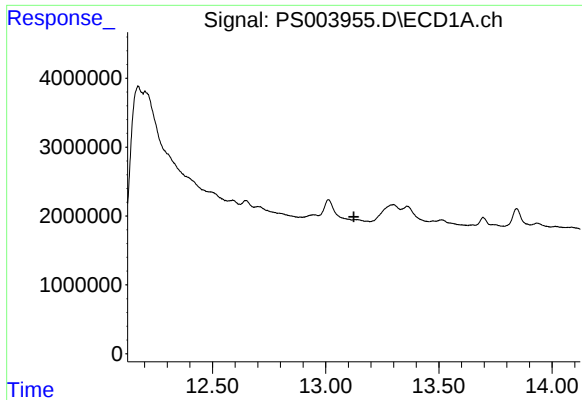

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S7C(2-10)COMP

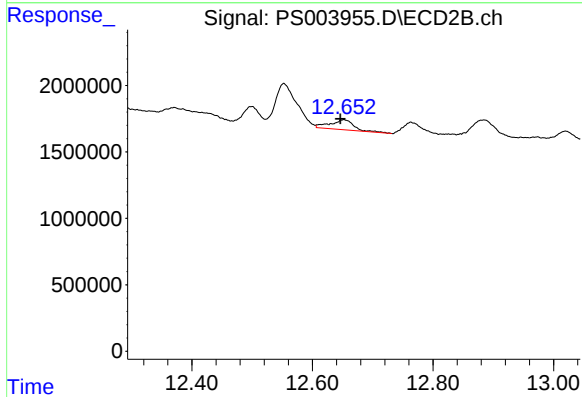


#9 2,4-D

R.T.: 12.652 min
Delta R.T.: 0.006 min
Response: 2054674
Conc: 3.86 ng/ml

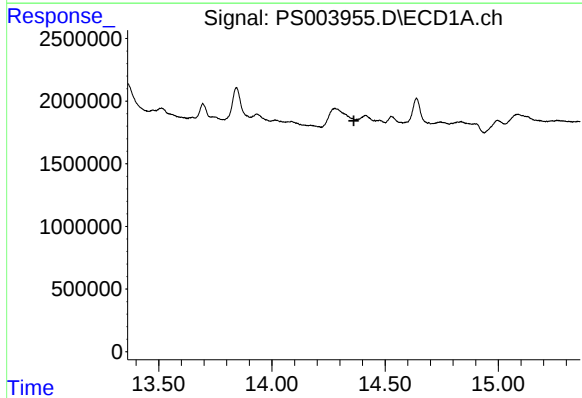


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

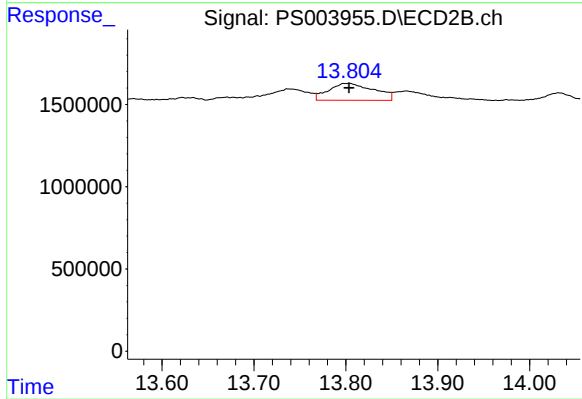

#11 2,4,5-TP (SILVEX)


R.T.: 13.802 min
Delta R.T.: -0.001 min
Response: 3518274
Conc: 1.33 ng/ml

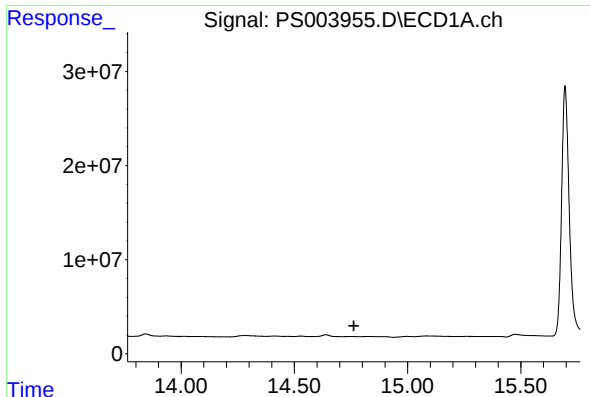

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S7C(2-10)COMP

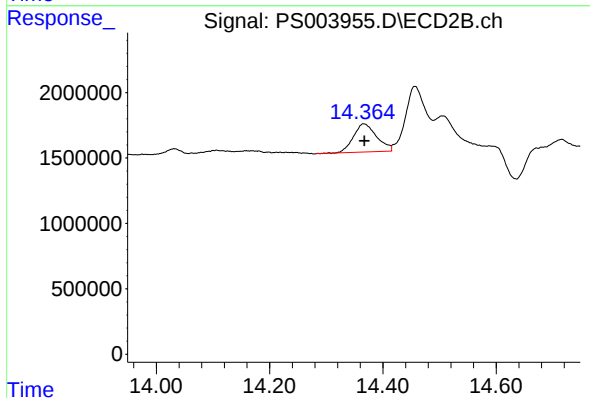


#12 2,4,5-T

R.T.: 14.366 min
Delta R.T.: 0.000 min
Response: 6188022
Conc: 2.85 ng/ml

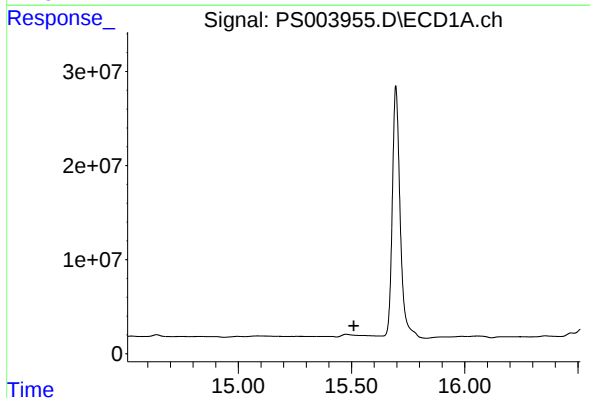


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

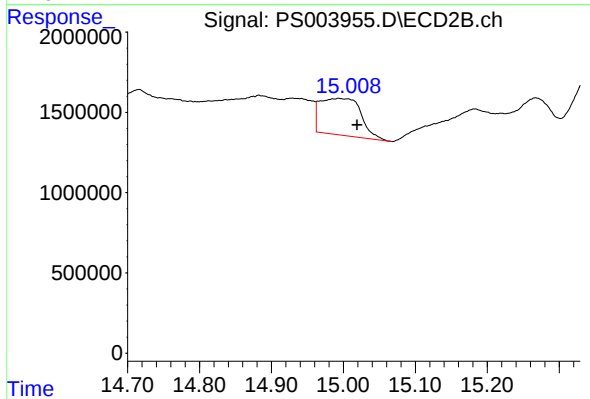

#13 2,4-DB


R.T.: 14.994 min
Delta R.T.: -0.025 min
Response: 8968460
Conc: 30.20 ng/ml

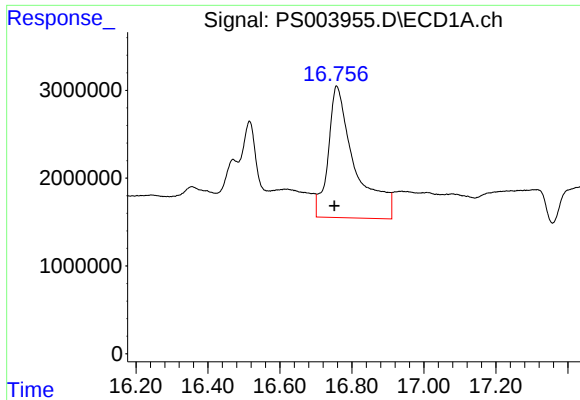

#15 Picloram


R.T.: 16.759 min
Delta R.T.: 0.007 min
Response: 77385679
Conc: 22.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
S7C(2-10)COMP

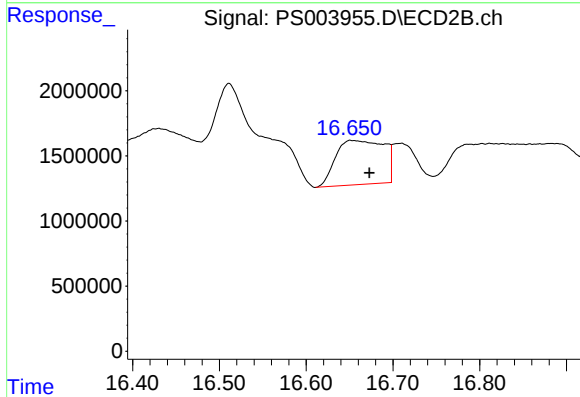


#15 Picloram

R.T.: 16.653 min
Delta R.T.: -0.020 min
Response: 13130151
Conc: 4.14 ng/ml

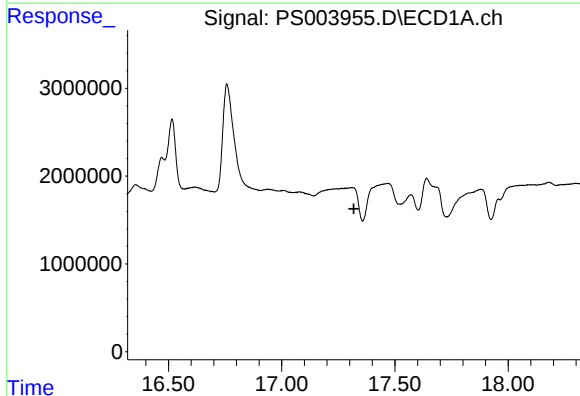

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.319 min
Response: 0
Conc: N.D.

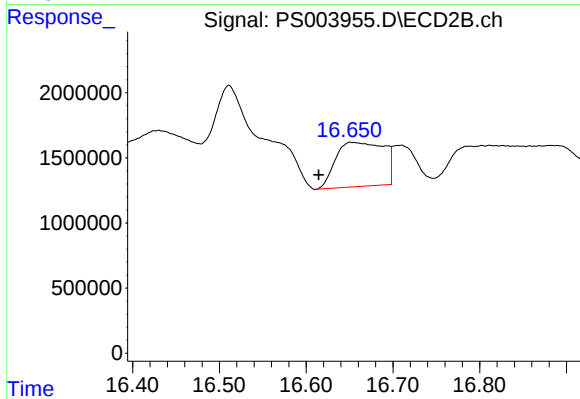

#16 DCPA

R.T.: 16.653 min
Delta R.T.: 0.039 min
Response: 13130151
Conc: 3.88 ng/ml