

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
 Data File : PS003957.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2019 15:21
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 16:47:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.294	10.792	228.9E6	209.1E6	524.832	426.157
Target Compounds							
3) T	4-Nitroph...	0.000	9.936	0	305128	N.D.	1.344
6) T	MCCP	0.000	11.266	0	18716	N.D.	<MDL
7) T	MCPA	0.000	11.615	0	19956089	N.D.	11.190
8) T	DICHLORPROP	0.000	12.167	0	1671903	N.D.	3.591
9) T	2,4-D	0.000	12.615	0	751309	N.D.	1.412
10) T	Pentachlo...	0.000	13.207	0	1143812	N.D.	<MDL
12) T	2,4,5-T	0.000	14.386	0	113959	N.D.	<MDL
13) T	2,4-DB	0.000	14.955	0	17676131	N.D.	59.526
15) T	Picloram	0.000	16.644	0	3456652	N.D.	1.090
16) T	DCPA	0.000	16.644	0	3456652	N.D.	1.023



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
Data File : PS003957.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2019 15:21
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 16:47:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

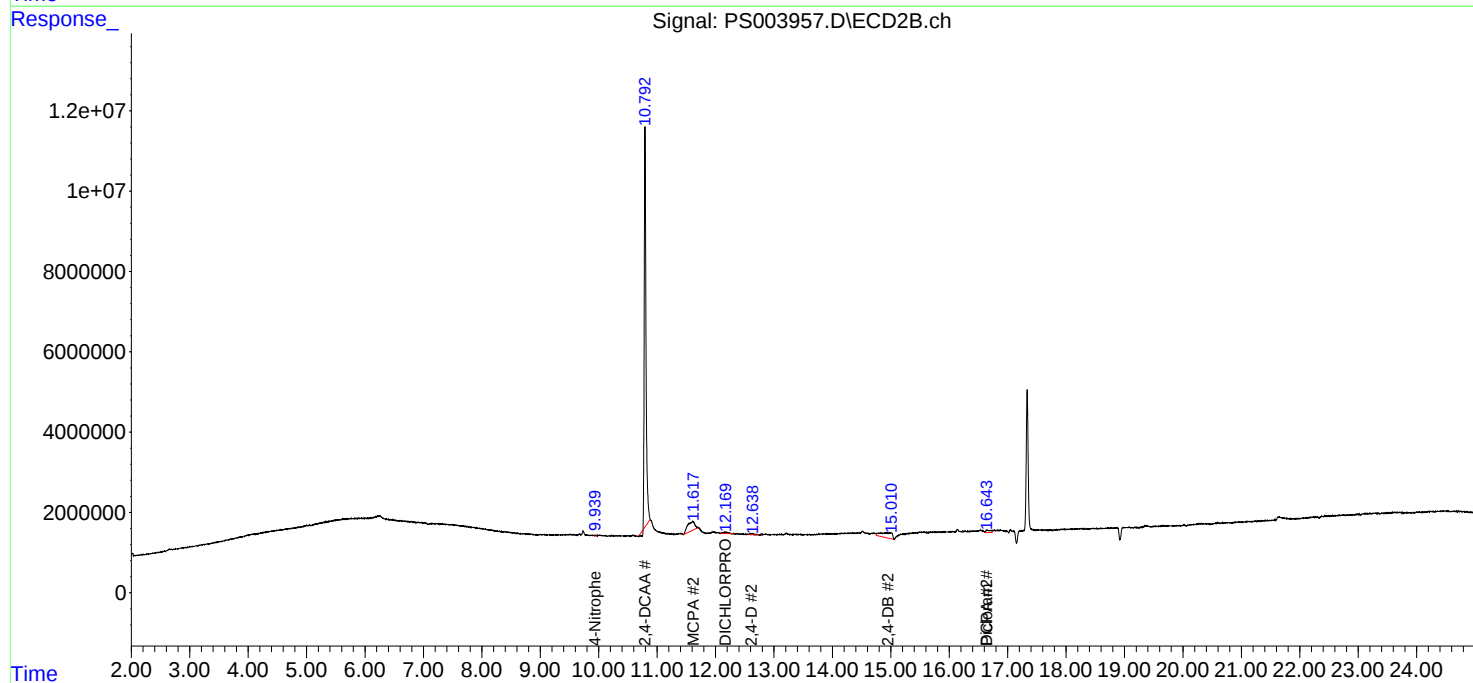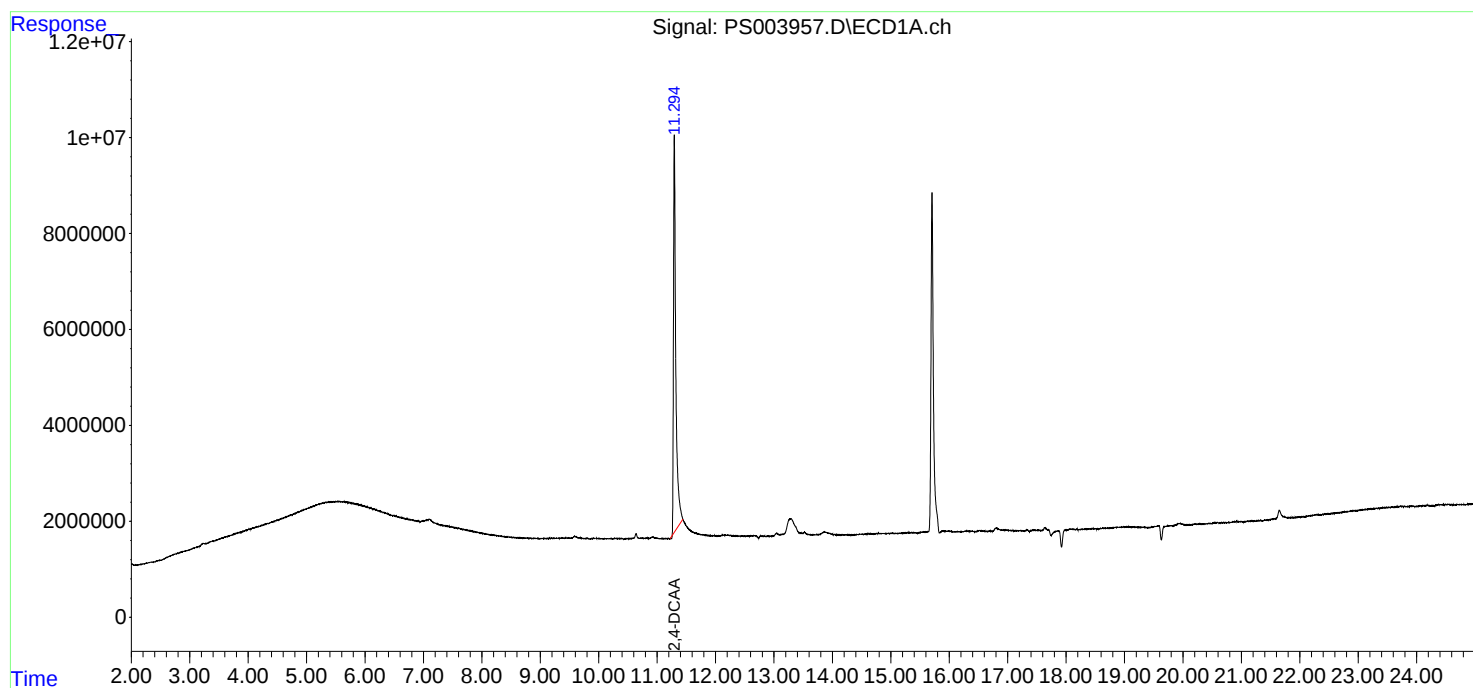


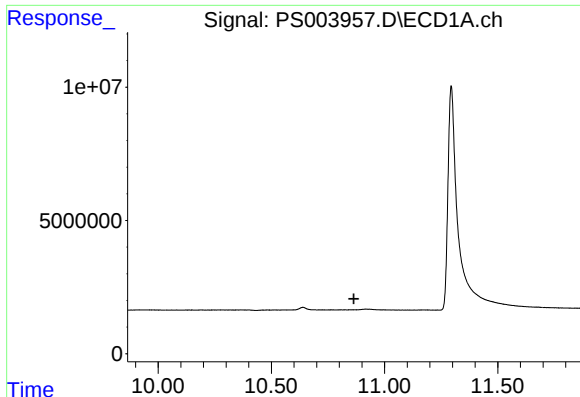

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

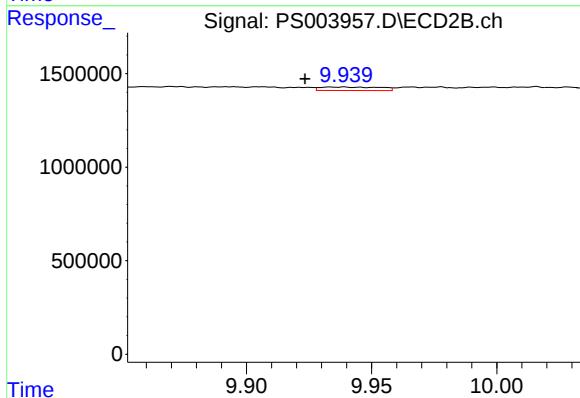


#3 4-Nitrophenol

R.T.: 9.936 min
Delta R.T.: 0.013 min
Response: 305128
Conc: 1.34 ng/ml

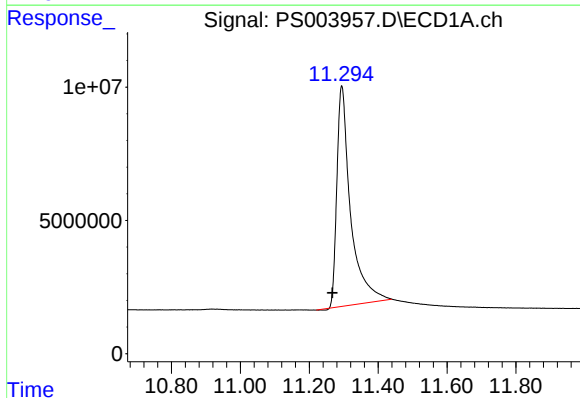


#4 2,4-DCAA

R.T.: 11.294 min
Delta R.T.: 0.028 min
Response: 228938060
Conc: 524.83 ng/ml

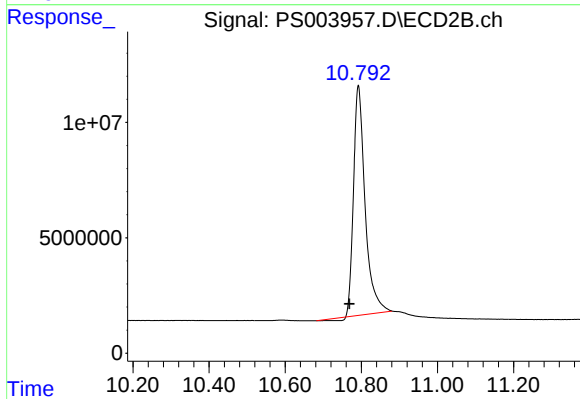

#4 2,4-DCAA


R.T.: 10.792 min
Delta R.T.: 0.024 min
Response: 209097724
Conc: 426.16 ng/ml

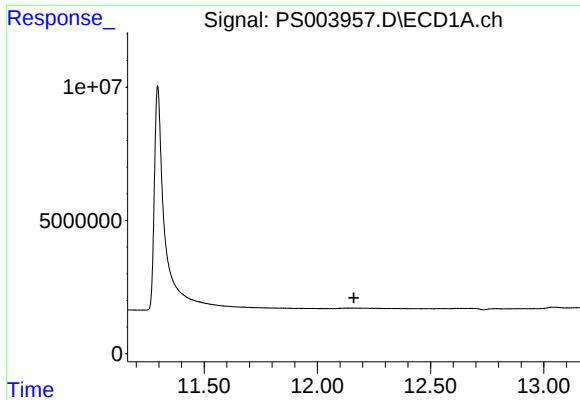

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

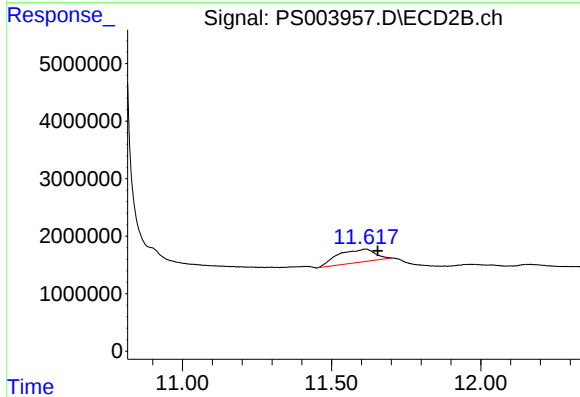


#7 MCPA

R.T.: 11.615 min
Delta R.T.: -0.040 min
Response: 19956089
Conc: 11.19 ug/ml

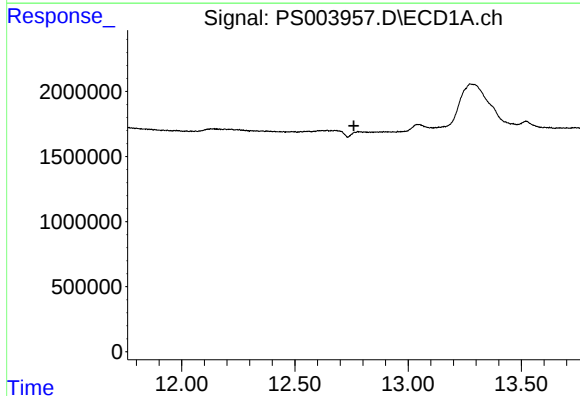


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.760 min
Response: 0
Conc: N.D.

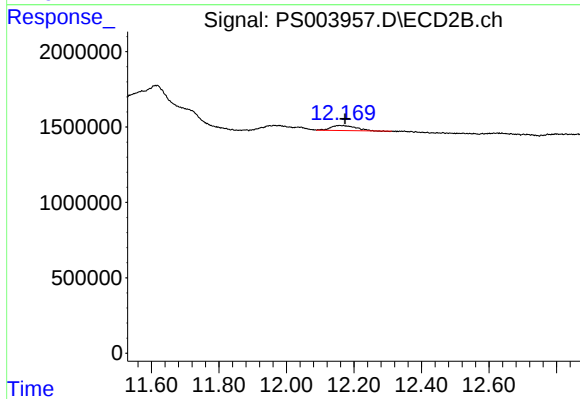

#8 DICHLORPROP


R.T.: 12.167 min
Delta R.T.: -0.006 min
Response: 1671903
Conc: 3.59 ng/ml

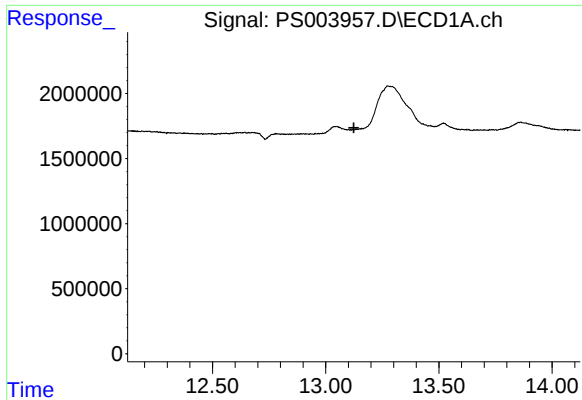

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

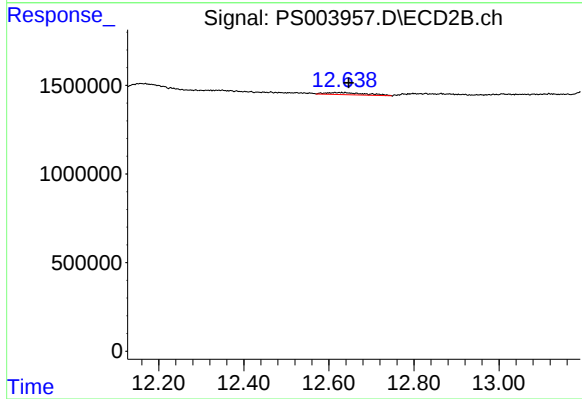


#9 2,4-D

R.T.: 12.615 min
Delta R.T.: -0.032 min
Response: 751309
Conc: 1.41 ng/ml

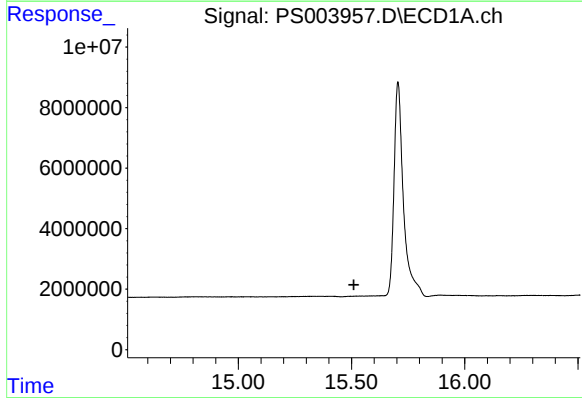


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

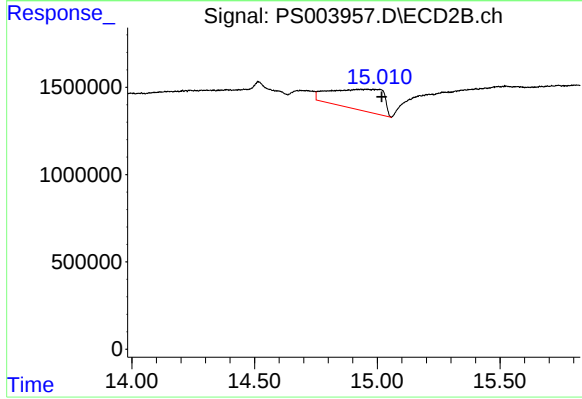

#13 2,4-DB


R.T.: 14.955 min
Delta R.T.: -0.063 min
Response: 17676131
Conc: 59.53 ng/ml

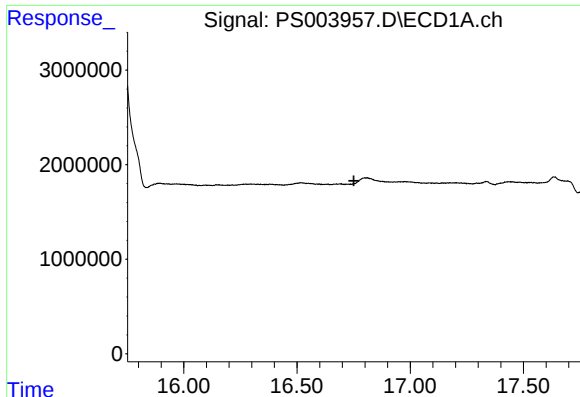

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

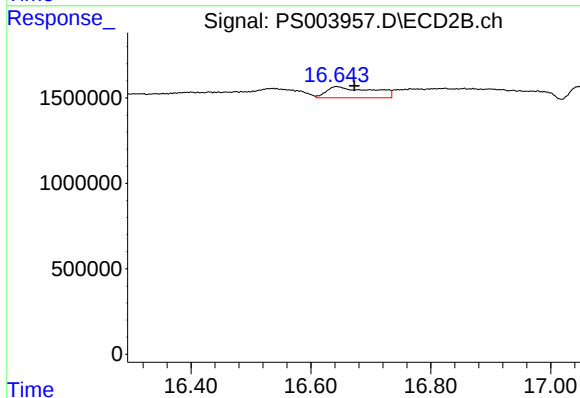


#15 Picloram

R.T.: 16.644 min
Delta R.T.: -0.029 min
Response: 3456652
Conc: 1.09 ng/ml

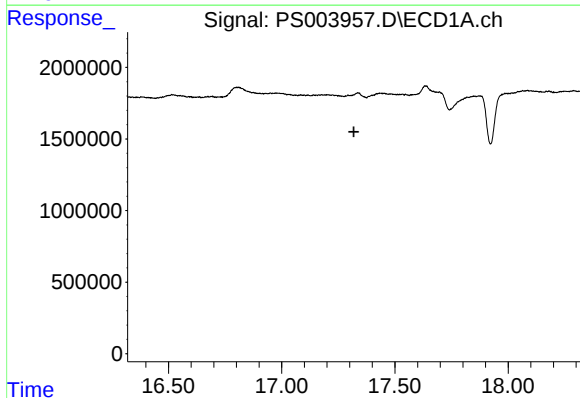

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.319 min
Response: 0
Conc: N.D.

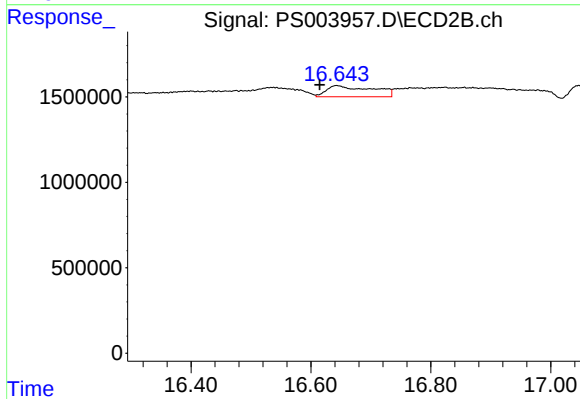

#16 DCPA

R.T.: 16.644 min
Delta R.T.: 0.029 min
Response: 3456652
Conc: 1.02 ng/ml