

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
 Data File : PS003963.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2019 19:02
 Operator : EI\SJ
 Sample : K2186-18
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 03:13:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.291	10.795	344.4E6	308.2E6	789.545	628.145
Target Compounds							
1) T	Dalapon	2.822	2.315	6895326	-3405211	9.249	N.D. #
2) T	3,5-DICHL...	0.000	8.962	0	5105655	N.D.	8.004
3) T	4-Nitroph...	0.000	9.960	0	22313366	N.D.	98.282
5) T	DICAMBA	0.000	11.036	0	6503530	N.D.	3.497
6) T	MCP	0.000	11.320	0	1544722	N.D.	1.308
7) T	MCPA	12.168	11.687	191.6E6	398729	90.811	<MDL #
9) T	2,4-D	0.000	12.653	0	1738923	N.D.	3.269
10) T	Pentachlo...	13.512	13.204	6223744	2621009	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	13.800	0	2826335	N.D.	1.067
12) T	2,4,5-T	0.000	14.376	0	1995064	N.D.	<MDL
13) T	2,4-DB	15.480	0.000	3980139	0	13.201	N.D. #
15) T	Picloram	16.774	16.656	11578210	10390736	3.408	3.277
16) T	DCPA	0.000	16.656	0	10390736	N.D.	3.074



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
Data File : PS003963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2019 19:02
Operator : EI\SJ
Sample : K2186-18
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 03:13:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

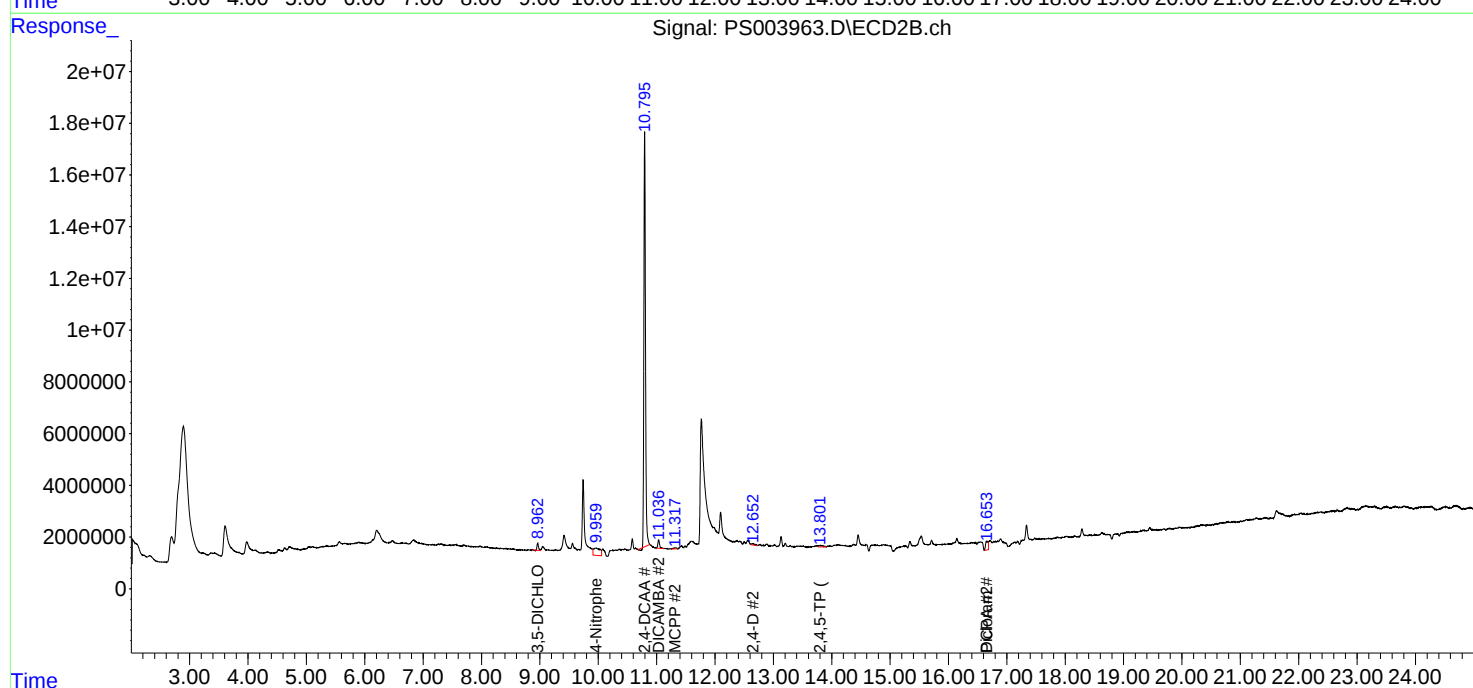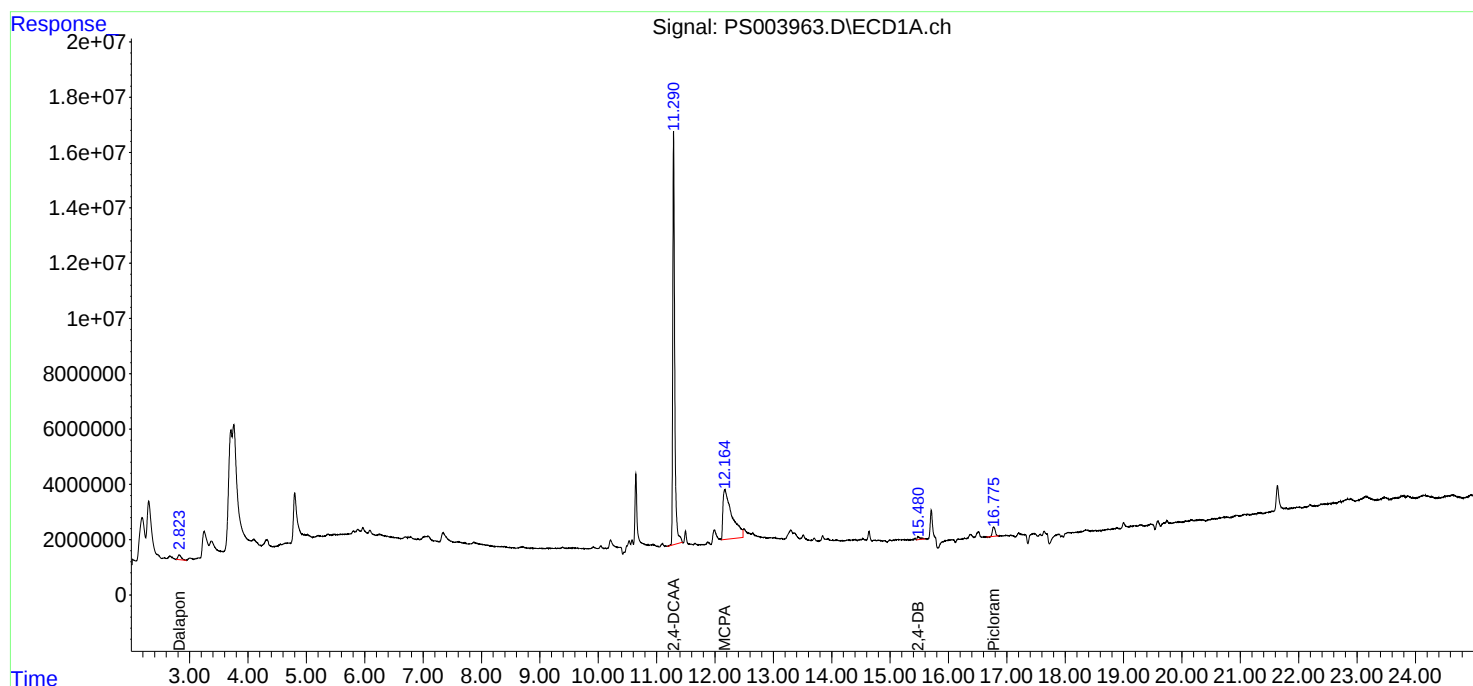


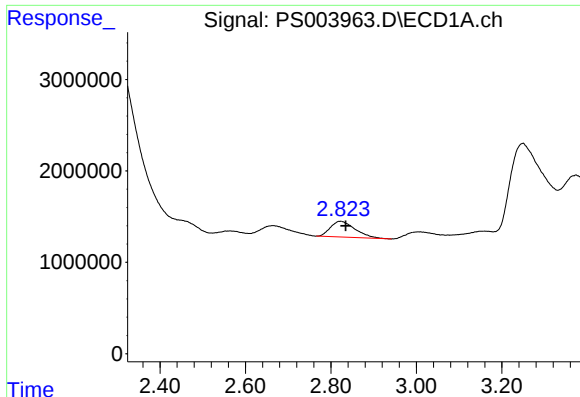

#1 Dalapon


R.T.: 2.822 min
Delta R.T.: -0.013 min
Response: 6895326
Conc: 9.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

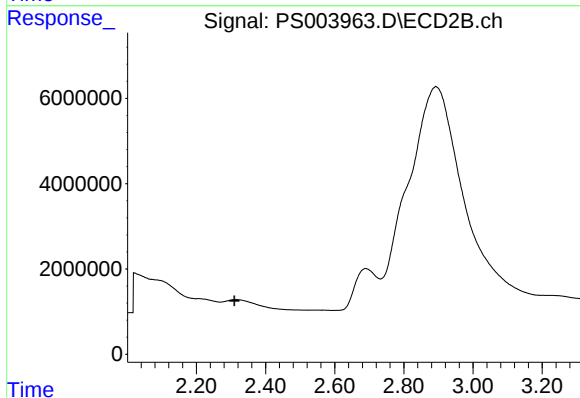


#1 Dalapon

R.T.: 2.315 min
Delta R.T.: 0.005 min
Response: -3405211
Conc: N.D.

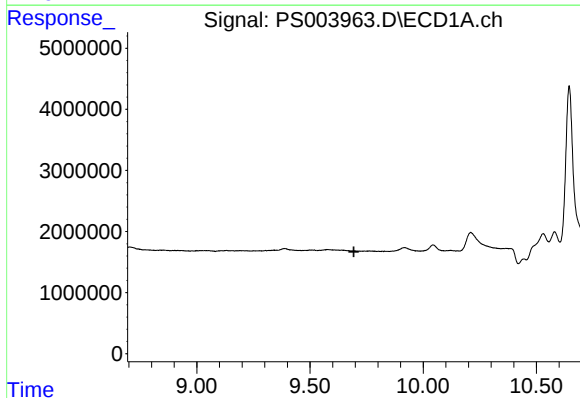


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

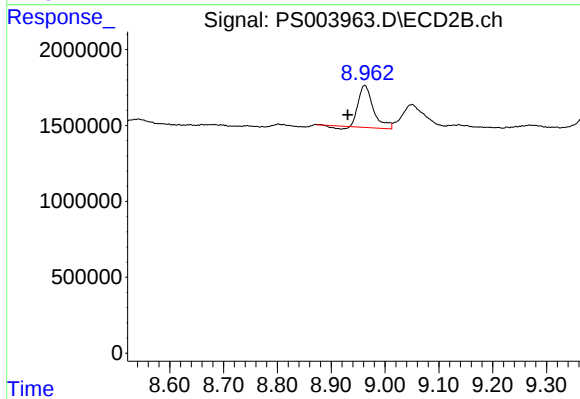

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.962 min
Delta R.T.: 0.031 min
Response: 5105655
Conc: 8.00 ng/ml

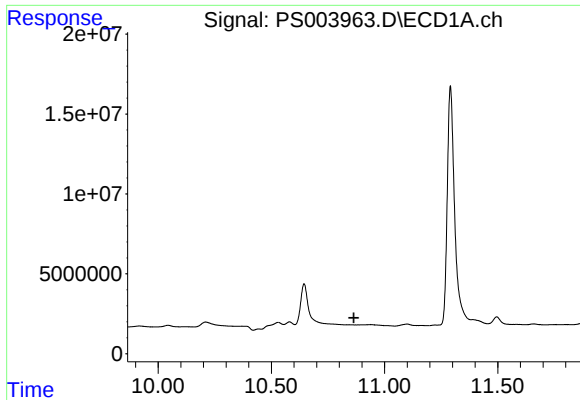

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

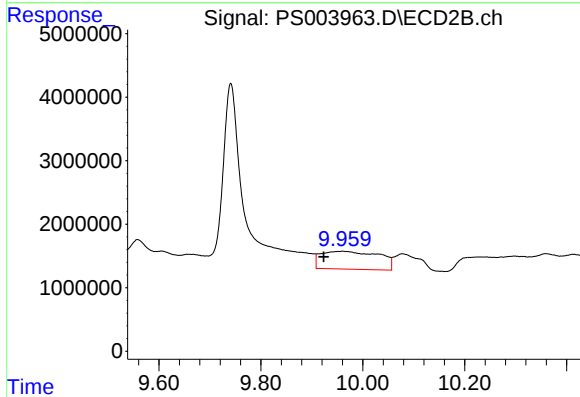


#3 4-Nitrophenol

R.T.: 9.960 min
Delta R.T.: 0.036 min
Response: 22313366
Conc: 98.28 ng/ml

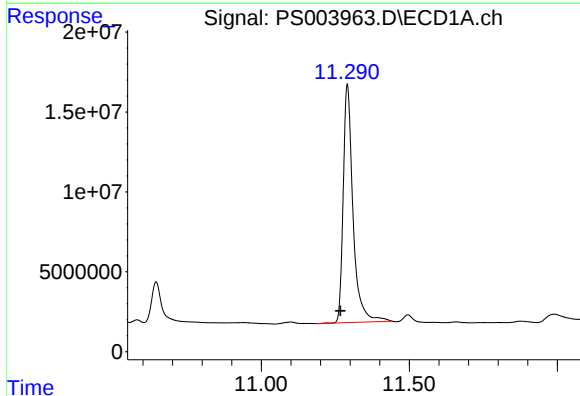


#4 2,4-DCAA

R.T.: 11.291 min
Delta R.T.: 0.024 min
Response: 344409479
Conc: 789.55 ng/ml

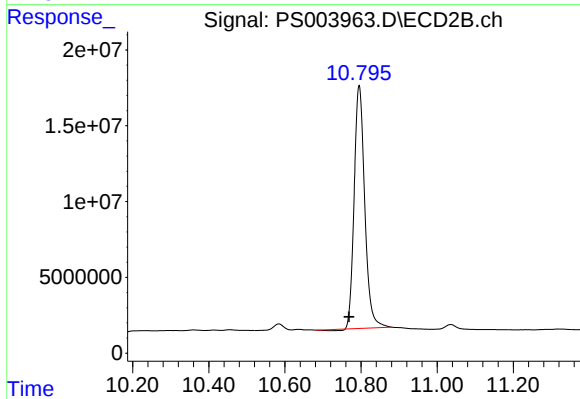

#4 2,4-DCAA


R.T.: 10.795 min
Delta R.T.: 0.026 min
Response: 308204751
Conc: 628.15 ng/ml

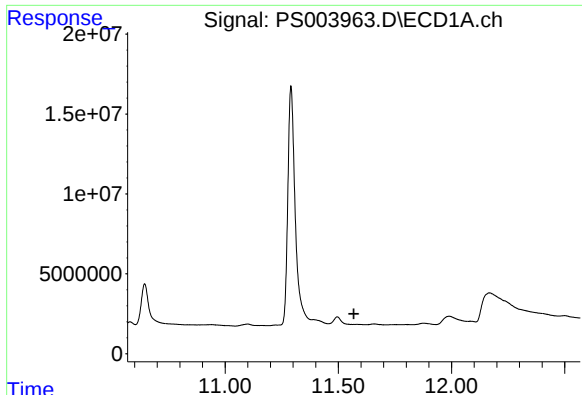

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

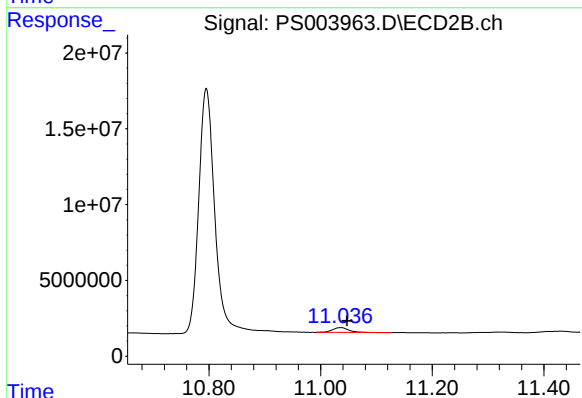


#5 DICAMBA

R.T.: 11.036 min
Delta R.T.: -0.012 min
Response: 6503530
Conc: 3.50 ng/ml

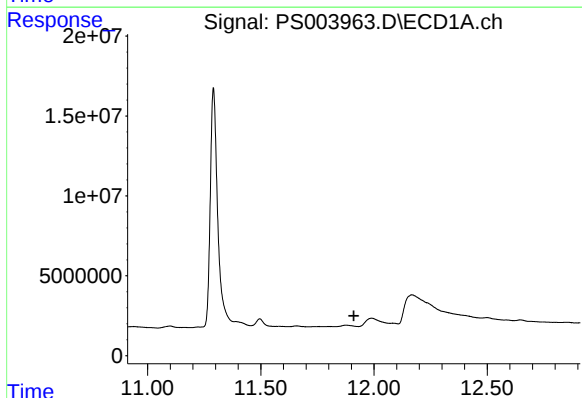


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 11.911 min
Response: 0
Conc: N.D.

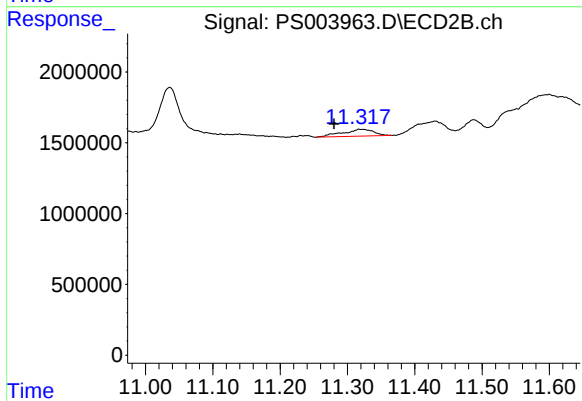

#6 MCPP


R.T.: 11.320 min
Delta R.T.: 0.040 min
Response: 1544722
Conc: 1.31 ug/ml

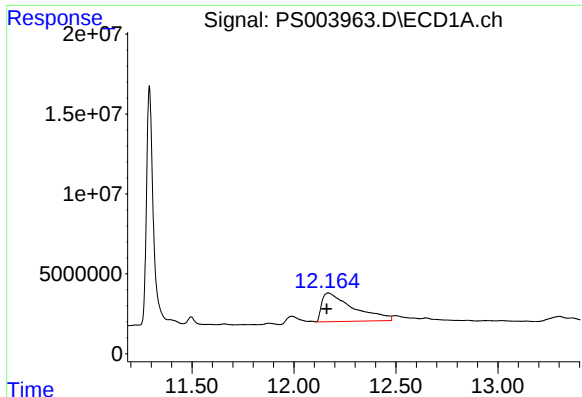

#7 MCPA


R.T.: 12.168 min
Delta R.T.: 0.006 min
Response: 191591233
Conc: 90.81 ug/ml

Instrument :
ECD_S
ClientSampleId :

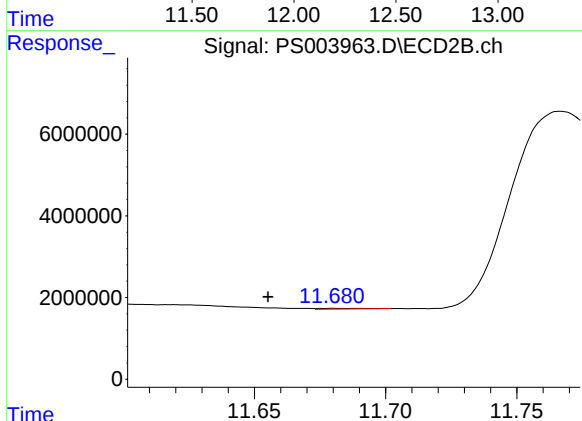


#7 MCPA

R.T.: 11.687 min
Delta R.T.: 0.032 min
Response: 398729
Conc: N.D.

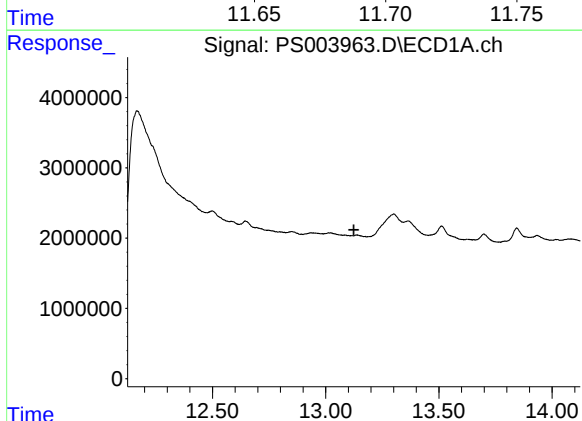


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.125 min
Response: 0
Conc: N.D.

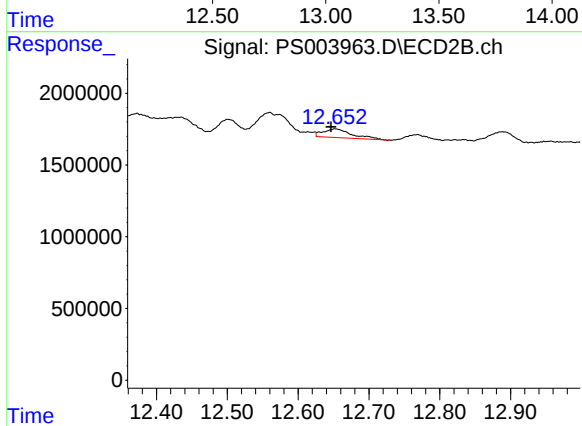

#9 2,4-D


R.T.: 12.653 min
Delta R.T.: 0.006 min
Response: 1738923
Conc: 3.27 ng/ml

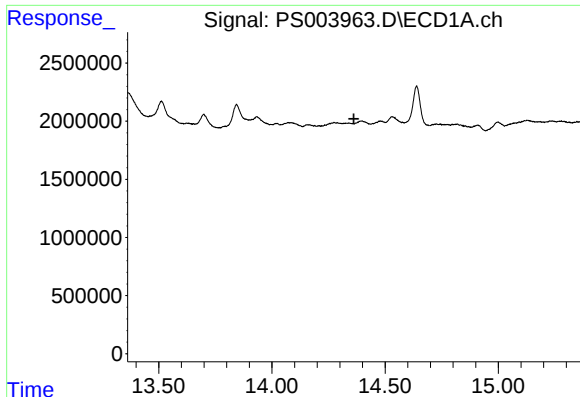

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

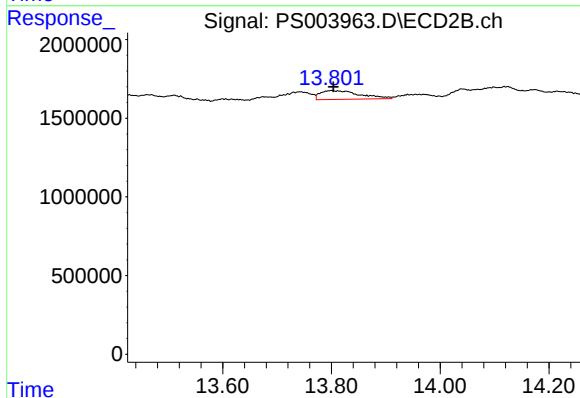


#11 2,4,5-TP (SILVEX)

R.T.: 13.800 min
Delta R.T.: -0.003 min
Response: 2826335
Conc: 1.07 ng/ml

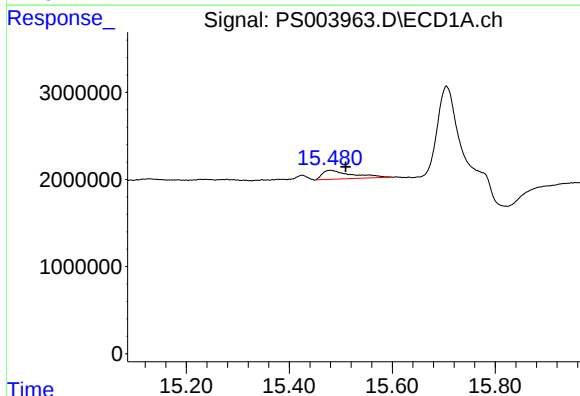


#13 2,4-DB

R.T.: 15.480 min
Delta R.T.: -0.030 min
Response: 3980139
Conc: 13.20 ng/ml

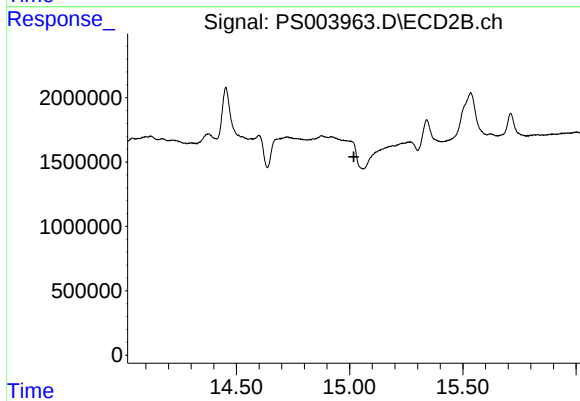

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.019 min
Response: 0
Conc: N.D.

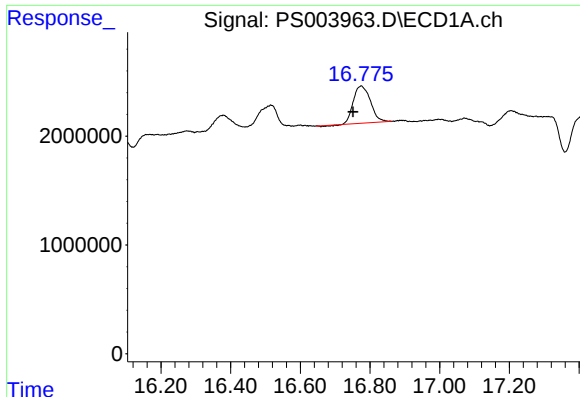

#15 Picloram


R.T.: 16.774 min
Delta R.T.: 0.023 min
Response: 11578210
Conc: 3.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

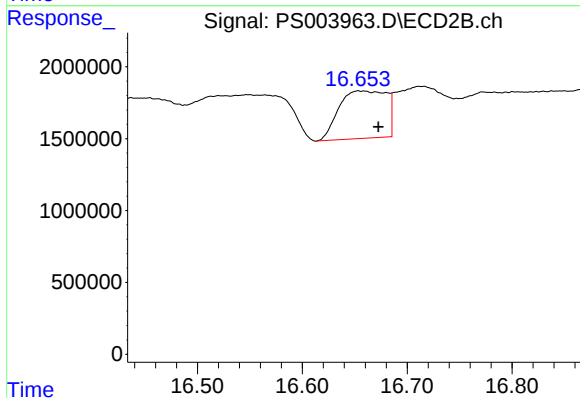


#15 Picloram

R.T.: 16.656 min
Delta R.T.: -0.017 min
Response: 10390736
Conc: 3.28 ng/ml

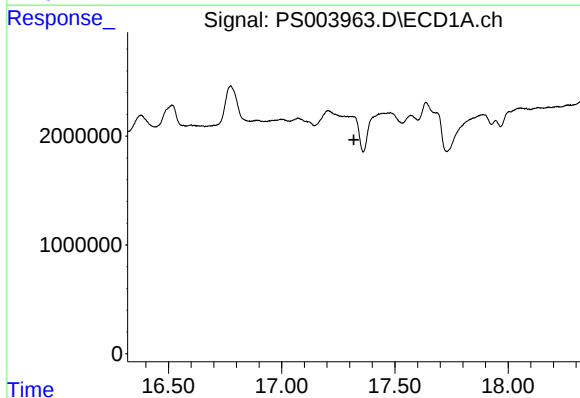

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.319 min
Response: 0
Conc: N.D.

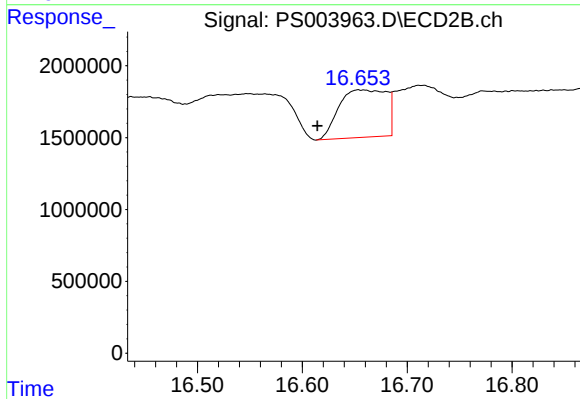

#16 DCPA

R.T.: 16.656 min
Delta R.T.: 0.041 min
Response: 10390736
Conc: 3.07 ng/ml