

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
 Data File : PS003966.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2019 20:36
 Operator : EI\SJ
 Sample : K2178-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-17

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 03:14:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.275	10.773	21062989	18700358	48.286	38.113
Target Compounds							
1) T	Dalapon	2.789	2.276	35694244	22287854	47.877	30.547 #
2) T	3,5-DICHL...	0.000	8.934	0	5519254	N.D.	8.653
3) T	4-Nitroph...	0.000	9.978	0	18813940	N.D.	82.868
5) T	DICAMBA	11.538	0.000	3166476	0	1.544	N.D. #
6) T	MCPD	11.938	11.285	7746520	11075272	5.569	9.380 #
7) T	MCPA	12.098	0.000	221.7E6	0	105.065	N.D. #
10) T	Pentachlo...	13.483	13.171	7509141	5932134	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	13.836	0	955812	N.D.	<MDL
12) T	2,4,5-T	0.000	14.349	0	5448357	N.D.	2.506
13) T	2,4-DB	15.520	14.978	7942050	6782182	26.342	22.839
14) T	DINOSEB	0.000	15.429	0	1752732	N.D.	<MDL
15) T	Picloram	16.745	16.719	3187468	51618458	<MDL	16.277 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
Data File : PS003966.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2019 20:36
Operator : EI\SJ
Sample : K2178-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-17

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 03:14:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

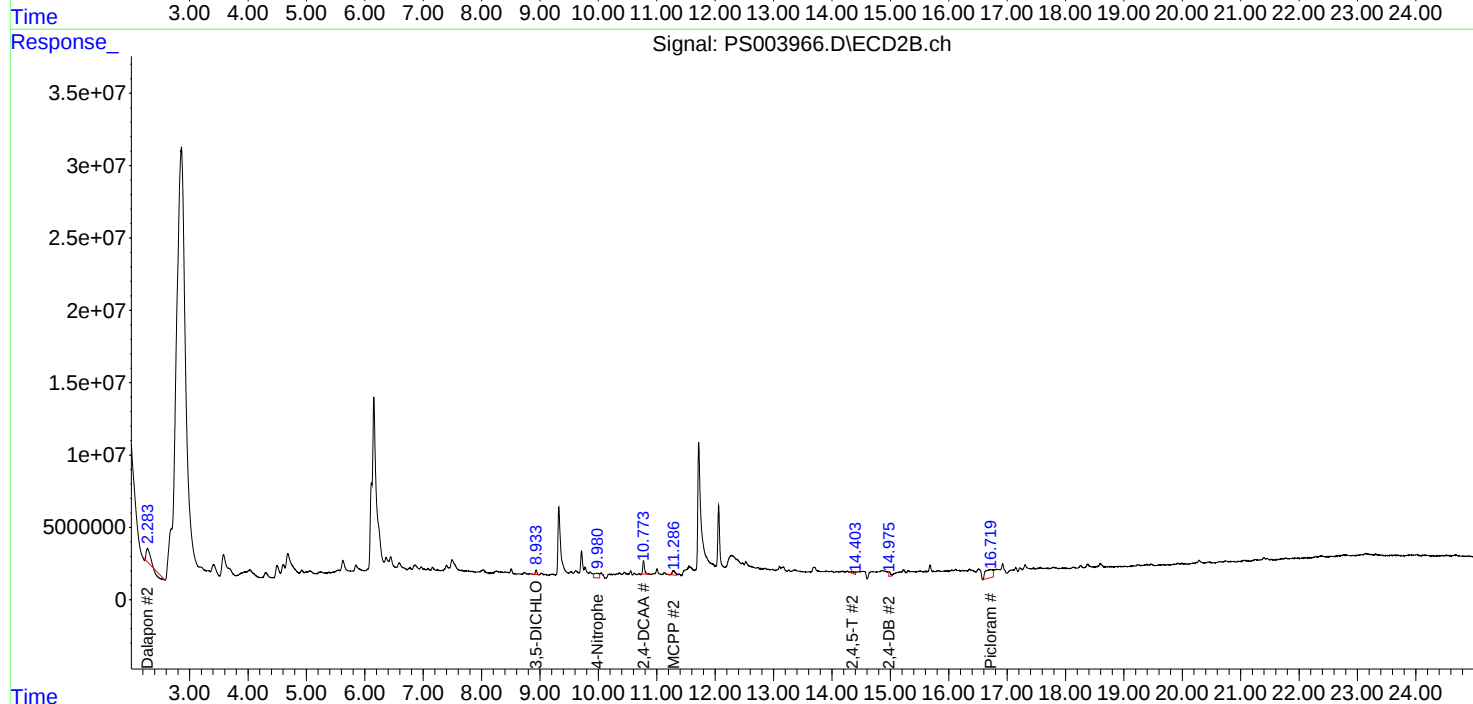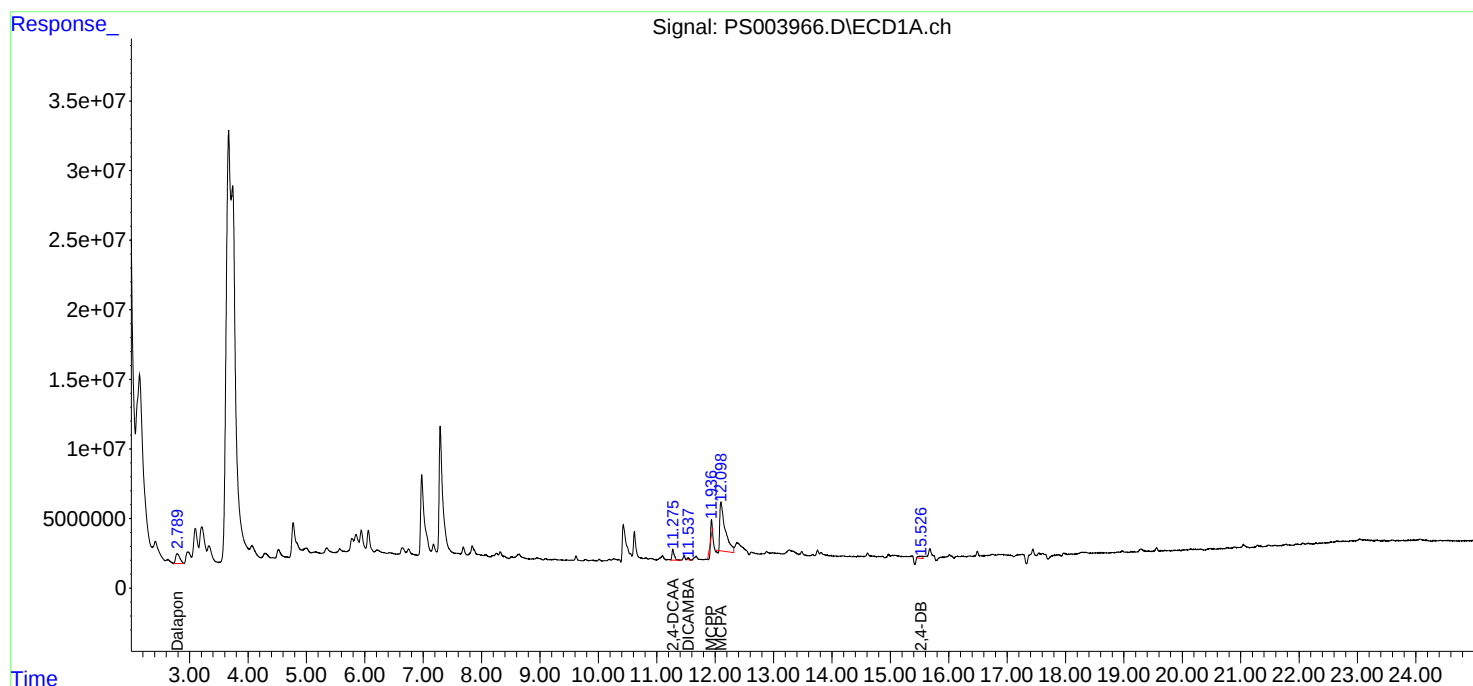


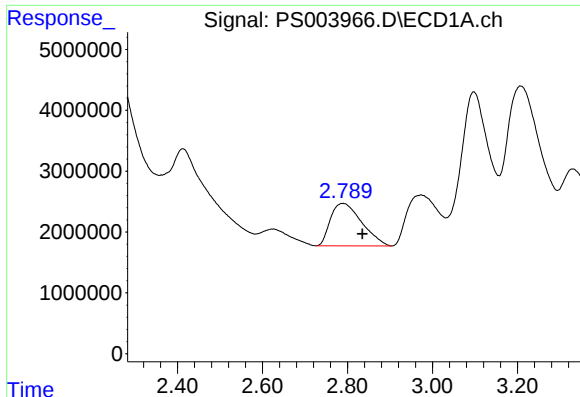

#1 Dalapon


R.T.: 2.789 min
Delta R.T.: -0.046 min
Response: 35694244
Conc: 47.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-17

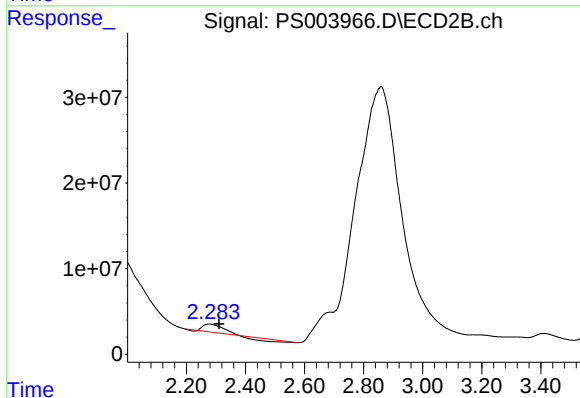


#1 Dalapon

R.T.: 2.276 min
Delta R.T.: -0.034 min
Response: 22287854
Conc: 30.55 ng/ml

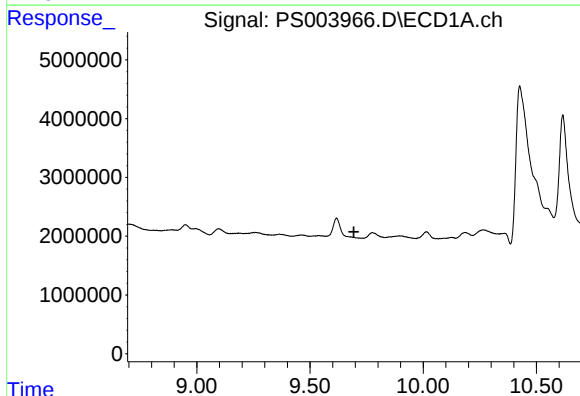


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

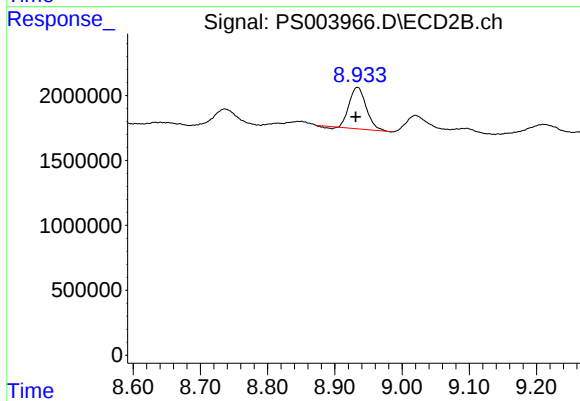

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.934 min
Delta R.T.: 0.003 min
Response: 5519254
Conc: 8.65 ng/ml

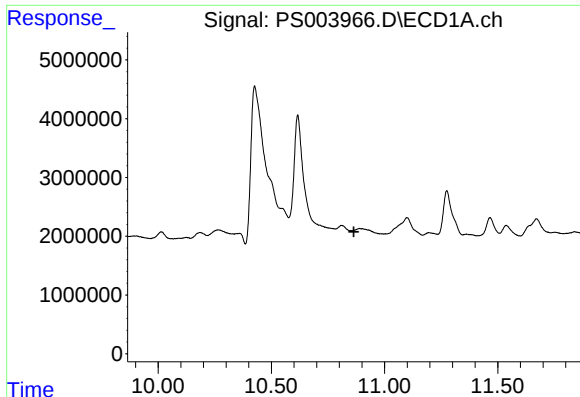

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-17

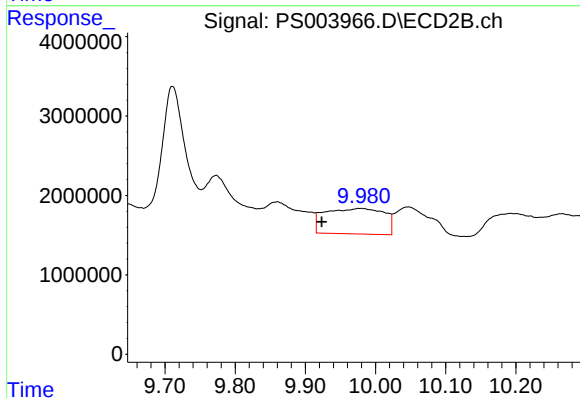


#3 4-Nitrophenol

R.T.: 9.978 min
Delta R.T.: 0.055 min
Response: 18813940
Conc: 82.87 ng/ml

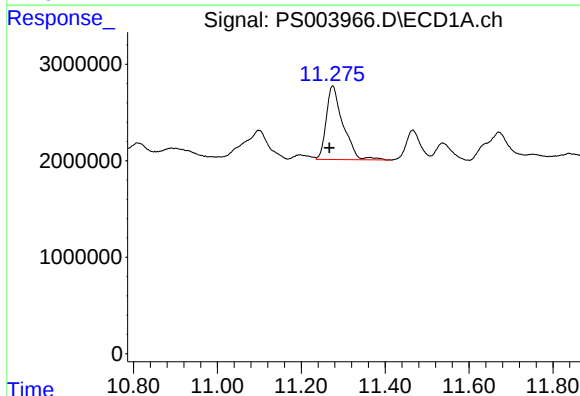


#4 2,4-DCAA

R.T.: 11.275 min
Delta R.T.: 0.008 min
Response: 21062989
Conc: 48.29 ng/ml

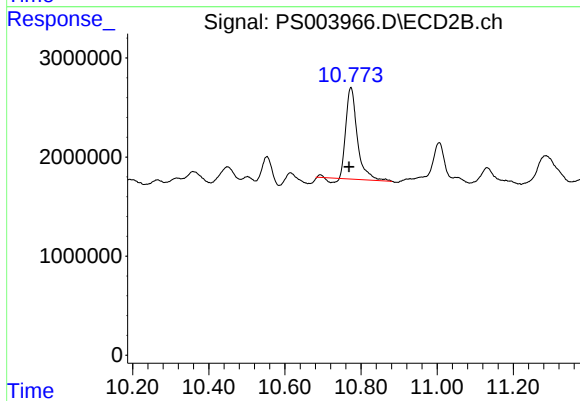

#4 2,4-DCAA


R.T.: 10.773 min
Delta R.T.: 0.004 min
Response: 18700358
Conc: 38.11 ng/ml

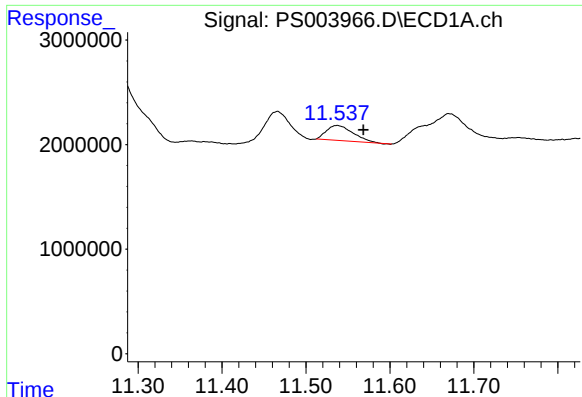

#5 DICAMBA


R.T.: 11.538 min
Delta R.T.: -0.031 min
Response: 3166476
Conc: 1.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-17

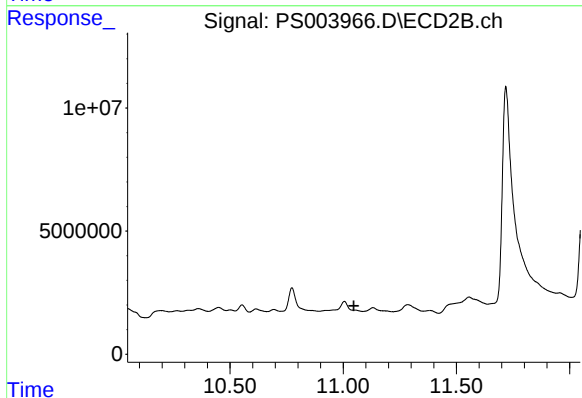


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.047 min
Response: 0
Conc: N.D.

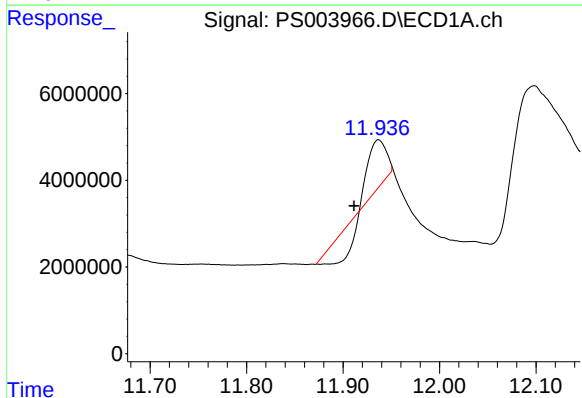


#6 MCP

R.T.: 11.938 min
Delta R.T.: 0.026 min
Response: 7746520
Conc: 5.57 ug/ml

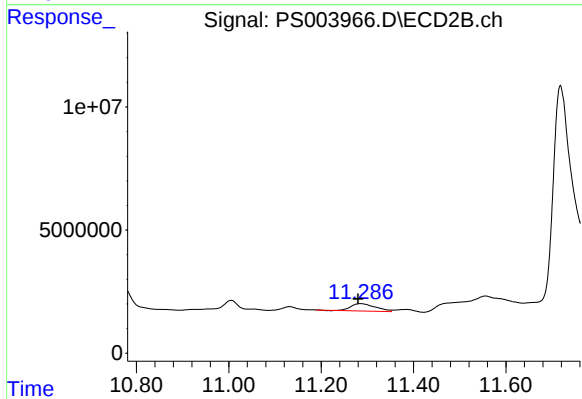

#6 MCP


R.T.: 11.285 min
Delta R.T.: 0.005 min
Response: 11075272
Conc: 9.38 ug/ml

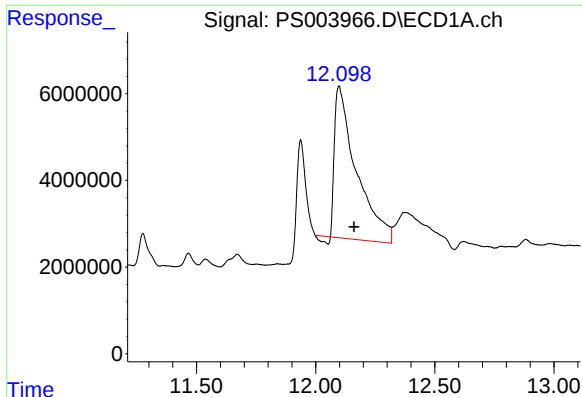

#7 MCPA


R.T.: 12.098 min
Delta R.T.: -0.063 min
Response: 221663618
Conc: 105.06 ug/ml

Instrument :
ECD_S
ClientSampleId :
COMP-17

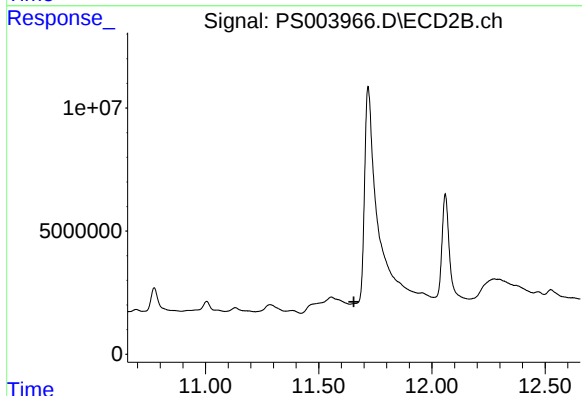


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.655 min
Response: 0
Conc: N.D.

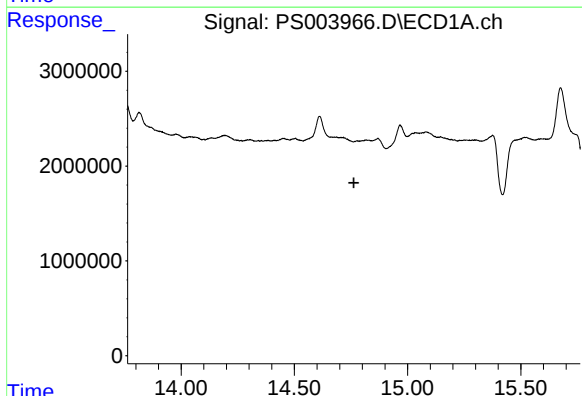


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.763 min
Response: 0
Conc: N.D.

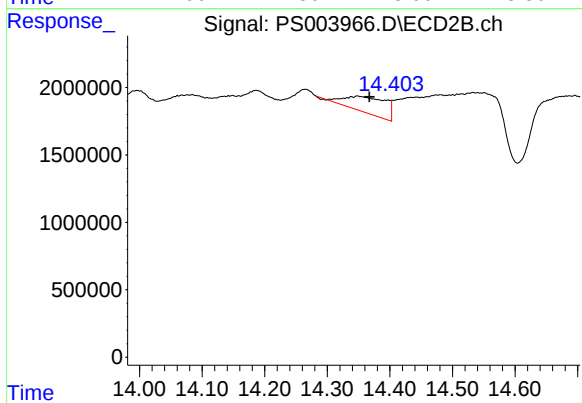

#12 2,4,5-T


R.T.: 14.349 min
Delta R.T.: -0.018 min
Response: 5448357
Conc: 2.51 ng/ml

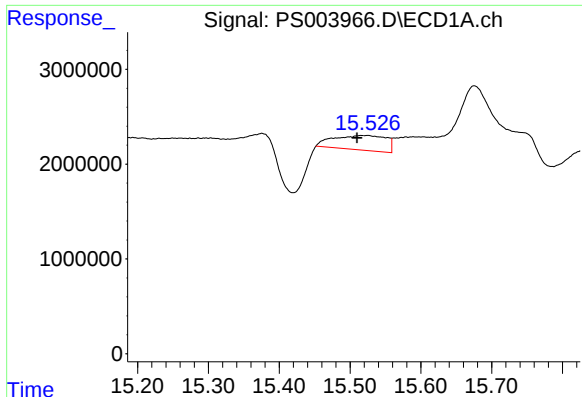

#13 2,4-DB


R.T.: 15.520 min
Delta R.T.: 0.010 min
Response: 7942050
Conc: 26.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-17

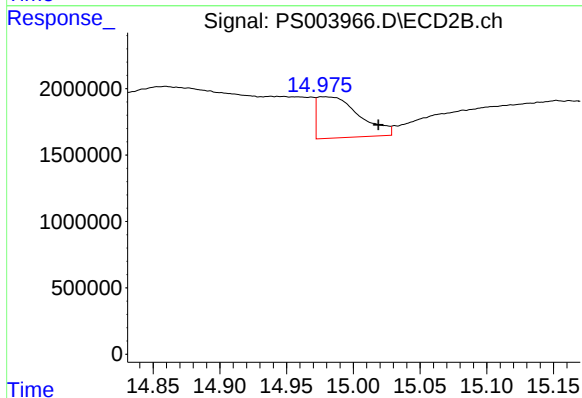


#13 2,4-DB

R.T.: 14.978 min
Delta R.T.: -0.041 min
Response: 6782182
Conc: 22.84 ng/ml

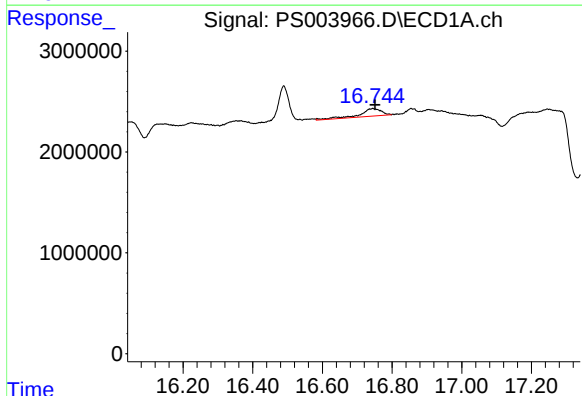

#15 Picloram

R.T.: 16.745 min
Delta R.T.: -0.007 min
Response: 3187468
Conc: N.D.

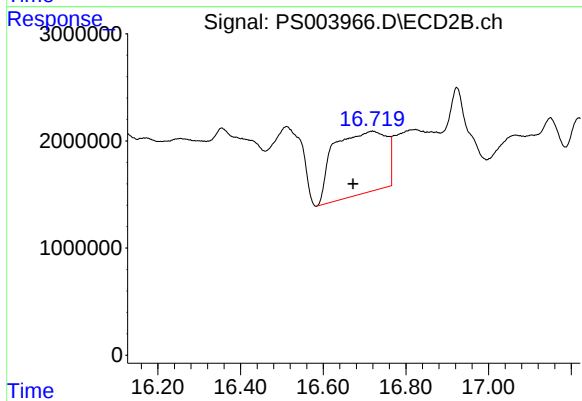

#15 Picloram

R.T.: 16.719 min
Delta R.T.: 0.046 min
Response: 51618458
Conc: 16.28 ng/ml