

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
 Data File : PS003968.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2019 21:39
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 03:15:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.259	10.762	252.0E6	219.9E6	577.637	448.212
Target Compounds							
1) T	Dalapon	0.000	2.279	0	858441	N.D.	1.177
3) T	4-Nitroph...	0.000	9.925	0	326631	N.D.	1.439
6) T	MCP	0.000	11.260	0	329196	N.D.	<MDL
7) T	MCPA	0.000	11.649	0	2667935	N.D.	1.496
9) T	2,4-D	0.000	12.661	0	235698	N.D.	<MDL
10) T	Pentachlo...	0.000	13.173	0	1287673	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.803	0	488210	N.D.	<MDL
13) T	2,4-DB	0.000	14.966	0	8252862	N.D.	27.792
14) T	DINOSEB	0.000	15.490	0	8285550	N.D.	4.318
15) T	Picloram	16.734	16.613	7353678	1929783	2.165	<MDL #
16) T	DCPA	0.000	16.613	0	1929783	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
Data File : PS003968.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2019 21:39
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 03:15:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

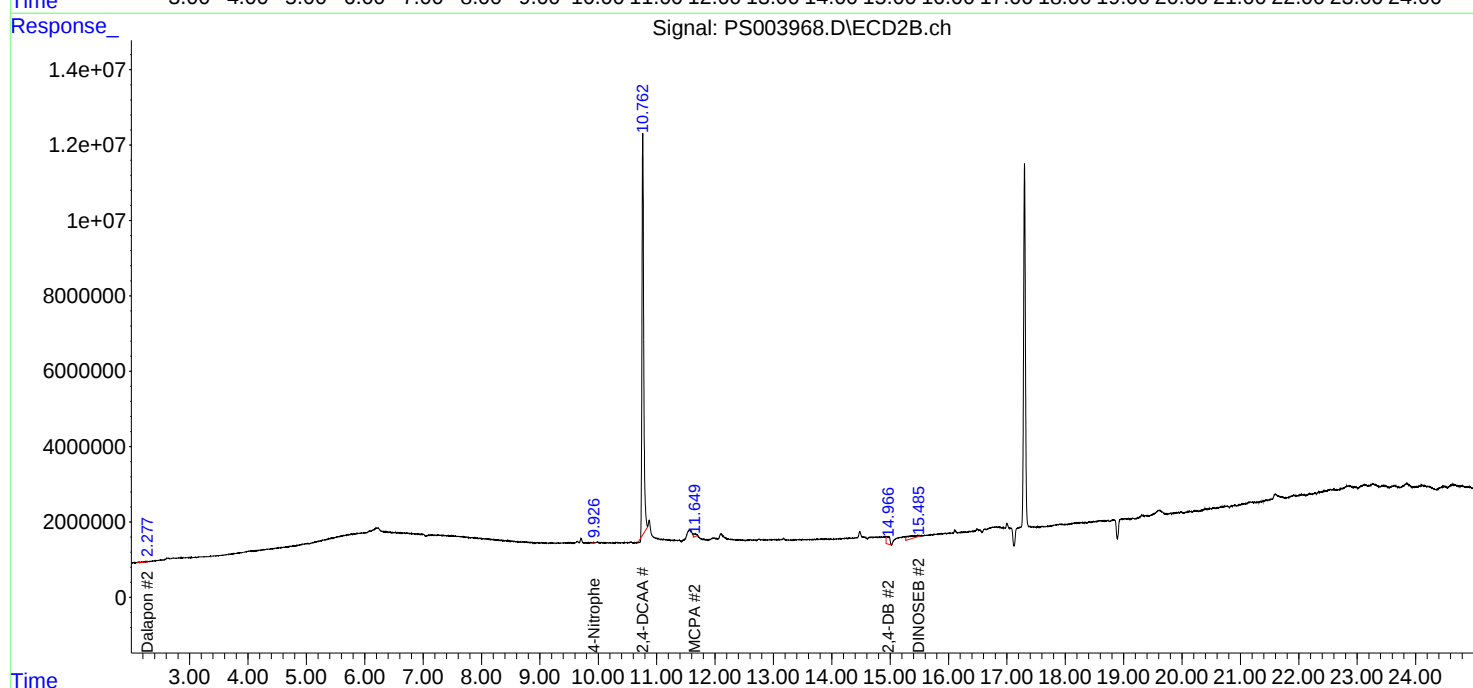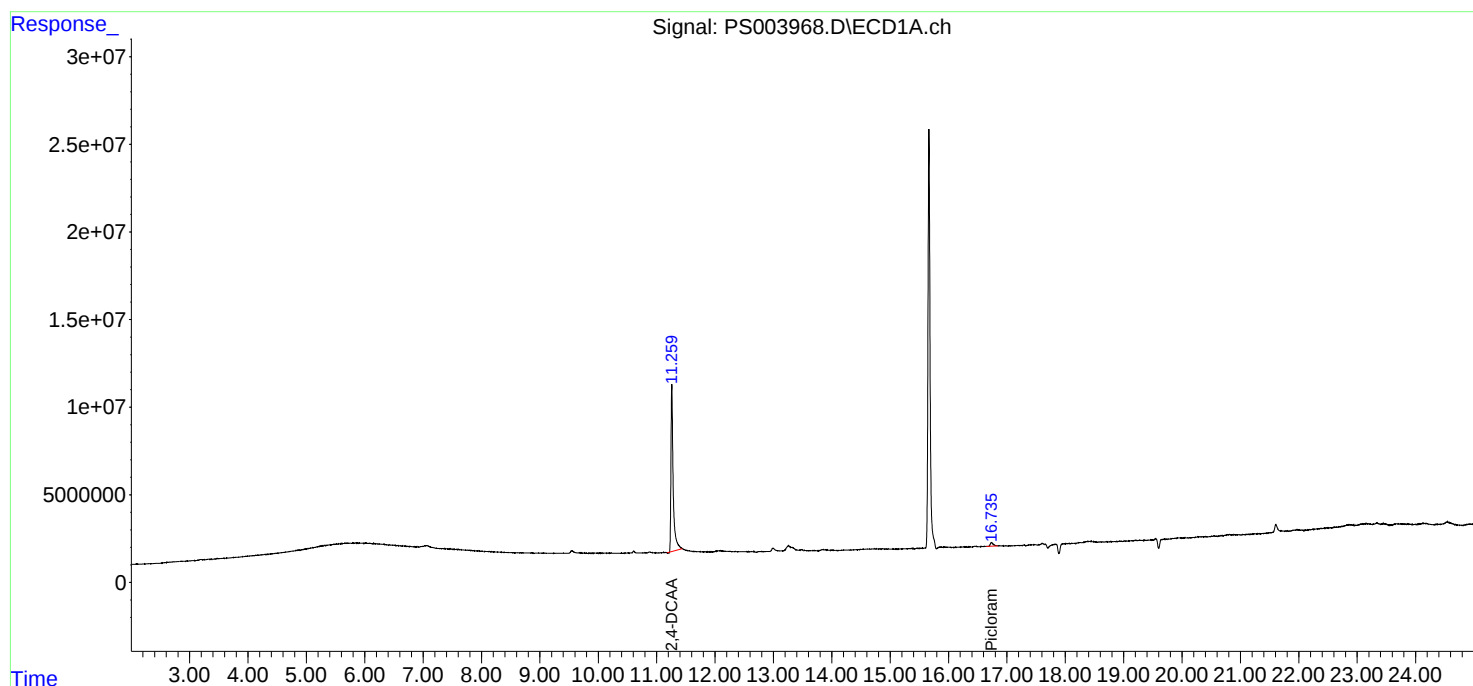


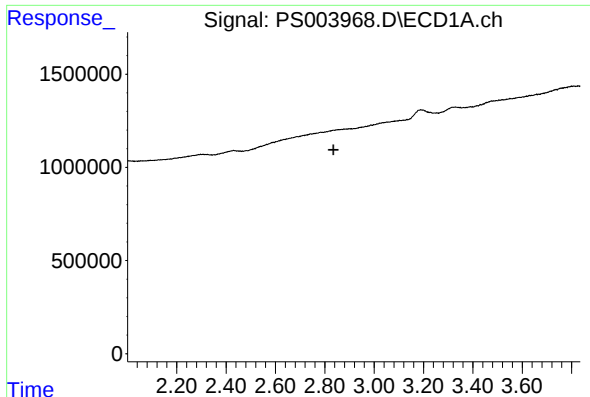

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.835 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

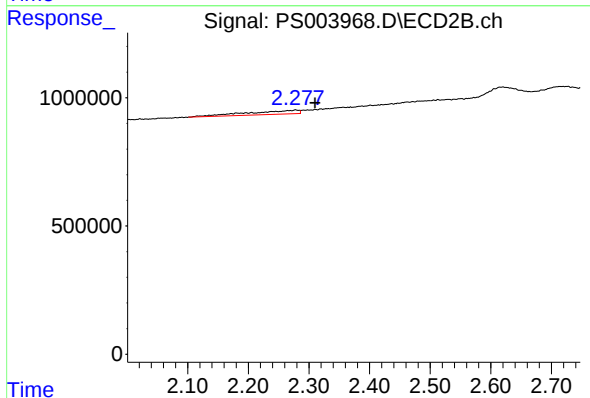


#1 Dalapon

R.T.: 2.279 min
Delta R.T.: -0.032 min
Response: 858441
Conc: 1.18 ng/ml

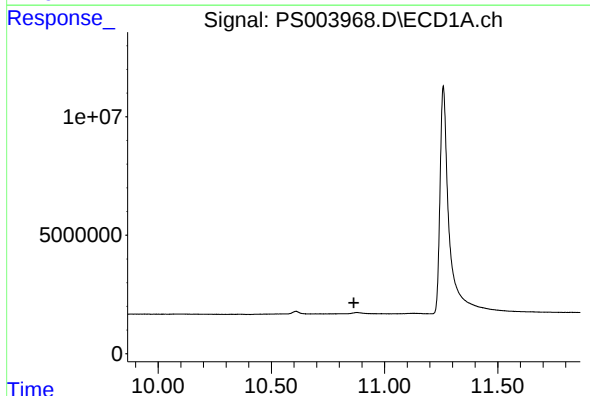


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

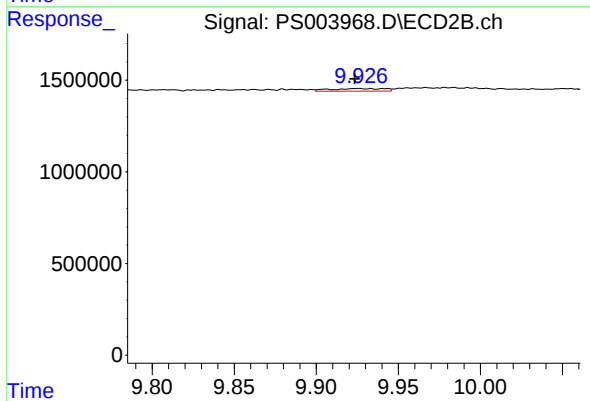

#3 4-Nitrophenol


R.T.: 9.925 min
Delta R.T.: 0.002 min
Response: 326631
Conc: 1.44 ng/ml

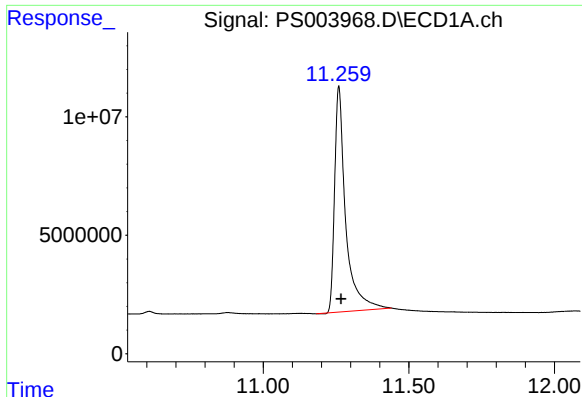

#4 2,4-DCAA


R.T.: 11.259 min
Delta R.T.: -0.007 min
Response: 251972331
Conc: 577.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

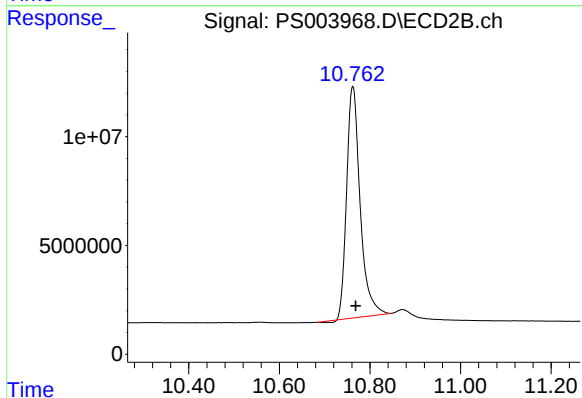


#4 2,4-DCAA

R.T.: 10.762 min
Delta R.T.: -0.007 min
Response: 219919057
Conc: 448.21 ng/ml

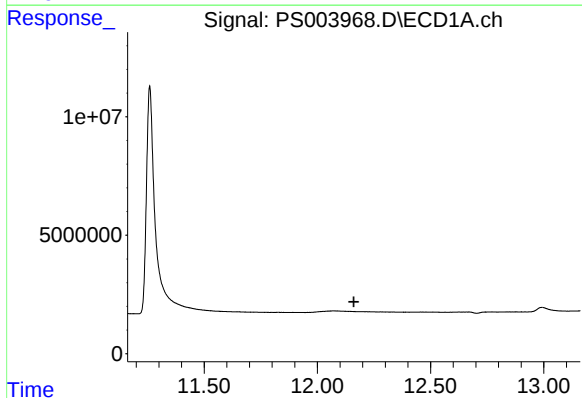


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.162 min
Response: 0
Conc: N.D.

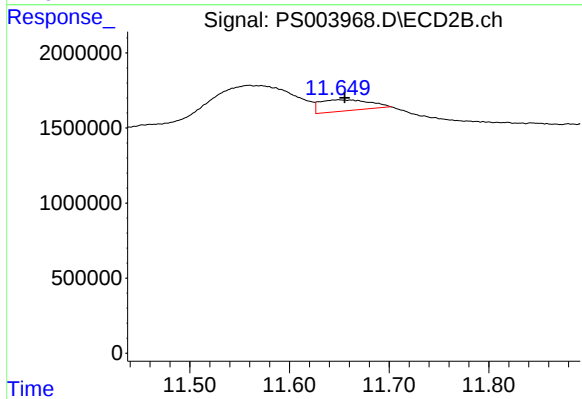

#7 MCPA


R.T.: 11.649 min
Delta R.T.: -0.006 min
Response: 2667935
Conc: 1.50 ug/ml

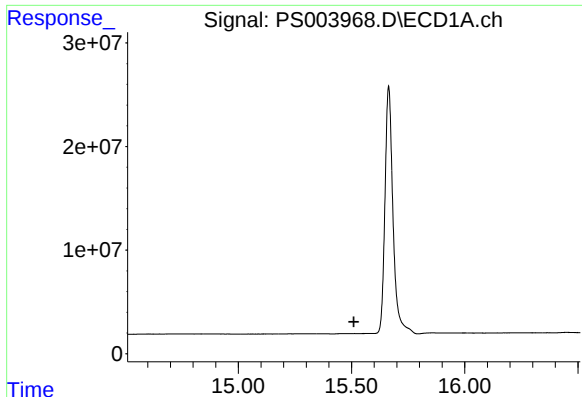

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

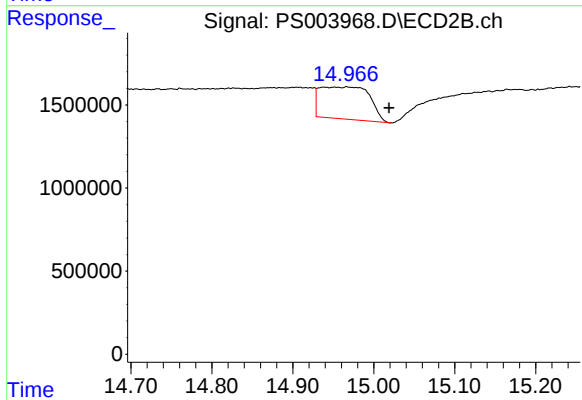


#13 2,4-DB

R.T.: 14.966 min
Delta R.T.: -0.052 min
Response: 8252862
Conc: 27.79 ng/ml

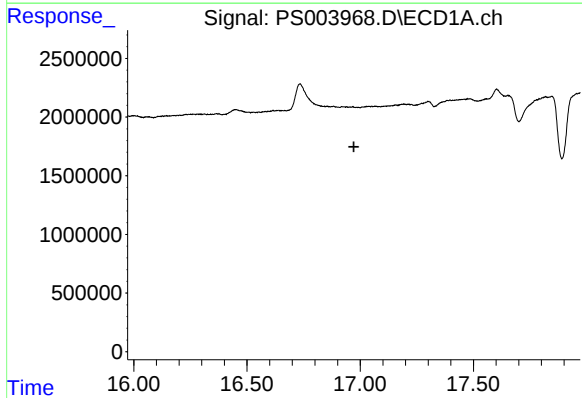


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

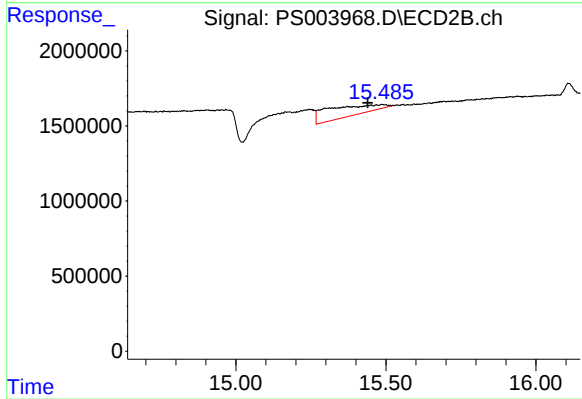

#14 DINOSEB


R.T.: 15.490 min
Delta R.T.: 0.050 min
Response: 8285550
Conc: 4.32 ng/ml

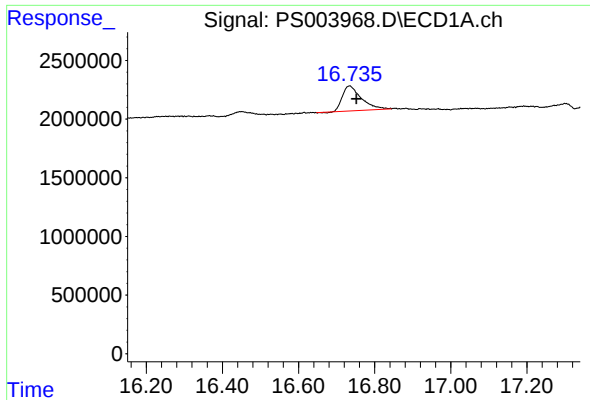

#15 Picloram

R.T.: 16.734 min
Delta R.T.: -0.018 min
Response: 7353678
Conc: 2.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

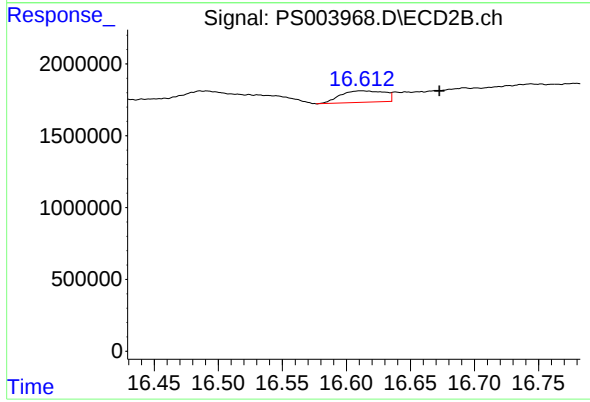

#15 Picloram

R.T.: 16.613 min
Delta R.T.: -0.059 min
Response: 1929783
Conc: N.D.