

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
 Data File : PS003977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2019 02:20
 Operator : EI\SJ
 Sample : K2213-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 03:18:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.275	10.776	202.0E6	179.9E6	463.040	366.664
Target Compounds							
1) T	Dalapon	2.798	2.306	65748187	203.6E6	88.189	279.051 #
2) T	3,5-DICHL...	0.000	8.942	0	5706215	N.D.	8.946
3) T	4-Nitroph...	0.000	9.945	0	16581585	N.D.	73.035
5) T	DICAMBA	0.000	11.015	0	6544057	N.D.	3.519
7) T	MCPA	12.126	0.000	335.9E6	0	159.219	N.D. #
9) T	2,4-D	0.000	12.633	0	2430012	N.D.	4.568
10) T	Pentachlo...	13.493	13.181	5935308	2688981	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	13.809	0	4437750	N.D.	1.676
12) T	2,4,5-T	0.000	14.365	0	1791752	N.D.	<MDL
13) T	2,4-DB	0.000	14.976	0	7087252	N.D.	23.867
14) T	DINOSEB	0.000	15.446	0	2025818	N.D.	1.056
15) T	Picloram	0.000	16.705	0	22399059	N.D.	7.063
16) T	DCPA	0.000	16.629	0	7965422	N.D.	2.357



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
Data File : PS003977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2019 02:20
Operator : EI\SJ
Sample : K2213-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 03:18:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

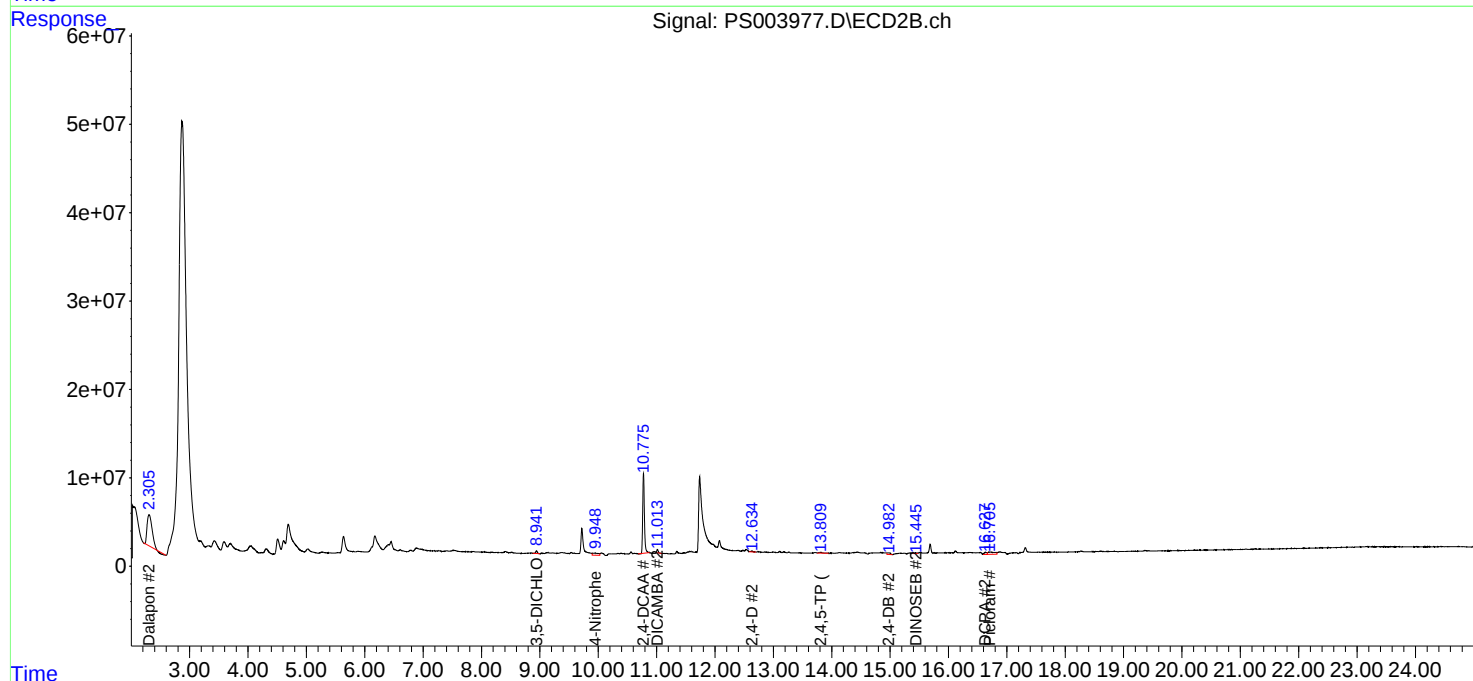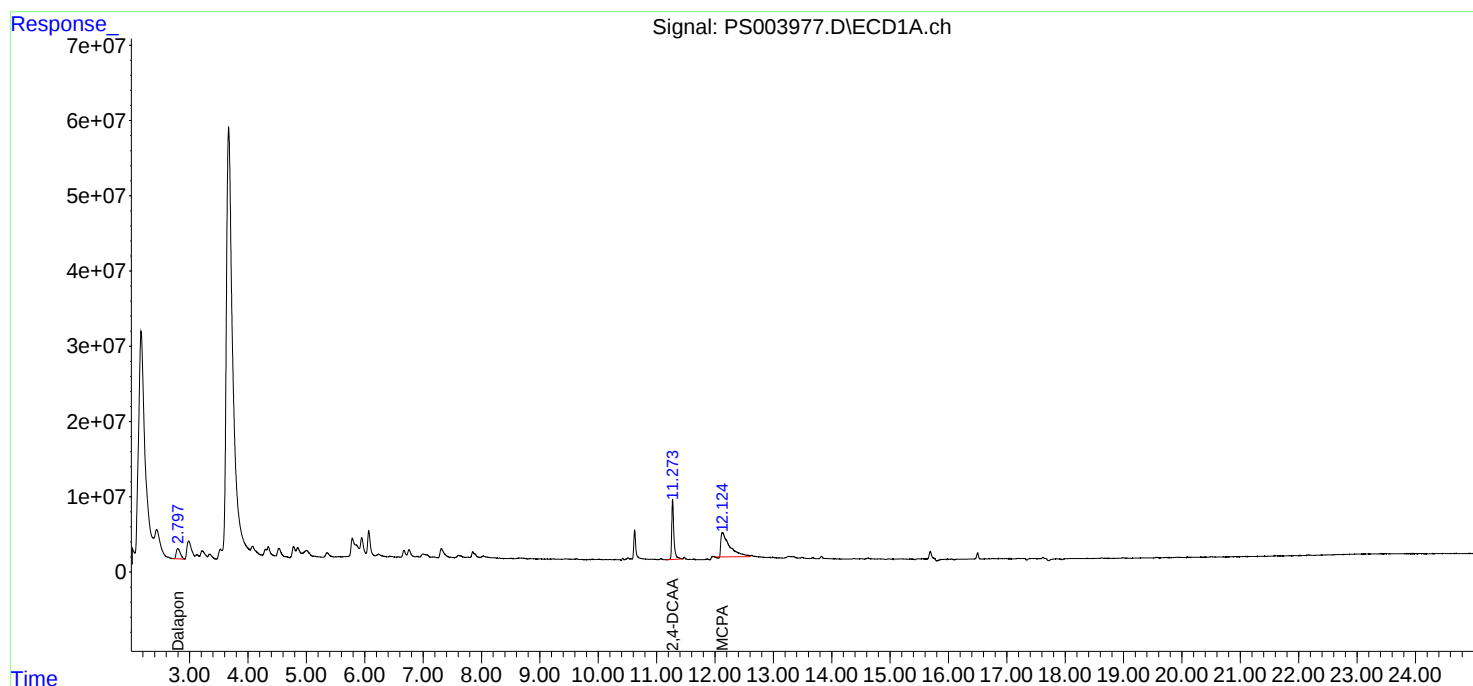


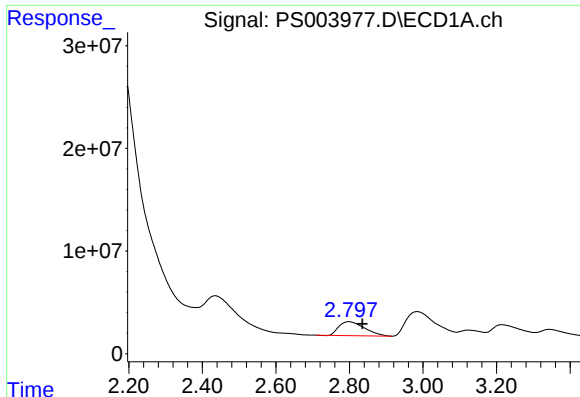

#1 Dalapon


R.T.: 2.798 min
Delta R.T.: -0.037 min
Response: 65748187
Conc: 88.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

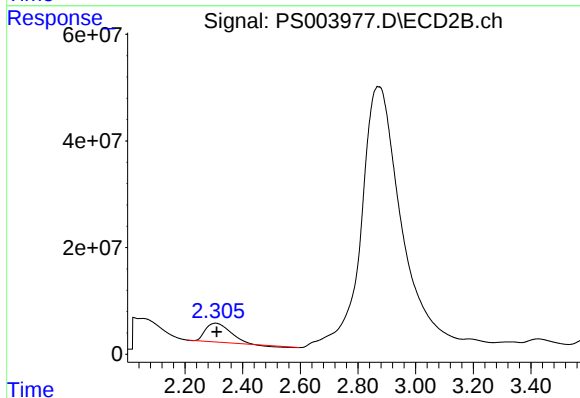


#1 Dalapon

R.T.: 2.306 min
Delta R.T.: -0.005 min
Response: 203603608
Conc: 279.05 ng/ml

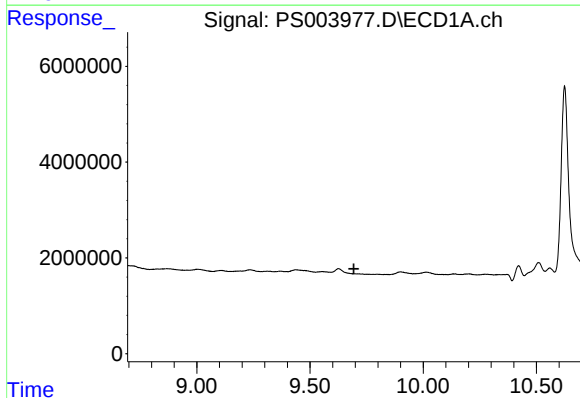


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

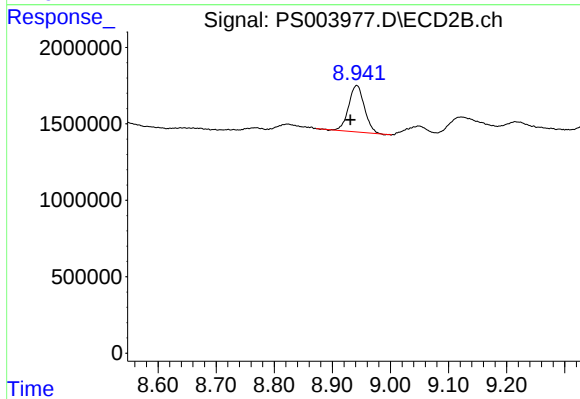

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.942 min
Delta R.T.: 0.011 min
Response: 5706215
Conc: 8.95 ng/ml

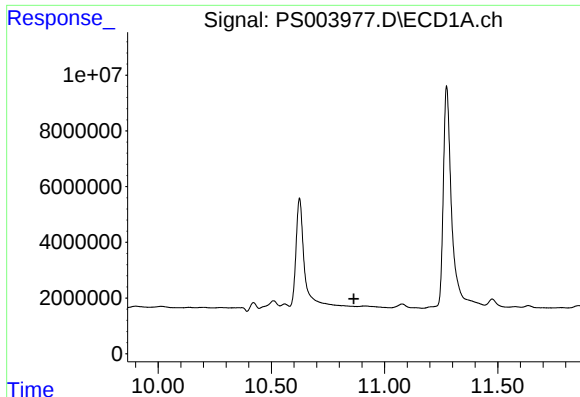

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

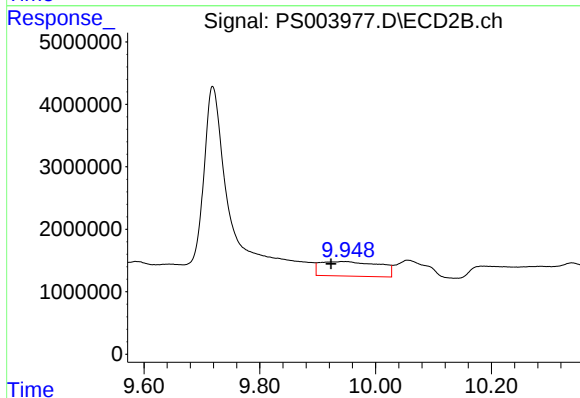


#3 4-Nitrophenol

R.T.: 9.945 min
Delta R.T.: 0.022 min
Response: 16581585
Conc: 73.04 ng/ml

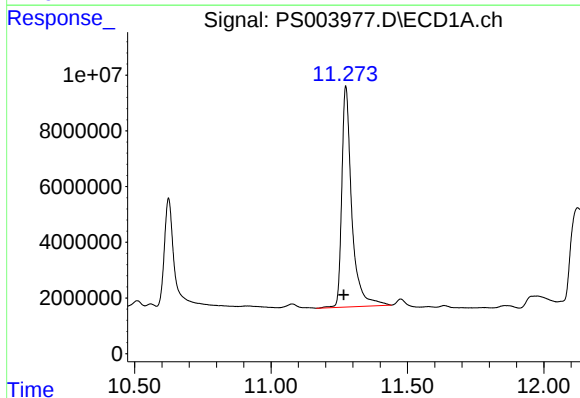


#4 2,4-DCAA

R.T.: 11.275 min
Delta R.T.: 0.008 min
Response: 201983864
Conc: 463.04 ng/ml

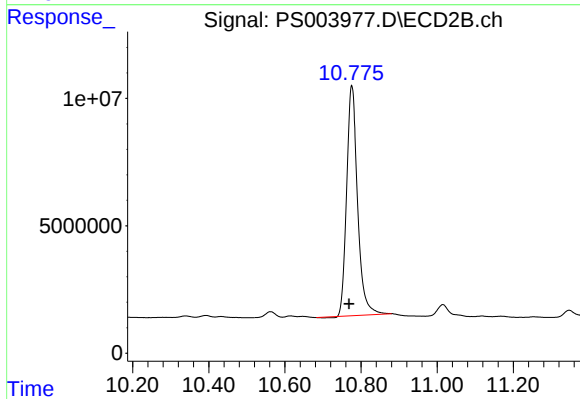

#4 2,4-DCAA


R.T.: 10.776 min
Delta R.T.: 0.007 min
Response: 179906871
Conc: 366.66 ng/ml

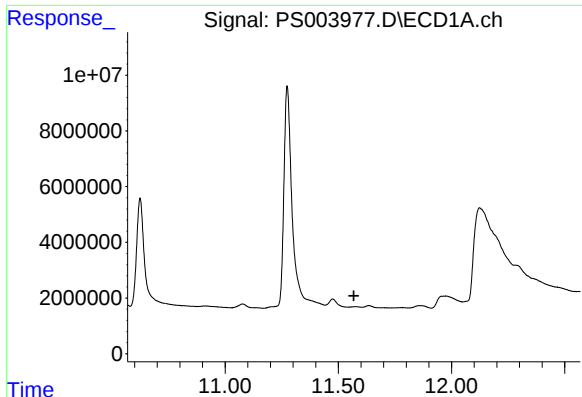

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

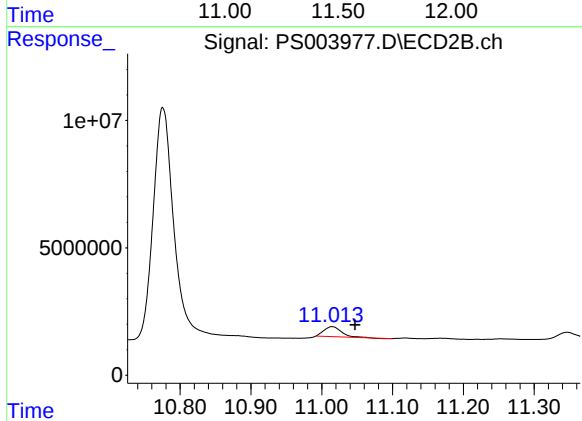


#5 DICAMBA

R.T.: 11.015 min
Delta R.T.: -0.033 min
Response: 6544057
Conc: 3.52 ng/ml

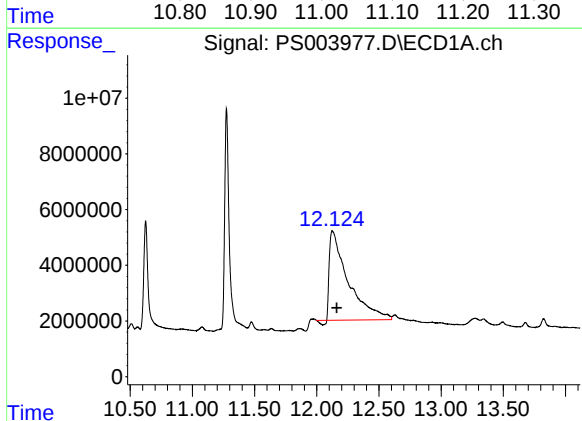


#7 MCPA

R.T.: 12.126 min
Delta R.T.: -0.036 min
Response: 335917806
Conc: 159.22 ug/ml

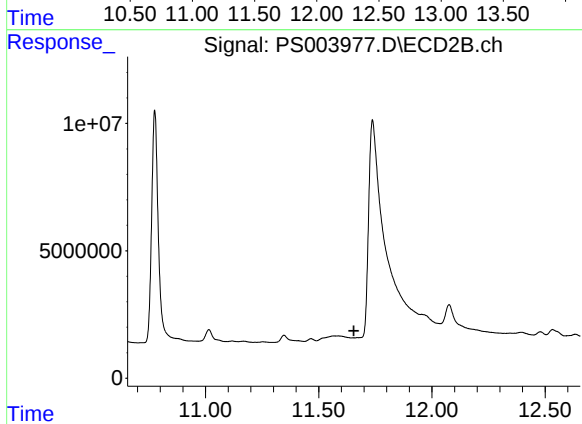

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.655 min
Response: 0
Conc: N.D.

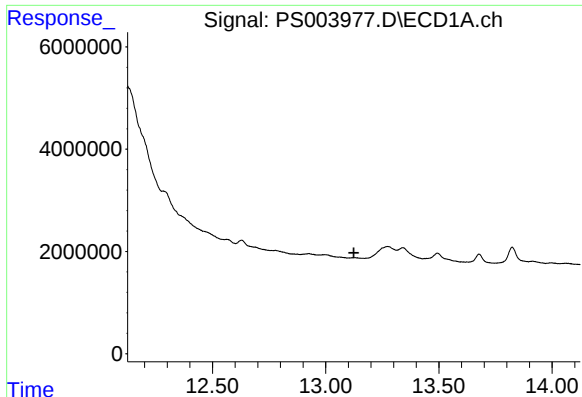

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

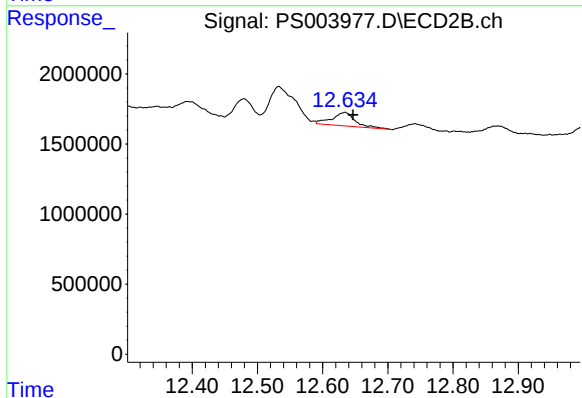


#9 2,4-D

R.T.: 12.633 min
Delta R.T.: -0.014 min
Response: 2430012
Conc: 4.57 ng/ml

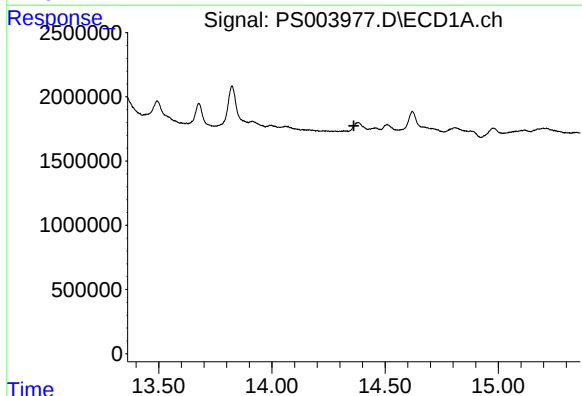


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

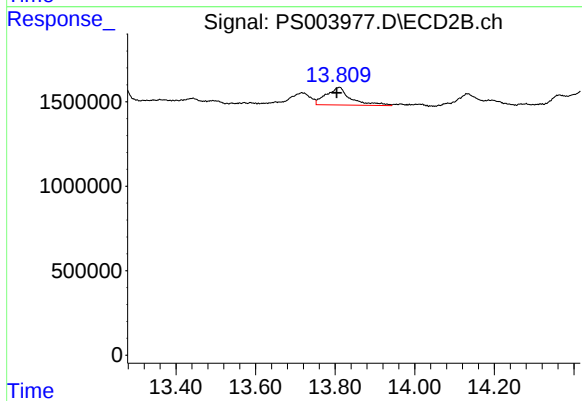

#11 2,4,5-TP (SILVEX)


R.T.: 13.809 min
Delta R.T.: 0.005 min
Response: 4437750
Conc: 1.68 ng/ml

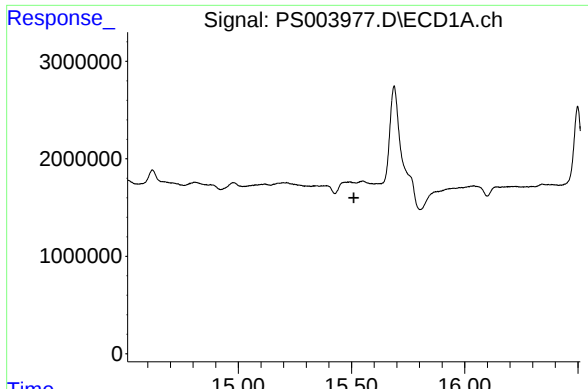

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

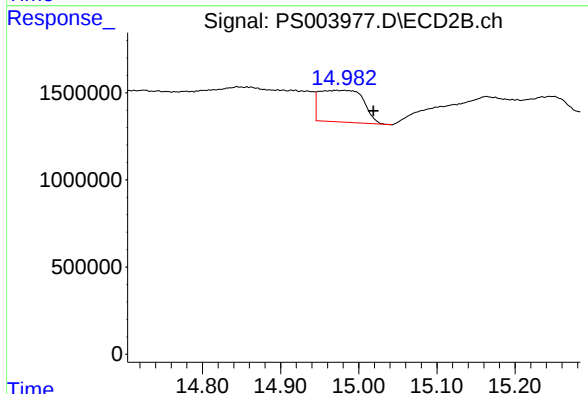


#13 2,4-DB

R.T.: 14.976 min
Delta R.T.: -0.043 min
Response: 7087252
Conc: 23.87 ng/ml

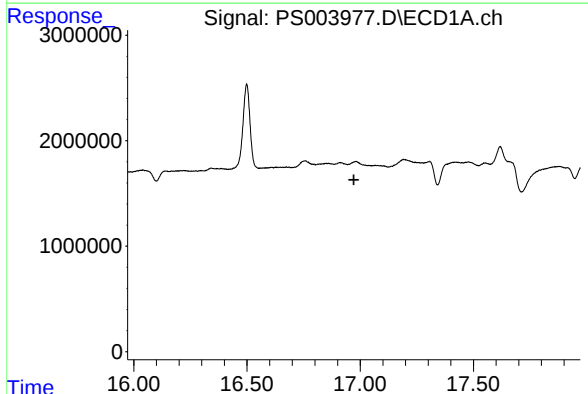


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

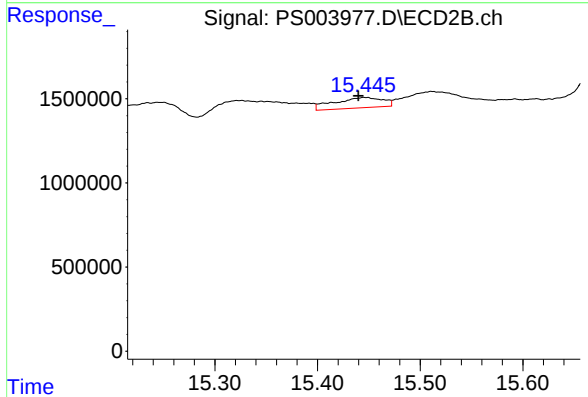

#14 DINOSEB


R.T.: 15.446 min
Delta R.T.: 0.006 min
Response: 2025818
Conc: 1.06 ng/ml

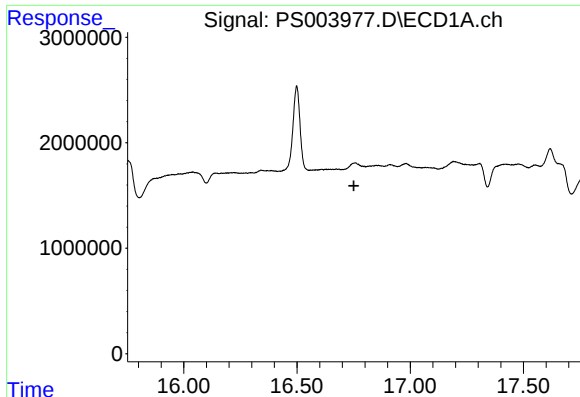

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

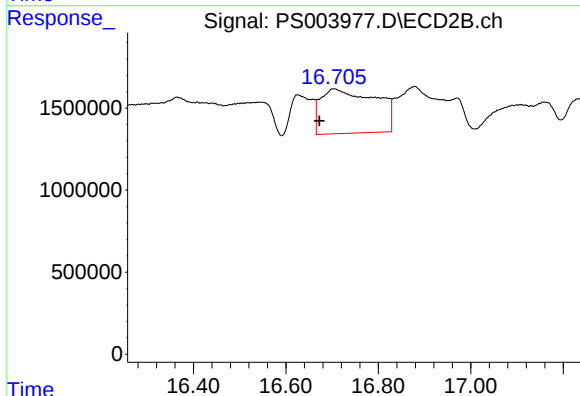


#15 Picloram

R.T.: 16.705 min
Delta R.T.: 0.032 min
Response: 22399059
Conc: 7.06 ng/ml

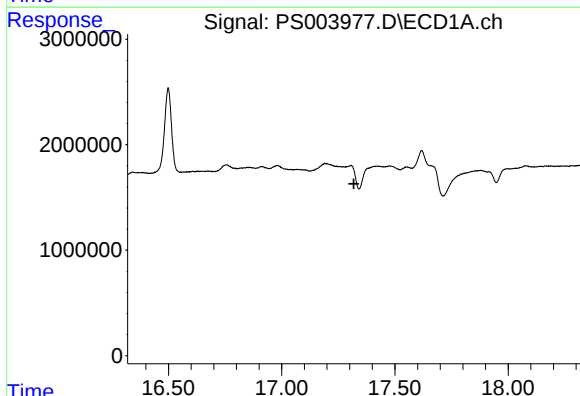

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

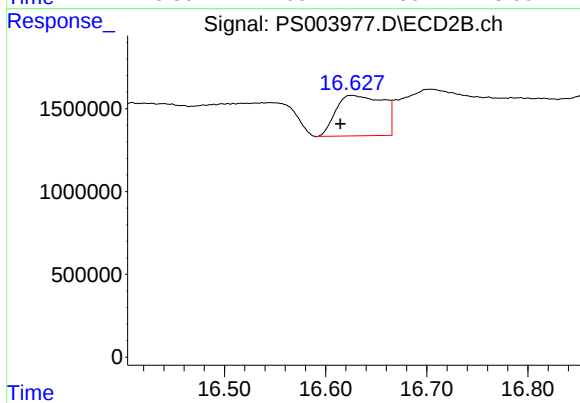

#16 DCPA

R.T.: 16.629 min
Delta R.T.: 0.014 min
Response: 7965422
Conc: 2.36 ng/ml