

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
 Data File : PS003979.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2019 03:22
 Operator : EI\SJ
 Sample : K2214-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-2-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 13:23:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.287	10.784	64483689	56251649	147.826	114.645
Target Compounds							
1) T	Dalapon	2.801	2.303	56995015	142.0E6	76.449	194.649 #
2) T	3,5-DICHL...	0.000	8.945	0	5317330	N.D.	8.336
3) T	4-Nitroph...	0.000	9.954	0	15886817	N.D.	69.975
7) T	MCPA	12.093	0.000	718.6E6	0	340.621	N.D. #
10) T	Pentachlo...	0.000	13.181	0	672213	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.781	0	5468949	N.D.	2.065
12) T	2,4,5-T	0.000	14.403	0	7213128	N.D.	3.318
13) T	2,4-DB	15.547	14.983	15236812	10111631	50.536	34.052 #
15) T	Picloram	16.755	16.713	2697363	41373805	<MDL	13.047 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
Data File : PS003979.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2019 03:22
Operator : EI\SJ
Sample : K2214-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-2-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 13:23:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

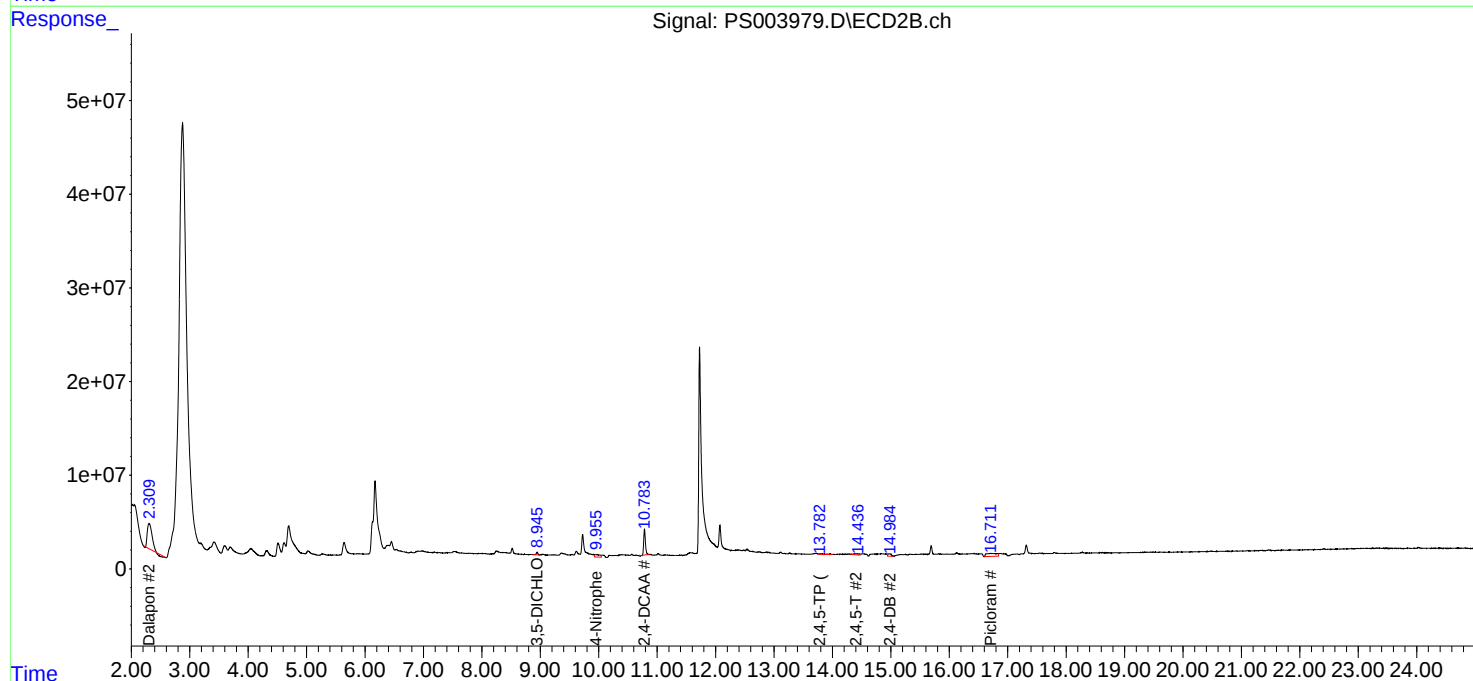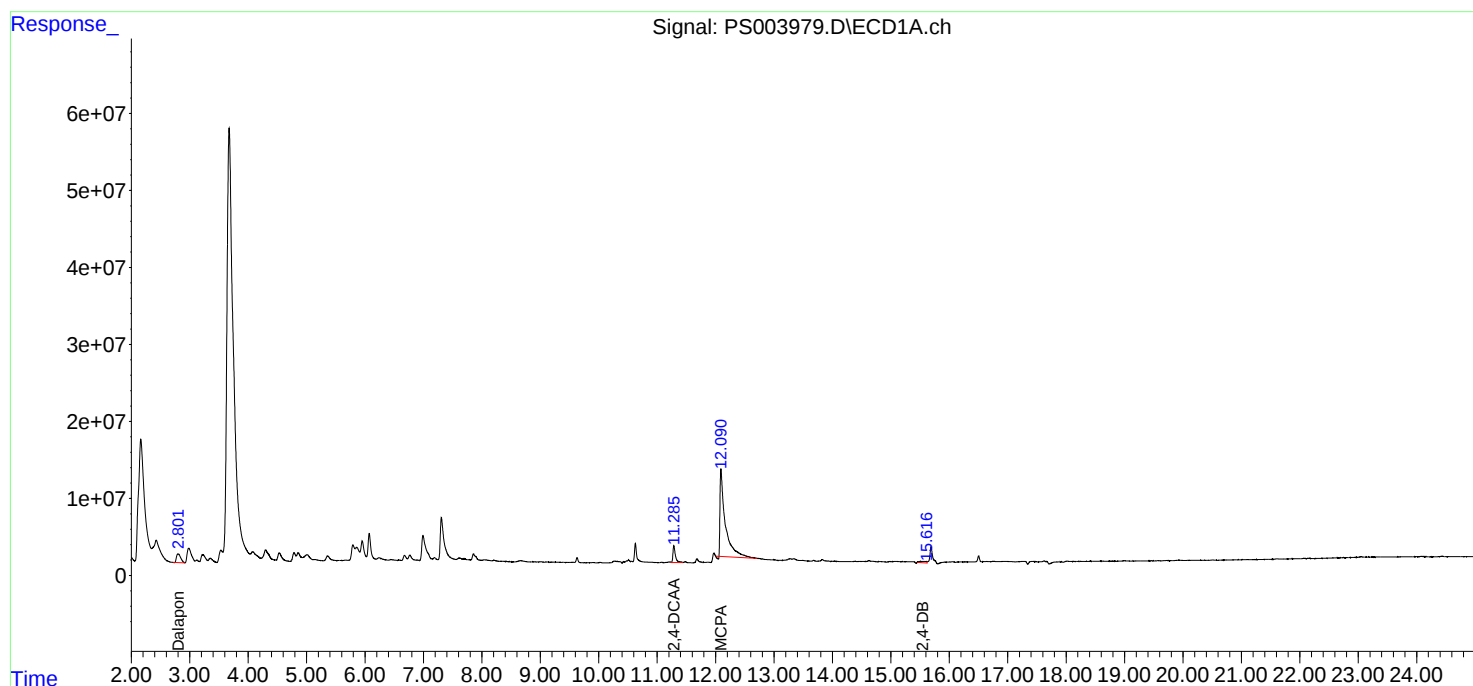


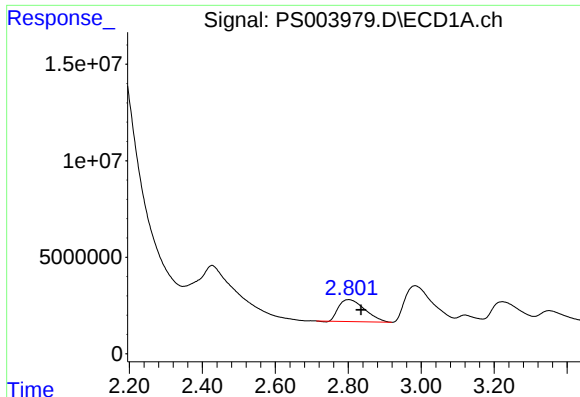

#1 Dalapon


R.T.: 2.801 min
Delta R.T.: -0.034 min
Response: 56995015
Conc: 76.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-2-D

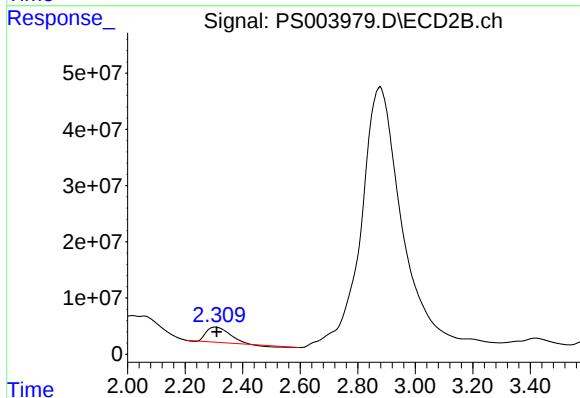


#1 Dalapon

R.T.: 2.303 min
Delta R.T.: -0.008 min
Response: 142021280
Conc: 194.65 ng/ml

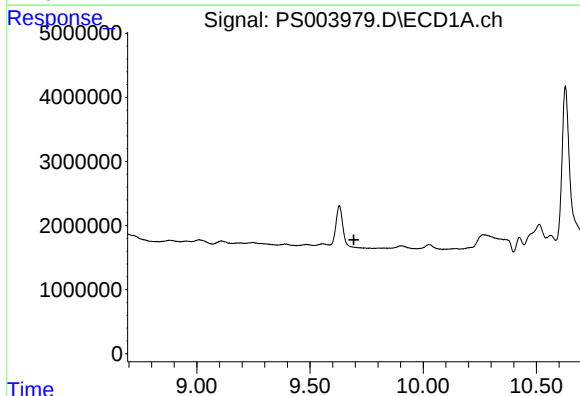


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

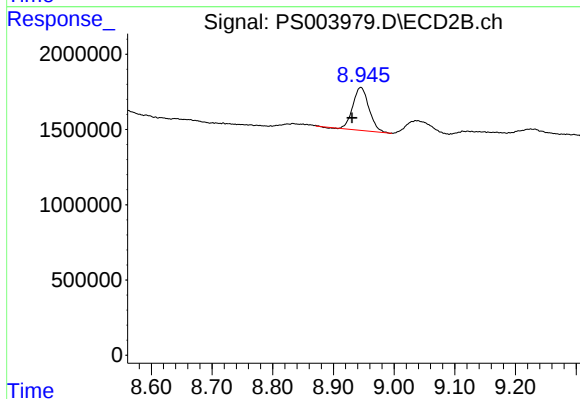

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.945 min
Delta R.T.: 0.014 min
Response: 5317330
Conc: 8.34 ng/ml

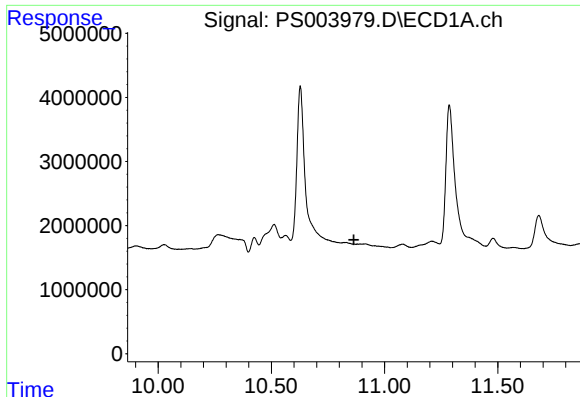

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2-D

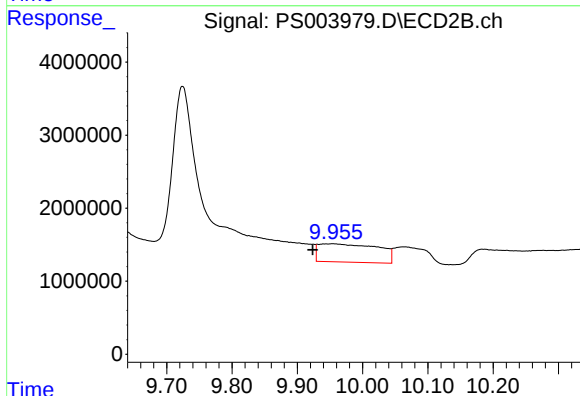


#3 4-Nitrophenol

R.T.: 9.954 min
Delta R.T.: 0.031 min
Response: 15886817
Conc: 69.98 ng/ml

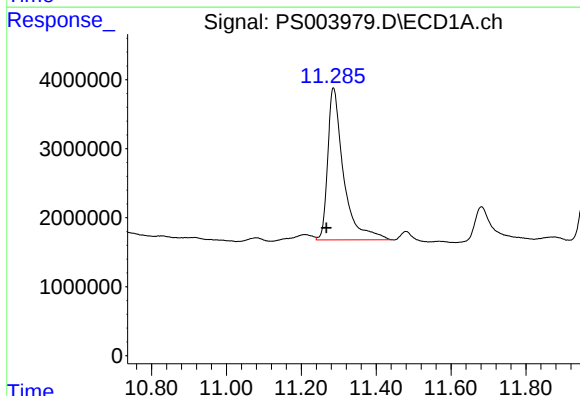


#4 2,4-DCAA

R.T.: 11.287 min
Delta R.T.: 0.020 min
Response: 64483689
Conc: 147.83 ng/ml

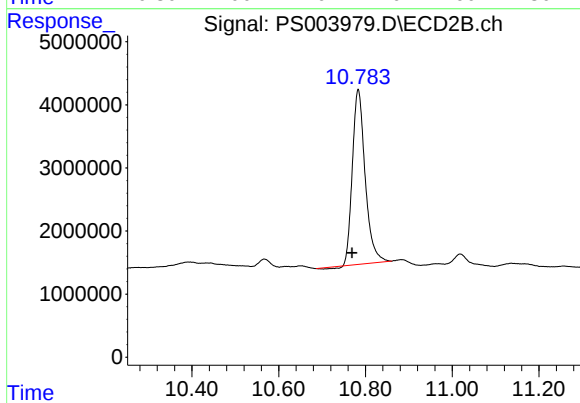

#4 2,4-DCAA


R.T.: 10.784 min
Delta R.T.: 0.015 min
Response: 56251649
Conc: 114.65 ng/ml

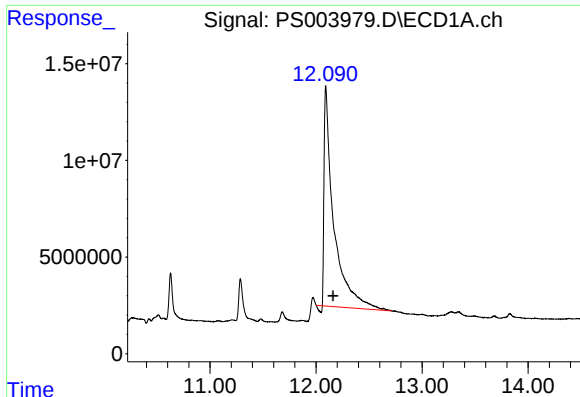

#7 MCPA


R.T.: 12.093 min
Delta R.T.: -0.069 min
Response: 718636031
Conc: 340.62 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-2-D

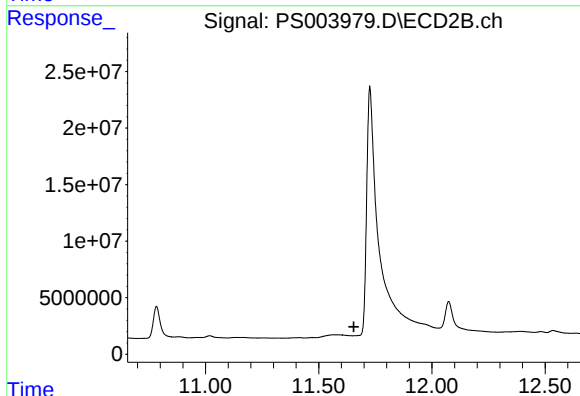


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.655 min
Response: 0
Conc: N.D.

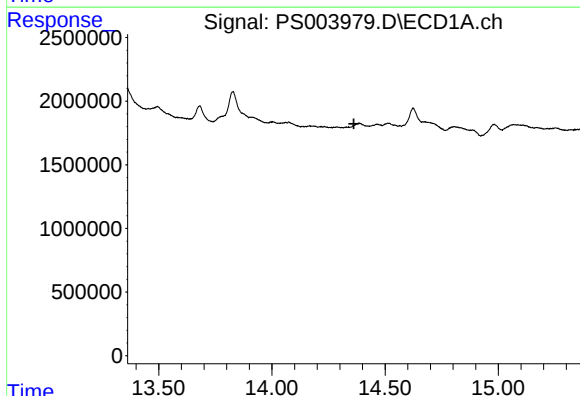


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.362 min
Response: 0
Conc: N.D.

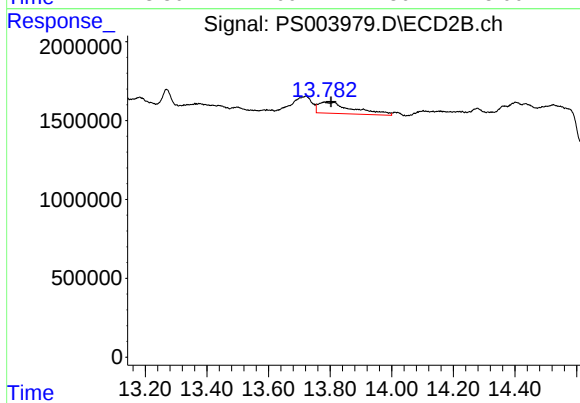

#11 2,4,5-TP (SILVEX)


R.T.: 13.781 min
Delta R.T.: -0.022 min
Response: 5468949
Conc: 2.07 ng/ml

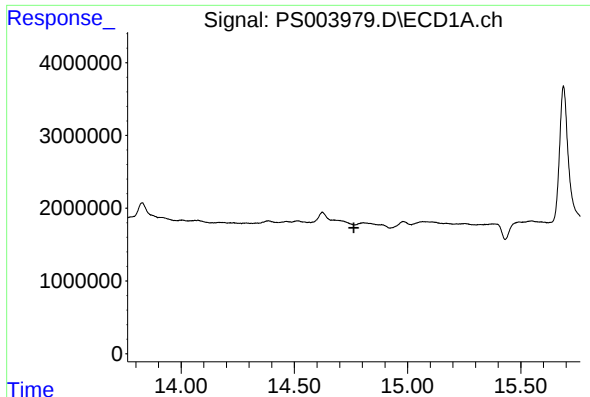

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2-D

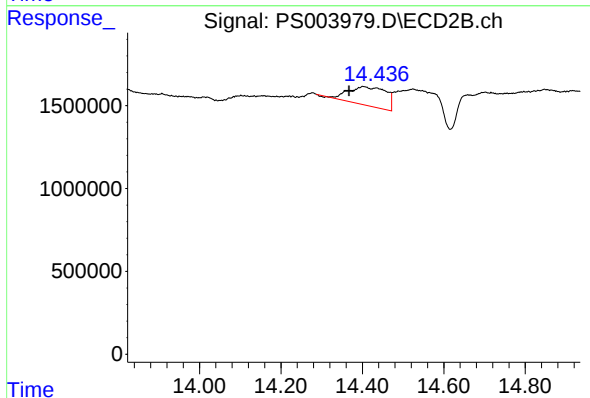


#12 2,4,5-T

R.T.: 14.403 min
Delta R.T.: 0.035 min
Response: 7213128
Conc: 3.32 ng/ml

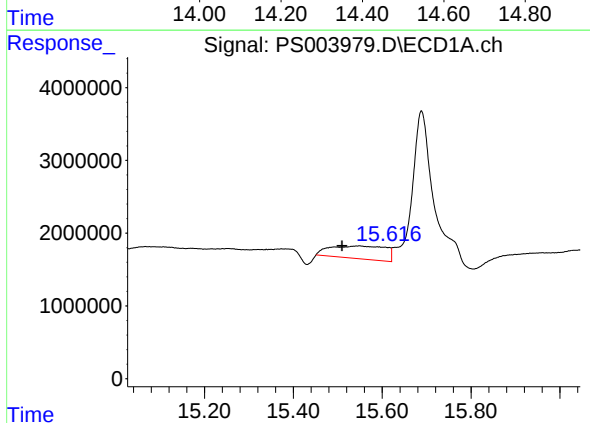


#13 2,4-DB

R.T.: 15.547 min
Delta R.T.: 0.037 min
Response: 15236812
Conc: 50.54 ng/ml

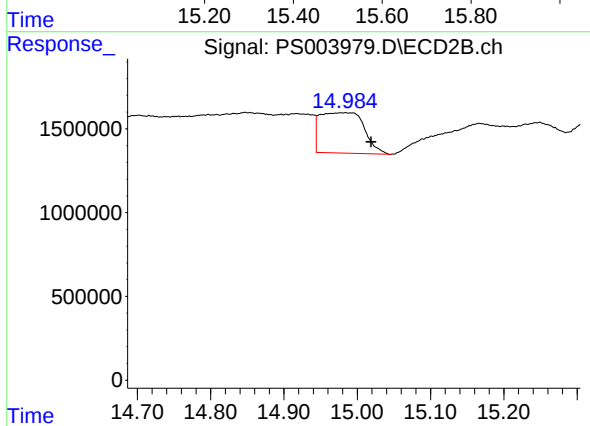

#13 2,4-DB


R.T.: 14.983 min
Delta R.T.: -0.035 min
Response: 10111631
Conc: 34.05 ng/ml

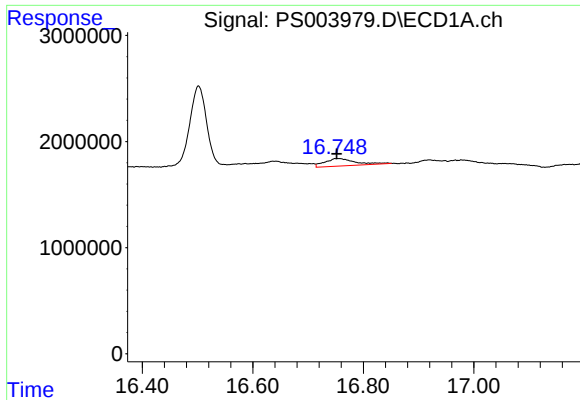

#15 Picloram

R.T.: 16.755 min
Delta R.T.: 0.003 min
Response: 2697363
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2-D

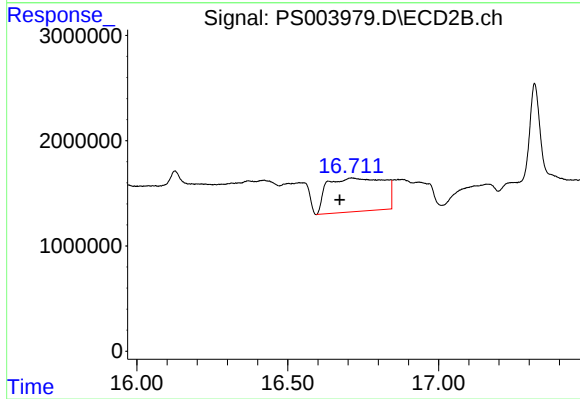

#15 Picloram

R.T.: 16.713 min
Delta R.T.: 0.040 min
Response: 41373805
Conc: 13.05 ng/ml