

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
 Data File : PS003980.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2019 03:53
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 13:23:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.296	10.796	241.2E6	212.7E6	552.914	433.520
Target Compounds							
3) T	4-Nitroph...	0.000	9.914	0	98168	N.D.	<MDL
7) T	MCPA	0.000	11.686	0	469897	N.D.	<MDL
8) T	DICHLORPROP	0.000	12.168	0	2049151	N.D.	4.402
9) T	2,4-D	0.000	12.629	0	487524	N.D.	<MDL
10) T	Pentachlo...	0.000	13.208	0	1028198	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.802	0	44214	N.D.	<MDL
12) T	2,4,5-T	0.000	14.369	0	14888	N.D.	<MDL
13) T	2,4-DB	0.000	15.027	0	578777	N.D.	1.949
14) T	DINOSEB	0.000	15.485	0	562653	N.D.	<MDL
15) T	Picloram	16.787	16.702	8197644	1627353	2.413	<MDL #
16) T	DCPA	0.000	16.641	0	3248625	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
Data File : PS003980.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2019 03:53
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 13:23:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

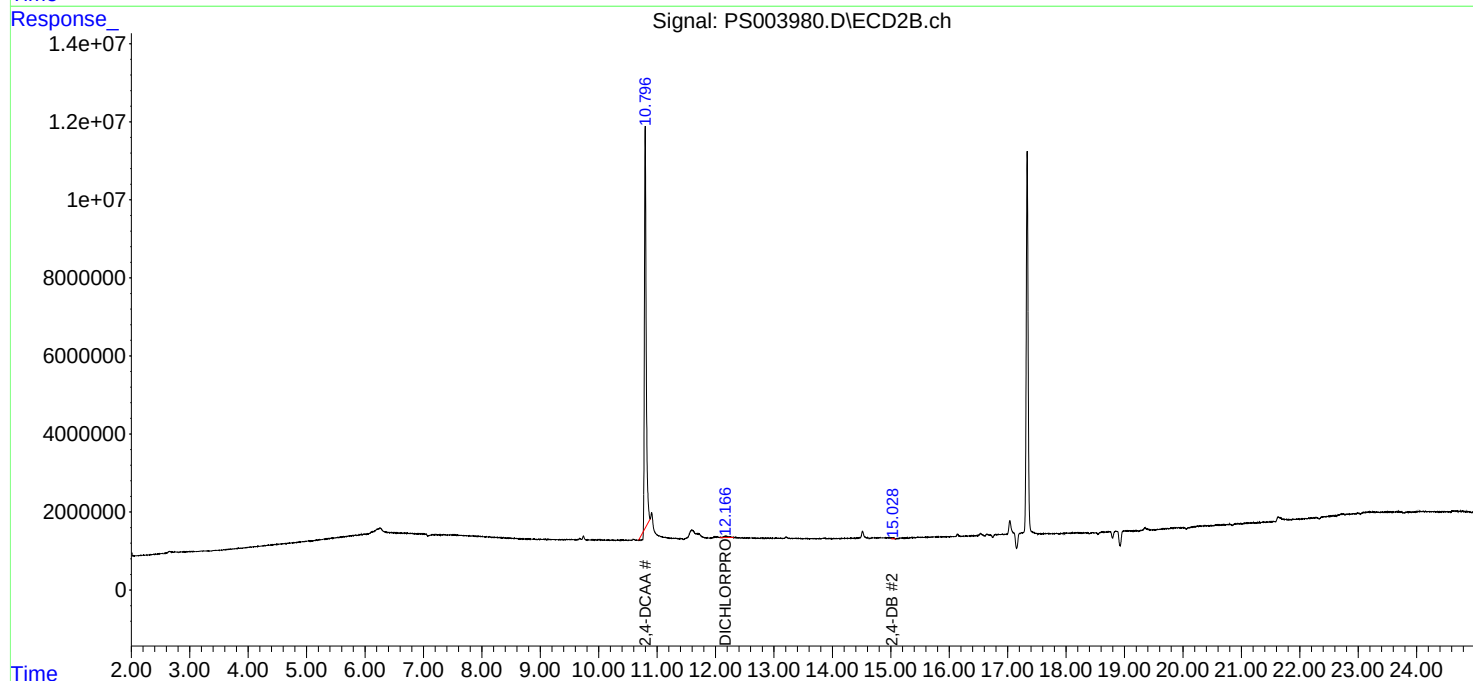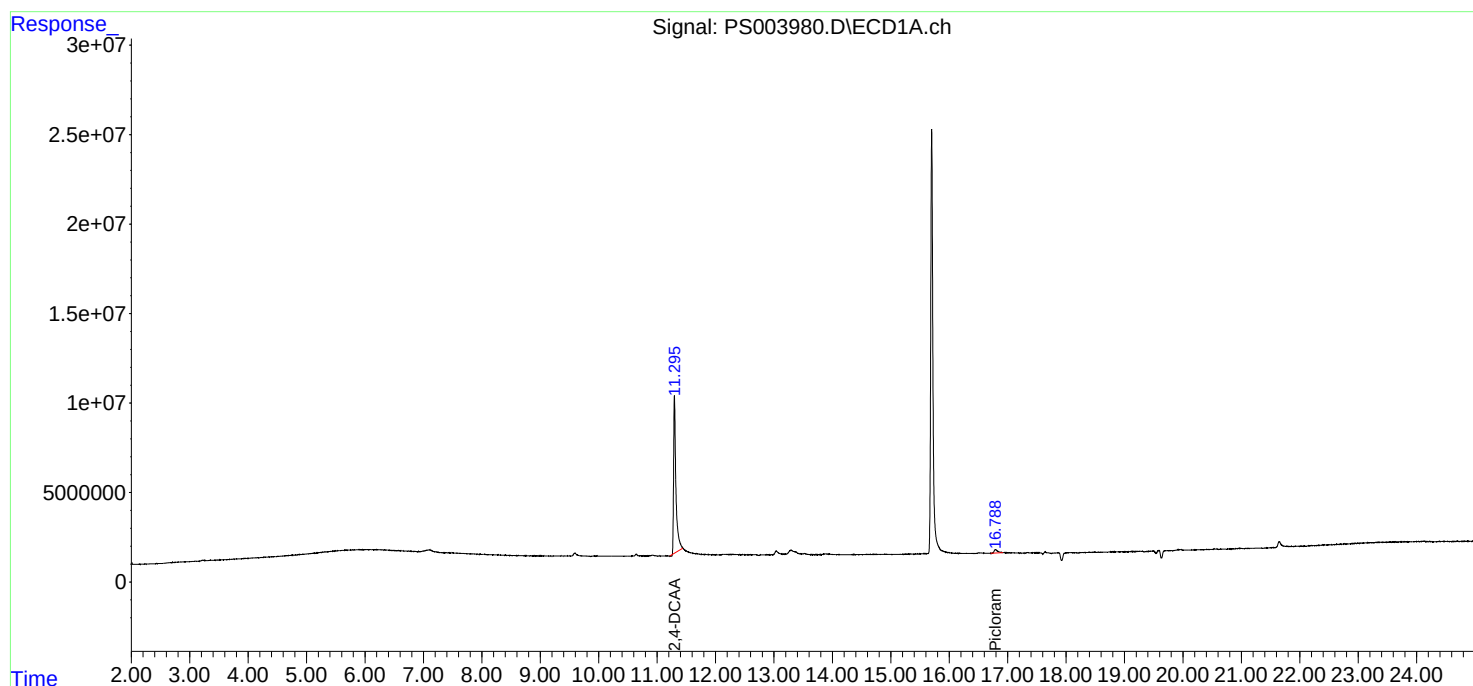


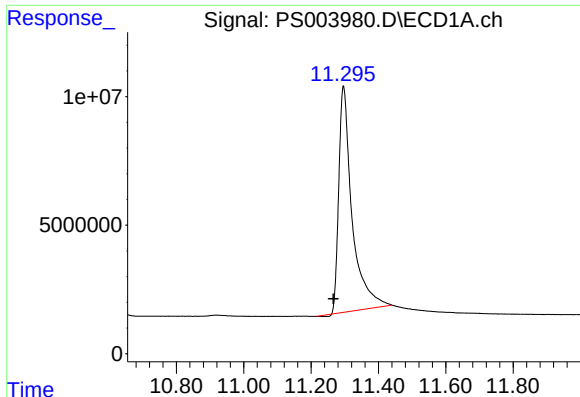

#4 2,4-DCAA


R.T.: 11.296 min
Delta R.T.: 0.029 min
Response: 241187767
Conc: 552.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

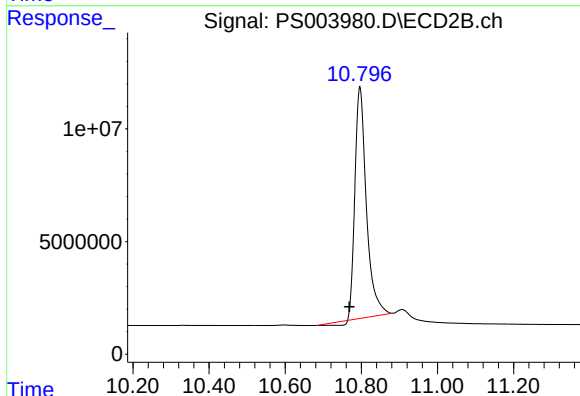


#4 2,4-DCAA

R.T.: 10.796 min
Delta R.T.: 0.028 min
Response: 212710299
Conc: 433.52 ng/ml

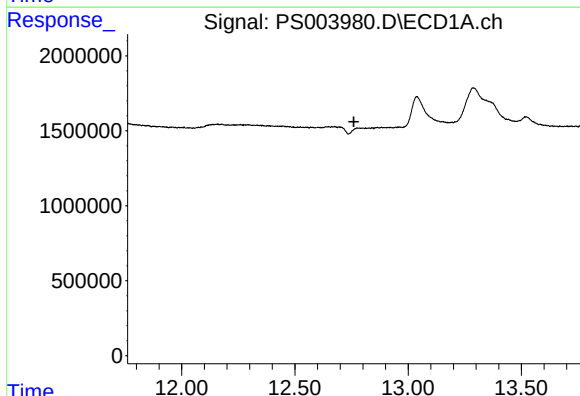


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.760 min
Response: 0
Conc: N.D.

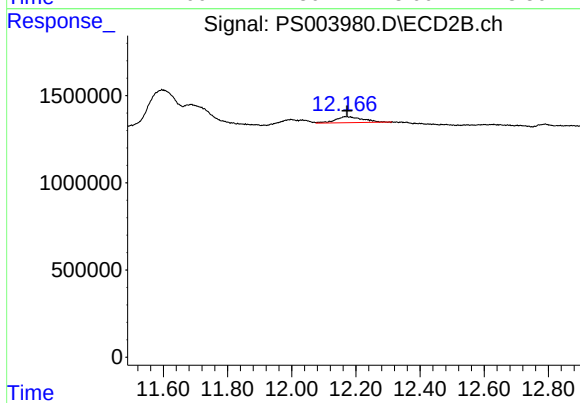

#8 DICHLORPROP


R.T.: 12.168 min
Delta R.T.: -0.005 min
Response: 2049151
Conc: 4.40 ng/ml

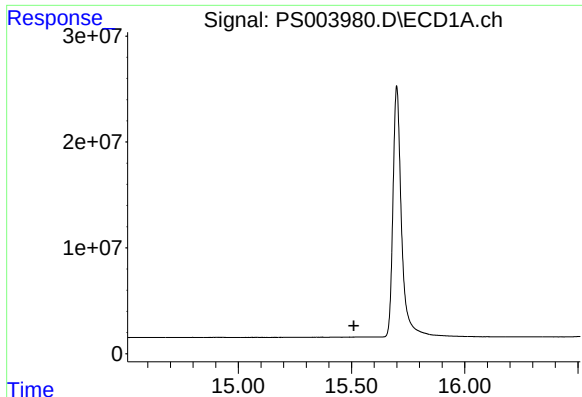

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

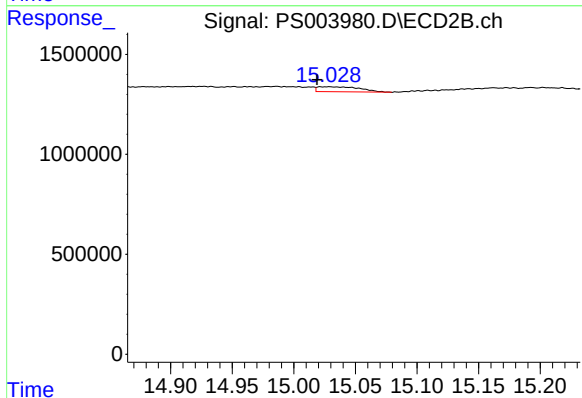


#13 2,4-DB

R.T.: 15.027 min
Delta R.T.: 0.008 min
Response: 578777
Conc: 1.95 ng/ml

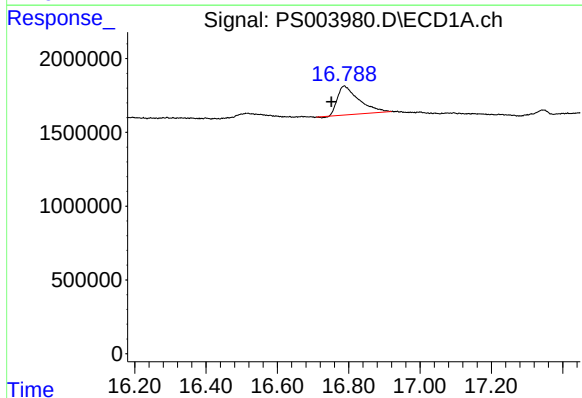

#15 Picloram

R.T.: 16.787 min
Delta R.T.: 0.036 min
Response: 8197644
Conc: 2.41 ng/ml

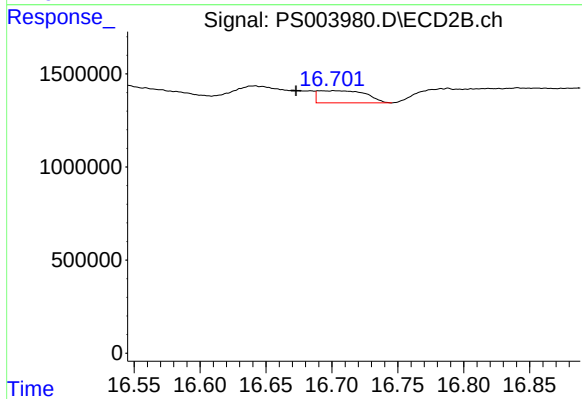

#15 Picloram

R.T.: 16.702 min
Delta R.T.: 0.029 min
Response: 1627353
Conc: N.D.