

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
 Data File : PS003983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2019 05:27
 Operator : EI\SJ
 Sample : K2214-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-2-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 12:35:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.290	10.785	55195254	49157807	126.533	100.187
Target Compounds							
1) T	Dalapon	2.801	2.302	52817684	92740203	70.845	127.106 #
2) T	3,5-DICHL...	0.000	8.945	0	5568635	N.D.	8.730
3) T	4-Nitroph...	0.000	9.949	0	13826756	N.D.	60.901
5) T	DICAMBA	0.000	11.020	0	2768015	N.D.	1.488
7) T	MCPA	12.097	0.000	759.8E6	0	360.143	N.D. #
9) T	2,4-D	0.000	12.637	0	1129626	N.D.	2.124
10) T	Pentachlo...	0.000	13.172	0	268047	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.782	0	2869861	N.D.	1.084
12) T	2,4,5-T	0.000	14.374	0	1225957	N.D.	<MDL
13) T	2,4-DB	15.545	14.988	6158940	8692886	20.427	29.274 #
14) T	DINOSEB	0.000	15.406	0	382201	N.D.	<MDL
15) T	Picloram	0.000	16.731	0	26234986	N.D.	8.273
16) T	DCPA	0.000	16.551	0	9632882	N.D.	2.850



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
Data File : PS003983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2019 05:27
Operator : EI\SJ
Sample : K2214-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-2-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 12:35:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

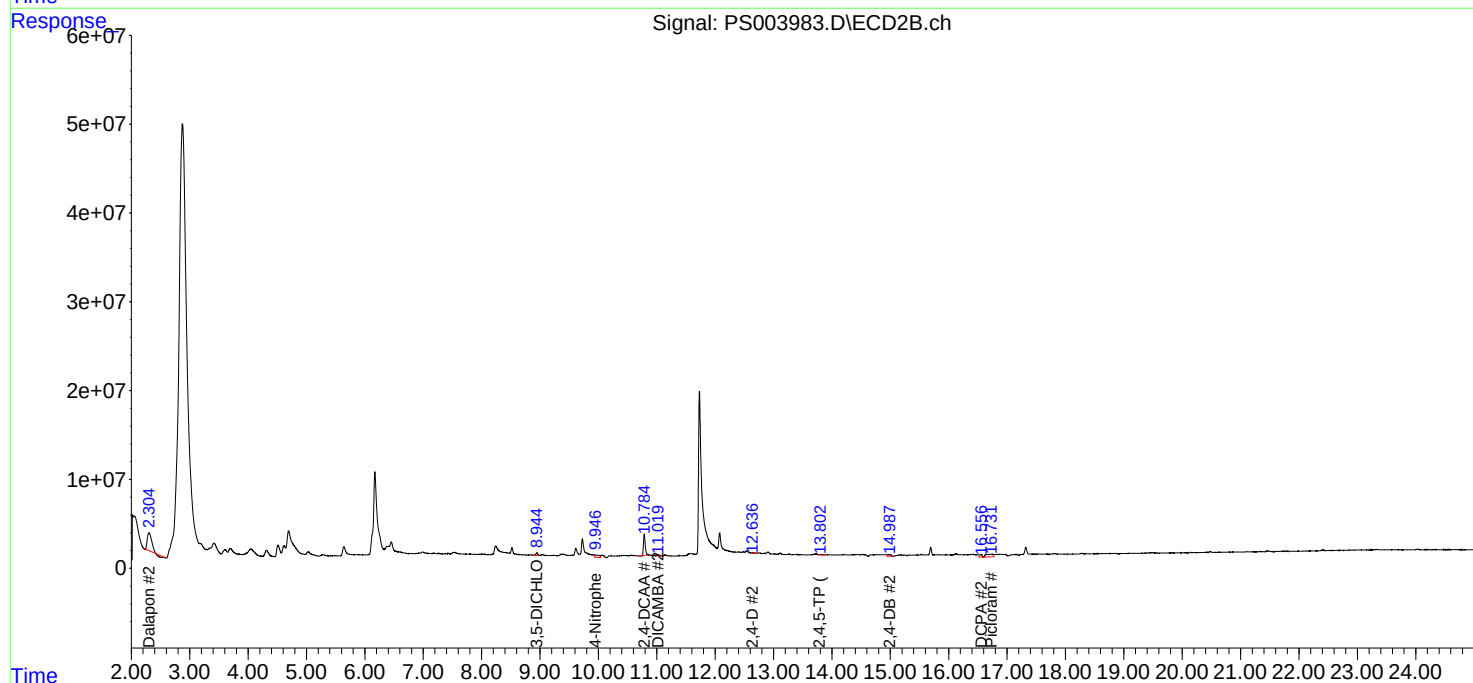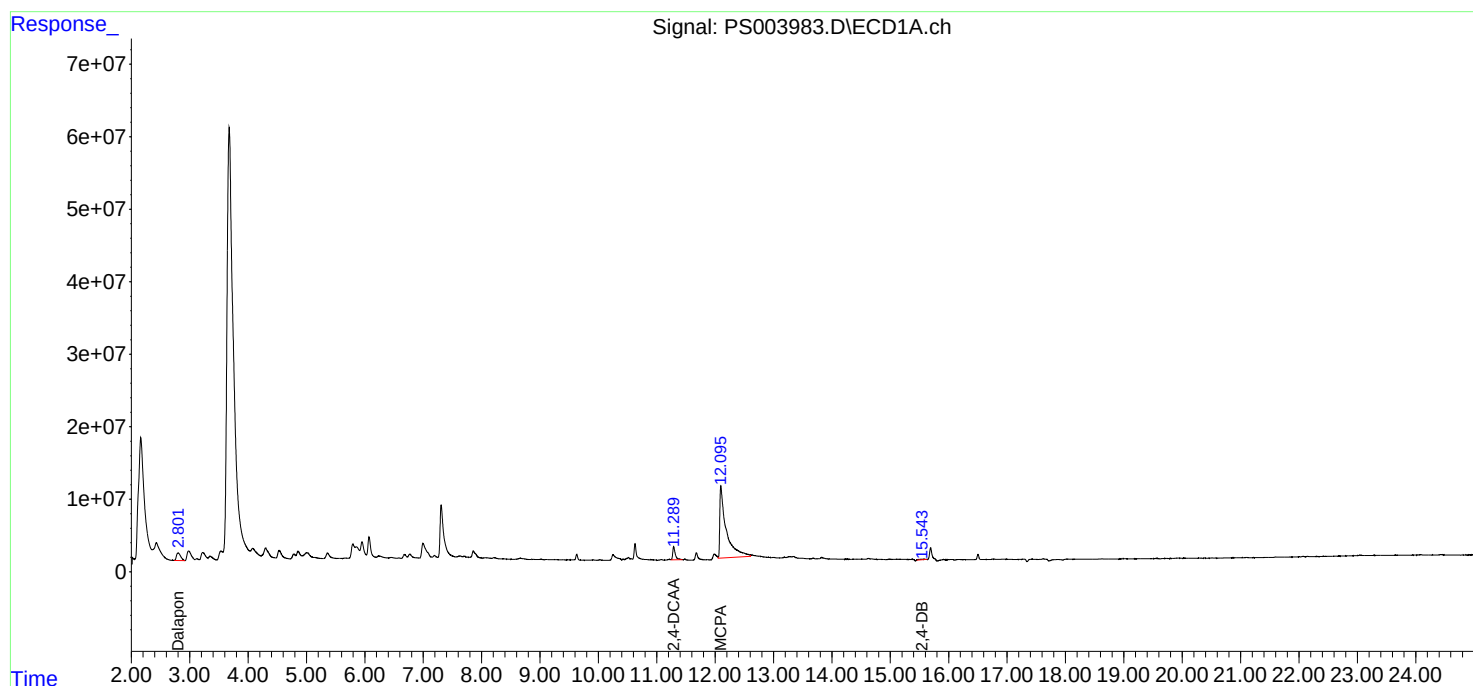


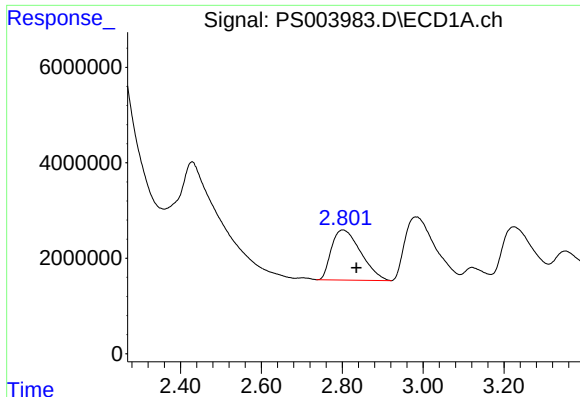

#1 Dalapon


R.T.: 2.801 min
Delta R.T.: -0.034 min
Response: 52817684
Conc: 70.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-2-S

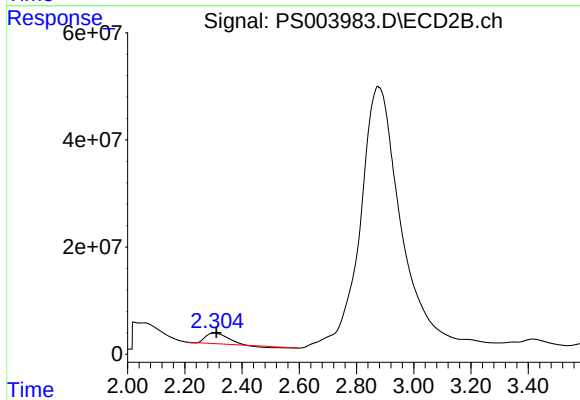


#1 Dalapon

R.T.: 2.302 min
Delta R.T.: -0.008 min
Response: 92740203
Conc: 127.11 ng/ml

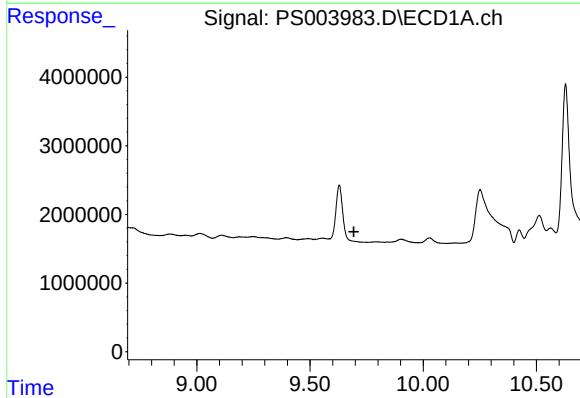


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

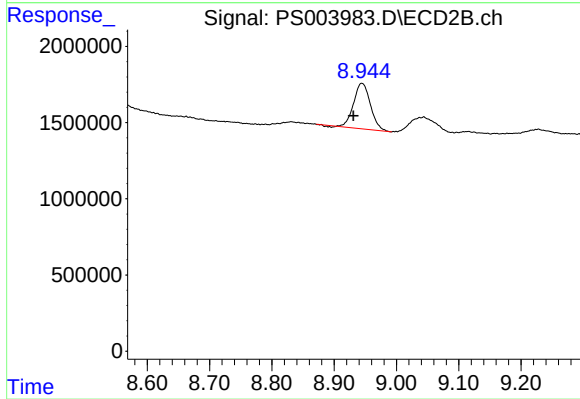

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.945 min
Delta R.T.: 0.014 min
Response: 5568635
Conc: 8.73 ng/ml

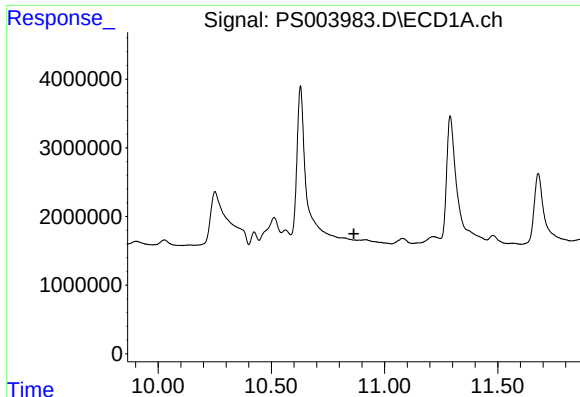

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2-S

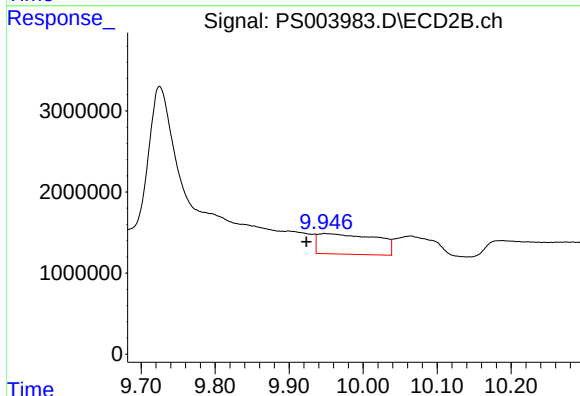


#3 4-Nitrophenol

R.T.: 9.949 min
Delta R.T.: 0.025 min
Response: 13826756
Conc: 60.90 ng/ml

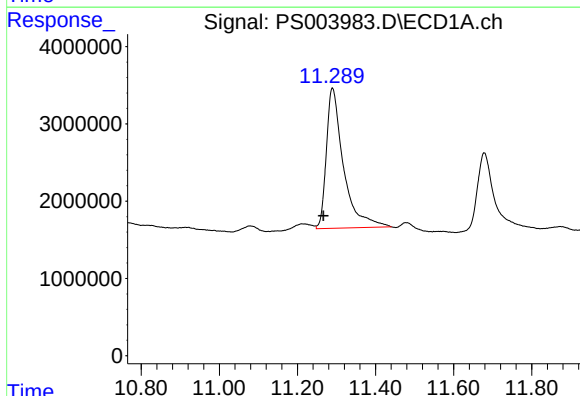


#4 2,4-DCAA

R.T.: 11.290 min
Delta R.T.: 0.023 min
Response: 55195254
Conc: 126.53 ng/ml

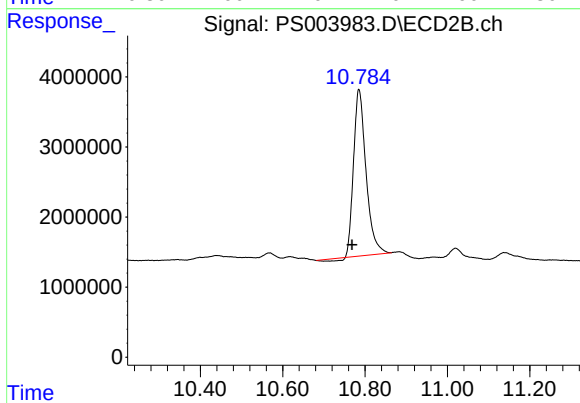

#4 2,4-DCAA


R.T.: 10.785 min
Delta R.T.: 0.017 min
Response: 49157807
Conc: 100.19 ng/ml

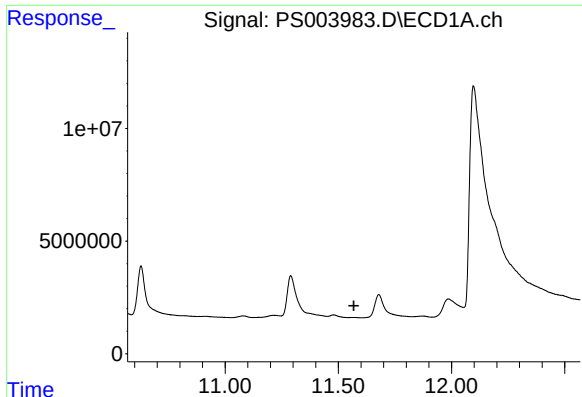

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2-S

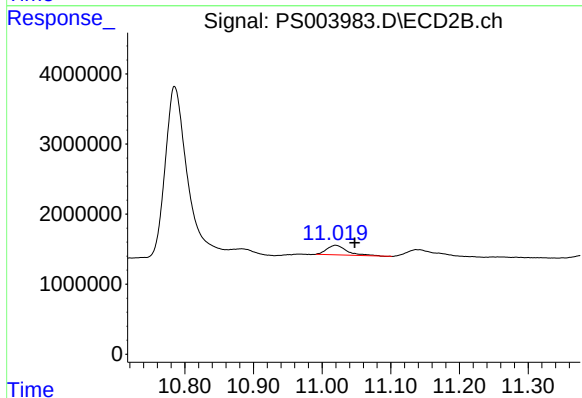


#5 DICAMBA

R.T.: 11.020 min
Delta R.T.: -0.028 min
Response: 2768015
Conc: 1.49 ng/ml

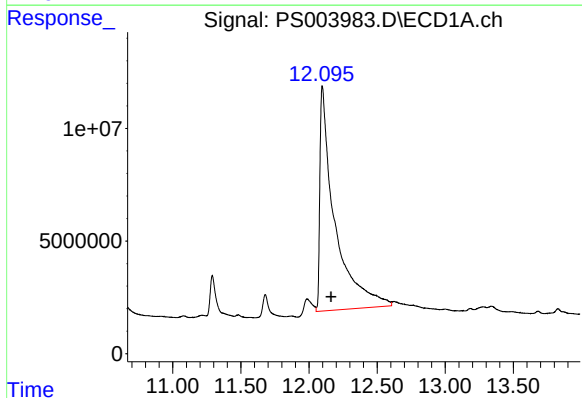


#7 MCPA

R.T.: 12.097 min
Delta R.T.: -0.064 min
Response: 759823255
Conc: 360.14 ug/ml

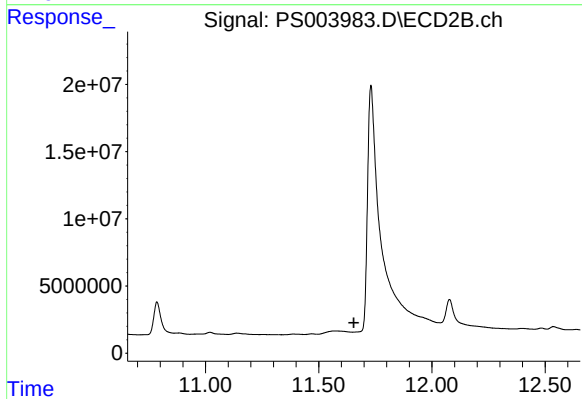

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.655 min
Response: 0
Conc: N.D.

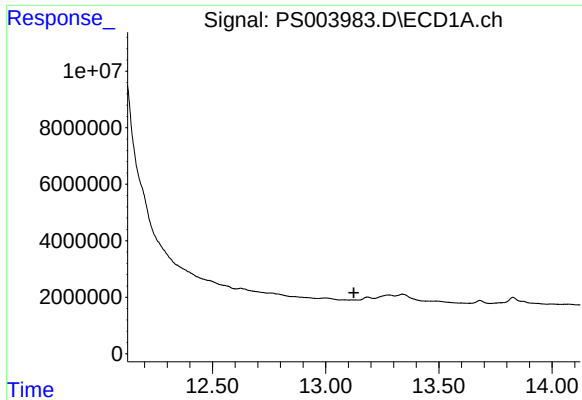

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2-S

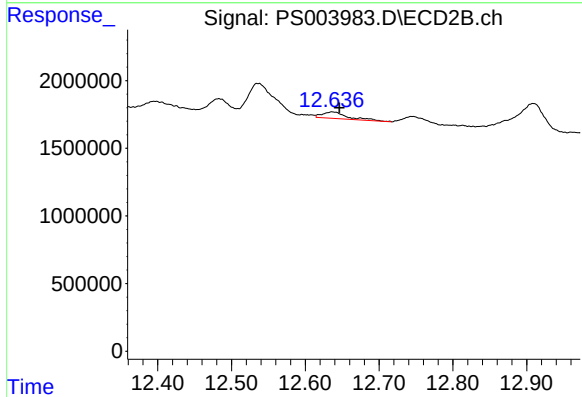


#9 2,4-D

R.T.: 12.637 min
Delta R.T.: -0.009 min
Response: 1129626
Conc: 2.12 ng/ml

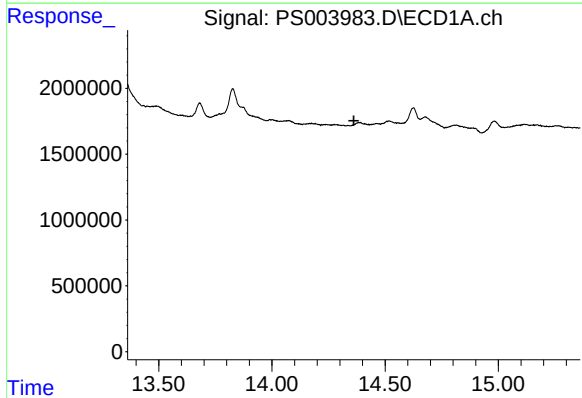


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

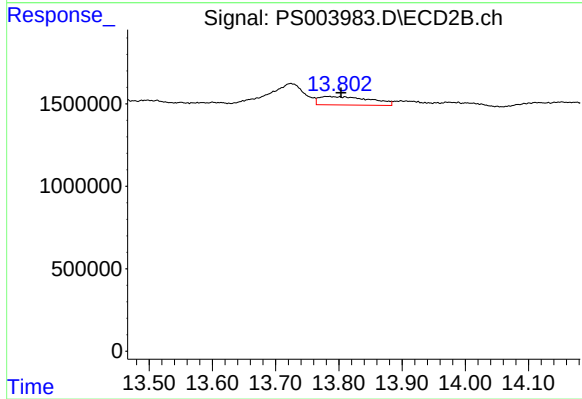

#11 2,4,5-TP (SILVEX)


R.T.: 13.782 min
Delta R.T.: -0.021 min
Response: 2869861
Conc: 1.08 ng/ml

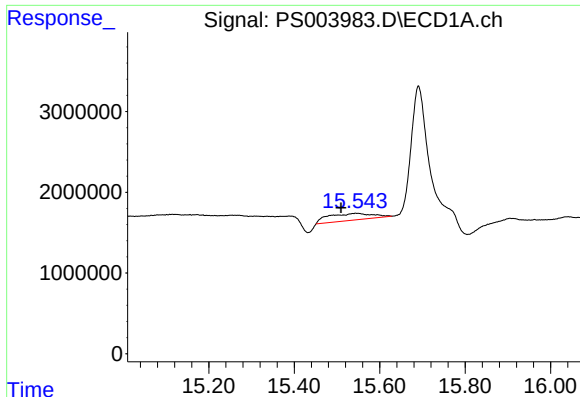

#13 2,4-DB


R.T.: 15.545 min
Delta R.T.: 0.035 min
Response: 6158940
Conc: 20.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-2-S

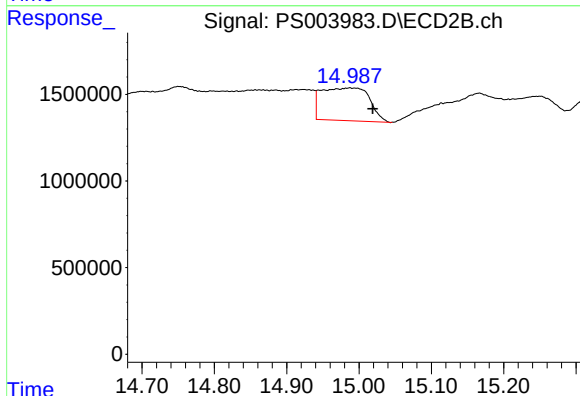


#13 2,4-DB

R.T.: 14.988 min
Delta R.T.: -0.031 min
Response: 8692886
Conc: 29.27 ng/ml

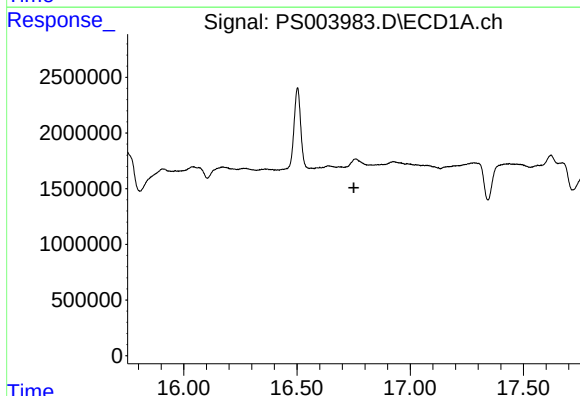


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.752 min
Response: 0
Conc: N.D.

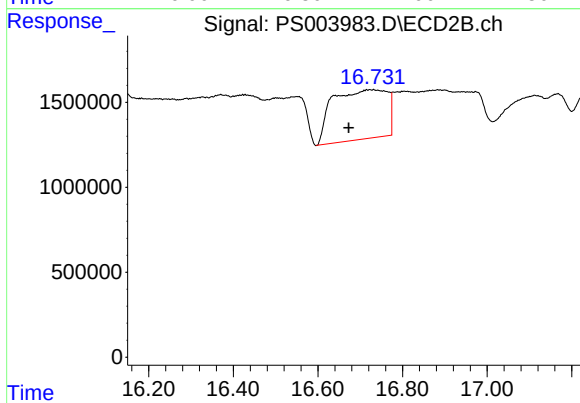

#15 Picloram


R.T.: 16.731 min
Delta R.T.: 0.058 min
Response: 26234986
Conc: 8.27 ng/ml

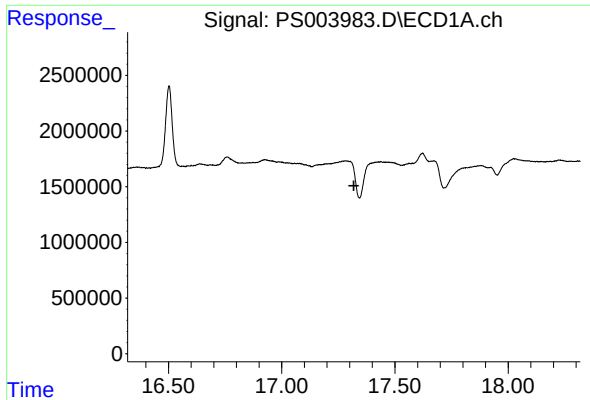

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2-S

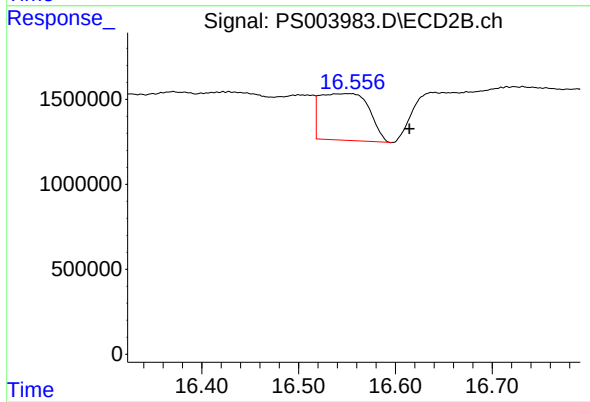

#16 DCPA

R.T.: 16.551 min
Delta R.T.: -0.064 min
Response: 9632882
Conc: 2.85 ng/ml