

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
 Data File : PS003984.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2019 05:58
 Operator : EI\SJ
 Sample : PB118510BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB118510BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 12:35:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.265	10.765	151.4E6	140.0E6	347.125	285.260
Target Compounds							
1) T	Dalapon	2.787	2.285	53397092	149.9E6	71.623	205.462 #
2) T	3,5-DICHL...	0.000	8.930	0	5650262	N.D.	8.858
3) T	4-Nitroph...	0.000	9.937	0	10410522	N.D.	45.854
7) T	MCPA	12.093	0.000	630.7E6	0	298.925	N.D. #
9) T	2,4-D	0.000	12.622	0	1636561	N.D.	3.077
11) T	2,4,5-TP ...	0.000	13.770	0	1930588	N.D.	<MDL
12) T	2,4,5-T	0.000	14.427	0	6576753	N.D.	3.025
13) T	2,4-DB	0.000	14.968	0	5494978	N.D.	18.505
14) T	DINOSEB	0.000	15.501	0	4267382	N.D.	2.224
15) T	Picloram	0.000	16.700	0	15192870	N.D.	4.791



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
Data File : PS003984.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2019 05:58
Operator : EI\SJ
Sample : PB118510BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB118510BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 12:35:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

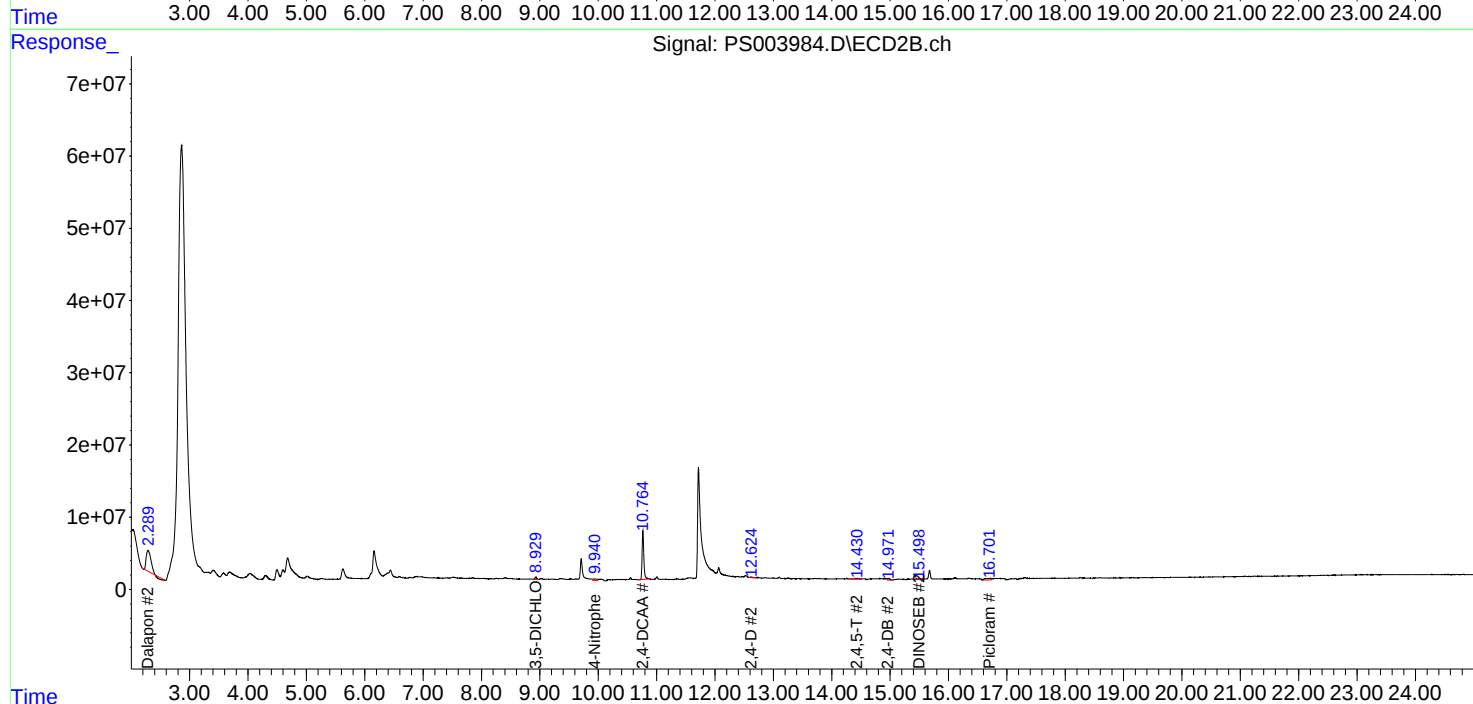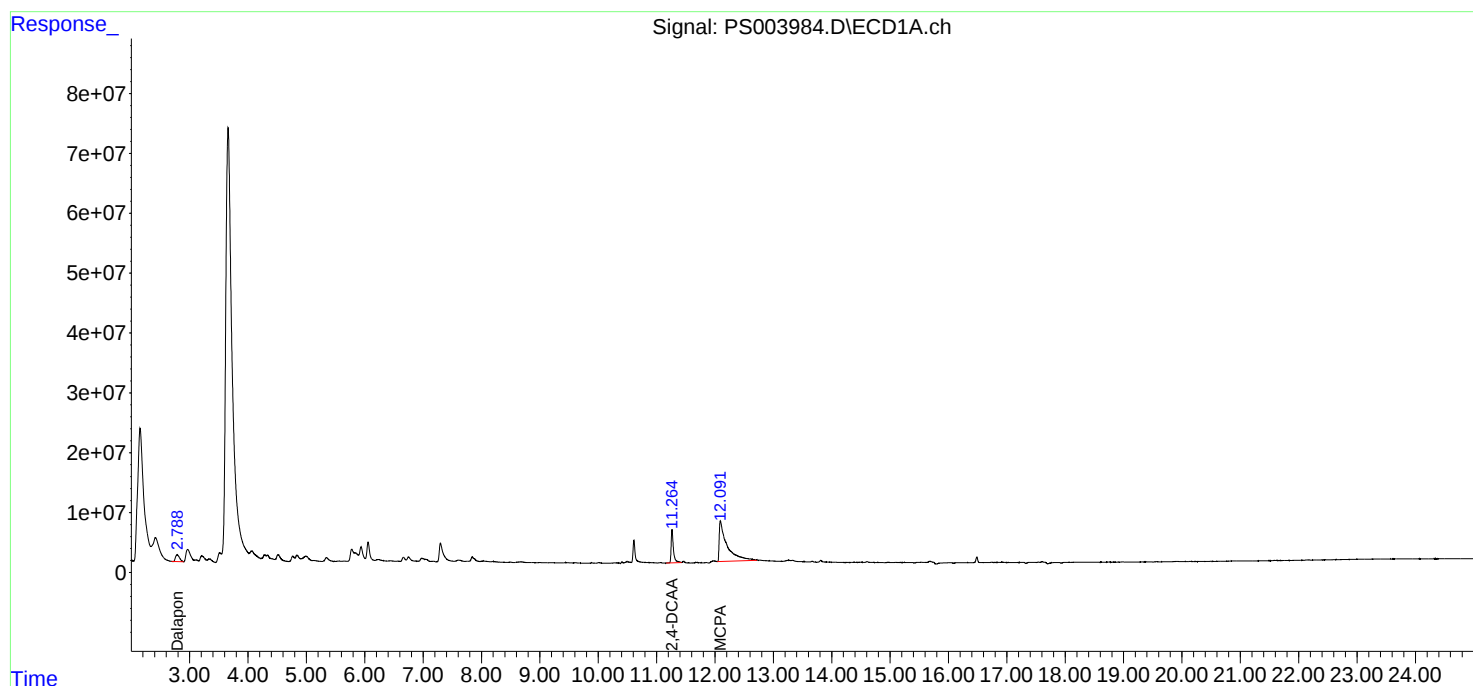


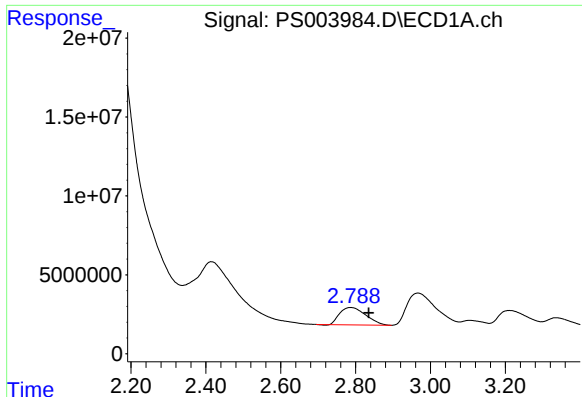

#1 Dalapon


R.T.: 2.787 min
Delta R.T.: -0.048 min
Response: 53397092
Conc: 71.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB118510BL

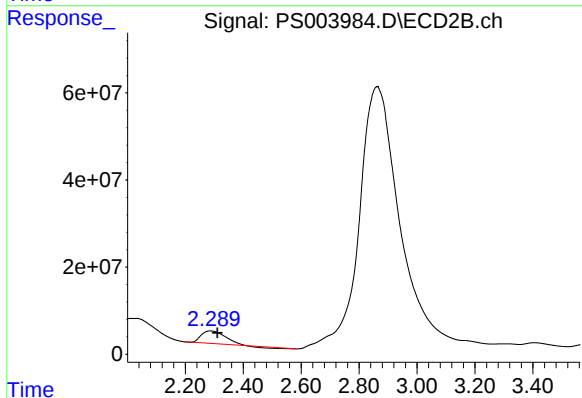


#1 Dalapon

R.T.: 2.285 min
Delta R.T.: -0.025 min
Response: 149910918
Conc: 205.46 ng/ml

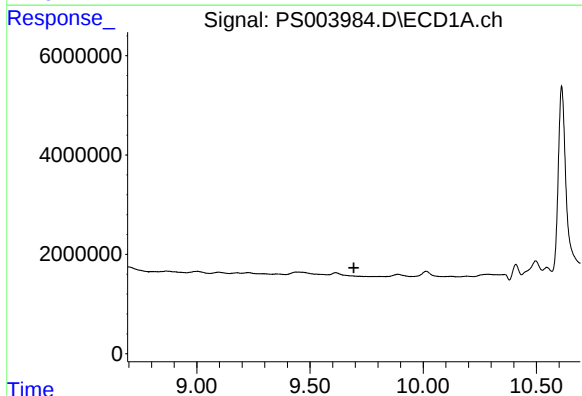


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

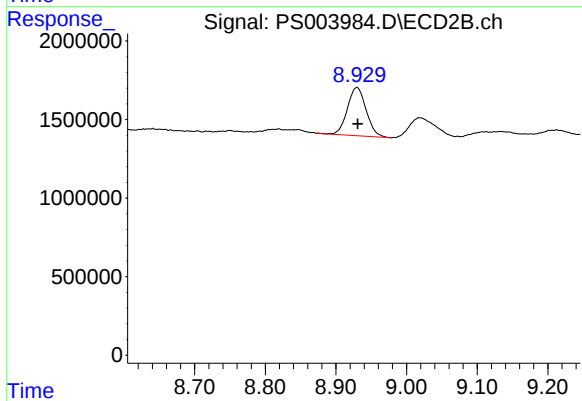

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.930 min
Delta R.T.: -0.001 min
Response: 5650262
Conc: 8.86 ng/ml

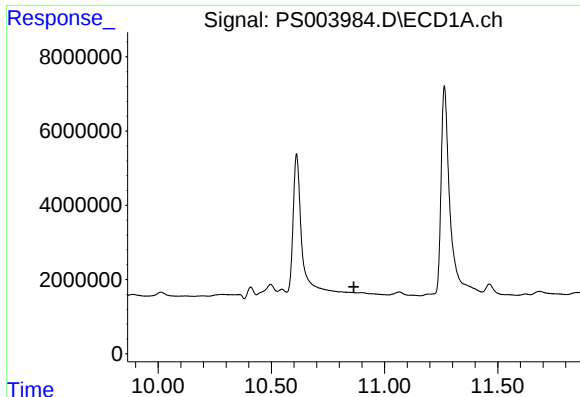

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118510BL

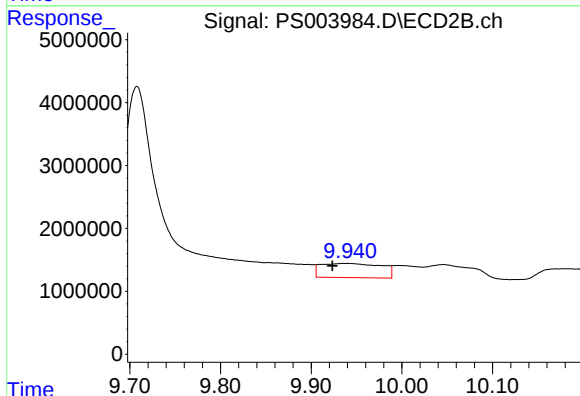


#3 4-Nitrophenol

R.T.: 9.937 min
Delta R.T.: 0.014 min
Response: 10410522
Conc: 45.85 ng/ml

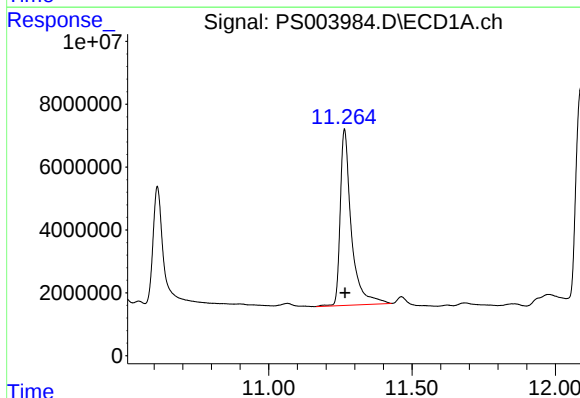


#4 2,4-DCAA

R.T.: 11.265 min
Delta R.T.: -0.002 min
Response: 151420065
Conc: 347.12 ng/ml

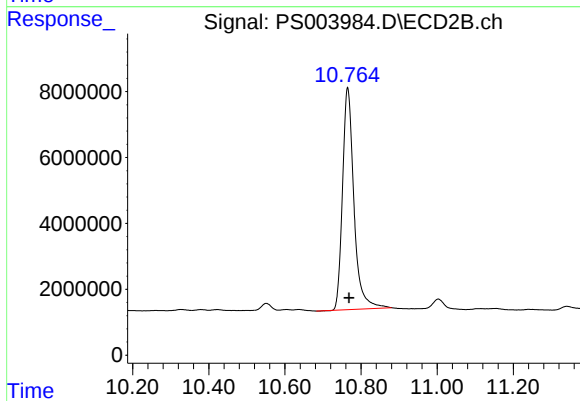

#4 2,4-DCAA


R.T.: 10.765 min
Delta R.T.: -0.004 min
Response: 139964975
Conc: 285.26 ng/ml

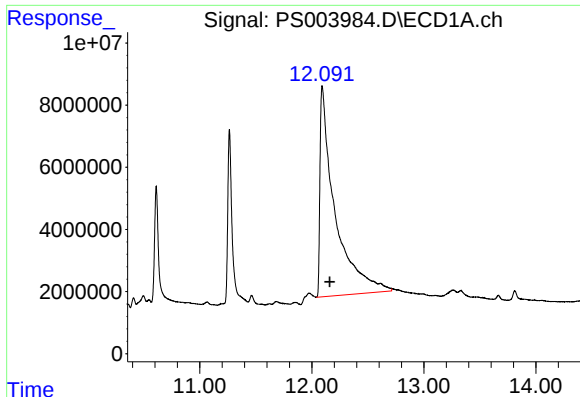

#7 MCPA


R.T.: 12.093 min
Delta R.T.: -0.068 min
Response: 630667171
Conc: 298.93 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB118510BL

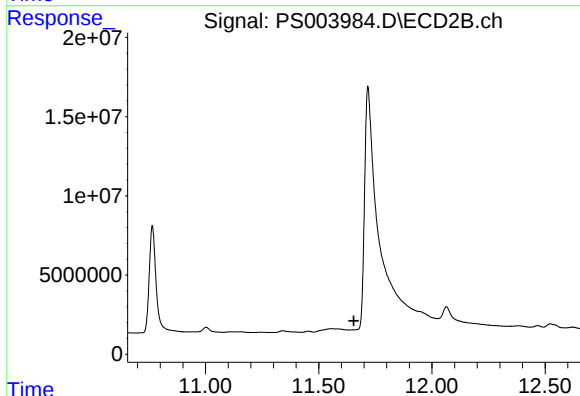


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.655 min
Response: 0
Conc: N.D.

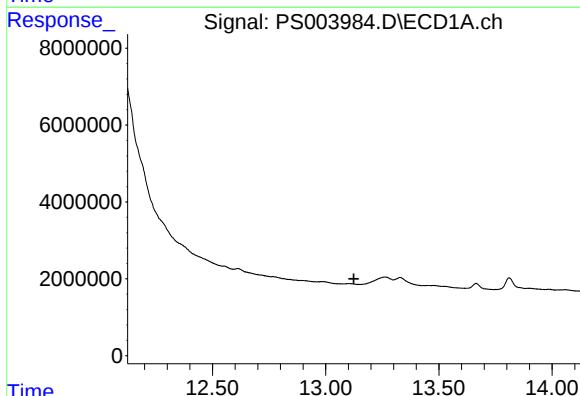


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.125 min
Response: 0
Conc: N.D.

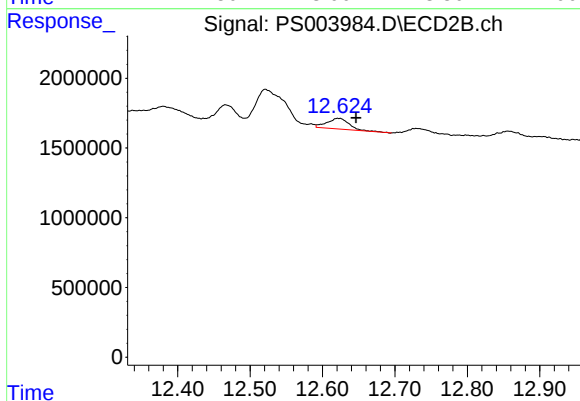

#9 2,4-D


R.T.: 12.622 min
Delta R.T.: -0.025 min
Response: 1636561
Conc: 3.08 ng/ml

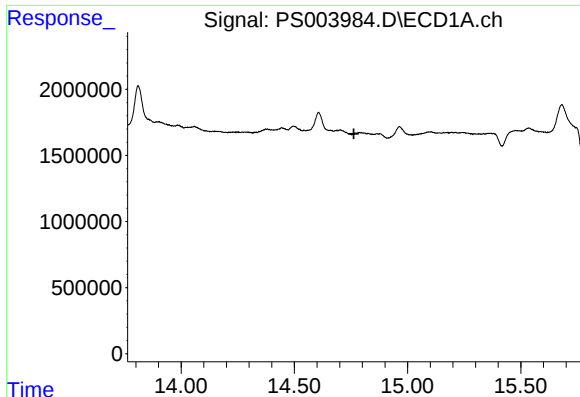

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118510BL

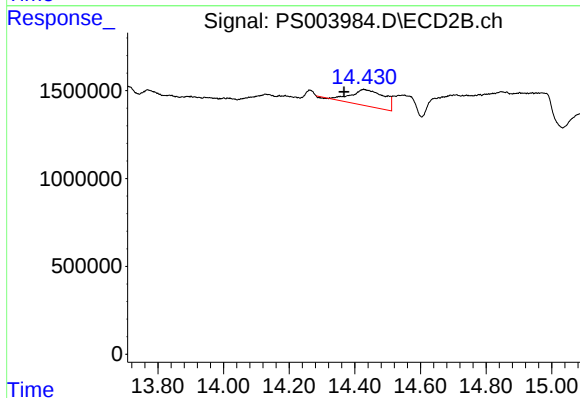


#12 2,4,5-T

R.T.: 14.427 min
Delta R.T.: 0.060 min
Response: 6576753
Conc: 3.03 ng/ml

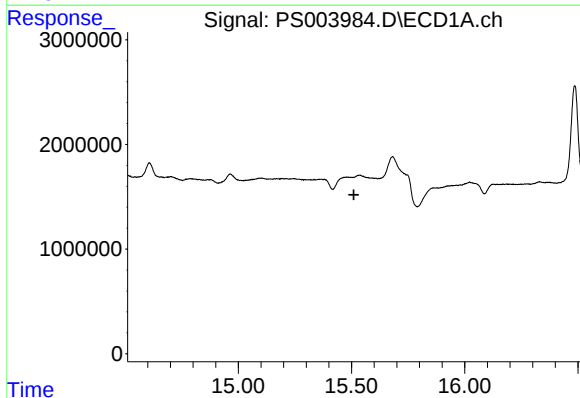


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

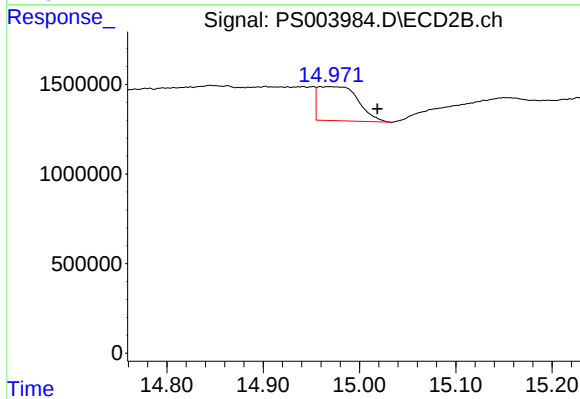

#13 2,4-DB


R.T.: 14.968 min
Delta R.T.: -0.051 min
Response: 5494978
Conc: 18.50 ng/ml

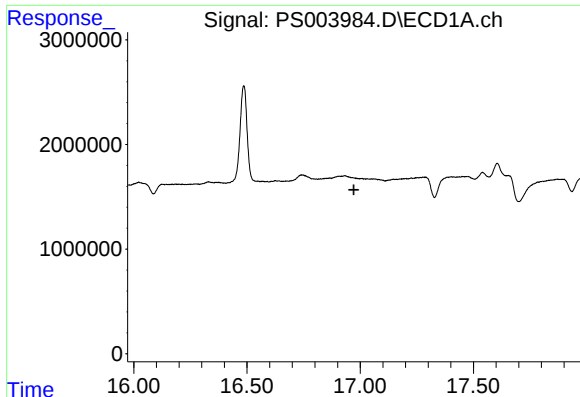

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118510BL

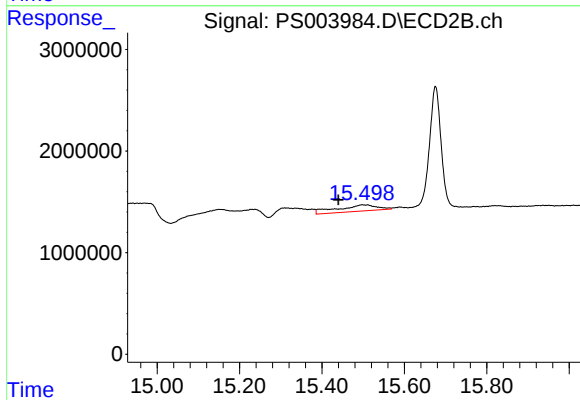


#14 DINOSEB

R.T.: 15.501 min
Delta R.T.: 0.061 min
Response: 4267382
Conc: 2.22 ng/ml

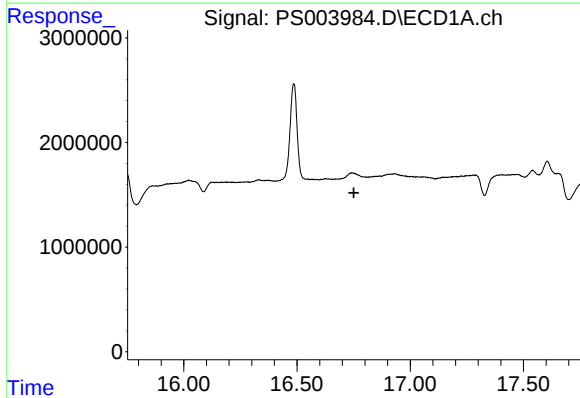

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.752 min
Response: 0
Conc: N.D.

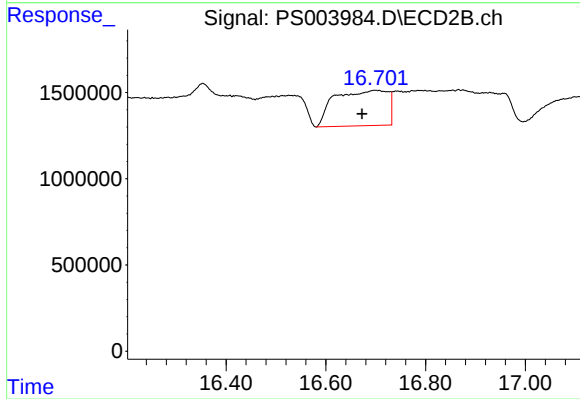

#15 Picloram

R.T.: 16.700 min
Delta R.T.: 0.027 min
Response: 15192870
Conc: 4.79 ng/ml