

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
 Data File : PS003987.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2019 07:32
 Operator : EI\SJ
 Sample : PB118577BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB118577BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 12:37:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.300	10.780	128.9E6	122.0E6	295.433	248.709
Target Compounds							
1) T	Dalapon	2.824	2.311	47547634	125.7E6	63.777	172.319 #
2) T	3,5-DICHL...	0.000	8.944	0	4071419	N.D.	6.383
3) T	4-Nitroph...	0.000	9.951	0	14415322	N.D.	63.494
5) T	DICAMBA	0.000	11.017	0	4050916	N.D.	2.178
7) T	MCPA	12.140	0.000	506.9E6	0	240.250	N.D. #
9) T	2,4-D	0.000	12.636	0	1401896	N.D.	2.636
10) T	Pentachlo...	0.000	13.176	0	381301	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.784	0	1438845	N.D.	<MDL
13) T	2,4-DB	15.567	14.988	14397751	4438624	47.753	14.947 #
15) T	Picloram	0.000	16.708	0	10447453	N.D.	3.294
16) T	DCPA	0.000	16.637	0	3363921	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
Data File : PS003987.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2019 07:32
Operator : EI\SJ
Sample : PB118577BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB118577BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 12:37:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

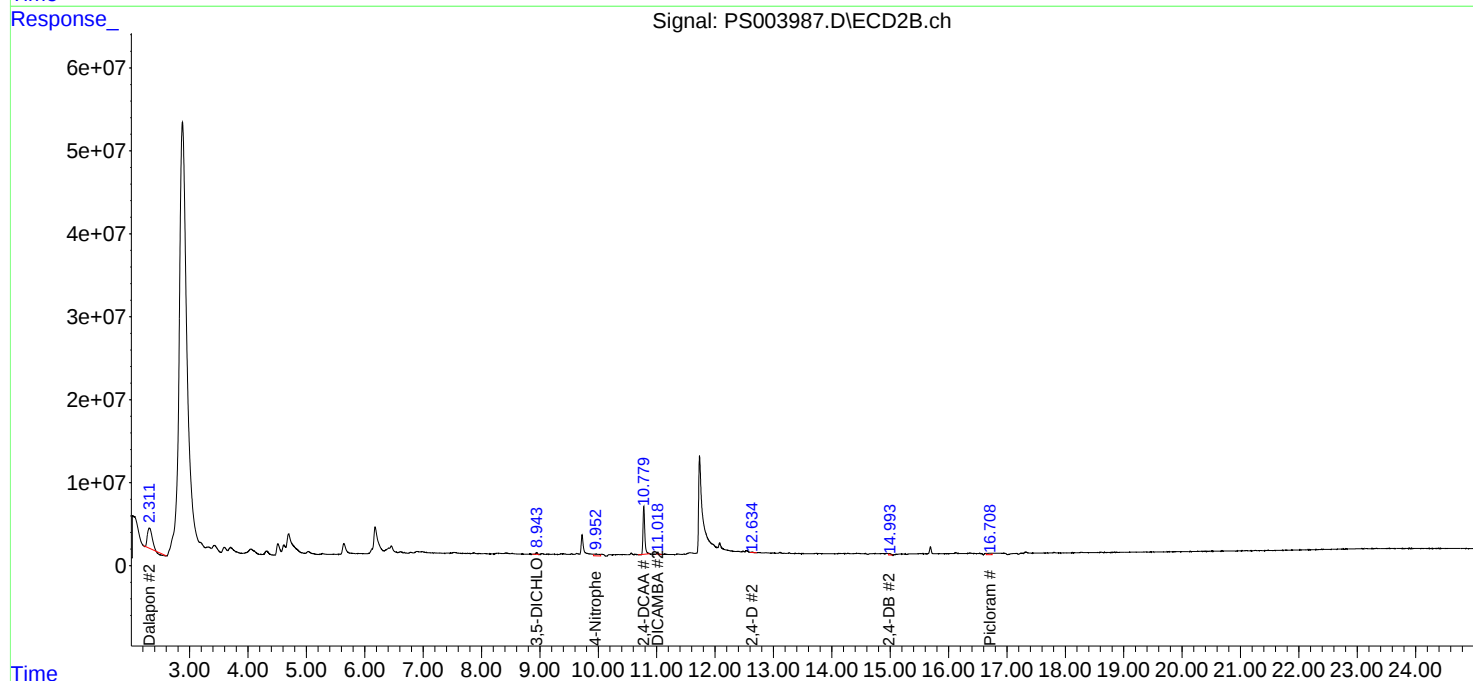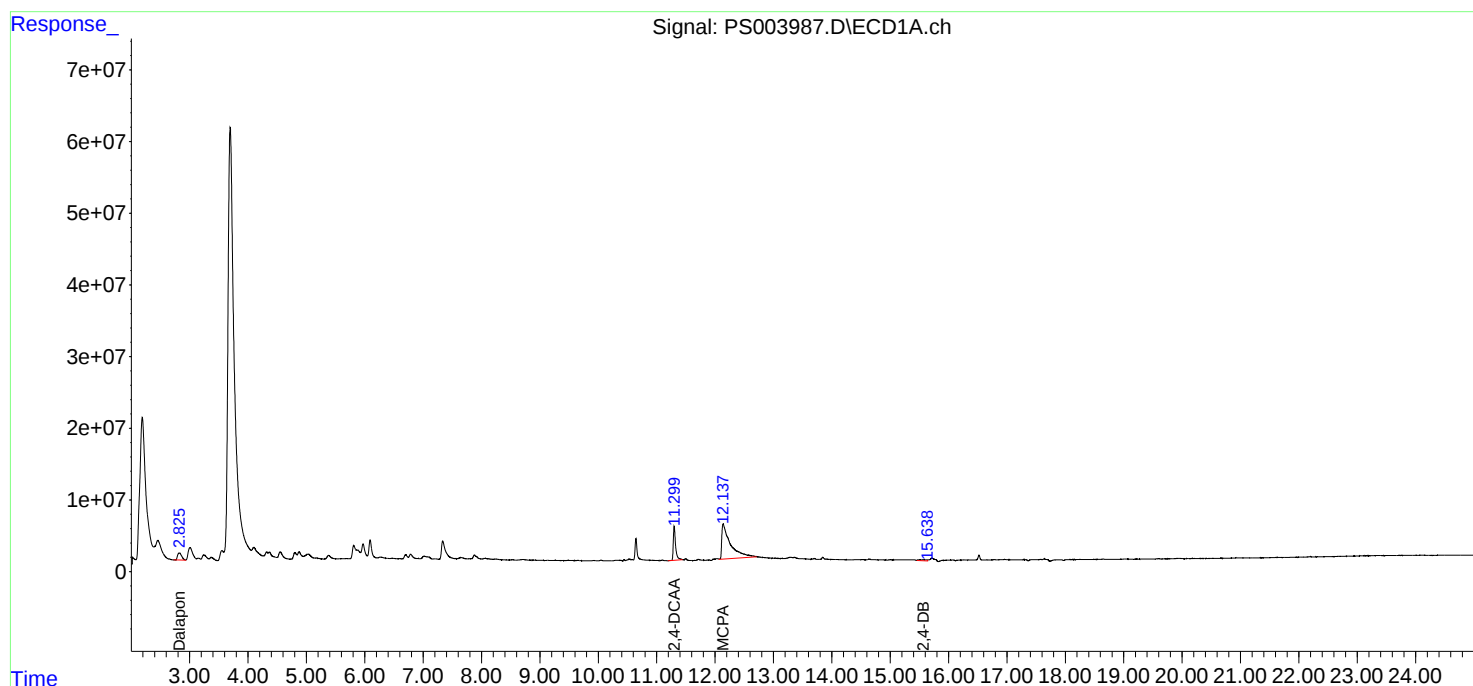


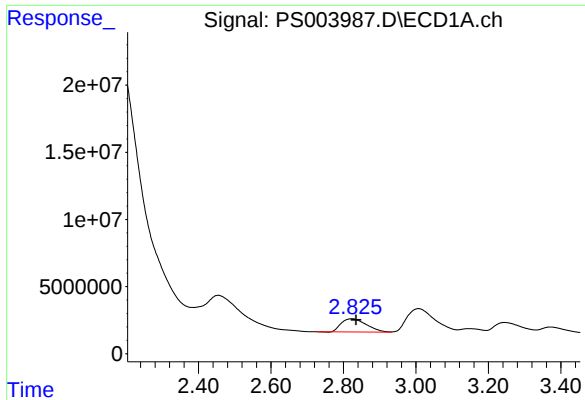

#1 Dalapon


R.T.: 2.824 min
Delta R.T.: -0.011 min
Response: 47547634
Conc: 63.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB118577BL

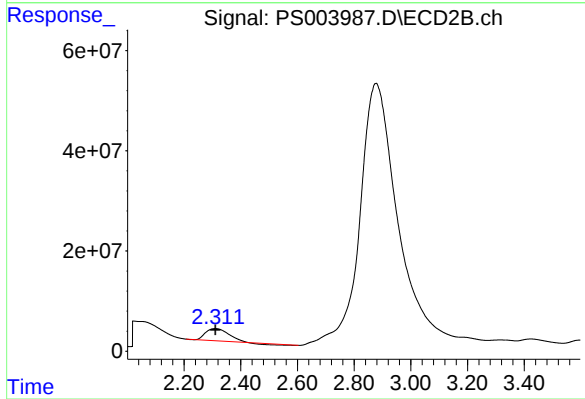


#1 Dalapon

R.T.: 2.311 min
Delta R.T.: 0.000 min
Response: 125728864
Conc: 172.32 ng/ml

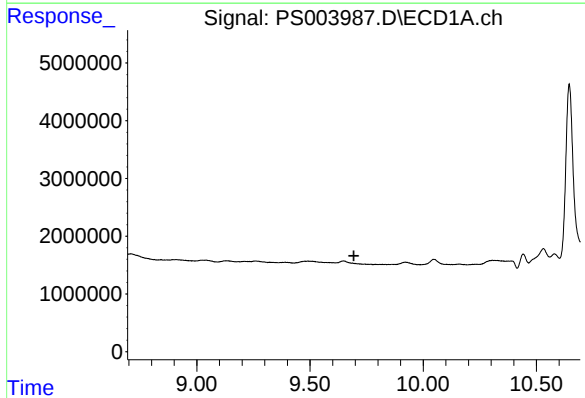


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

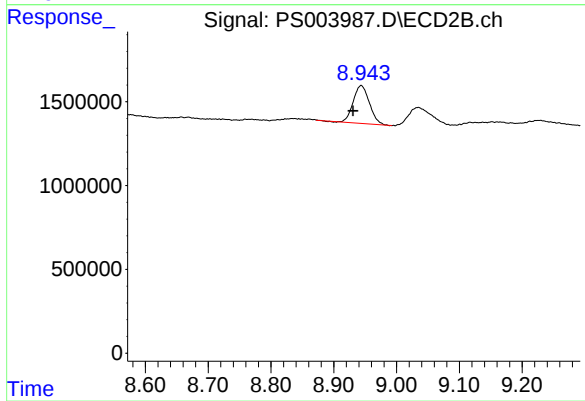

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.944 min
Delta R.T.: 0.013 min
Response: 4071419
Conc: 6.38 ng/ml

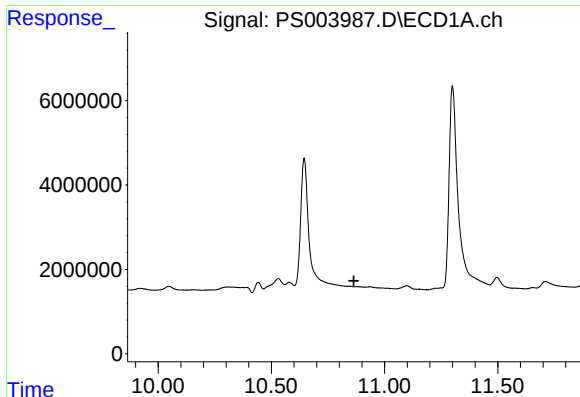

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118577BL

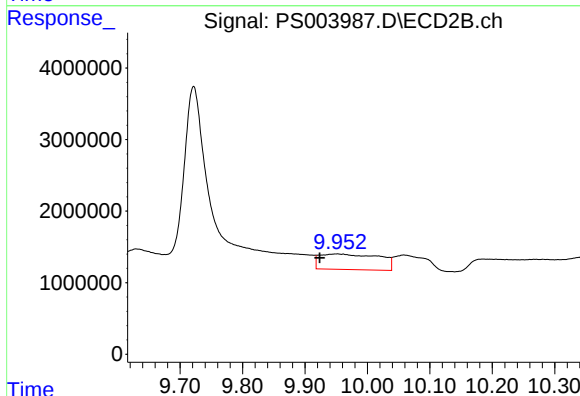


#3 4-Nitrophenol

R.T.: 9.951 min
Delta R.T.: 0.028 min
Response: 14415322
Conc: 63.49 ng/ml

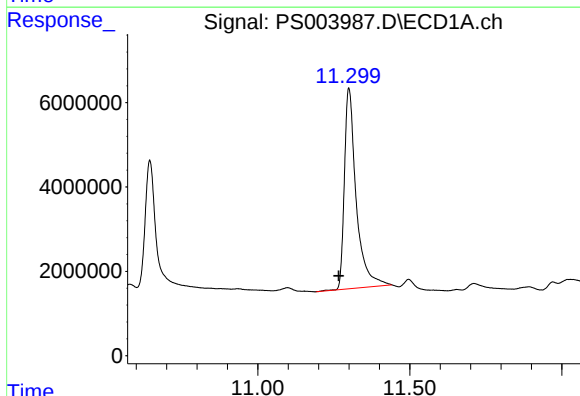


#4 2,4-DCAA

R.T.: 11.300 min
Delta R.T.: 0.034 min
Response: 128871448
Conc: 295.43 ng/ml

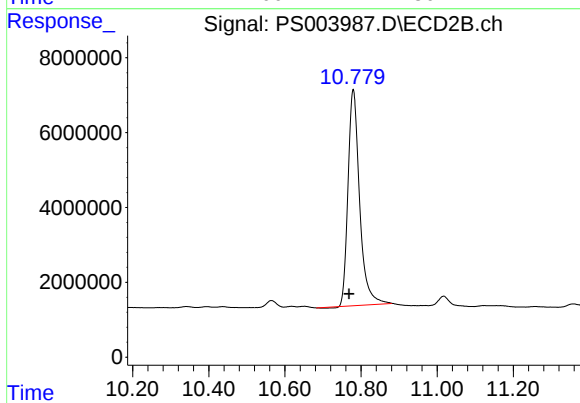

#4 2,4-DCAA


R.T.: 10.780 min
Delta R.T.: 0.011 min
Response: 122031233
Conc: 248.71 ng/ml

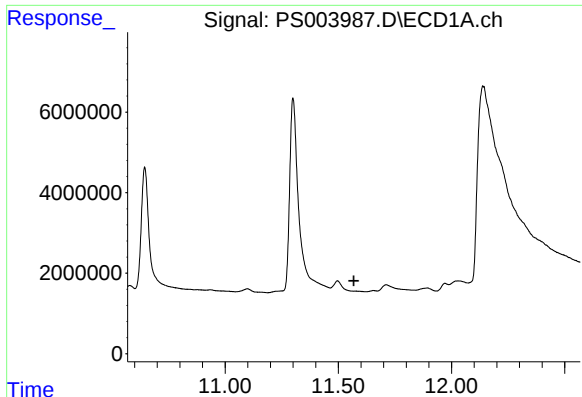

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118577BL

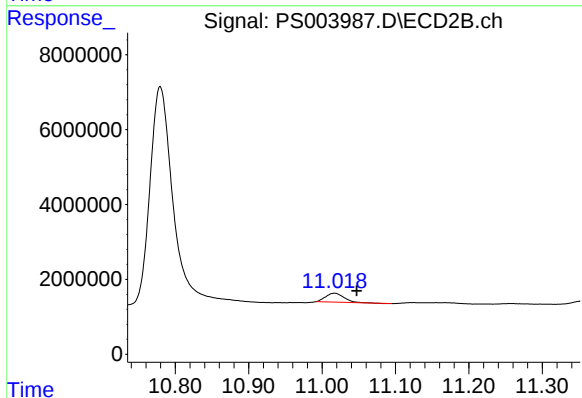


#5 DICAMBA

R.T.: 11.017 min
Delta R.T.: -0.030 min
Response: 4050916
Conc: 2.18 ng/ml

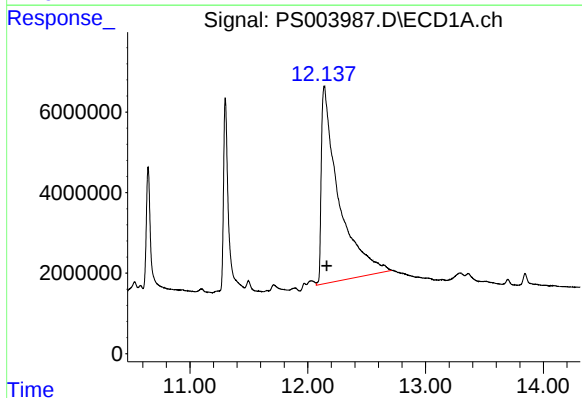


#7 MCPA

R.T.: 12.140 min
Delta R.T.: -0.022 min
Response: 506876272
Conc: 240.25 ug/ml

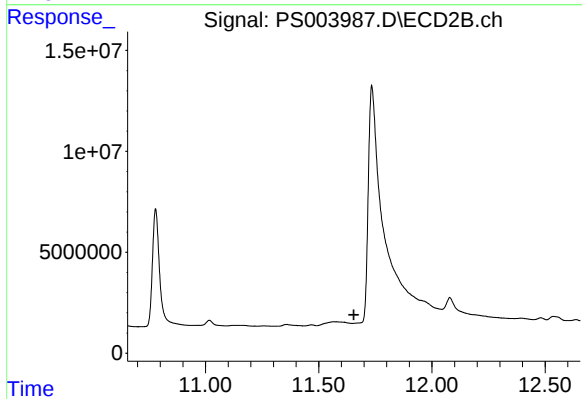

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.655 min
Response: 0
Conc: N.D.

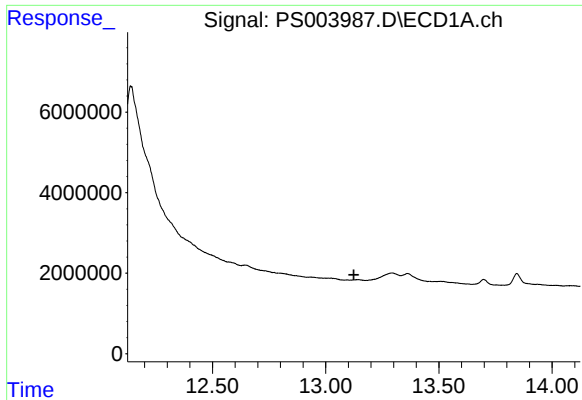

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118577BL

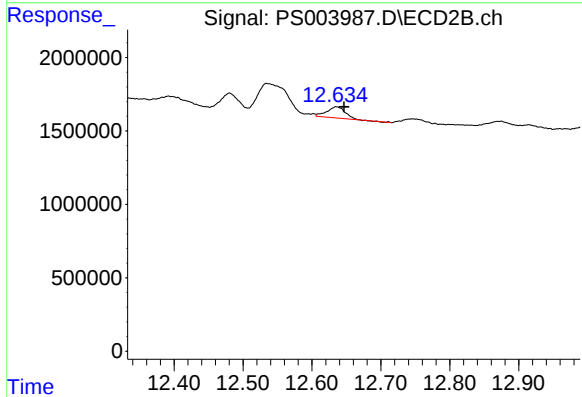


#9 2,4-D

R.T.: 12.636 min
Delta R.T.: -0.011 min
Response: 1401896
Conc: 2.64 ng/ml

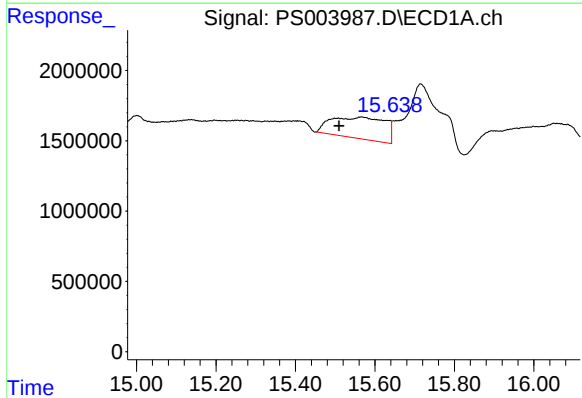


#13 2,4-DB

R.T.: 15.567 min
Delta R.T.: 0.057 min
Response: 14397751
Conc: 47.75 ng/ml

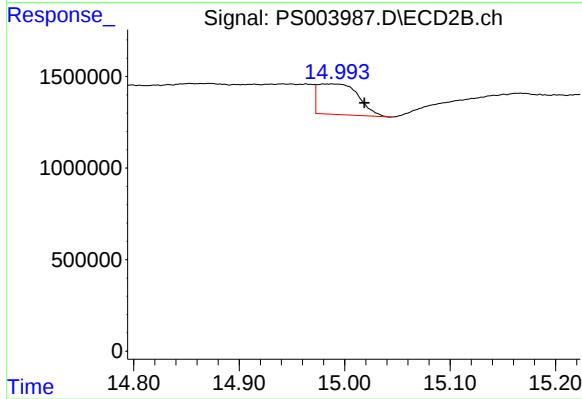

#13 2,4-DB


R.T.: 14.988 min
Delta R.T.: -0.031 min
Response: 4438624
Conc: 14.95 ng/ml

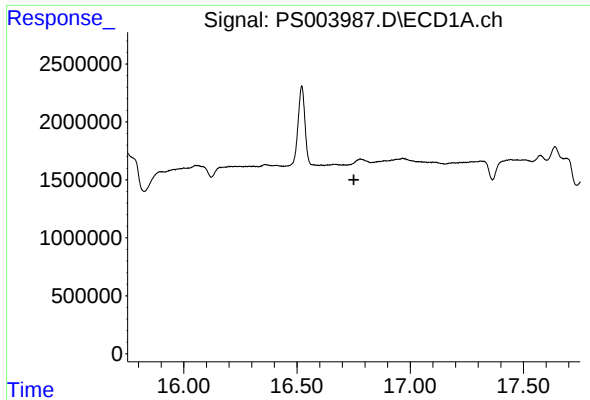

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118577BL

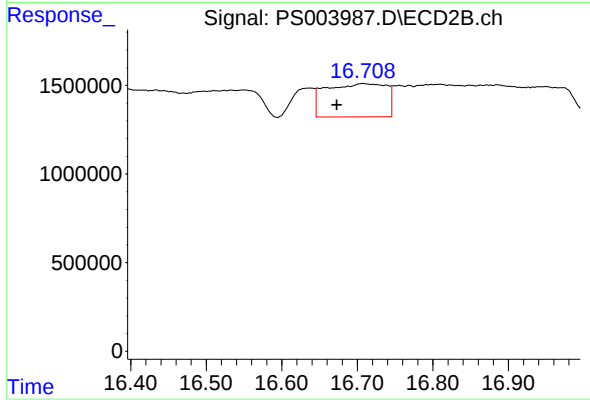

#15 Picloram

R.T.: 16.708 min
Delta R.T.: 0.035 min
Response: 10447453
Conc: 3.29 ng/ml