

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
 Data File : PS003989.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2019 08:34
 Operator : EI\SJ
 Sample : PB118577TB
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB118577TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 12:37:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.283	10.780	138.7E6	123.6E6	317.871	251.834
Target Compounds							
1) T	Dalapon	2.804	2.309	49551560	127.5E6	66.465	174.721 #
2) T	3,5-DICHL...	0.000	8.944	0	4611214	N.D.	7.229
3) T	4-Nitroph...	0.000	9.952	0	9021009	N.D.	39.734
5) T	DICAMBA	0.000	11.017	0	4535551	N.D.	2.439
7) T	MCPA	12.129	0.000	435.4E6	0	206.387	N.D. #
9) T	2,4-D	0.000	12.635	0	1542948	N.D.	2.901
10) T	Pentachlo...	0.000	13.185	0	1626152	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.810	0	1973994	N.D.	<MDL
14) T	DINOSEB	0.000	15.449	0	2204649	N.D.	1.149
15) T	Picloram	0.000	16.632	0	4330252	N.D.	1.365
16) T	DCPA	0.000	16.632	0	4330252	N.D.	1.281



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040419\
Data File : PS003989.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2019 08:34
Operator : EI\SJ
Sample : PB118577TB
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PB118577TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 12:37:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

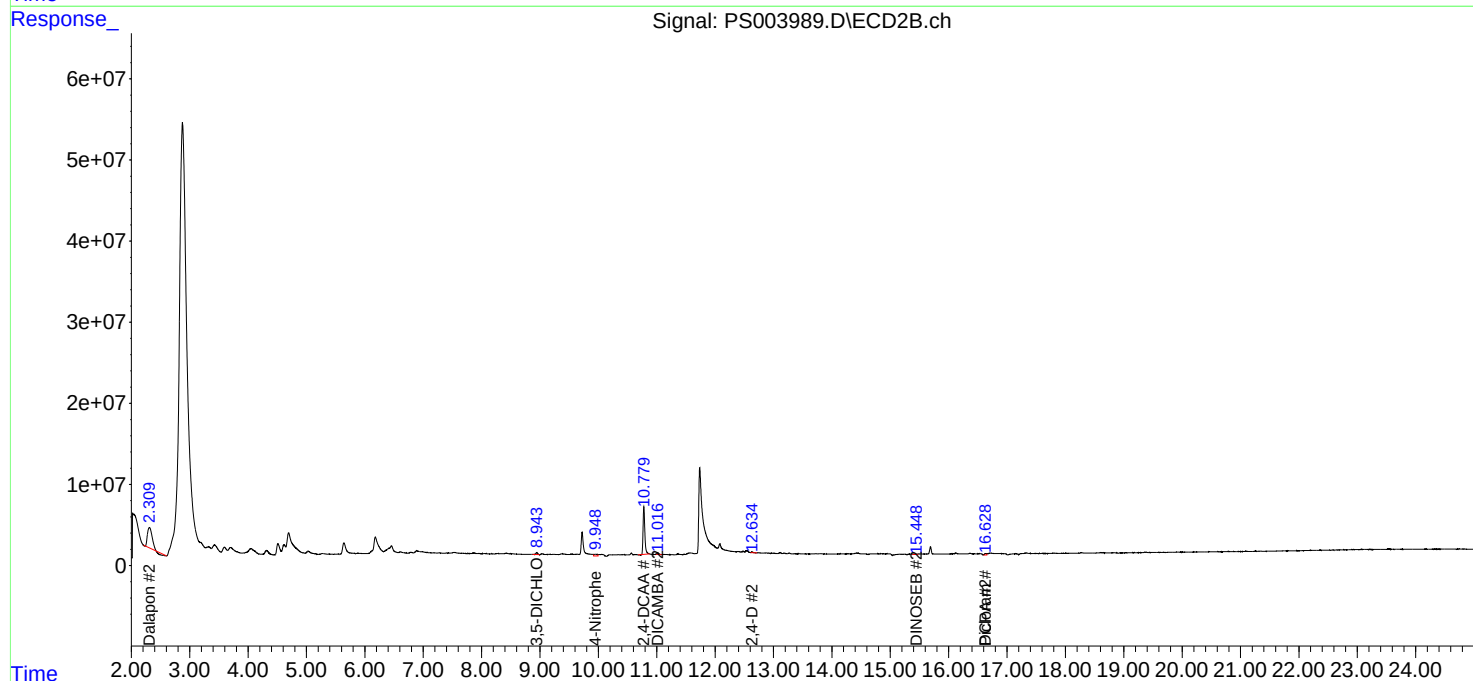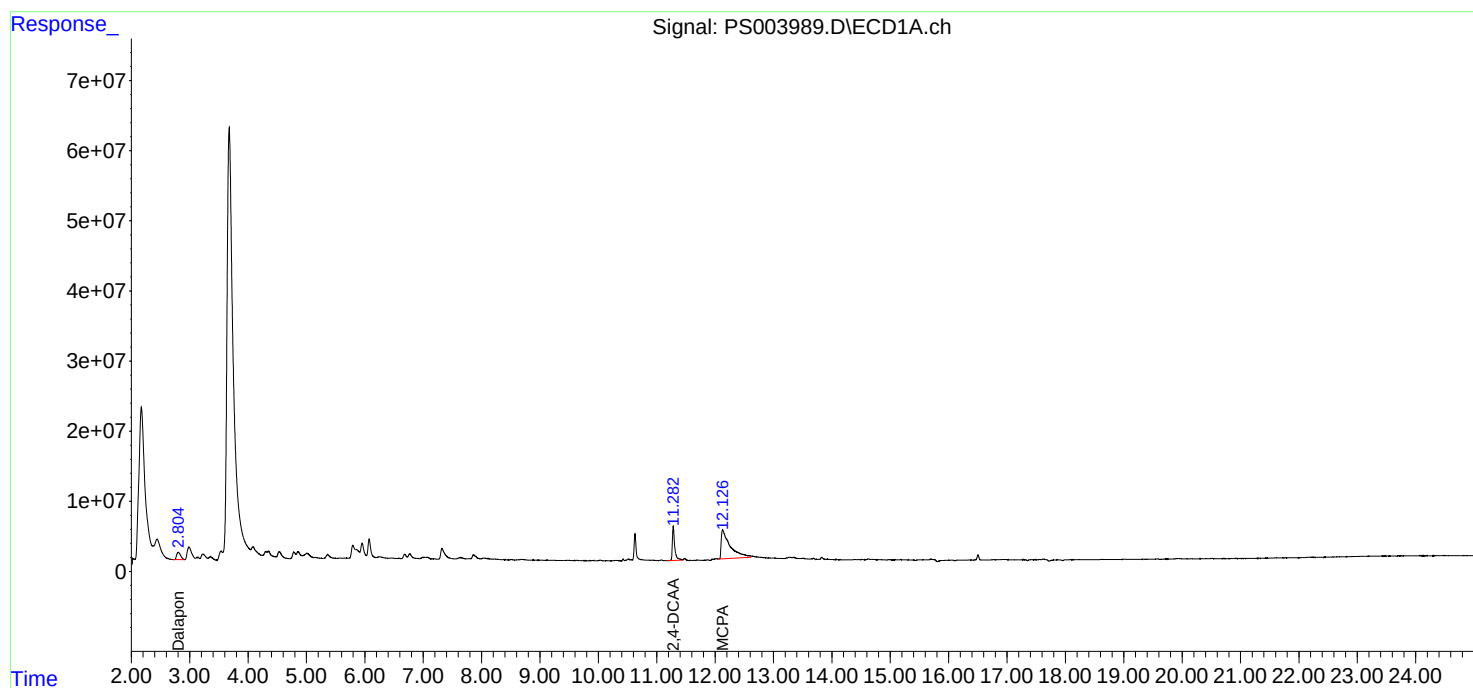


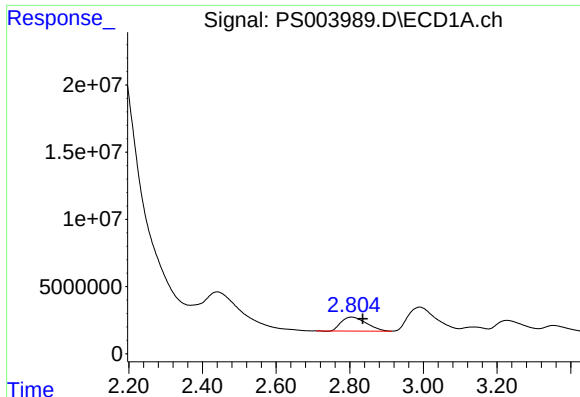

#1 Dalapon


R.T.: 2.804 min
Delta R.T.: -0.031 min
Response: 49551560
Conc: 66.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB118577TB

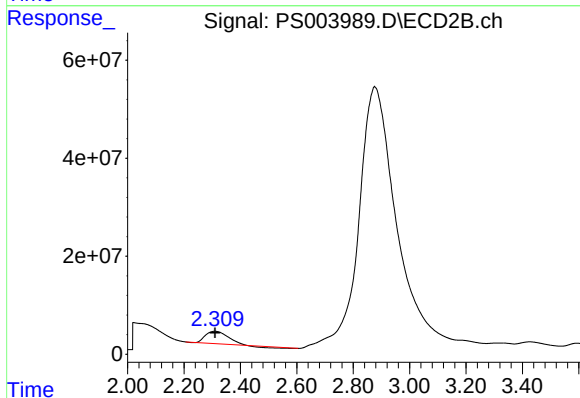


#1 Dalapon

R.T.: 2.309 min
Delta R.T.: 0.000 min
Response: 127481514
Conc: 174.72 ng/ml

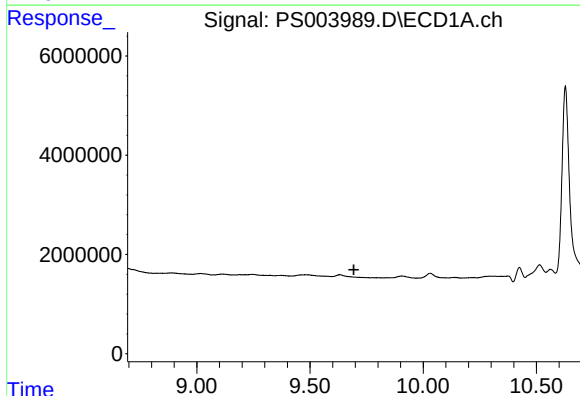


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

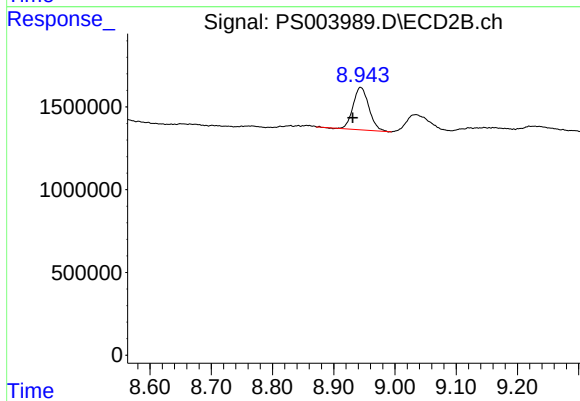

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.944 min
Delta R.T.: 0.013 min
Response: 4611214
Conc: 7.23 ng/ml

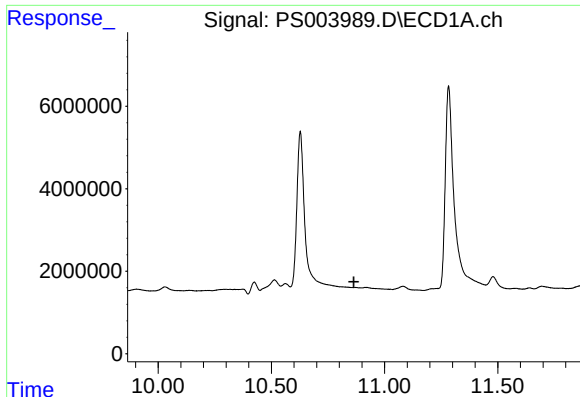

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118577TB

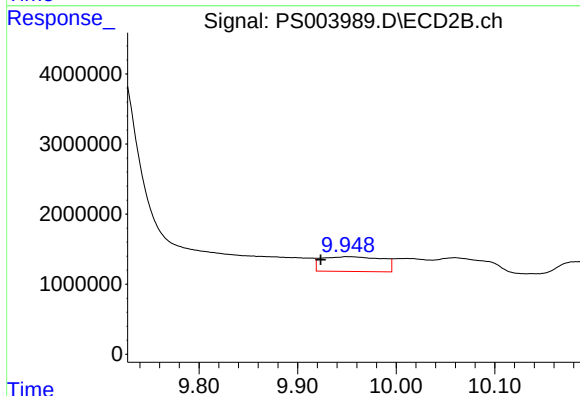


#3 4-Nitrophenol

R.T.: 9.952 min
Delta R.T.: 0.028 min
Response: 9021009
Conc: 39.73 ng/ml

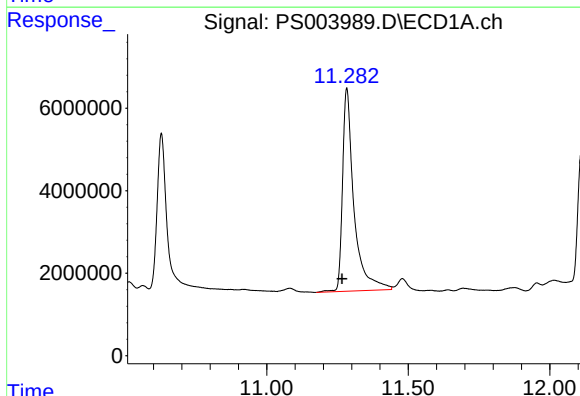


#4 2,4-DCAA

R.T.: 11.283 min
Delta R.T.: 0.016 min
Response: 138659053
Conc: 317.87 ng/ml

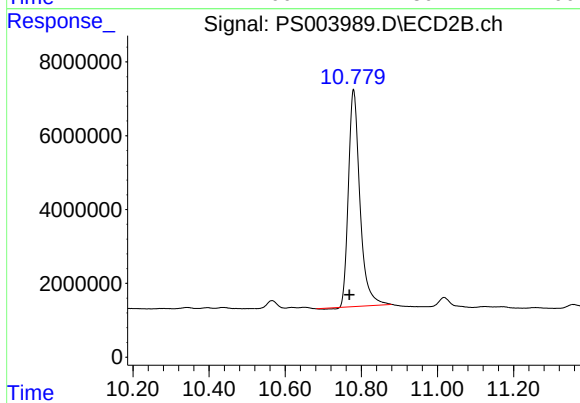

#4 2,4-DCAA


R.T.: 10.780 min
Delta R.T.: 0.011 min
Response: 123564343
Conc: 251.83 ng/ml

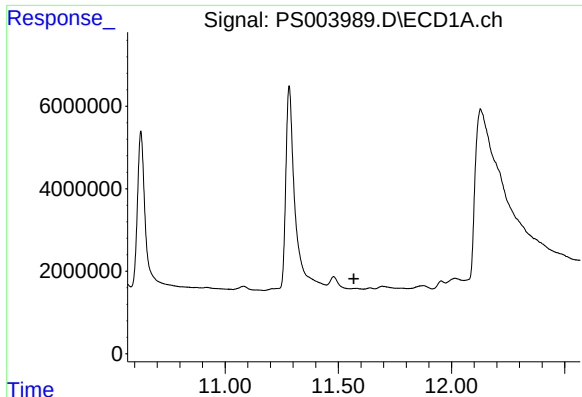

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118577TB

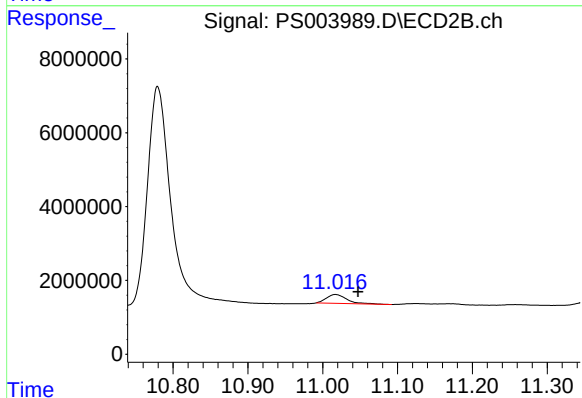


#5 DICAMBA

R.T.: 11.017 min
Delta R.T.: -0.030 min
Response: 4535551
Conc: 2.44 ng/ml

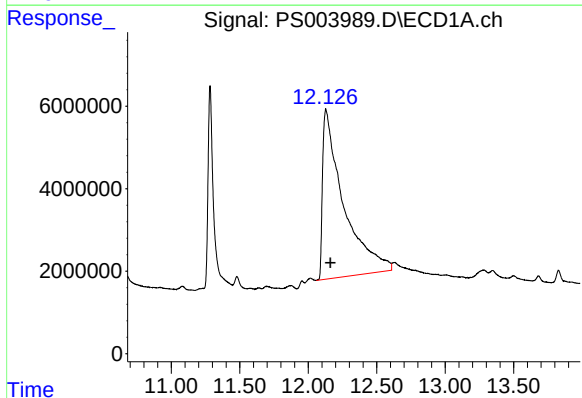


#7 MCPA

R.T.: 12.129 min
Delta R.T.: -0.032 min
Response: 435432247
Conc: 206.39 ug/ml

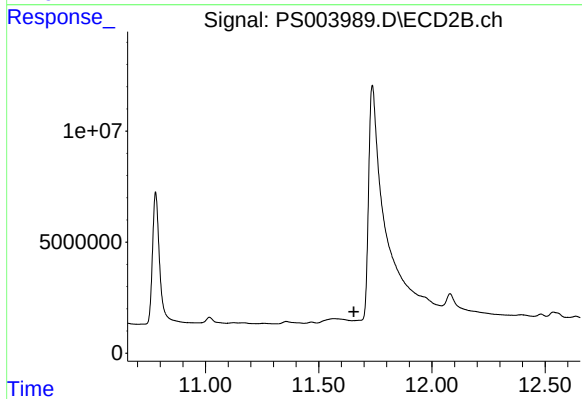

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.655 min
Response: 0
Conc: N.D.

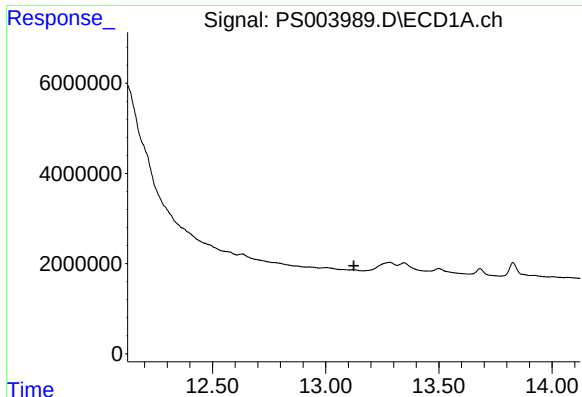

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118577TB

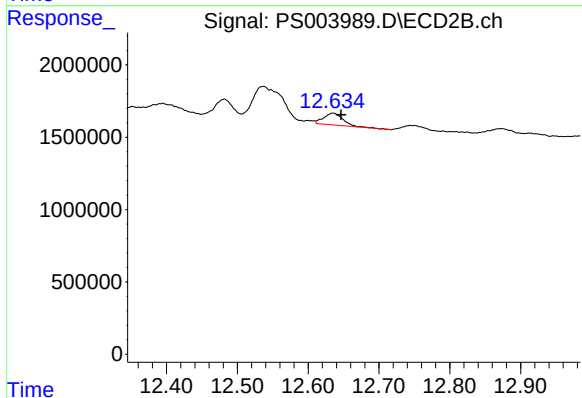


#9 2,4-D

R.T.: 12.635 min
Delta R.T.: -0.011 min
Response: 1542948
Conc: 2.90 ng/ml

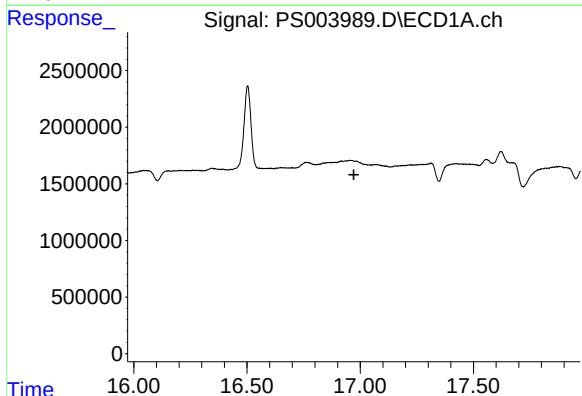


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

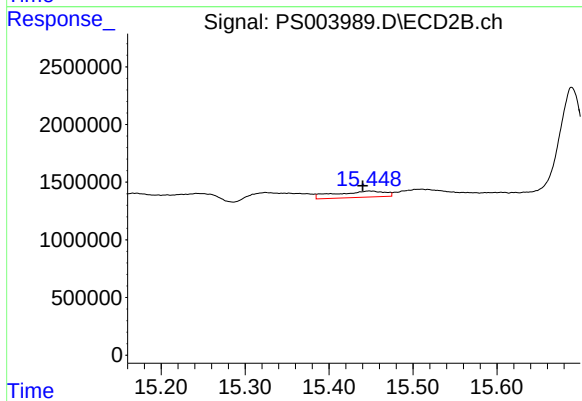

#14 DINOSEB


R.T.: 15.449 min
Delta R.T.: 0.009 min
Response: 2204649
Conc: 1.15 ng/ml

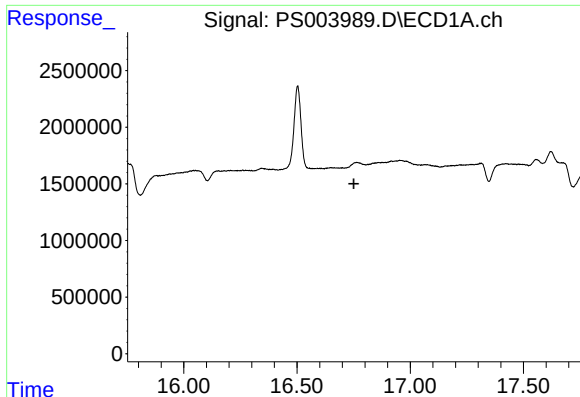

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118577TB

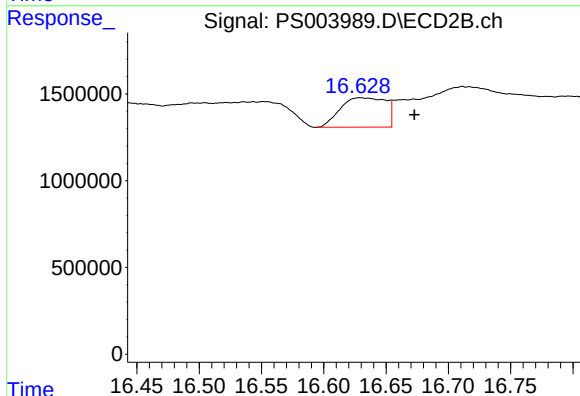


#15 Picloram

R.T.: 16.632 min
Delta R.T.: -0.041 min
Response: 4330252
Conc: 1.37 ng/ml

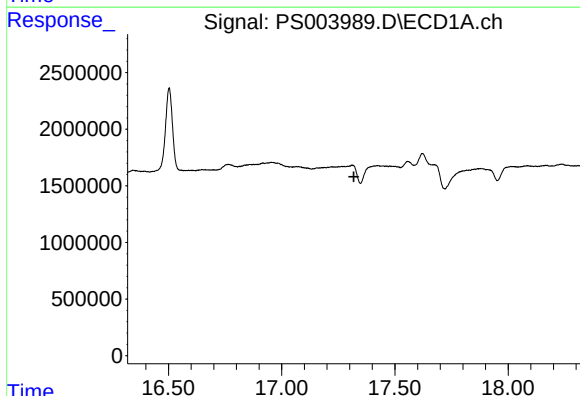

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.319 min
Response: 0
Conc: N.D.

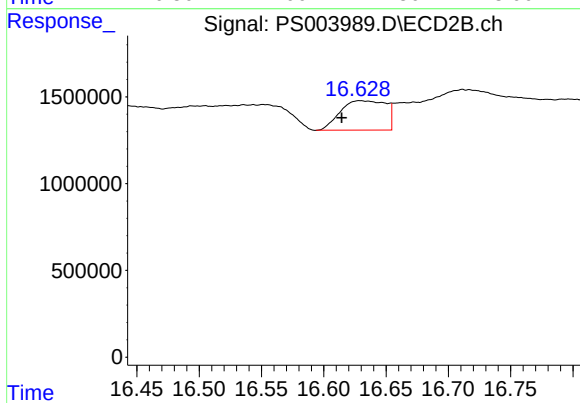

#16 DCPA

R.T.: 16.632 min
Delta R.T.: 0.018 min
Response: 4330252
Conc: 1.28 ng/ml