

Data Path : P:\HPCHEM1\ECD_S\Data\PS041018\
 Data File : PS000113.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2018 18:59
 Operator : UA
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 07:09:52 2018
 Quant Method : P:\HPCHEM1\ECD_S\Method\PS041018.M
 Quant Title : 8080.M
 QLast Update : Wed Apr 11 07:08:18 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.816	11.193	265.1E6	226.6E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.165	2.549	323.9E6	258.4E6	682.500	682.500
2) T	3,5-DICHL...	10.230	9.337	359.3E6	289.0E6	697.500	697.500
3) T	4-Nitroph...	11.414	10.340	154.5E6	120.5E6	682.500	682.500
5) T	DICAMBA	12.136	11.483	945.9E6	773.3E6	705.000	705.000
6) T	MCPD	12.476	11.708	79501849	64083136	70.500	70.500
7) T	MCPA	12.728	12.086	142.3E6	117.8E6	69.750	69.750
8) T	DICHLORPROP	13.329	12.606	243.3E6	198.0E6	705.000	705.000
9) T	2,4-D	13.687	13.077	317.0E6	262.2E6	705.000	705.000
10) T	Pentachlo...	14.086	13.641	3544.9E6	2992.4E6	712.500	712.500
11) T	2,4,5-TP ...	14.953	14.249	1427.4E6	1184.0E6	712.500	712.500
12) T	2,4,5-T	15.350	14.781	1386.1E6	1109.6E6	712.500	712.500
13) T	2,4-DB	16.105	15.468	195.1E6	144.1E6	712.500	712.500
14) T	DINOSEB	17.619	15.902	977.5E6	800.9E6	705.000	705.000
15) T	Picloram	17.373	17.148	1823.1E6	1452.7E6	712.500	712.500
16) T	DCPA	17.958	17.089	1704.5E6	1411.3E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_S\Data\PS041018\
Data File : PS000113.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2018 18:59
Operator : UA
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 07:09:52 2018
Quant Method : P:\HPCHEM1\ECD_S\Method\PS041018.M
Quant Title : 8080.M
QLast Update : Wed Apr 11 07:08:18 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

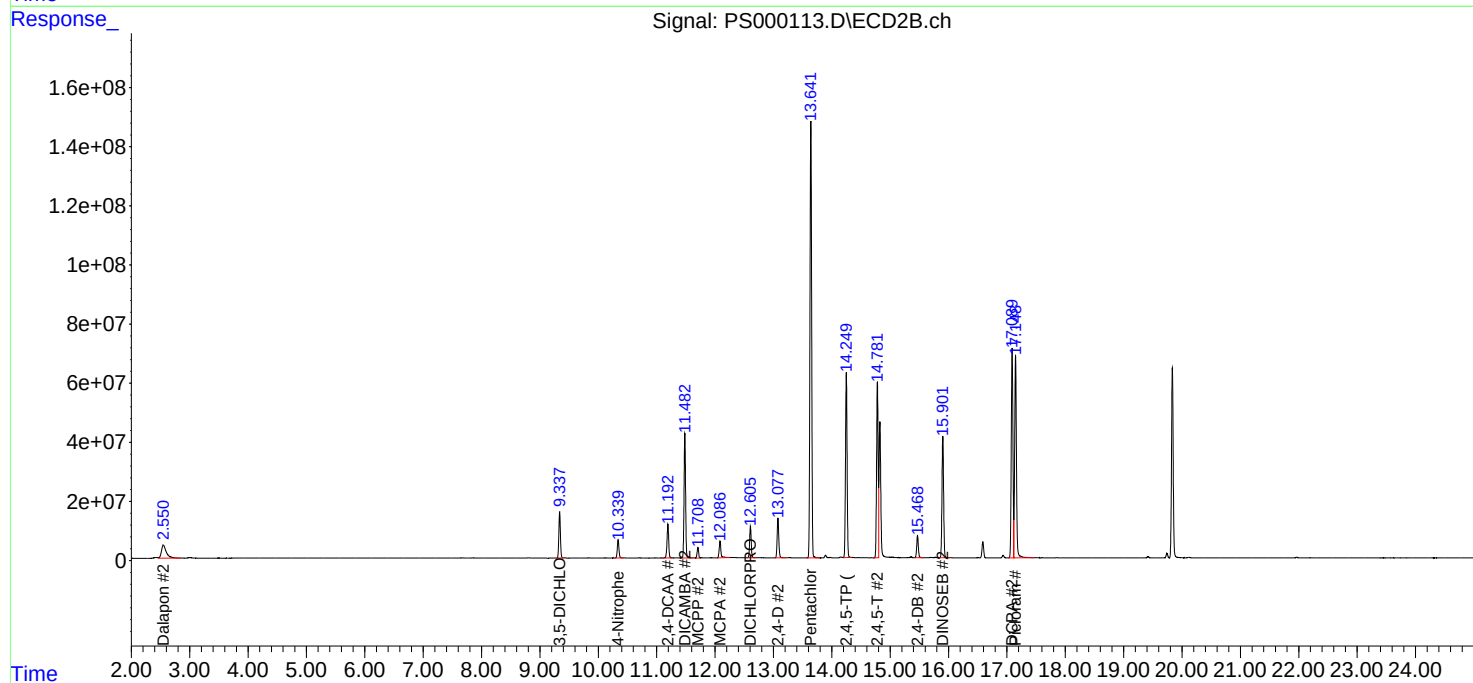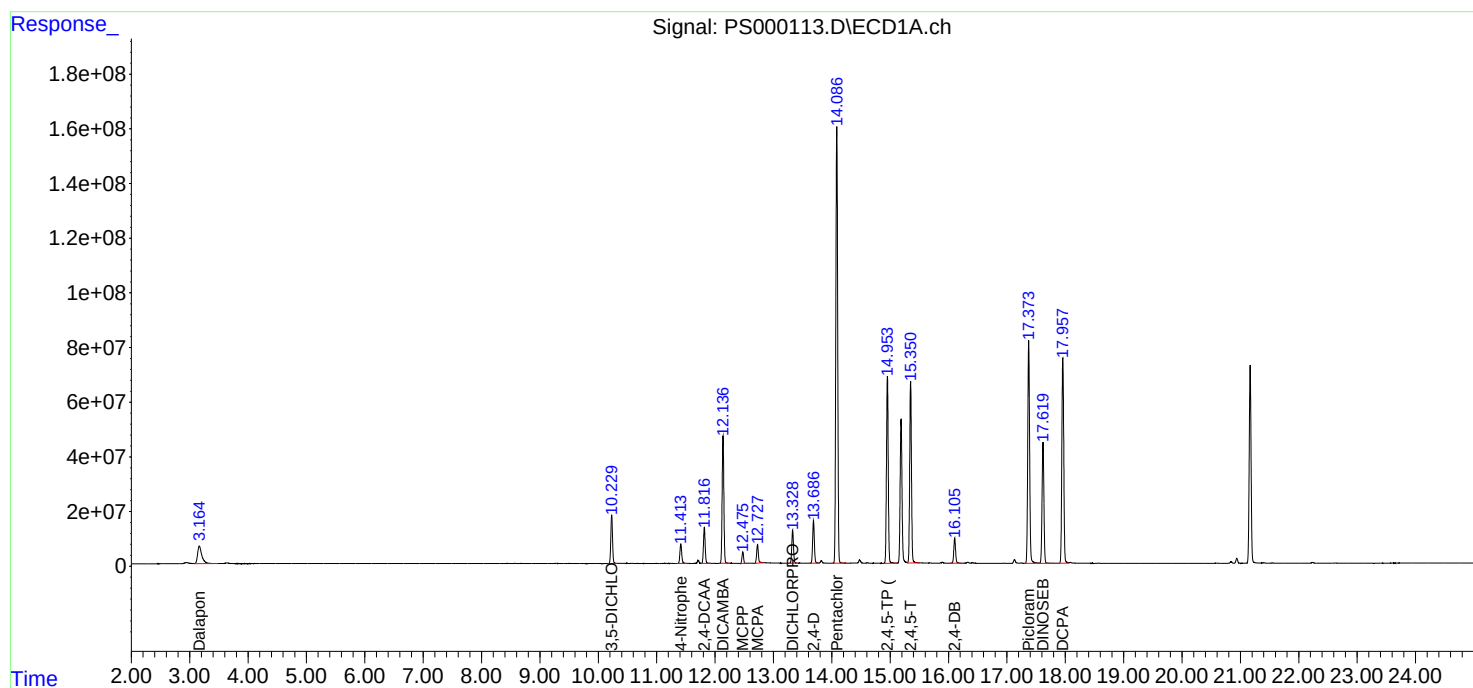


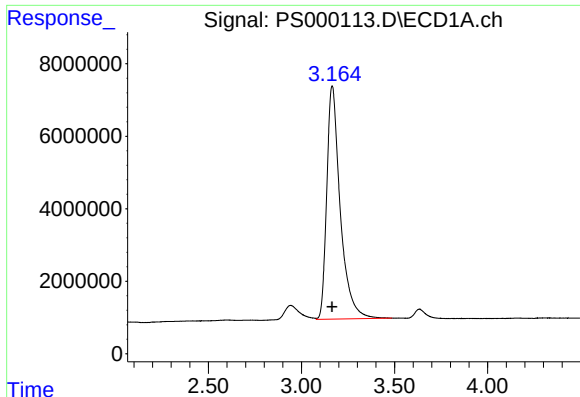

#1 Dalapon


R.T.: 3.165 min
Delta R.T.: 0.000 min
Response: 323886393
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

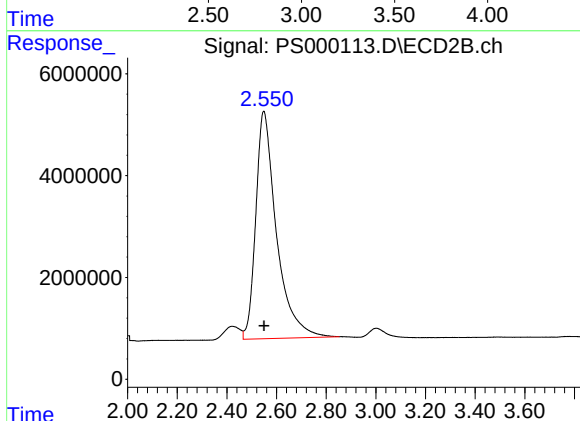


#1 Dalapon

R.T.: 2.549 min
Delta R.T.: 0.000 min
Response: 258418586
Conc: 682.50 ng/ml

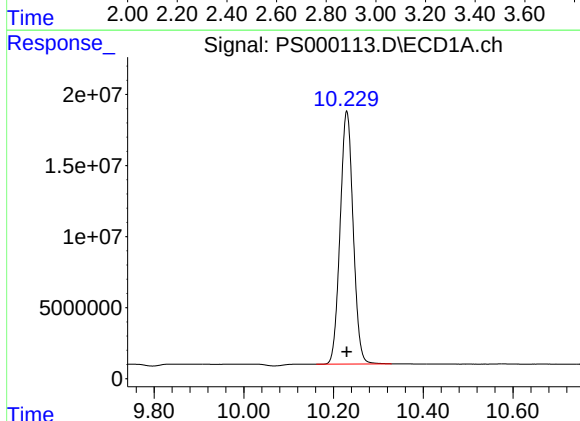


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.230 min
Delta R.T.: 0.000 min
Response: 359312615
Conc: 697.50 ng/ml

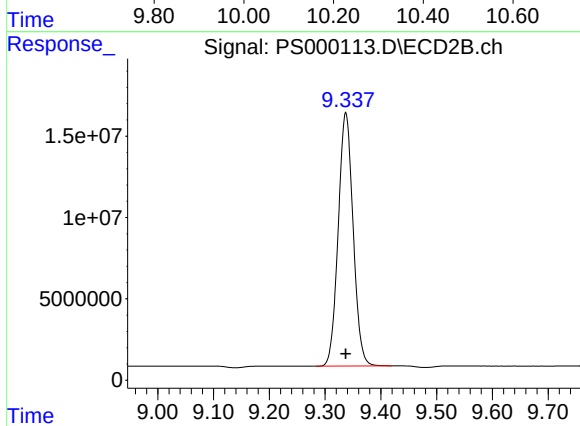

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.337 min
Delta R.T.: 0.000 min
Response: 288997282
Conc: 697.50 ng/ml

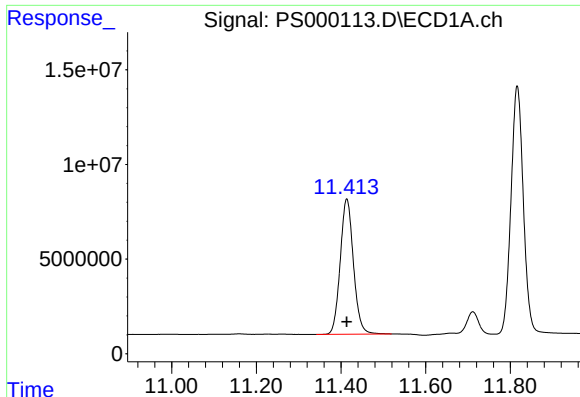

#3 4-Nitrophenol


R.T.: 11.414 min
Delta R.T.: 0.000 min
Response: 154456831
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

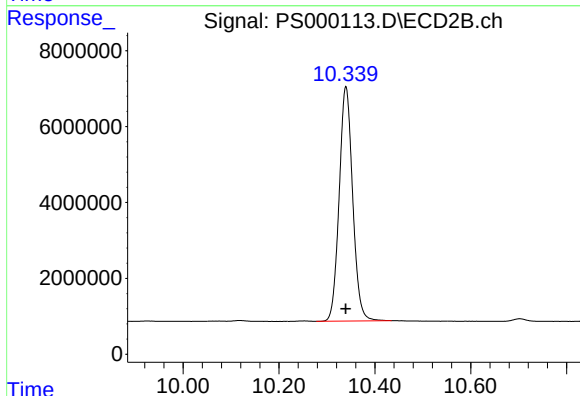


#3 4-Nitrophenol

R.T.: 10.340 min
Delta R.T.: 0.000 min
Response: 120465863
Conc: 682.50 ng/ml

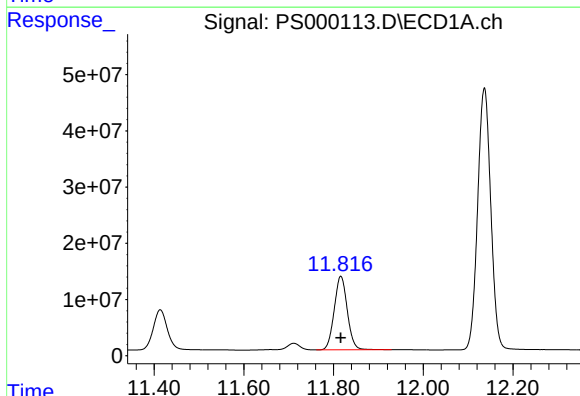


#4 2,4-DCAA

R.T.: 11.816 min
Delta R.T.: 0.000 min
Response: 265147825
Conc: 750.00 ng/ml

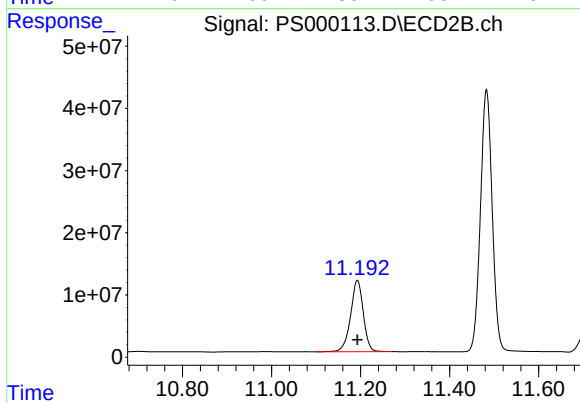

#4 2,4-DCAA


R.T.: 11.193 min
Delta R.T.: 0.000 min
Response: 226638976
Conc: 750.00 ng/ml

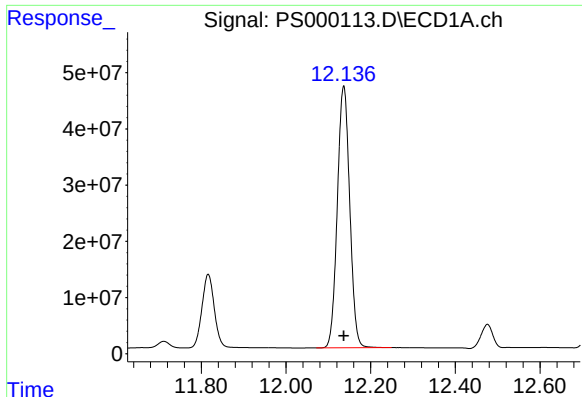

#5 DICAMBA


R.T.: 12.136 min
Delta R.T.: 0.000 min
Response: 945899147
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

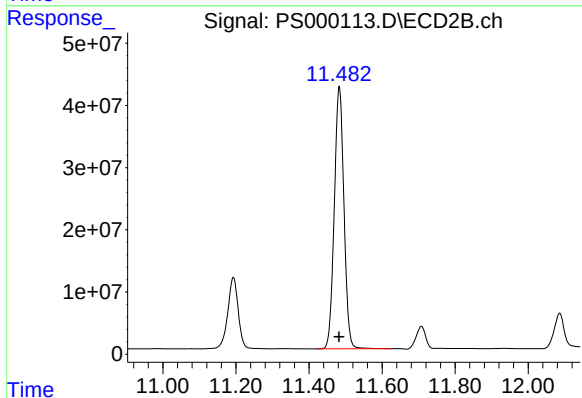


#5 DICAMBA

R.T.: 11.483 min
Delta R.T.: 0.000 min
Response: 773330508
Conc: 705.00 ng/ml

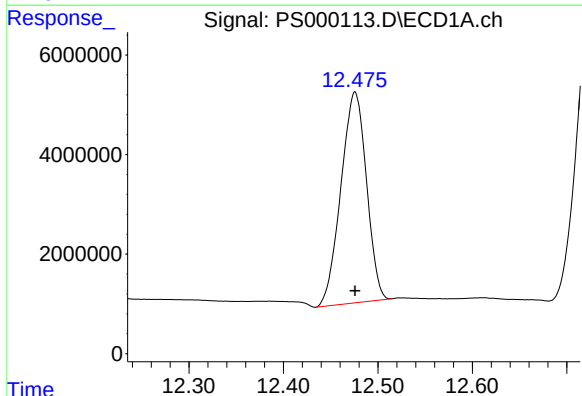


#6 MCP

R.T.: 12.476 min
Delta R.T.: 0.000 min
Response: 79501849
Conc: 70.50 ug/ml

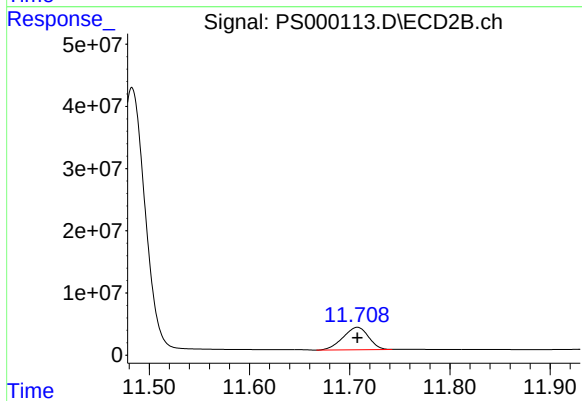

#6 MCP


R.T.: 11.708 min
Delta R.T.: 0.000 min
Response: 64083136
Conc: 70.50 ug/ml

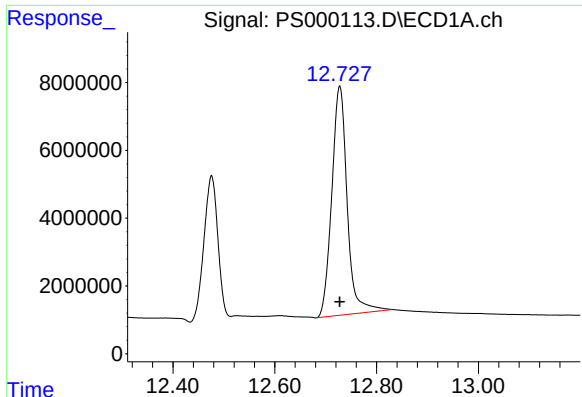

#7 MCPA


R.T.: 12.728 min
Delta R.T.: 0.000 min
Response: 142325640
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

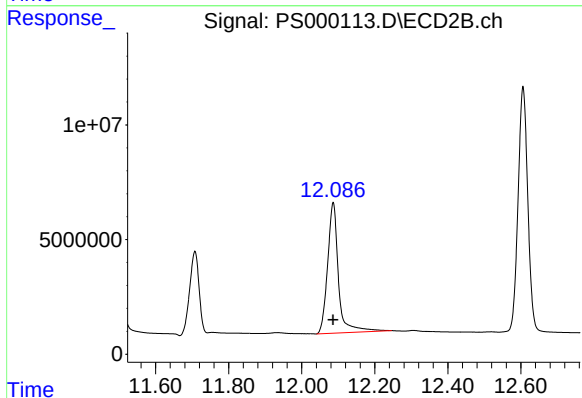


#7 MCPA

R.T.: 12.086 min
Delta R.T.: 0.000 min
Response: 117771403
Conc: 69.75 ug/ml

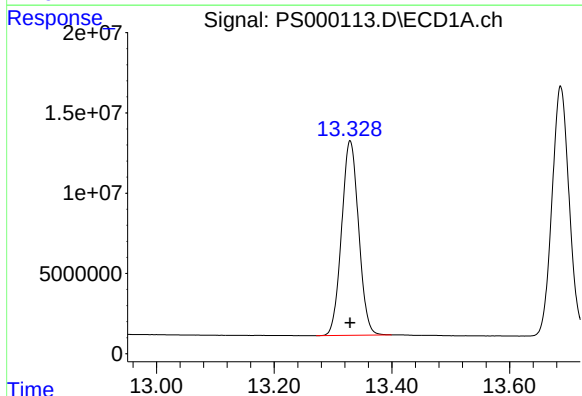


#8 DICHLORPROP

R.T.: 13.329 min
Delta R.T.: 0.000 min
Response: 243261653
Conc: 705.00 ng/ml

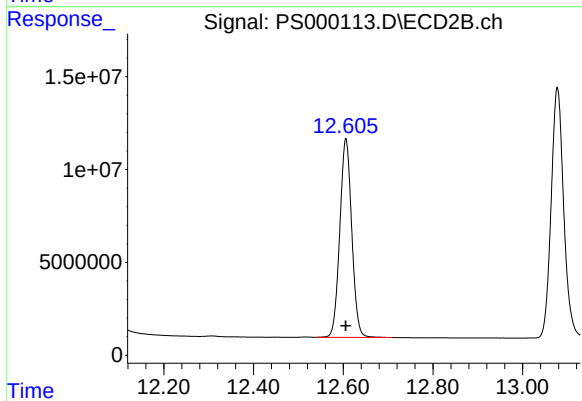

#8 DICHLORPROP


R.T.: 12.606 min
Delta R.T.: 0.000 min
Response: 198015782
Conc: 705.00 ng/ml

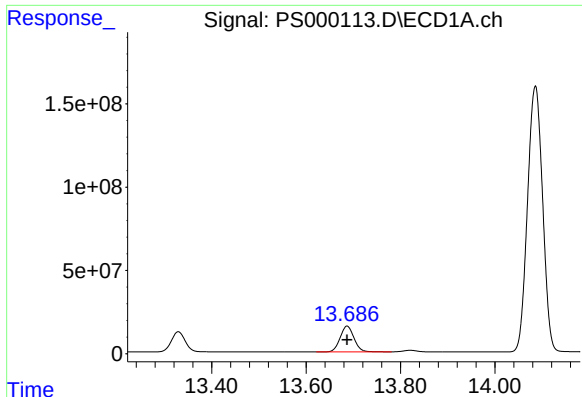

#9 2,4-D


R.T.: 13.687 min
Delta R.T.: 0.000 min
Response: 316957752
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

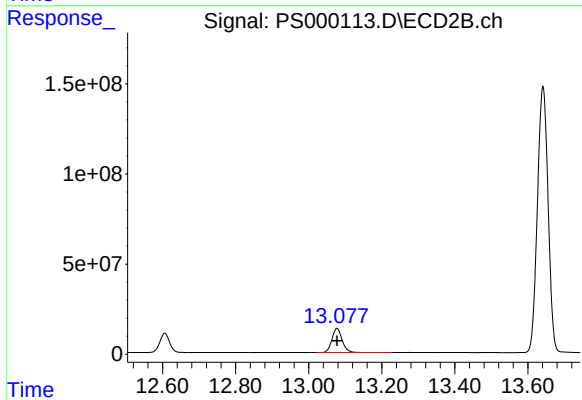


#9 2,4-D

R.T.: 13.077 min
Delta R.T.: 0.000 min
Response: 262211727
Conc: 705.00 ng/ml

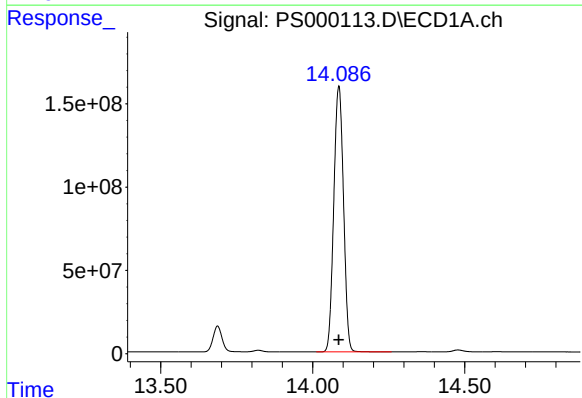


#10 Pentachlorophenol

R.T.: 14.086 min
Delta R.T.: 0.000 min
Response: 3544869006
Conc: 712.50 ng/ml

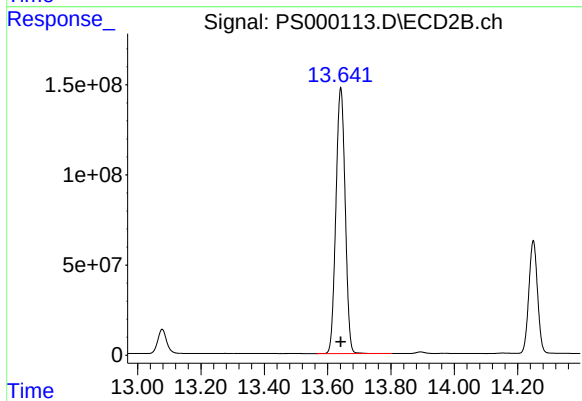

#10 Pentachlorophenol


R.T.: 13.641 min
Delta R.T.: 0.000 min
Response: 2992396256
Conc: 712.50 ng/ml

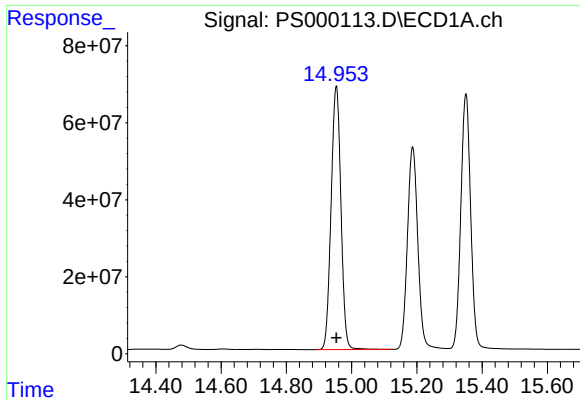

#11 2,4,5-TP (SILVEX)


R.T.: 14.953 min
Delta R.T.: 0.000 min
Response: 1427394993
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

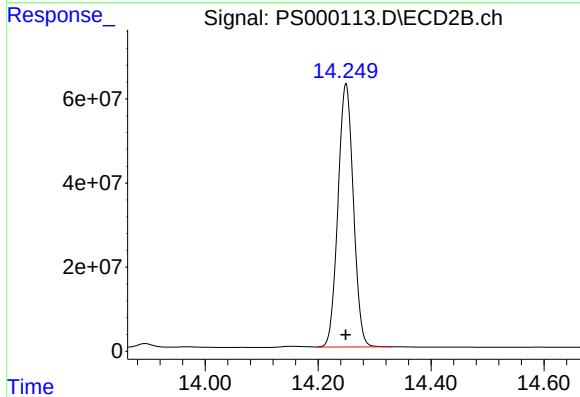


#11 2,4,5-TP (SILVEX)

R.T.: 14.249 min
Delta R.T.: 0.000 min
Response: 1184011189
Conc: 712.50 ng/ml

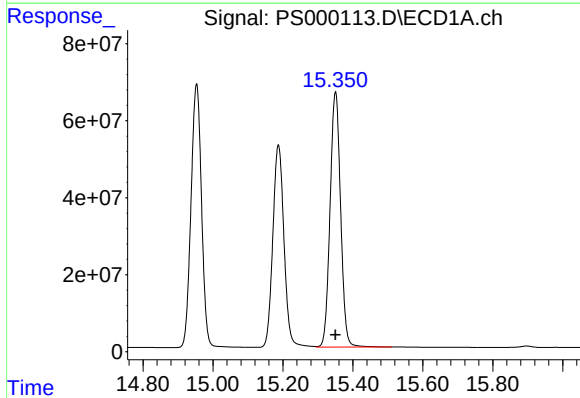


#12 2,4,5-T

R.T.: 15.350 min
Delta R.T.: 0.000 min
Response: 1386051742
Conc: 712.50 ng/ml

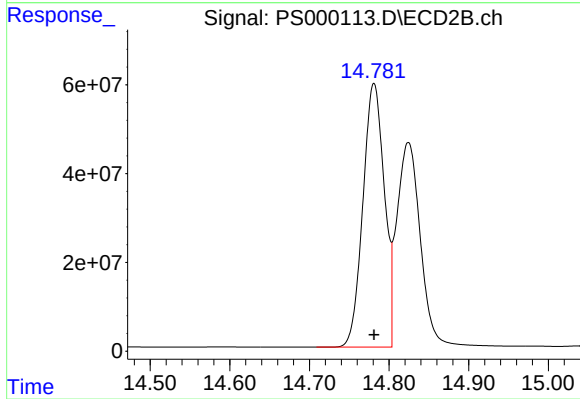

#12 2,4,5-T


R.T.: 14.781 min
Delta R.T.: 0.000 min
Response: 1109609108
Conc: 712.50 ng/ml

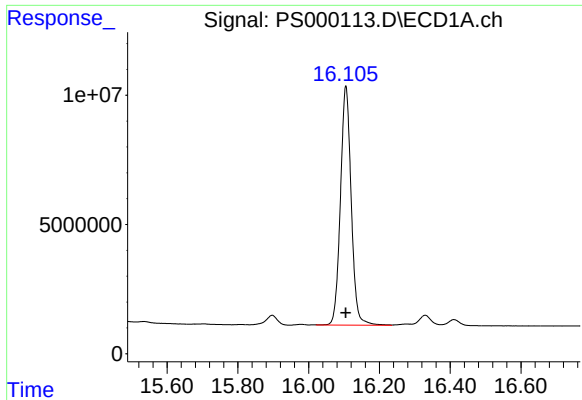

#13 2,4-DB


R.T.: 16.105 min
Delta R.T.: 0.000 min
Response: 195078252
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

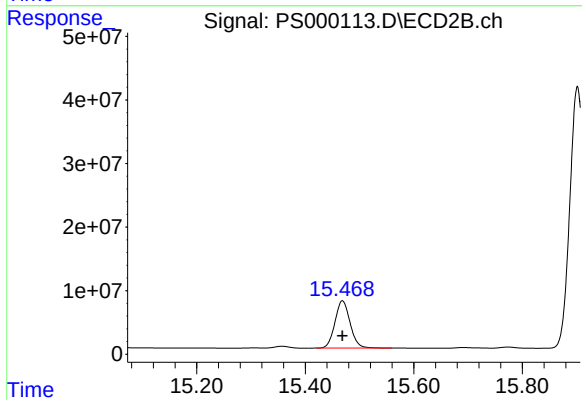


#13 2,4-DB

R.T.: 15.468 min
Delta R.T.: 0.000 min
Response: 144056114
Conc: 712.50 ng/ml

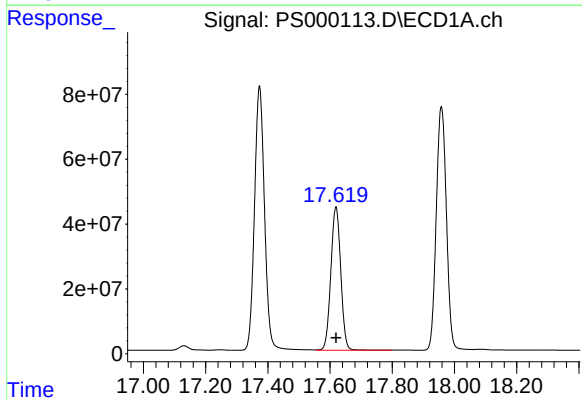


#14 DINOSEB

R.T.: 17.619 min
Delta R.T.: 0.000 min
Response: 977514532
Conc: 705.00 ng/ml

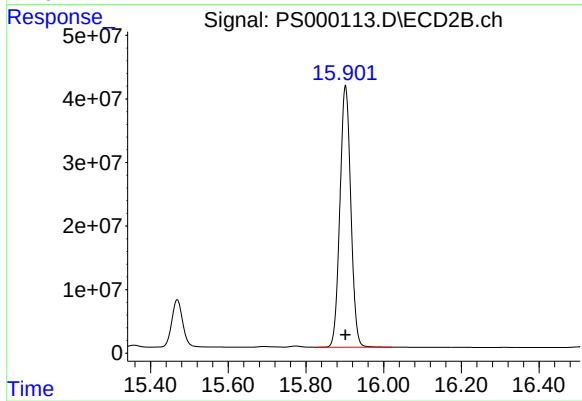

#14 DINOSEB


R.T.: 15.902 min
Delta R.T.: 0.000 min
Response: 800897056
Conc: 705.00 ng/ml

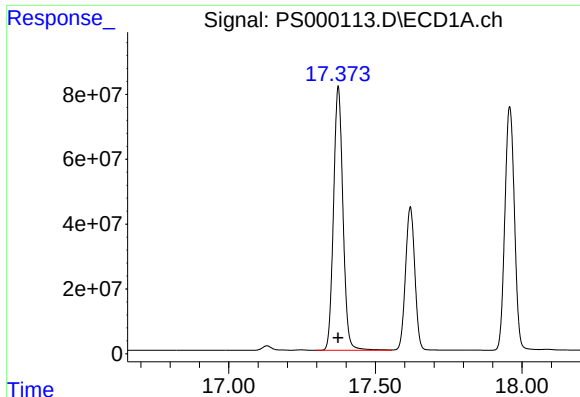

#15 Picloram


R.T.: 17.373 min
Delta R.T.: 0.000 min
Response: 1823113571
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

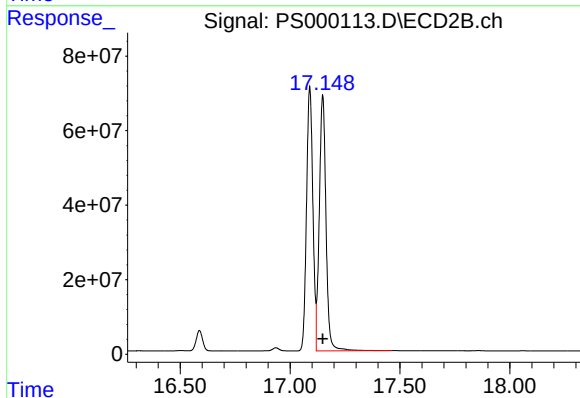


#15 Picloram

R.T.: 17.148 min
Delta R.T.: 0.000 min
Response: 1452655487
Conc: 712.50 ng/ml

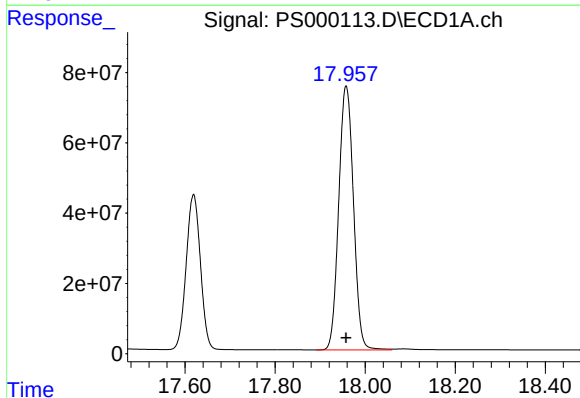

#16 DCPA

R.T.: 17.958 min
Delta R.T.: 0.000 min
Response: 1704525421
Conc: 720.00 ng/ml

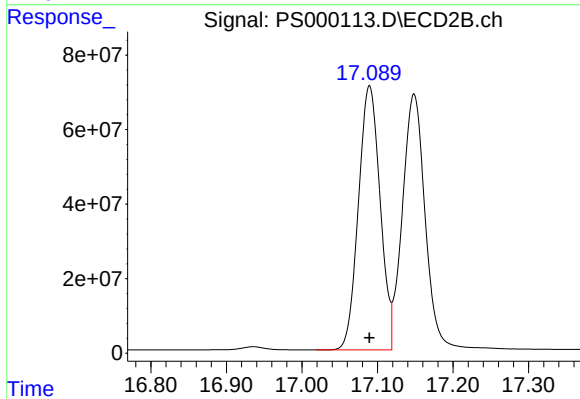

#16 DCPA

R.T.: 17.089 min
Delta R.T.: 0.000 min
Response: 1411252263
Conc: 720.00 ng/ml