

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041119\
 Data File : PS004025.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2019 10:41
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 16:21:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.815	0	398.1E6	N.D.	866.776
Target Compounds							
1) T	Dalapon	0.000	2.321	0	7947666	N.D.	12.646
3) T	4-Nitroph...	10.831	9.928	7385244	1682206	29.237	7.015 #
7) T	MCPA	12.193	11.608	787924	8340632	<MDL	4.584 #
9) T	2,4-D	0.000	12.691	0	2994326	N.D.	5.852
11) T	2,4,5-TP ...	14.339	13.783	618224	1772801	<MDL	<MDL #
12) T	2,4,5-T	14.709	0.000	2297685	0	<MDL	N.D. #
13) T	2,4-DB	0.000	15.048	0	5746992	N.D.	18.654
14) T	DINOSEB	16.897	15.440	9612078	13420963	3.837	7.181 #
15) T	Picloram	16.662	16.621	208.2E6	42411427	58.062	12.389 #
16) T	DCPA	17.244	16.621	1170143	42411427	<MDL	13.344 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041119\
Data File : PS004025.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2019 10:41
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 16:21:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

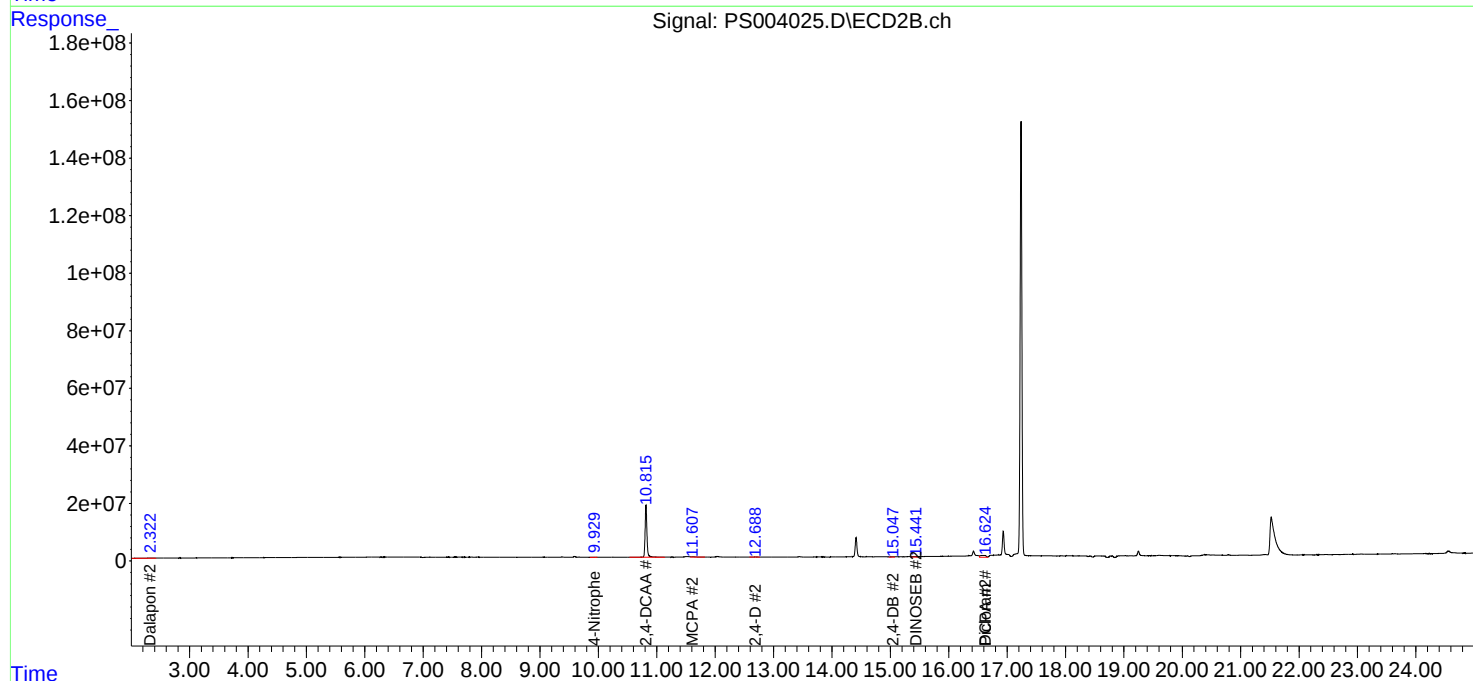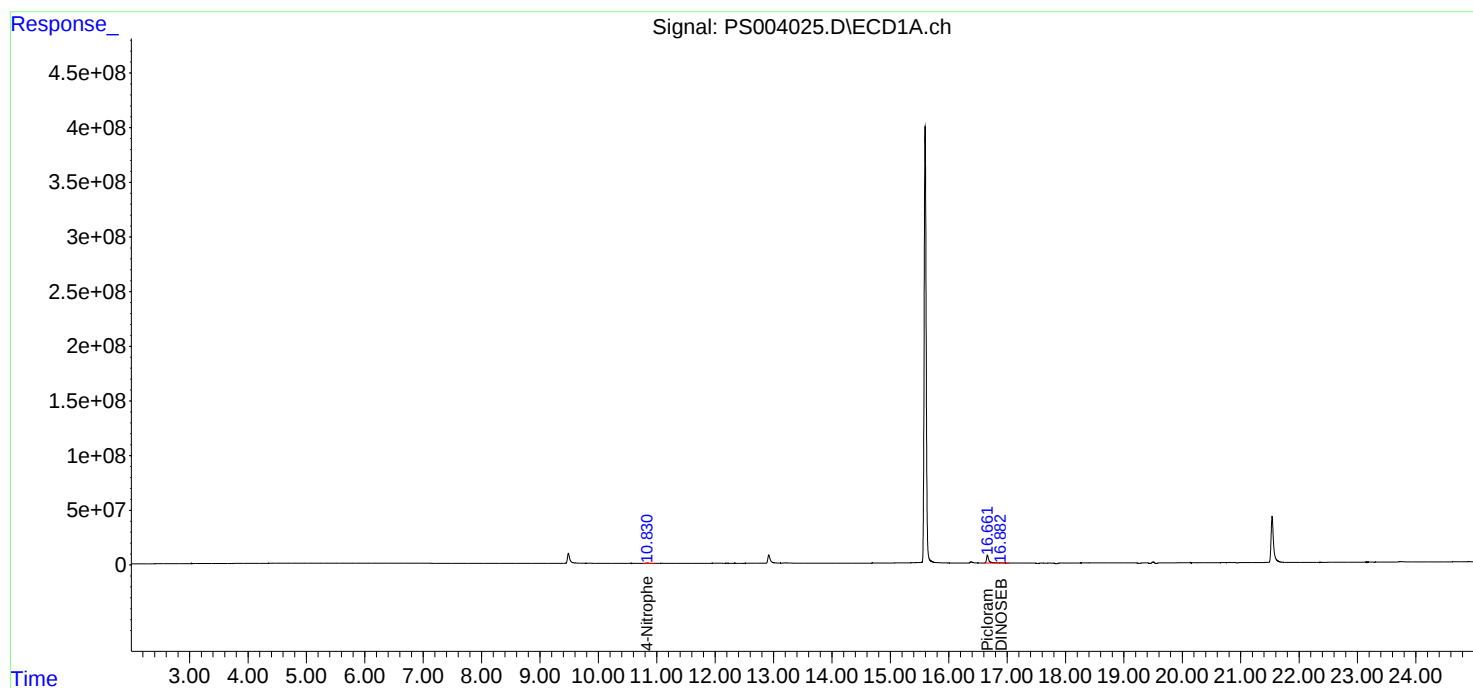


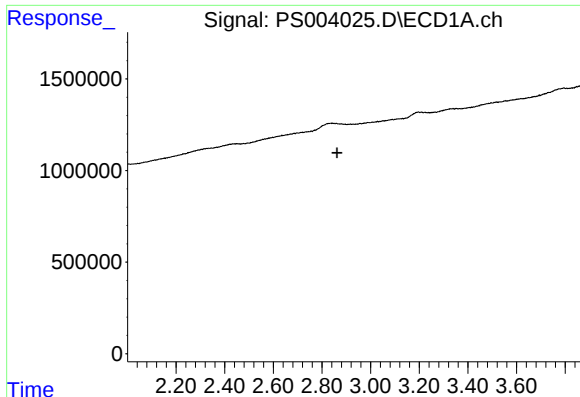

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.862 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

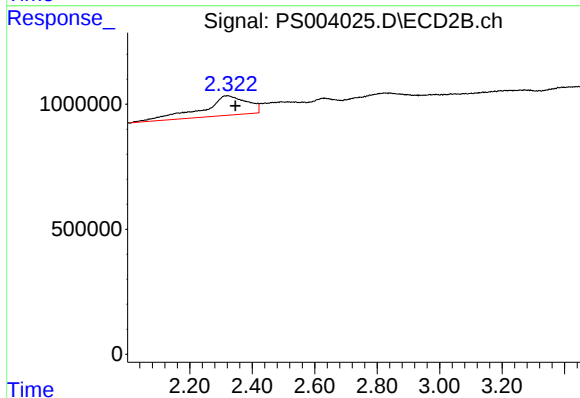


#1 Dalapon

R.T.: 2.321 min
Delta R.T.: -0.025 min
Response: 7947666
Conc: 12.65 ng/ml

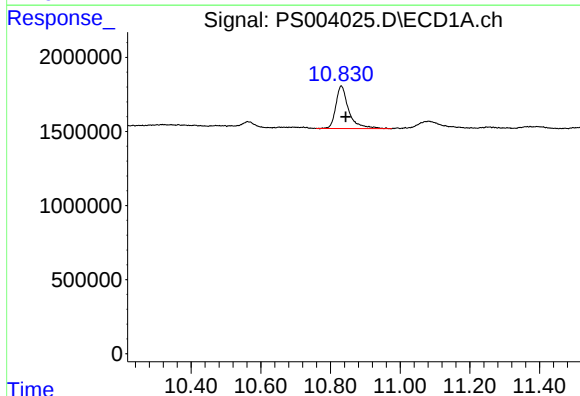


#3 4-Nitrophenol

R.T.: 10.831 min
Delta R.T.: -0.012 min
Response: 7385244
Conc: 29.24 ng/ml

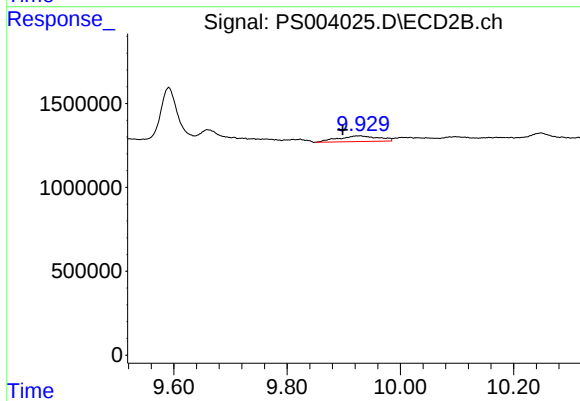

#3 4-Nitrophenol


R.T.: 9.928 min
Delta R.T.: 0.029 min
Response: 1682206
Conc: 7.01 ng/ml

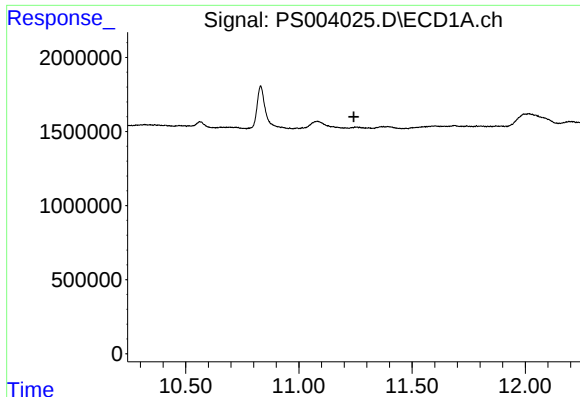

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.243 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

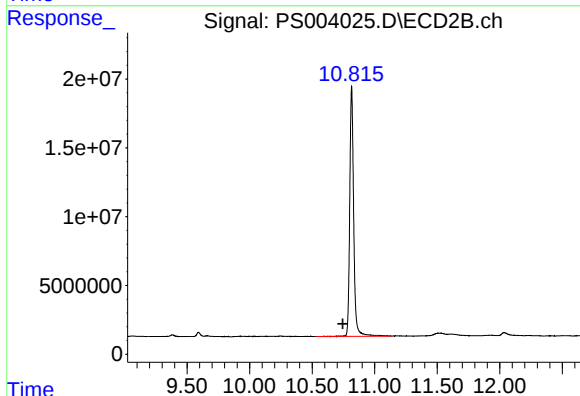


#4 2,4-DCAA

R.T.: 10.815 min
Delta R.T.: 0.069 min
Response: 398060039
Conc: 866.78 ng/ml

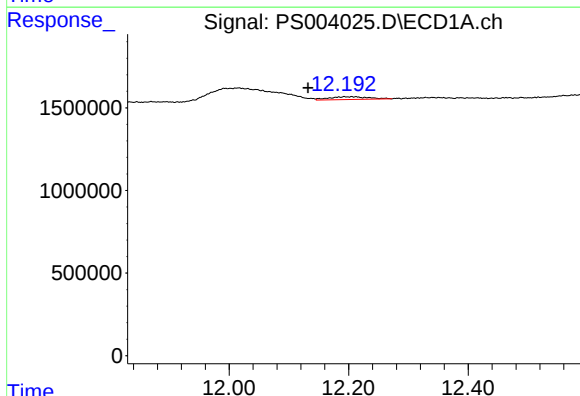


#7 MCPA

R.T.: 12.193 min
Delta R.T.: 0.061 min
Response: 787924
Conc: N.D.

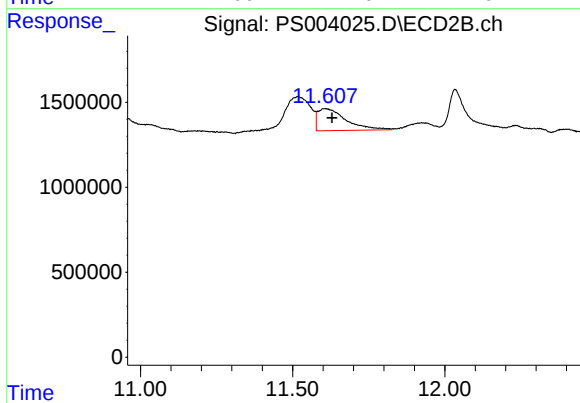

#7 MCPA


R.T.: 11.608 min
Delta R.T.: -0.022 min
Response: 8340632
Conc: 4.58 ug/ml

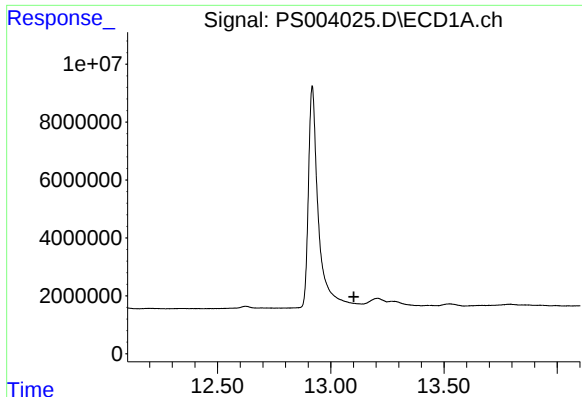

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

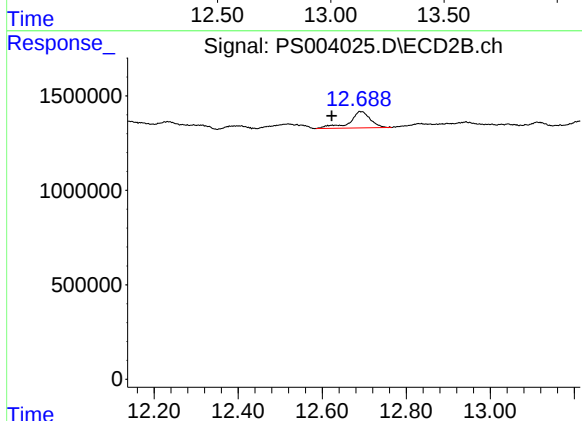


#9 2,4-D

R.T.: 12.691 min
Delta R.T.: 0.068 min
Response: 2994326
Conc: 5.85 ng/ml

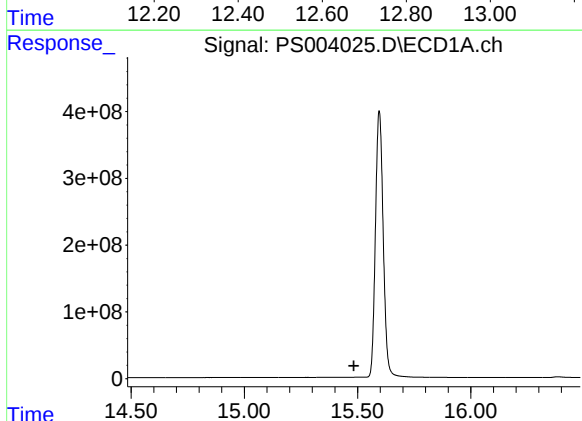


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.484 min
Response: 0
Conc: N.D.

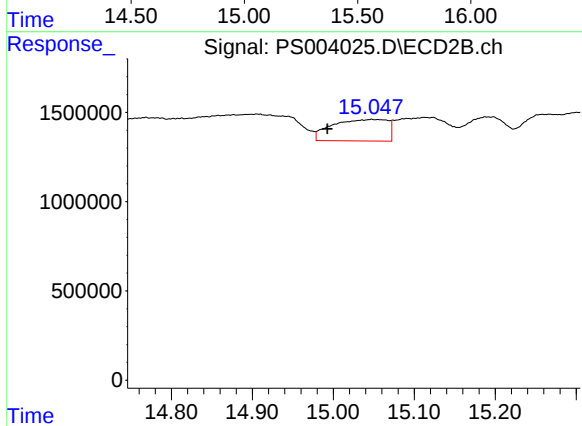

#13 2,4-DB


R.T.: 15.048 min
Delta R.T.: 0.055 min
Response: 5746992
Conc: 18.65 ng/ml

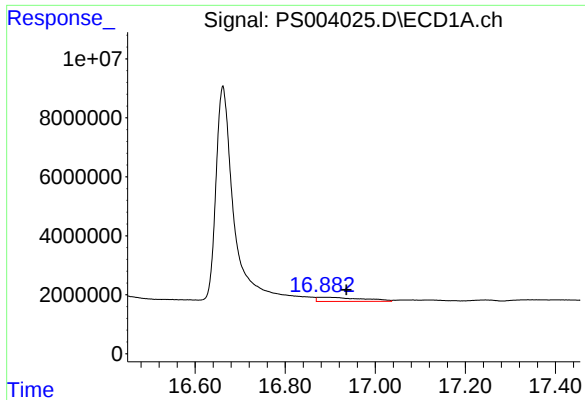

#14 DINOSEB


R.T.: 16.897 min
Delta R.T.: -0.039 min
Response: 9612078
Conc: 3.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

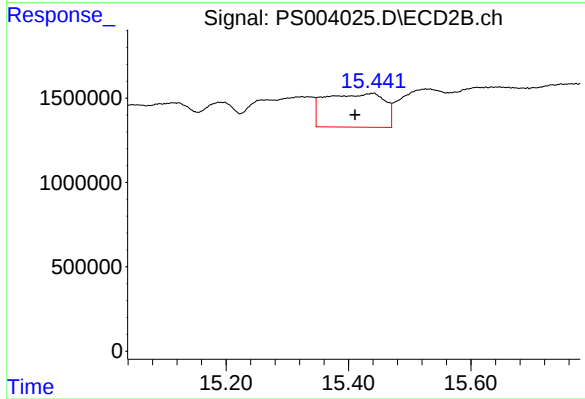


#14 DINOSEB

R.T.: 15.440 min
Delta R.T.: 0.029 min
Response: 13420963
Conc: 7.18 ng/ml

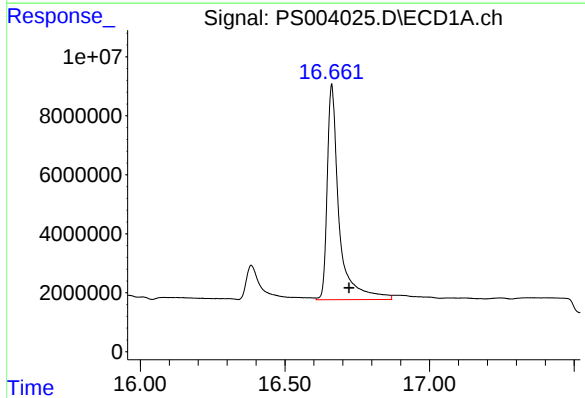


#15 Picloram

R.T.: 16.662 min
Delta R.T.: -0.059 min
Response: 208220271
Conc: 58.06 ng/ml

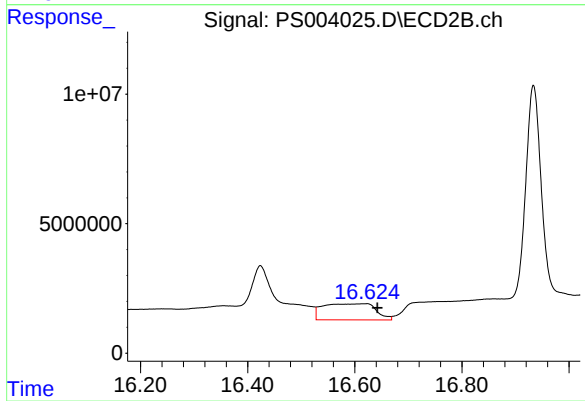

#15 Picloram


R.T.: 16.621 min
Delta R.T.: -0.022 min
Response: 42411427
Conc: 12.39 ng/ml

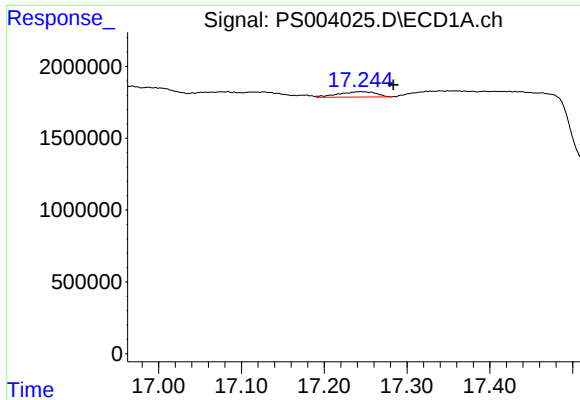

#16 DCPA

R.T.: 17.244 min
Delta R.T.: -0.039 min
Response: 1170143
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

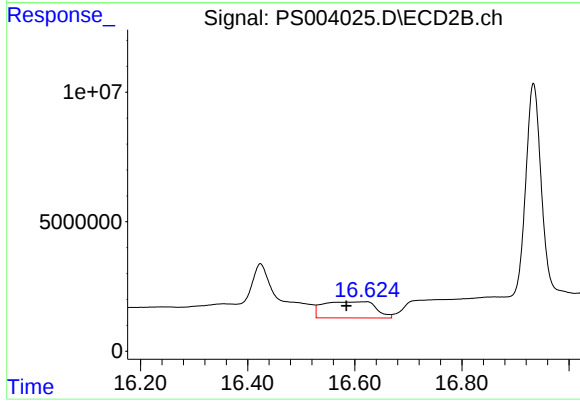

#16 DCPA

R.T.: 16.621 min
Delta R.T.: 0.036 min
Response: 42411427
Conc: 13.34 ng/ml