

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041119\
 Data File : PS004038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2019 17:27
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 17:57:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.214	10.715	288.4E6	235.3E6	594.336	512.301
Target Compounds							
7) T	MCPA	0.000	11.594	0	7932272	N.D.	4.360
14) T	DINOSEB	16.964	0.000	7700080	0	3.073	N.D. #
15) T	Picloram	16.774	16.701	6272254	1536488	1.749	<MDL #
16) T	DCPA	17.245	16.562	3020975	425115	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041119\
Data File : PS004038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2019 17:27
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 17:57:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

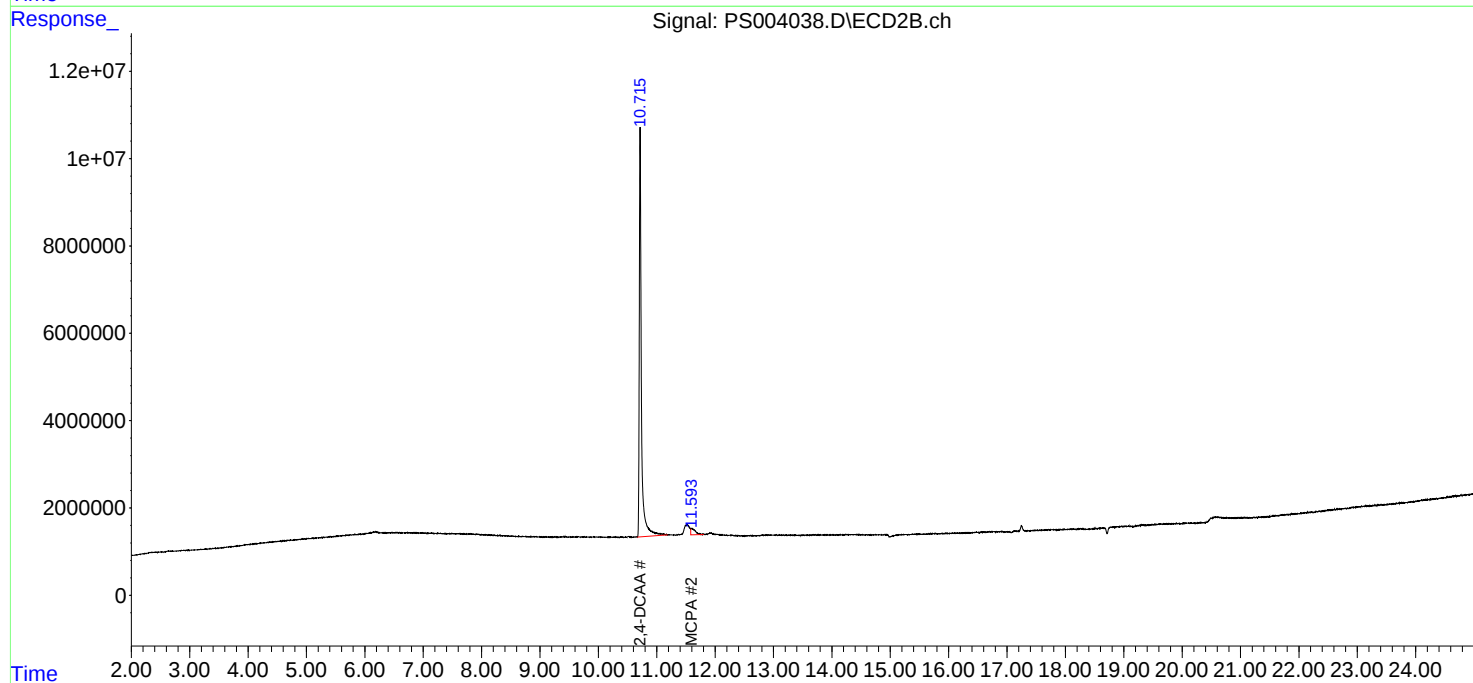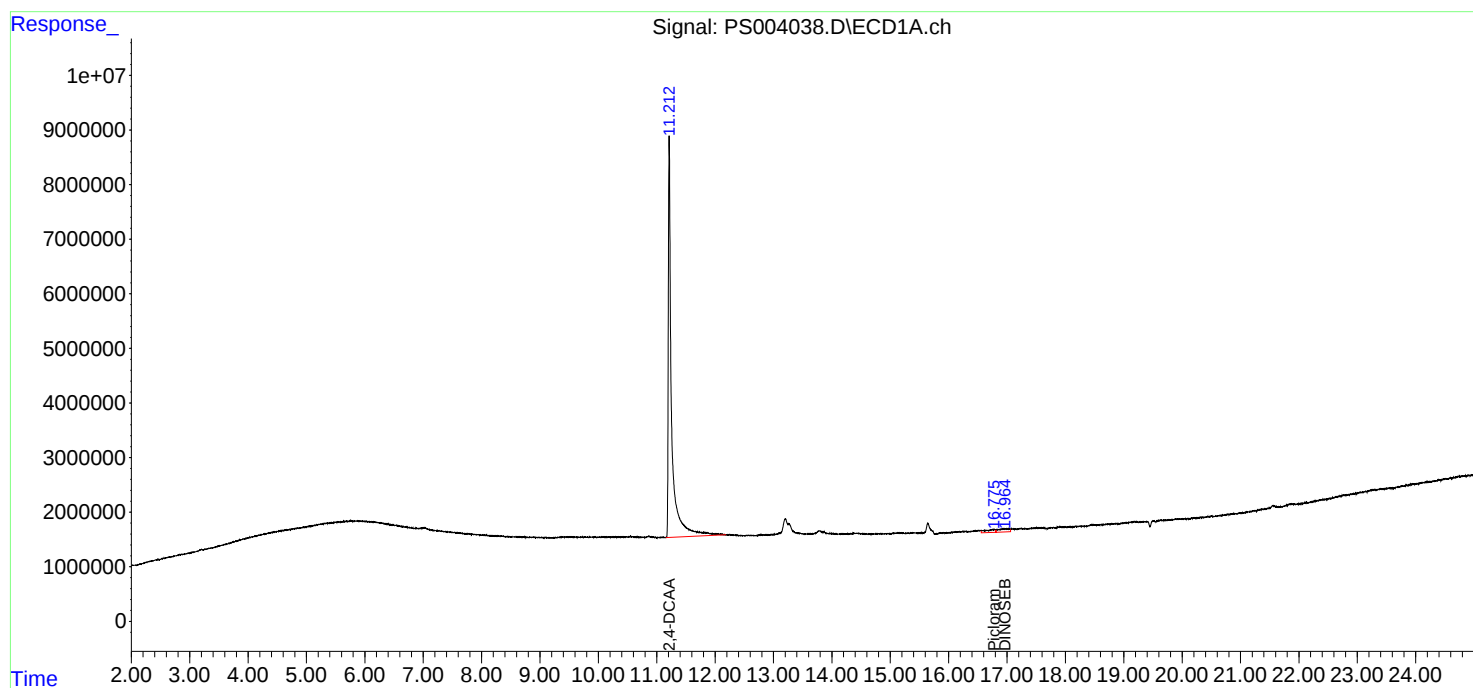


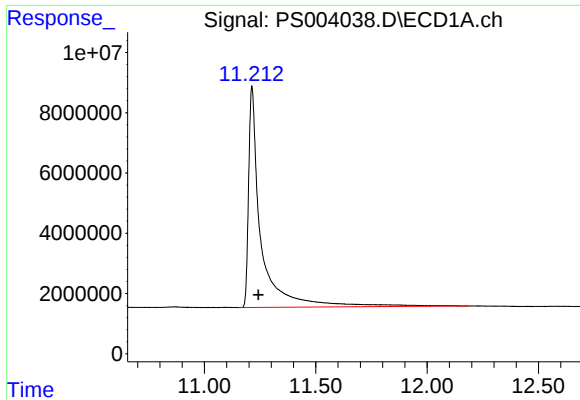

#4 2,4-DCAA


R.T.: 11.214 min
Delta R.T.: -0.029 min
Response: 288380331
Conc: 594.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

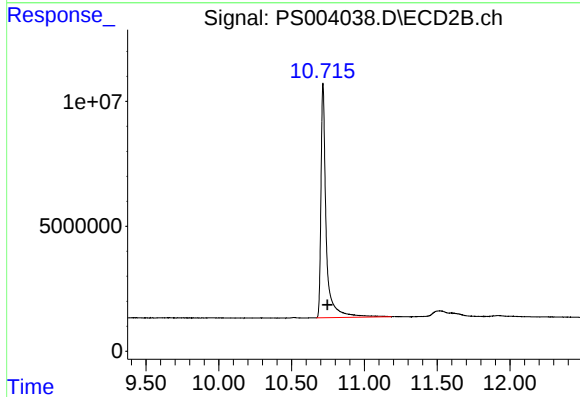


#4 2,4-DCAA

R.T.: 10.715 min
Delta R.T.: -0.030 min
Response: 235269991
Conc: 512.30 ng/ml

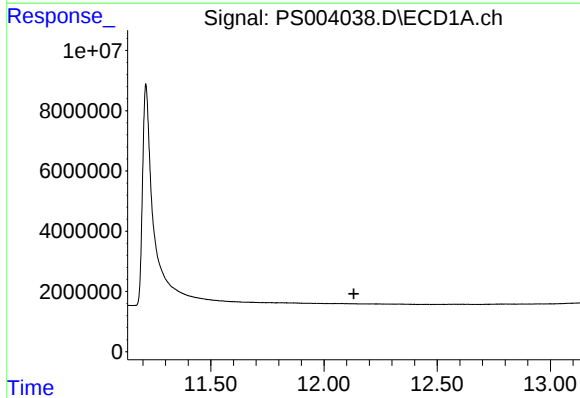


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.132 min
Response: 0
Conc: N.D.

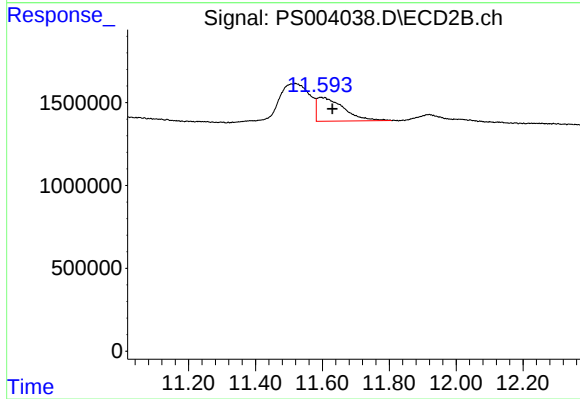

#7 MCPA


R.T.: 11.594 min
Delta R.T.: -0.036 min
Response: 7932272
Conc: 4.36 ug/ml

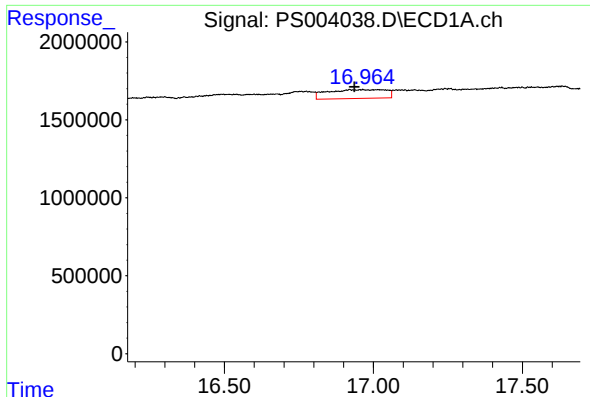

#14 DINOSEB


R.T.: 16.964 min
Delta R.T.: 0.027 min
Response: 7700080
Conc: 3.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

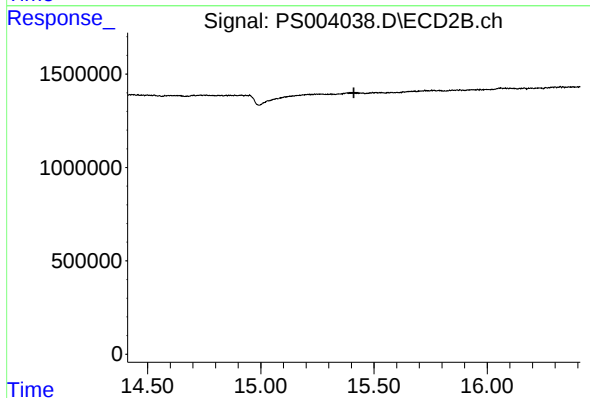


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 15.411 min
Response: 0
Conc: N.D.

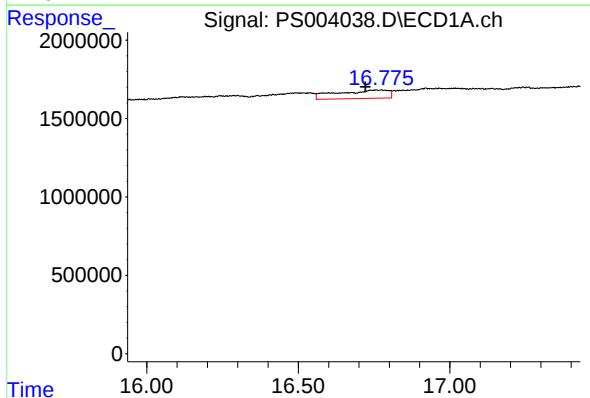

#15 Picloram

R.T.: 16.774 min
Delta R.T.: 0.053 min
Response: 6272254
Conc: 1.75 ng/ml

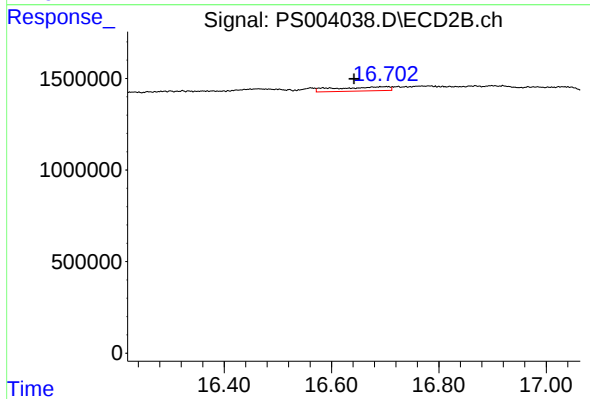

#15 Picloram

R.T.: 16.701 min
Delta R.T.: 0.059 min
Response: 1536488
Conc: N.D.