

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041119\
 Data File : PS004045.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2019 21:05
 Operator : EI\SJ
 Sample : PB118725TB
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB118725TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 07:37:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.207	10.714	194.1E6	169.9E6	399.929	369.901
Target Compounds							
3) T	4-Nitroph...	10.825	0.000	2028473	0	8.030	N.D. #
7) T	MCPA	0.000	11.601	0	11193712	N.D.	6.152
8) T	DICHLORPROP	12.716	0.000	1981163	0	4.092	N.D. #
11) T	2,4,5-TP ...	0.000	13.758	0	1210225	N.D.	<MDL
12) T	2,4,5-T	14.668	14.366	1172598	803545	<MDL	<MDL #
14) T	DINOSEB	16.965	15.384	1595417	1065913	<MDL	<MDL #
15) T	Picloram	16.676	16.663	1155972	3587924	<MDL	1.048 #
16) T	DCPA	17.287	16.555	168573	437900	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041119\
Data File : PS004045.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2019 21:05
Operator : EI\SJ
Sample : PB118725TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB118725TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 07:37:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

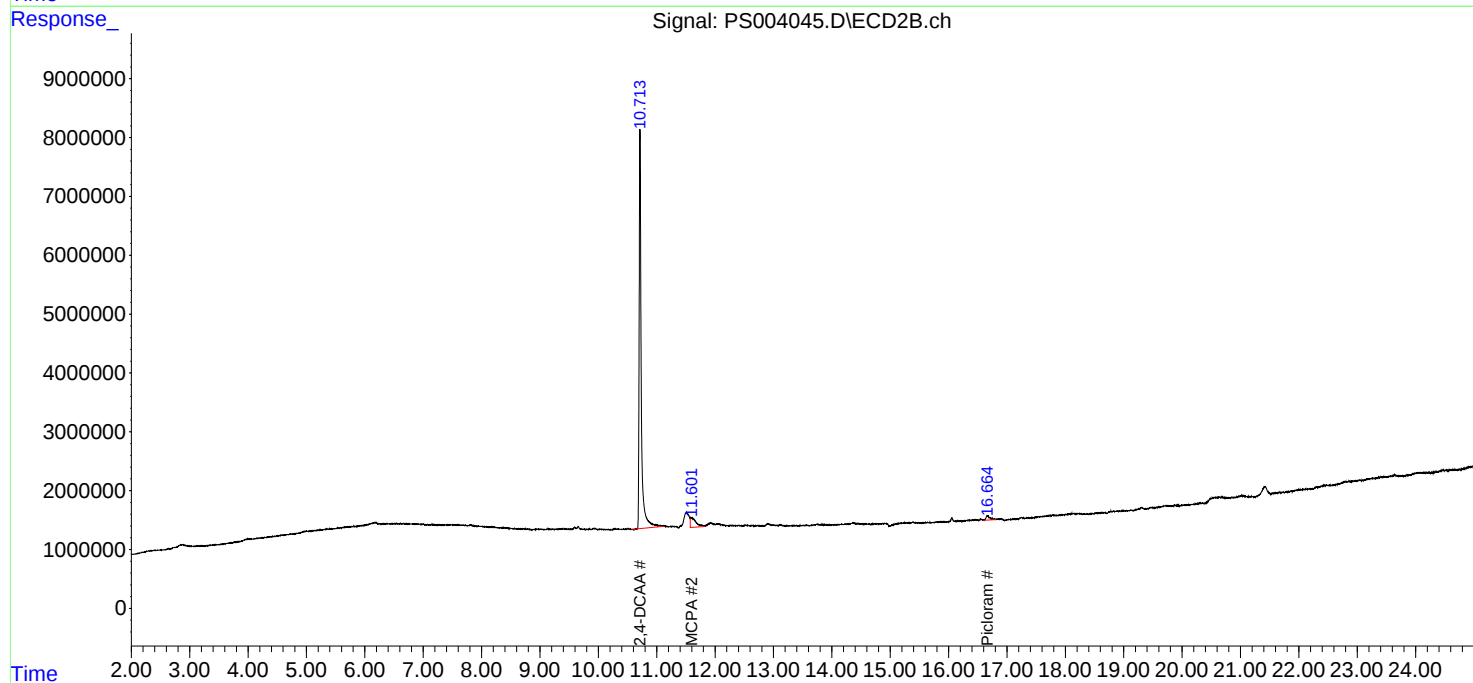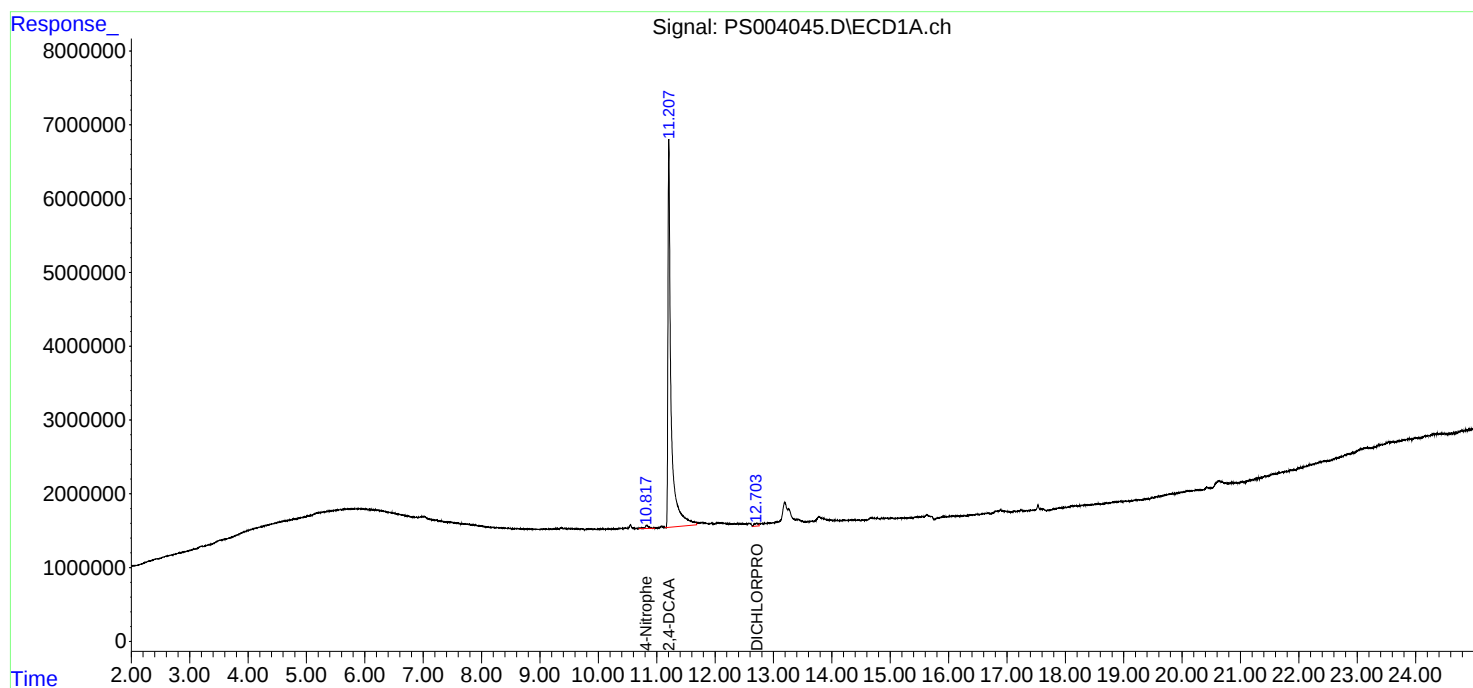


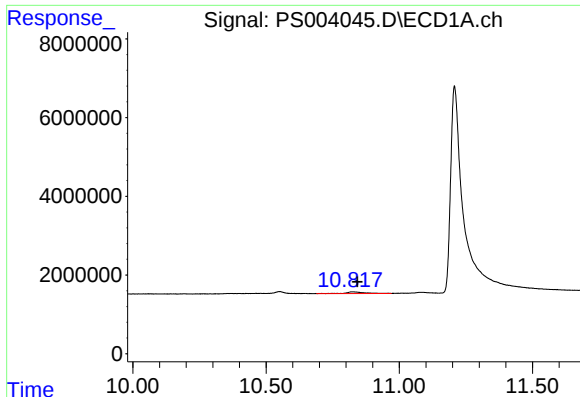

#3 4-Nitrophenol


R.T.: 10.825 min
Delta R.T.: -0.019 min
Response: 2028473
Conc: 8.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB118725TB

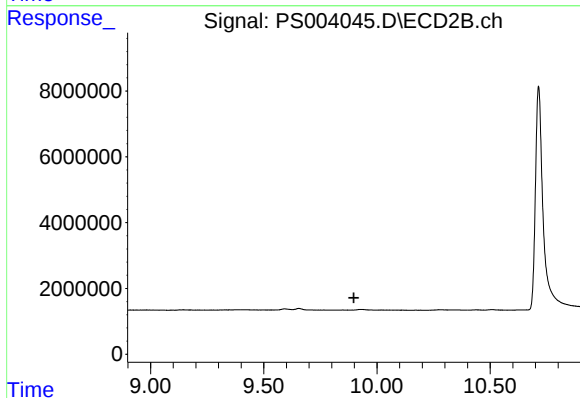


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 9.898 min
Response: 0
Conc: N.D.

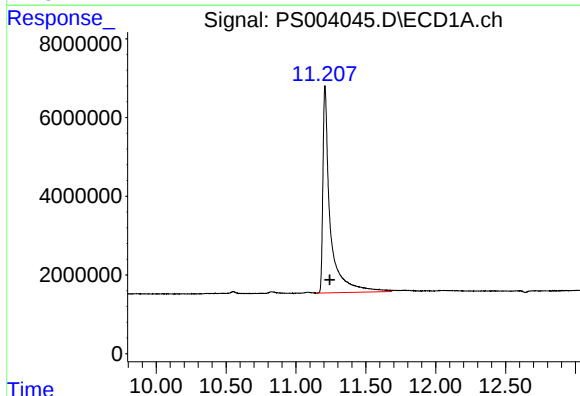


#4 2,4-DCAA

R.T.: 11.207 min
Delta R.T.: -0.036 min
Response: 194051331
Conc: 399.93 ng/ml

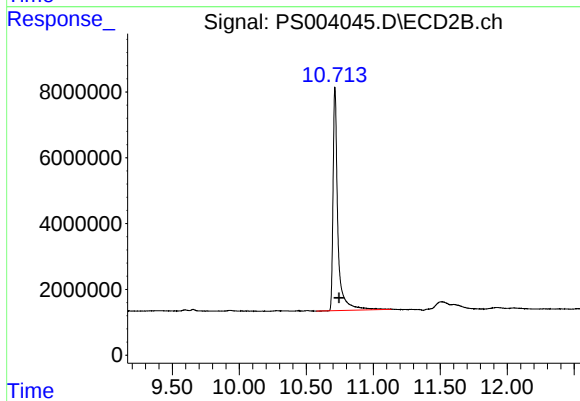

#4 2,4-DCAA


R.T.: 10.714 min
Delta R.T.: -0.032 min
Response: 169874095
Conc: 369.90 ng/ml

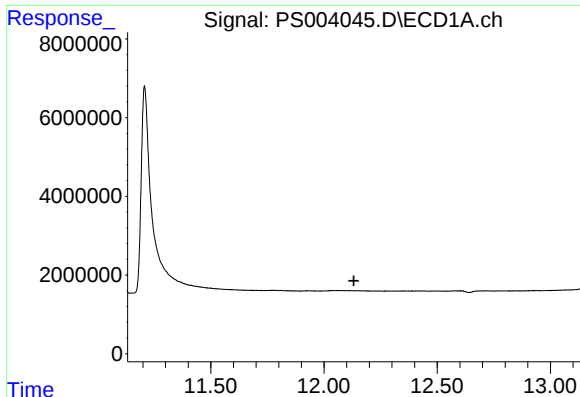

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.132 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118725TB

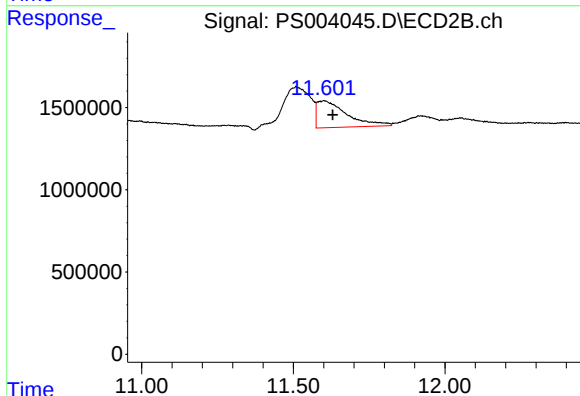


#7 MCPA

R.T.: 11.601 min
Delta R.T.: -0.029 min
Response: 11193712
Conc: 6.15 ug/ml

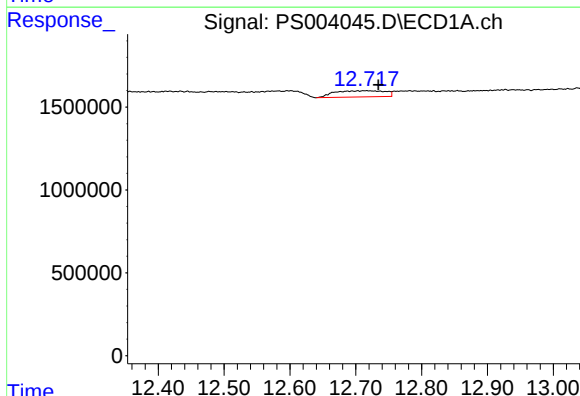


#8 DICHLORPROP

R.T.: 12.716 min
Delta R.T.: -0.019 min
Response: 1981163
Conc: 4.09 ng/ml

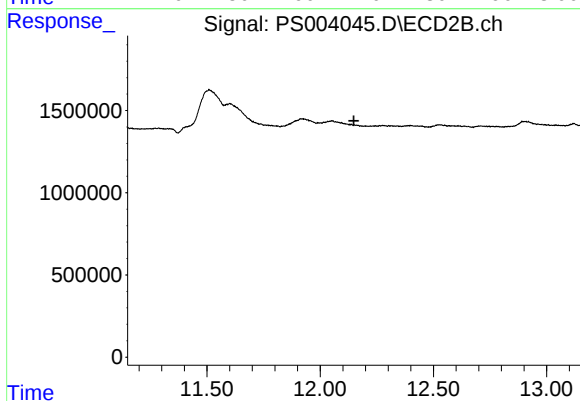

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.149 min
Response: 0
Conc: N.D.

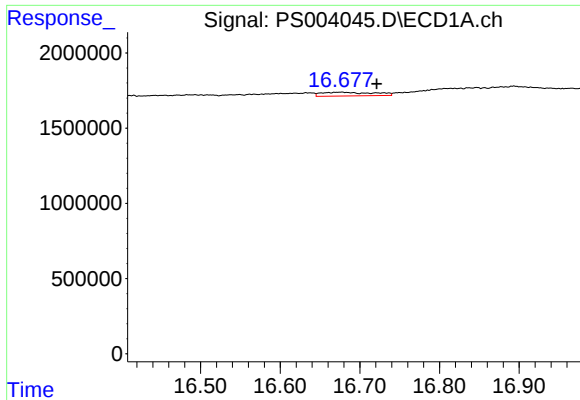

#15 Picloram

R.T.: 16.676 min
Delta R.T.: -0.045 min
Response: 1155972
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB118725TB

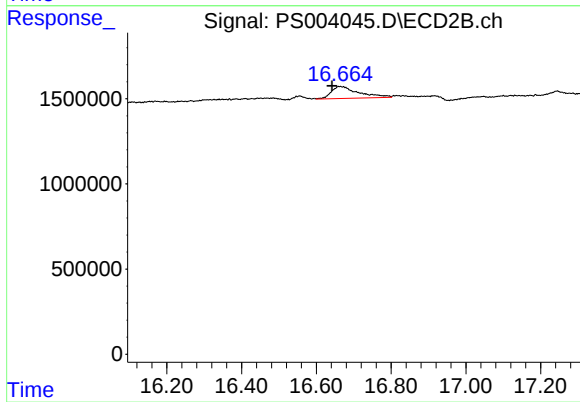

#15 Picloram

R.T.: 16.663 min
Delta R.T.: 0.021 min
Response: 3587924
Conc: 1.05 ng/ml