

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041119\
 Data File : PS004058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2019 03:50
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 07:41:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.217	10.730	282.2E6	245.3E6	581.614	534.135
Target Compounds							
7) T	MCPA	0.000	11.616	0	6731460	N.D.	3.700
10) T	Pentachlo...	0.000	13.138	0	1721623	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.777	0	2081169	N.D.	<MDL
15) T	Picloram	16.713	0.000	26666601	0	7.436	N.D. #
16) T	DCPA	17.252	0.000	28762078	0	7.990	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041119\
Data File : PS004058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2019 03:50
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 07:41:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

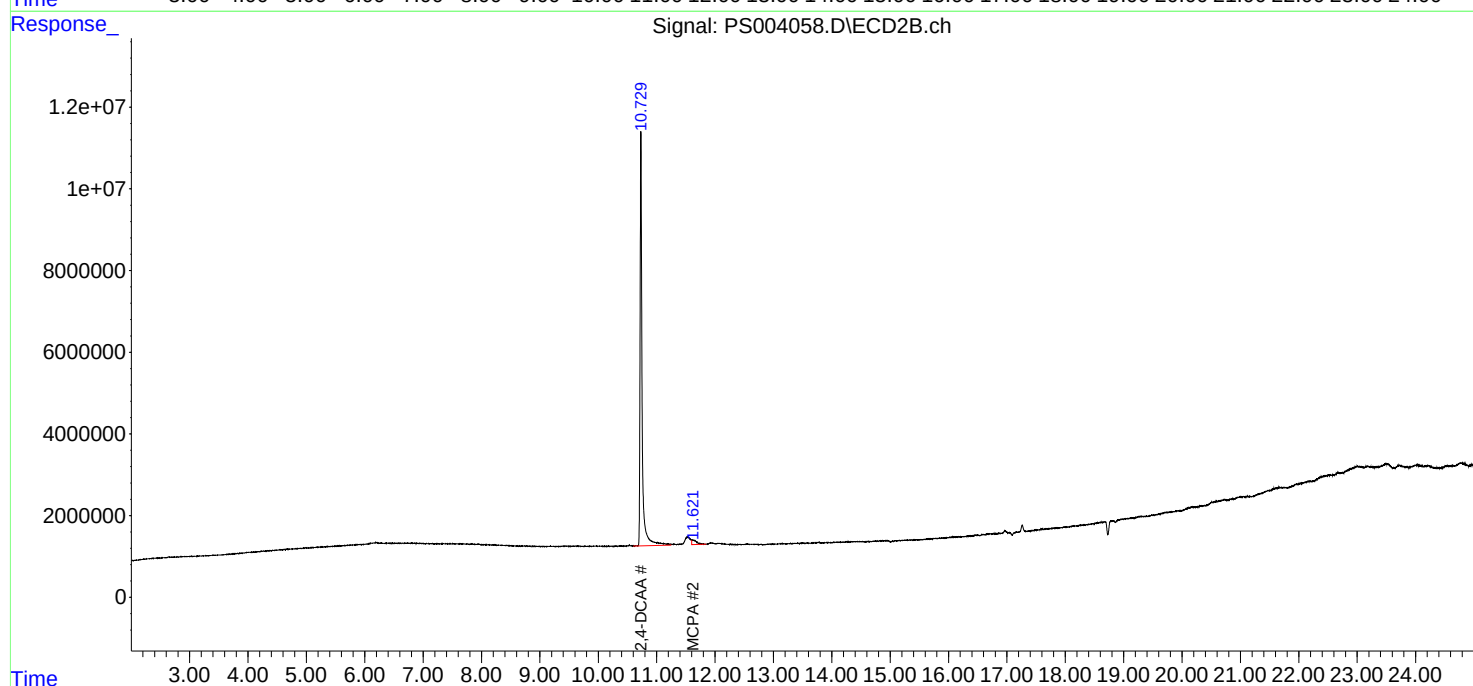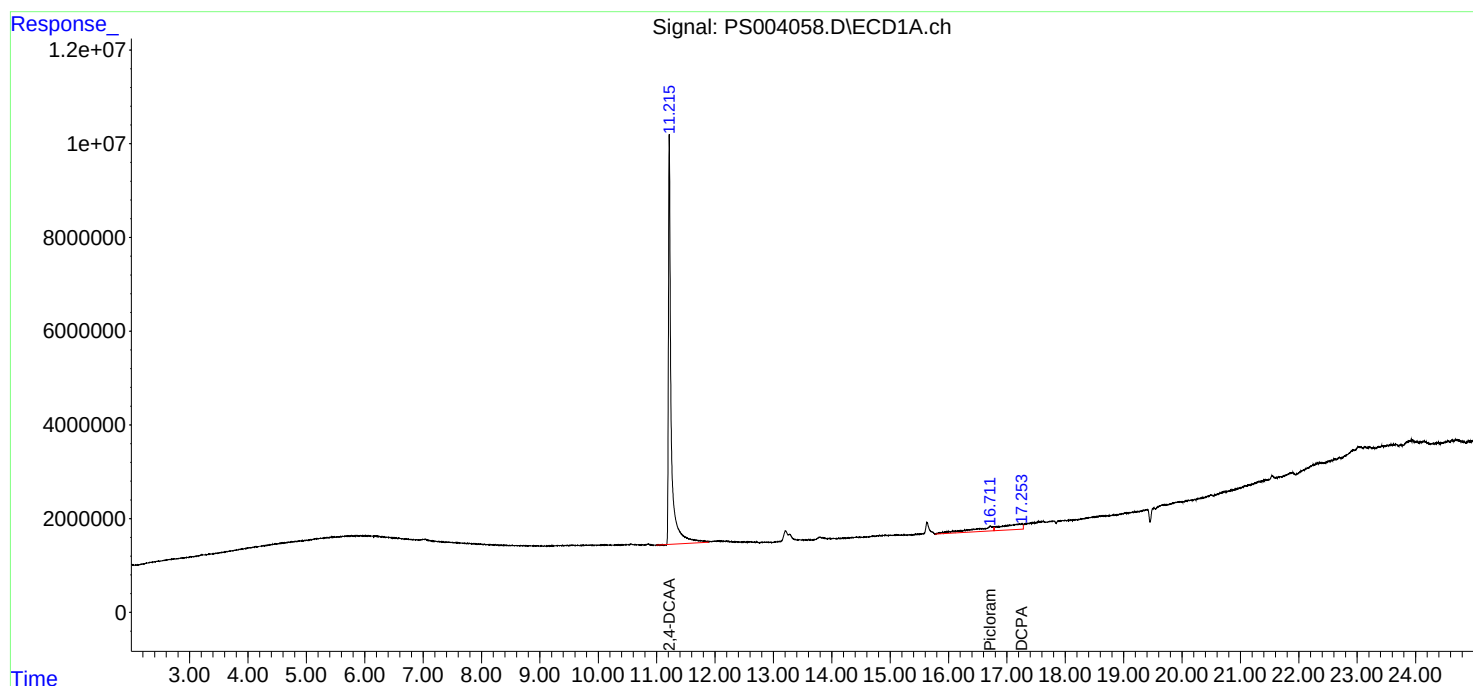


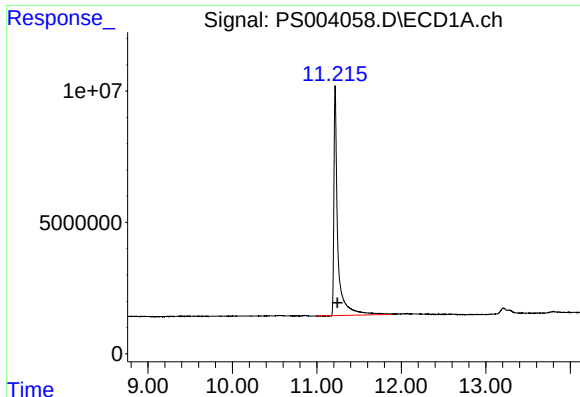

#4 2,4-DCAA


R.T.: 11.217 min
Delta R.T.: -0.027 min
Response: 282207463
Conc: 581.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

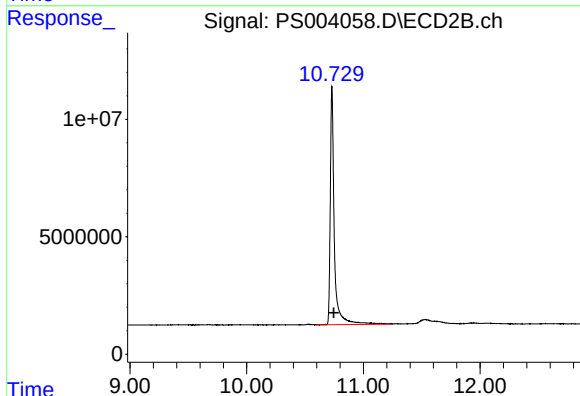


#4 2,4-DCAA

R.T.: 10.730 min
Delta R.T.: -0.015 min
Response: 245297023
Conc: 534.13 ng/ml

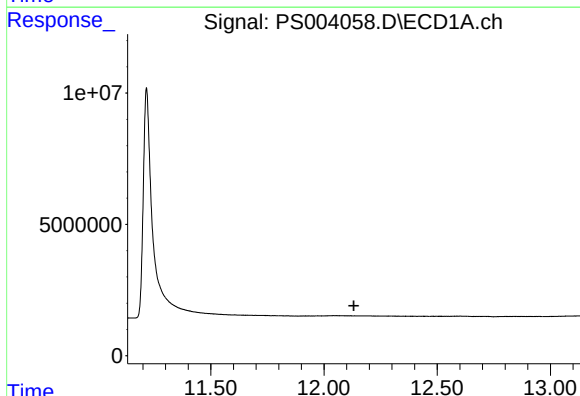


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.132 min
Response: 0
Conc: N.D.

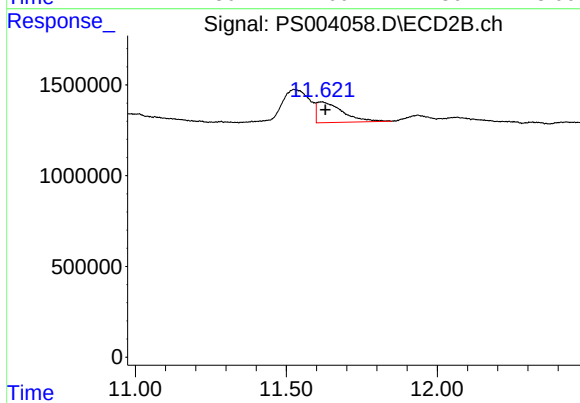

#7 MCPA


R.T.: 11.616 min
Delta R.T.: -0.014 min
Response: 6731460
Conc: 3.70 ug/ml

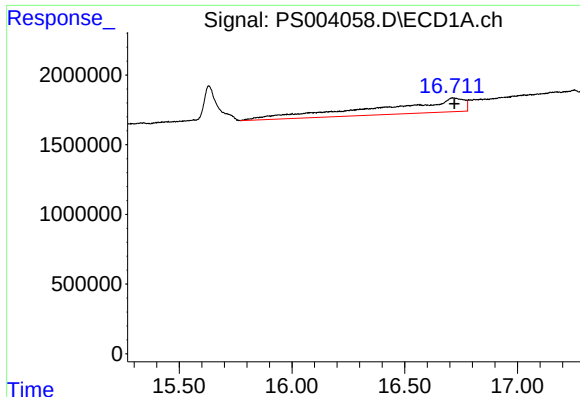

#15 Picloram


R.T.: 16.713 min
Delta R.T.: -0.008 min
Response: 26666601
Conc: 7.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

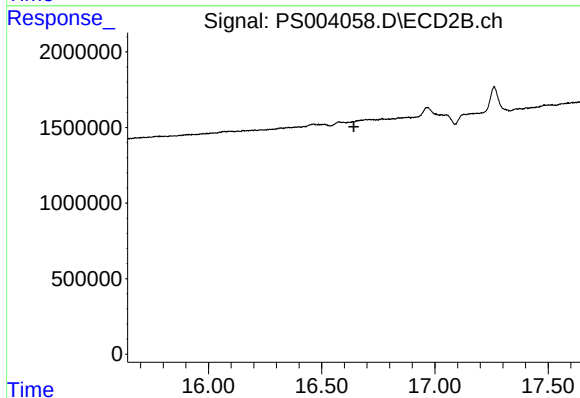


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.642 min
Response: 0
Conc: N.D.

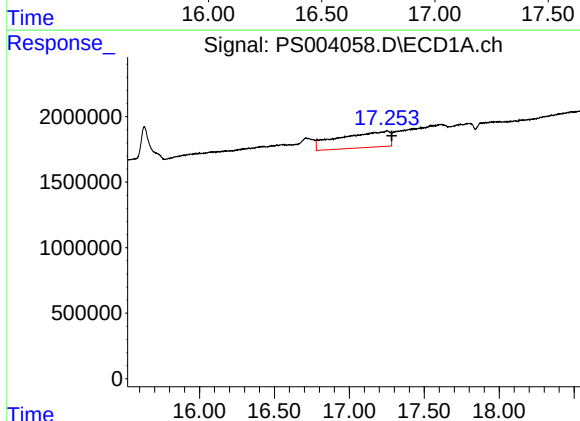

#16 DCPA

R.T.: 17.252 min
Delta R.T.: -0.032 min
Response: 28762078
Conc: 7.99 ng/ml

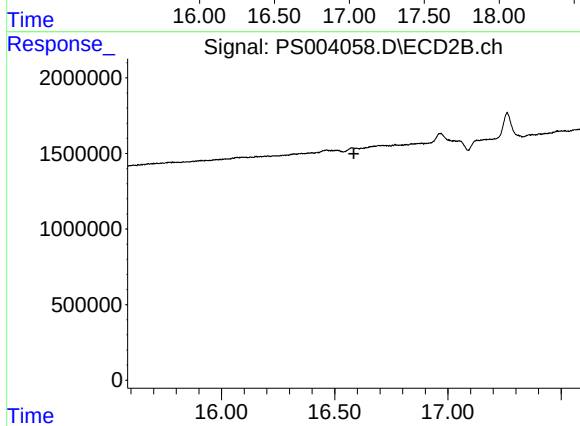

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 16.584 min
Response: 0
Conc: N.D.