

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042219\
 Data File : PS004183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2019 13:19
 Operator : EI\SJ
 Sample : MDL-BL-WATER-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 MDL-BL-WATER-04

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 01:11:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.214	10.714	214.5E6	168.9E6	442.085	367.761
Target Compounds							
3) T	4-Nitroph...	10.852	0.000	428841	0	1.698	N.D. #
6) T	MCP	11.853	0.000	2992605	0	2.292	N.D. #
8) T	DICHLORPROP	12.721	0.000	400199	0	<MDL	N.D. #
10) T	Pentachlo...	13.426	0.000	326991	0	<MDL	N.D. #
11) T	2,4,5-TP ...	14.296	0.000	394874	0	<MDL	N.D. #
12) T	2,4,5-T	14.743	0.000	817551	0	<MDL	N.D. #
13) T	2,4-DB	15.437	0.000	591687	0	1.900	N.D. #
15) T	Picloram	16.709	0.000	108013	0	<MDL	N.D. #
16) T	DCPA	17.269	0.000	986620	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042219\
Data File : PS004183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2019 13:19
Operator : EI\SJ
Sample : MDL-BL-WATER-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-04

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 01:11:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

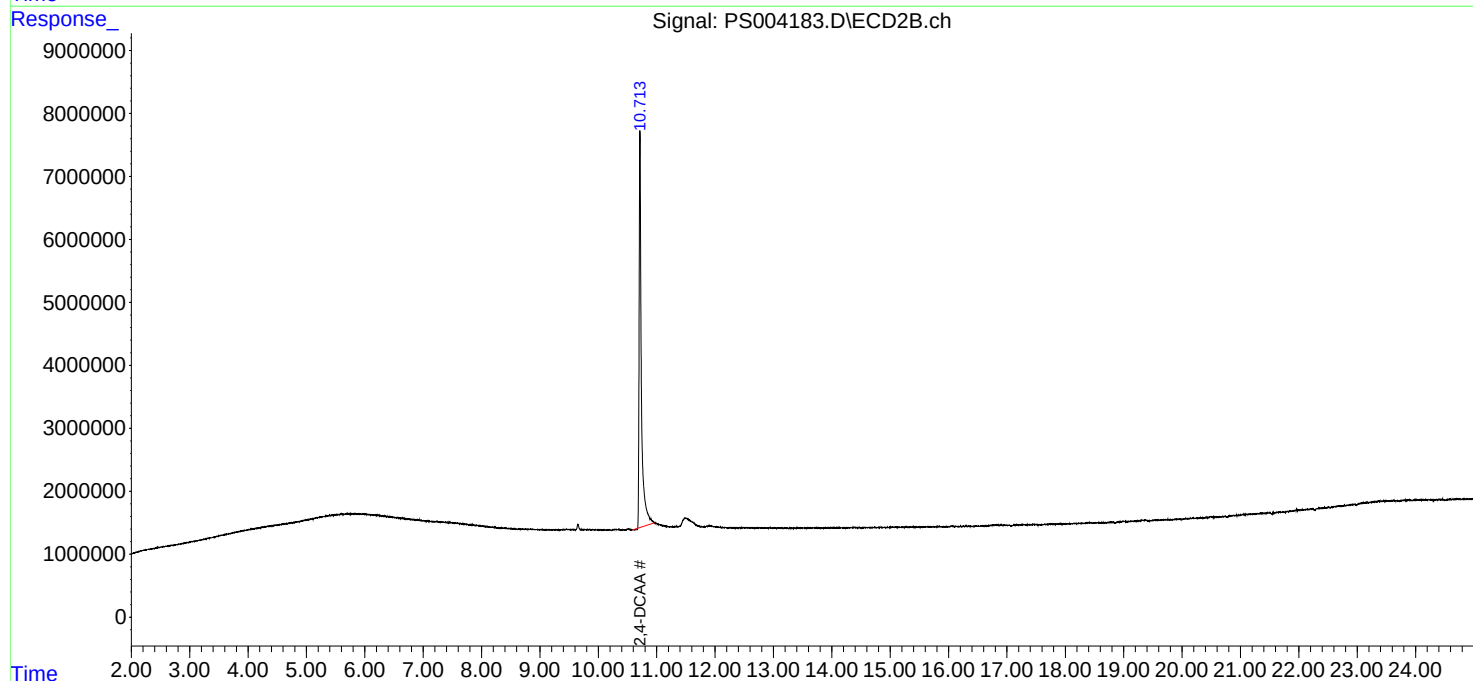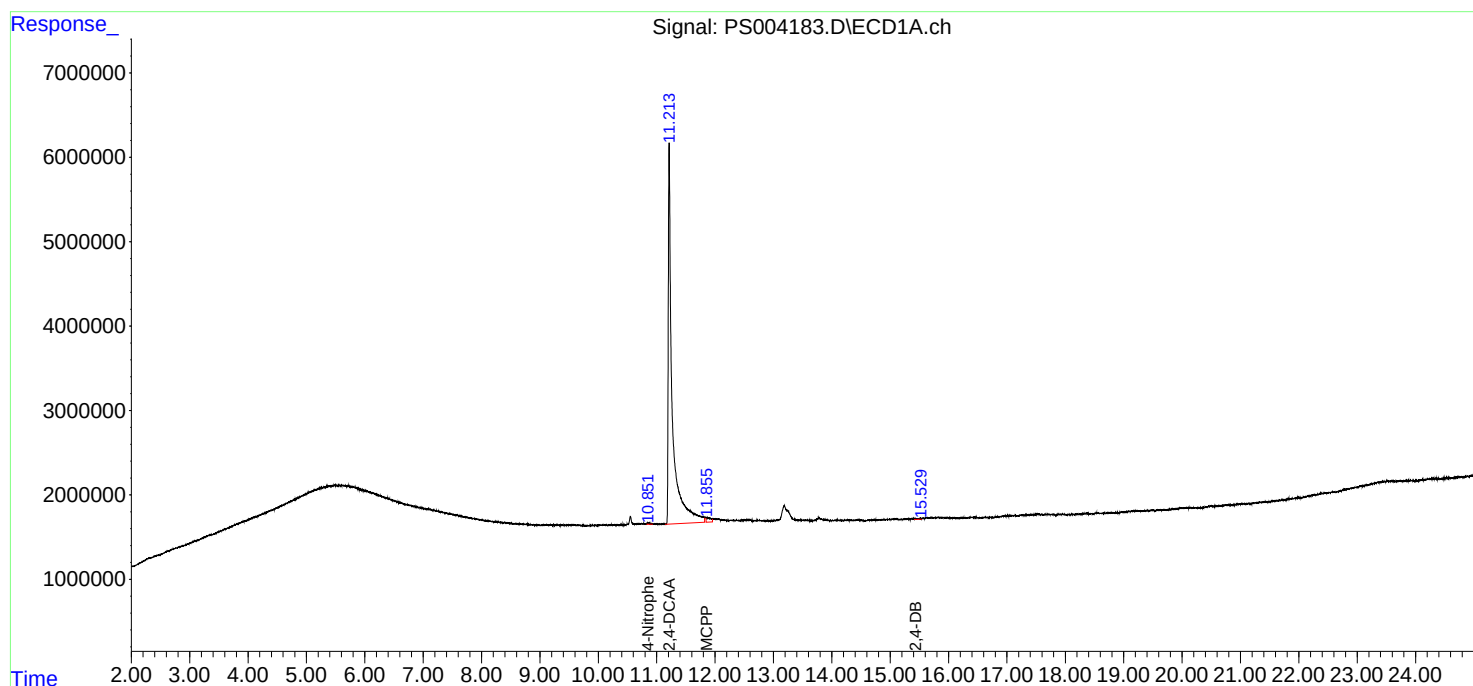


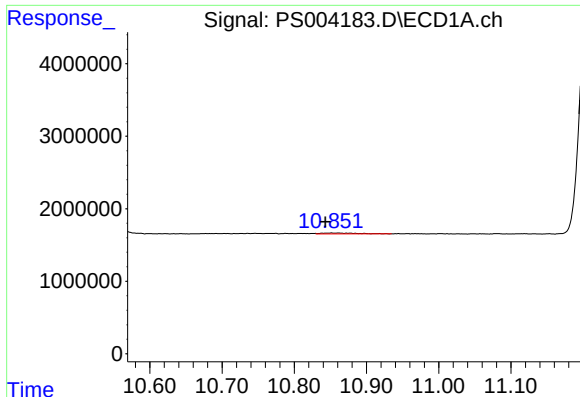

#3 4-Nitrophenol


R.T.: 10.852 min
Delta R.T.: 0.008 min
Response: 428841
Conc: 1.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-04

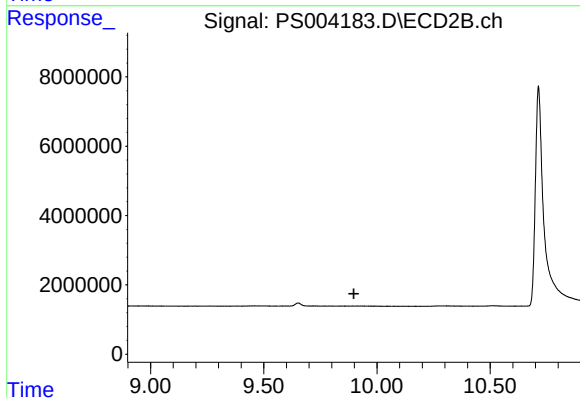


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 9.898 min
Response: 0
Conc: N.D.

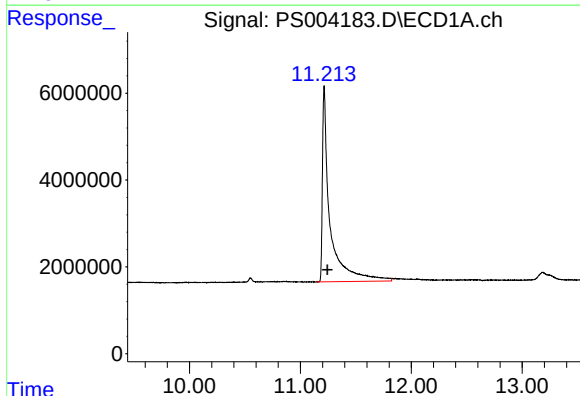


#4 2,4-DCAA

R.T.: 11.214 min
Delta R.T.: -0.029 min
Response: 214505949
Conc: 442.08 ng/ml

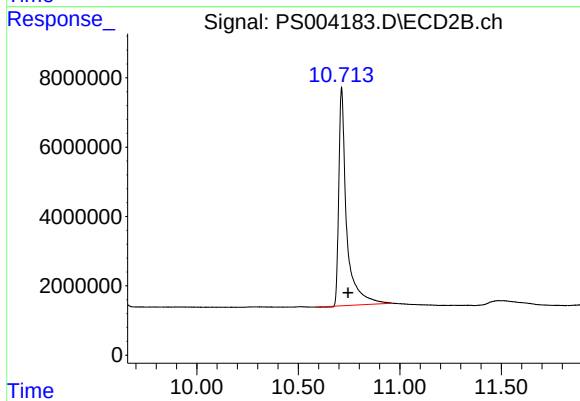

#4 2,4-DCAA


R.T.: 10.714 min
Delta R.T.: -0.032 min
Response: 168891113
Conc: 367.76 ng/ml

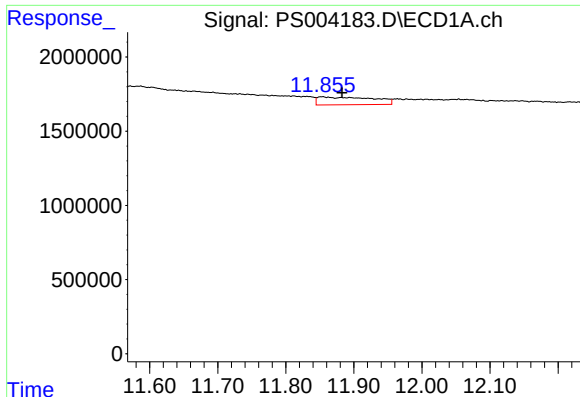

#6 MCP


R.T.: 11.853 min
Delta R.T.: -0.029 min
Response: 2992605
Conc: 2.29 ug/ml

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-04

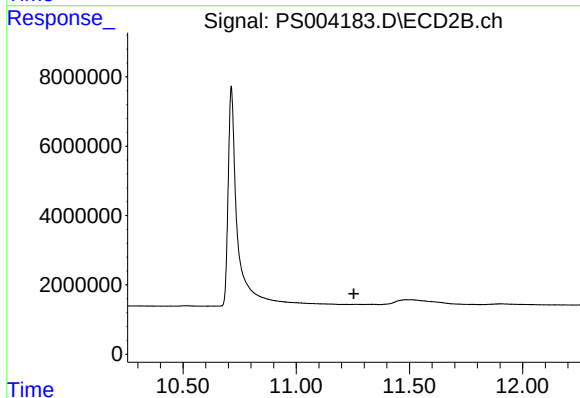


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.255 min
Response: 0
Conc: N.D.

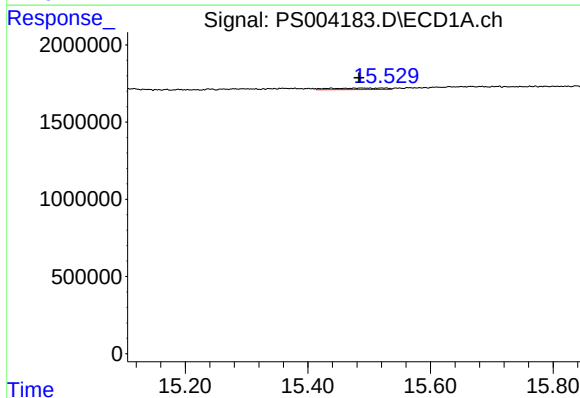

#13 2,4-DB

R.T.: 15.437 min
Delta R.T.: -0.046 min
Response: 591687
Conc: 1.90 ng/ml

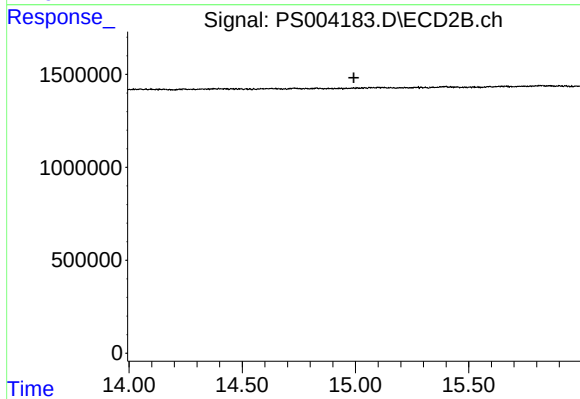

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 14.993 min
Response: 0
Conc: N.D.