

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042219\
 Data File : PS004185.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2019 14:25
 Operator : EI\SJ
 Sample : MDL-BL-WATER-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 MDL-BL-WATER-05

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 01:12:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.217	10.716	209.2E6	168.9E6	431.098	367.730
Target Compounds							
3) T	4-Nitroph...	10.869	0.000	1482010	0	5.867	N.D. #
6) T	MCP	11.877	0.000	2813192	0	2.155	N.D. #
7) T	MCPA	12.187	0.000	2354573	0	1.141	N.D. #
8) T	DICHLORPROP	12.716	0.000	1213384	0	2.506	N.D. #
10) T	Pentachlo...	13.433	0.000	1519698	0	<MDL	N.D. #
14) T	DINOSEB	16.920	0.000	674796	0	<MDL	N.D. #
15) T	Picloram	16.696	0.000	593071	0	<MDL	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042219\
Data File : PS004185.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2019 14:25
Operator : EI\SJ
Sample : MDL-BL-WATER-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-05

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 01:12:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

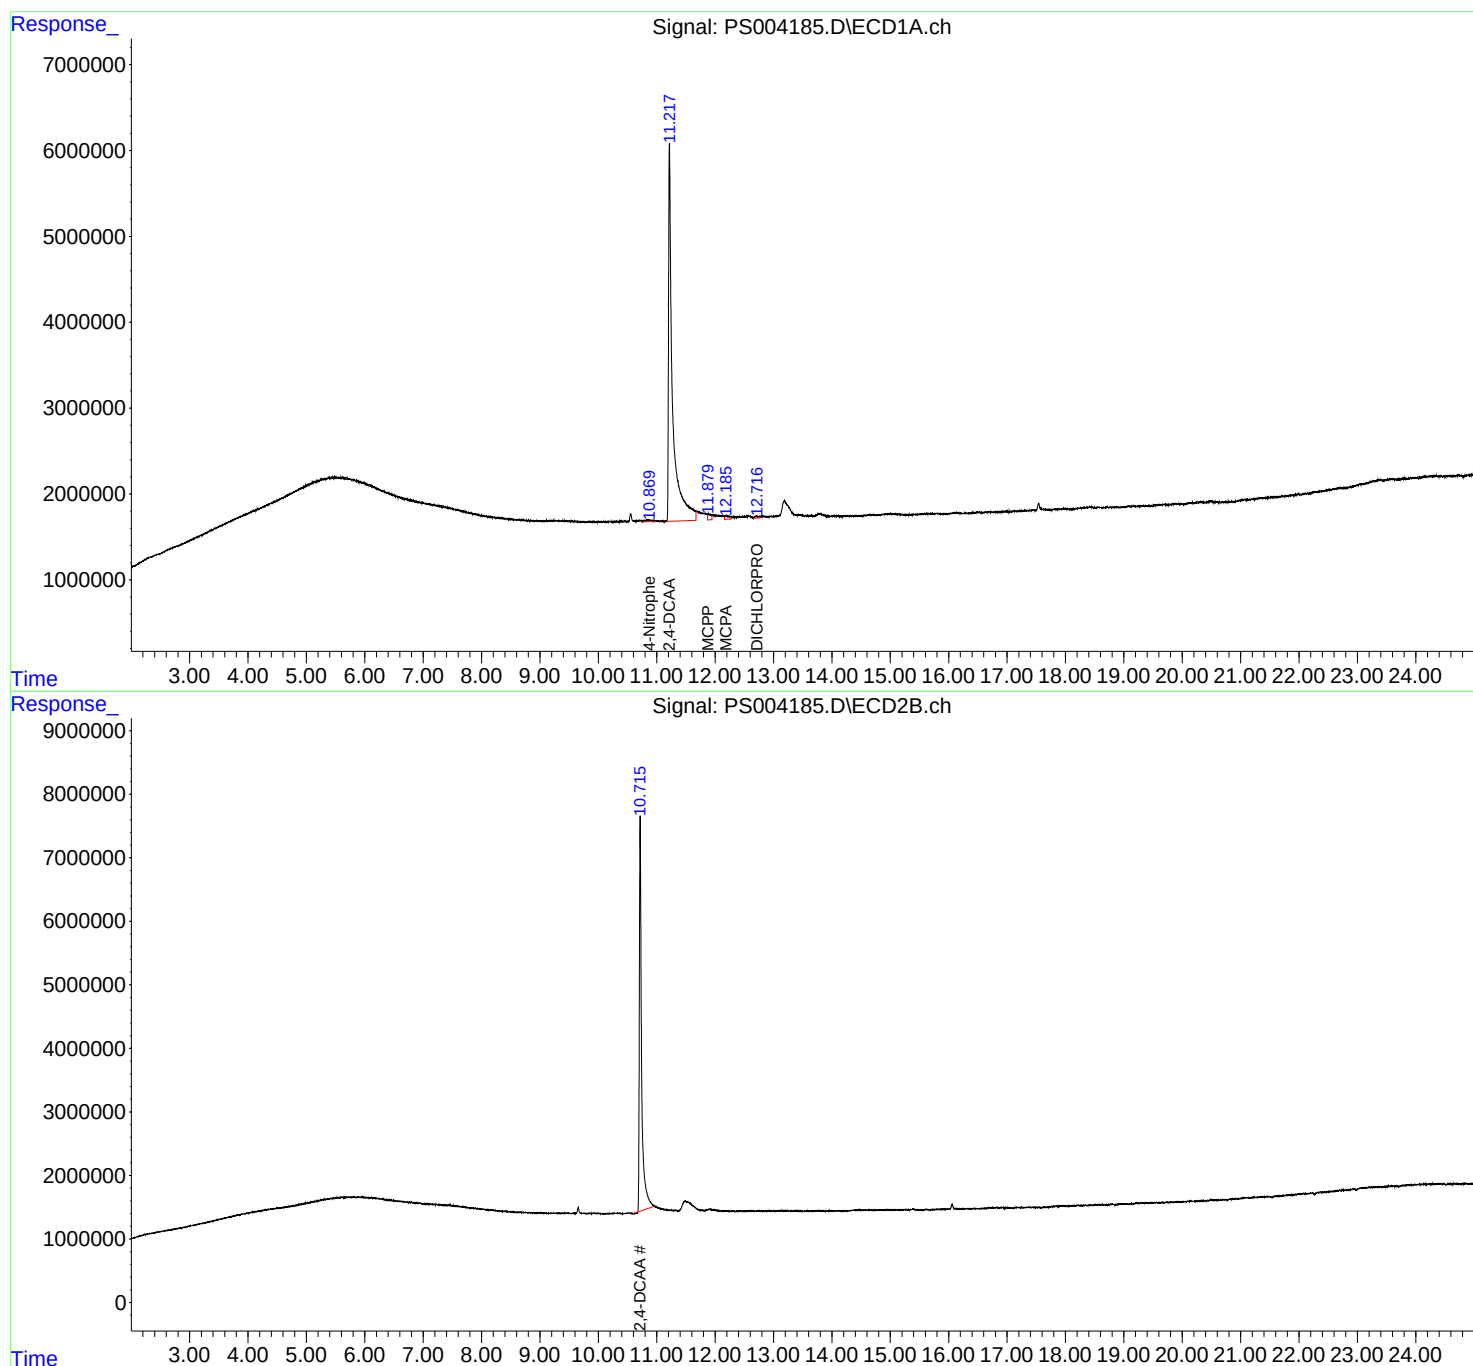


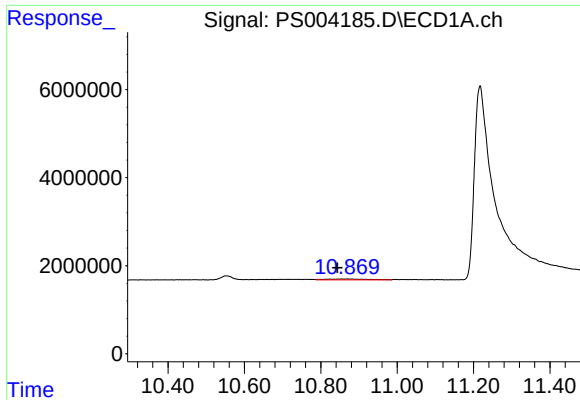

#3 4-Nitrophenol


R.T.: 10.869 min
Delta R.T.: 0.026 min
Response: 1482010
Conc: 5.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-05

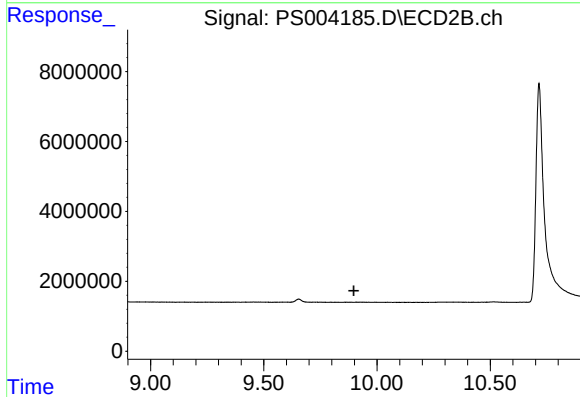


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 9.898 min
Response: 0
Conc: N.D.

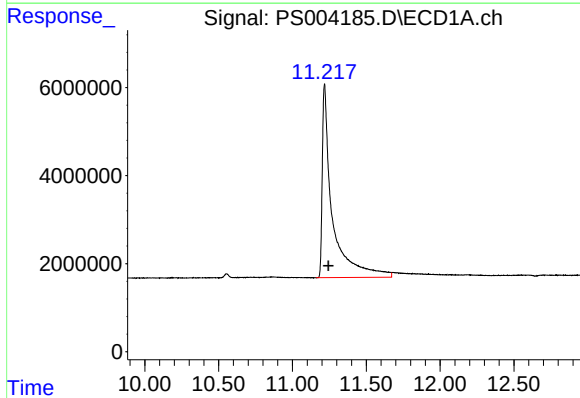


#4 2,4-DCAA

R.T.: 11.217 min
Delta R.T.: -0.026 min
Response: 209175137
Conc: 431.10 ng/ml

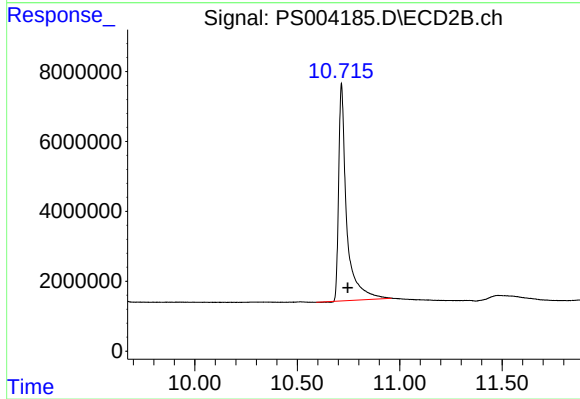

#4 2,4-DCAA


R.T.: 10.716 min
Delta R.T.: -0.030 min
Response: 168877203
Conc: 367.73 ng/ml

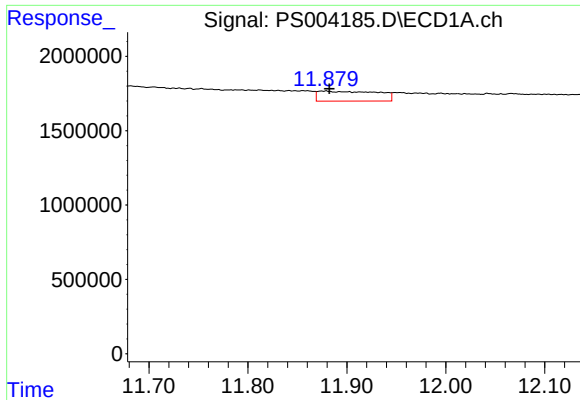

#6 MCPP


R.T.: 11.877 min
Delta R.T.: -0.005 min
Response: 2813192
Conc: 2.15 ug/ml

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-05

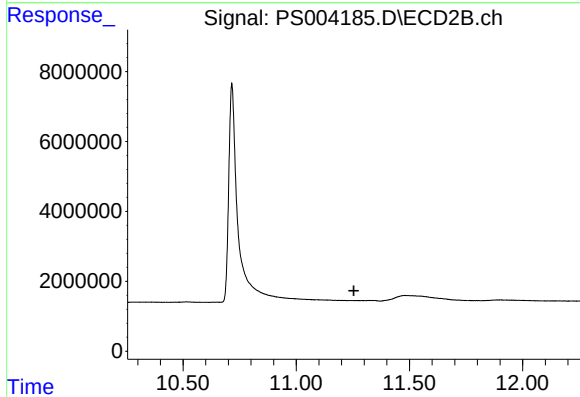


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.255 min
Response: 0
Conc: N.D.

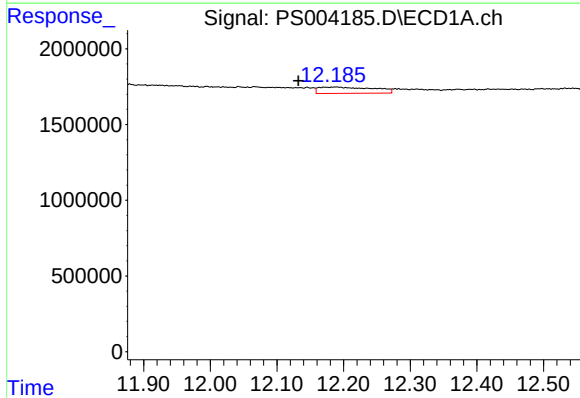


#7 MCPA

R.T.: 12.187 min
Delta R.T.: 0.055 min
Response: 2354573
Conc: 1.14 ug/ml

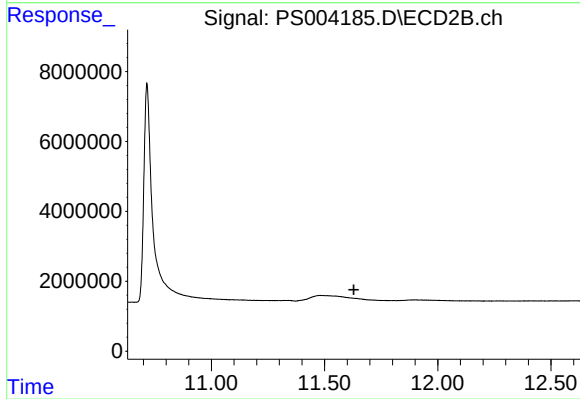

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 11.630 min
Response: 0
Conc: N.D.

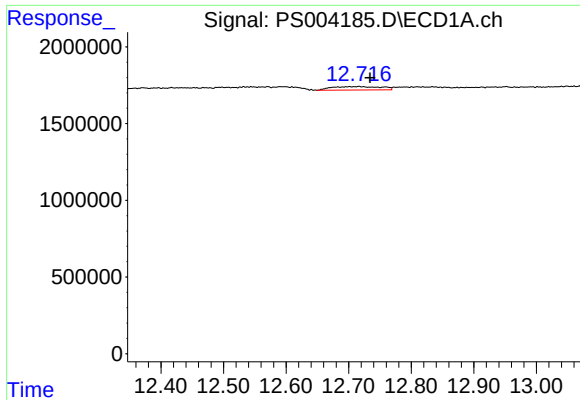

#8 DICHLORPROP

R.T.: 12.716 min
Delta R.T.: -0.018 min
Response: 1213384
Conc: 2.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-05

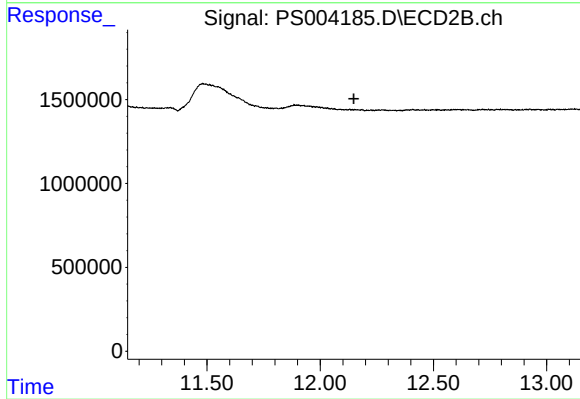

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.149 min
Response: 0
Conc: N.D.