

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042219\
 Data File : PS004214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 06:10
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 07:07:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.208	10.708	268.3E6	228.2E6	552.996	496.844
Target Compounds							
2) T	3,5-DICHL...	9.684	0.000	126924	0	<MDL	N.D. #
3) T	4-Nitroph...	10.874	0.000	1157412	0	4.582	N.D. #
5) T	DICAMBA	11.509	10.991	33493340	687639	17.075	<MDL #
6) T	MCPD	11.910	0.000	5371024	0	4.114	N.D. #
7) T	MCPA	12.158	0.000	792609	0	<MDL	N.D. #
8) T	DICHLORPROP	12.783	0.000	237883	0	<MDL	N.D. #
10) T	Pentachlo...	13.459	0.000	621877	0	<MDL	N.D. #
11) T	2,4,5-TP ...	14.369	13.777	3470939	1616725	1.282	<MDL #
13) T	2,4-DB	15.552	0.000	7402959	0	23.772	N.D. #
14) T	DINOSEB	16.905	15.388	39121393	2089833	15.615	1.118 #
15) T	Picloram	16.669	16.702	27741766	534742	7.736	<MDL #
16) T	DCPA	17.260	0.000	49489567	0	13.748	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042219\
Data File : PS004214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2019 06:10
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 07:07:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

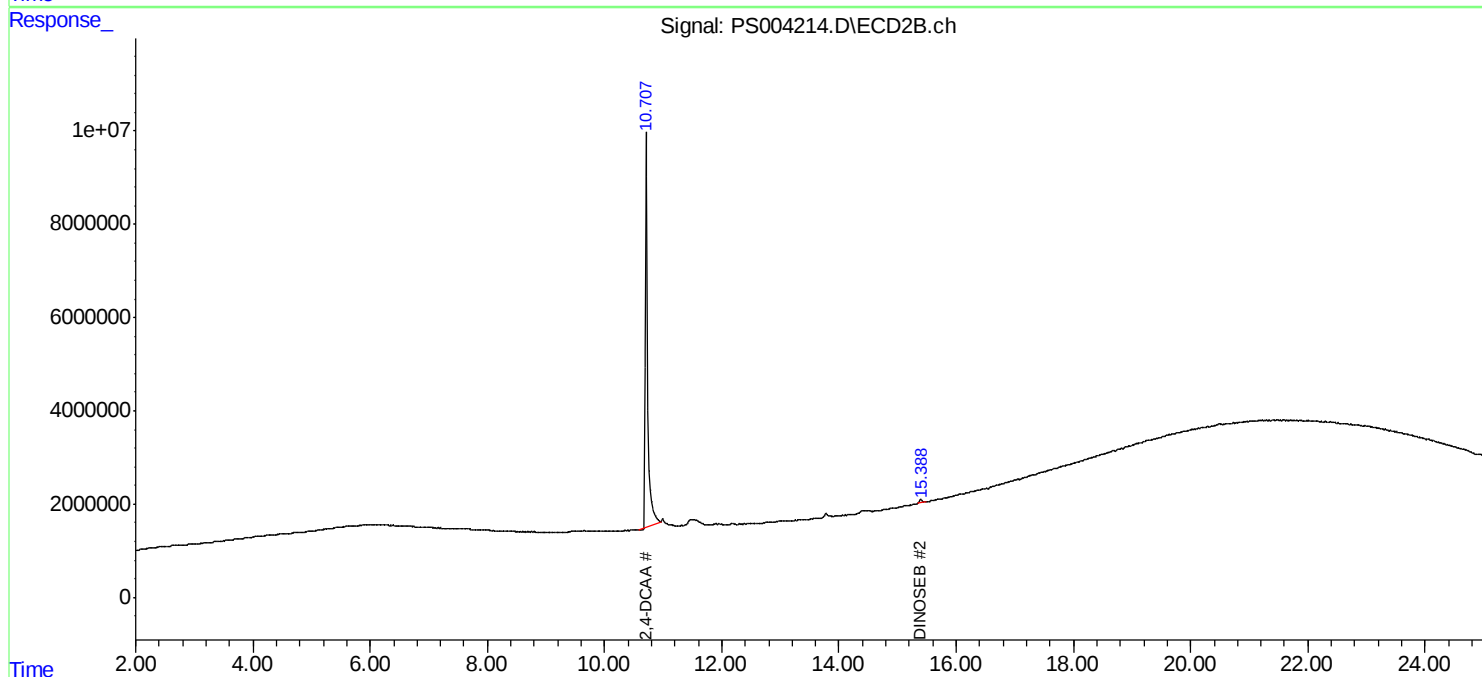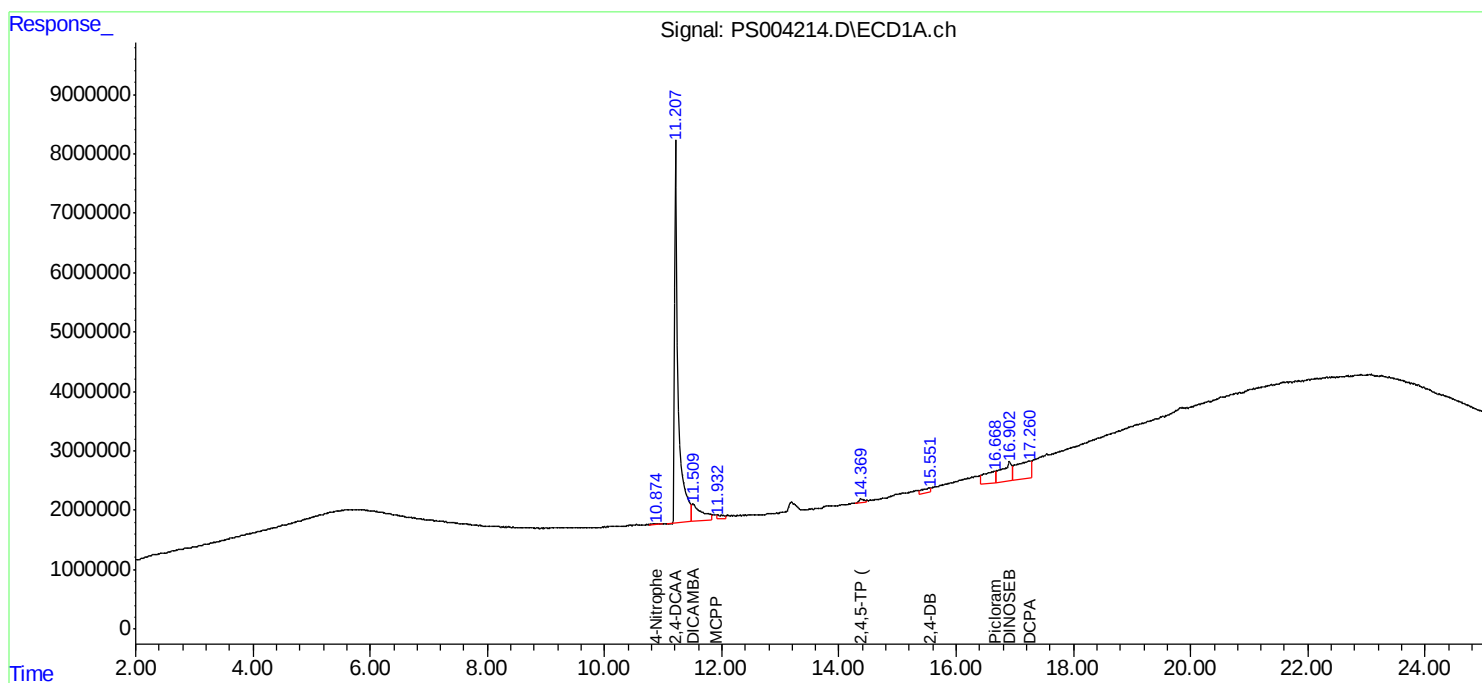


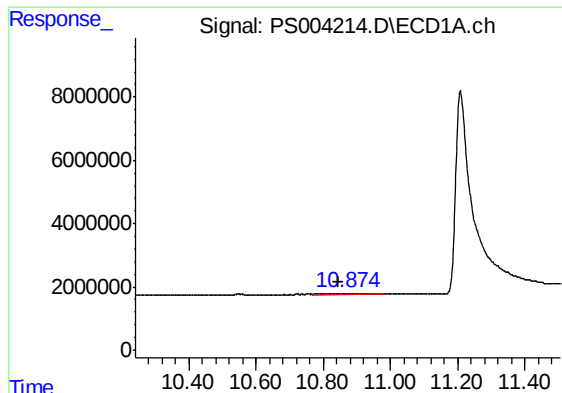

#3 4-Nitrophenol


R.T.: 10.874 min
Delta R.T.: 0.031 min
Response: 1157412
Conc: 4.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

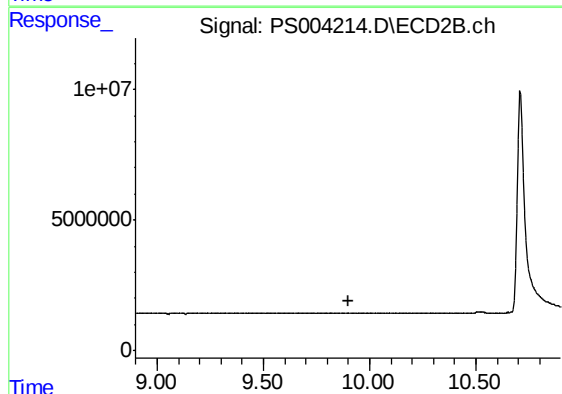


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 9.898 min
Response: 0
Conc: N.D.

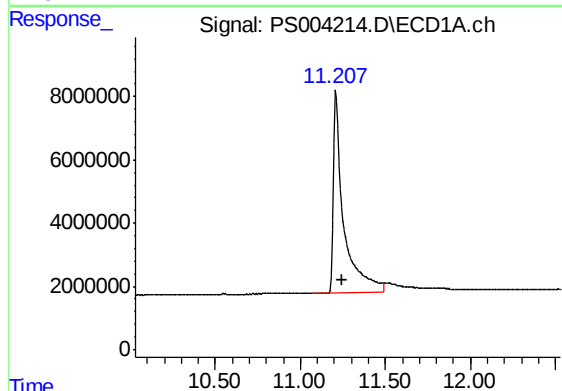


#4 2,4-DCAA

R.T.: 11.208 min
Delta R.T.: -0.035 min
Response: 268321981
Conc: 553.00 ng/ml

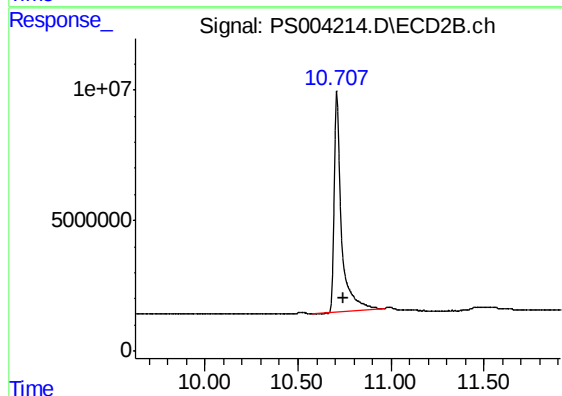

#4 2,4-DCAA


R.T.: 10.708 min
Delta R.T.: -0.037 min
Response: 228171621
Conc: 496.84 ng/ml

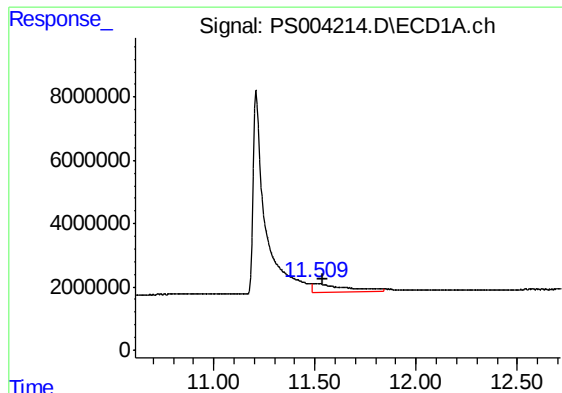

#5 DICAMBA


R.T.: 11.509 min
Delta R.T.: -0.033 min
Response: 33493340
Conc: 17.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

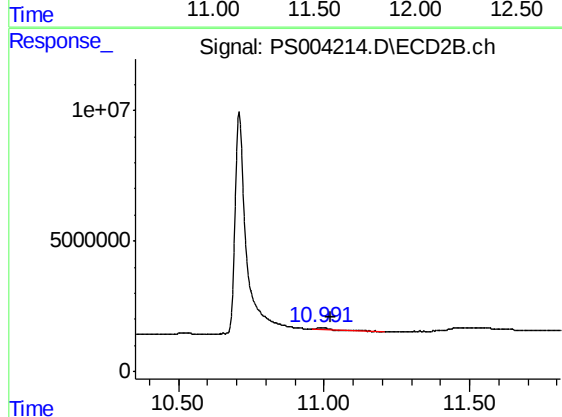


#5 DICAMBA

R.T.: 10.991 min
Delta R.T.: -0.032 min
Response: 687639
Conc: N.D.

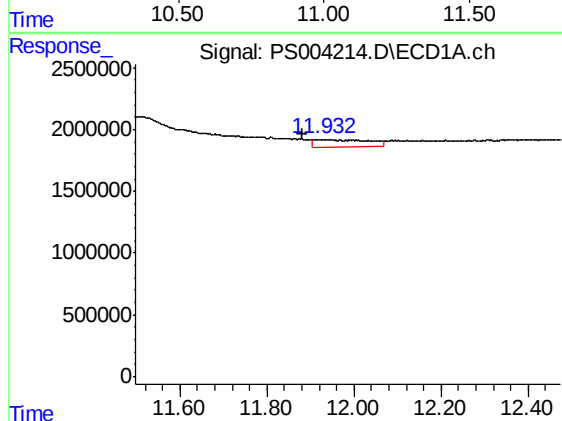


#6 MCPP

R.T.: 11.910 min
Delta R.T.: 0.027 min
Response: 5371024
Conc: 4.11 ug/ml

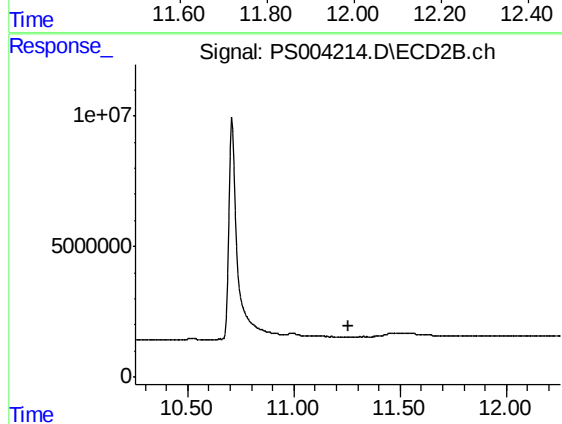

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 11.255 min
Response: 0
Conc: N.D.

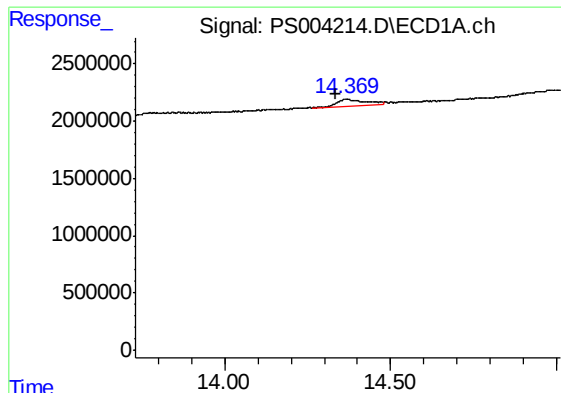

#11 2,4,5-TP (SILVEX)


R.T.: 14.369 min
Delta R.T.: 0.036 min
Response: 3470939
Conc: 1.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

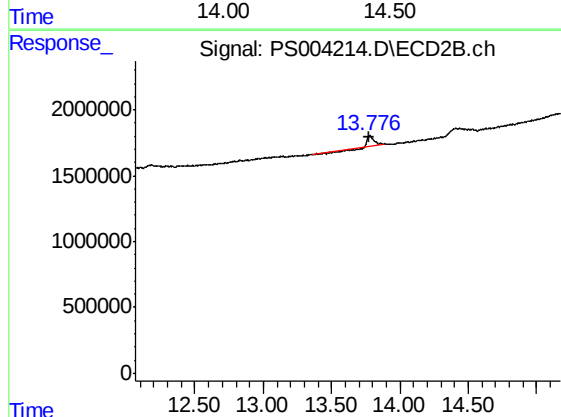


#11 2,4,5-TP (SILVEX)

R.T.: 13.777 min
Delta R.T.: 0.000 min
Response: 1616725
Conc: N.D.

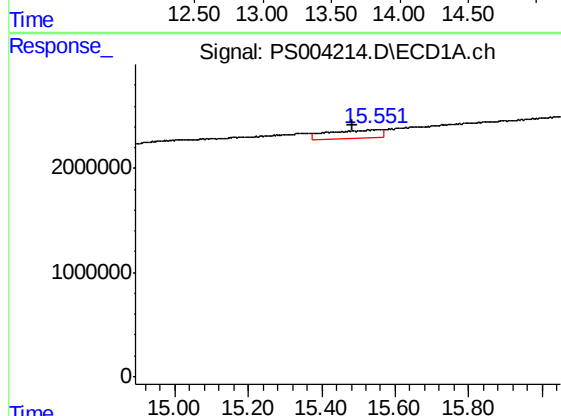


#13 2,4-DB

R.T.: 15.552 min
Delta R.T.: 0.069 min
Response: 7402959
Conc: 23.77 ng/ml

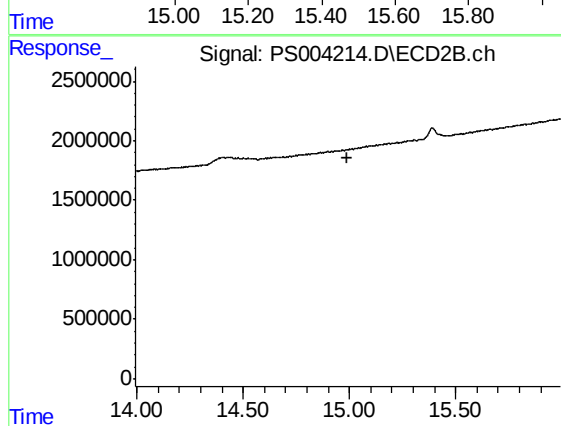

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 14.993 min
Response: 0
Conc: N.D.

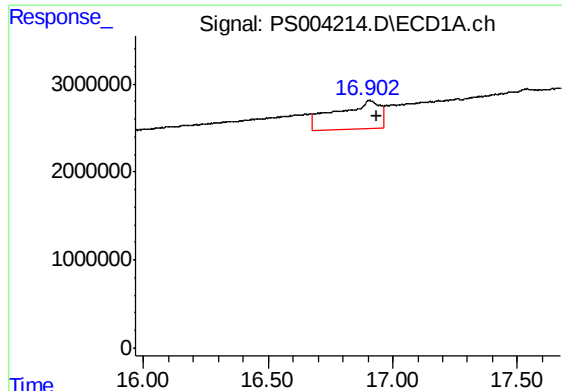

#14 DINOSEB


R.T.: 16.905 min
Delta R.T.: -0.031 min
Response: 39121393
Conc: 15.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

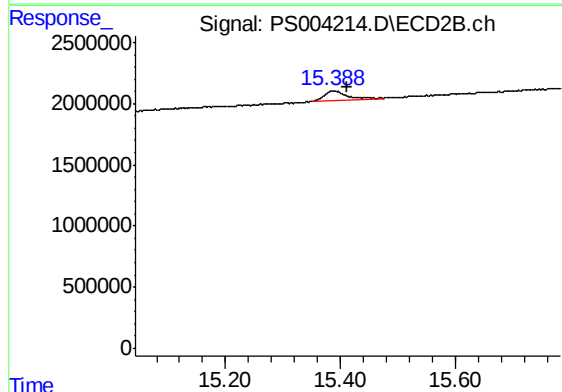


#14 DINOSEB

R.T.: 15.388 min
Delta R.T.: -0.023 min
Response: 2089833
Conc: 1.12 ng/ml

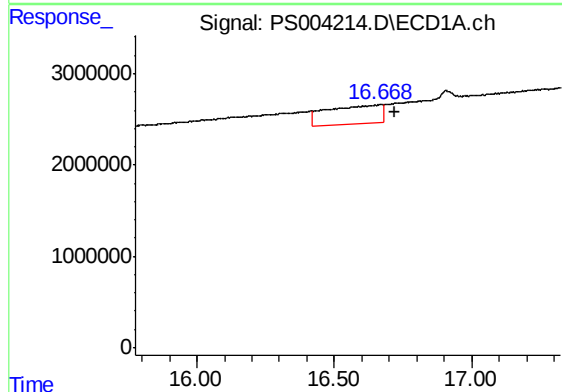


#15 Picloram

R.T.: 16.669 min
Delta R.T.: -0.052 min
Response: 27741766
Conc: 7.74 ng/ml

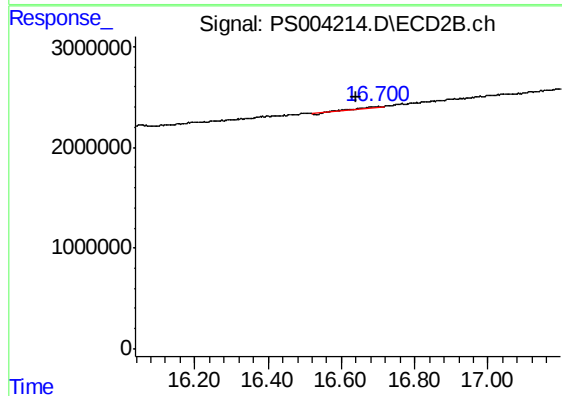

#15 Picloram


R.T.: 16.702 min
Delta R.T.: 0.060 min
Response: 534742
Conc: N.D.

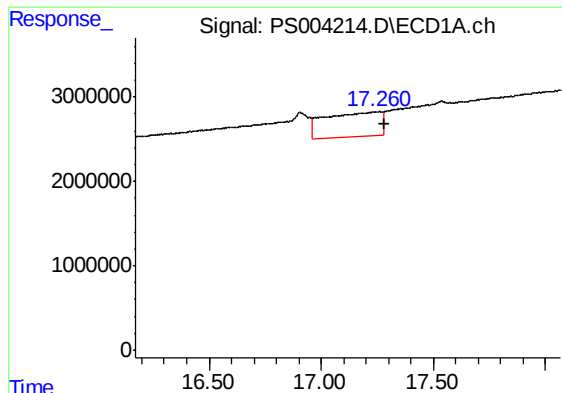

#16 DCPA

R.T.: 17.260 min
Delta R.T.: -0.023 min
Response: 49489567
Conc: 13.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

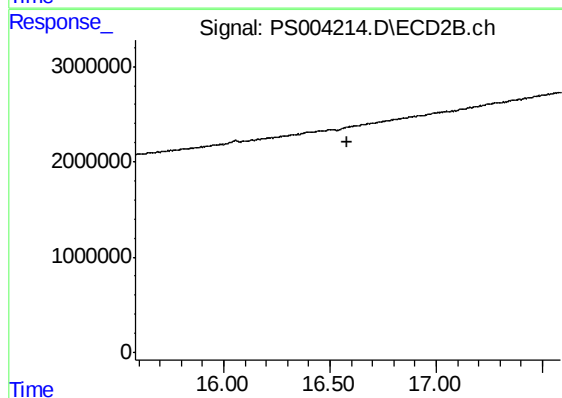

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 16.584 min
Response: 0
Conc: N.D.