

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042219\
 Data File : PS004183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2019 13:19
 Operator : EI\SJ
 Sample : MDL-BL-WATER-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 MDL-BL-WATER-04

Manual Integrations
 APPROVED

mohammad
 4/25/2019 4:56:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 01:11:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	11.213	10.713	193.3E6	183.5E6	398.343m	399.487m
------	----------	--------	--------	---------	---------	----------	----------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042219\
Data File : PS004183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2019 13:19
Operator : EI\SJ
Sample : MDL-BL-WATER-04
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-04


Manual Integrations
APPROVED

mohammad
4/25/2019 4:56:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 01:11:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

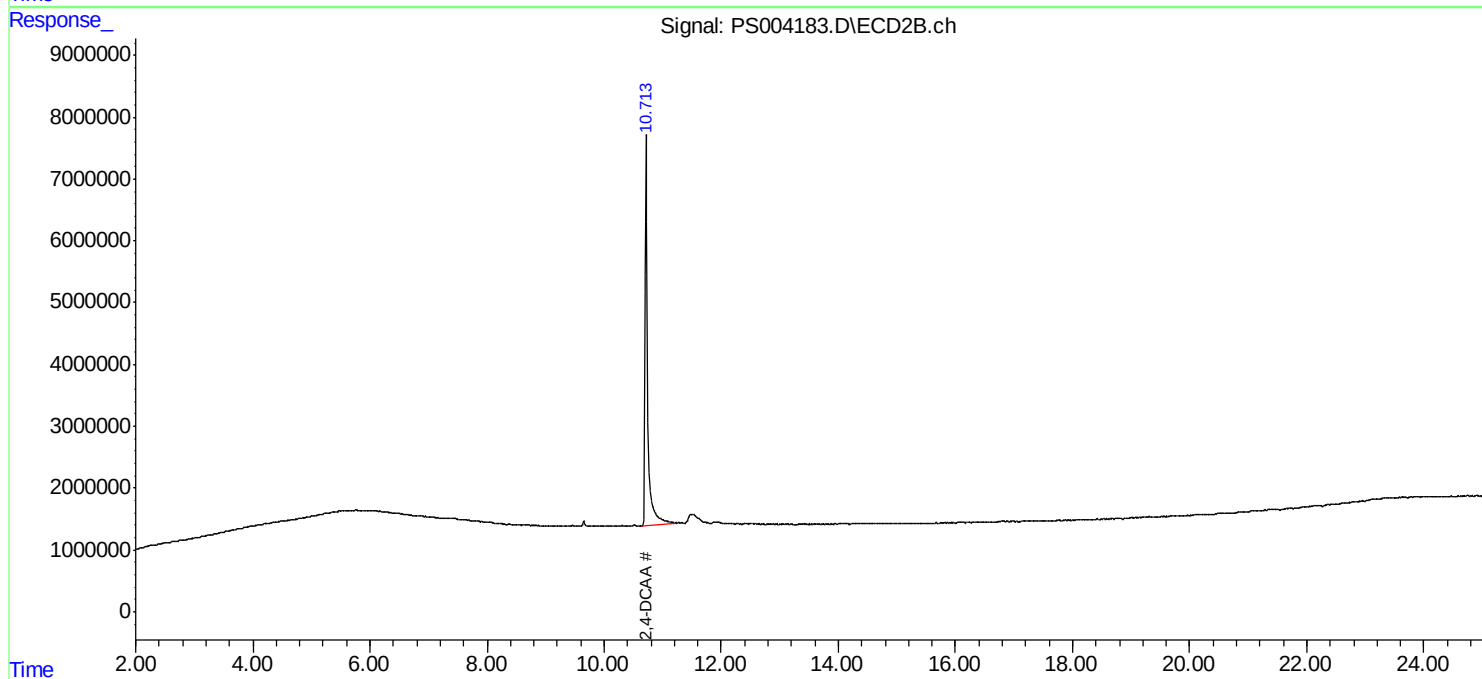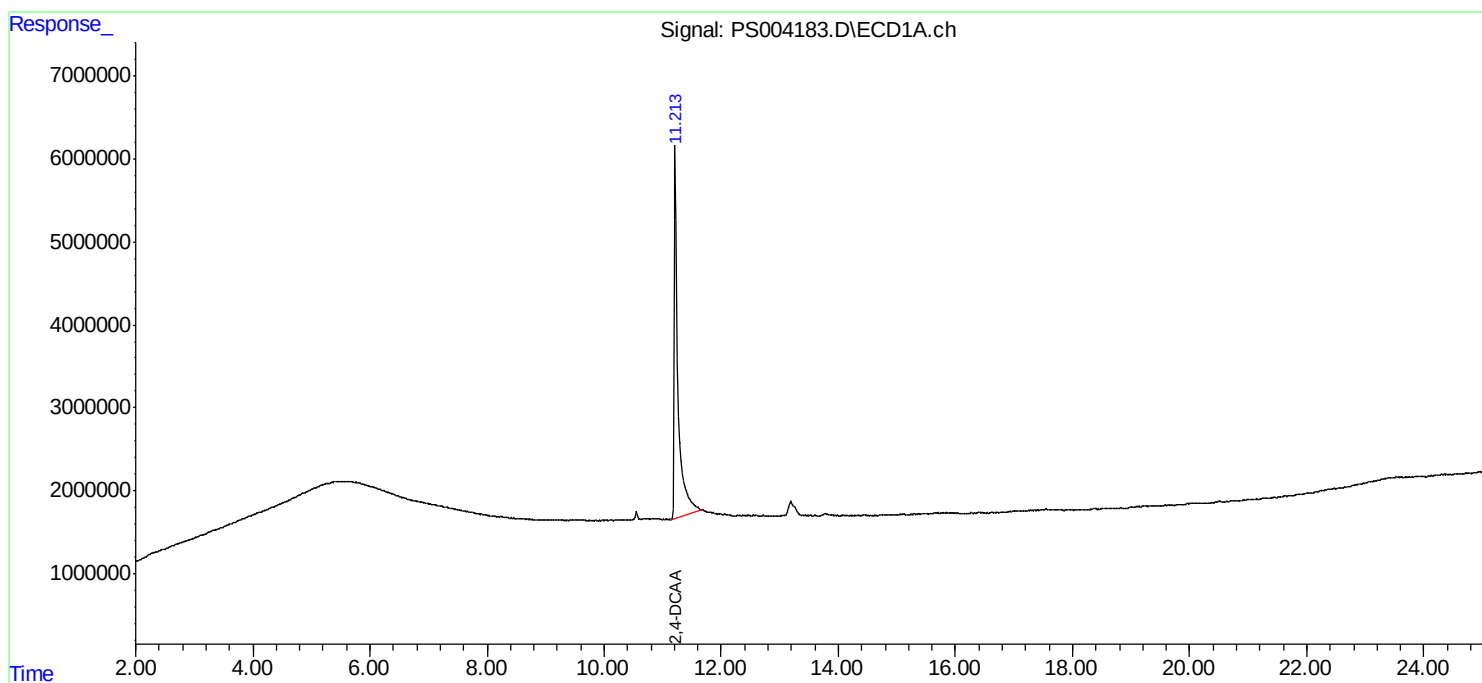

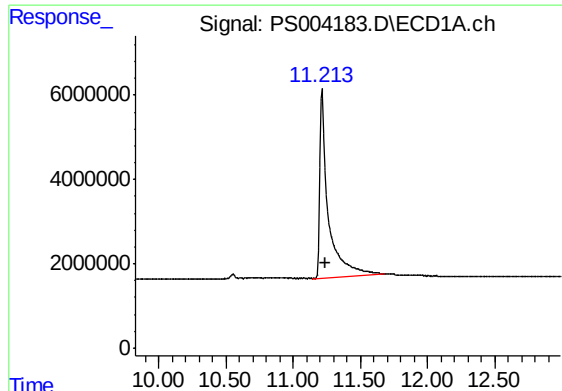


#4 2,4-DCAA

R.T.: 11.213 min
Delta R.T.: -0.030 min
Response: 193282086
Conc: 398.34 ng/ml m

Instrument :
ECD_S
ClientSampleId :
MDL-BL-WATER-04

Manual Integrations
APPROVED

mohammad
4/25/2019 4:56:58 PM

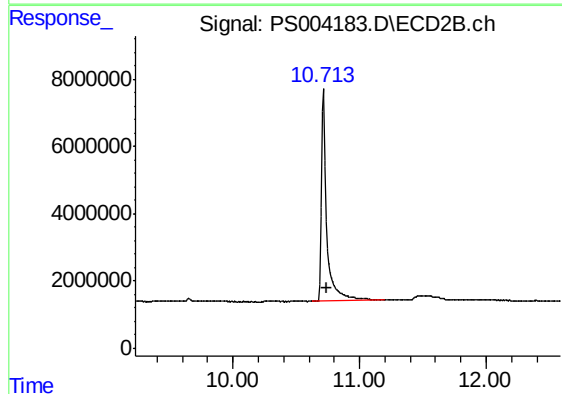

#4 2,4-DCAA

R.T.: 10.713 min
Delta R.T.: -0.033 min
Response: 183461257
Conc: 399.49 ng/ml m