

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042220\
 Data File : PS009963.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2020 14:39
 Operator : DD\AJ
 Sample : PB128359TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB128359TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 15:32:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.236	6.922	277.3E6	272.6E6	459.278	550.408
Target Compounds							
5) T	DICAMBA	0.000	7.091	0	1969299	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.717	0	952770	N.D.	1.893
9) T	2,4-D	0.000	8.016	0	626117	N.D.	1.045
11) T	2,4,5-TP ...	0.000	8.804	0	1817845	N.D.	<MDL
12) T	2,4,5-T	0.000	9.186	0	2766719	N.D.	1.060
14) T	DINOSEB	0.000	10.025	0	1057363	N.D.	<MDL
15) T	Picloram	11.034	11.008	8502744	11513844	2.745	3.385
16) T	DCPA	0.000	10.954	0	2752168	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042220\
Data File : PS009963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2020 14:39
Operator : DD\AJ
Sample : PB128359TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB128359TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 15:32:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

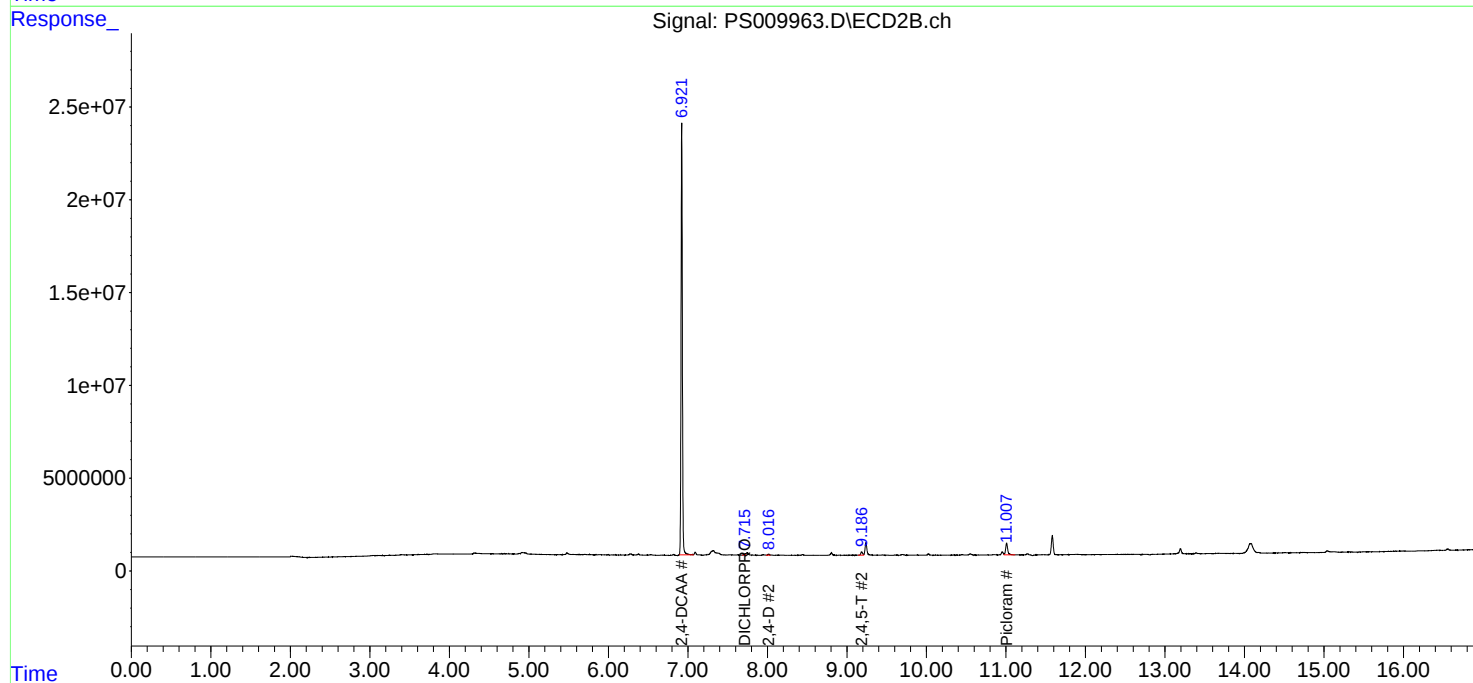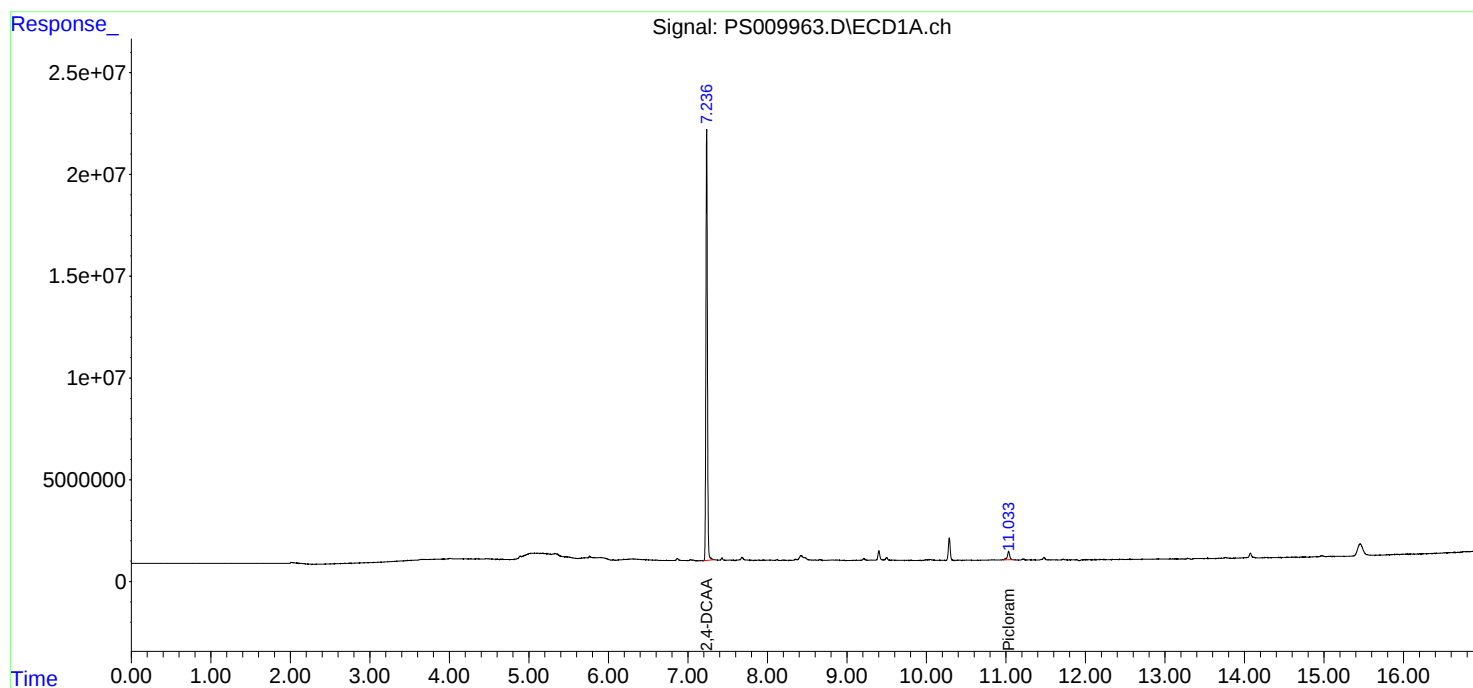


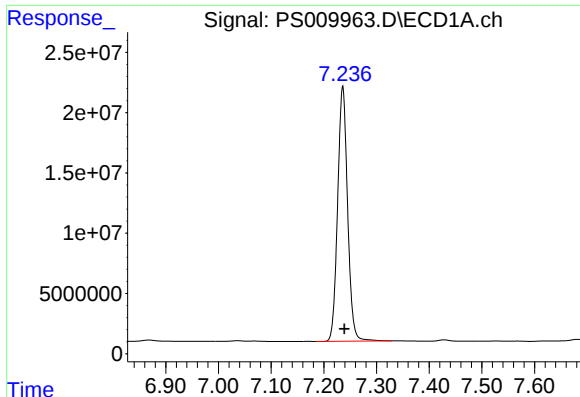

#4 2,4-DCAA


R.T.: 7.236 min
Delta R.T.: -0.003 min
Response: 277318813
Conc: 459.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB128359TB

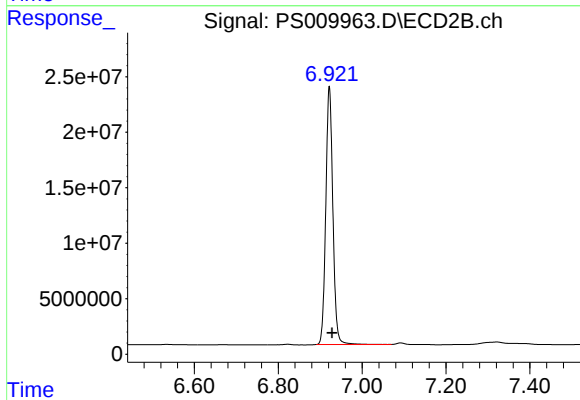


#4 2,4-DCAA

R.T.: 6.922 min
Delta R.T.: -0.006 min
Response: 272589414
Conc: 550.41 ng/ml

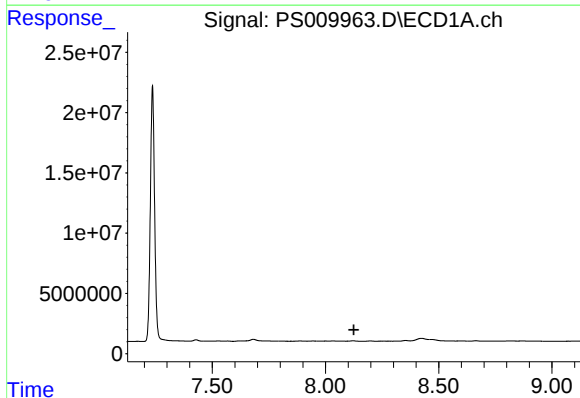


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.125 min
Response: 0
Conc: N.D.

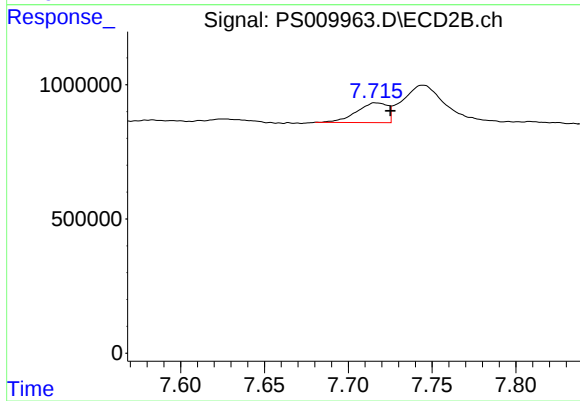

#8 DICHLORPROP


R.T.: 7.717 min
Delta R.T.: -0.009 min
Response: 952770
Conc: 1.89 ng/ml

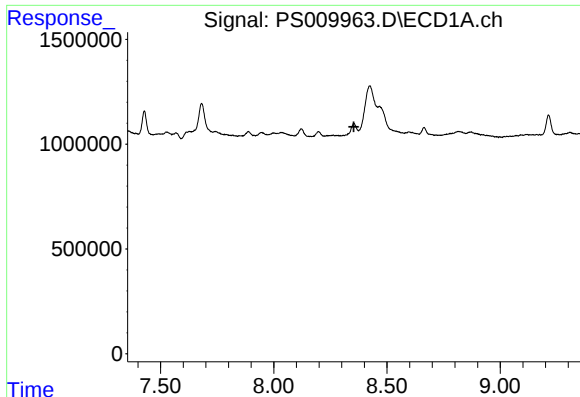

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.354 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB128359TB

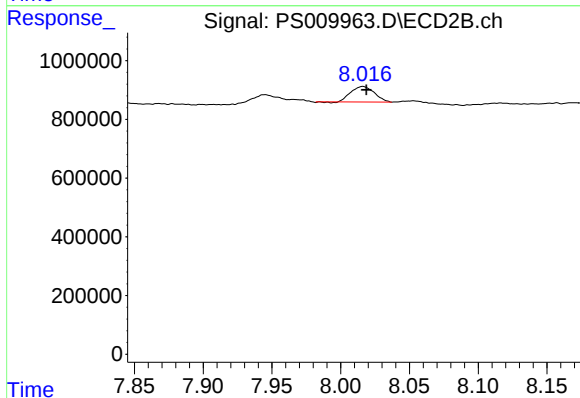


#9 2,4-D

R.T.: 8.016 min
Delta R.T.: -0.003 min
Response: 626117
Conc: 1.04 ng/ml

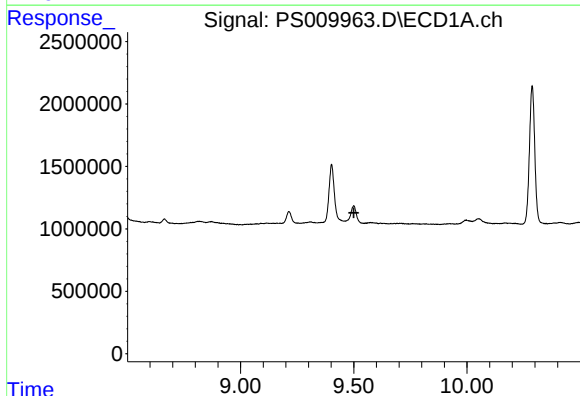


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.501 min
Response: 0
Conc: N.D.

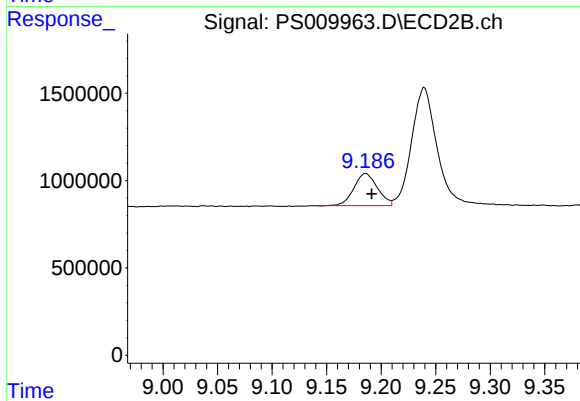

#12 2,4,5-T


R.T.: 9.186 min
Delta R.T.: -0.006 min
Response: 2766719
Conc: 1.06 ng/ml

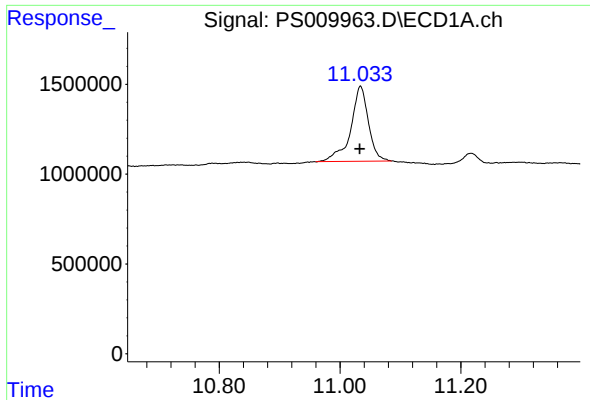

#15 Picloram

R.T.: 11.034 min
Delta R.T.: 0.001 min
Response: 8502744
Conc: 2.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB128359TB

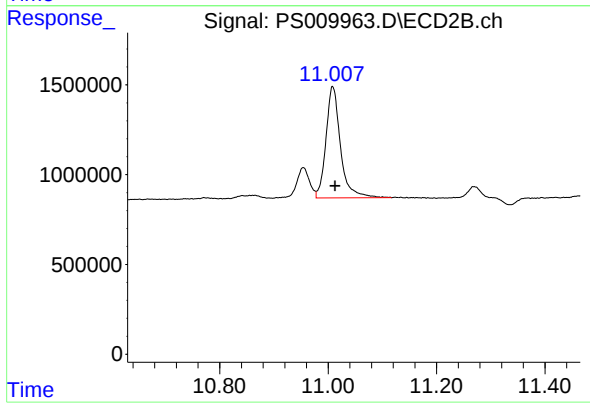

#15 Picloram

R.T.: 11.008 min
Delta R.T.: -0.005 min
Response: 11513844
Conc: 3.39 ng/ml