

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042419\
 Data File : PS004252.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 12:31
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 00:51:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.223	10.712	178.3E6	162.8E6	367.539	354.496
Target Compounds							
5) T	DICAMBA	11.528	10.991	14866103	3275490	7.579	1.989 #
6) T	MCPD	0.000	11.312	0	1507527	N.D.	1.445
7) T	MCPA	0.000	11.614	0	5745923	N.D.	3.158
9) T	2,4-D	13.213	0.000	33570590	0	73.728	N.D. #
10) T	Pentachlo...	13.435	13.120	9237806	6637799	1.274	1.069
11) T	2,4,5-TP ...	14.370	13.779	699546	3163634	<MDL	1.314 #
14) T	DINOSEB	16.910	15.389	36136134	2332309	14.423	1.248 #
15) T	Picloram	16.675	16.701	750460	31089906	<MDL	9.081 #
16) T	DCPA	17.251	16.555	9897188	4070430	2.749	1.281 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042419\
Data File : PS004252.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 12:31
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 00:51:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

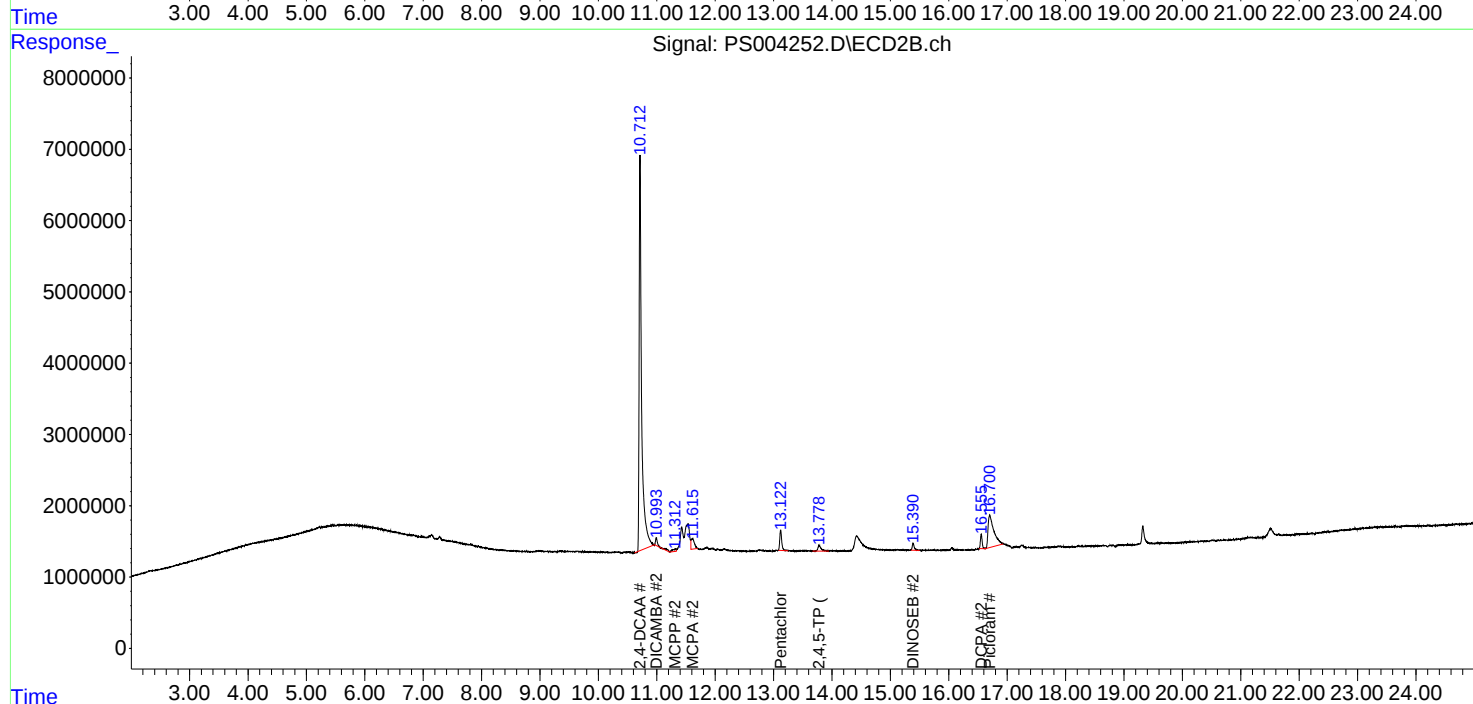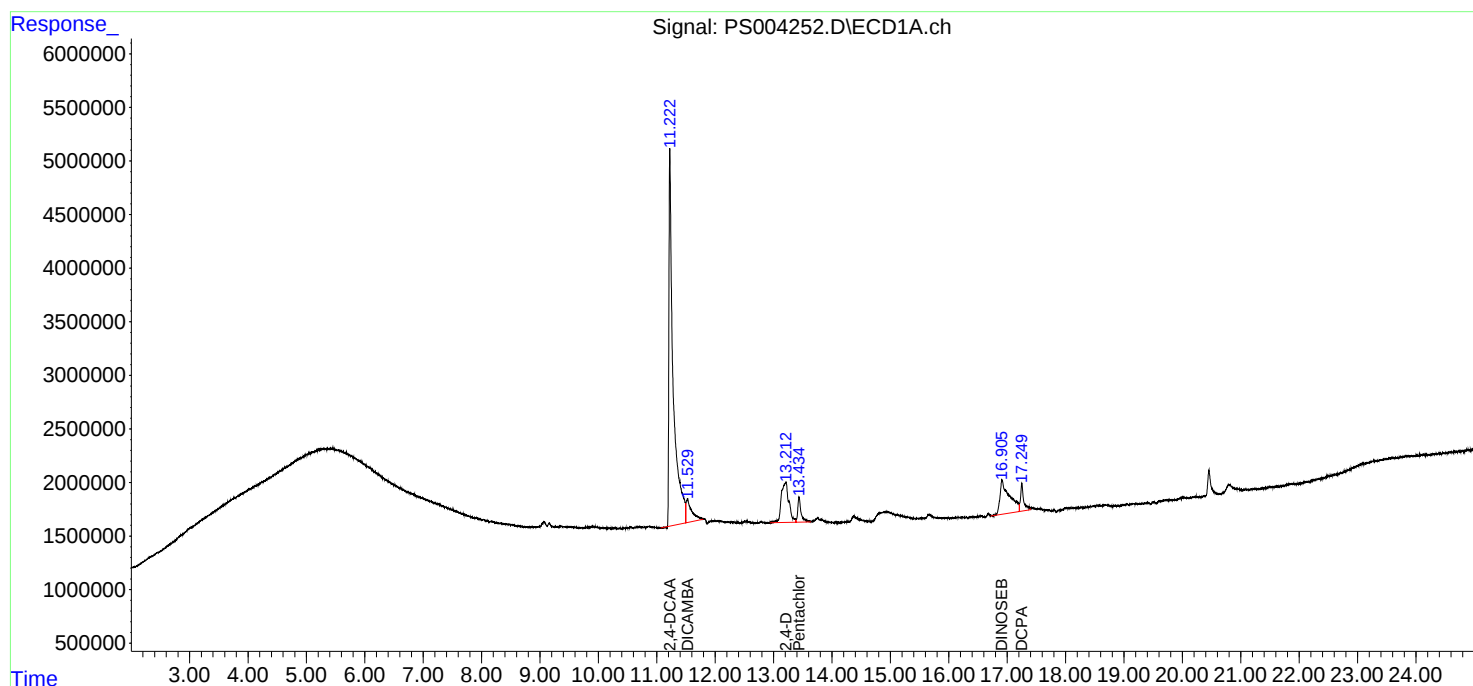


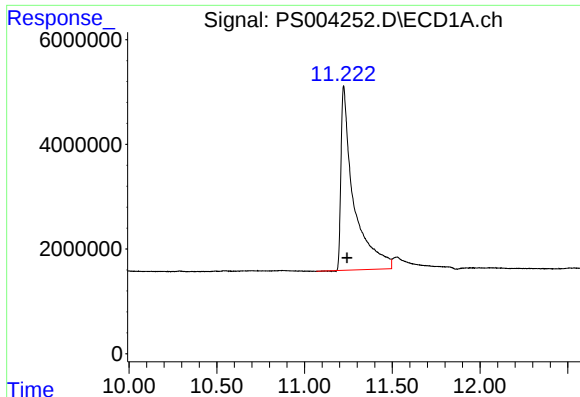

#4 2,4-DCAA


R.T.: 11.223 min
Delta R.T.: -0.020 min
Response: 178335292
Conc: 367.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

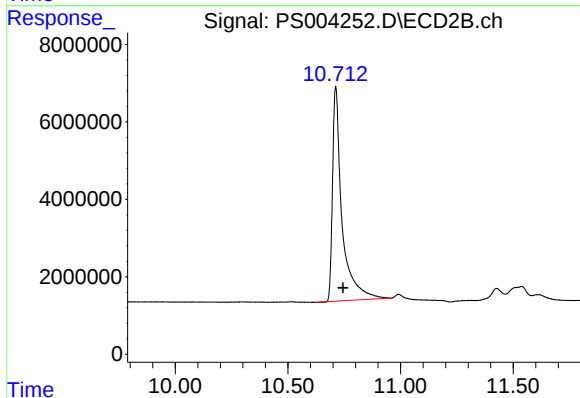


#4 2,4-DCAA

R.T.: 10.712 min
Delta R.T.: -0.033 min
Response: 162799338
Conc: 354.50 ng/ml

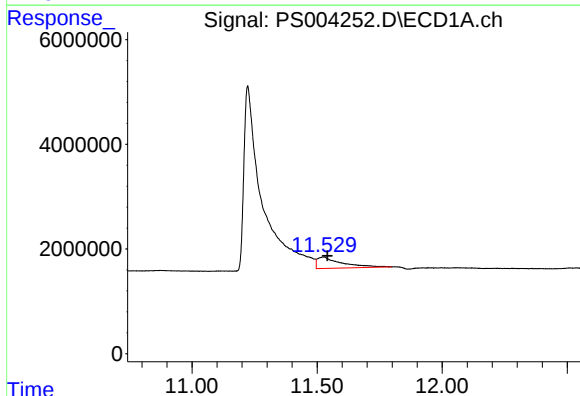


#5 DICAMBA

R.T.: 11.528 min
Delta R.T.: -0.014 min
Response: 14866103
Conc: 7.58 ng/ml

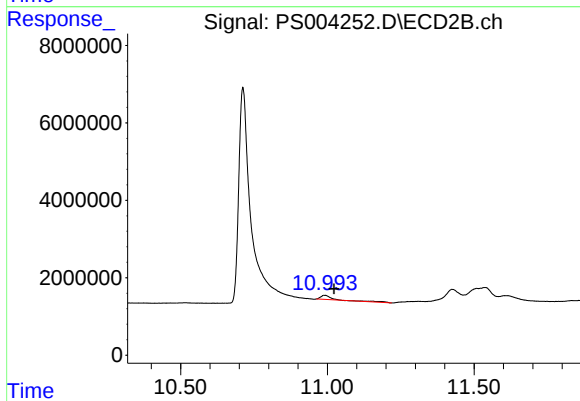

#5 DICAMBA


R.T.: 10.991 min
Delta R.T.: -0.032 min
Response: 3275490
Conc: 1.99 ng/ml

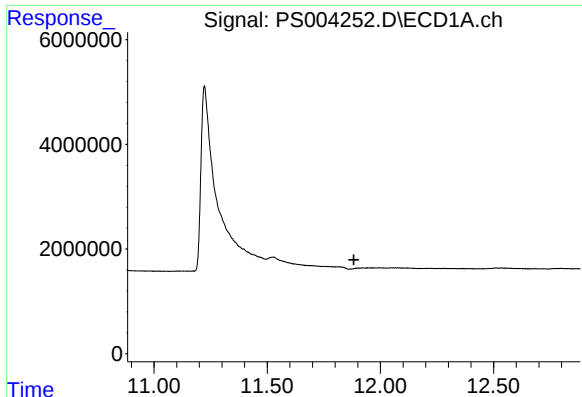

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

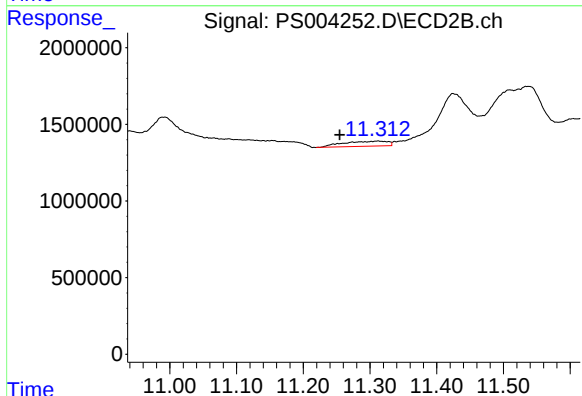


#6 MCPP

R.T.: 11.312 min
Delta R.T.: 0.057 min
Response: 1507527
Conc: 1.45 ug/ml

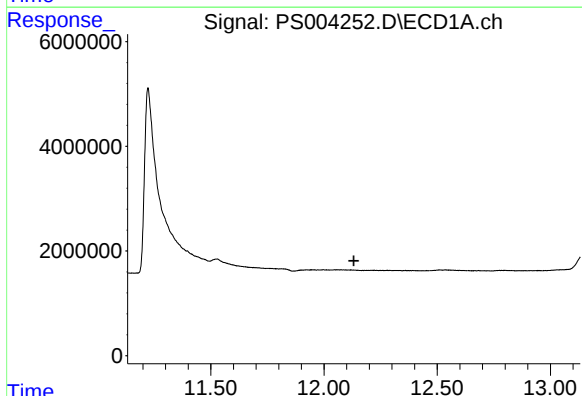


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 12.132 min
Response: 0
Conc: N.D.

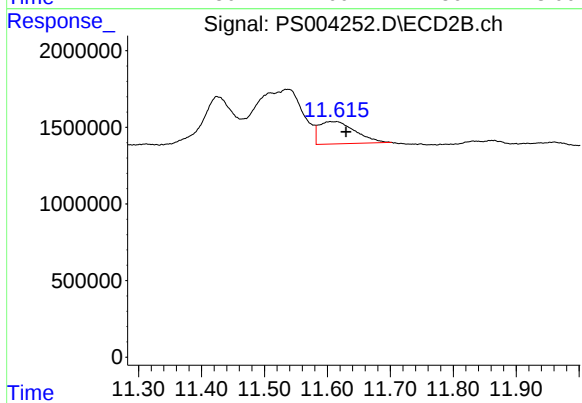

#7 MCPA


R.T.: 11.614 min
Delta R.T.: -0.016 min
Response: 5745923
Conc: 3.16 ug/ml

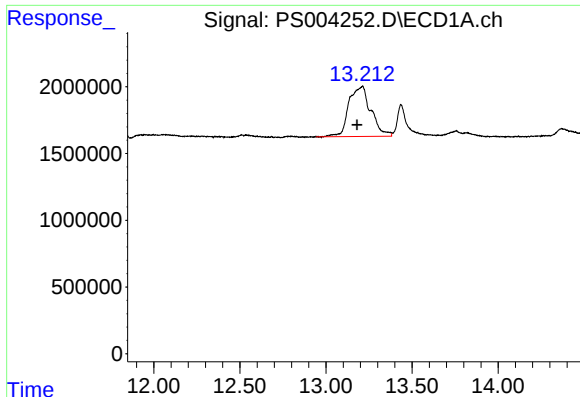

#9 2,4-D


R.T.: 13.213 min
Delta R.T.: 0.033 min
Response: 33570590
Conc: 73.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

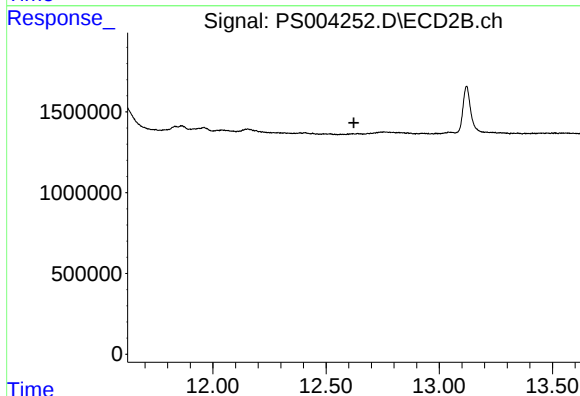


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 12.623 min
Response: 0
Conc: N.D.

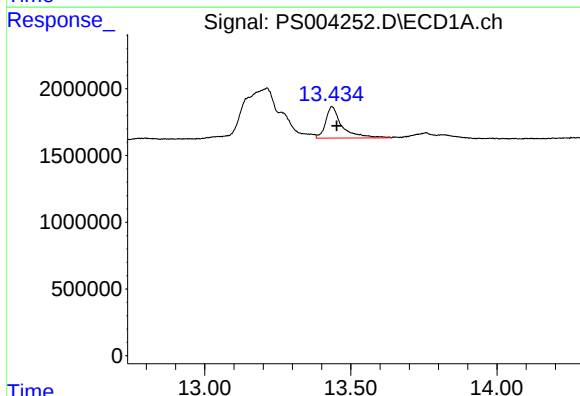


#10 Pentachlorophenol

R.T.: 13.435 min
Delta R.T.: -0.017 min
Response: 9237806
Conc: 1.27 ng/ml

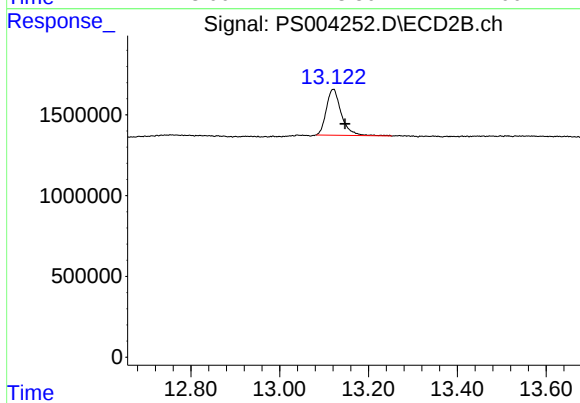

#10 Pentachlorophenol


R.T.: 13.120 min
Delta R.T.: -0.026 min
Response: 6637799
Conc: 1.07 ng/ml

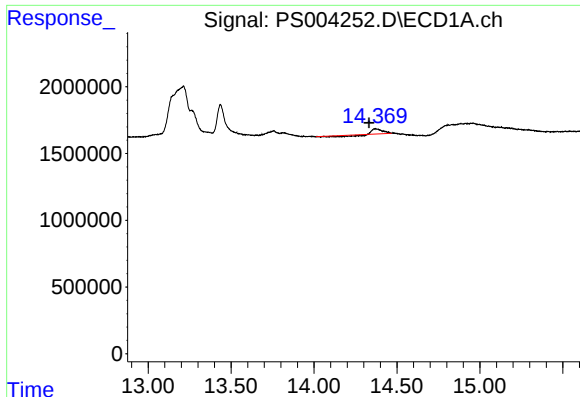

#11 2,4,5-TP (SILVEX)


R.T.: 14.370 min
Delta R.T.: 0.037 min
Response: 699546
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

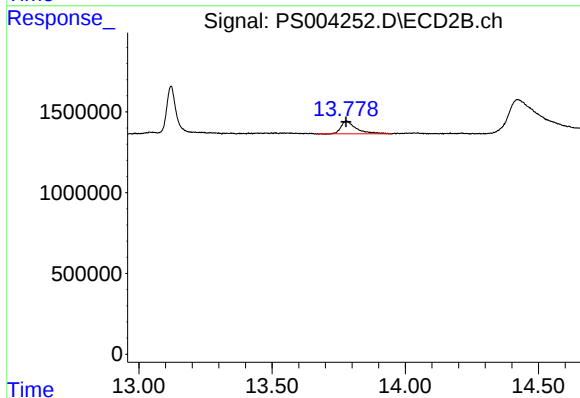


#11 2,4,5-TP (SILVEX)

R.T.: 13.779 min
Delta R.T.: 0.001 min
Response: 3163634
Conc: 1.31 ng/ml

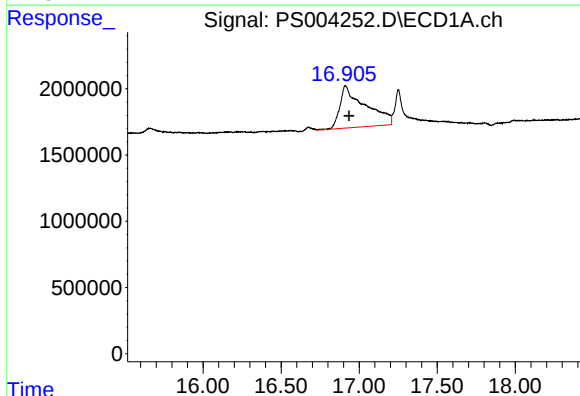


#14 DINOSEB

R.T.: 16.910 min
Delta R.T.: -0.027 min
Response: 36136134
Conc: 14.42 ng/ml

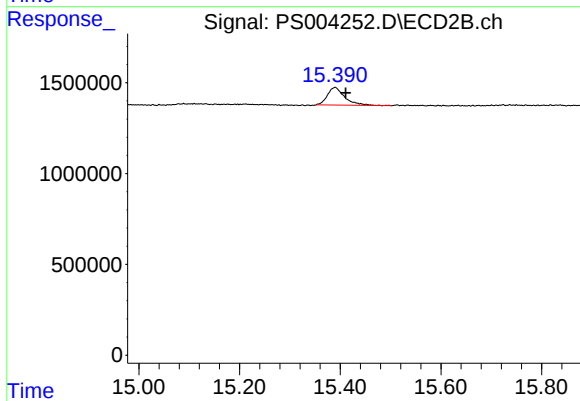

#14 DINOSEB


R.T.: 15.389 min
Delta R.T.: -0.022 min
Response: 2332309
Conc: 1.25 ng/ml

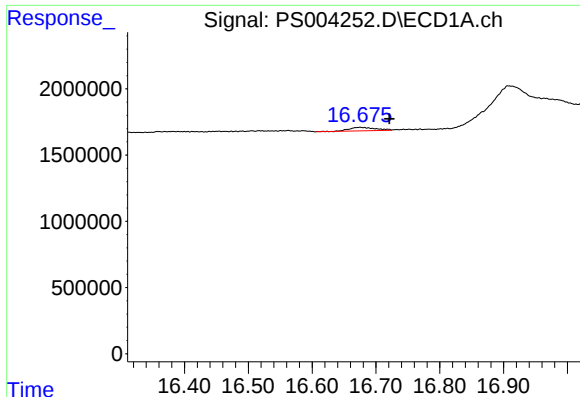

#15 Picloram


R.T.: 16.675 min
Delta R.T.: -0.046 min
Response: 750460
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

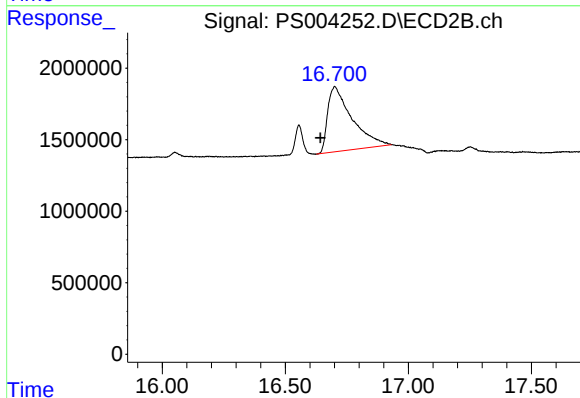


#15 Picloram

R.T.: 16.701 min
Delta R.T.: 0.059 min
Response: 31089906
Conc: 9.08 ng/ml

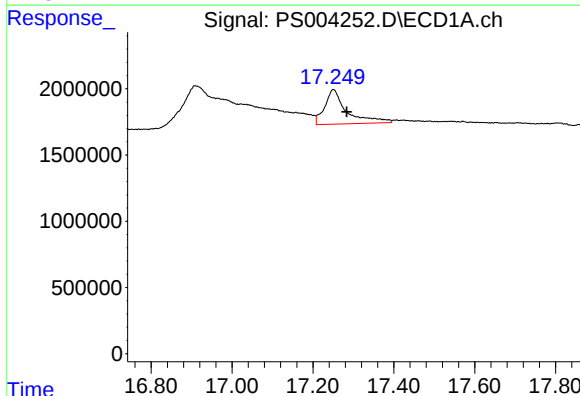

#16 DCPA

R.T.: 17.251 min
Delta R.T.: -0.033 min
Response: 9897188
Conc: 2.75 ng/ml

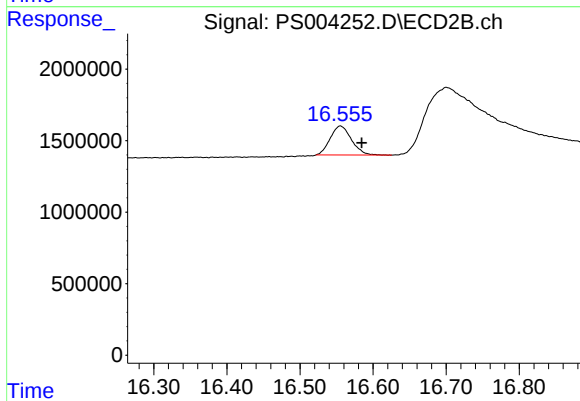

#16 DCPA

R.T.: 16.555 min
Delta R.T.: -0.029 min
Response: 4070430
Conc: 1.28 ng/ml