

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042419\
 Data File : PS004257.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 15:13
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 00:53:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.201	10.704	201.0E6	160.3E6	414.168	349.122
Target Compounds							
9) T	2,4-D	13.174	0.000	18805771	0	41.301	N.D. #
10) T	Pentachlo...	13.402	0.000	738860	0	<MDL	N.D. #
16) T	DCPA	17.233	0.000	6322849	0	1.756	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042419\
Data File : PS004257.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 15:13
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 00:53:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

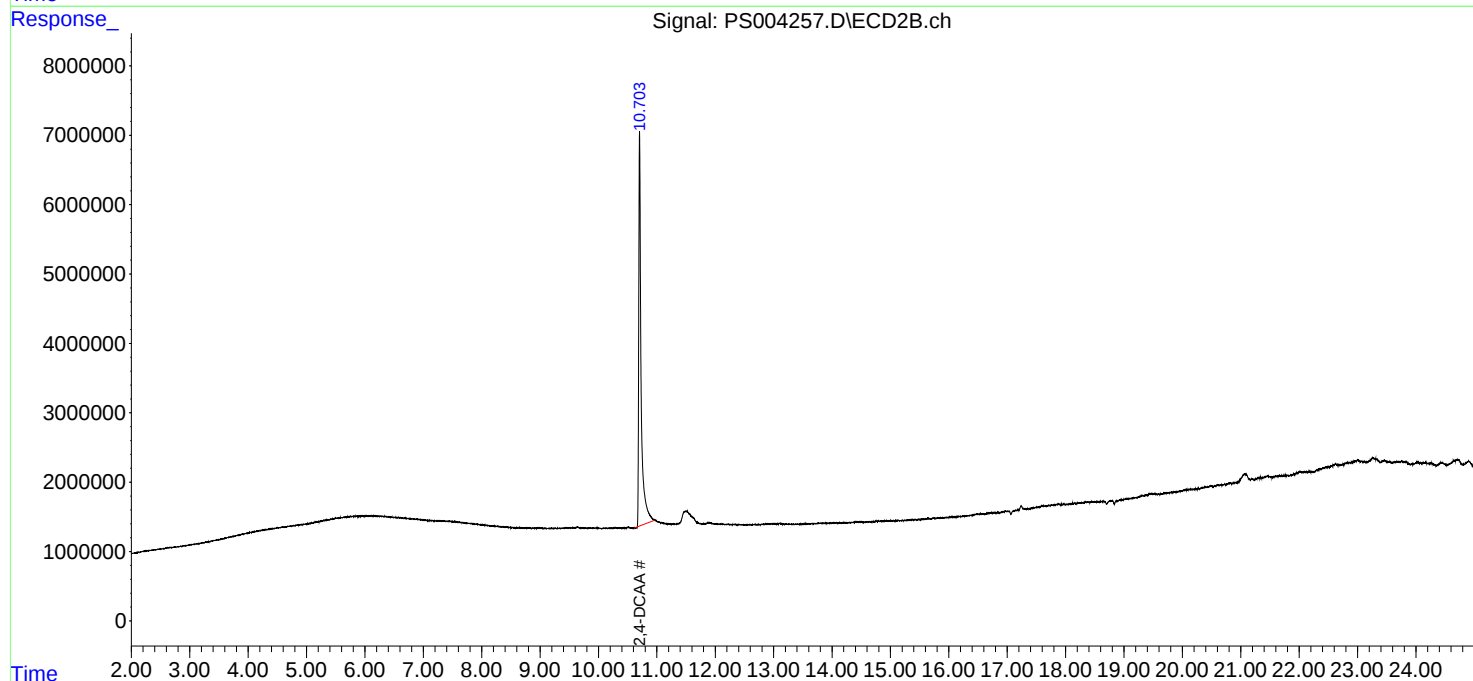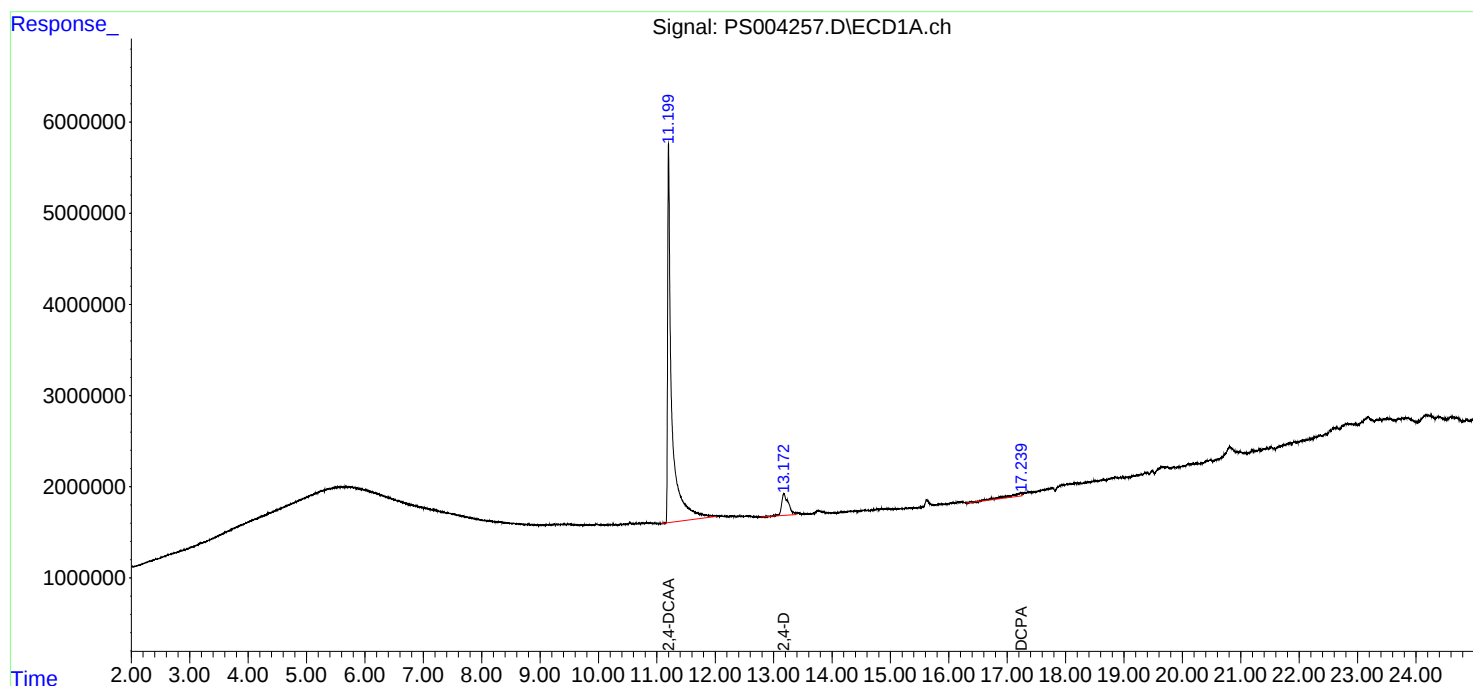


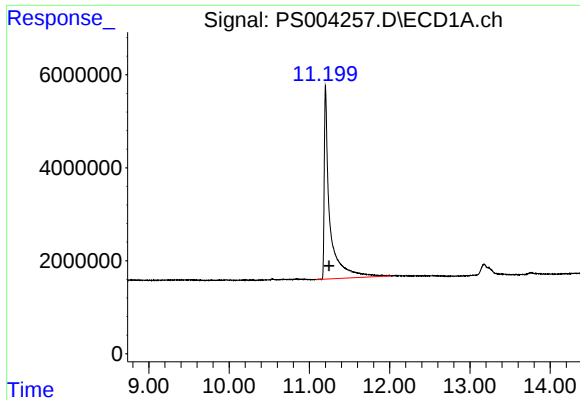

#4 2,4-DCAA


R.T.: 11.201 min
Delta R.T.: -0.042 min
Response: 200960262
Conc: 414.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

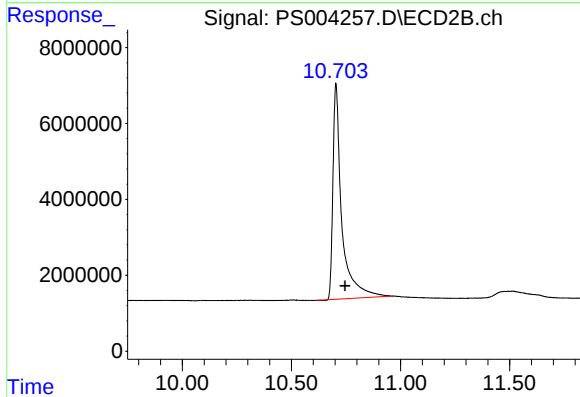


#4 2,4-DCAA

R.T.: 10.704 min
Delta R.T.: -0.042 min
Response: 160331276
Conc: 349.12 ng/ml

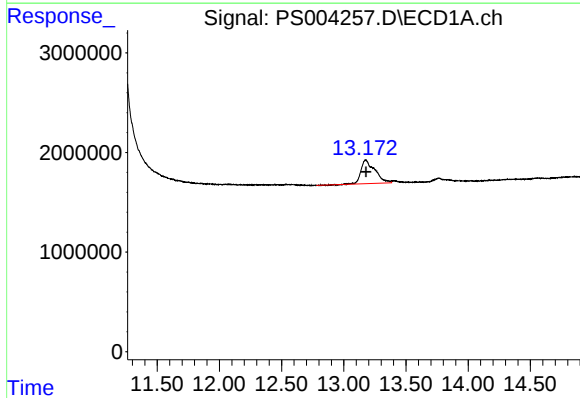


#9 2,4-D

R.T.: 13.174 min
Delta R.T.: -0.006 min
Response: 18805771
Conc: 41.30 ng/ml

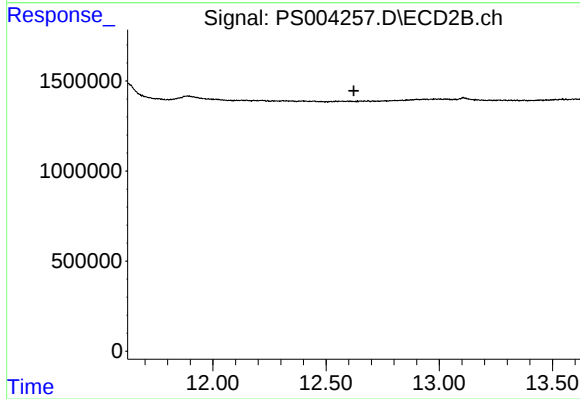

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 12.623 min
Response: 0
Conc: N.D.

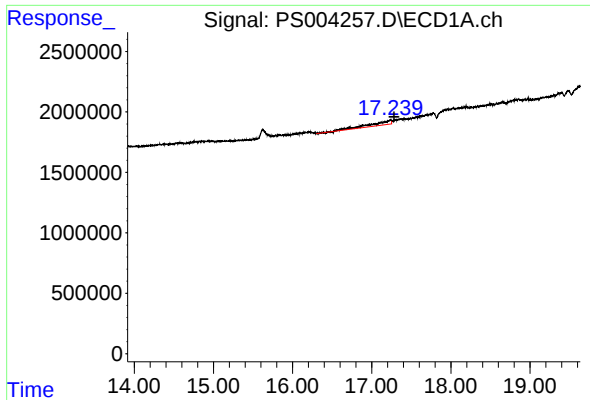

#16 DCPA

R.T.: 17.233 min
Delta R.T.: -0.050 min
Response: 6322849
Conc: 1.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

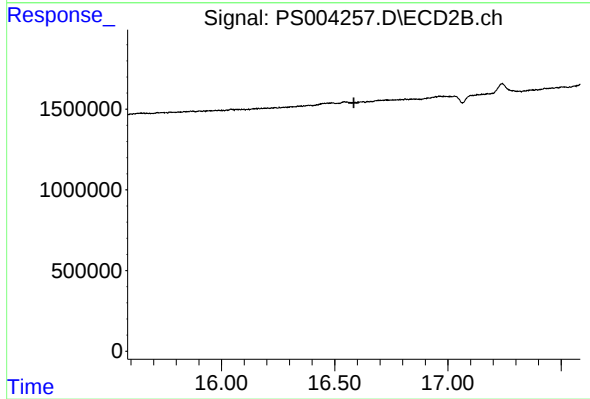

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 16.584 min
Response: 0
Conc: N.D.