

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042419\
 Data File : PS004260.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 16:54
 Operator : EI\SJ
 Sample : K2518-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 MUDDY-BAGS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 00:54:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.195	10.702	250.9E6	219.9E6	517.081	478.852
Target Compounds							
2) T	3,5-DICHL...	0.000	8.952	0	119.6E6	N.D.	209.298
3) T	4-Nitroph...	10.828	9.916	13662350	11434647	54.088	47.683
6) T	MCP	11.867	11.316	13330188	947446	10.211	<MDL #
9) T	2,4-D	13.179	12.558	15370272	691788	33.756	1.352 #
10) T	Pentachlo...	0.000	13.190	0	1533534	N.D.	<MDL
11) T	2,4,5-TP ...	14.298	0.000	2046894	0	<MDL	N.D. #
12) T	2,4,5-T	0.000	14.374	0	2927692	N.D.	1.269
14) T	DINOSEB	0.000	15.431	0	1178318	N.D.	<MDL
15) T	Picloram	16.674	16.665	1465726	16382838	<MDL	4.785 #
16) T	DCPA	17.325	0.000	10478527	0	2.911	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042419\
Data File : PS004260.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 16:54
Operator : EI\SJ
Sample : K2518-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
MUDDY-BAGS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 00:54:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

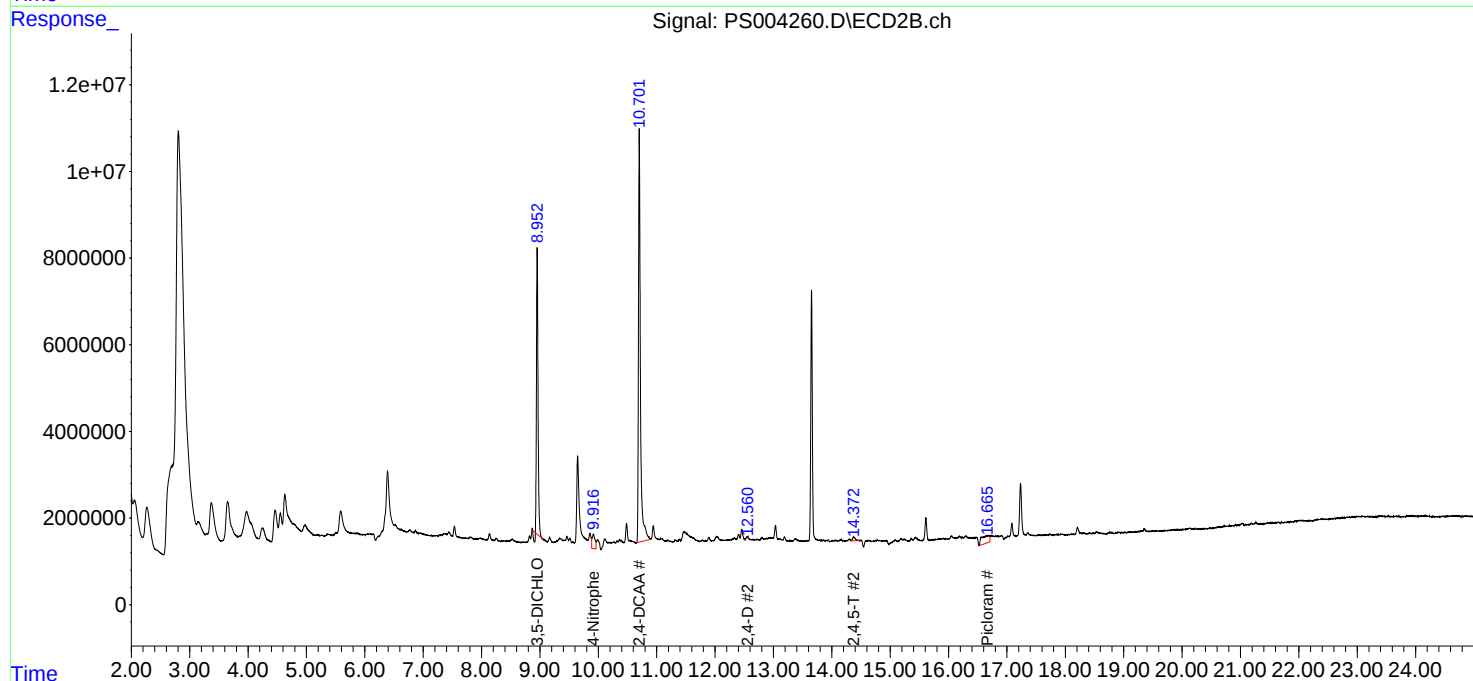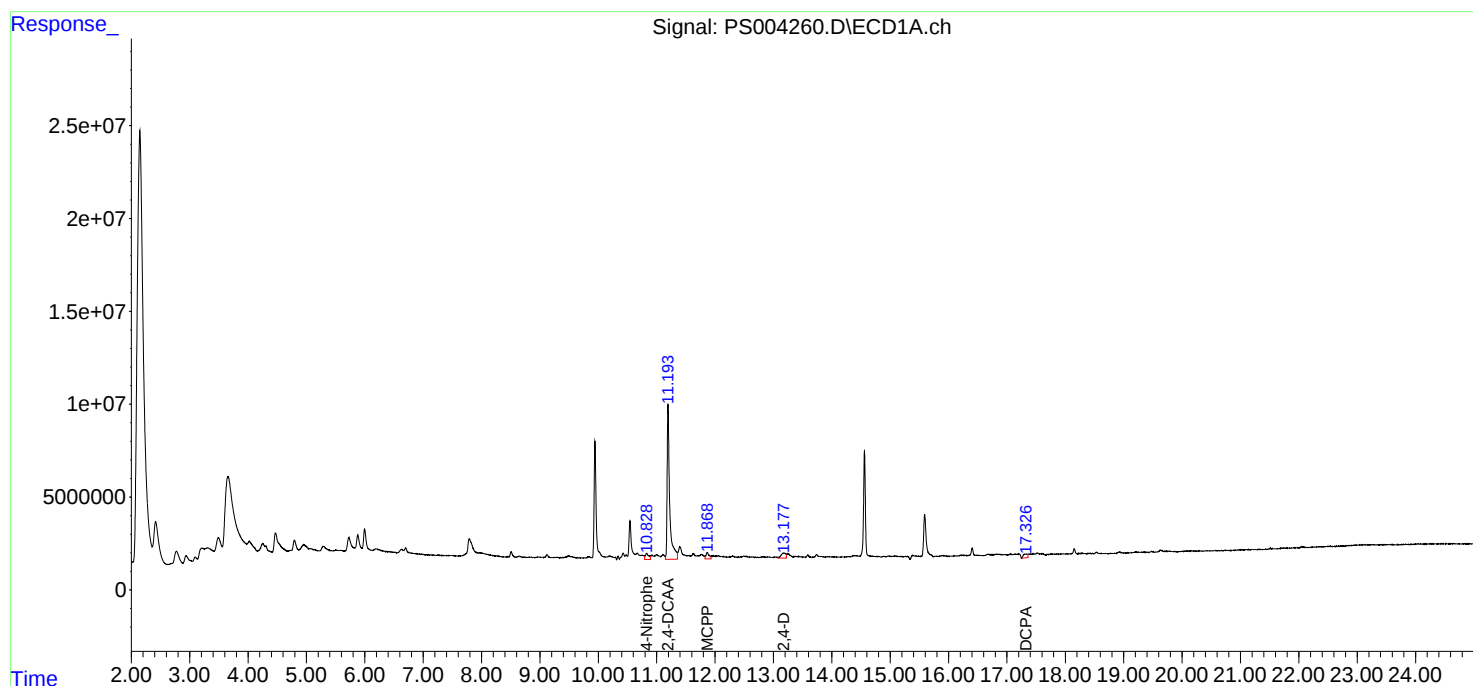


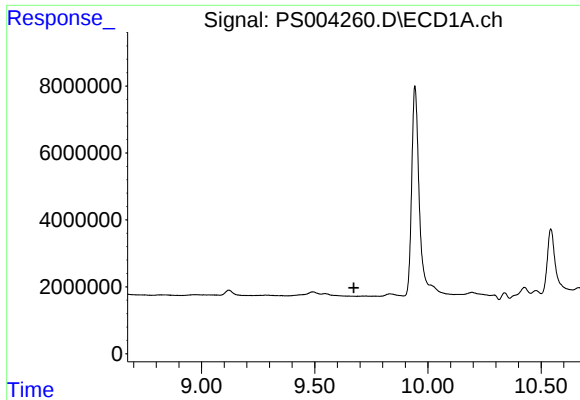

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.673 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
MUDDY-BAGS

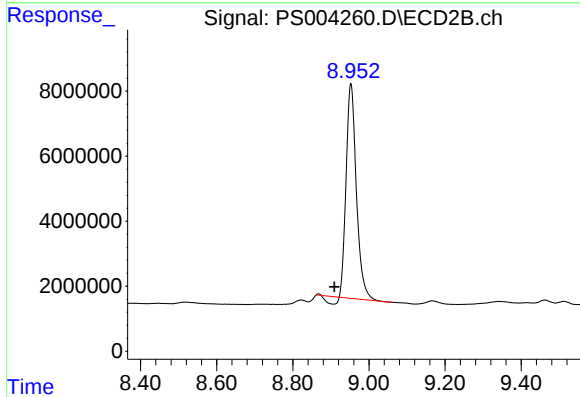


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.952 min
Delta R.T.: 0.043 min
Response: 119640160
Conc: 209.30 ng/ml

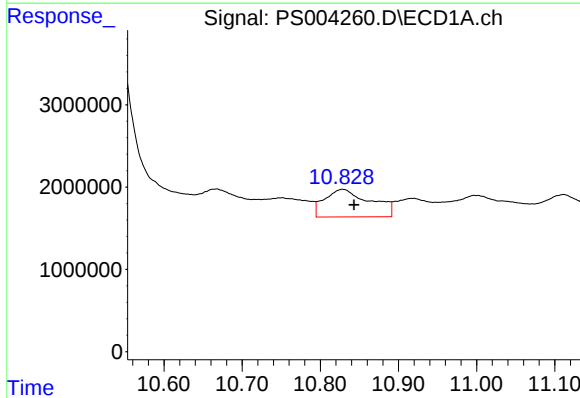


#3 4-Nitrophenol

R.T.: 10.828 min
Delta R.T.: -0.015 min
Response: 13662350
Conc: 54.09 ng/ml

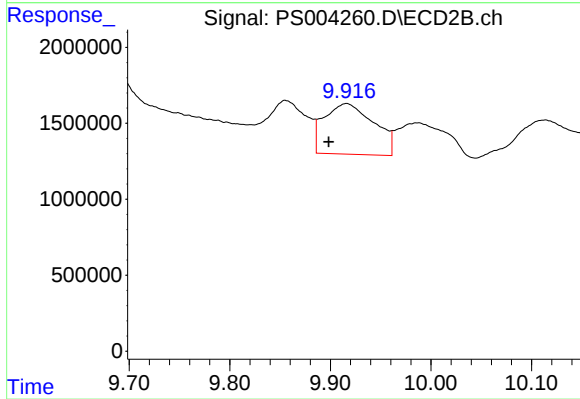

#3 4-Nitrophenol


R.T.: 9.916 min
Delta R.T.: 0.018 min
Response: 11434647
Conc: 47.68 ng/ml

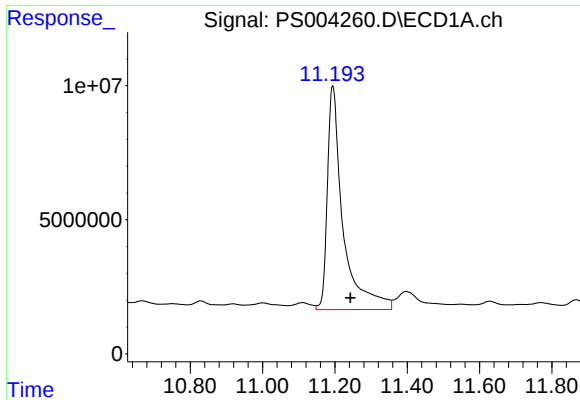

#4 2,4-DCAA


R.T.: 11.195 min
Delta R.T.: -0.049 min
Response: 250895265
Conc: 517.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
MUDDY-BAGS

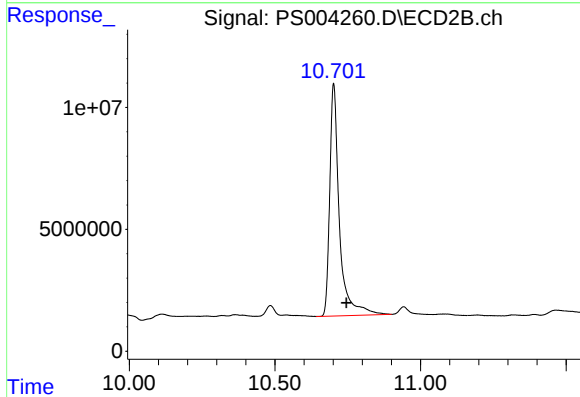


#4 2,4-DCAA

R.T.: 10.702 min
Delta R.T.: -0.044 min
Response: 219908949
Conc: 478.85 ng/ml

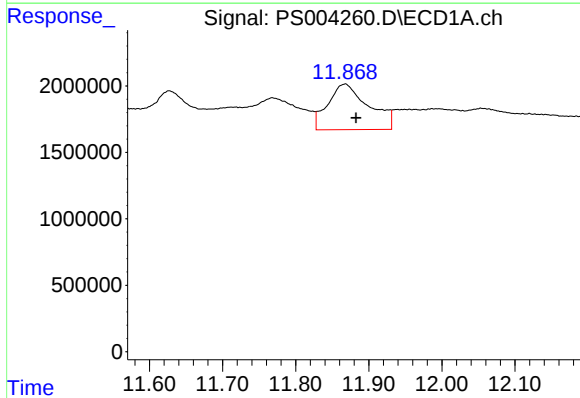


#6 MCPP

R.T.: 11.867 min
Delta R.T.: -0.016 min
Response: 13330188
Conc: 10.21 ug/ml

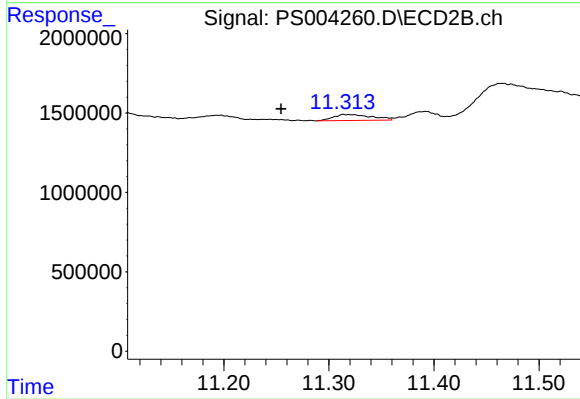

#6 MCPP


R.T.: 11.316 min
Delta R.T.: 0.062 min
Response: 947446
Conc: N.D.

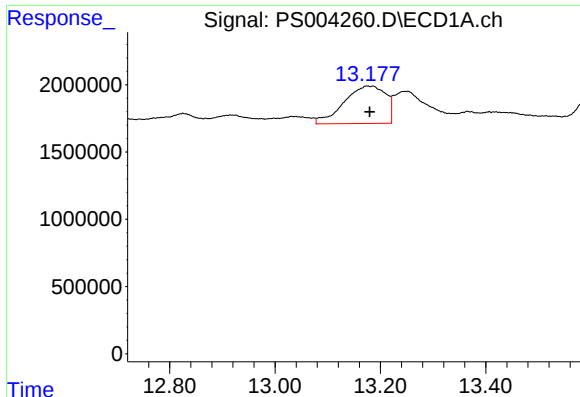

#9 2,4-D


R.T.: 13.179 min
Delta R.T.: -0.001 min
Response: 15370272
Conc: 33.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
MUDDY-BAGS

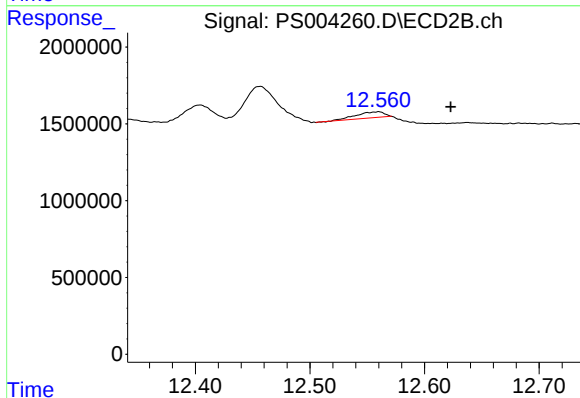


#9 2,4-D

R.T.: 12.558 min
Delta R.T.: -0.065 min
Response: 691788
Conc: 1.35 ng/ml

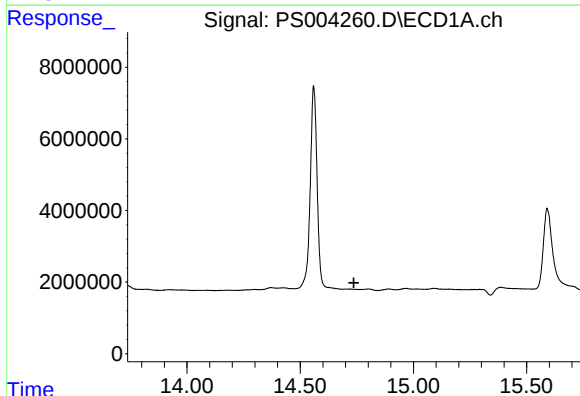


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.737 min
Response: 0
Conc: N.D.

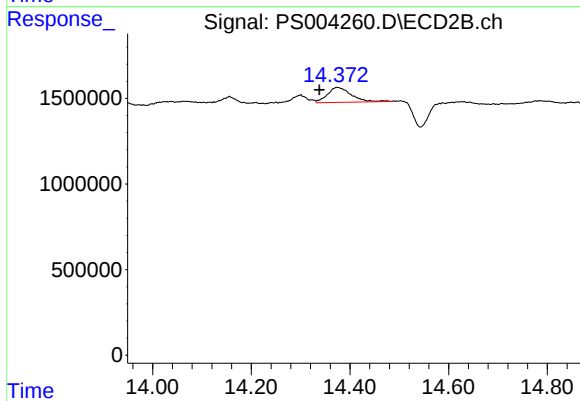

#12 2,4,5-T


R.T.: 14.374 min
Delta R.T.: 0.036 min
Response: 2927692
Conc: 1.27 ng/ml

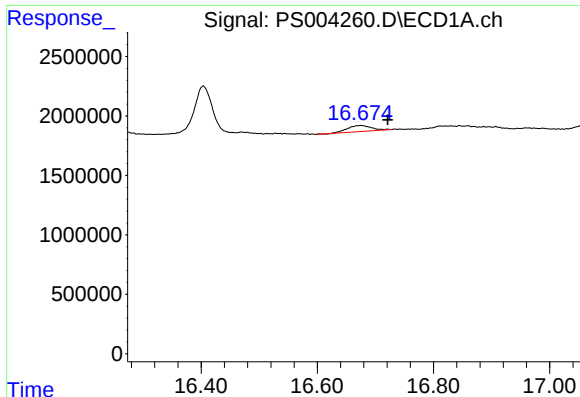

#15 Picloram


R.T.: 16.674 min
Delta R.T.: -0.047 min
Response: 1465726
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
MUDDY-BAGS

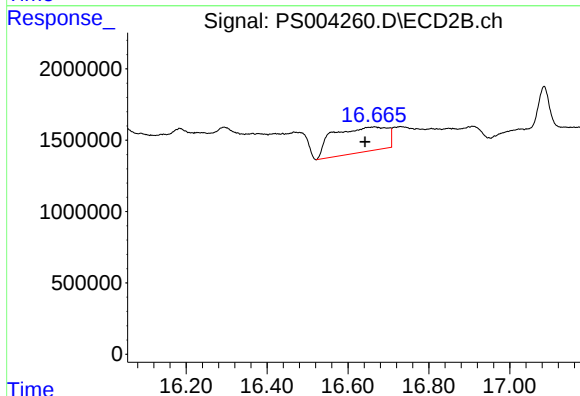


#15 Picloram

R.T.: 16.665 min
Delta R.T.: 0.023 min
Response: 16382838
Conc: 4.79 ng/ml

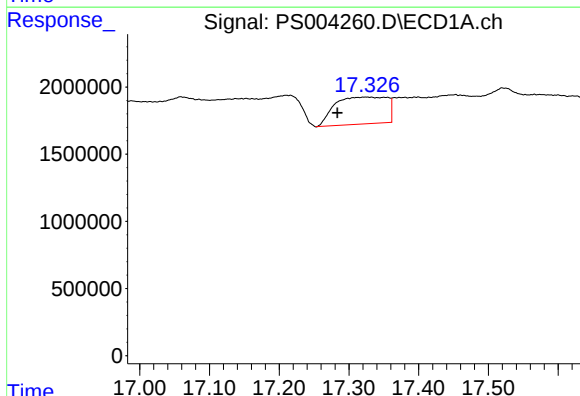

#16 DCPA

R.T.: 17.325 min
Delta R.T.: 0.041 min
Response: 10478527
Conc: 2.91 ng/ml

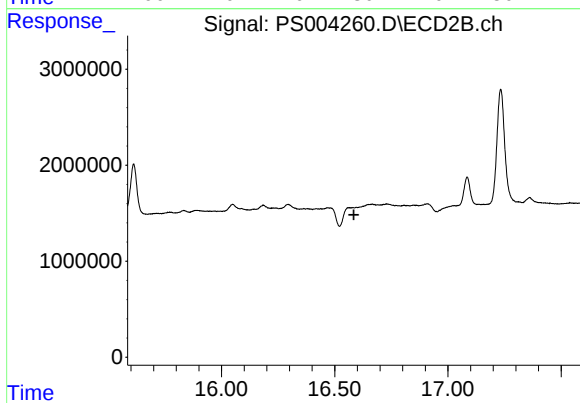

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 16.584 min
Response: 0
Conc: N.D.