

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042419\
 Data File : PS004265.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 19:32
 Operator : EI\SJ
 Sample : K2532-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 00:55:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.231	10.740	227.8E6	202.0E6	469.431	439.749
Target Compounds							
1) T	Dalapon	2.803	2.300	59859544	107.5E6	87.374	171.029 #
2) T	3,5-DICHL...	0.000	8.904	0	3381510	N.D.	5.916
3) T	4-Nitroph...	10.863	9.893	12239423	10112679	48.454	42.170
5) T	DICAMBA	0.000	10.980	0	2199374	N.D.	1.336
6) T	MCPD	11.905	0.000	12258256	0	9.390	N.D. #
7) T	MCPA	12.094	0.000	13428676	0	6.509	N.D. #
9) T	2,4-D	13.216	12.595	12669119	738205	27.824	1.443 #
12) T	2,4,5-T	0.000	14.338	0	6258848	N.D.	2.713
13) T	2,4-DB	15.427	0.000	18914827	0	60.738	N.D. #
14) T	DINOSEB	16.933	15.398	6448159	1245484	2.574	<MDL #
15) T	Picloram	16.718	16.602	16939342	-3200812	4.724	N.D. #
16) T	DCPA	17.247	16.602	16744958	-3200812	4.652	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042419\
Data File : PS004265.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 19:32
Operator : EI\SJ
Sample : K2532-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 00:55:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

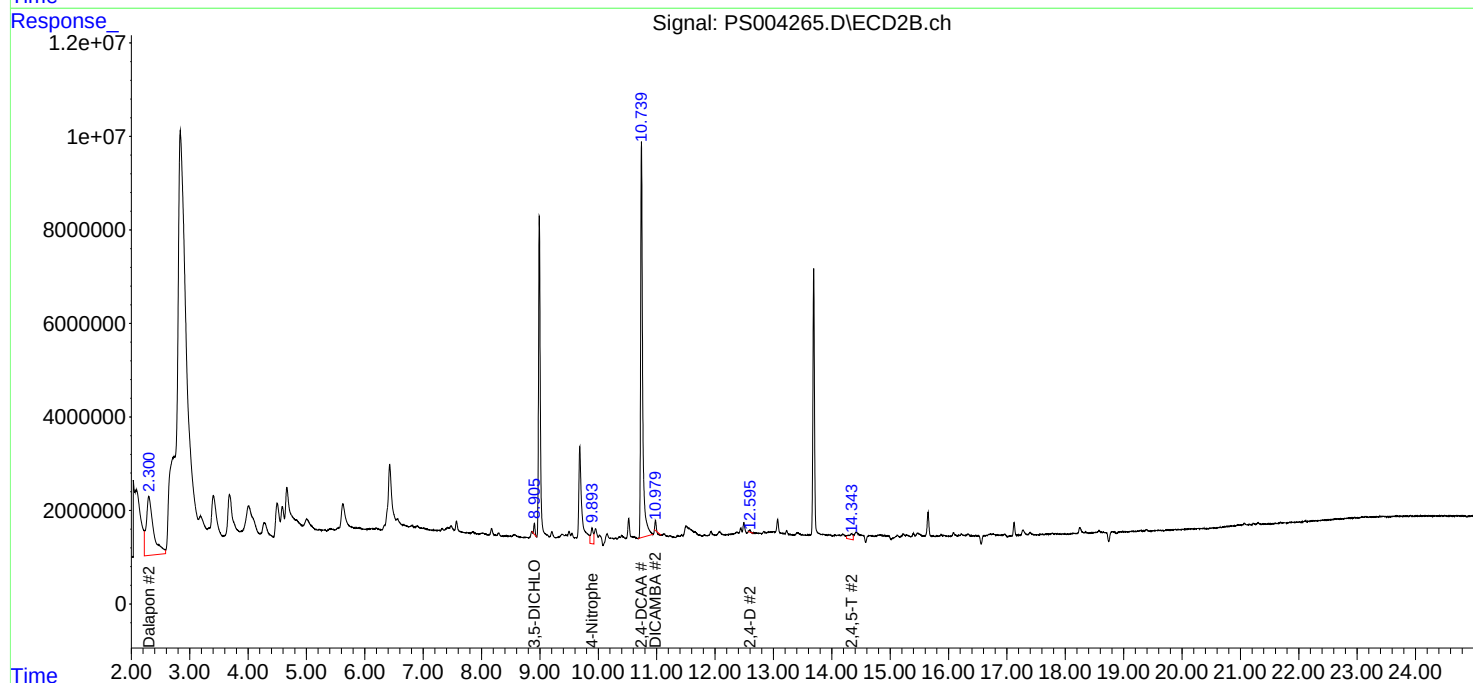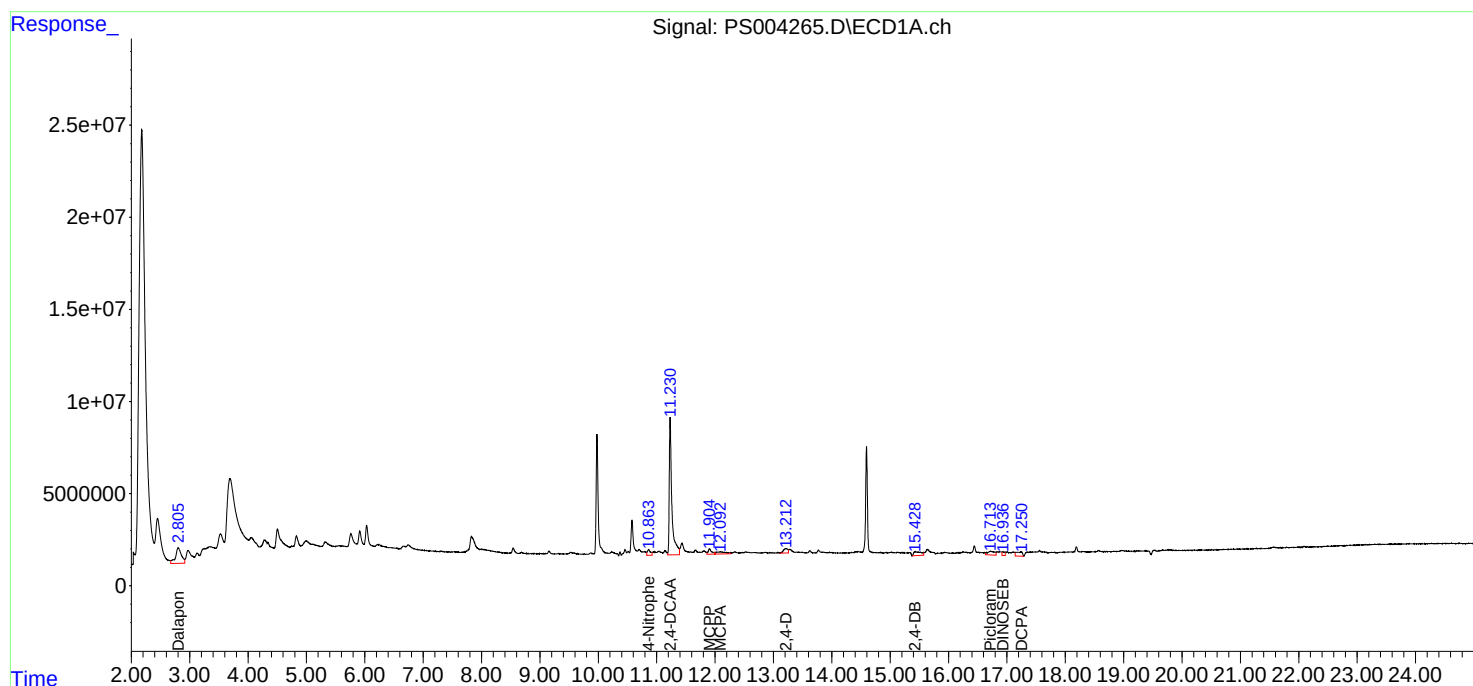


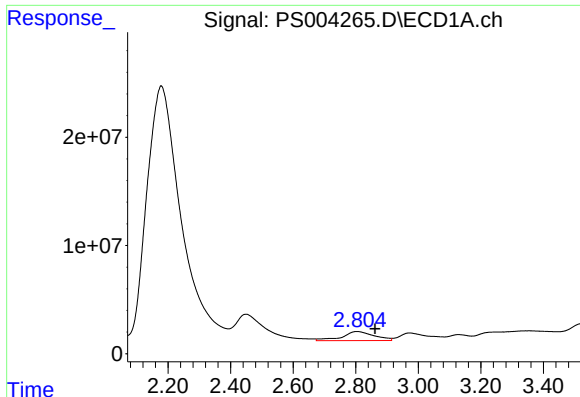

#1 Dalapon


R.T.: 2.803 min
Delta R.T.: -0.059 min
Response: 59859544
Conc: 87.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-5

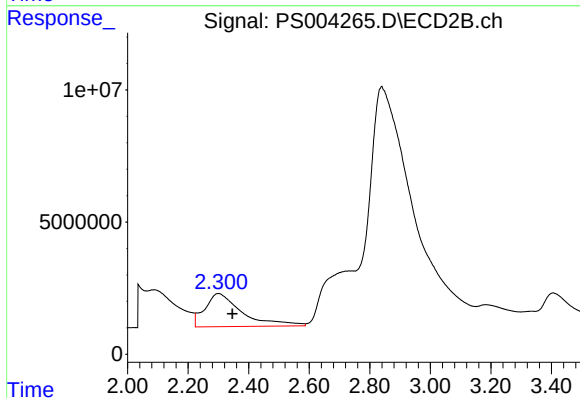


#1 Dalapon

R.T.: 2.300 min
Delta R.T.: -0.046 min
Response: 107484020
Conc: 171.03 ng/ml

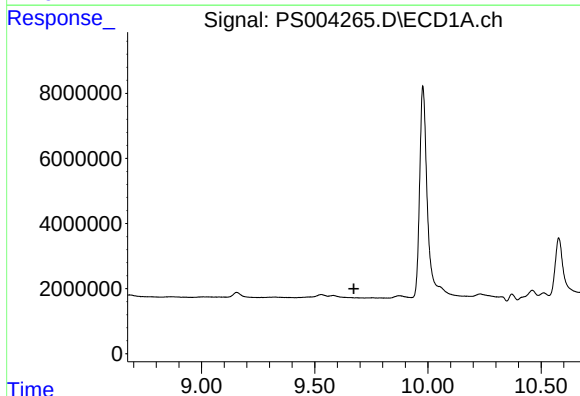


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.673 min
Response: 0
Conc: N.D.

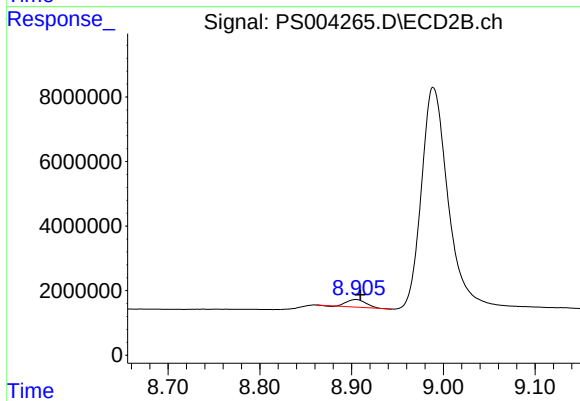

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.904 min
Delta R.T.: -0.005 min
Response: 3381510
Conc: 5.92 ng/ml

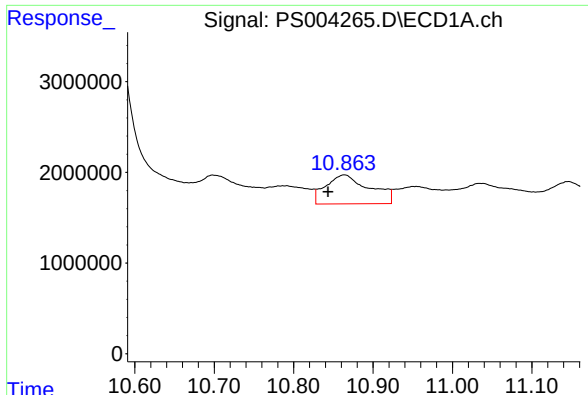

#3 4-Nitrophenol


R.T.: 10.863 min
Delta R.T.: 0.020 min
Response: 12239423
Conc: 48.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-5

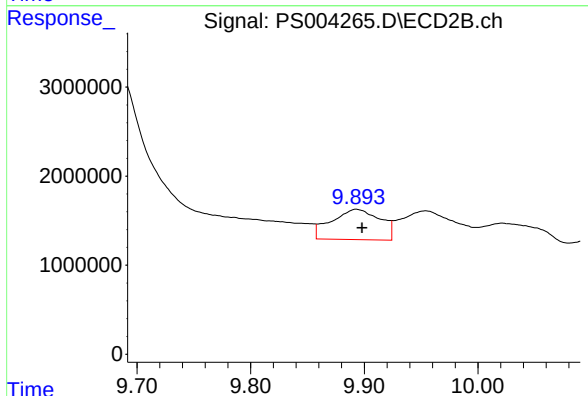


#3 4-Nitrophenol

R.T.: 9.893 min
Delta R.T.: -0.005 min
Response: 10112679
Conc: 42.17 ng/ml

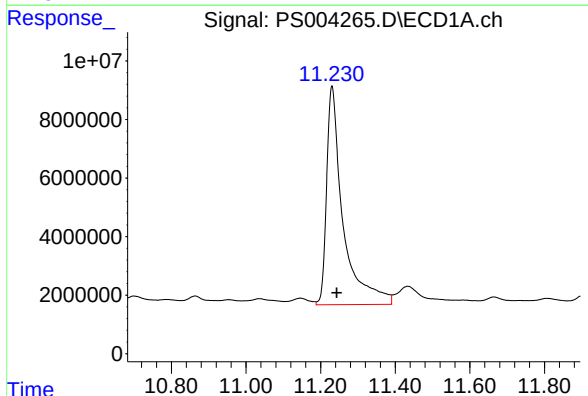


#4 2,4-DCAA

R.T.: 11.231 min
Delta R.T.: -0.012 min
Response: 227774928
Conc: 469.43 ng/ml

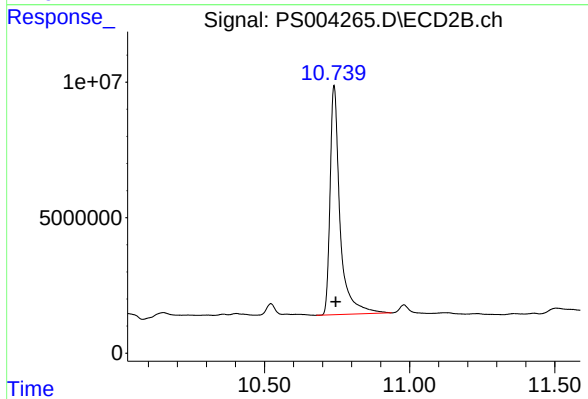

#4 2,4-DCAA


R.T.: 10.740 min
Delta R.T.: -0.006 min
Response: 201951141
Conc: 439.75 ng/ml

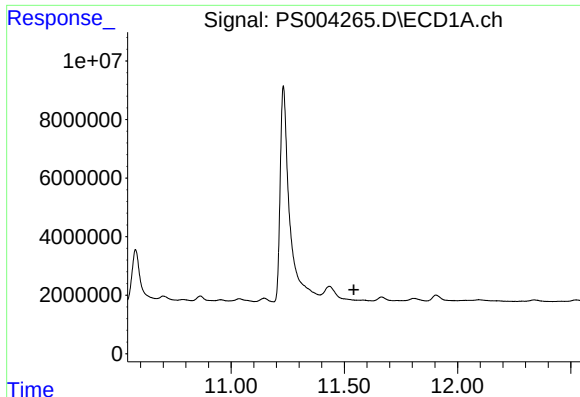

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-5

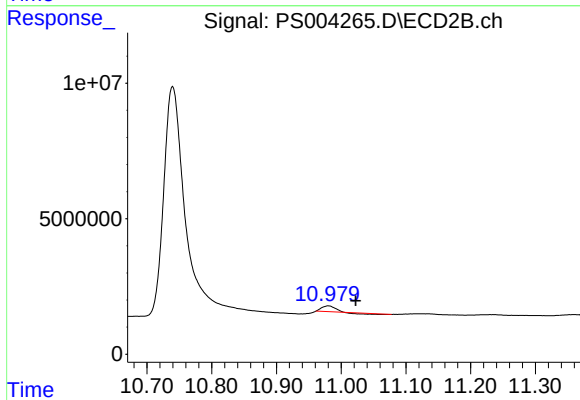


#5 DICAMBA

R.T.: 10.980 min
Delta R.T.: -0.043 min
Response: 2199374
Conc: 1.34 ng/ml

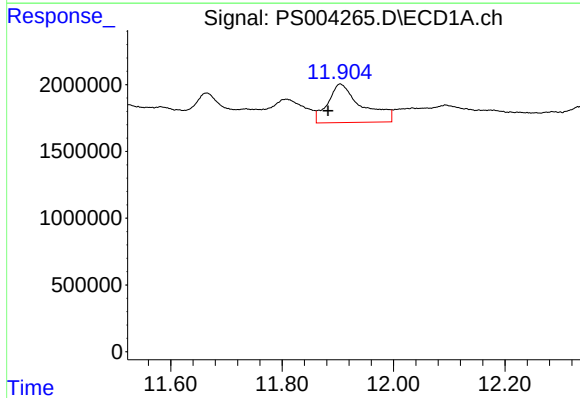


#6 MCP

R.T.: 11.905 min
Delta R.T.: 0.022 min
Response: 12258256
Conc: 9.39 ug/ml

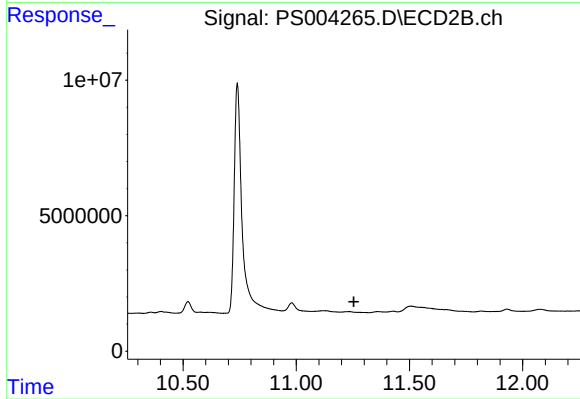

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.255 min
Response: 0
Conc: N.D.

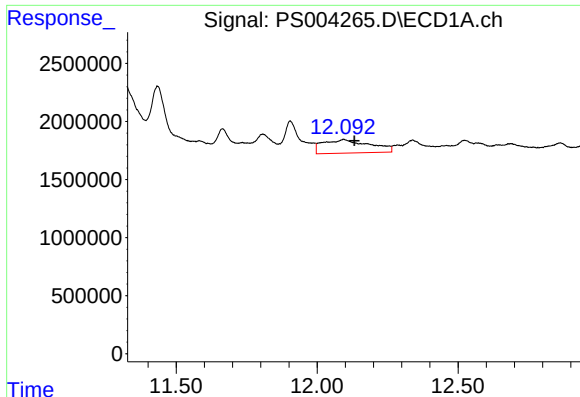

#7 MCPA


R.T.: 12.094 min
Delta R.T.: -0.038 min
Response: 13428676
Conc: 6.51 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-5

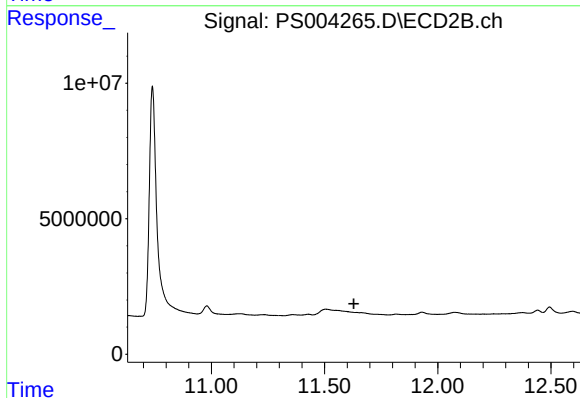


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.630 min
Response: 0
Conc: N.D.

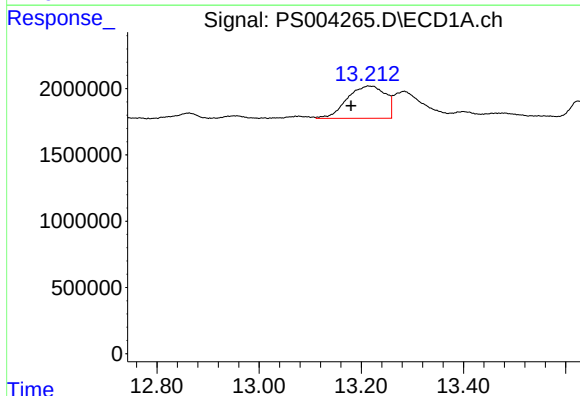


#9 2,4-D

R.T.: 13.216 min
Delta R.T.: 0.036 min
Response: 12669119
Conc: 27.82 ng/ml

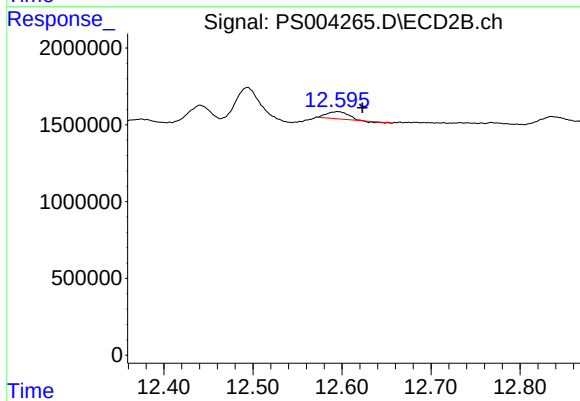

#9 2,4-D


R.T.: 12.595 min
Delta R.T.: -0.028 min
Response: 738205
Conc: 1.44 ng/ml

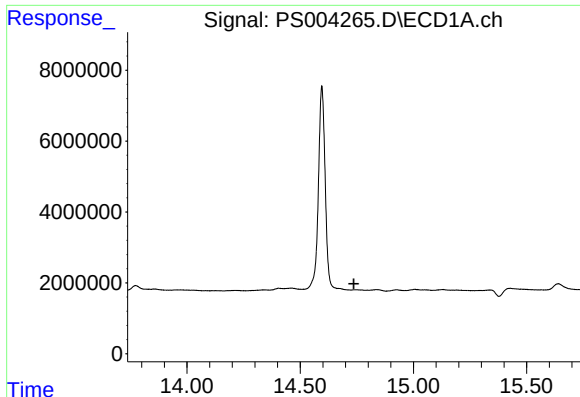

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.737 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-5

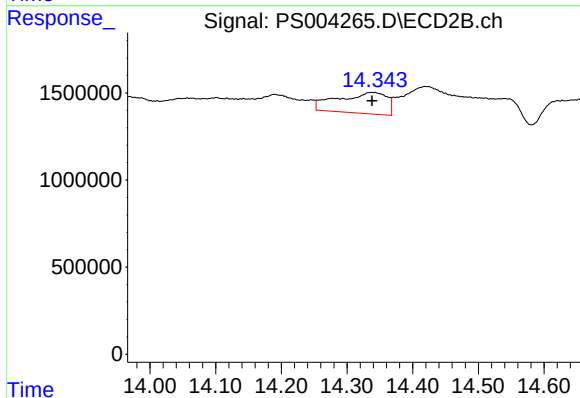


#12 2,4,5-T

R.T.: 14.338 min
Delta R.T.: 0.000 min
Response: 6258848
Conc: 2.71 ng/ml

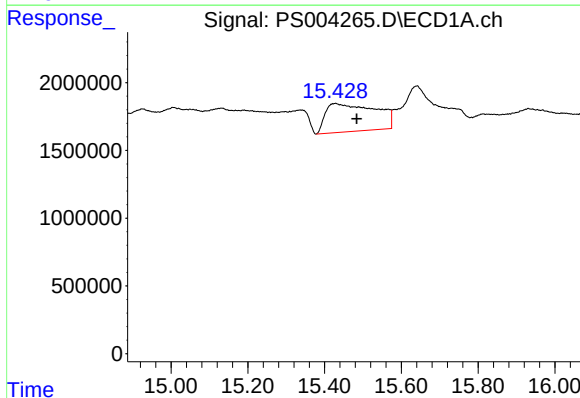


#13 2,4-DB

R.T.: 15.427 min
Delta R.T.: -0.056 min
Response: 18914827
Conc: 60.74 ng/ml

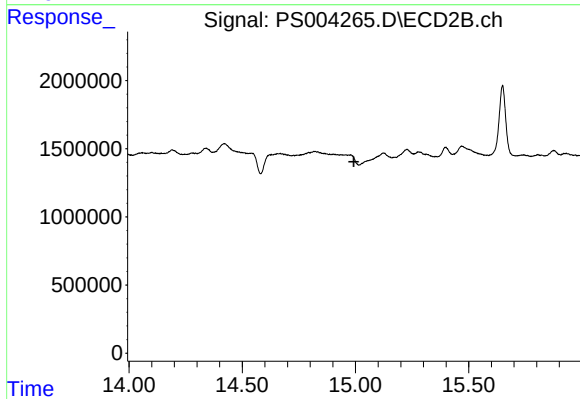

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 14.993 min
Response: 0
Conc: N.D.

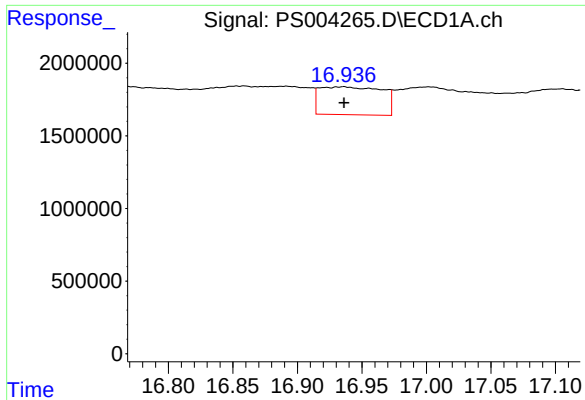

#14 DINOSEB


R.T.: 16.933 min
Delta R.T.: -0.003 min
Response: 6448159
Conc: 2.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-5

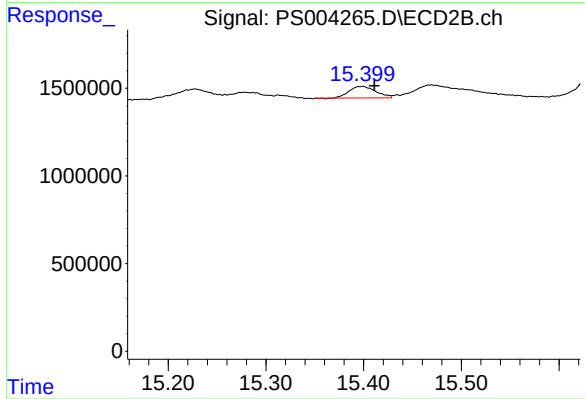


#14 DINOSEB

R.T.: 15.398 min
Delta R.T.: -0.013 min
Response: 1245484
Conc: N.D.

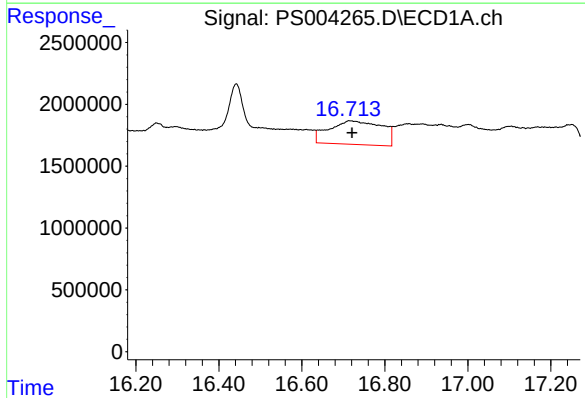


#15 Picloram

R.T.: 16.718 min
Delta R.T.: -0.003 min
Response: 16939342
Conc: 4.72 ng/ml

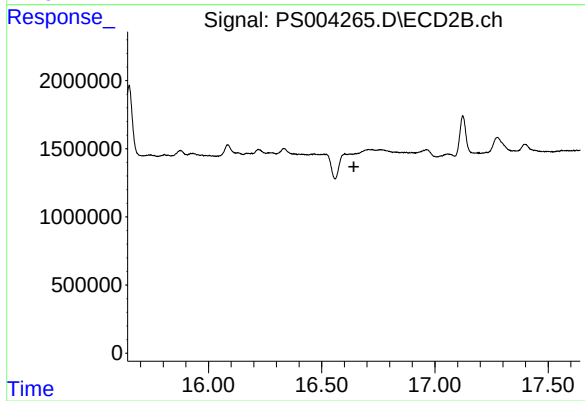

#15 Picloram


R.T.: 16.602 min
Delta R.T.: -0.040 min
Response: -3200812
Conc: N.D.

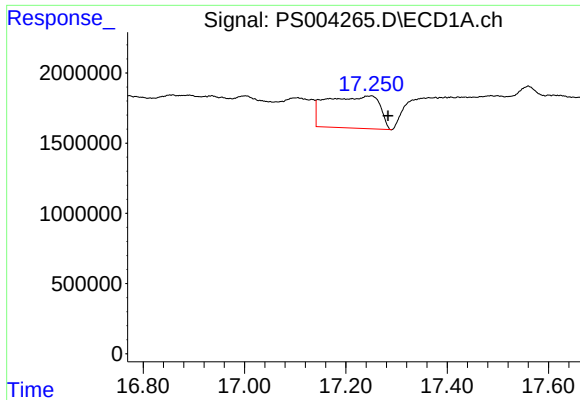

#16 DCPA

R.T.: 17.247 min
Delta R.T.: -0.037 min
Response: 16744958
Conc: 4.65 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-5

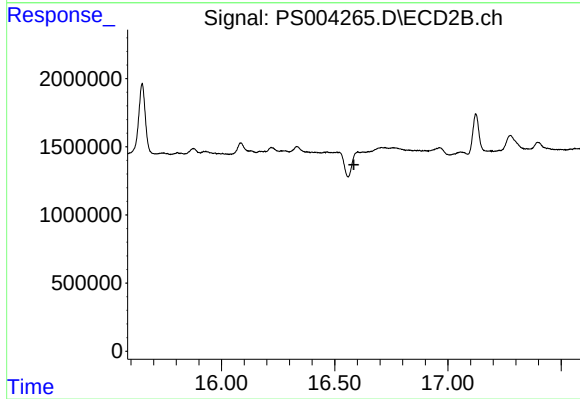

#16 DCPA

R.T.: 16.602 min
Delta R.T.: 0.018 min
Response: -3200812
Conc: N.D.