

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042419\
 Data File : PS004266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 20:04
 Operator : EI\SJ
 Sample : K2532-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 00:56:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.211	10.721	248.3E6	219.3E6	511.783	477.553
Target Compounds							
1) T	Dalapon	0.000	2.280	0	101.4E6	N.D.	161.361
2) T	3,5-DICHL...	0.000	8.885	0	4030594	N.D.	7.051
3) T	4-Nitroph...	10.843	9.875	12061552	10575331	47.750	44.099
6) T	MCP	11.885	0.000	11948359	0	9.153	N.D. #
9) T	2,4-D	13.197	0.000	12218524	0	26.834	N.D. #
10) T	Pentachlo...	0.000	13.209	0	1278445	N.D.	<MDL
12) T	2,4,5-T	14.731	14.319	1509760	7977287	<MDL	3.458 #
14) T	DINOSEB	16.873	15.379	1426112	3225732	<MDL	1.726 #
15) T	Picloram	16.694	16.692	2635215	3905196	<MDL	1.141 #
16) T	DCPA	17.228	0.000	13105050	0	3.641	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042419\
Data File : PS004266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 20:04
Operator : EI\SJ
Sample : K2532-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 00:56:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

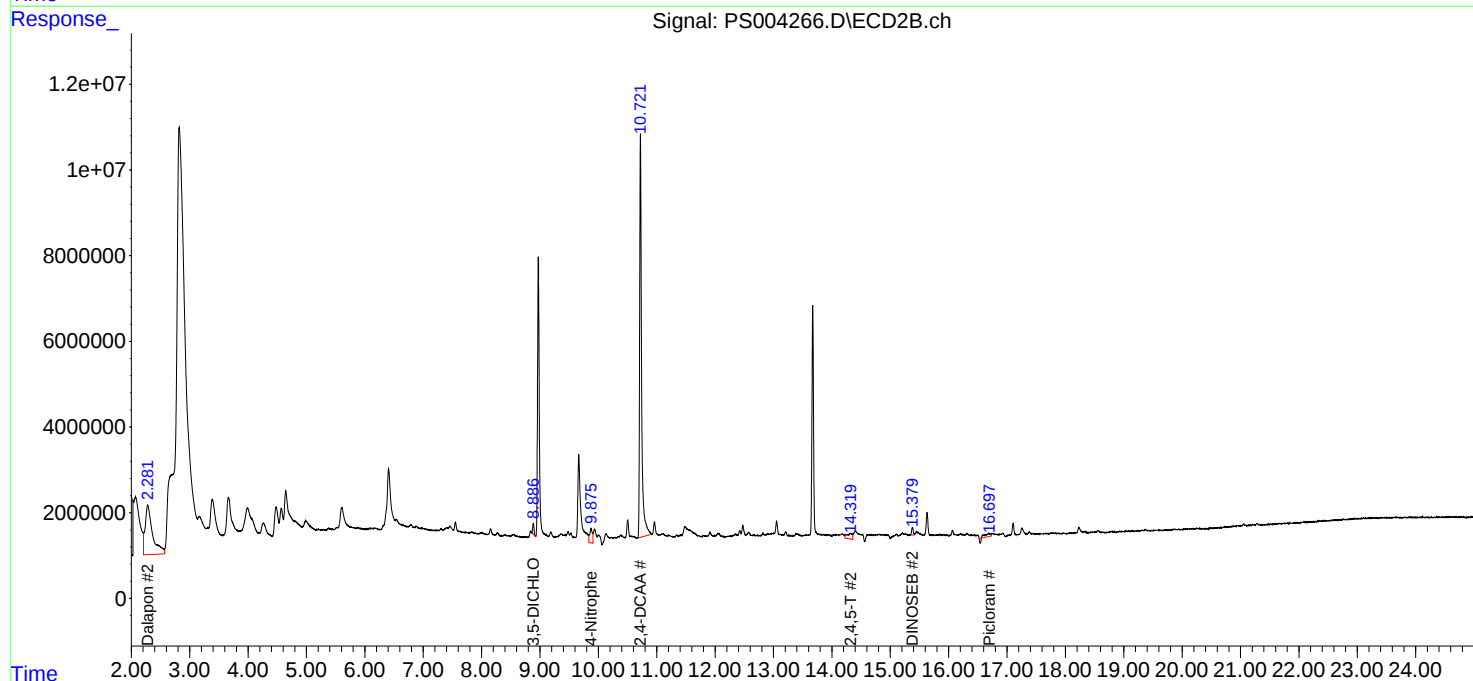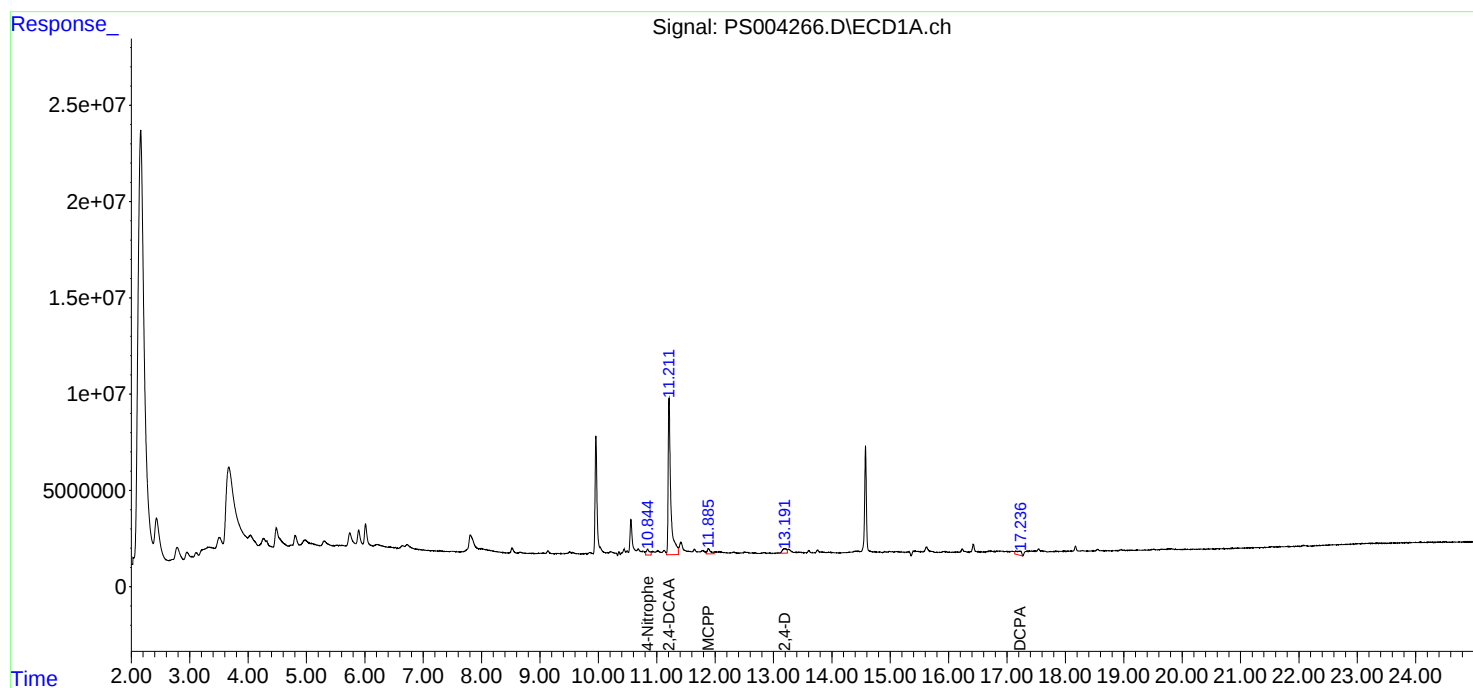


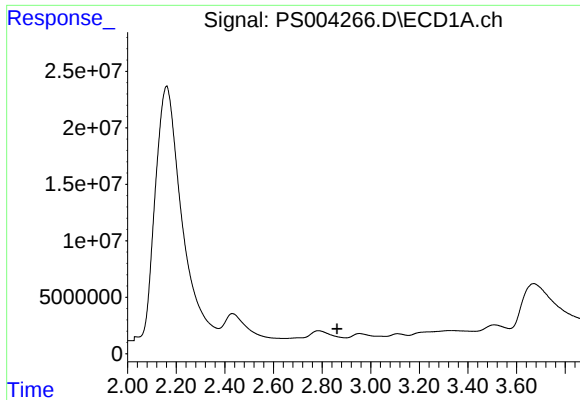

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.862 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2

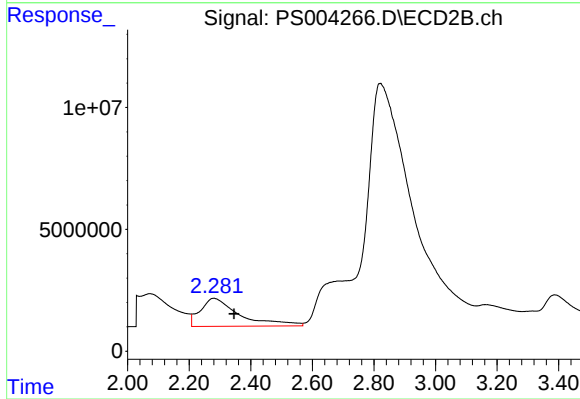


#1 Dalapon

R.T.: 2.280 min
Delta R.T.: -0.067 min
Response: 101408176
Conc: 161.36 ng/ml

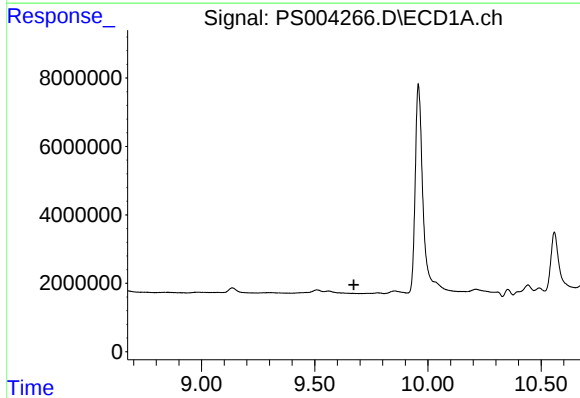


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.673 min
Response: 0
Conc: N.D.

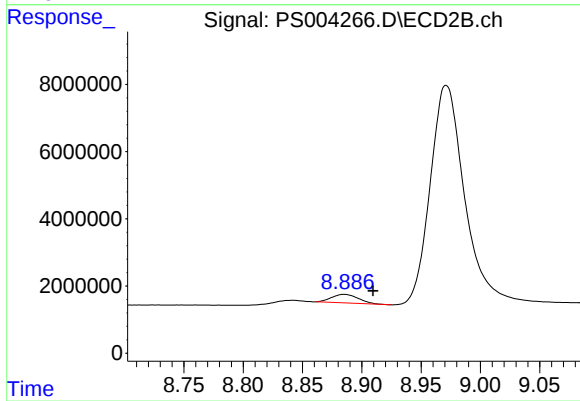

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.885 min
Delta R.T.: -0.024 min
Response: 4030594
Conc: 7.05 ng/ml

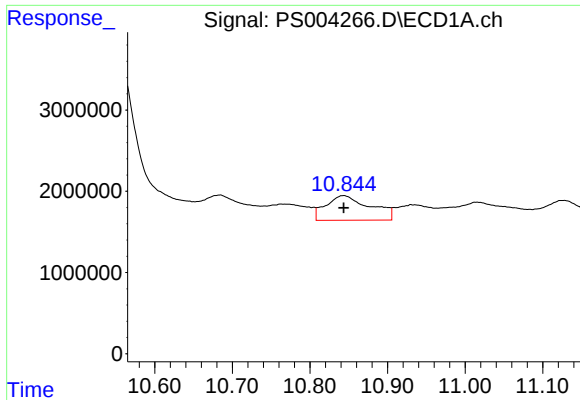

#3 4-Nitrophenol


R.T.: 10.843 min
Delta R.T.: 0.000 min
Response: 12061552
Conc: 47.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-2

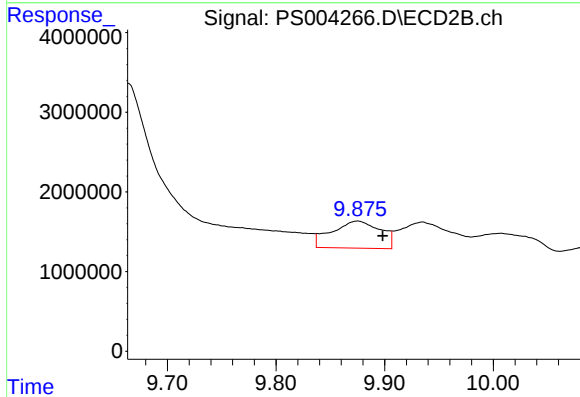


#3 4-Nitrophenol

R.T.: 9.875 min
Delta R.T.: -0.023 min
Response: 10575331
Conc: 44.10 ng/ml

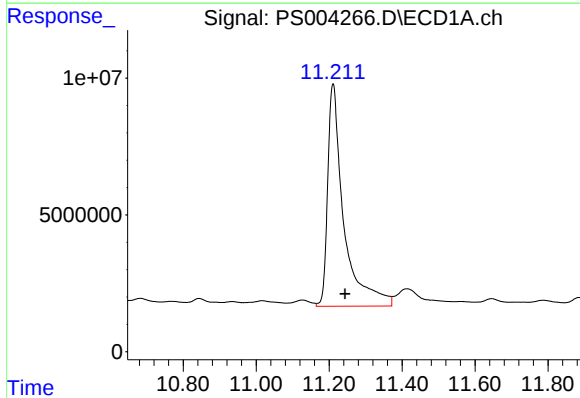


#4 2,4-DCAA

R.T.: 11.211 min
Delta R.T.: -0.032 min
Response: 248324386
Conc: 511.78 ng/ml

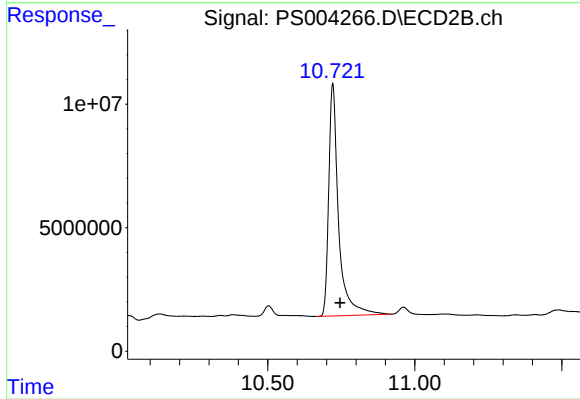

#4 2,4-DCAA


R.T.: 10.721 min
Delta R.T.: -0.025 min
Response: 219312379
Conc: 477.55 ng/ml

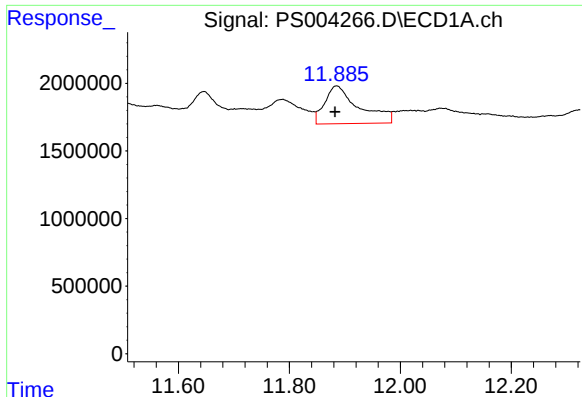

#6 MCP


R.T.: 11.885 min
Delta R.T.: 0.003 min
Response: 11948359
Conc: 9.15 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-2

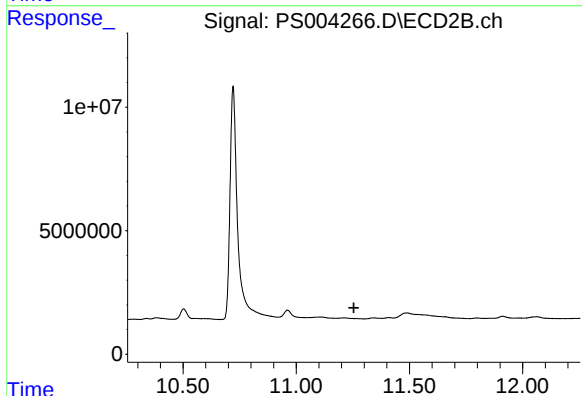


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.255 min
Response: 0
Conc: N.D.

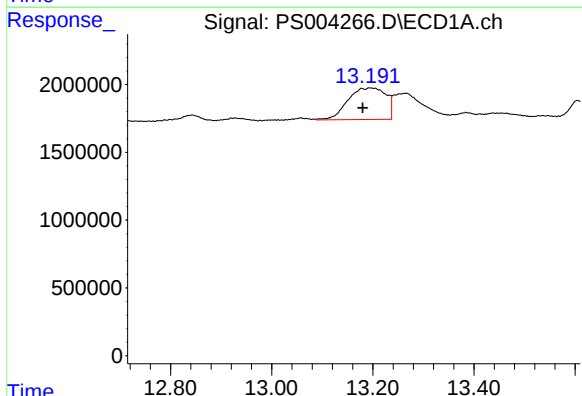


#9 2,4-D

R.T.: 13.197 min
Delta R.T.: 0.017 min
Response: 12218524
Conc: 26.83 ng/ml

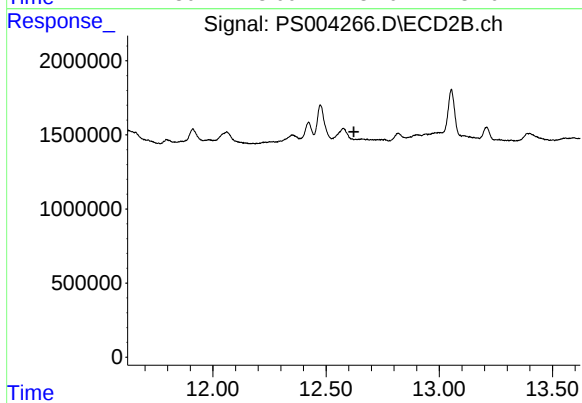

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 12.623 min
Response: 0
Conc: N.D.

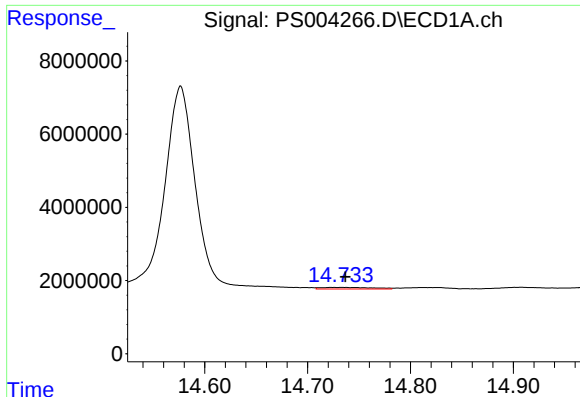

#12 2,4,5-T


R.T.: 14.731 min
Delta R.T.: -0.006 min
Response: 1509760
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2

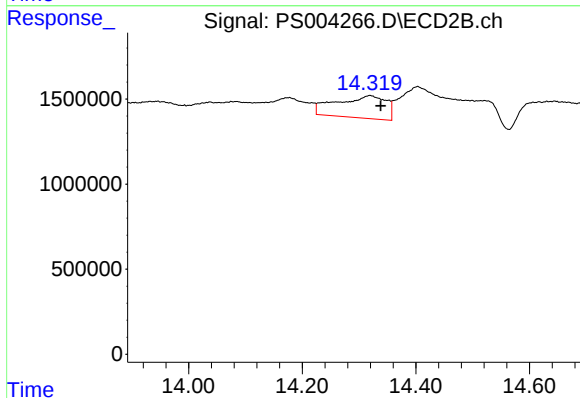


#12 2,4,5-T

R.T.: 14.319 min
Delta R.T.: -0.019 min
Response: 7977287
Conc: 3.46 ng/ml

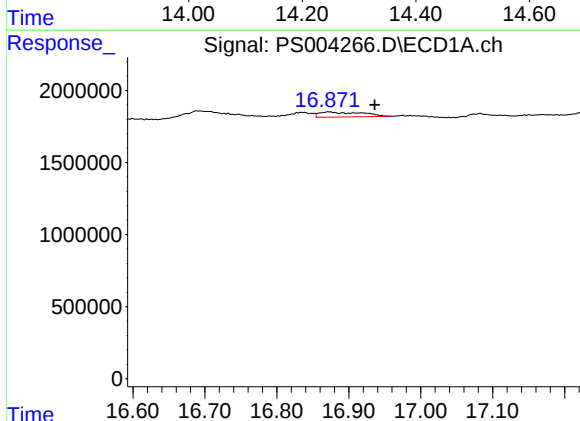


#14 DINOSEB

R.T.: 16.873 min
Delta R.T.: -0.064 min
Response: 1426112
Conc: N.D.

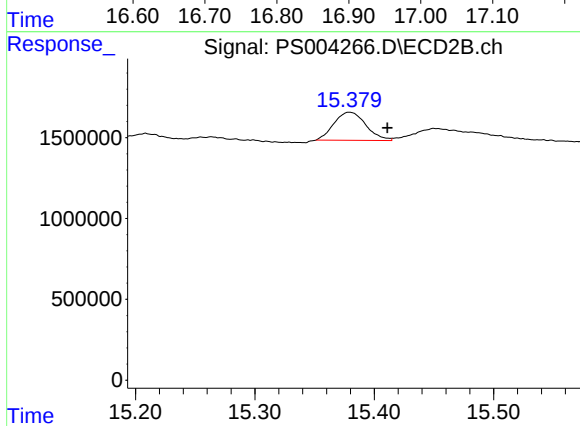

#14 DINOSEB


R.T.: 15.379 min
Delta R.T.: -0.032 min
Response: 3225732
Conc: 1.73 ng/ml

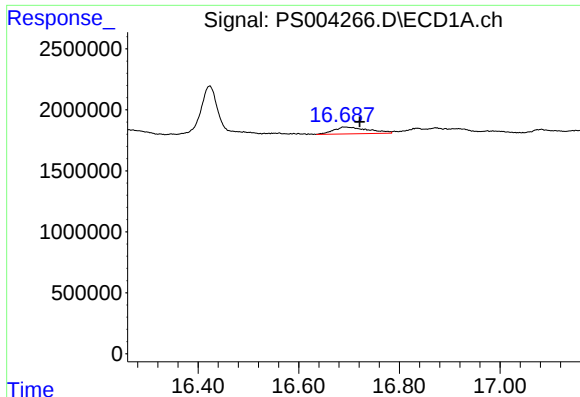

#15 Picloram


R.T.: 16.694 min
Delta R.T.: -0.027 min
Response: 2635215
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2

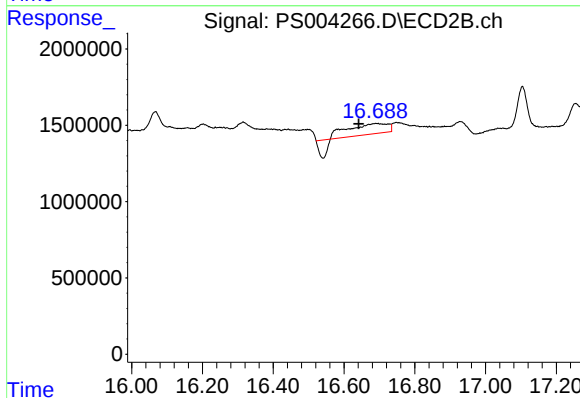


#15 Picloram

R.T.: 16.692 min
Delta R.T.: 0.050 min
Response: 3905196
Conc: 1.14 ng/ml

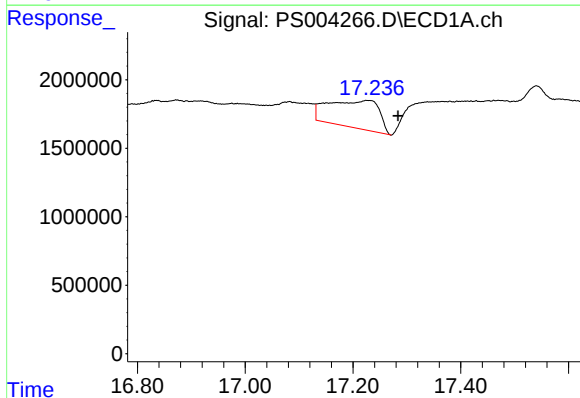

#16 DCPA

R.T.: 17.228 min
Delta R.T.: -0.056 min
Response: 13105050
Conc: 3.64 ng/ml

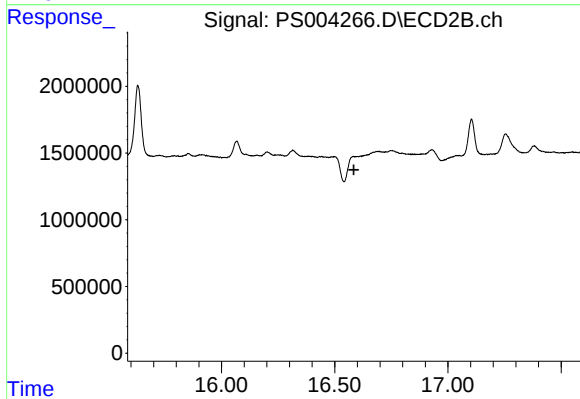

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 16.584 min
Response: 0
Conc: N.D.