

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042419\
 Data File : PS004267.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 20:36
 Operator : EI\SJ
 Sample : K2532-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 00:56:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.185	10.692	222.2E6	194.2E6	457.996	422.774
Target Compounds							
1) T	Dalapon	2.925	0.000	24950990	0	36.420	N.D. #
2) T	3,5-DICHL...	0.000	8.943	0	114.6E6	N.D.	200.408
3) T	4-Nitroph...	10.816	9.906	13005292	11265106	51.486	46.976
6) T	MCP	11.859	11.310	14343167	775877	10.987	<MDL #
9) T	2,4-D	13.173	0.000	13602302	0	29.874	N.D. #
10) T	Pentachlo...	13.402	13.179	6722816	-809142	<MDL	N.D. #
11) T	2,4,5-TP ...	14.359	0.000	2531845	0	<MDL	N.D. #
12) T	2,4,5-T	0.000	14.373	0	13138930	N.D.	5.696
14) T	DINOSEB	16.887	15.426	1128723	-816706	<MDL	N.D. #
15) T	Picloram	16.671	16.660	7381631	7420861	2.058	2.168
16) T	DCPA	17.315	16.567	7974485	4180839	2.215	1.315 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042419\
Data File : PS004267.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 20:36
Operator : EI\SJ
Sample : K2532-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 00:56:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

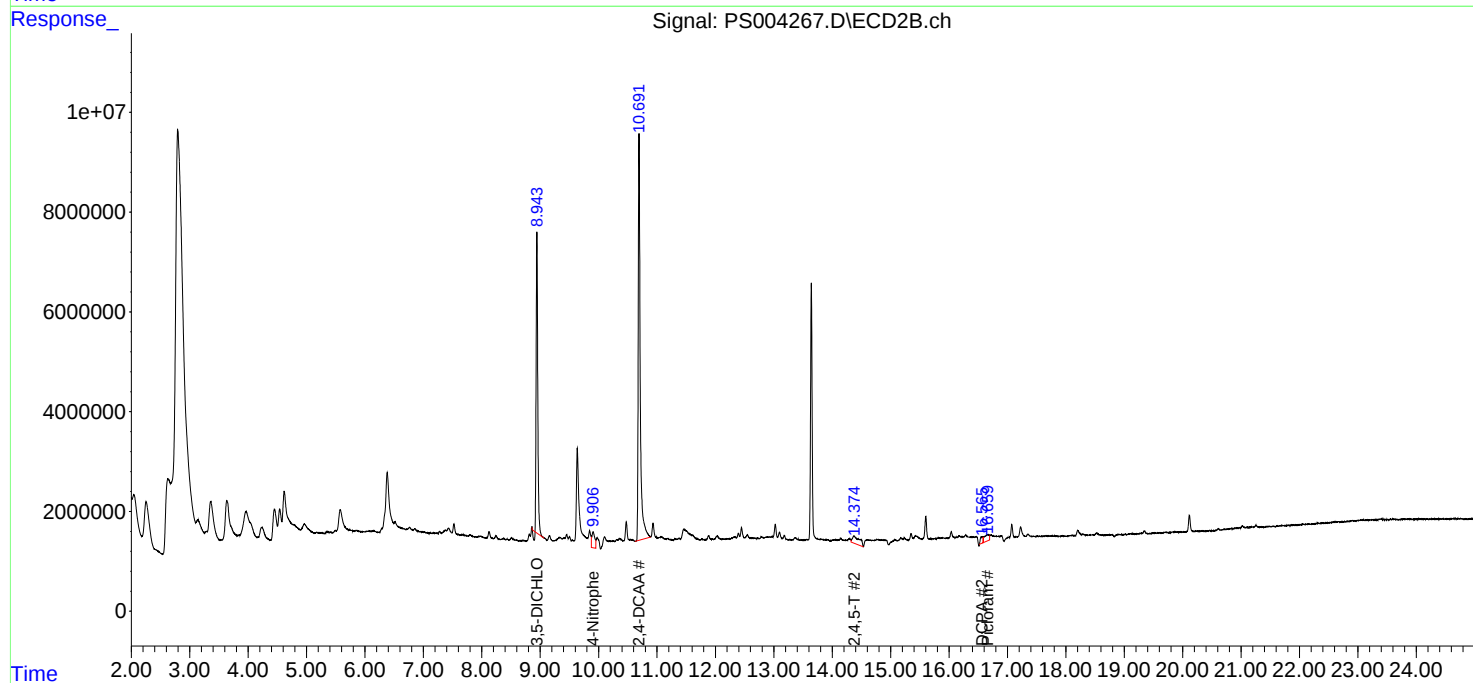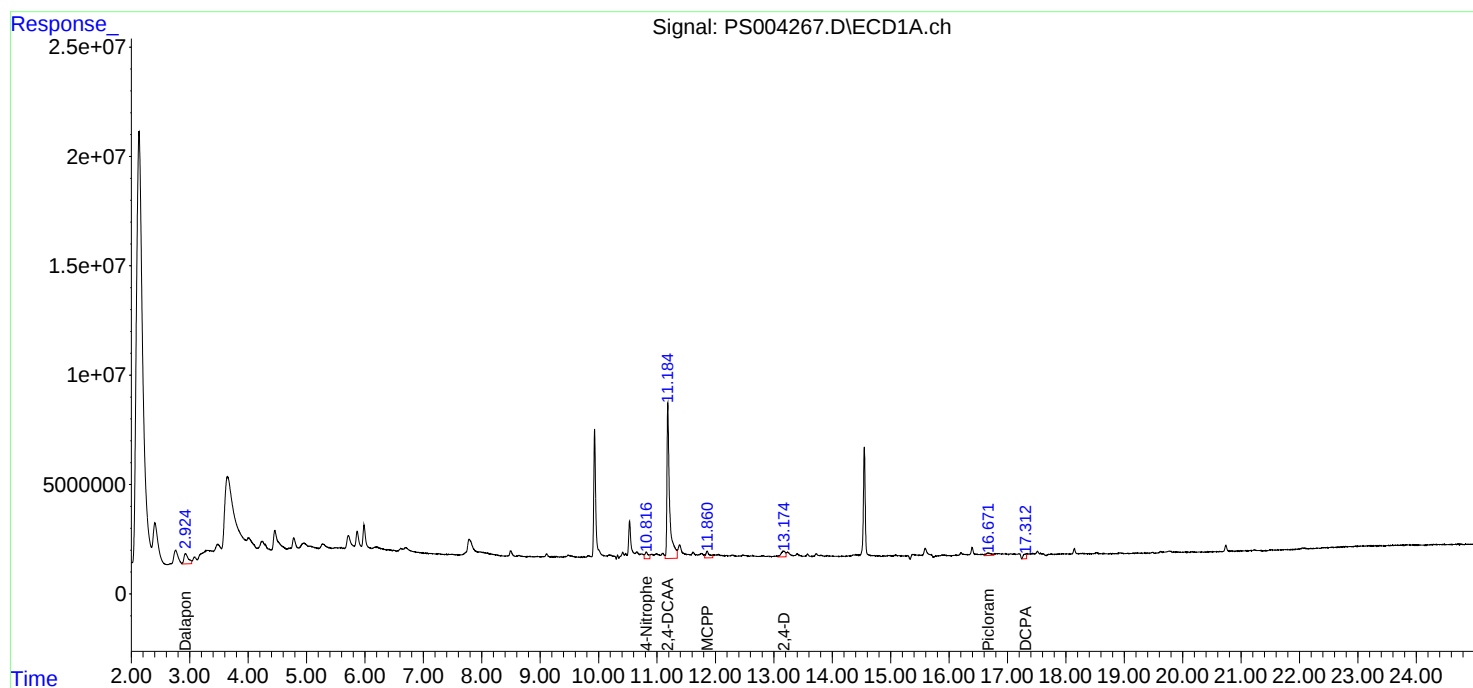


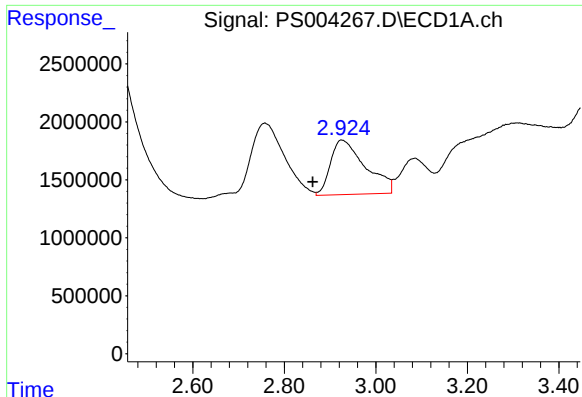

#1 Dalapon


R.T.: 2.925 min
Delta R.T.: 0.063 min
Response: 24950990
Conc: 36.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

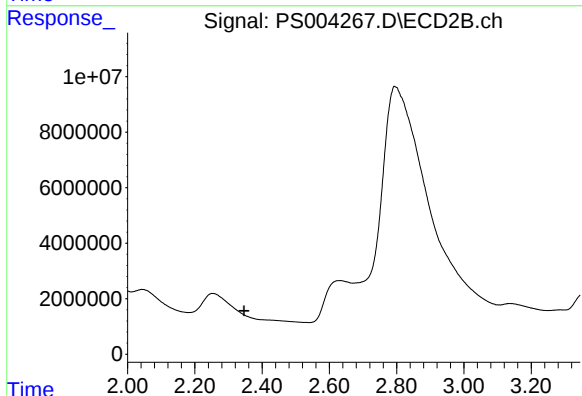


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.346 min
Response: 0
Conc: N.D.

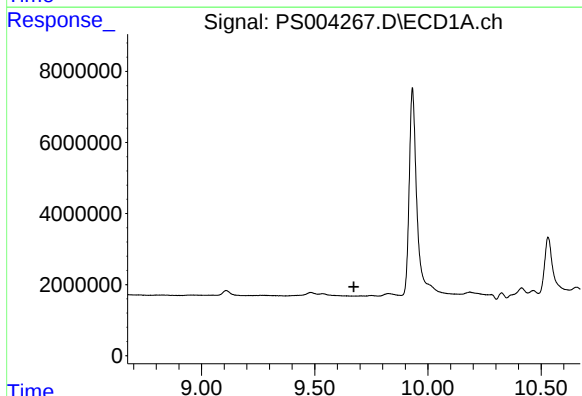


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.673 min
Response: 0
Conc: N.D.

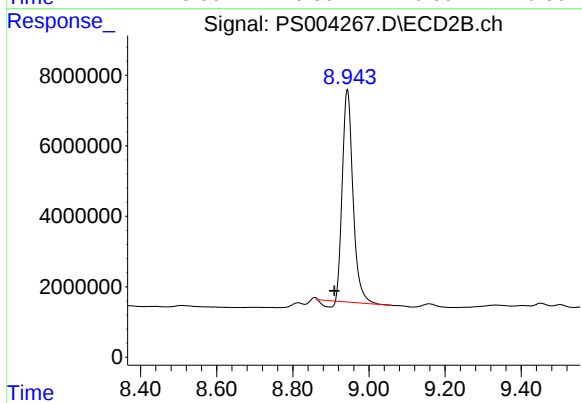

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.943 min
Delta R.T.: 0.034 min
Response: 114558373
Conc: 200.41 ng/ml

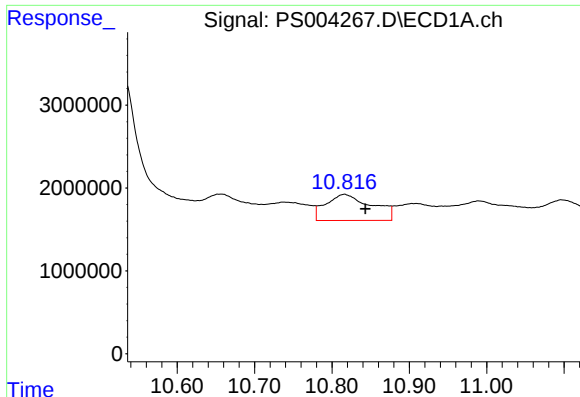

#3 4-Nitrophenol


R.T.: 10.816 min
Delta R.T.: -0.028 min
Response: 13005292
Conc: 51.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

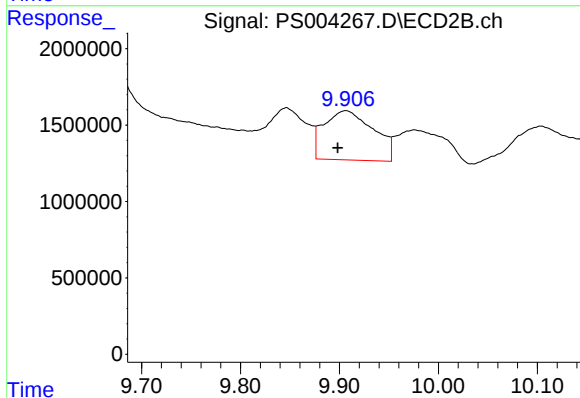


#3 4-Nitrophenol

R.T.: 9.906 min
Delta R.T.: 0.008 min
Response: 11265106
Conc: 46.98 ng/ml

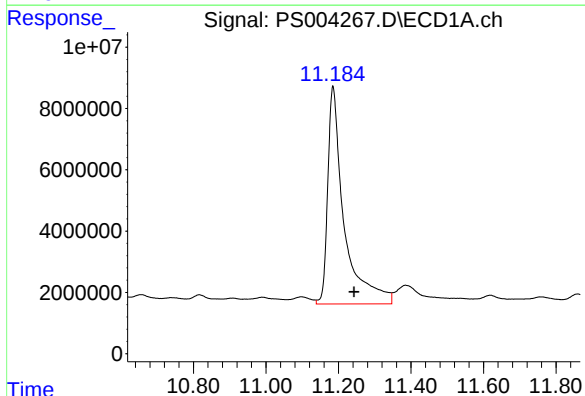


#4 2,4-DCAA

R.T.: 11.185 min
Delta R.T.: -0.058 min
Response: 222226516
Conc: 458.00 ng/ml

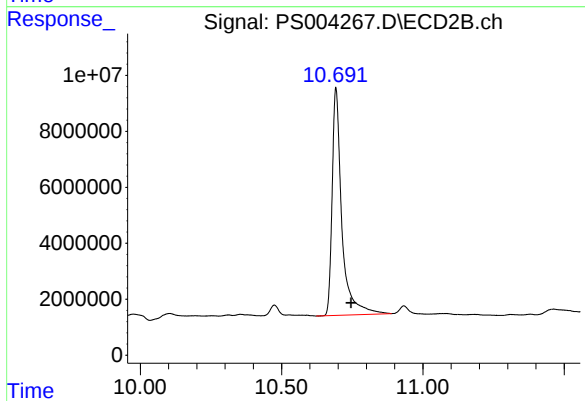

#4 2,4-DCAA


R.T.: 10.692 min
Delta R.T.: -0.053 min
Response: 194155629
Conc: 422.77 ng/ml

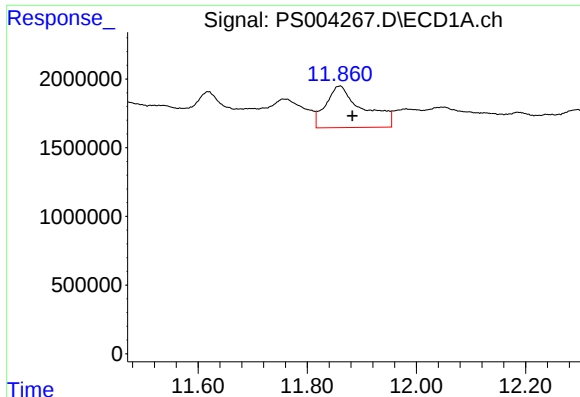

#6 MCP


R.T.: 11.859 min
Delta R.T.: -0.023 min
Response: 14343167
Conc: 10.99 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

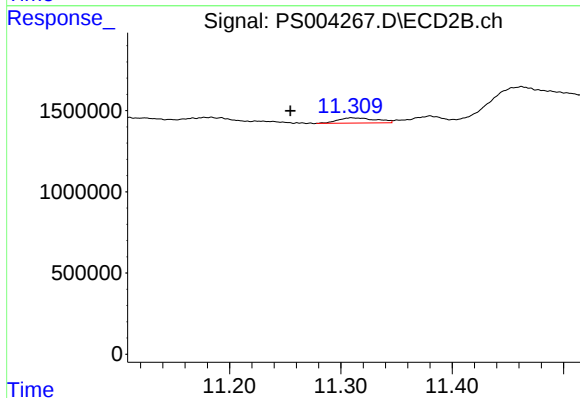


#6 MCP

R.T.: 11.310 min
Delta R.T.: 0.055 min
Response: 775877
Conc: N.D.

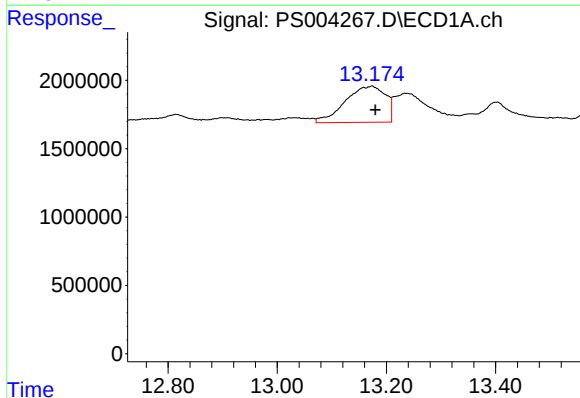


#9 2,4-D

R.T.: 13.173 min
Delta R.T.: -0.007 min
Response: 13602302
Conc: 29.87 ng/ml

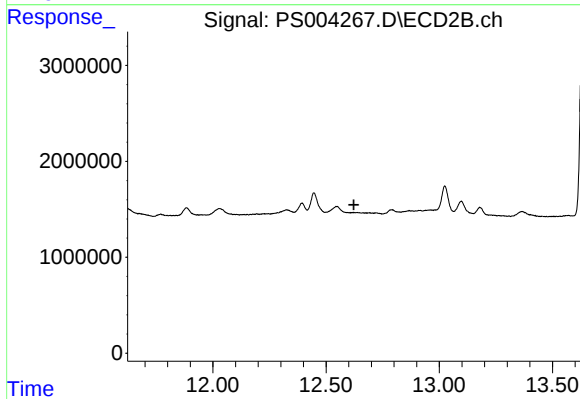

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 12.623 min
Response: 0
Conc: N.D.

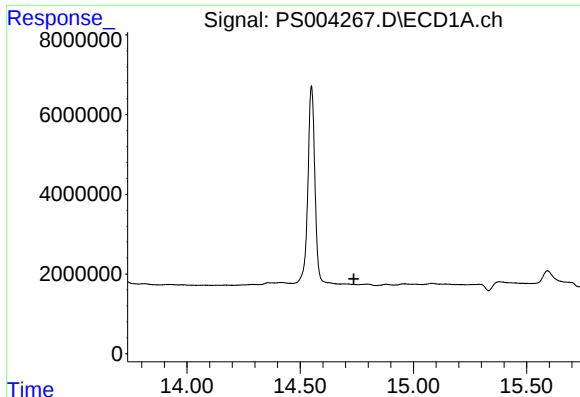

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.737 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3

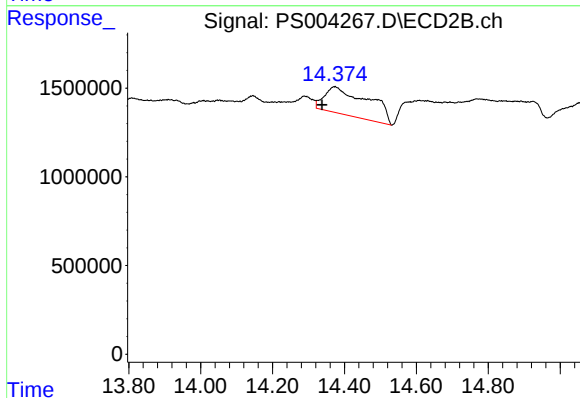


#12 2,4,5-T

R.T.: 14.373 min
Delta R.T.: 0.035 min
Response: 13138930
Conc: 5.70 ng/ml

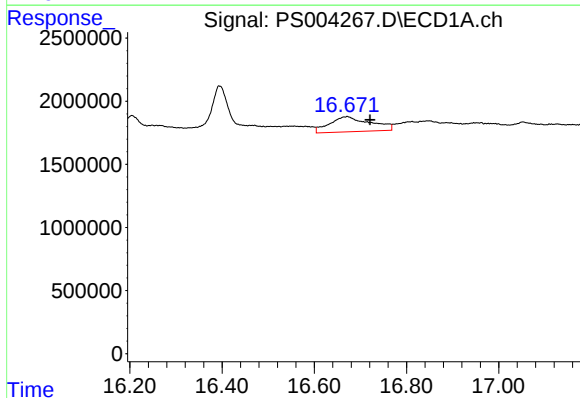


#15 Picloram

R.T.: 16.671 min
Delta R.T.: -0.050 min
Response: 7381631
Conc: 2.06 ng/ml

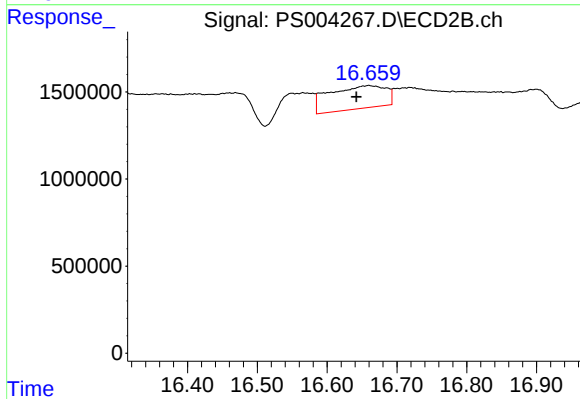

#15 Picloram


R.T.: 16.660 min
Delta R.T.: 0.018 min
Response: 7420861
Conc: 2.17 ng/ml

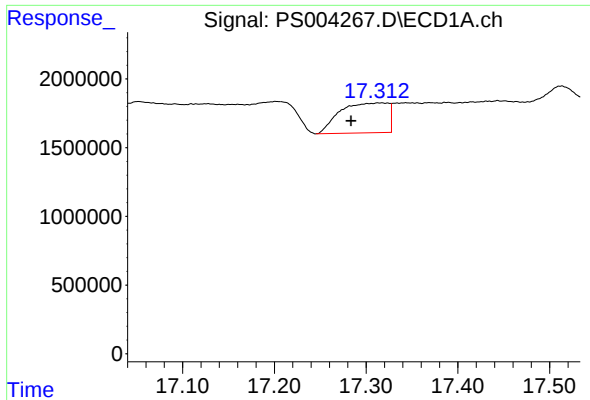

#16 DCPA

R.T.: 17.315 min
Delta R.T.: 0.032 min
Response: 7974485
Conc: 2.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

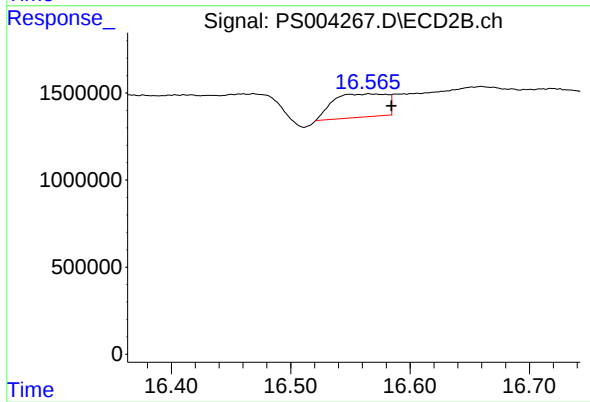

#16 DCPA

R.T.: 16.567 min
Delta R.T.: -0.018 min
Response: 4180839
Conc: 1.32 ng/ml