

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042419\
 Data File : PS004283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2019 05:09
 Operator : EI\SJ
 Sample : K2200-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 EO-02-042319-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 07:54:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.219	10.725	228.3E6	195.0E6	470.484	424.710
Target Compounds							
1) T	Dalapon	0.000	2.289	0	82471205	N.D.	131.229
2) T	3,5-DICHL...	0.000	8.890	0	4671105	N.D.	8.172
3) T	4-Nitroph...	10.851	9.878	15684974	9004770	62.095	37.550 #
6) T	MCP	11.891	0.000	14953475	0	11.455	N.D. #
7) T	MCPA	12.078	0.000	11852539	0	5.745	N.D. #
8) T	DICHLORPROP	0.000	12.187	0	446574	N.D.	1.052
9) T	2,4-D	13.203	0.000	11820994	0	25.961	N.D. #
10) T	Pentachlo...	0.000	13.213	0	1215934	N.D.	<MDL
11) T	2,4,5-TP ...	14.333	0.000	825805	0	<MDL	N.D. #
12) T	2,4,5-T	0.000	14.322	0	620196	N.D.	<MDL
14) T	DINOSEB	16.922	15.383	1057317	835601	<MDL	<MDL #
15) T	Picloram	16.699	0.000	4690418	0	1.308	N.D. #
16) T	DCPA	17.235	0.000	3329232	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042419\
Data File : PS004283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2019 05:09
Operator : EI\SJ
Sample : K2200-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
EO-02-042319-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 07:54:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

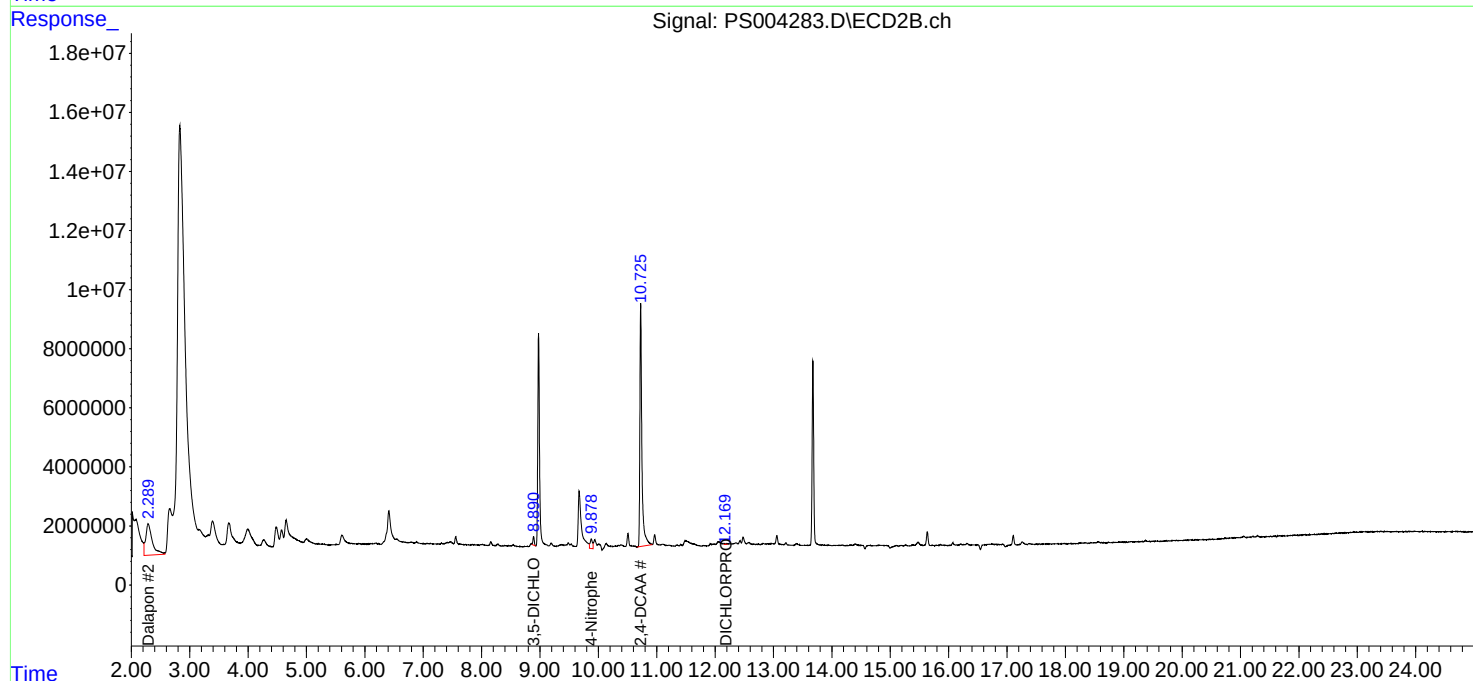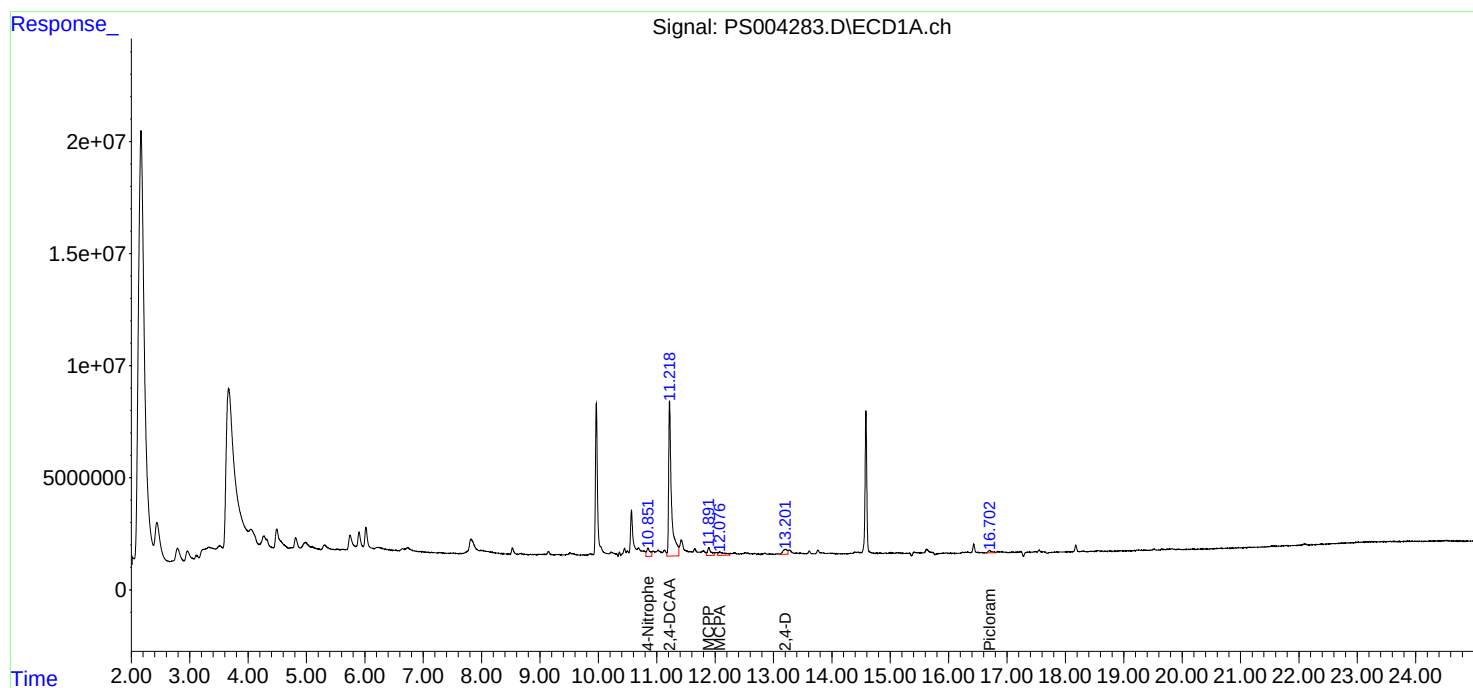


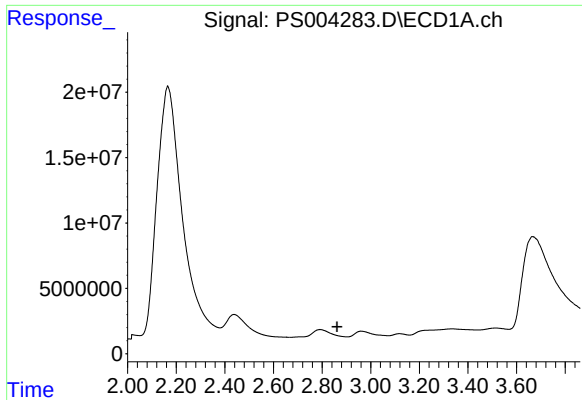

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.862 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-02-042319-C

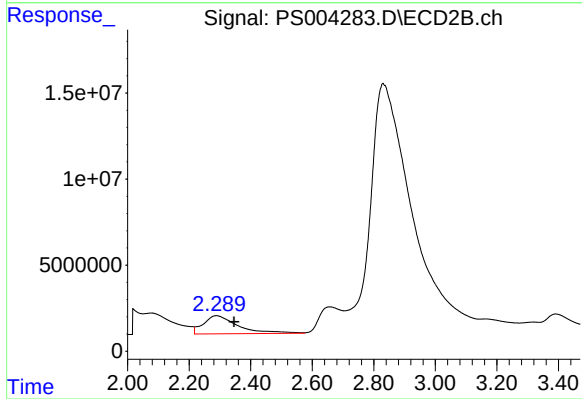


#1 Dalapon

R.T.: 2.289 min
Delta R.T.: -0.058 min
Response: 82471205
Conc: 131.23 ng/ml

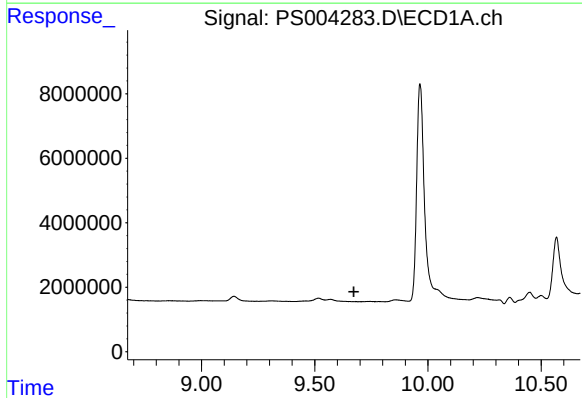


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.673 min
Response: 0
Conc: N.D.

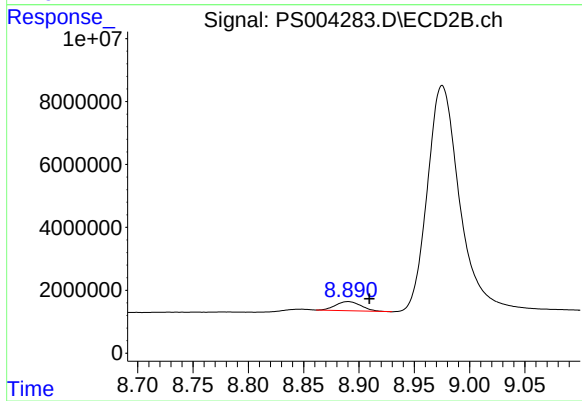

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.890 min
Delta R.T.: -0.019 min
Response: 4671105
Conc: 8.17 ng/ml

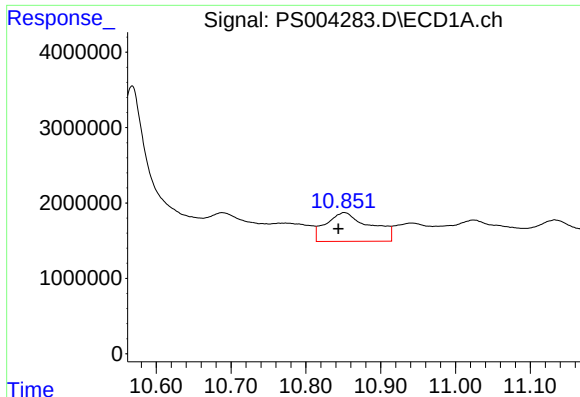

#3 4-Nitrophenol


R.T.: 10.851 min
Delta R.T.: 0.008 min
Response: 15684974
Conc: 62.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-02-042319-C

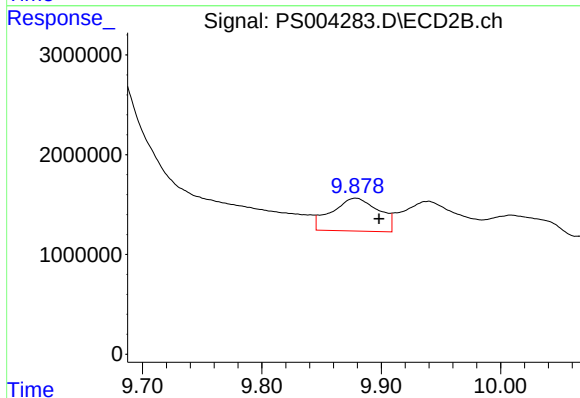


#3 4-Nitrophenol

R.T.: 9.878 min
Delta R.T.: -0.020 min
Response: 9004770
Conc: 37.55 ng/ml

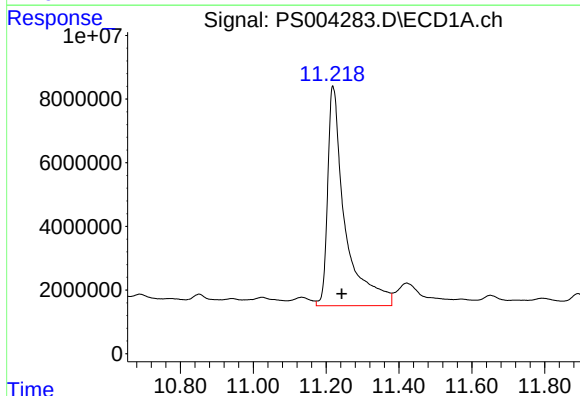


#4 2,4-DCAA

R.T.: 11.219 min
Delta R.T.: -0.024 min
Response: 228285913
Conc: 470.48 ng/ml

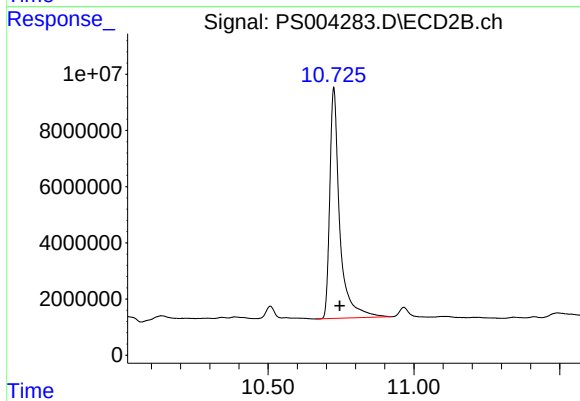

#4 2,4-DCAA


R.T.: 10.725 min
Delta R.T.: -0.020 min
Response: 195044884
Conc: 424.71 ng/ml

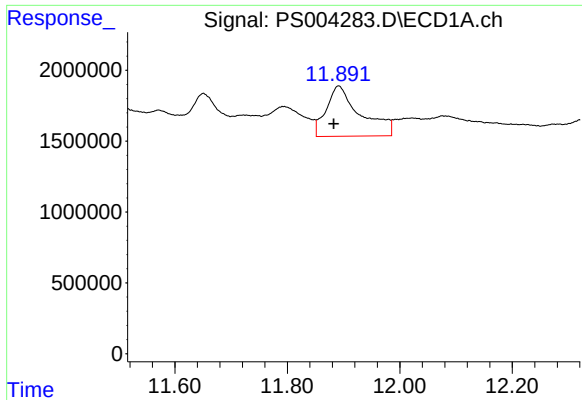

#6 MCPP


R.T.: 11.891 min
Delta R.T.: 0.009 min
Response: 14953475
Conc: 11.45 ug/ml

Instrument :
ECD_S
ClientSampleId :
EO-02-042319-C

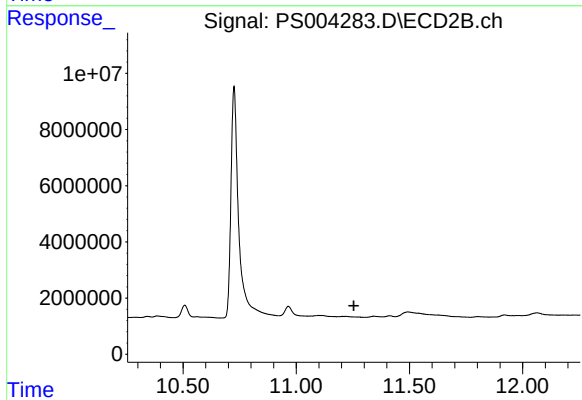


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.255 min
Response: 0
Conc: N.D.

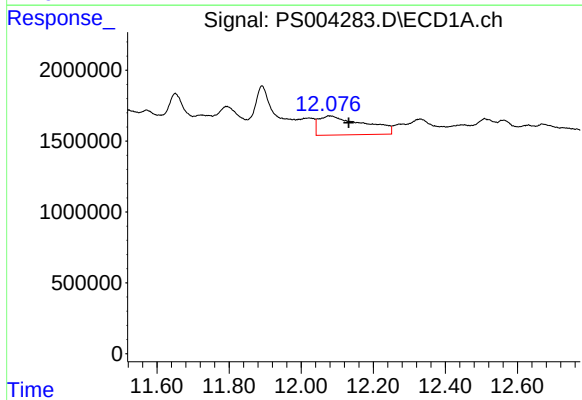


#7 MCPA

R.T.: 12.078 min
Delta R.T.: -0.054 min
Response: 11852539
Conc: 5.74 ug/ml

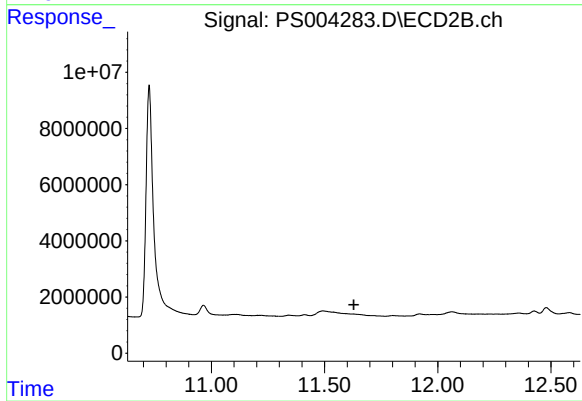

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 11.630 min
Response: 0
Conc: N.D.

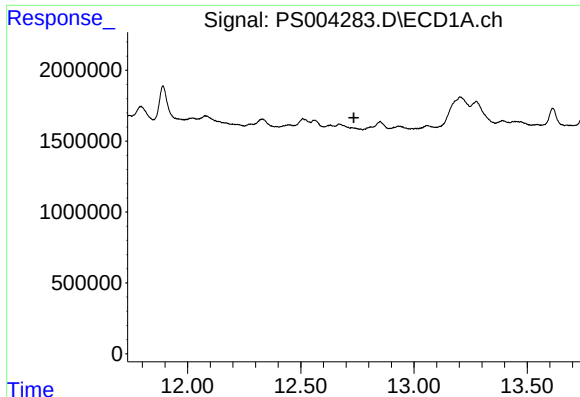

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.734 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-02-042319-C

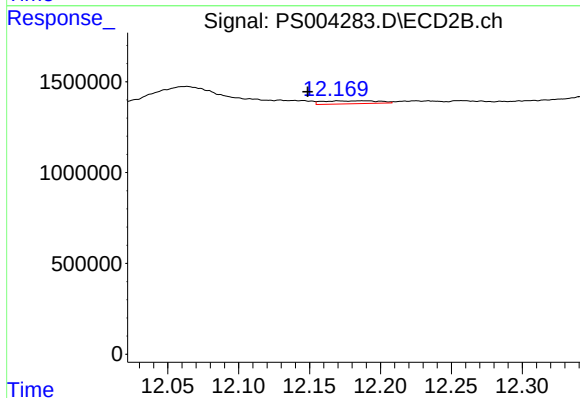


#8 DICHLORPROP

R.T.: 12.187 min
Delta R.T.: 0.039 min
Response: 446574
Conc: 1.05 ng/ml

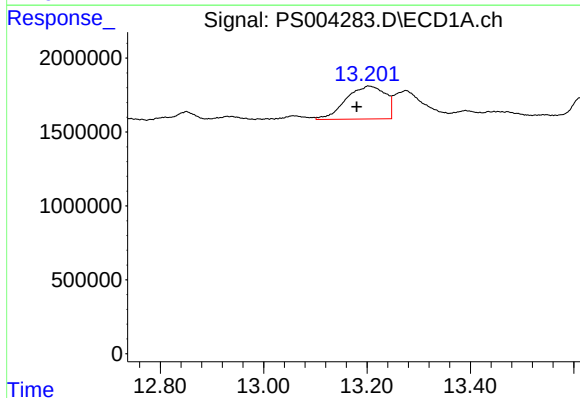


#9 2,4-D

R.T.: 13.203 min
Delta R.T.: 0.023 min
Response: 11820994
Conc: 25.96 ng/ml

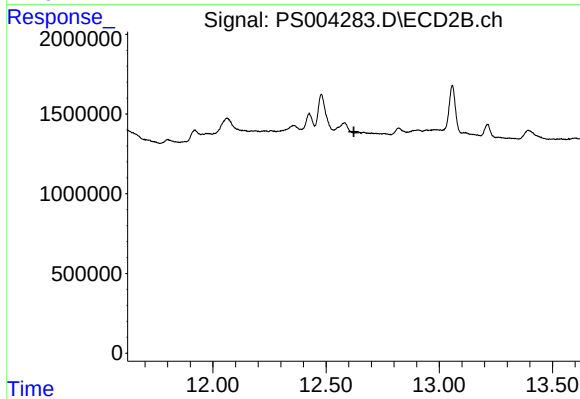

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 12.623 min
Response: 0
Conc: N.D.

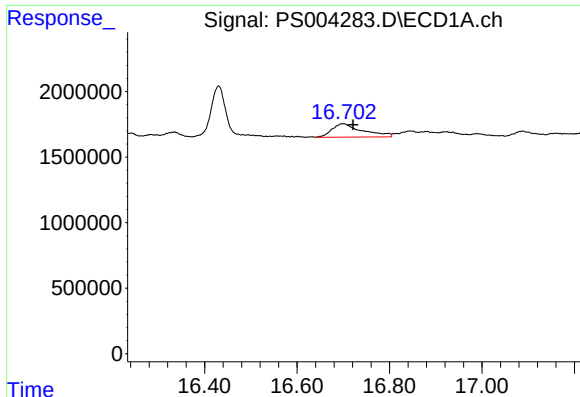

#15 Picloram

R.T.: 16.699 min
Delta R.T.: -0.022 min
Response: 4690418
Conc: 1.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-02-042319-C

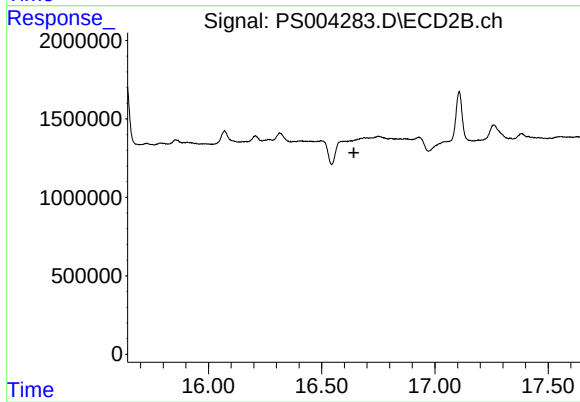

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.642 min
Response: 0
Conc: N.D.