

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042419\
 Data File : PS004291.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2019 09:26
 Operator : EI\SJ
 Sample : K2542-08
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 10:05:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:18:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.202	10.708	233.2E6	201.2E6	480.577	438.141
Target Compounds							
2) T	3,5-DICHL...	0.000	8.958	0	129.8E6	N.D.	227.123
3) T	4-Nitroph...	10.833	9.921	14128601	11081775	55.933	46.211
6) T	MCP	11.876	0.000	13048148	0	9.995	N.D. #
7) T	MCPA	12.070	0.000	5934652	0	2.876	N.D. #
9) T	2,4-D	0.000	12.562	0	392661	N.D.	<MDL
10) T	Pentachlo...	0.000	13.193	0	1200109	N.D.	<MDL
11) T	2,4,5-TP ...	14.376	0.000	2256797	0	<MDL	N.D. #
12) T	2,4,5-T	0.000	14.304	0	1152373	N.D.	<MDL
14) T	DINOSEB	16.910	15.464	1147654	3058570	<MDL	1.637 #
15) T	Picloram	16.691	16.670	6595755	8190880	1.839	2.393 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042419\
Data File : PS004291.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2019 09:26
Operator : EI\SJ
Sample : K2542-08
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 10:05:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041119.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:18:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

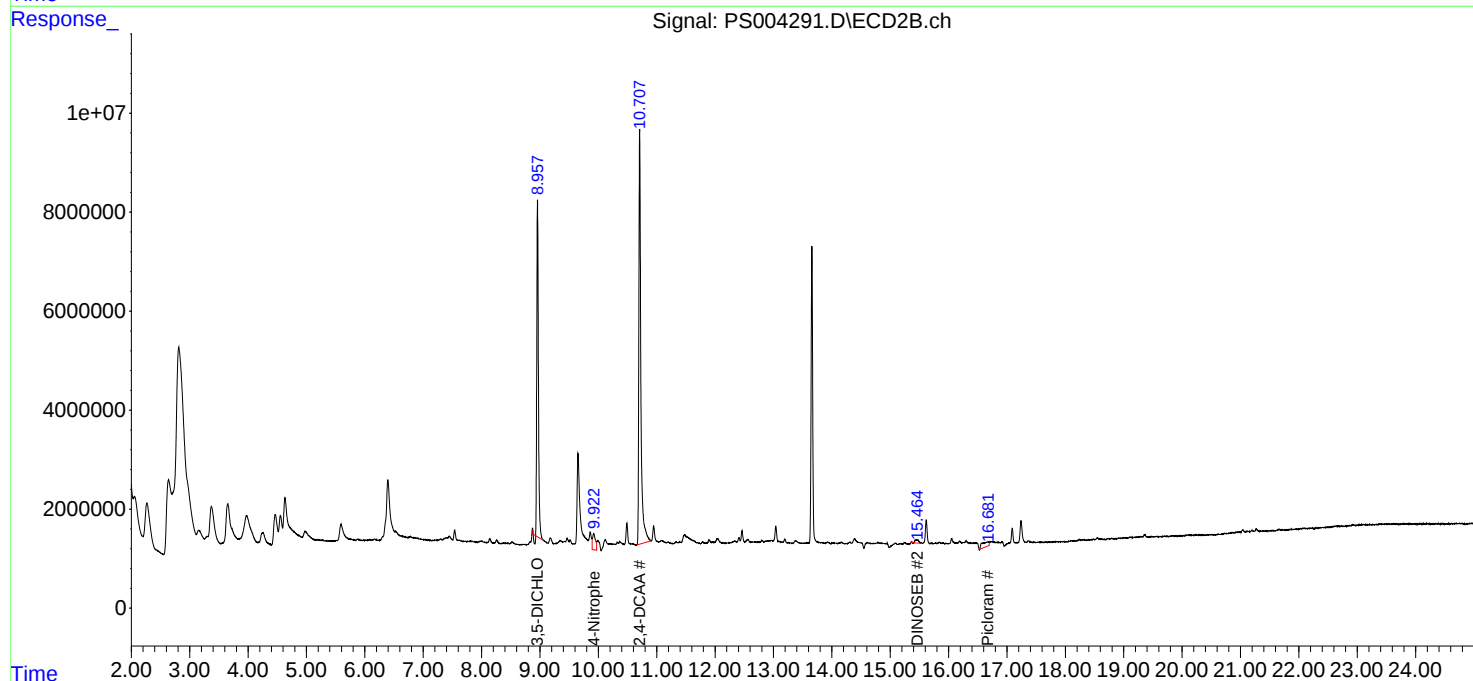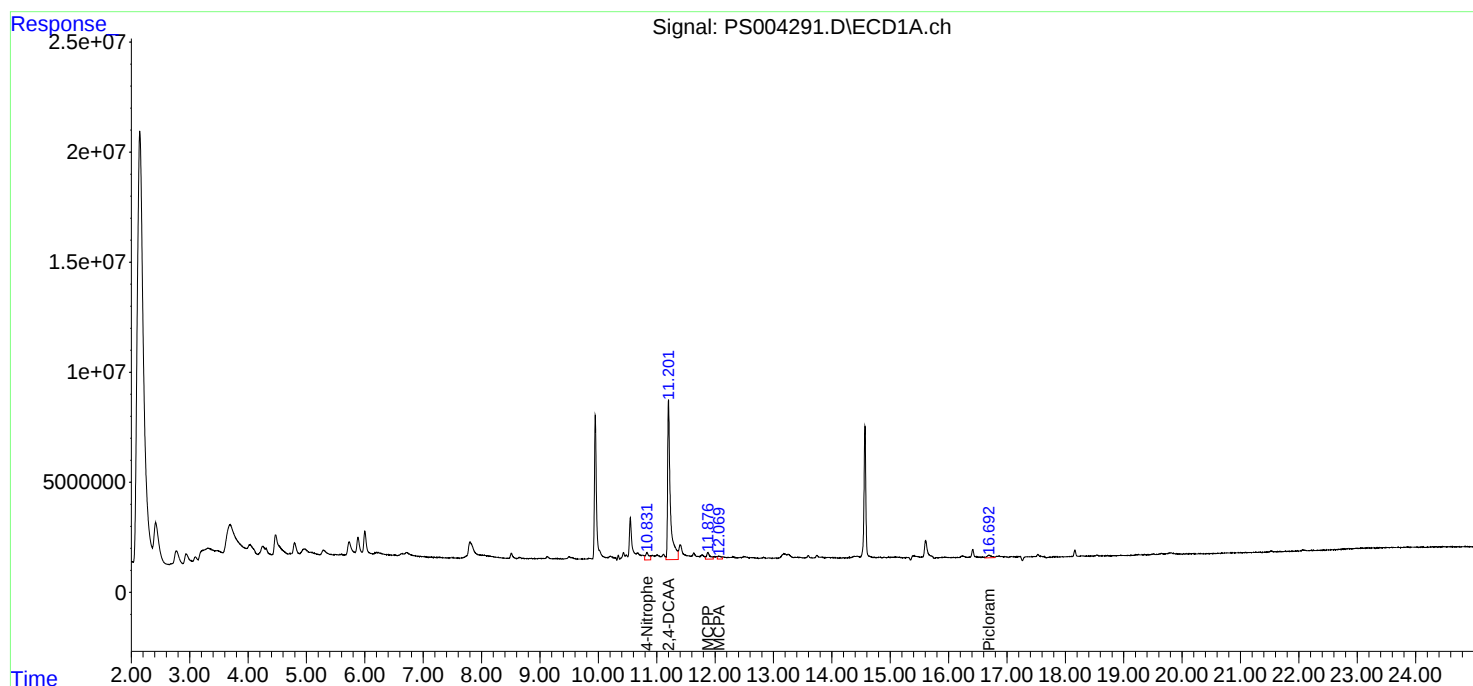


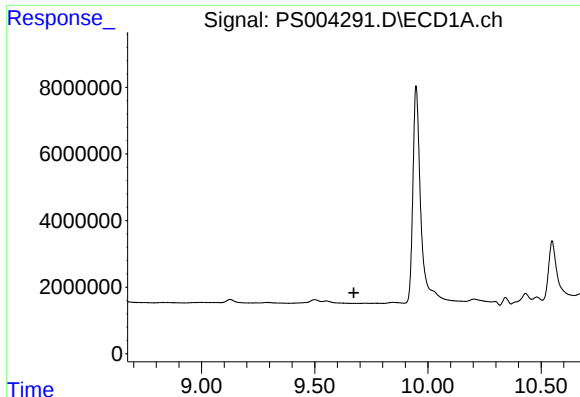

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.673 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-1

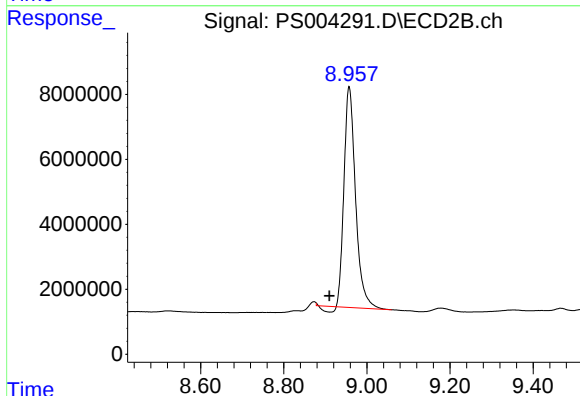


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.958 min
Delta R.T.: 0.048 min
Response: 129829468
Conc: 227.12 ng/ml

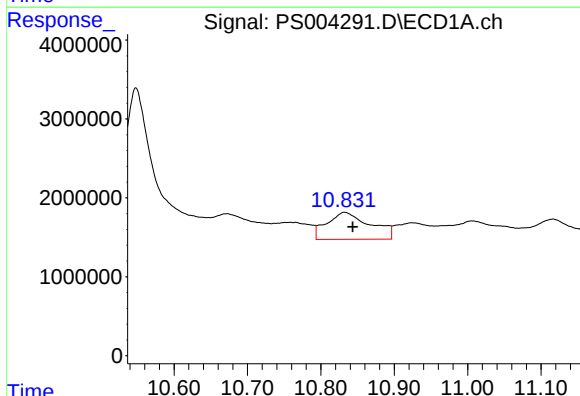


#3 4-Nitrophenol

R.T.: 10.833 min
Delta R.T.: -0.011 min
Response: 14128601
Conc: 55.93 ng/ml

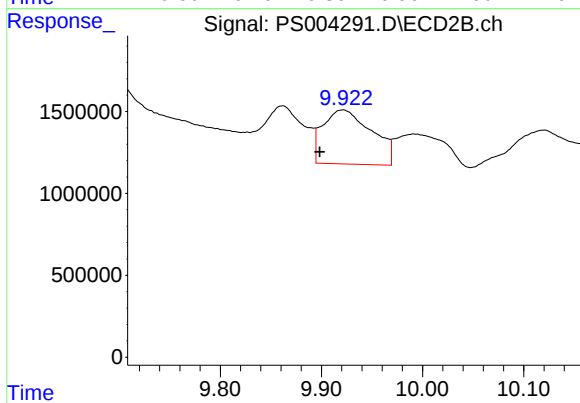

#3 4-Nitrophenol


R.T.: 9.921 min
Delta R.T.: 0.023 min
Response: 11081775
Conc: 46.21 ng/ml

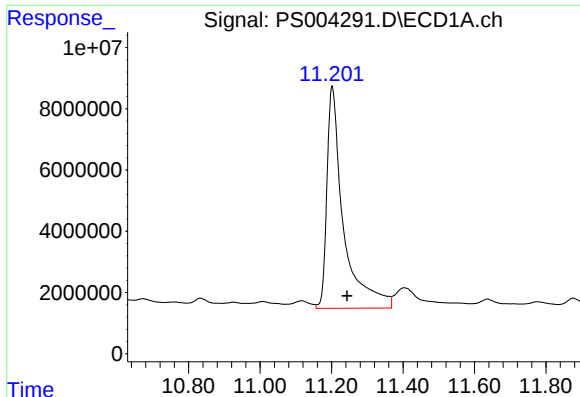

#4 2,4-DCAA


R.T.: 11.202 min
Delta R.T.: -0.041 min
Response: 233182935
Conc: 480.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1

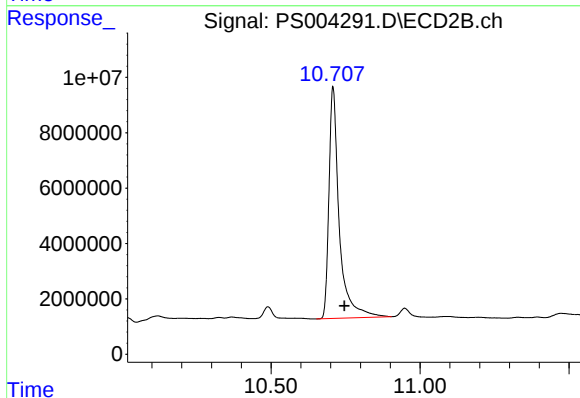


#4 2,4-DCAA

R.T.: 10.708 min
Delta R.T.: -0.038 min
Response: 201212748
Conc: 438.14 ng/ml

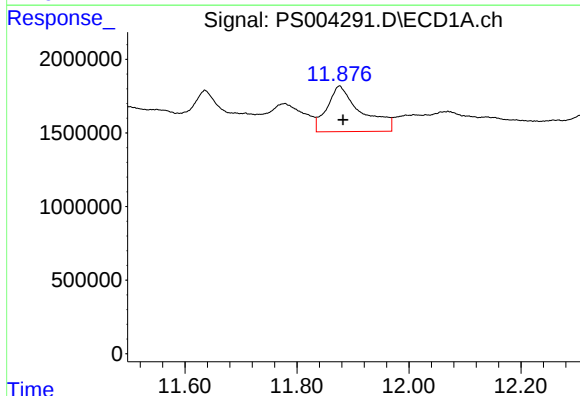


#6 MCP

R.T.: 11.876 min
Delta R.T.: -0.007 min
Response: 13048148
Conc: 10.00 ug/ml

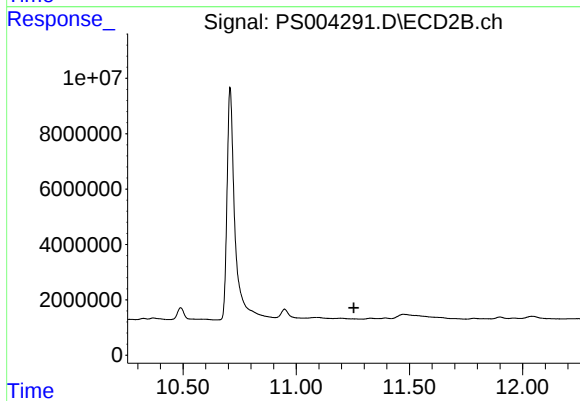

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.255 min
Response: 0
Conc: N.D.

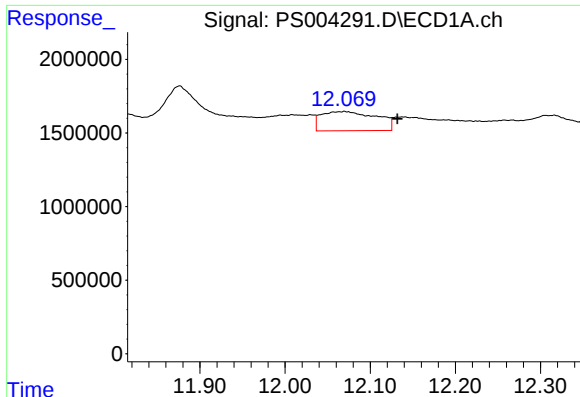

#7 MCPA


R.T.: 12.070 min
Delta R.T.: -0.063 min
Response: 5934652
Conc: 2.88 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-1

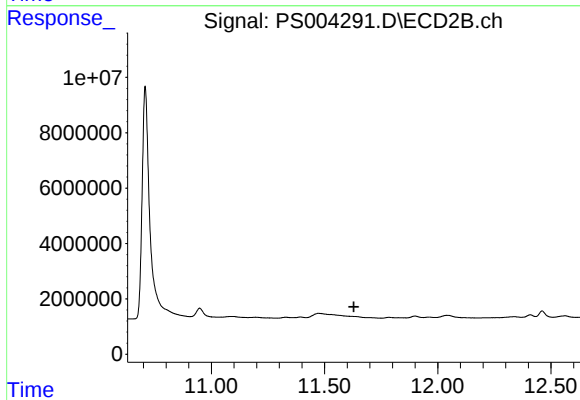


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.630 min
Response: 0
Conc: N.D.

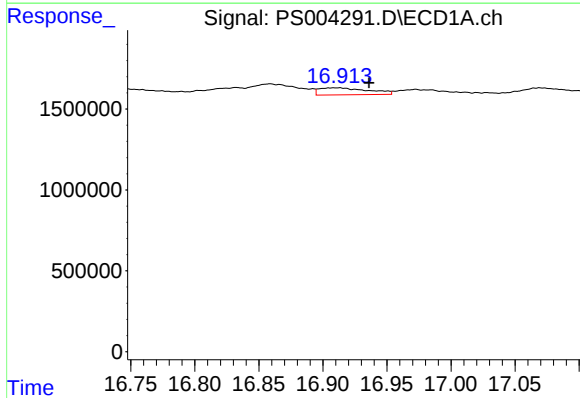


#14 DINOSEB

R.T.: 16.910 min
Delta R.T.: -0.027 min
Response: 1147654
Conc: N.D.

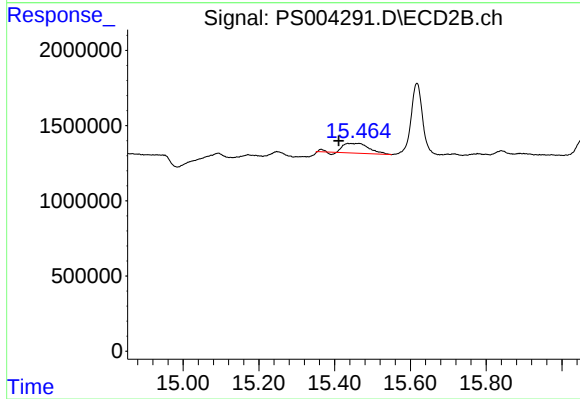

#14 DINOSEB


R.T.: 15.464 min
Delta R.T.: 0.053 min
Response: 3058570
Conc: 1.64 ng/ml

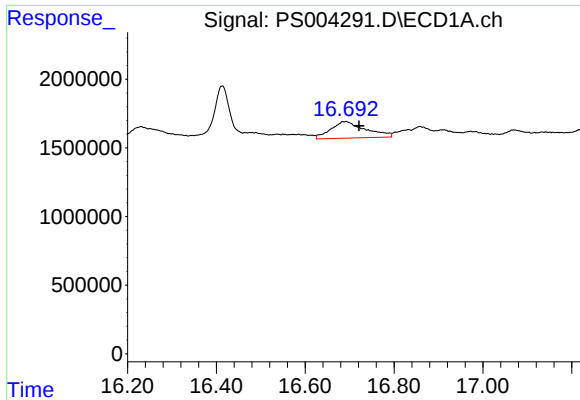

#15 Picloram

R.T.: 16.691 min
Delta R.T.: -0.030 min
Response: 6595755
Conc: 1.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1

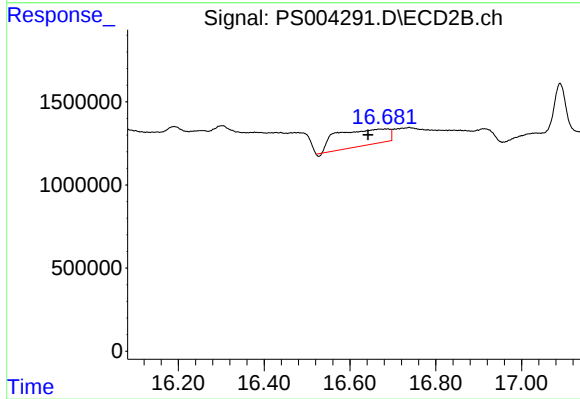

#15 Picloram

R.T.: 16.670 min
Delta R.T.: 0.028 min
Response: 8190880
Conc: 2.39 ng/ml