

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042622\
 Data File : PS019148.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2022 09:47
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 01:04:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 18 17:28:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.222	6.798	1281.3E6	355.3E6	342.598	489.460	#
Target Compounds								
12) T	2,4,5-T	9.477	0.000	12616505	0	<MDL	N.D.	#
15) T	Picloram	0.000	10.925f	0	6848930	N.D.	1.157	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042622\
Data File : PS019148.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2022 09:47
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 01:04:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
Quant Title : 8080.M
QLast Update : Mon Apr 18 17:28:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

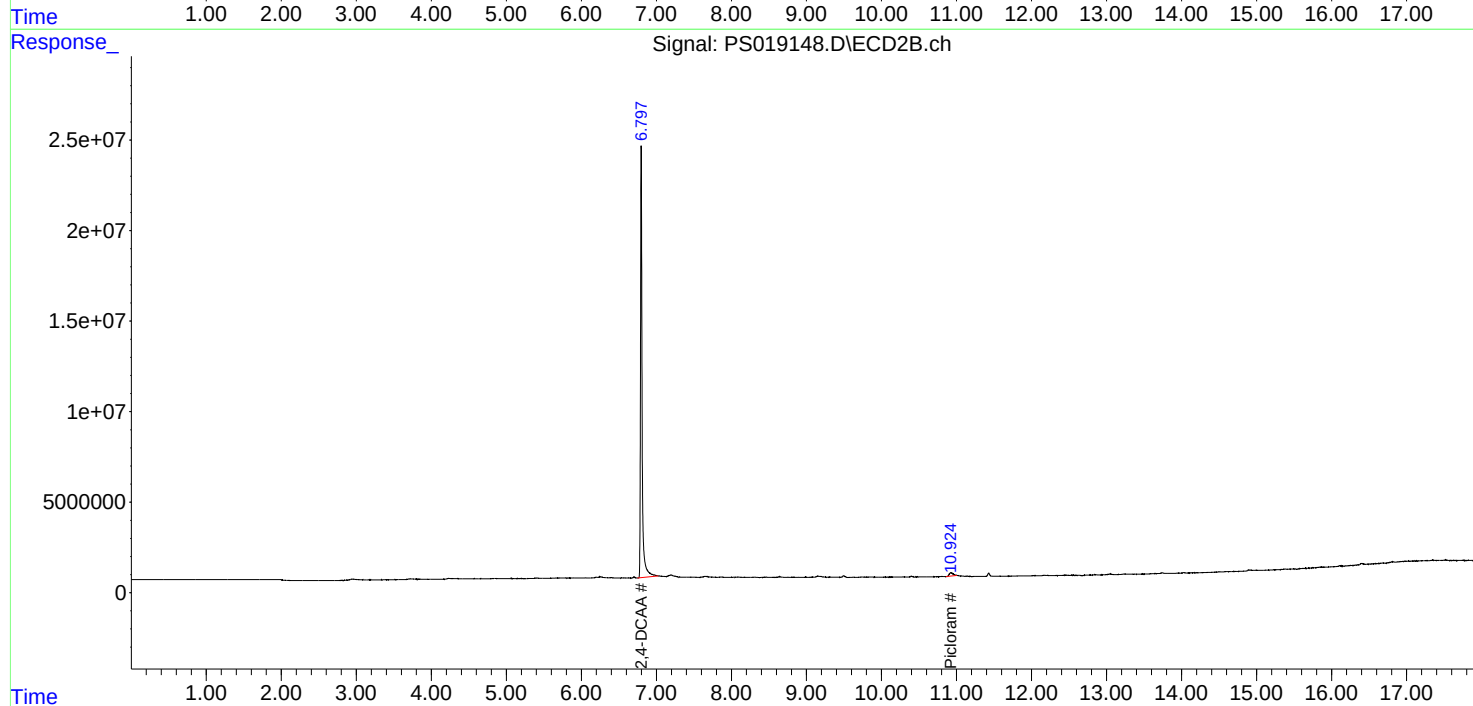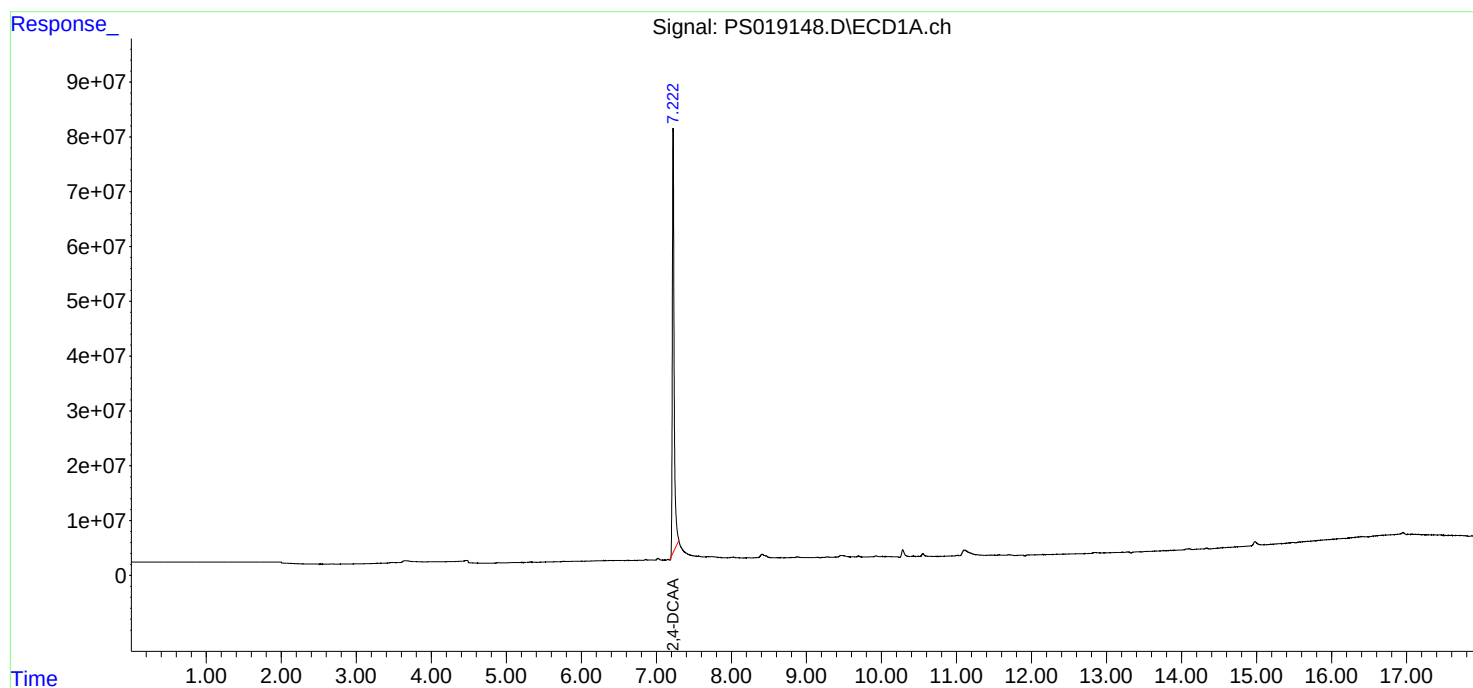


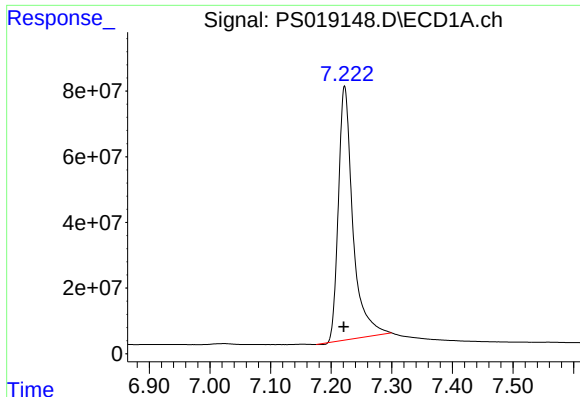

#4 2,4-DCAA


R.T.: 7.222 min
Delta R.T.: 0.001 min
Response: 1281334931
Conc: 342.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

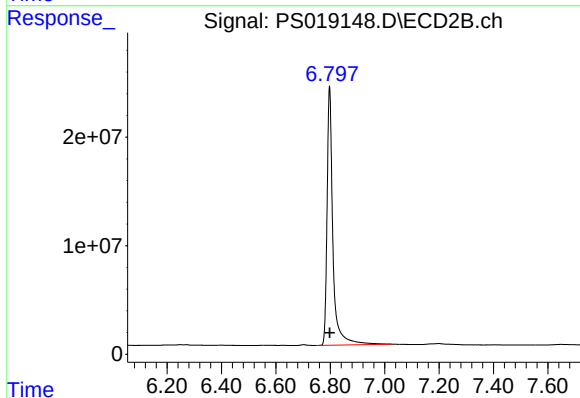


#4 2,4-DCAA

R.T.: 6.798 min
Delta R.T.: -0.001 min
Response: 355287775
Conc: 489.46 ng/ml

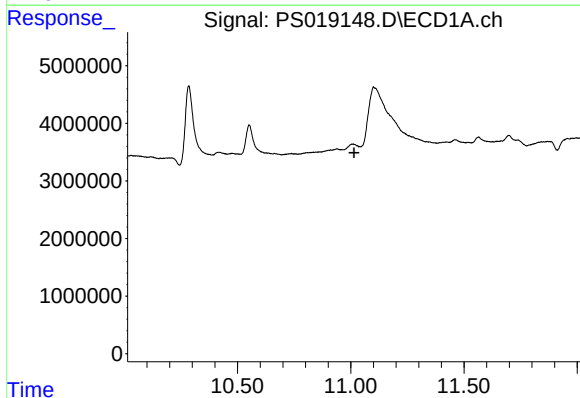

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.014 min
Response: 0
Conc: N.D.

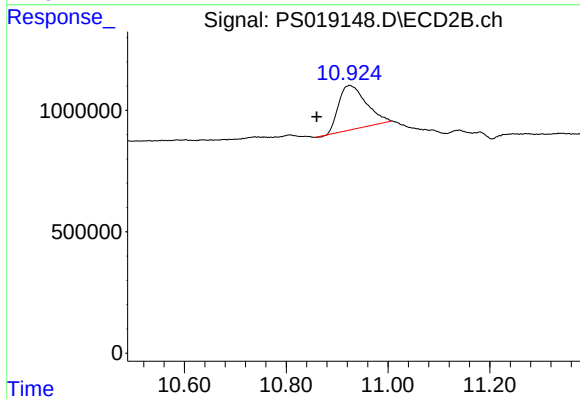

#15 Picloram

R.T.: 10.925 min
Delta R.T.: 0.065 min
Response: 6848930
Conc: 1.16 ng/ml