

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS043020\
 Data File : PS010071.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2020 08:52
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 10:28:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.235	6.921	280.3E6	260.3E6	464.216	525.598
Target Compounds							
5) T	DICAMBA	0.000	7.090	0	1207343	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.714	0	507471	N.D.	1.008
9) T	2,4-D	0.000	8.014	0	973657	N.D.	1.625
11) T	2,4,5-TP ...	0.000	8.802	0	2197893	N.D.	<MDL
12) T	2,4,5-T	0.000	9.183	0	3923702	N.D.	1.504
14) T	DINOSEB	0.000	10.023	0	1314855	N.D.	<MDL
15) T	Picloram	11.031	11.004	59055257	80765634	19.062	23.746
16) T	DCPA	0.000	10.951	0	3346723	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS043020\
Data File : PS010071.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2020 08:52
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 10:28:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

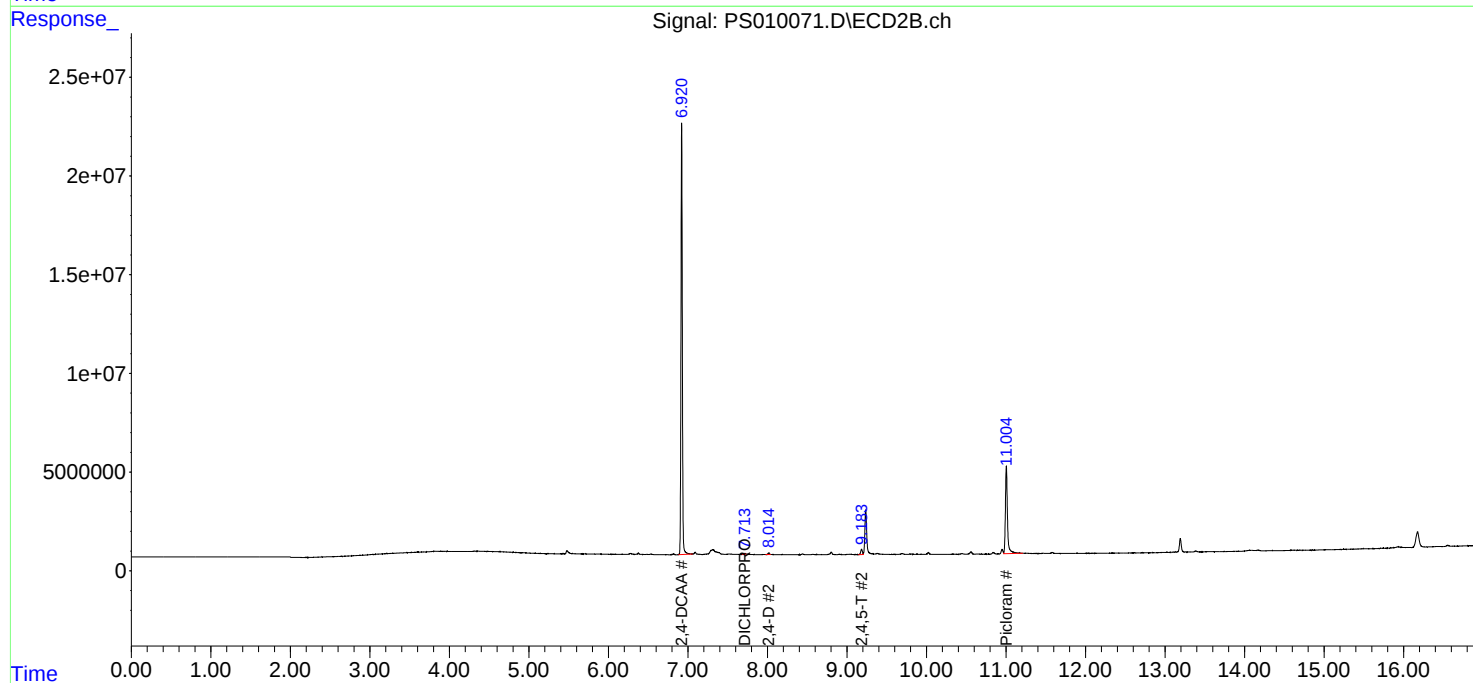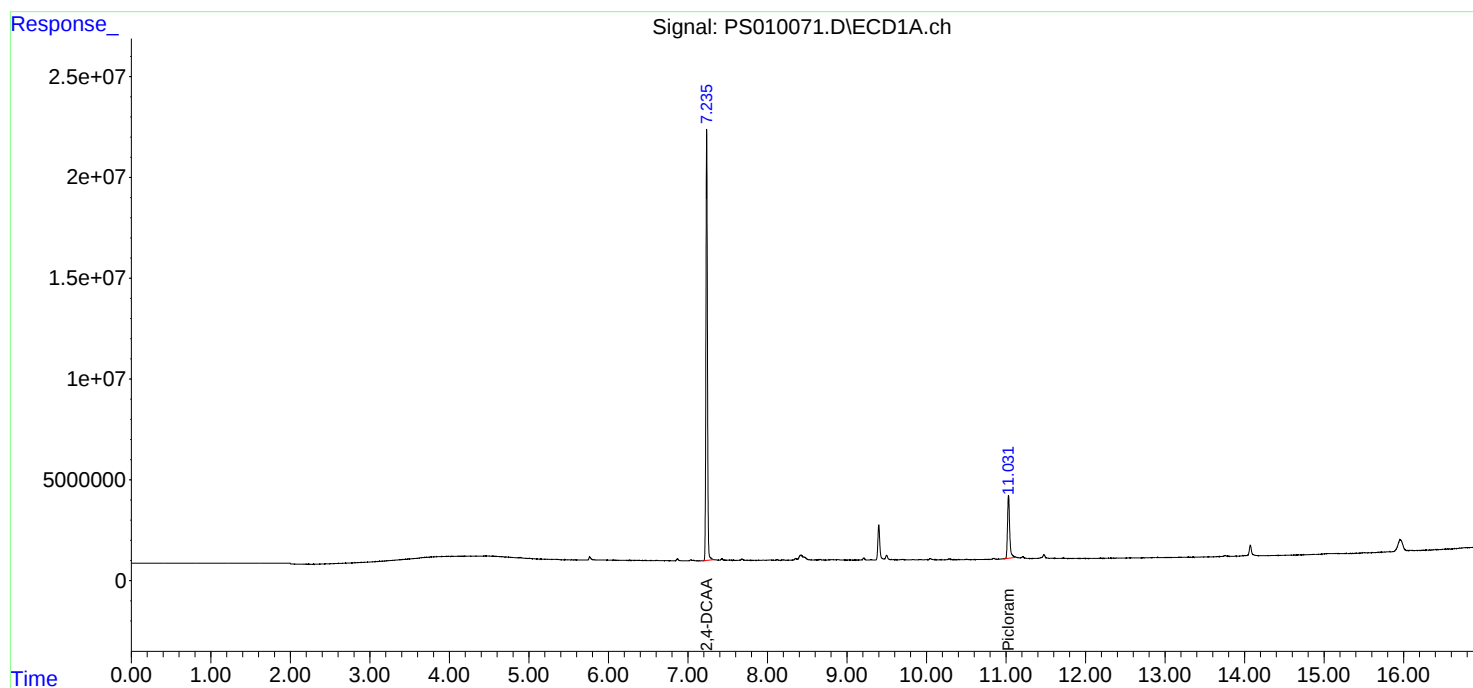


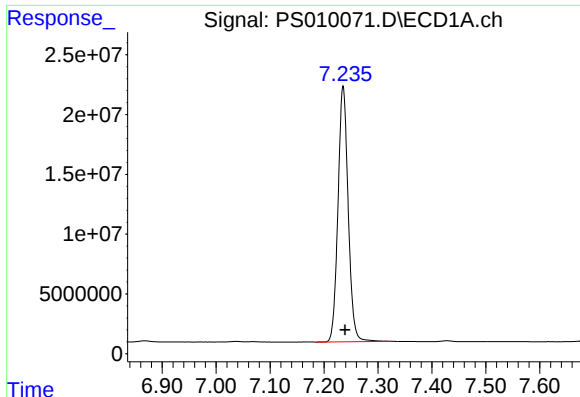

#4 2,4-DCAA


R.T.: 7.235 min
Delta R.T.: -0.004 min
Response: 280300971
Conc: 464.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

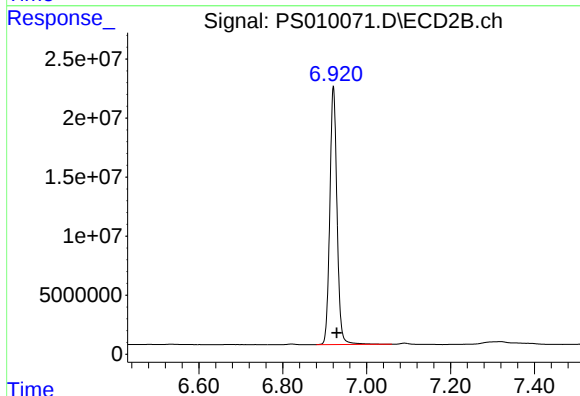


#4 2,4-DCAA

R.T.: 6.921 min
Delta R.T.: -0.007 min
Response: 260302183
Conc: 525.60 ng/ml

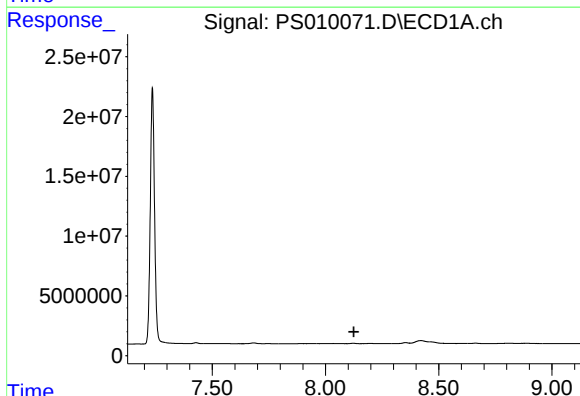


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.125 min
Response: 0
Conc: N.D.

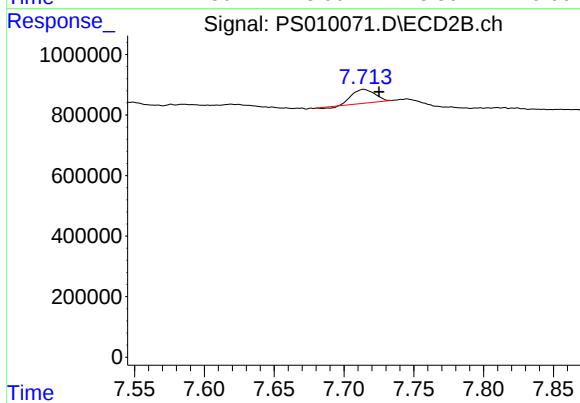

#8 DICHLORPROP


R.T.: 7.714 min
Delta R.T.: -0.011 min
Response: 507471
Conc: 1.01 ng/ml

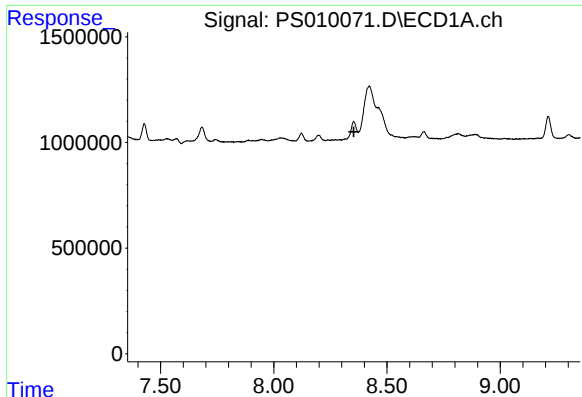

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.354 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

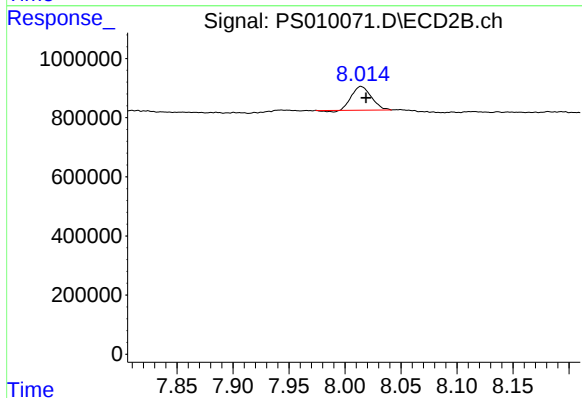


#9 2,4-D

R.T.: 8.014 min
Delta R.T.: -0.004 min
Response: 973657
Conc: 1.62 ng/ml

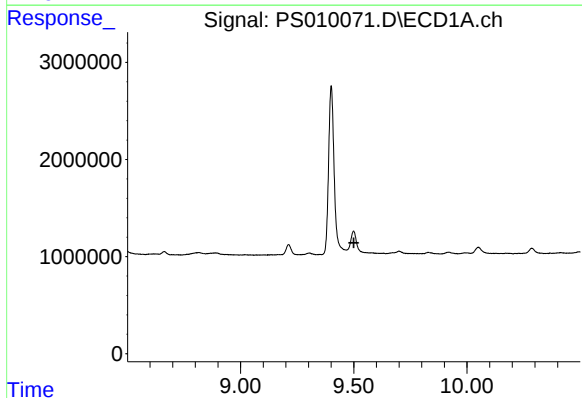


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.501 min
Response: 0
Conc: N.D.

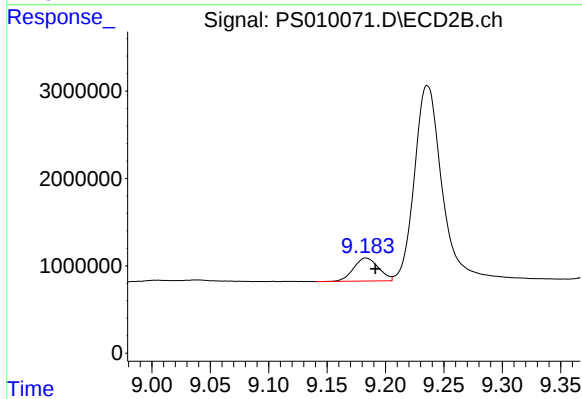

#12 2,4,5-T


R.T.: 9.183 min
Delta R.T.: -0.008 min
Response: 3923702
Conc: 1.50 ng/ml

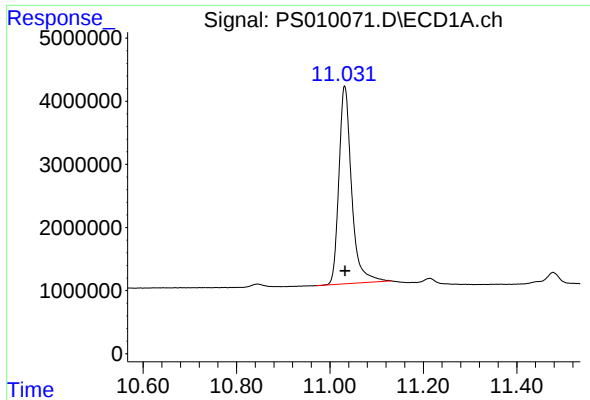

#15 Picloram

R.T.: 11.031 min
Delta R.T.: -0.001 min
Response: 59055257
Conc: 19.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

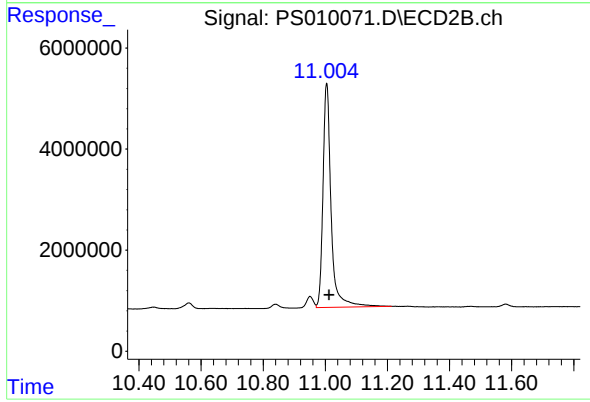

#15 Picloram

R.T.: 11.004 min
Delta R.T.: -0.008 min
Response: 80765634
Conc: 23.75 ng/ml