

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS043020\
 Data File : PS010083.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2020 14:11
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 14:47:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.235	6.922	290.9E6	273.5E6	481.852	552.202
Target Compounds							
2) T	3,5-DICHL...	0.000	6.074	0	351961	N.D.	<MDL
5) T	DICAMBA	0.000	7.091	0	2512583	N.D.	1.263
8) T	DICHLORPROP	0.000	7.718	0	337832	N.D.	<MDL
9) T	2,4-D	0.000	8.015	0	927135	N.D.	1.547
10) T	Pentachlo...	0.000	8.442	0	4626848	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.803	0	3781752	N.D.	1.446
12) T	2,4,5-T	0.000	9.185	0	3872583	N.D.	1.484
15) T	Picloram	0.000	11.007	0	9143662	N.D.	2.688
16) T	DCPA	0.000	10.951	0	5099775	N.D.	1.521



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS043020\
Data File : PS010083.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2020 14:11
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 14:47:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

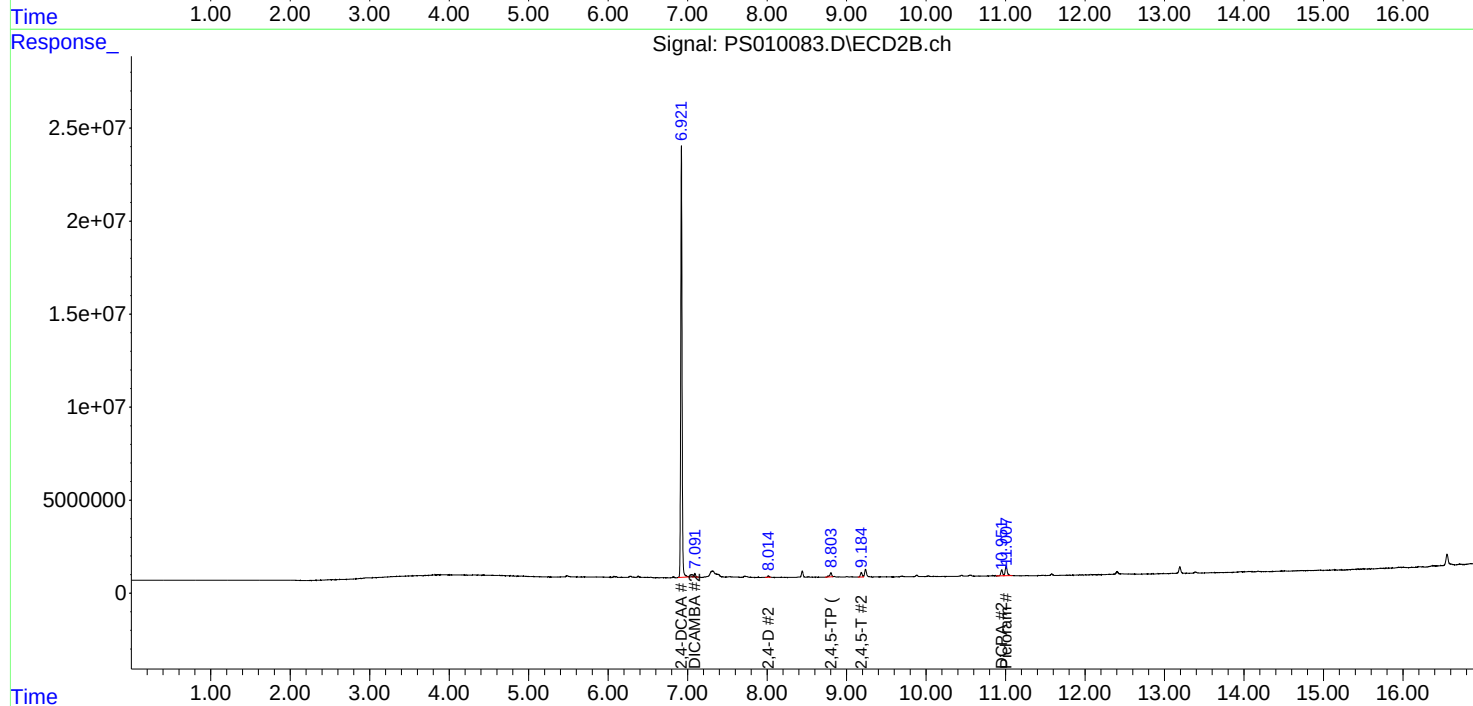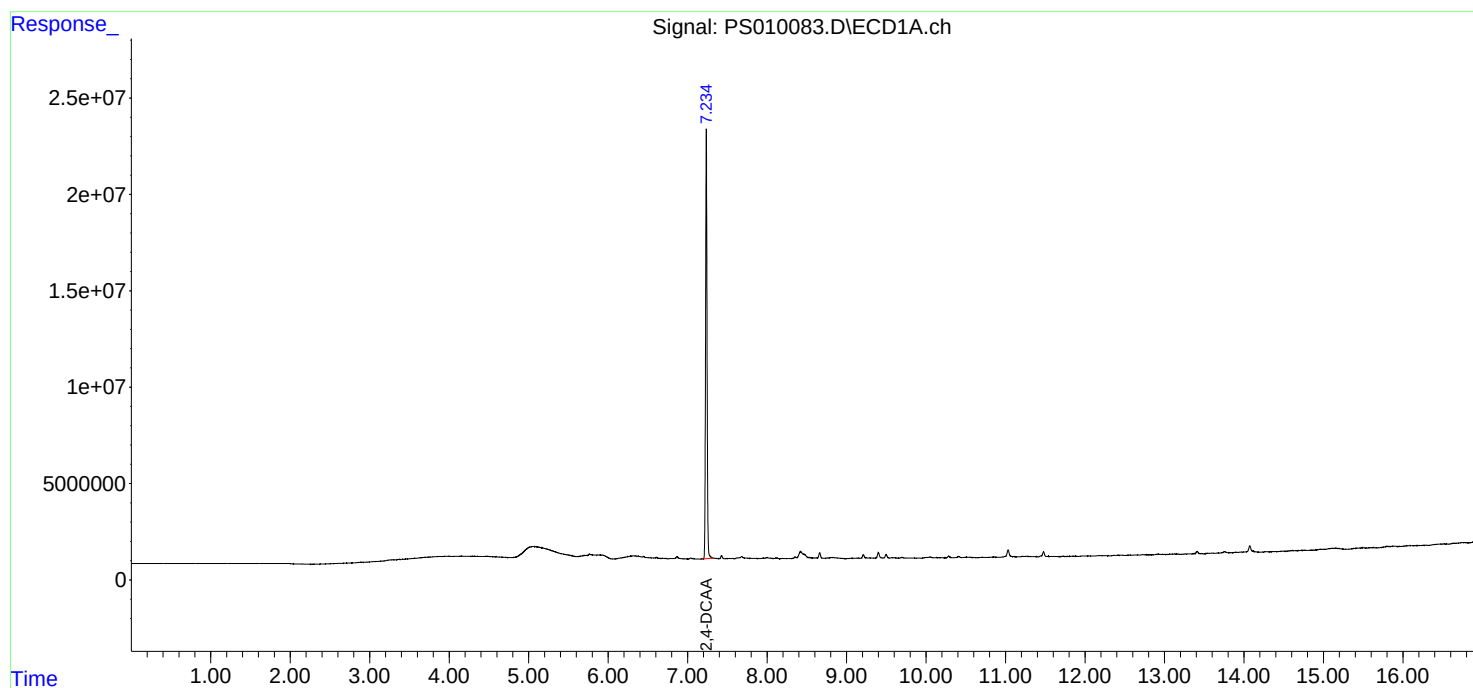


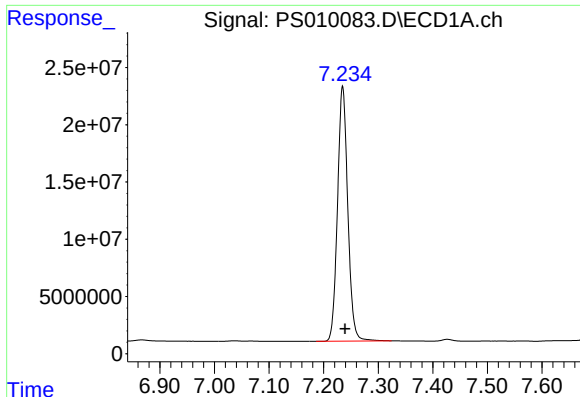

#4 2,4-DCAA


R.T.: 7.235 min
Delta R.T.: -0.004 min
Response: 290949596
Conc: 481.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

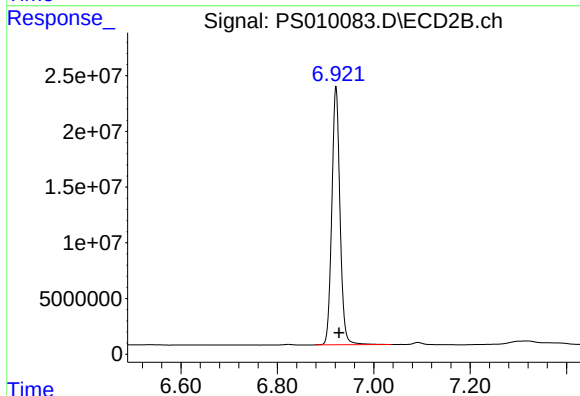


#4 2,4-DCAA

R.T.: 6.922 min
Delta R.T.: -0.007 min
Response: 273478169
Conc: 552.20 ng/ml

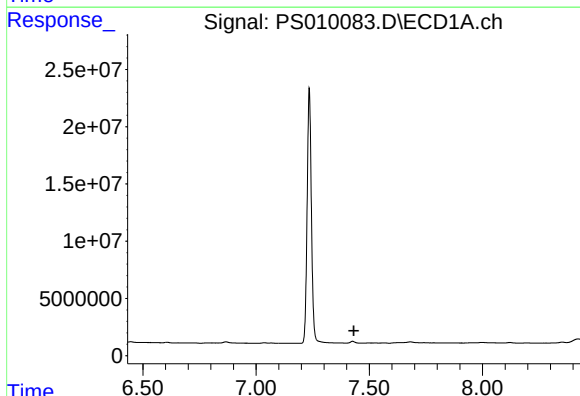


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.432 min
Response: 0
Conc: N.D.

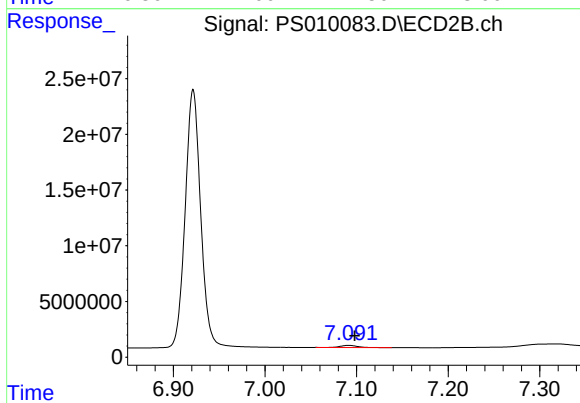

#5 DICAMBA


R.T.: 7.091 min
Delta R.T.: -0.007 min
Response: 2512583
Conc: 1.26 ng/ml

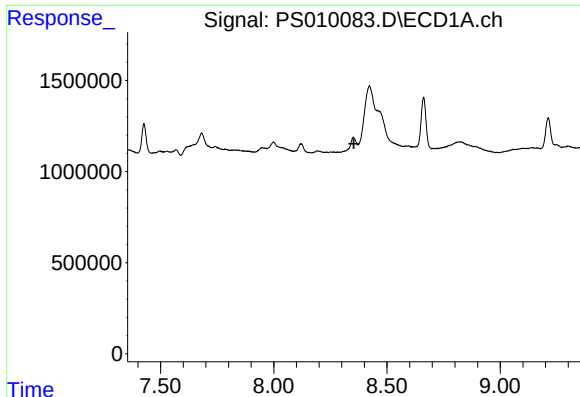

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.354 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

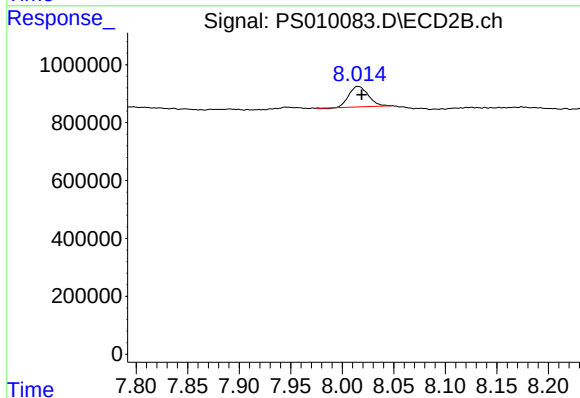


#9 2,4-D

R.T.: 8.015 min
Delta R.T.: -0.003 min
Response: 927135
Conc: 1.55 ng/ml

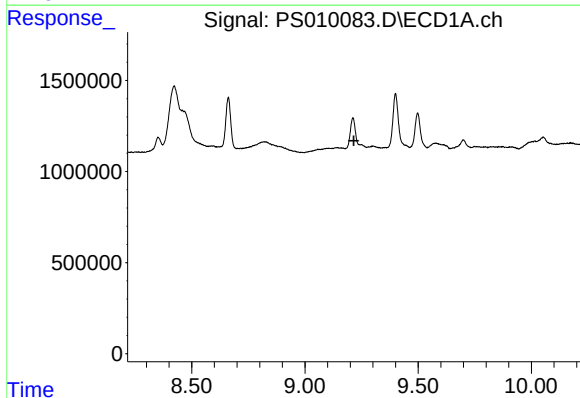


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.216 min
Response: 0
Conc: N.D.

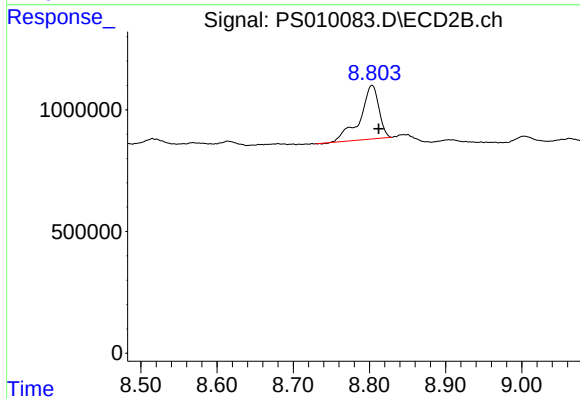

#11 2,4,5-TP (SILVEX)


R.T.: 8.803 min
Delta R.T.: -0.009 min
Response: 3781752
Conc: 1.45 ng/ml

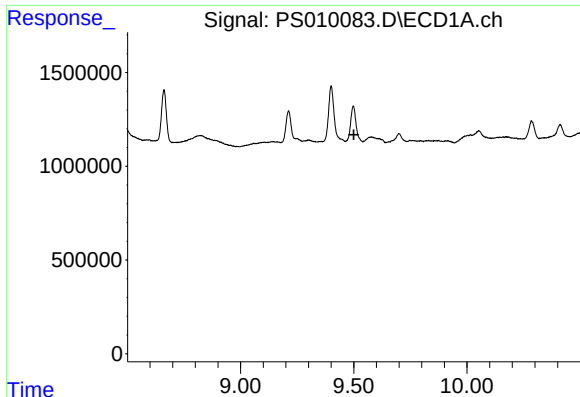

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

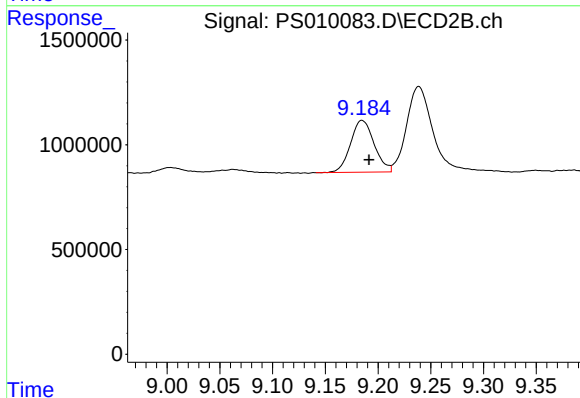


#12 2,4,5-T

R.T.: 9.185 min
Delta R.T.: -0.007 min
Response: 3872583
Conc: 1.48 ng/ml

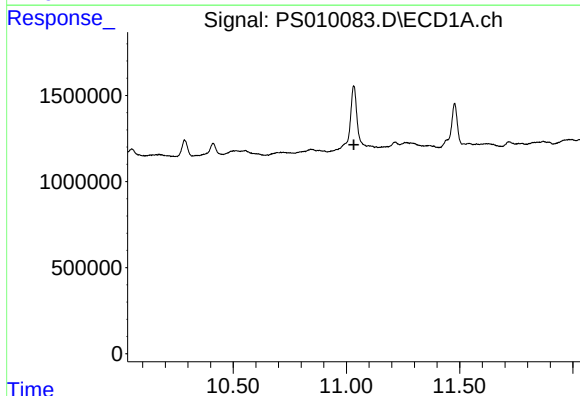


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.033 min
Response: 0
Conc: N.D.

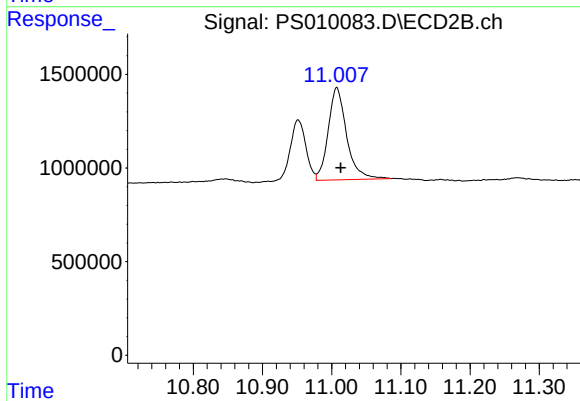

#15 Picloram


R.T.: 11.007 min
Delta R.T.: -0.006 min
Response: 9143662
Conc: 2.69 ng/ml

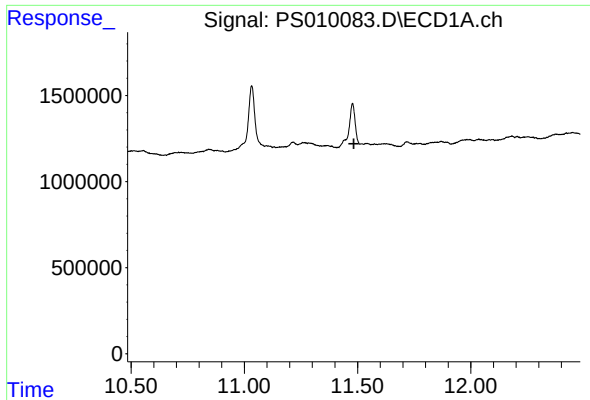

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

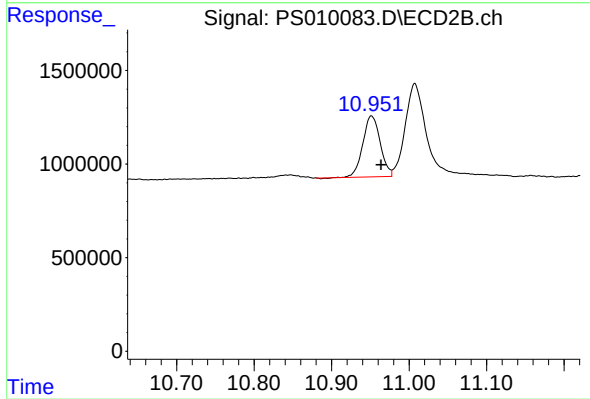

#16 DCPA

R.T.: 10.951 min
Delta R.T.: -0.012 min
Response: 5099775
Conc: 1.52 ng/ml