

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052019\
 Data File : PS004655.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2019 15:50
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 04:56:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) T	3,5-DICHL...	4.947	0.000	192.1E6	0	111.367	N.D.	#
5) T	DICAMBA	0.000	5.442	0	207.1E6	N.D.	56.055	
6) T	MCP	0.000	5.579	0	95119455	N.D.	34.715	
9) T	2,4-D	6.627	0.000	477.2E6	0	348.852	N.D.	#
12) T	2,4,5-T	0.000	7.404	0	38976780	N.D.	8.746	
15) T	Picloram	9.176	9.110	97834371	88646957	9.389	11.882	#
16) T	DCPA	0.000	9.110	0	88646957	N.D.	13.684	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052019\
Data File : PS004655.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2019 15:50
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 04:56:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

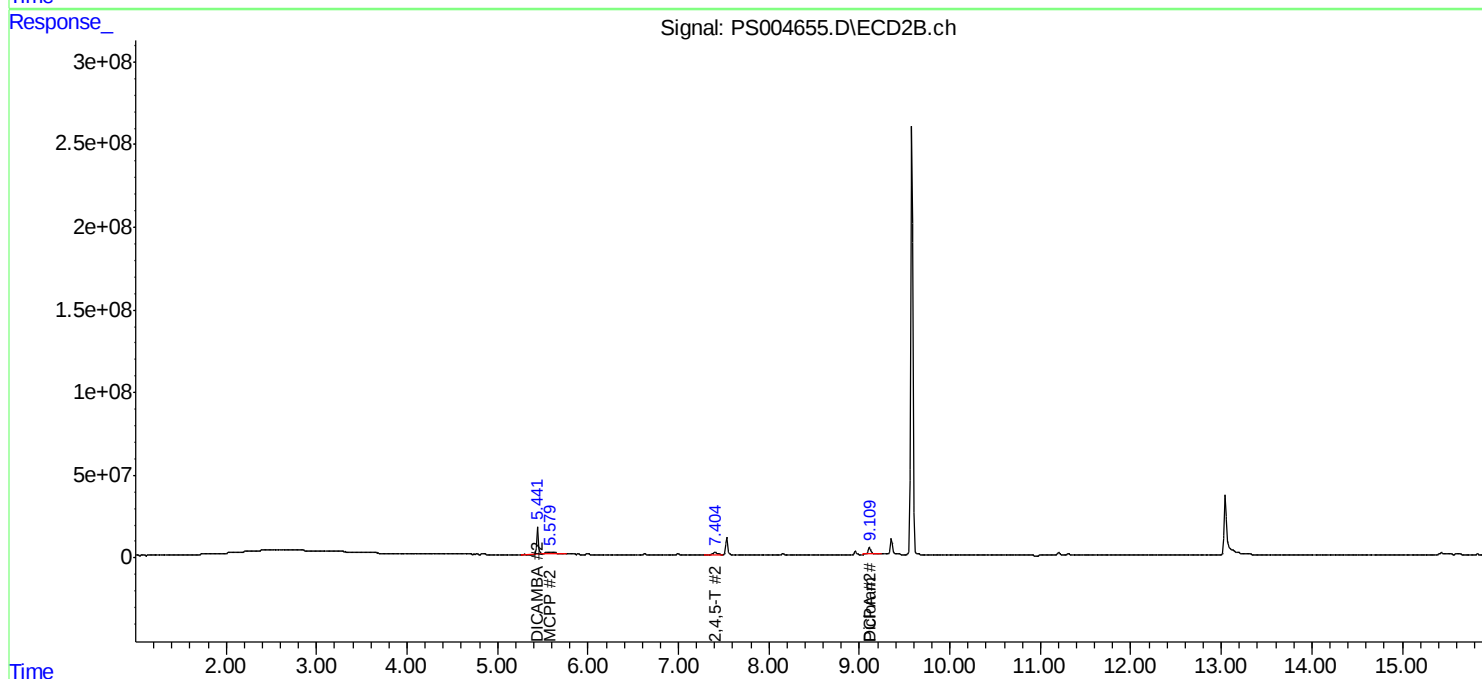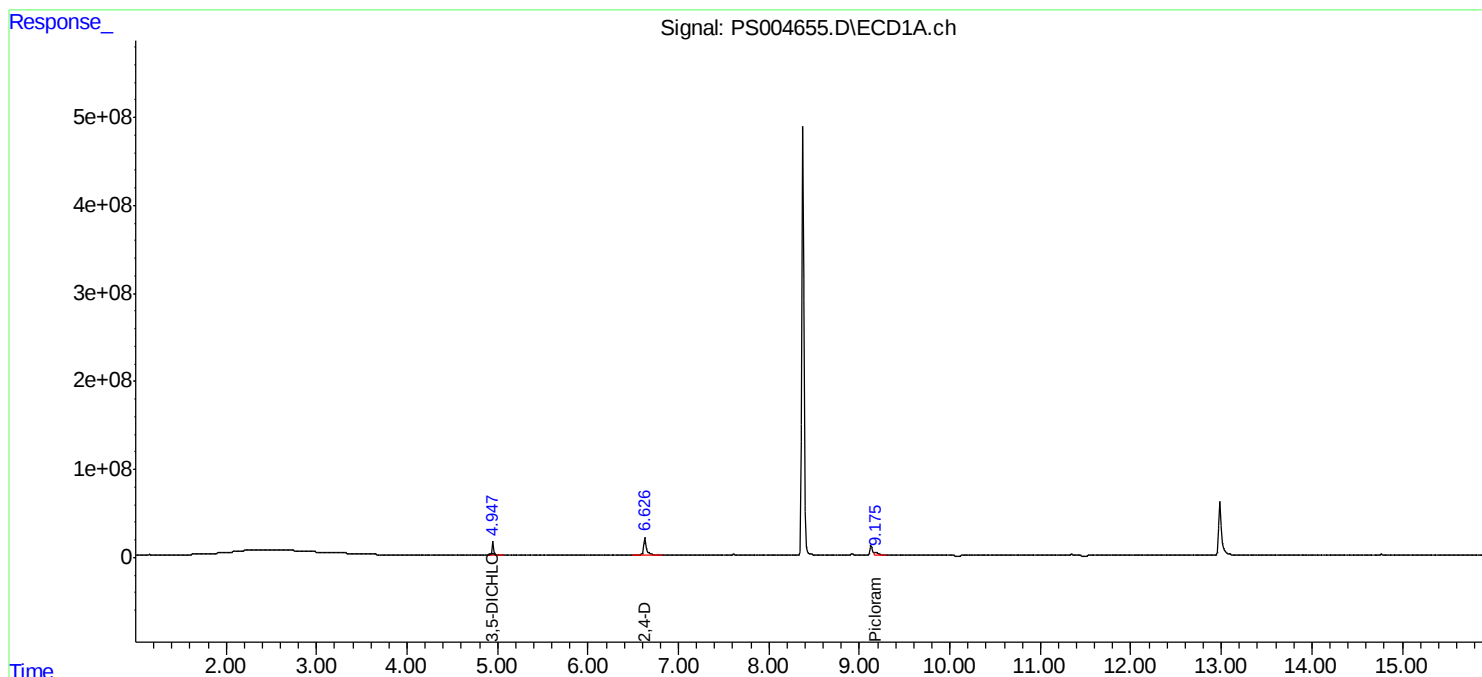


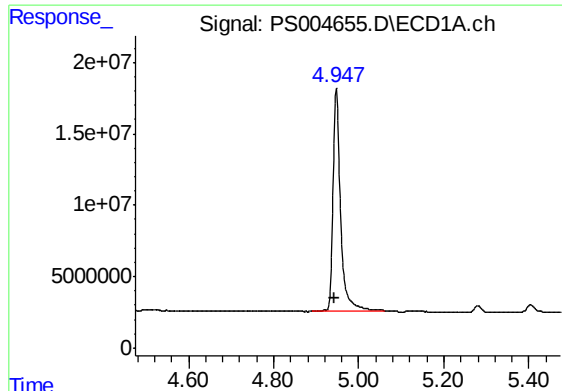

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.947 min
Delta R.T.: 0.005 min
Response: 192061041
Conc: 111.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

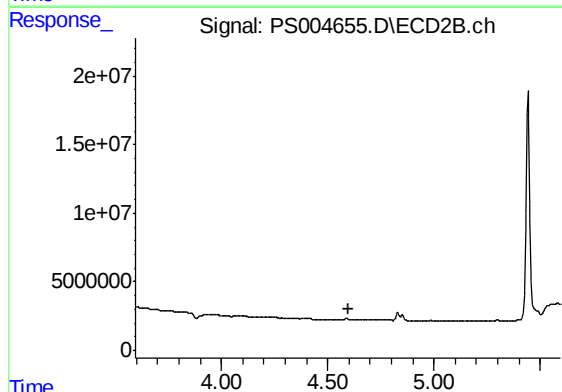


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.596 min
Response: 0
Conc: N.D.

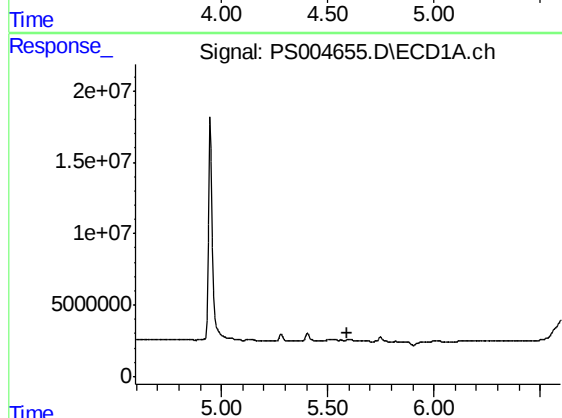


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.595 min
Response: 0
Conc: N.D.

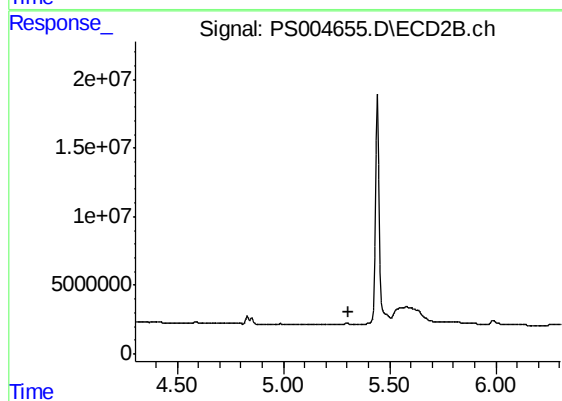

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.304 min
Response: 0
Conc: N.D.

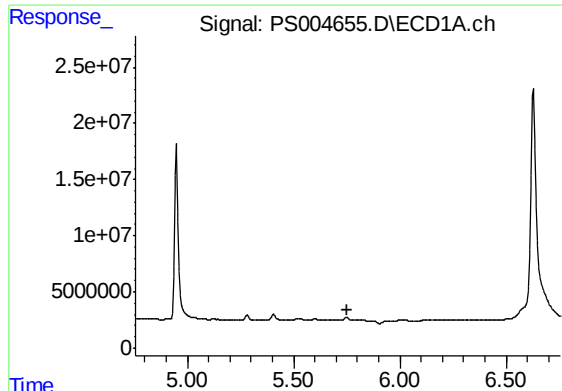

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

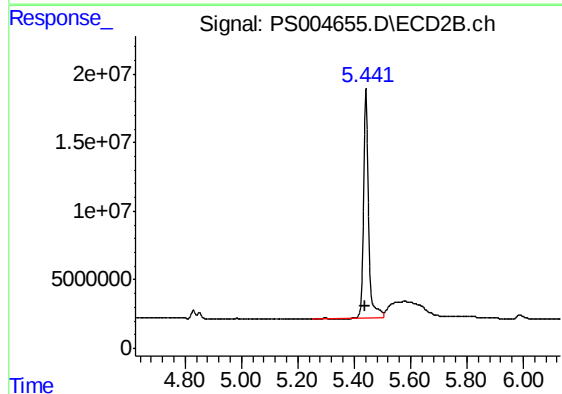


#5 DICAMBA

R.T.: 5.442 min
Delta R.T.: 0.005 min
Response: 207080706
Conc: 56.06 ng/ml

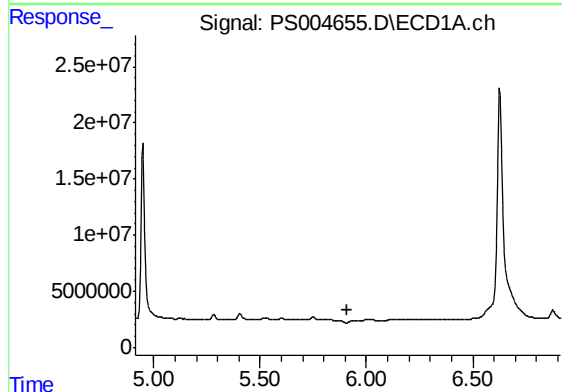


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 5.913 min
Response: 0
Conc: N.D.

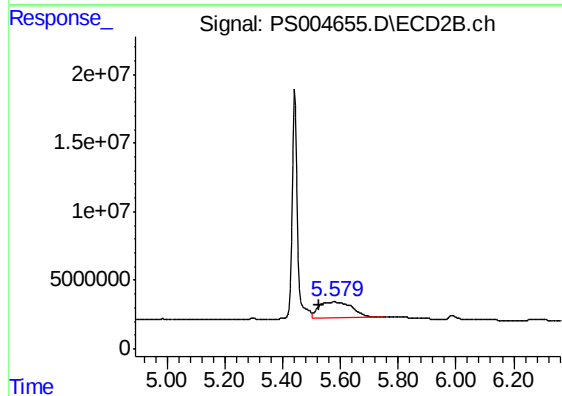

#6 MCPP


R.T.: 5.579 min
Delta R.T.: 0.054 min
Response: 95119455
Conc: 34.72 ug/ml

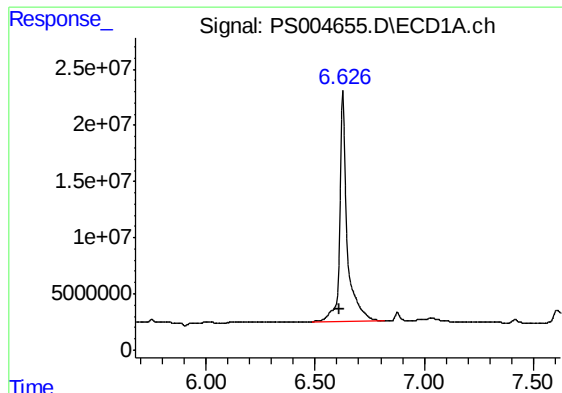

#9 2,4-D


R.T.: 6.627 min
Delta R.T.: 0.015 min
Response: 477197860
Conc: 348.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

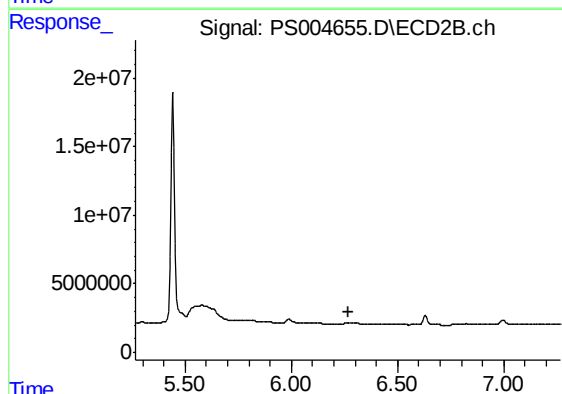


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

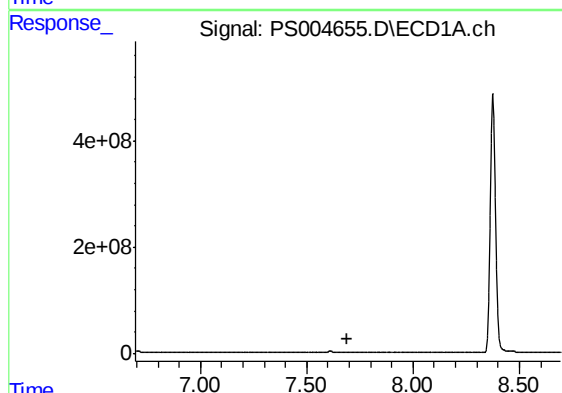


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.693 min
Response: 0
Conc: N.D.

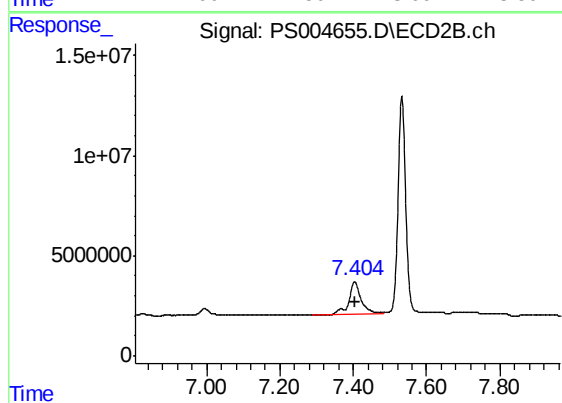

#12 2,4,5-T


R.T.: 7.404 min
Delta R.T.: 0.000 min
Response: 38976780
Conc: 8.75 ng/ml

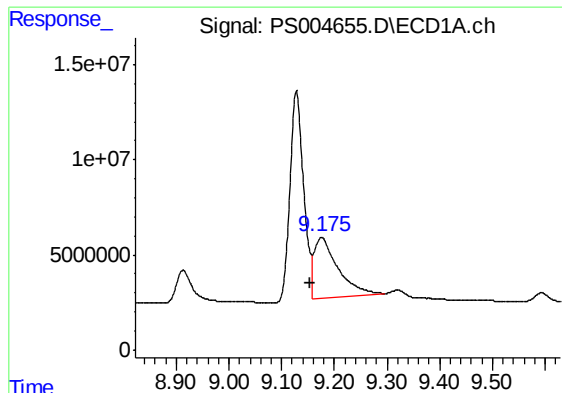

#15 Picloram


R.T.: 9.176 min
Delta R.T.: 0.020 min
Response: 97834371
Conc: 9.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

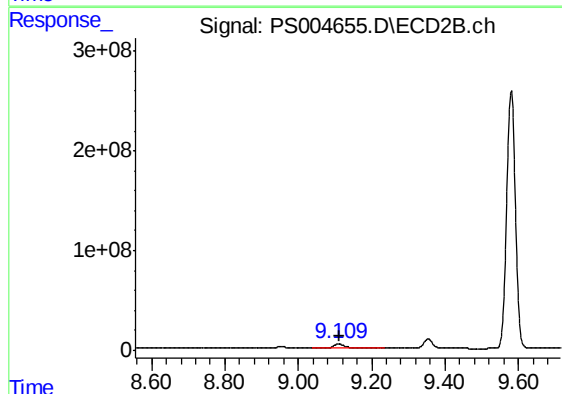


#15 Picloram

R.T.: 9.110 min
Delta R.T.: -0.003 min
Response: 88646957
Conc: 11.88 ng/ml

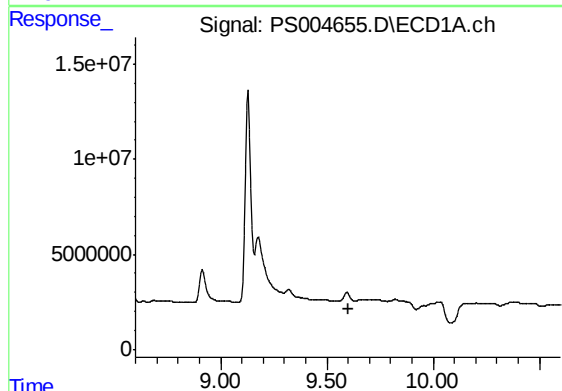

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.599 min
Response: 0
Conc: N.D.

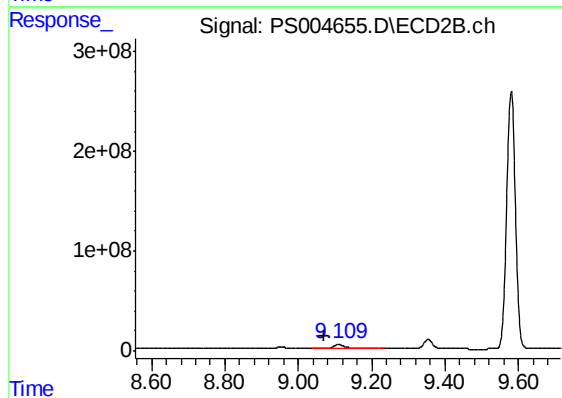

#16 DCPA

R.T.: 9.110 min
Delta R.T.: 0.038 min
Response: 88646957
Conc: 13.68 ng/ml