

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052219\
 Data File : PS004707.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2019 13:35
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 01:49:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	4.959	0.000	524.5E6	0	304.112	N.D. #
3) T	4-Nitroph...	5.416	0.000	13492368	0	21.639	N.D. #
5) T	DICAMBA	0.000	5.454	0	400.1E6	N.D.	108.302
9) T	2,4-D	6.637	0.000	757.2E6	0	553.540	N.D. #
15) T	Picloram	9.138	9.123	396.1E6	30964713	38.012	4.150 #
16) T	DCPA	0.000	9.123	0	30964713	N.D.	4.780



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052219\
Data File : PS004707.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2019 13:35
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 01:49:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

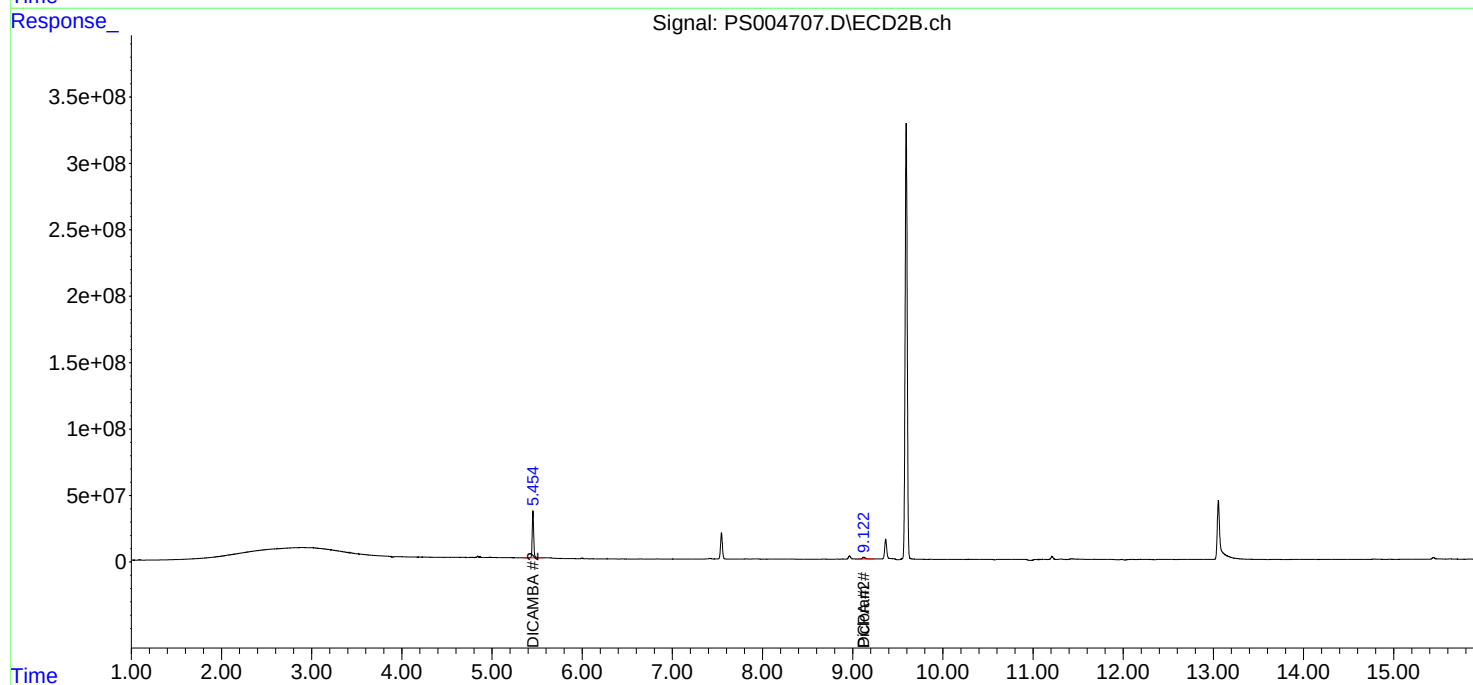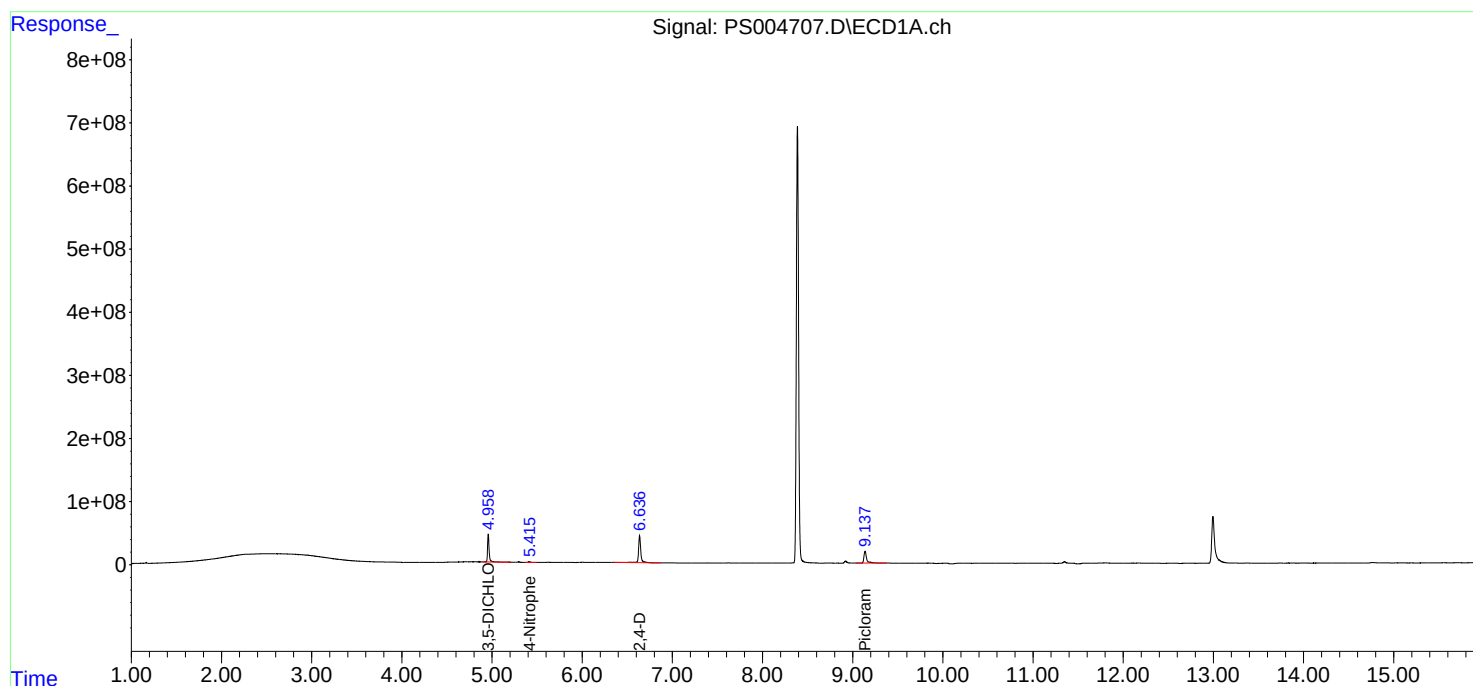


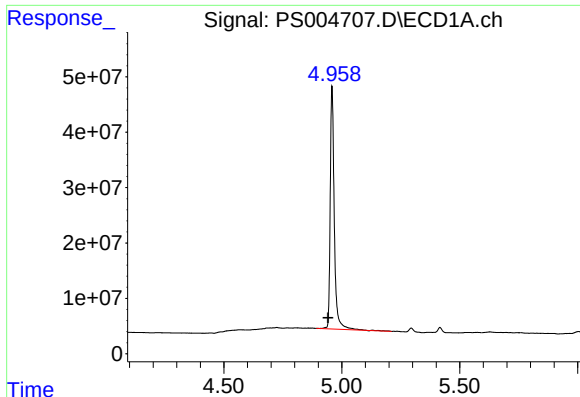

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.959 min
Delta R.T.: 0.017 min
Response: 524463615
Conc: 304.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

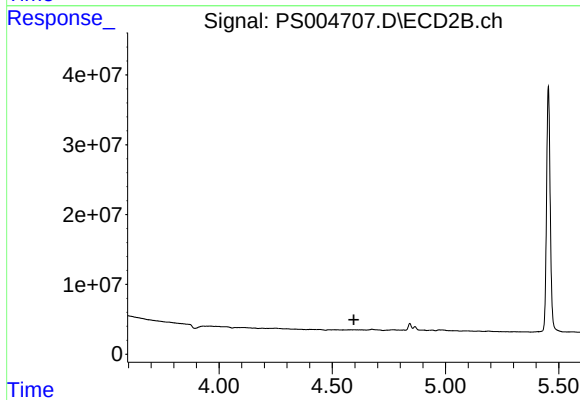


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.596 min
Response: 0
Conc: N.D.

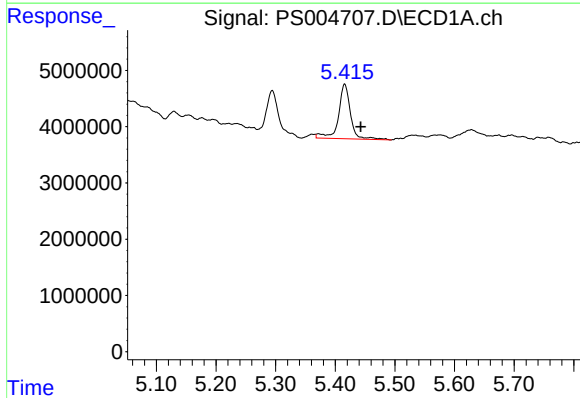


#3 4-Nitrophenol

R.T.: 5.416 min
Delta R.T.: -0.027 min
Response: 13492368
Conc: 21.64 ng/ml

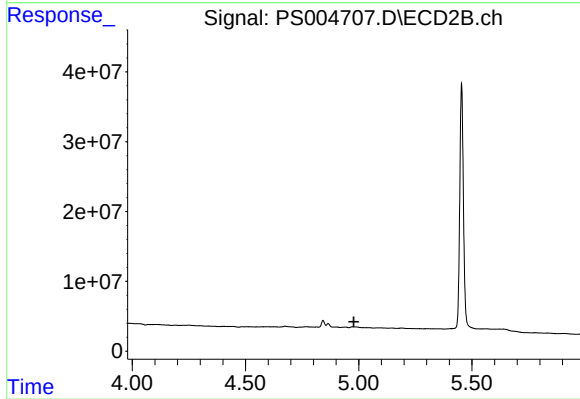

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

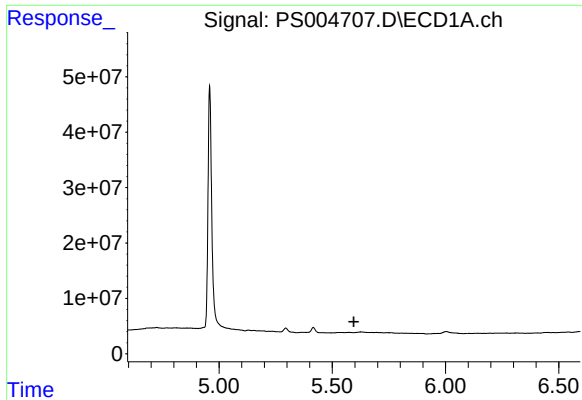

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 5.595 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

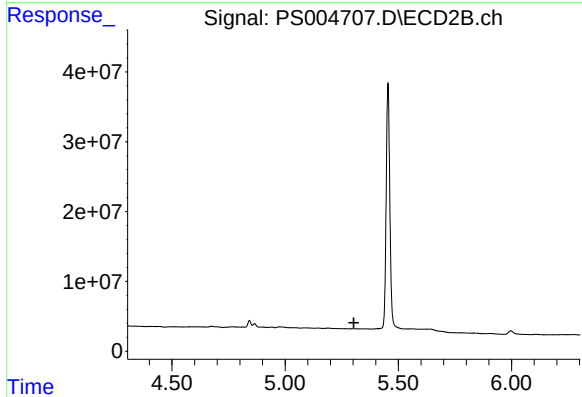


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 5.304 min
Response: 0
Conc: N.D.

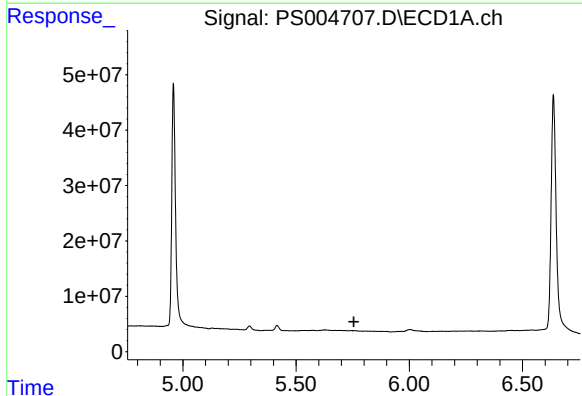


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 5.755 min
Response: 0
Conc: N.D.

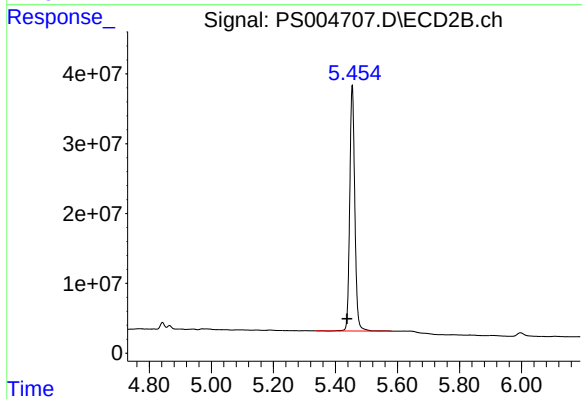

#5 DICAMBA


R.T.: 5.454 min
Delta R.T.: 0.017 min
Response: 400093731
Conc: 108.30 ng/ml

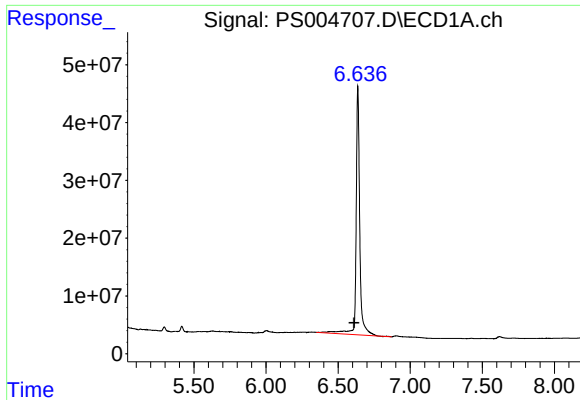

#9 2,4-D


R.T.: 6.637 min
Delta R.T.: 0.025 min
Response: 757191661
Conc: 553.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

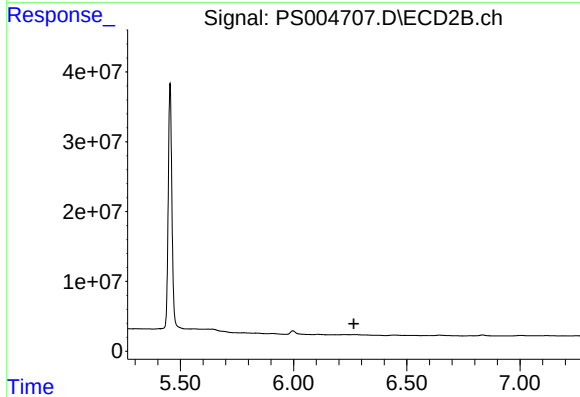


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

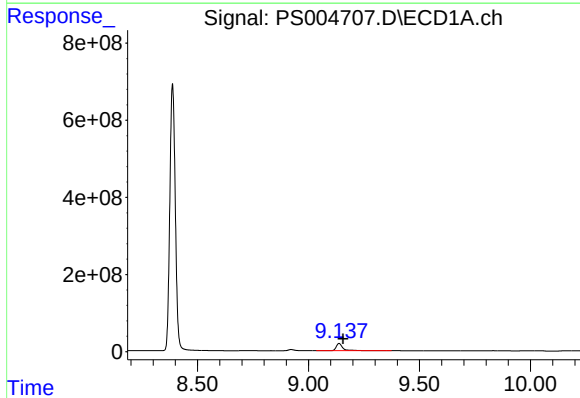


#15 Picloram

R.T.: 9.138 min
Delta R.T.: -0.018 min
Response: 396085666
Conc: 38.01 ng/ml

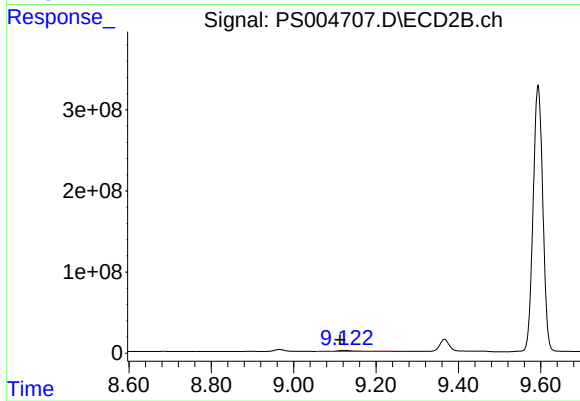

#15 Picloram


R.T.: 9.123 min
Delta R.T.: 0.010 min
Response: 30964713
Conc: 4.15 ng/ml

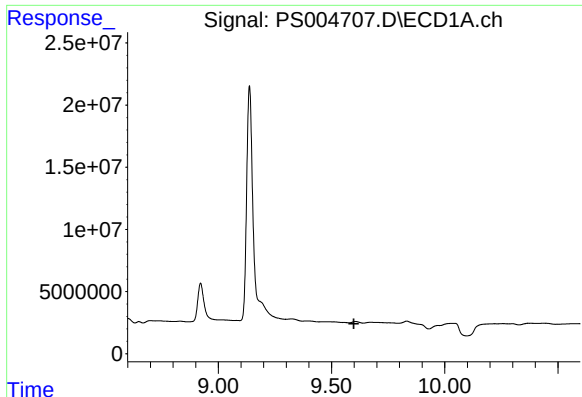

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

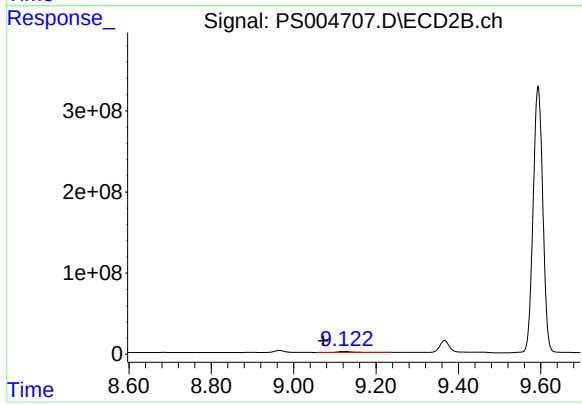

#16 DCPA

R.T.: 9.123 min
Delta R.T.: 0.051 min
Response: 30964713
Conc: 4.78 ng/ml