

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052319\
 Data File : PS004722.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2019 08:42
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 02:13:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.575	5.283	693.3E6	489.6E6	494.617	507.495
Target Compounds							
9) T	2,4-D	6.622	0.000	22925249	0	16.759	N.D. #
15) T	Picloram	9.115	9.105	212.9E6	21683174	20.429	2.906 #
16) T	DCPA	0.000	9.105	0	21683174	N.D.	3.347



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052319\
Data File : PS004722.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2019 08:42
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 02:13:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

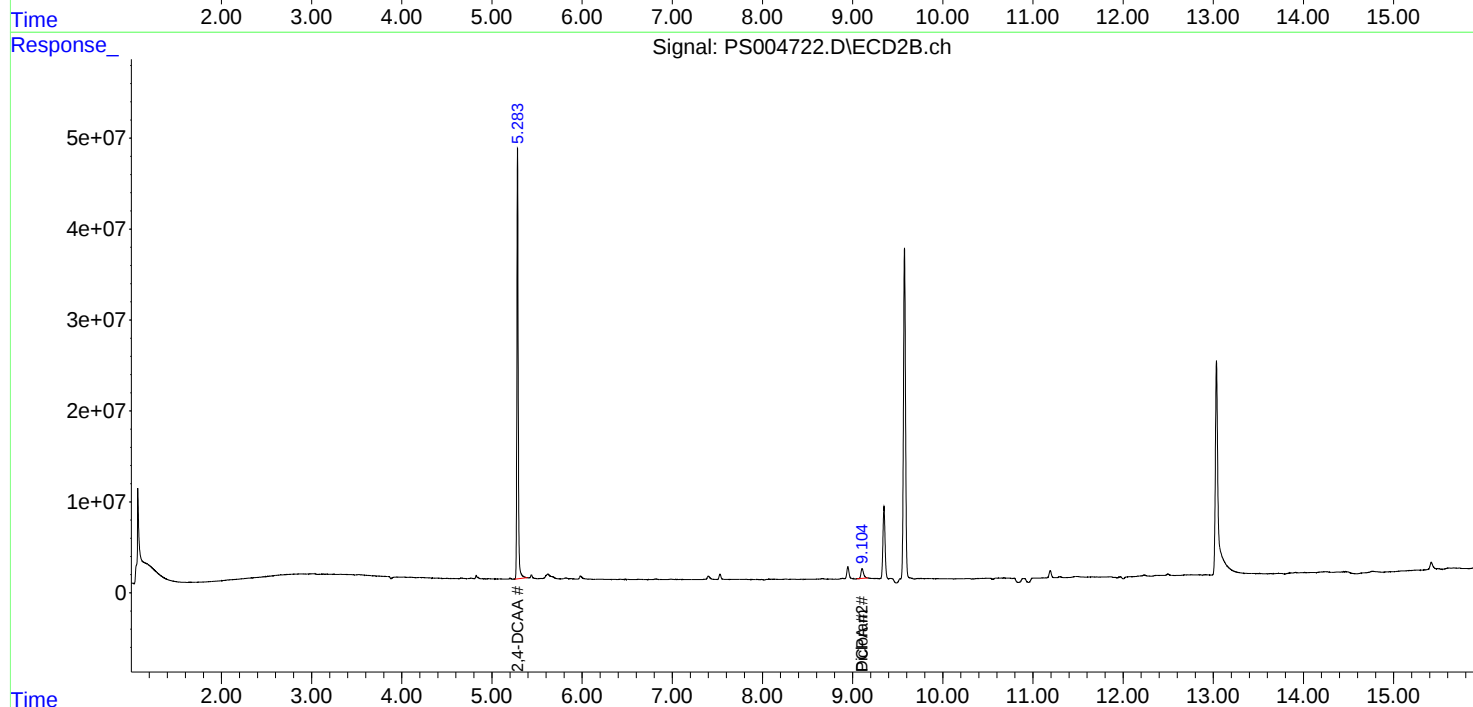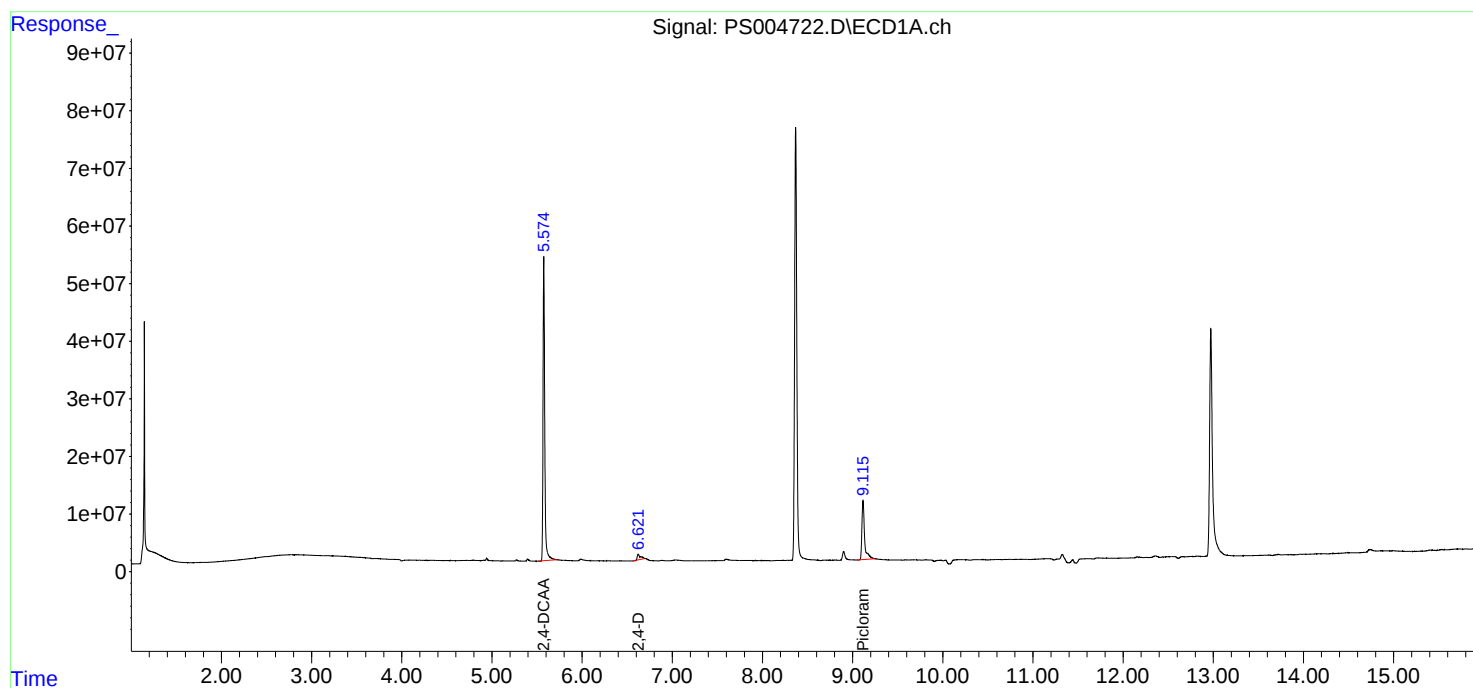


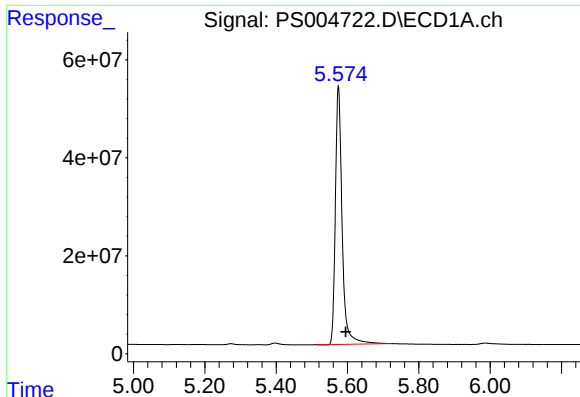

#4 2,4-DCAA


R.T.: 5.575 min
Delta R.T.: -0.020 min
Response: 693332047
Conc: 494.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

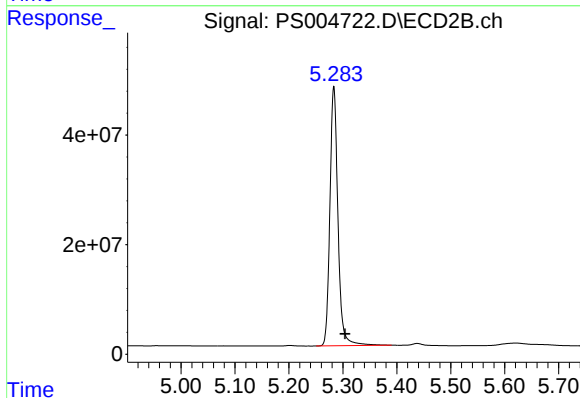


#4 2,4-DCAA

R.T.: 5.283 min
Delta R.T.: -0.020 min
Response: 489649527
Conc: 507.50 ng/ml

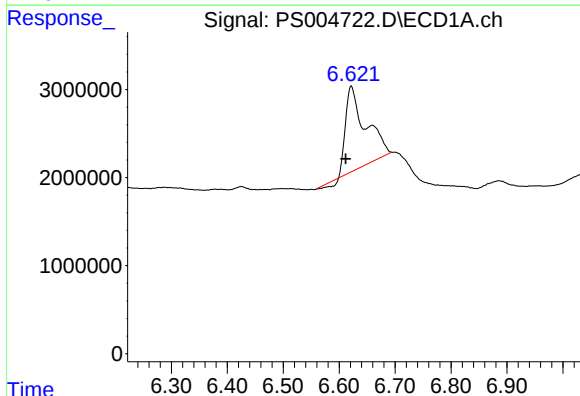


#9 2,4-D

R.T.: 6.622 min
Delta R.T.: 0.010 min
Response: 22925249
Conc: 16.76 ng/ml

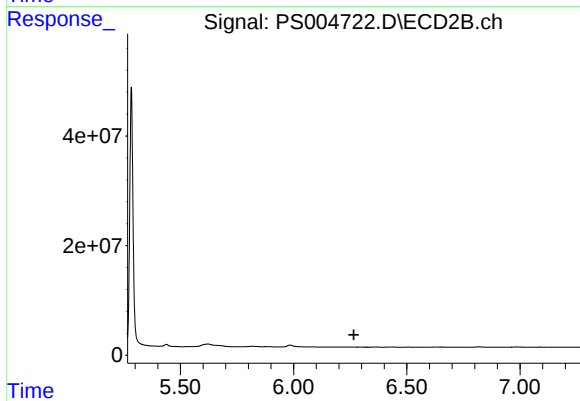

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

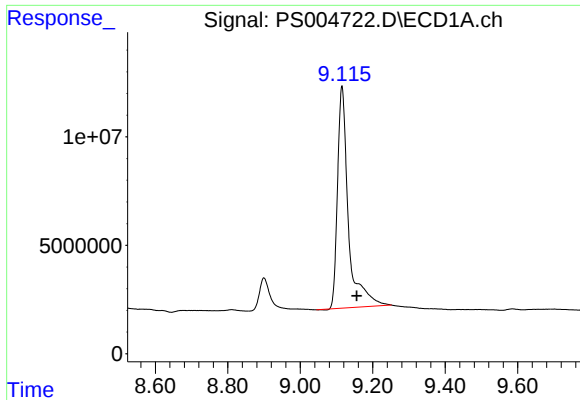

#15 Picloram


R.T.: 9.115 min
Delta R.T.: -0.040 min
Response: 212870086
Conc: 20.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

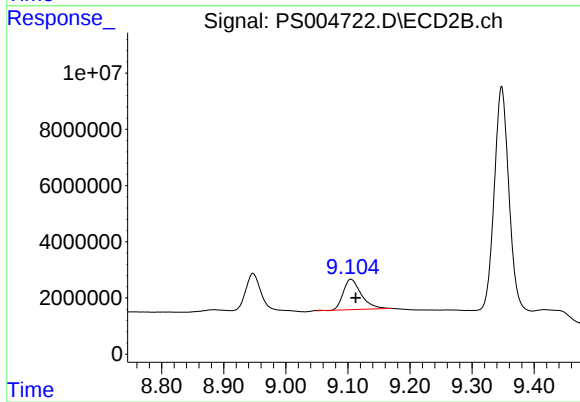


#15 Picloram

R.T.: 9.105 min
Delta R.T.: -0.008 min
Response: 21683174
Conc: 2.91 ng/ml

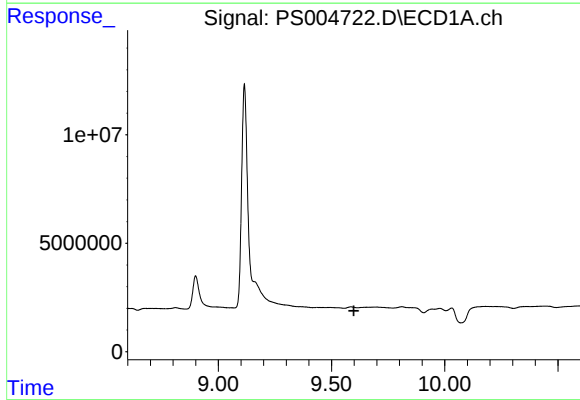

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.599 min
Response: 0
Conc: N.D.

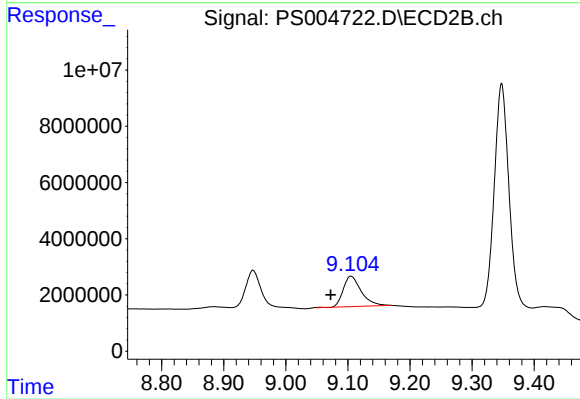

#16 DCPA

R.T.: 9.105 min
Delta R.T.: 0.033 min
Response: 21683174
Conc: 3.35 ng/ml