

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052319\
 Data File : PS004749.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2019 00:38
 Operator : SM\AJ
 Sample : K2994-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-6-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 02:21:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.608	5.318	415.0E6	290.6E6	296.075	301.239
Target Compounds							
1) T	Dalapon	2.109	0.000	47696250	0	28.773	N.D. #
2) T	3,5-DICHL...	0.000	4.580	0	20650277	N.D.	16.760
3) T	4-Nitroph...	0.000	4.983	0	24006442	N.D.	50.655
5) T	DICAMBA	5.707	5.425	20854479	12412565	3.928	3.360
6) T	MCPD	5.963	0.000	12746360	0	3.062	N.D. #
7) T	MCPA	6.071	0.000	41125220	0	7.100	N.D. #
8) T	DICHLORPROP	0.000	6.008	0	15545431	N.D.	16.488
9) T	2,4-D	0.000	6.200	0	37865755	N.D.	35.033
10) T	Pentachlo...	0.000	6.586	0	24750880	N.D.	2.015
11) T	2,4,5-TP ...	7.423	6.973	16822616	171.0E6	2.296	33.236 #
12) T	2,4,5-T	7.634	0.000	267.1E6	0	35.859	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052319\
Data File : PS004749.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2019 00:38
Operator : SM\AJ
Sample : K2994-16
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-6-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 02:21:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

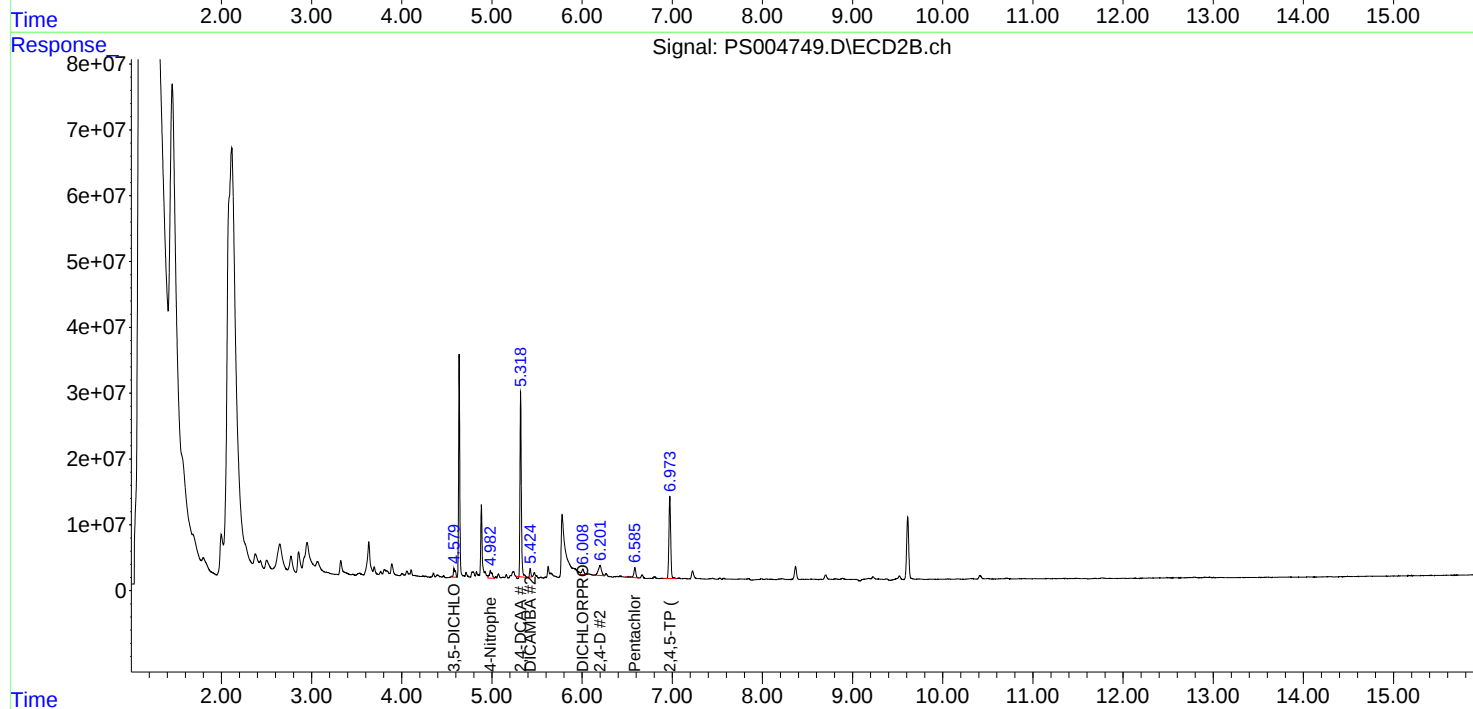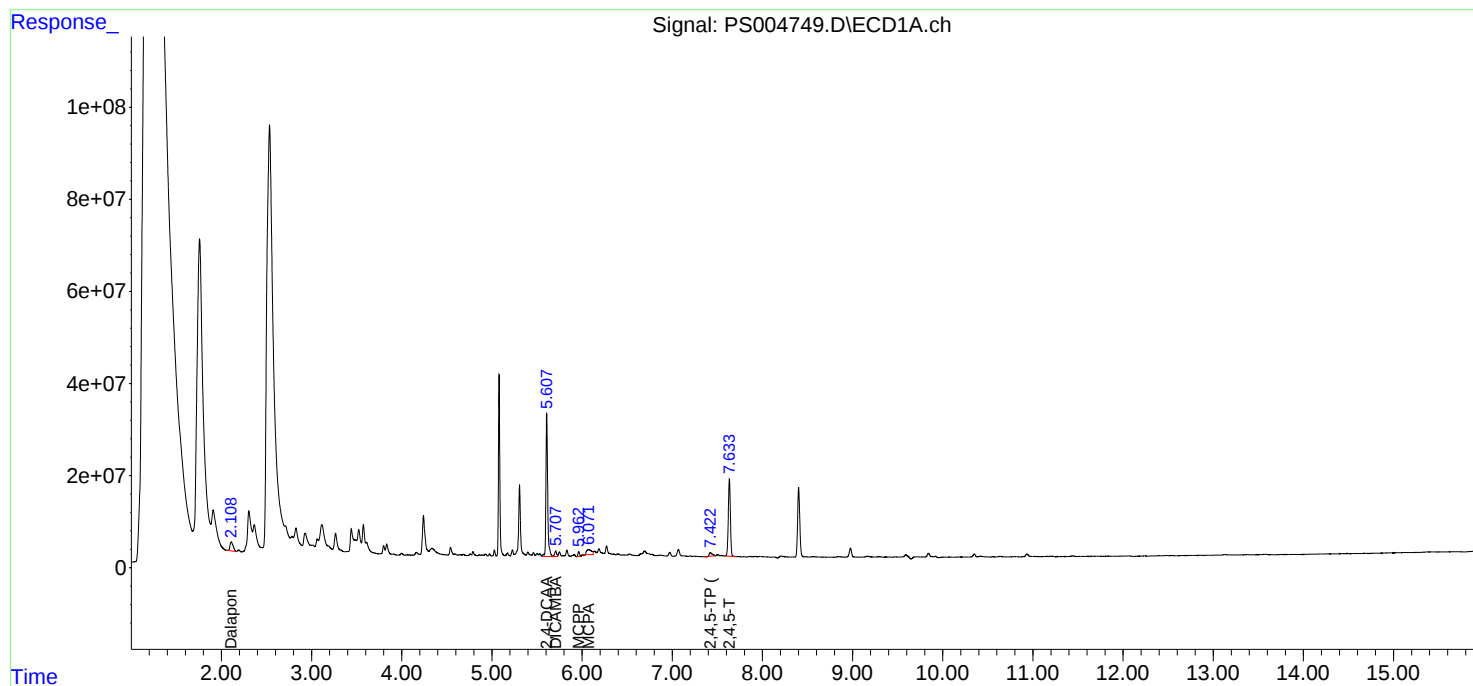


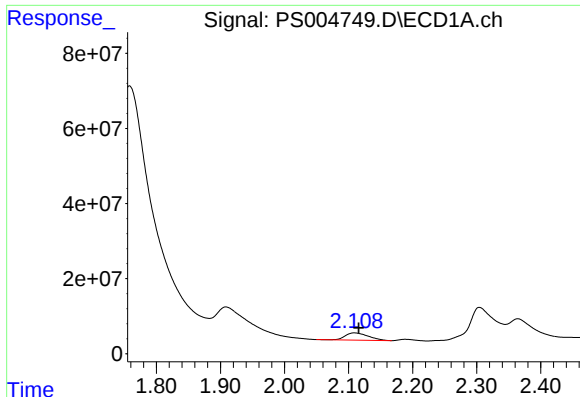

#1 Dalapon


R.T.: 2.109 min
Delta R.T.: -0.007 min
Response: 47696250
Conc: 28.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6-S

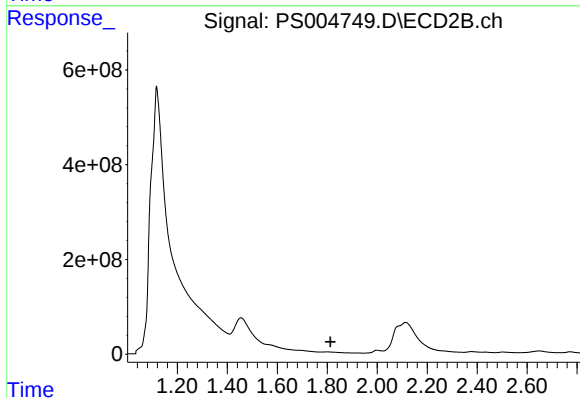


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

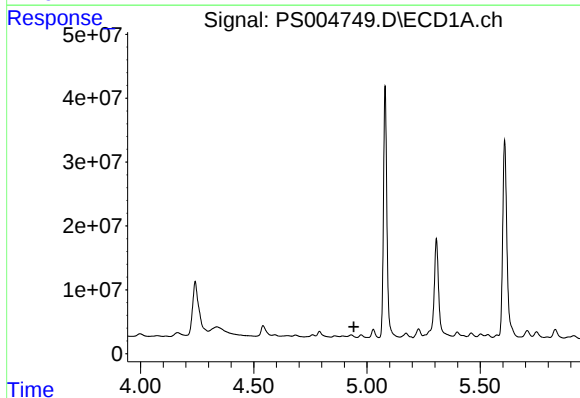


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

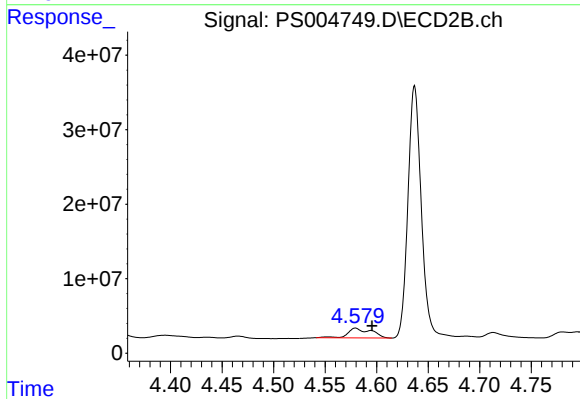

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.580 min
Delta R.T.: -0.016 min
Response: 20650277
Conc: 16.76 ng/ml

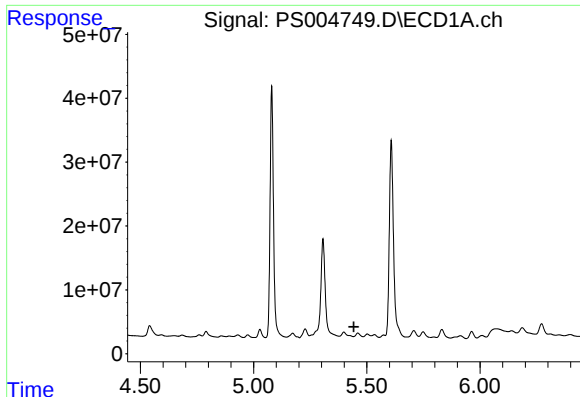

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.443 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6-S

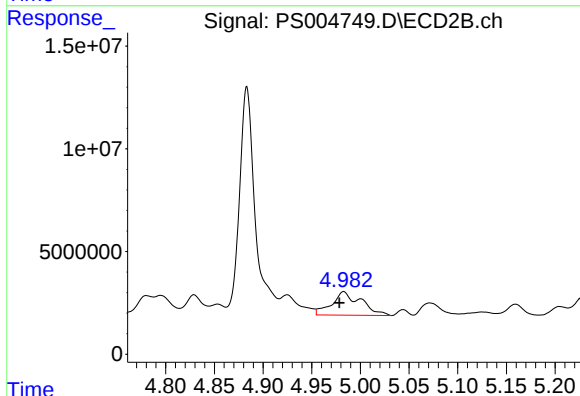


#3 4-Nitrophenol

R.T.: 4.983 min
Delta R.T.: 0.004 min
Response: 24006442
Conc: 50.66 ng/ml

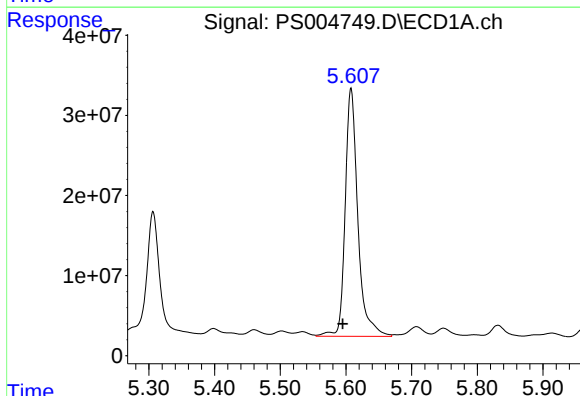


#4 2,4-DCAA

R.T.: 5.608 min
Delta R.T.: 0.013 min
Response: 415024995
Conc: 296.08 ng/ml

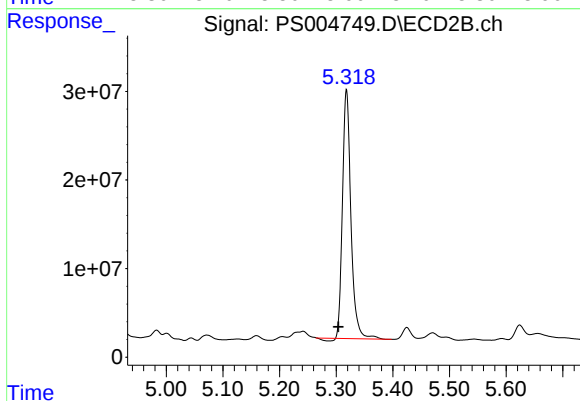

#4 2,4-DCAA


R.T.: 5.318 min
Delta R.T.: 0.015 min
Response: 290645791
Conc: 301.24 ng/ml

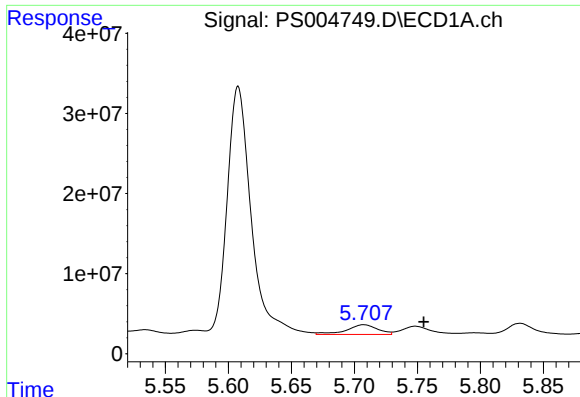

#5 DICAMBA


R.T.: 5.707 min
Delta R.T.: -0.048 min
Response: 20854479
Conc: 3.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6-S

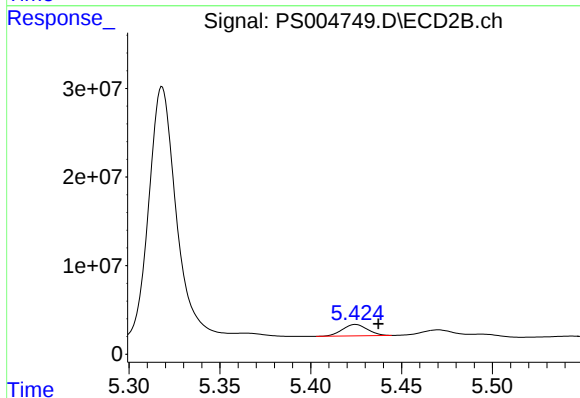


#5 DICAMBA

R.T.: 5.425 min
Delta R.T.: -0.013 min
Response: 12412565
Conc: 3.36 ng/ml

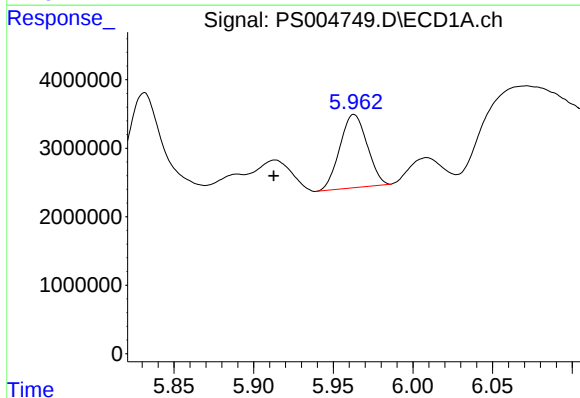


#6 MCPP

R.T.: 5.963 min
Delta R.T.: 0.050 min
Response: 12746360
Conc: 3.06 ug/ml

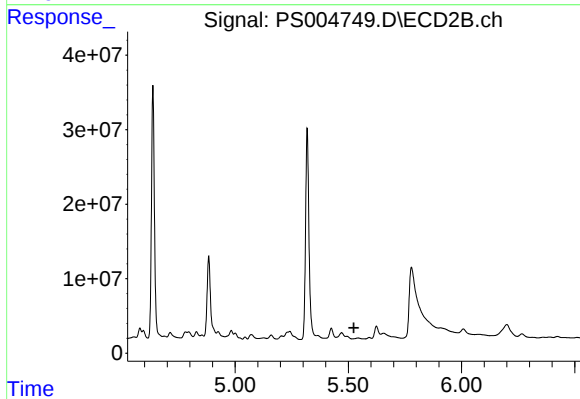

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

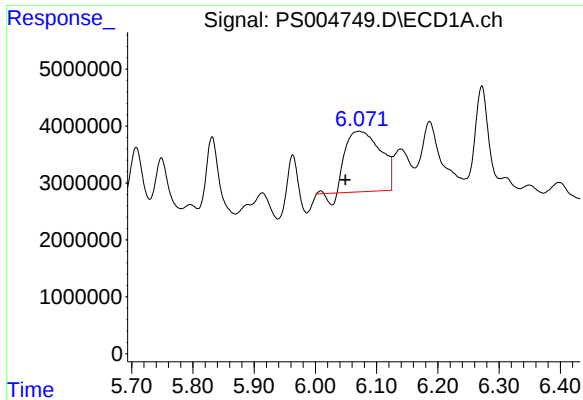

#7 MCPA


R.T.: 6.071 min
Delta R.T.: 0.022 min
Response: 41125220
Conc: 7.10 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-6-S

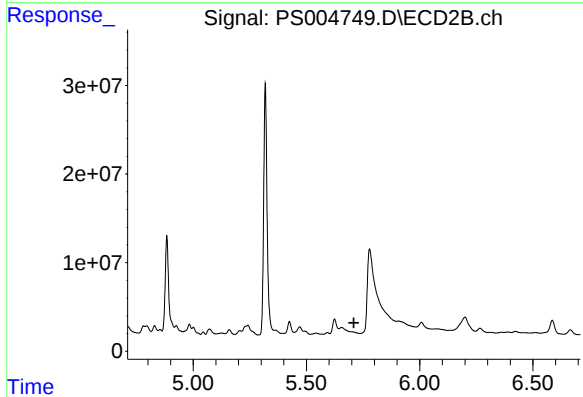


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.709 min
Response: 0
Conc: N.D.

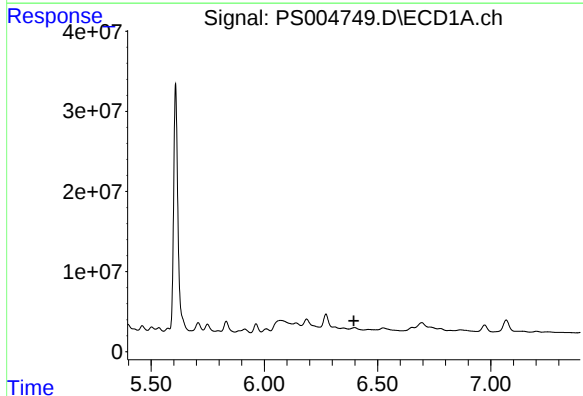


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.396 min
Response: 0
Conc: N.D.

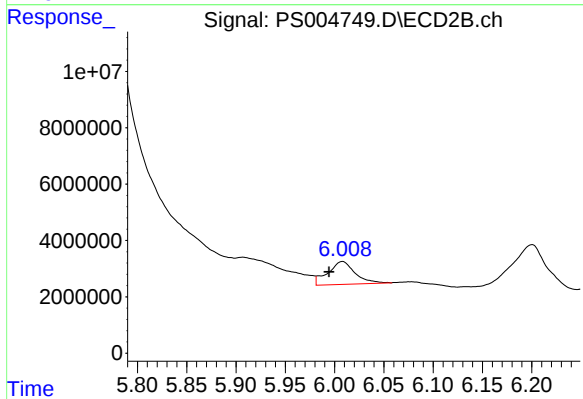

#8 DICHLORPROP


R.T.: 6.008 min
Delta R.T.: 0.014 min
Response: 15545431
Conc: 16.49 ng/ml

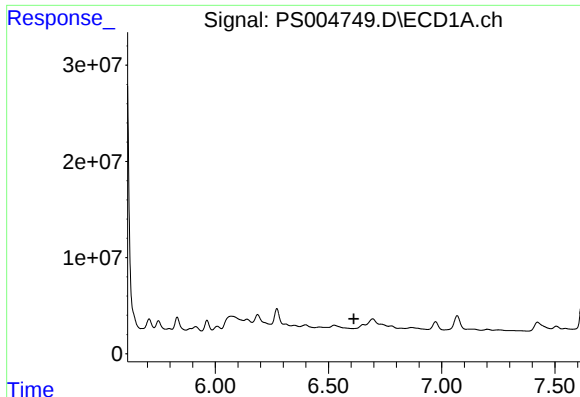

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.612 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6-S

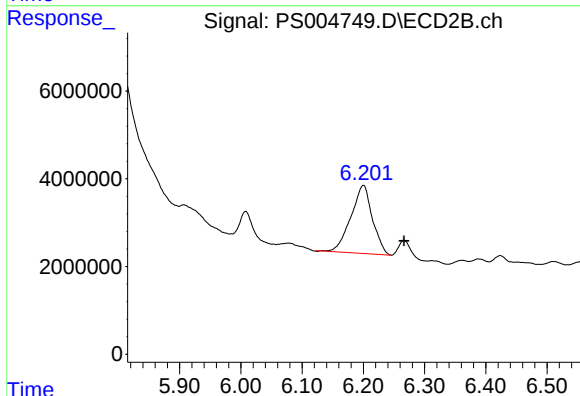


#9 2,4-D

R.T.: 6.200 min
Delta R.T.: -0.067 min
Response: 37865755
Conc: 35.03 ng/ml

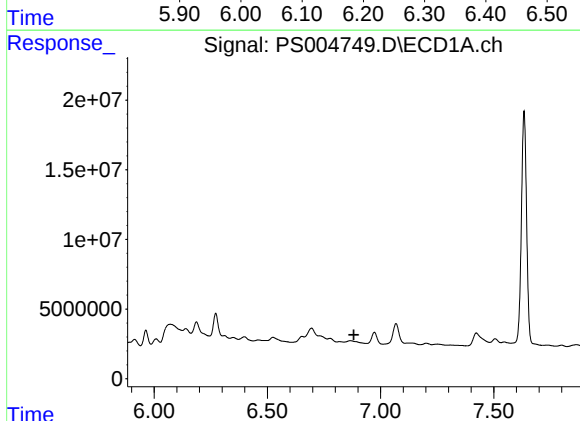


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.882 min
Response: 0
Conc: N.D.

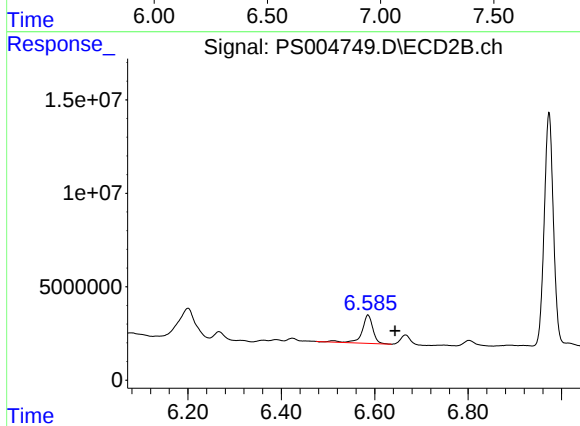

#10 Pentachlorophenol


R.T.: 6.586 min
Delta R.T.: -0.058 min
Response: 24750880
Conc: 2.01 ng/ml

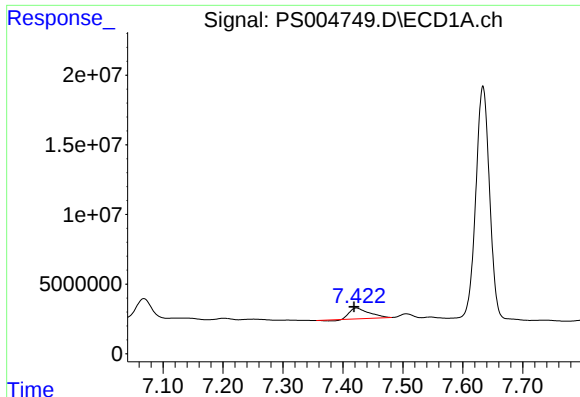

#11 2,4,5-TP (SILVEX)


R.T.: 7.423 min
Delta R.T.: 0.004 min
Response: 16822616
Conc: 2.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6-S

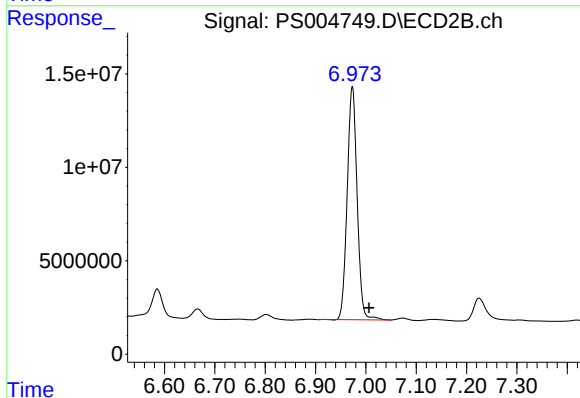


#11 2,4,5-TP (SILVEX)

R.T.: 6.973 min
Delta R.T.: -0.033 min
Response: 171011533
Conc: 33.24 ng/ml

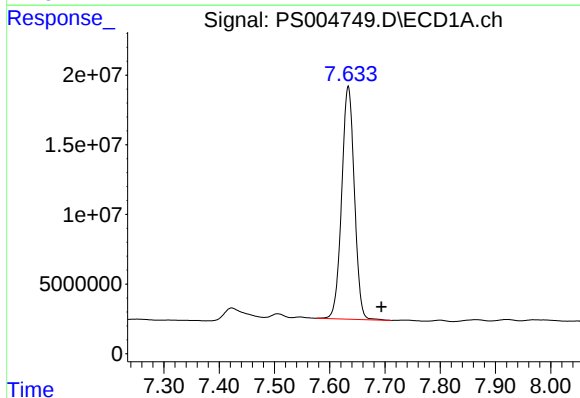

#12 2,4,5-T

R.T.: 7.634 min
Delta R.T.: -0.060 min
Response: 267057969
Conc: 35.86 ng/ml

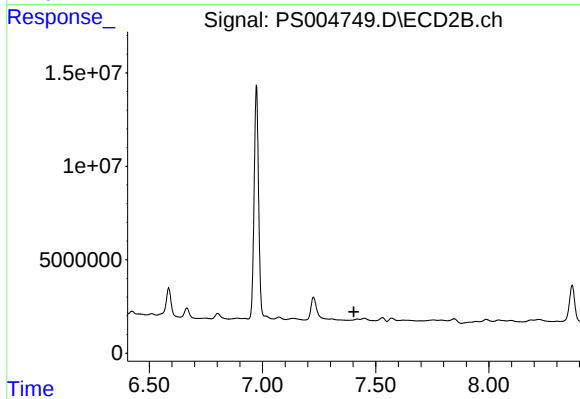

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.404 min
Response: 0
Conc: N.D.