

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052819\
 Data File : PS004804.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2019 14:23
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 02:11:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.592	5.297	496.0E6	353.0E6	353.813	365.915
Target Compounds							
12) T	2,4,5-T	0.000	7.407	0	73712912	N.D.	16.540
15) T	Picloram	9.169	9.115	237.4E6	197.6E6	22.782	26.492
16) T	DCPA	0.000	9.115	0	197.6E6	N.D.	30.510



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052819\
Data File : PS004804.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2019 14:23
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 02:11:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

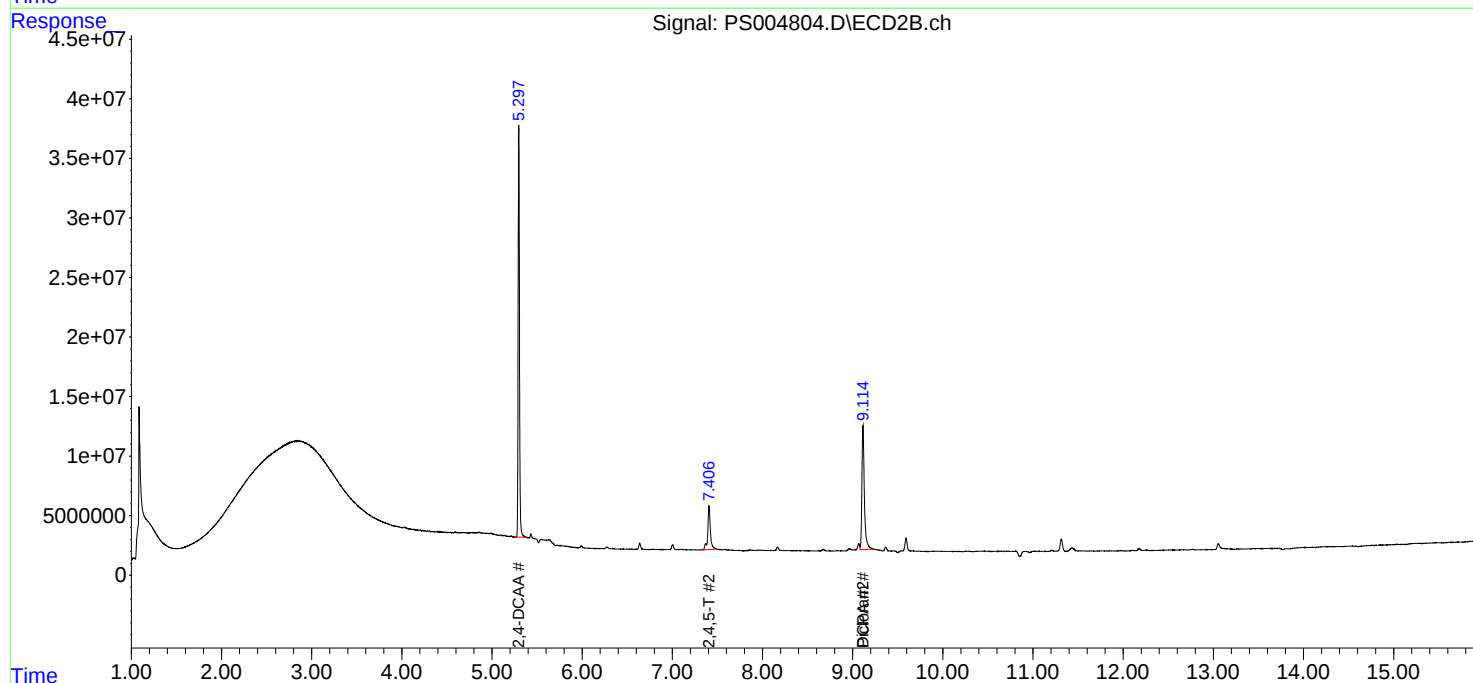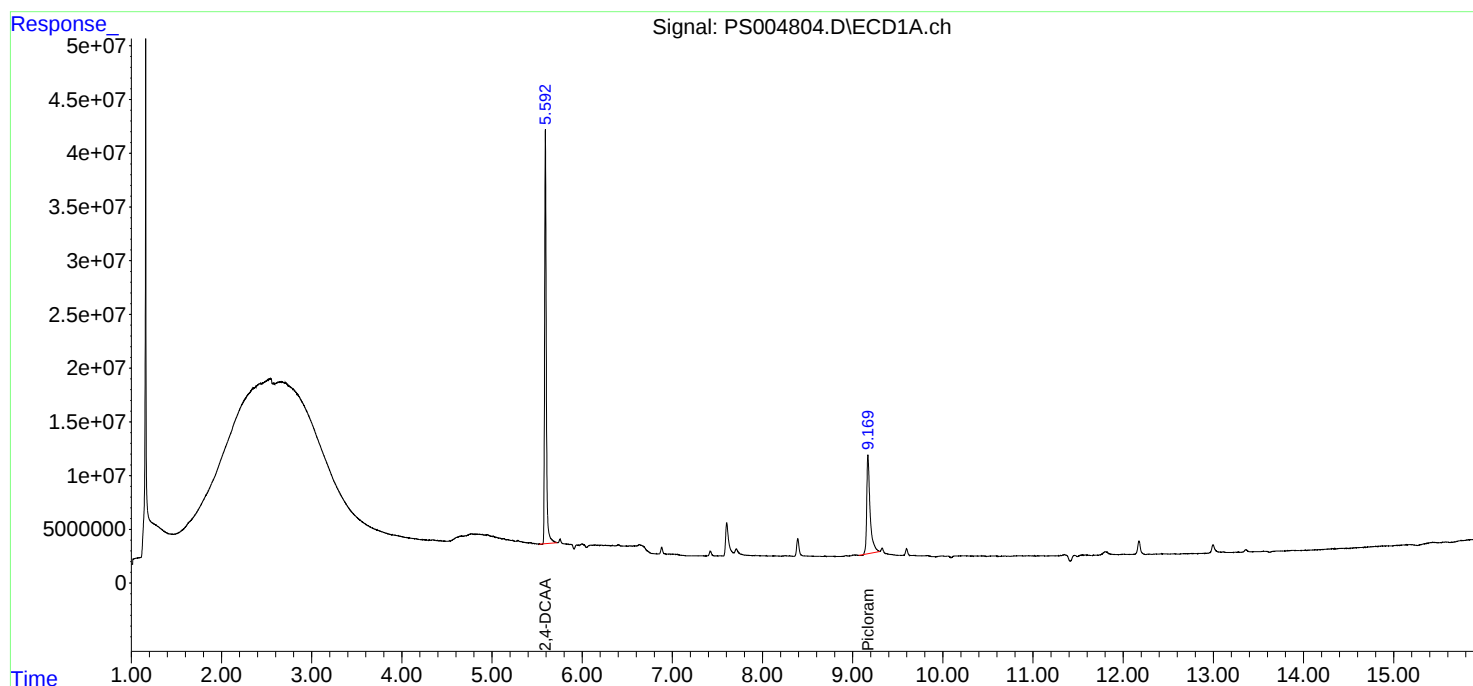


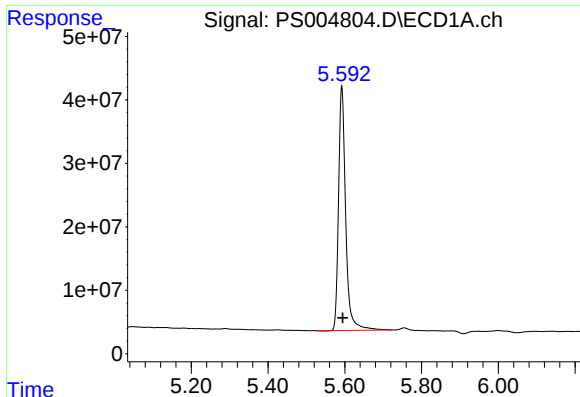

#4 2,4-DCAA


R.T.: 5.592 min
Delta R.T.: -0.003 min
Response: 495960182
Conc: 353.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

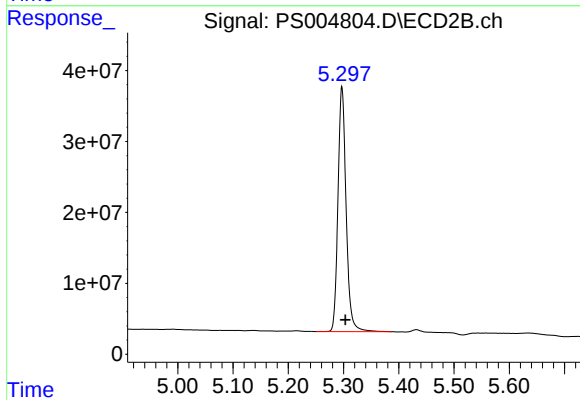


#4 2,4-DCAA

R.T.: 5.297 min
Delta R.T.: -0.007 min
Response: 353047610
Conc: 365.91 ng/ml

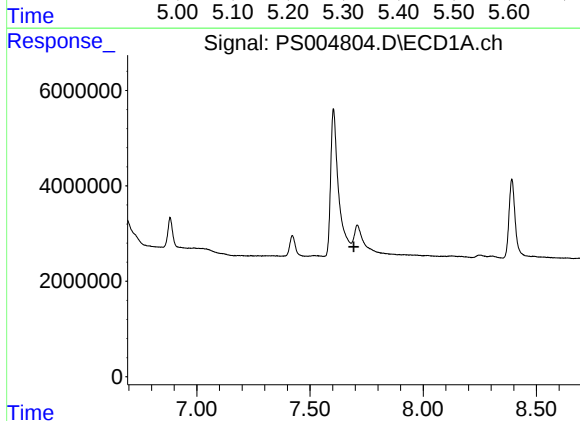


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.693 min
Response: 0
Conc: N.D.

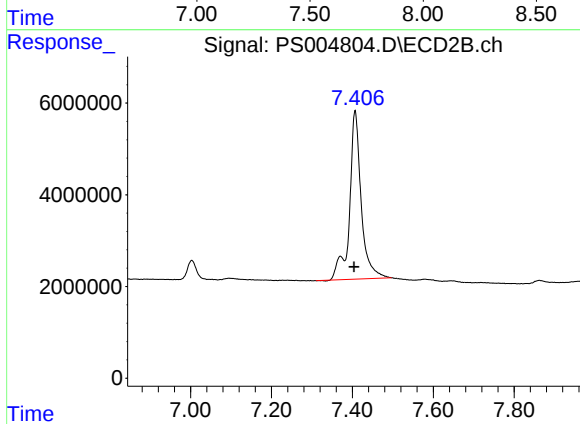

#12 2,4,5-T


R.T.: 7.407 min
Delta R.T.: 0.003 min
Response: 73712912
Conc: 16.54 ng/ml

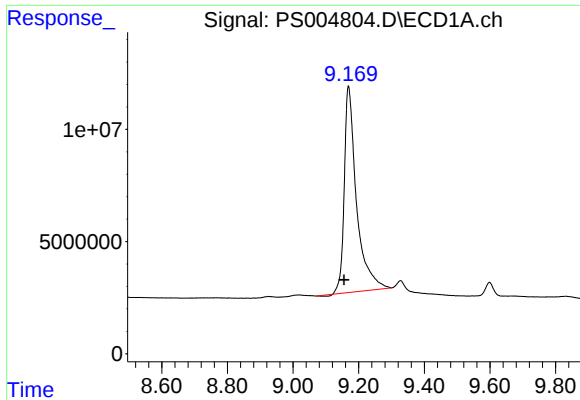

#15 Picloram


R.T.: 9.169 min
Delta R.T.: 0.014 min
Response: 237388667
Conc: 22.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

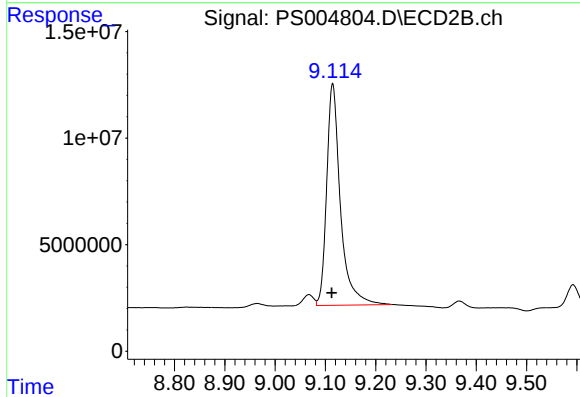


#15 Picloram

R.T.: 9.115 min
Delta R.T.: 0.002 min
Response: 197646584
Conc: 26.49 ng/ml

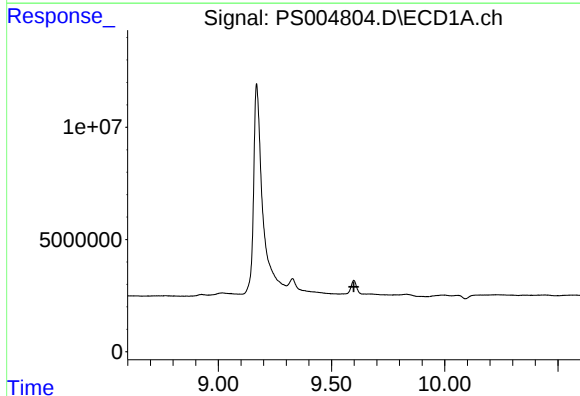

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.599 min
Response: 0
Conc: N.D.

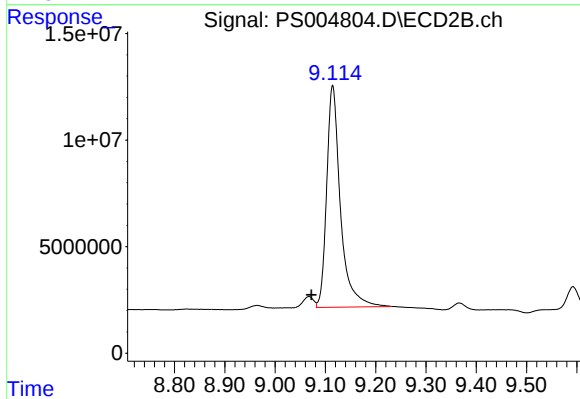

#16 DCPA

R.T.: 9.115 min
Delta R.T.: 0.042 min
Response: 197646584
Conc: 30.51 ng/ml