

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052819\
 Data File : PS004806.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2019 17:20
 Operator : SM\AJ
 Sample : PB120096BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB120096BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 02:12:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.597	5.303	903.4E6	639.7E6	644.450	663.038
Target Compounds							
2) T	3,5-DICHL...	0.000	4.621	0	315.6E6	N.D.	256.108
3) T	4-Nitroph...	5.401	0.000	35083105	0	56.267	N.D. #
5) T	DICAMBA	5.738	5.410	12158665	11471174	2.290	3.105 #
6) T	MCP	5.903	0.000	15328830	0	3.682	N.D. #
7) T	MCPA	6.092	5.696	9082286	16116277	1.568	3.939 #
11) T	2,4,5-TP ...	0.000	6.960	0	65111353	N.D.	12.654
12) T	2,4,5-T	0.000	7.415	0	54830014	N.D.	12.303
13) T	2,4-DB	8.260	0.000	135.5E6	0	140.274	N.D. #
14) T	DINOSEB	0.000	8.169	0	54579802	N.D.	14.198
15) T	Picloram	9.176	9.121	284.9E6	233.5E6	27.345	31.298
16) T	DCPA	0.000	9.121	0	233.5E6	N.D.	36.044



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052819\
Data File : PS004806.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2019 17:20
Operator : SM\AJ
Sample : PB120096BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PB120096BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 02:12:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

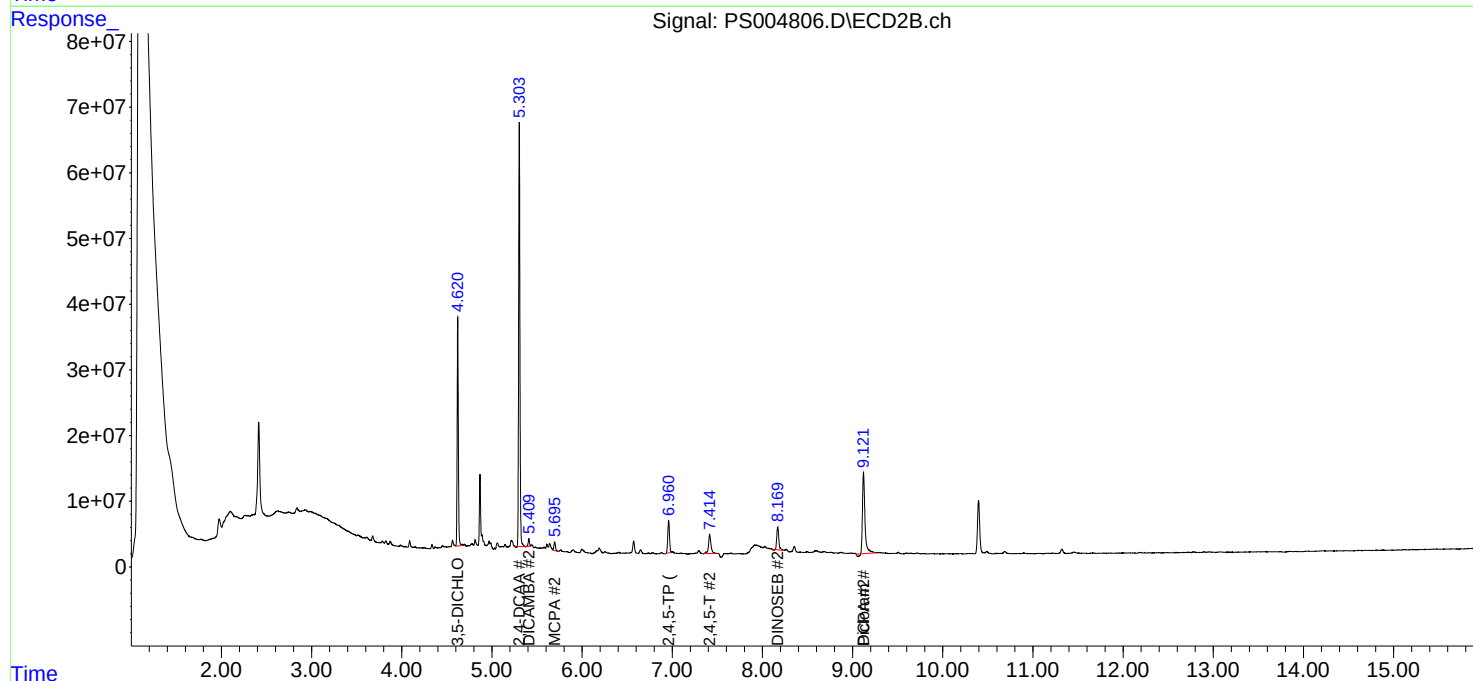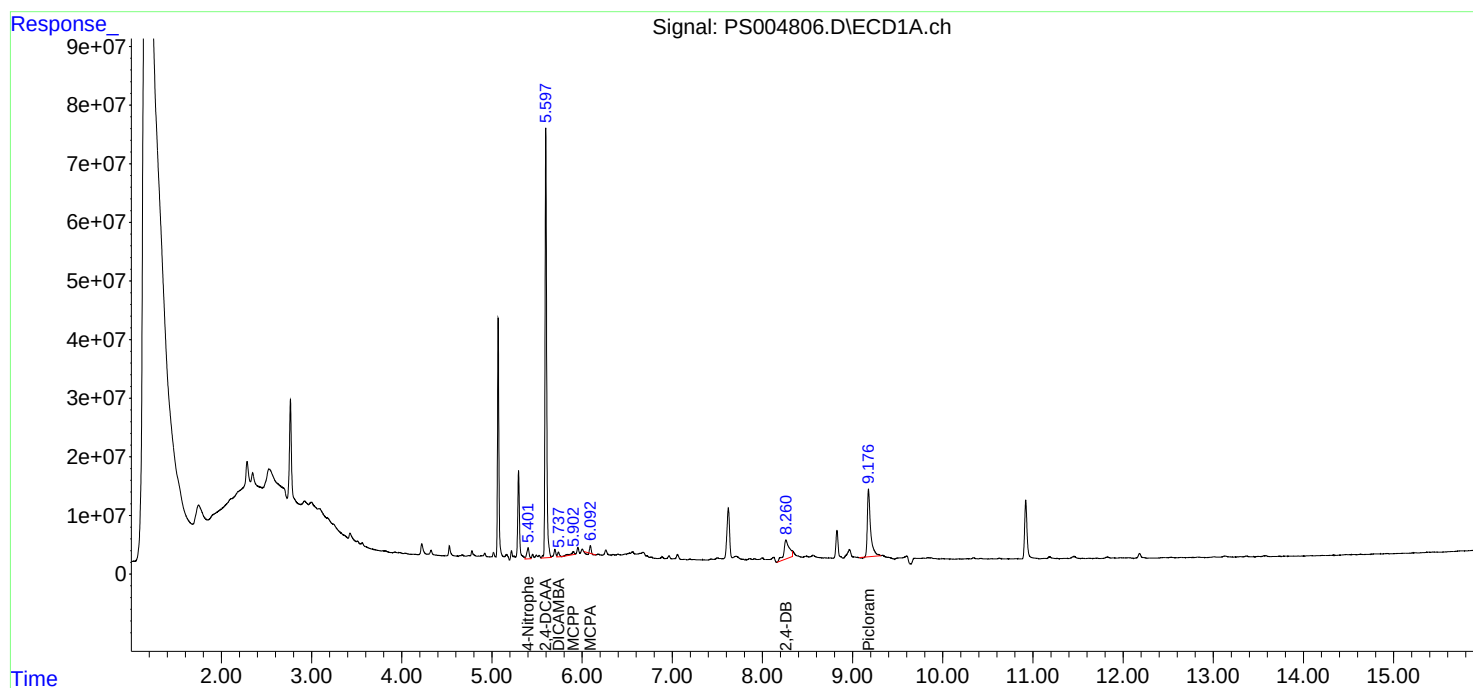


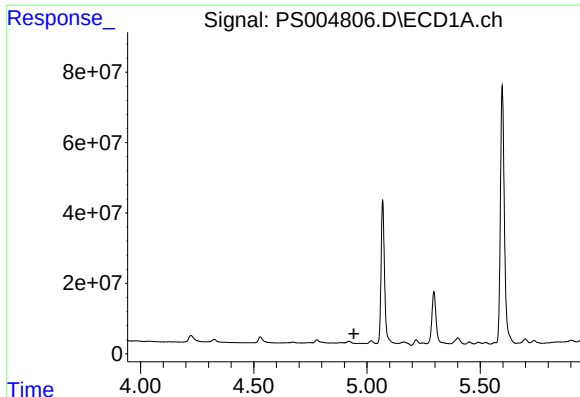

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB120096BL

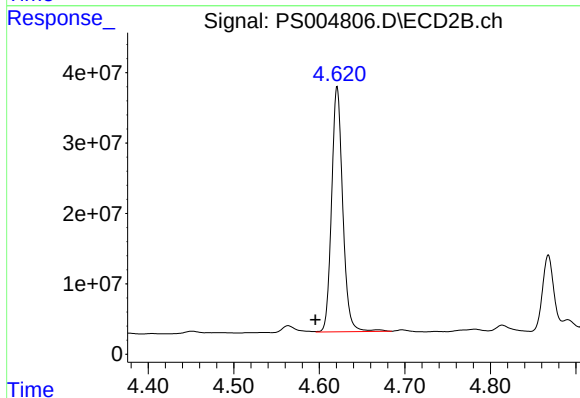


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.621 min
Delta R.T.: 0.025 min
Response: 31558505
Conc: 256.11 ng/ml

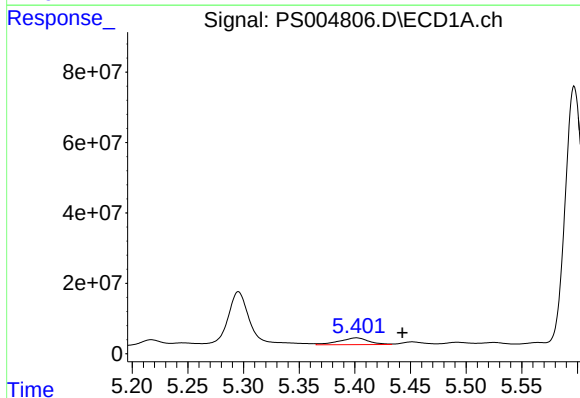


#3 4-Nitrophenol

R.T.: 5.401 min
Delta R.T.: -0.041 min
Response: 35083105
Conc: 56.27 ng/ml

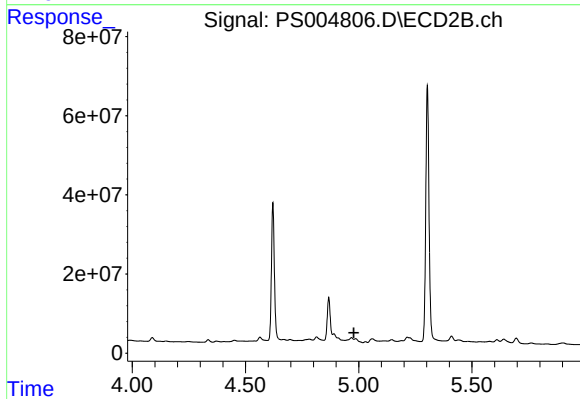

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

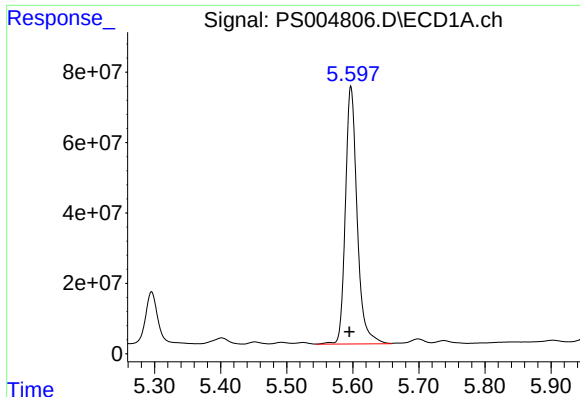

#4 2,4-DCAA


R.T.: 5.597 min
Delta R.T.: 0.002 min
Response: 903360988
Conc: 644.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB120096BL

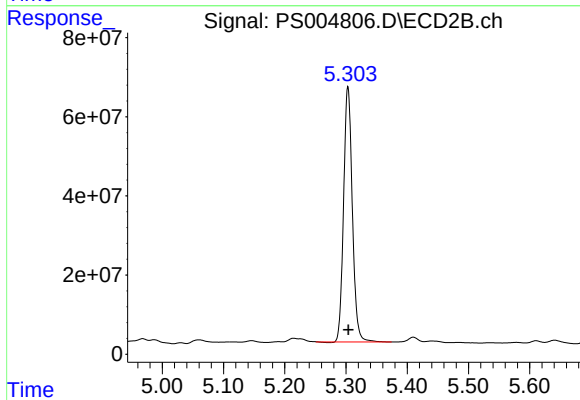


#4 2,4-DCAA

R.T.: 5.303 min
Delta R.T.: 0.000 min
Response: 639722700
Conc: 663.04 ng/ml

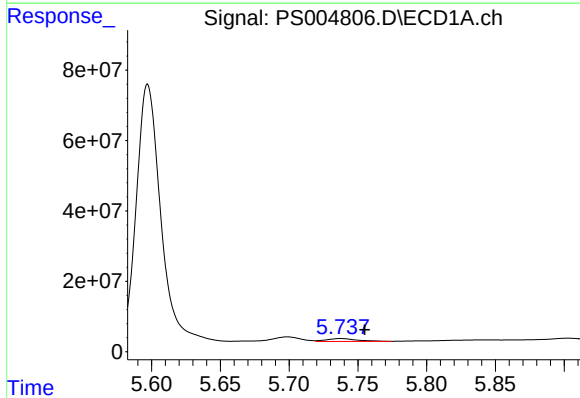


#5 DICAMBA

R.T.: 5.738 min
Delta R.T.: -0.017 min
Response: 12158665
Conc: 2.29 ng/ml

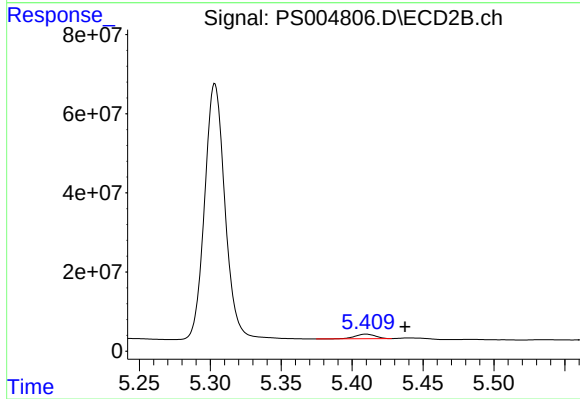

#5 DICAMBA


R.T.: 5.410 min
Delta R.T.: -0.027 min
Response: 11471174
Conc: 3.11 ng/ml

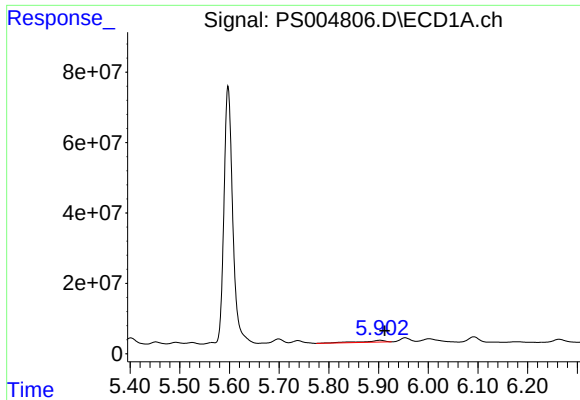

#6 MCPP


R.T.: 5.903 min
Delta R.T.: -0.010 min
Response: 15328830
Conc: 3.68 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB120096BL

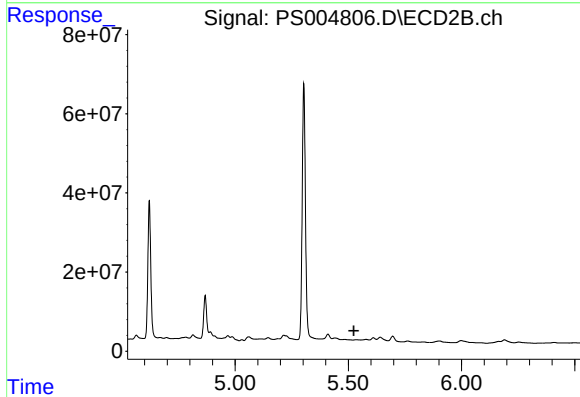


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

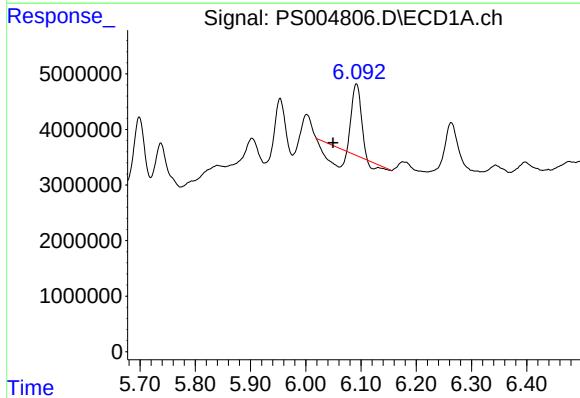


#7 MCPA

R.T.: 6.092 min
Delta R.T.: 0.042 min
Response: 9082286
Conc: 1.57 ug/ml

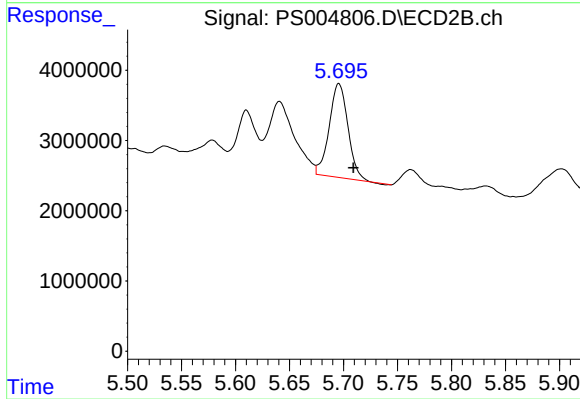

#7 MCPA


R.T.: 5.696 min
Delta R.T.: -0.013 min
Response: 16116277
Conc: 3.94 ug/ml

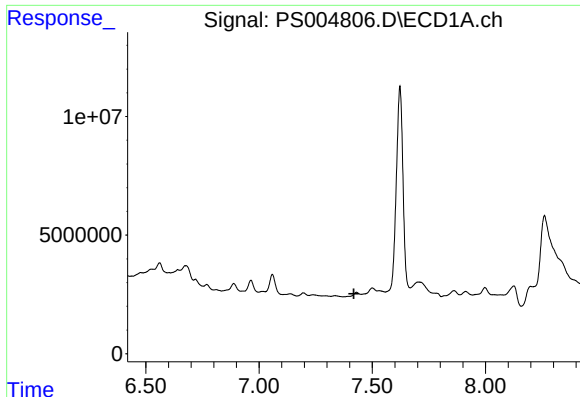

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB120096BL

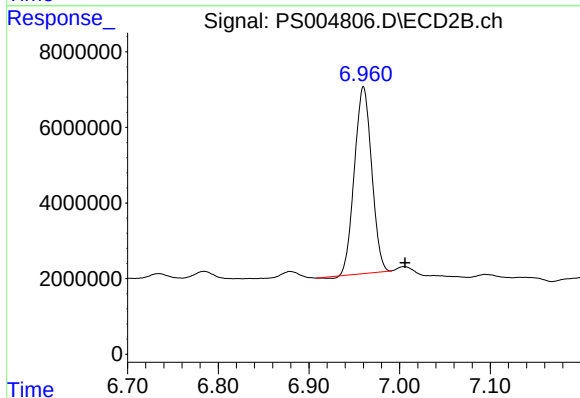


#11 2,4,5-TP (SILVEX)

R.T.: 6.960 min
Delta R.T.: -0.046 min
Response: 65111353
Conc: 12.65 ng/ml

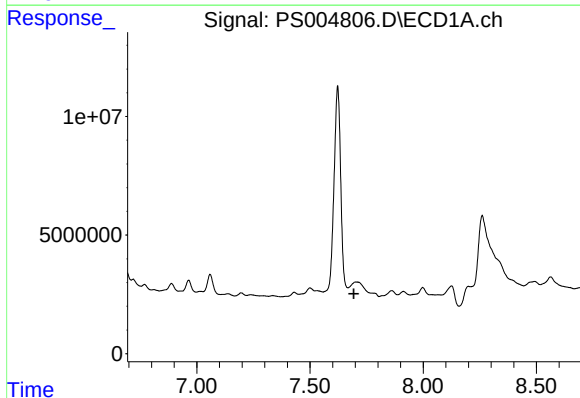


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.693 min
Response: 0
Conc: N.D.

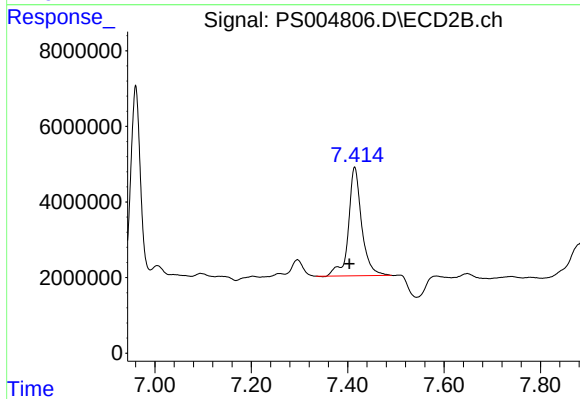

#12 2,4,5-T


R.T.: 7.415 min
Delta R.T.: 0.011 min
Response: 54830014
Conc: 12.30 ng/ml

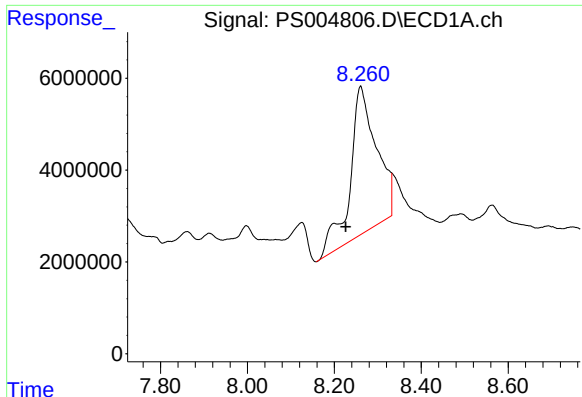

#13 2,4-DB


R.T.: 8.260 min
Delta R.T.: 0.034 min
Response: 135499347
Conc: 140.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB120096BL

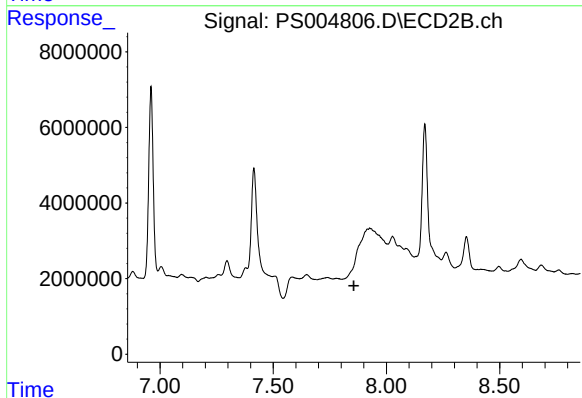


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.856 min
Response: 0
Conc: N.D.

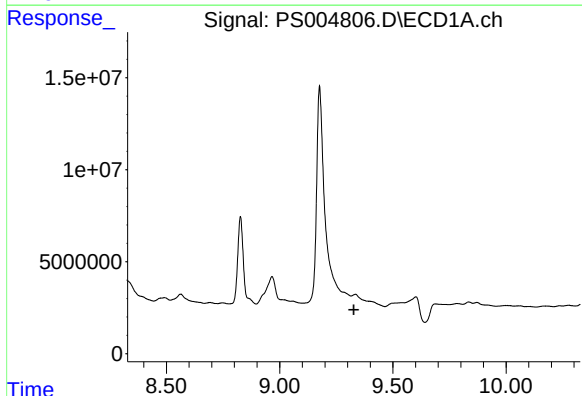


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.328 min
Response: 0
Conc: N.D.

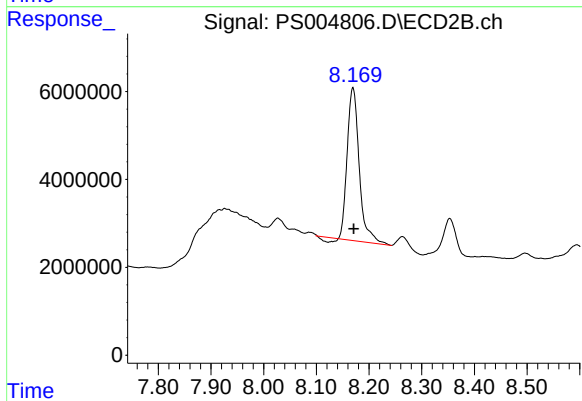

#14 DINOSEB


R.T.: 8.169 min
Delta R.T.: -0.002 min
Response: 54579802
Conc: 14.20 ng/ml

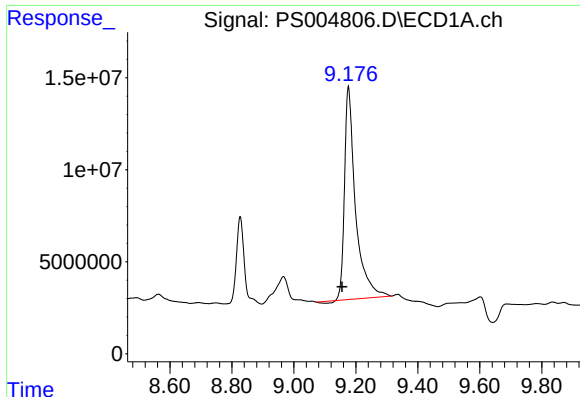

#15 Picloram


R.T.: 9.176 min
Delta R.T.: 0.021 min
Response: 284939966
Conc: 27.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB120096BL

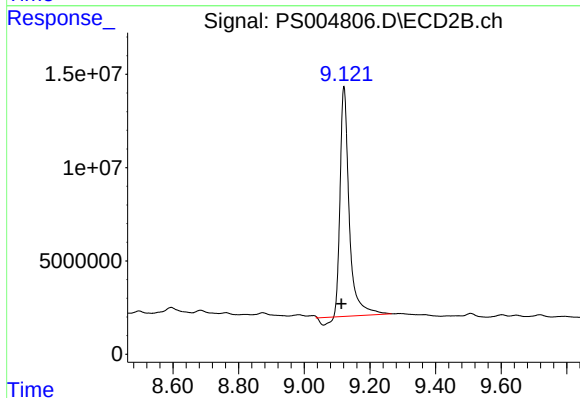


#15 Picloram

R.T.: 9.121 min
Delta R.T.: 0.008 min
Response: 233495882
Conc: 31.30 ng/ml

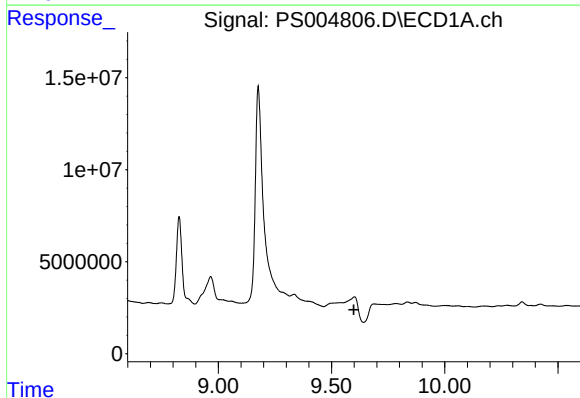

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.599 min
Response: 0
Conc: N.D.

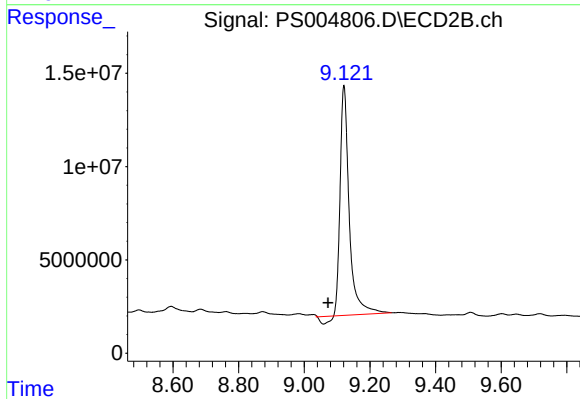

#16 DCPA

R.T.: 9.121 min
Delta R.T.: 0.049 min
Response: 233495882
Conc: 36.04 ng/ml