

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052819\
 Data File : PS004815.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2019 20:38
 Operator : SM\AJ
 Sample : K3052-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-SF-03-007-B

Manual Integrations
 APPROVED

Ankita
 5/29/2019 2:17:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 02:16:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	5.573	5.283	166.3E6	123.6E6	118.644m	128.107m
------	----------	-------	-------	---------	---------	----------	----------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052819\
Data File : PS004815.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2019 20:38
Operator : SM\AJ
Sample : K3052-03
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
FK-SF-03-007-B


Manual Integrations
APPROVED

Ankita
5/29/2019 2:17:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 02:16:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

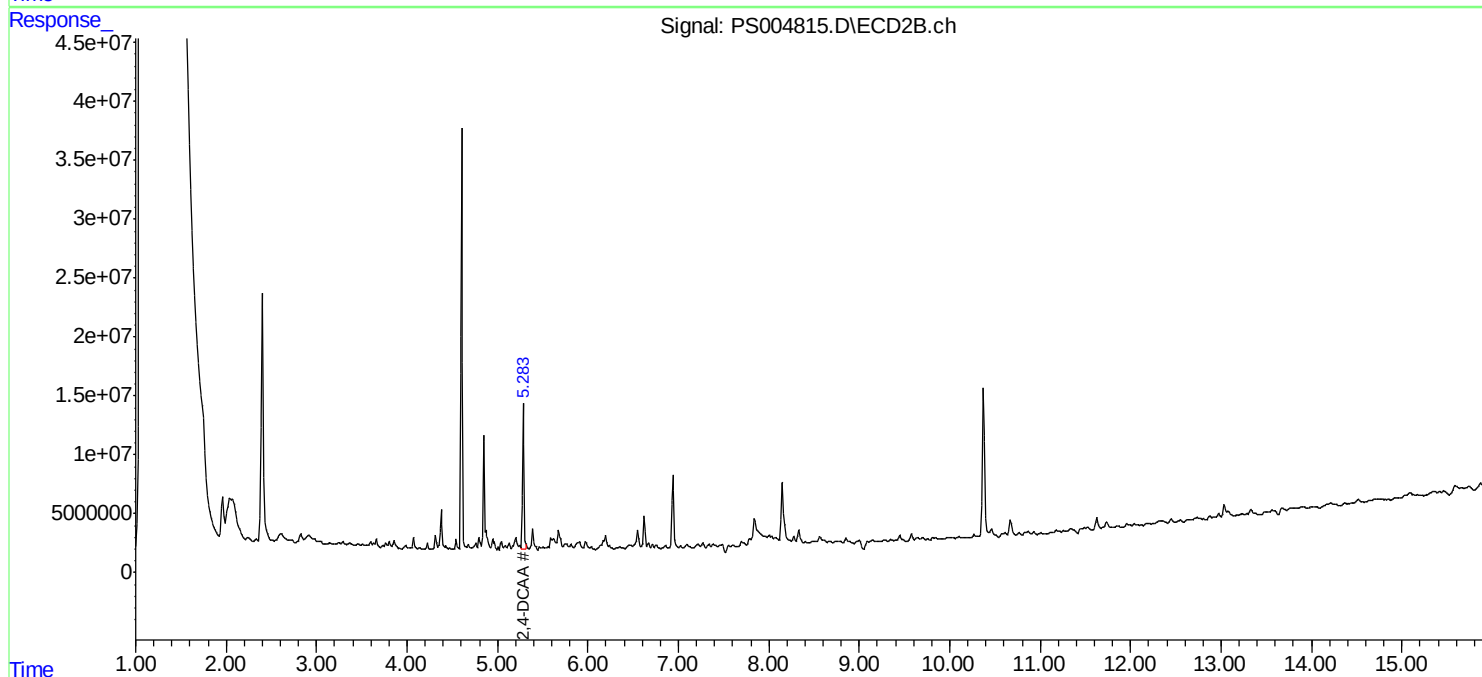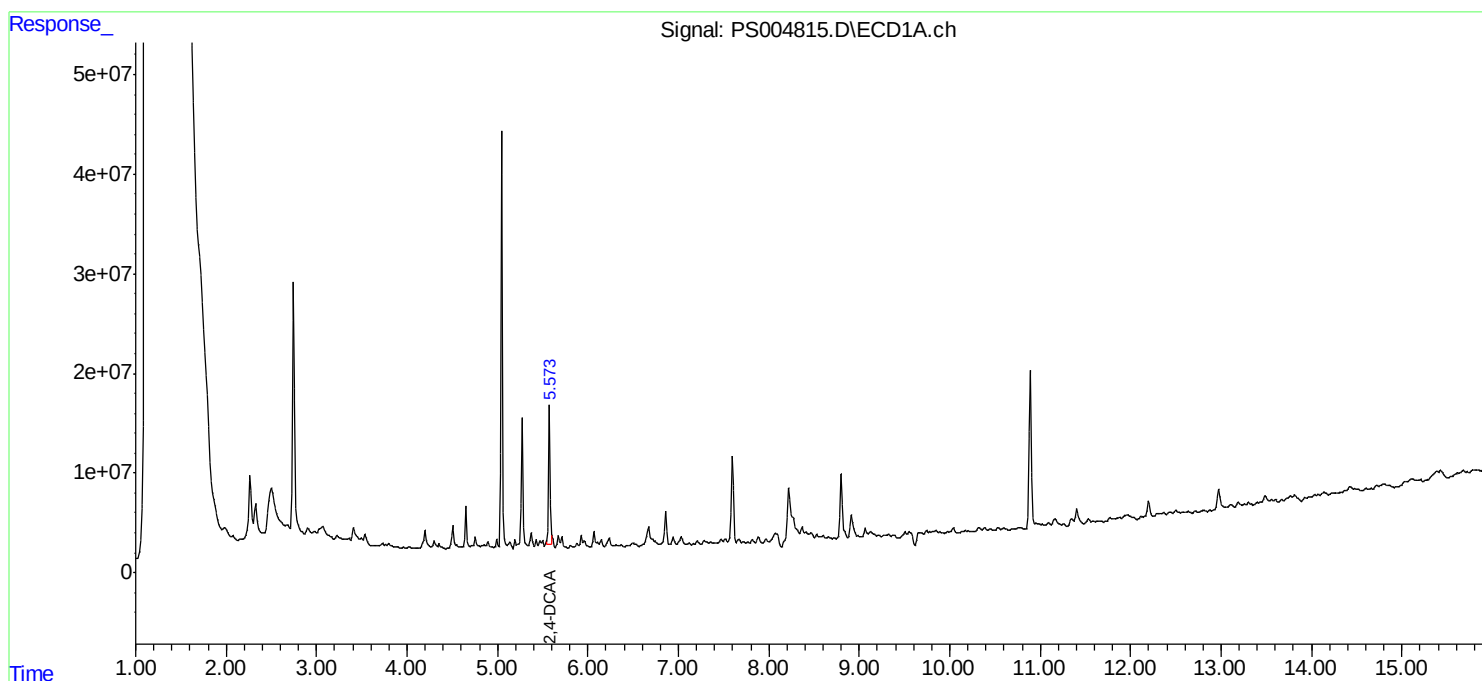

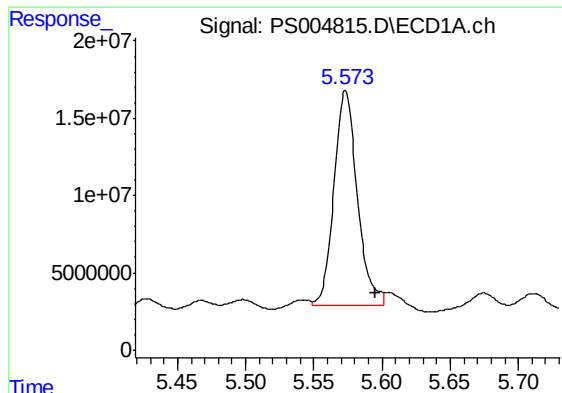


#4 2,4-DCAA

R.T.: 5.573 min
Delta R.T.: -0.022 min
Response: 166309375
Conc: 118.64 ng/ml m

Instrument :
ECD_S
ClientSampleId :
FK-SF-03-007-B

Manual Integrations
APPROVED

Ankita
5/29/2019 2:17:18 PM

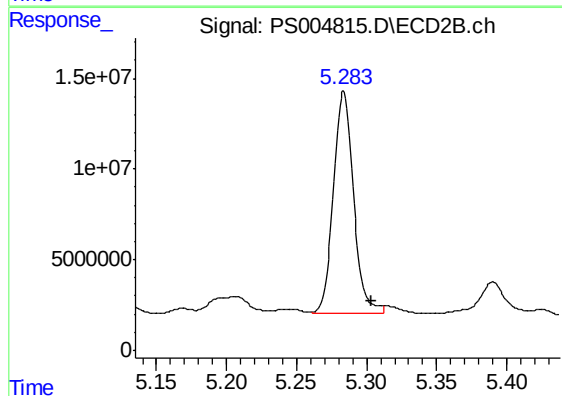

#4 2,4-DCAA

R.T.: 5.283 min
Delta R.T.: -0.020 min
Response: 123602274
Conc: 128.11 ng/ml m