

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052919\
 Data File : PS004820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2019 07:59
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 12:17:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.589	5.300	509.9E6	361.1E6	363.793	374.270
Target Compounds							
12) T	2,4,5-T	0.000	7.406	0	39411367	N.D.	8.843
15) T	Picloram	9.156	9.113	286.9E6	166.3E6	27.531	22.289
16) T	DCPA	0.000	9.113	0	166.3E6	N.D.	25.669



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052919\
Data File : PS004820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2019 07:59
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 12:17:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

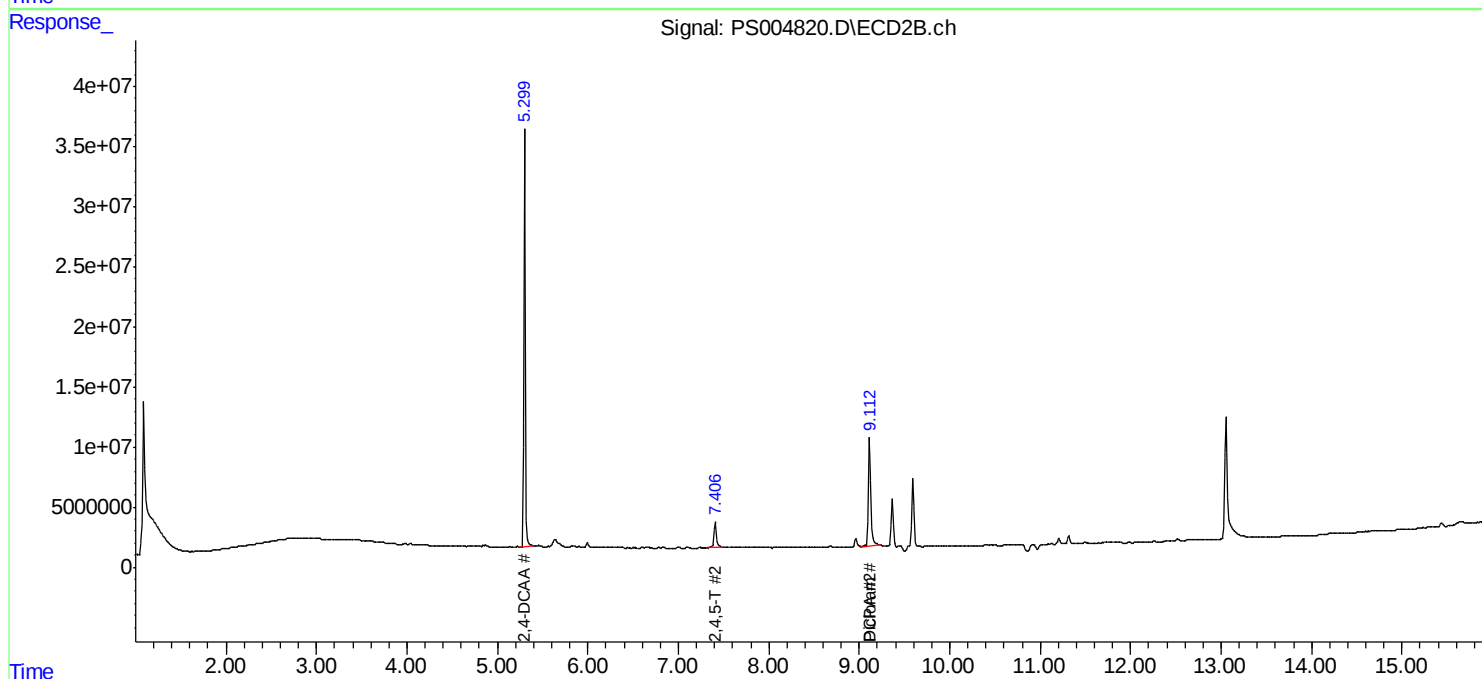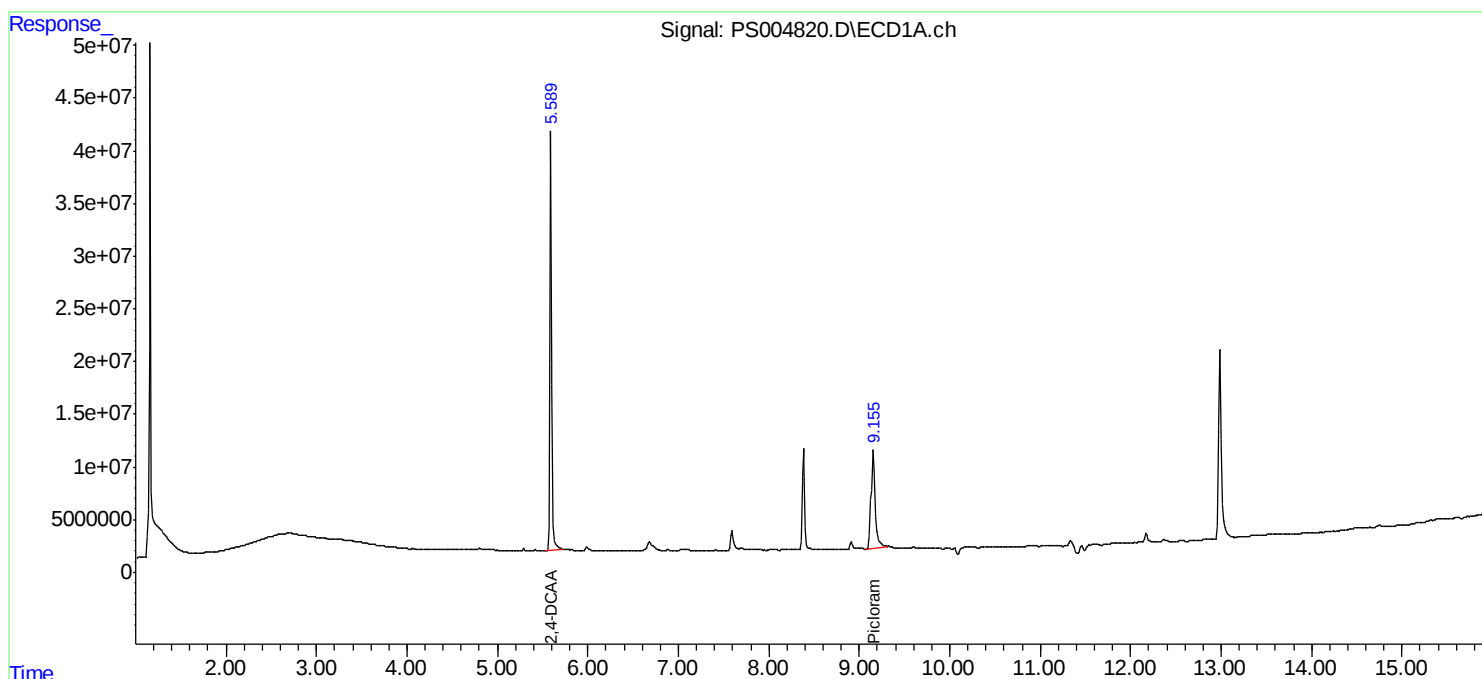


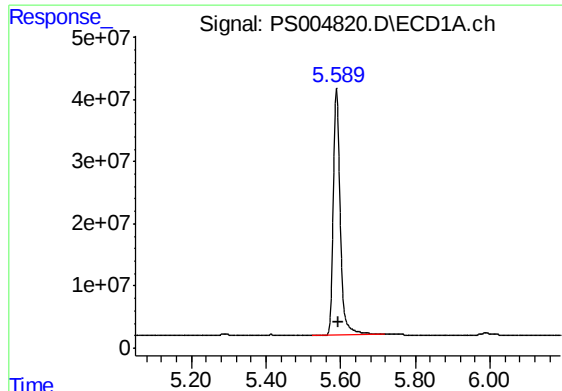

#4 2,4-DCAA


R.T.: 5.589 min
Delta R.T.: -0.006 min
Response: 509949196
Conc: 363.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

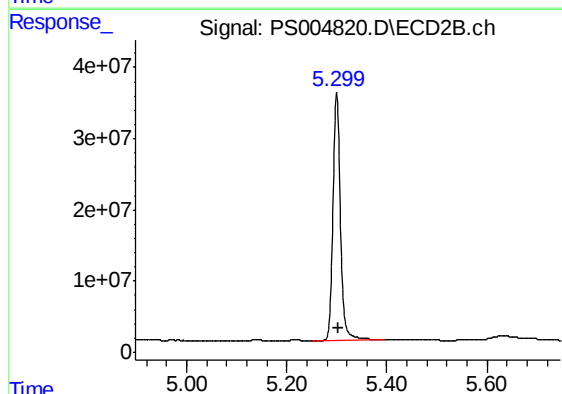


#4 2,4-DCAA

R.T.: 5.300 min
Delta R.T.: -0.004 min
Response: 361109283
Conc: 374.27 ng/ml

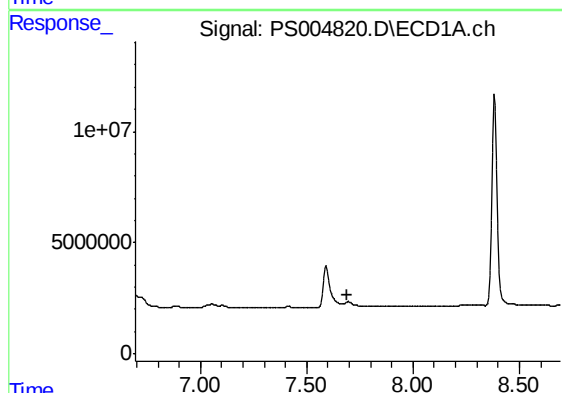


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.693 min
Response: 0
Conc: N.D.

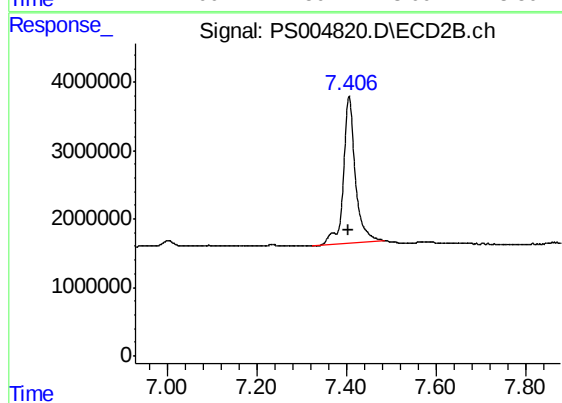

#12 2,4,5-T


R.T.: 7.406 min
Delta R.T.: 0.002 min
Response: 39411367
Conc: 8.84 ng/ml

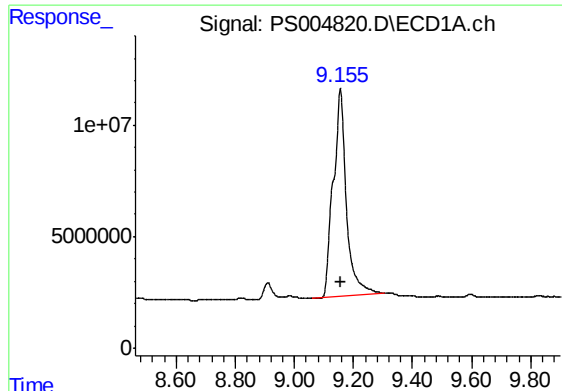

#15 Picloram


R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 286873403
Conc: 27.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

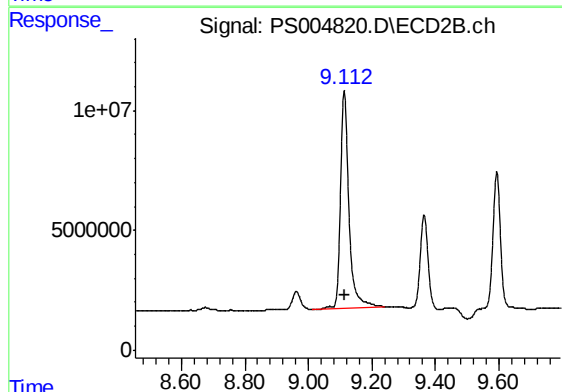


#15 Picloram

R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 166286959
Conc: 22.29 ng/ml

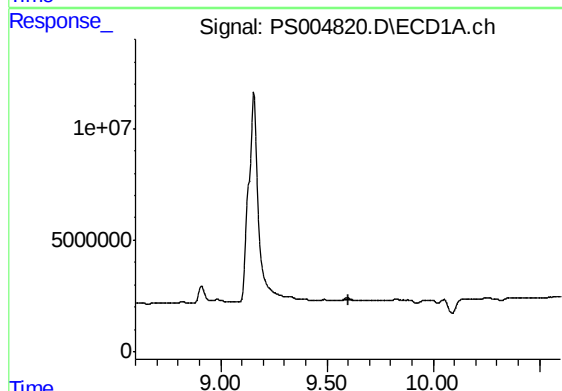

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.599 min
Response: 0
Conc: N.D.

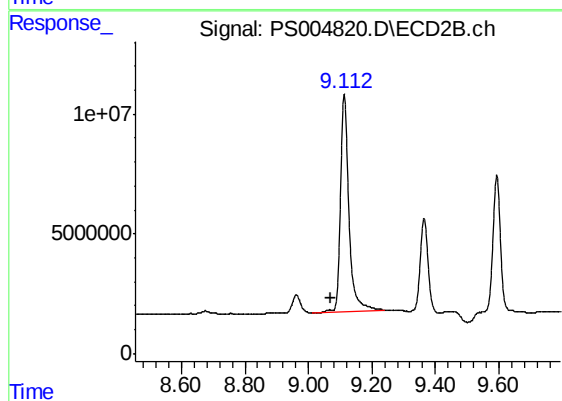

#16 DCPA

R.T.: 9.113 min
Delta R.T.: 0.041 min
Response: 166286959
Conc: 25.67 ng/ml