

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052919\
 Data File : PS004824.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2019 10:22
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 12:18:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.578	5.285	502.3E6	369.1E6	358.365	382.576
Target Compounds							
9) T	2,4-D	6.647	0.000	103.3E6	0	75.542	N.D. #
12) T	2,4,5-T	0.000	7.390	0	77792101	N.D.	17.455
15) T	Picloram	9.142	9.098	285.0E6	166.9E6	27.349	22.372
16) T	DCPA	0.000	9.098	0	166.9E6	N.D.	25.765



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052919\
Data File : PS004824.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2019 10:22
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 12:18:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

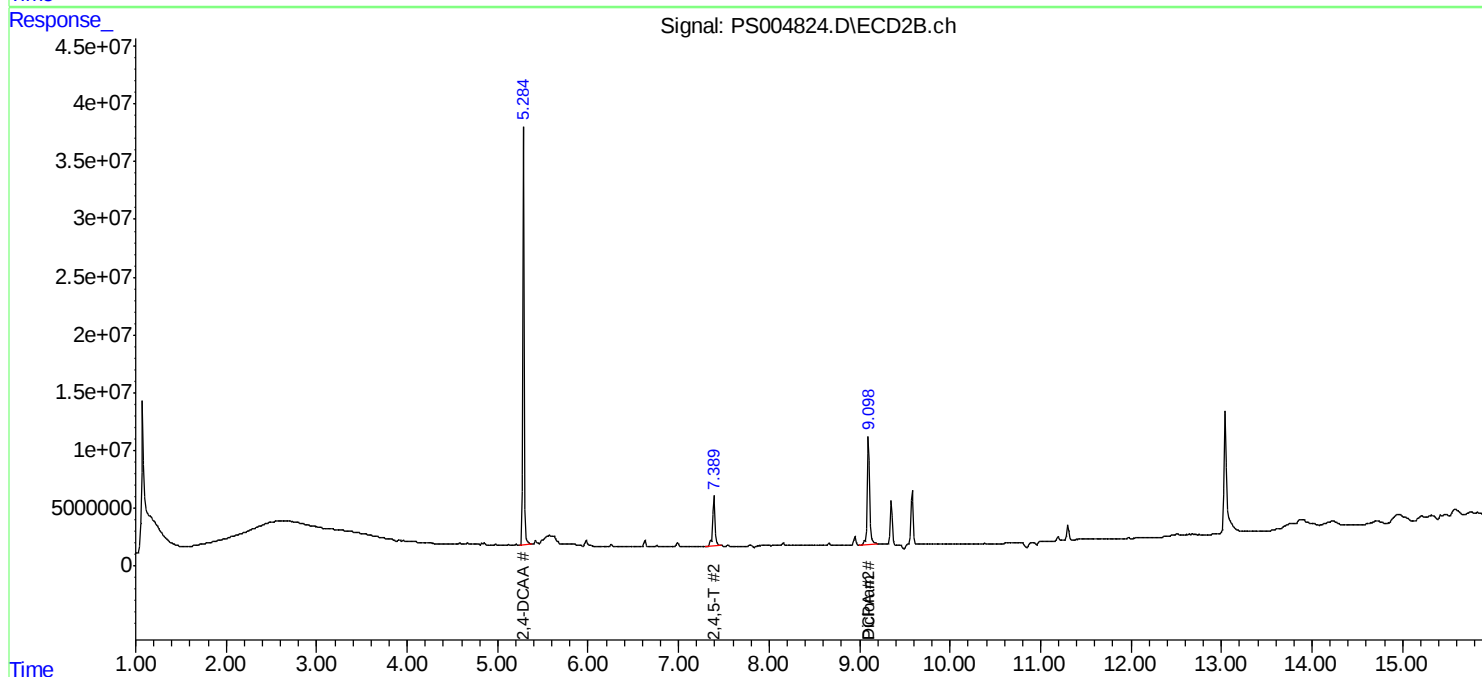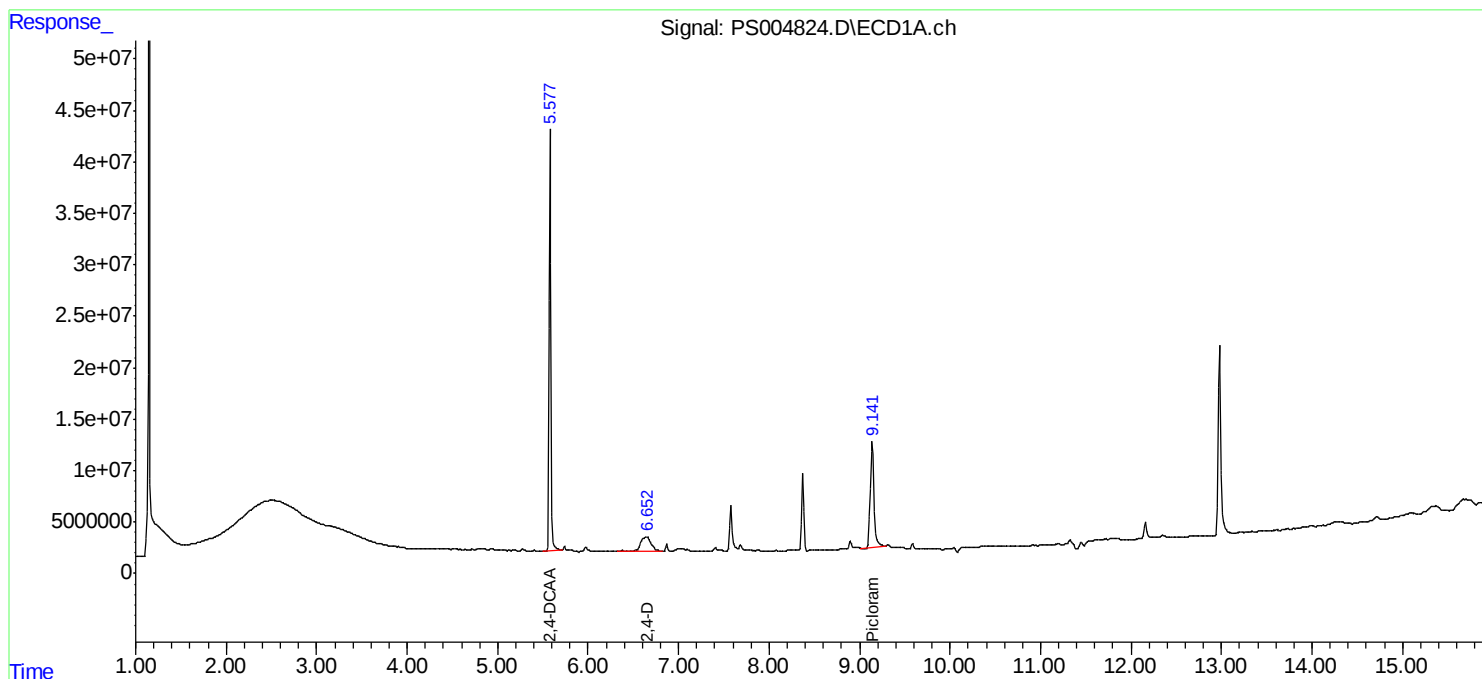


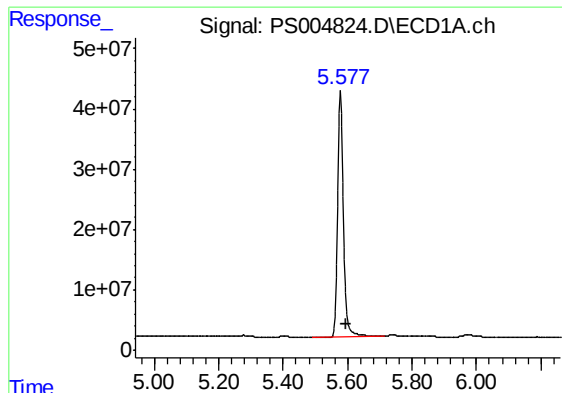

#4 2,4-DCAA


R.T.: 5.578 min
Delta R.T.: -0.017 min
Response: 502340355
Conc: 358.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

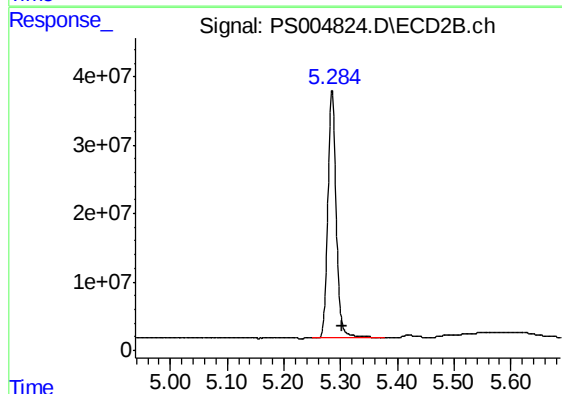


#4 2,4-DCAA

R.T.: 5.285 min
Delta R.T.: -0.019 min
Response: 369123324
Conc: 382.58 ng/ml

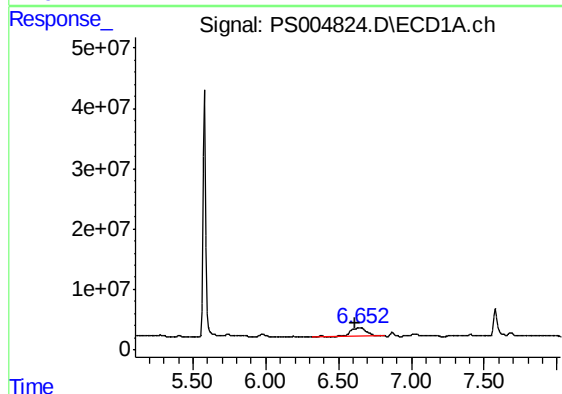


#9 2,4-D

R.T.: 6.647 min
Delta R.T.: 0.036 min
Response: 103334039
Conc: 75.54 ng/ml

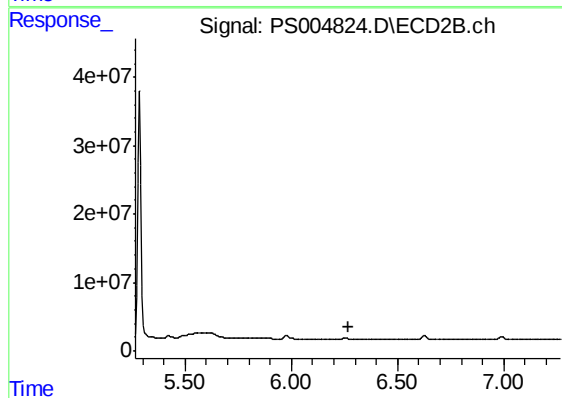

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

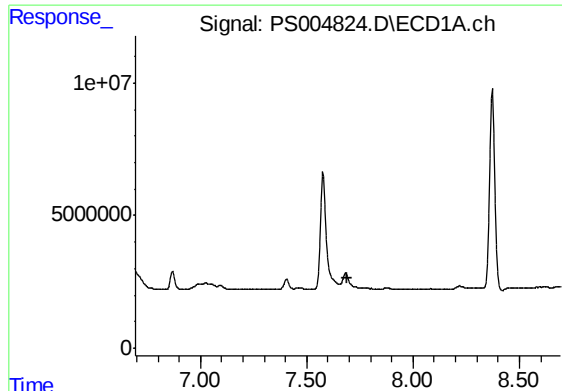

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.693 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

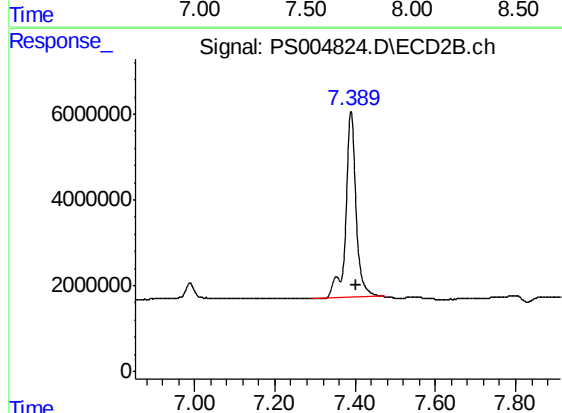


#12 2,4,5-T

R.T.: 7.390 min
Delta R.T.: -0.014 min
Response: 77792101
Conc: 17.45 ng/ml

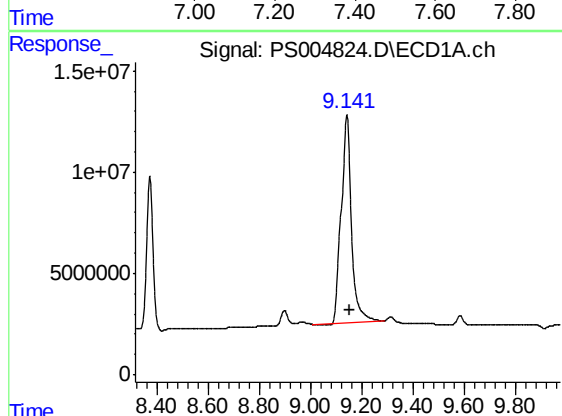


#15 Picloram

R.T.: 9.142 min
Delta R.T.: -0.014 min
Response: 284975548
Conc: 27.35 ng/ml

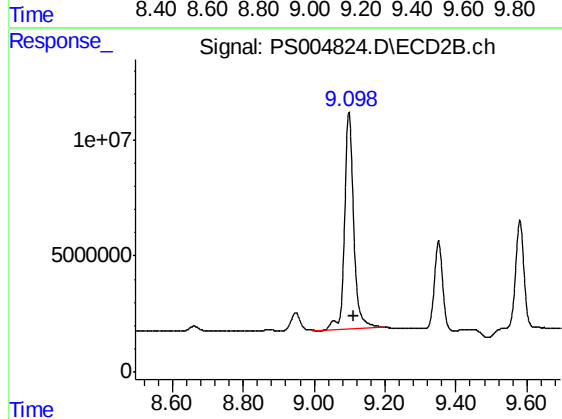

#15 Picloram


R.T.: 9.098 min
Delta R.T.: -0.014 min
Response: 166908817
Conc: 22.37 ng/ml

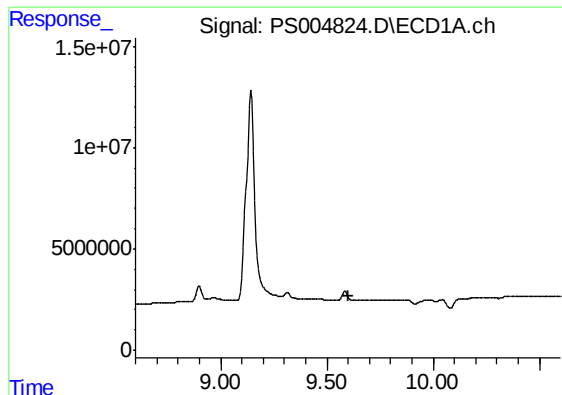

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

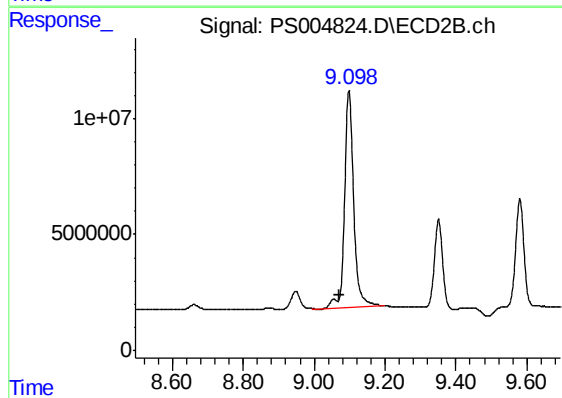

#16 DCPA

R.T.: 9.098 min
Delta R.T.: 0.026 min
Response: 166908817
Conc: 25.77 ng/ml