

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053019\
 Data File : PS004836.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2019 17:49
 Operator : SM\AJ
 Sample : K3075-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 02:18:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.613	5.323	489.4E6	309.8E6	349.098	321.130
Target Compounds							
2) T	3,5-DICHL...	0.000	4.583	0	8155797	N.D.	6.619
3) T	4-Nitroph...	5.415	0.000	40352053	0	64.718	N.D. #
5) T	DICAMBA	5.715	5.429	15306901	13113658	2.883	3.550
6) T	MCP	5.967	0.000	10371495	0	2.491	N.D. #
7) T	MCPA	6.108	5.716	23633739	23574982	4.080	5.762 #
10) T	Pentachlo...	0.000	6.592	0	30627947	N.D.	2.493
11) T	2,4,5-TP ...	0.000	6.979	0	102.6E6	N.D.	19.945
12) T	2,4,5-T	7.639	0.000	168.3E6	0	22.596	N.D. #
13) T	2,4-DB	8.266	0.000	88187813	0	91.295	N.D. #
14) T	DINOSEB	0.000	8.188	0	68487226	N.D.	17.816
16) T	DCPA	9.587	0.000	54180171	0	6.083	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053019\
Data File : PS004836.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2019 17:49
Operator : SM\AJ
Sample : K3075-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 02:18:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

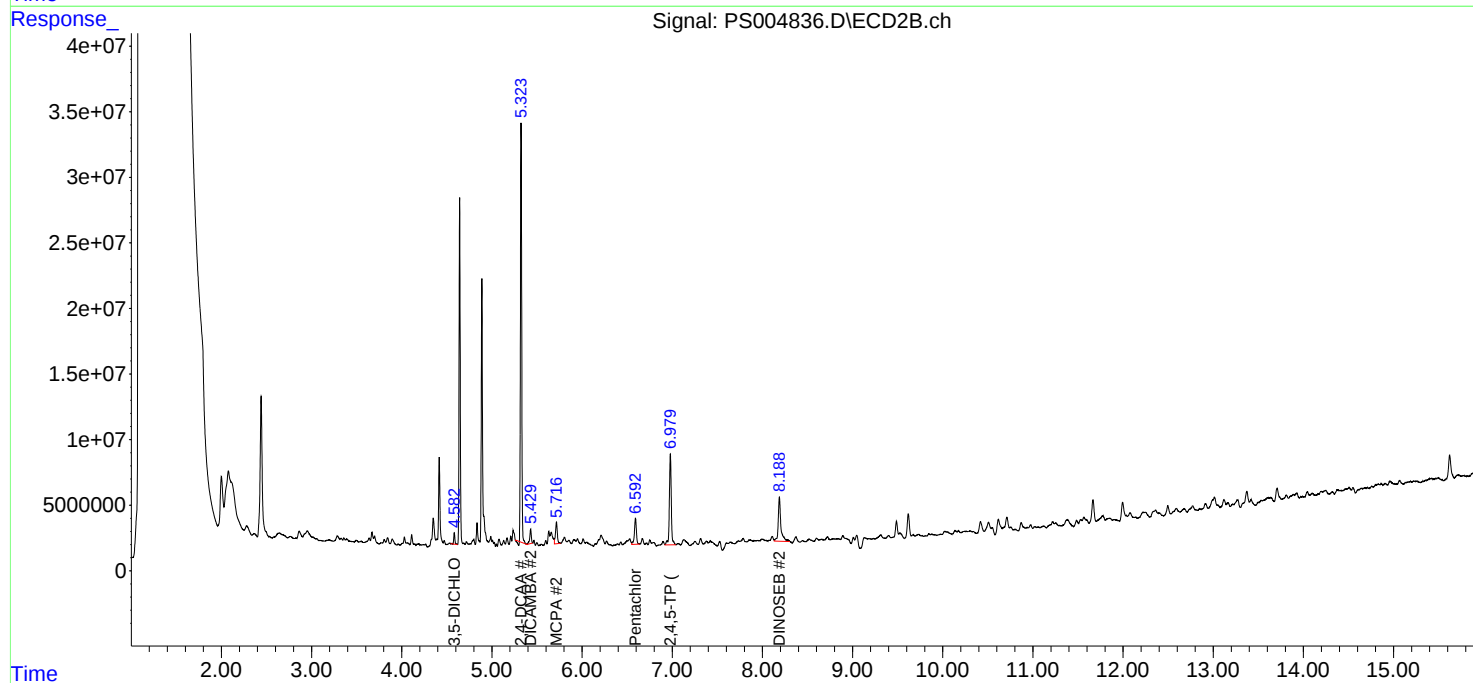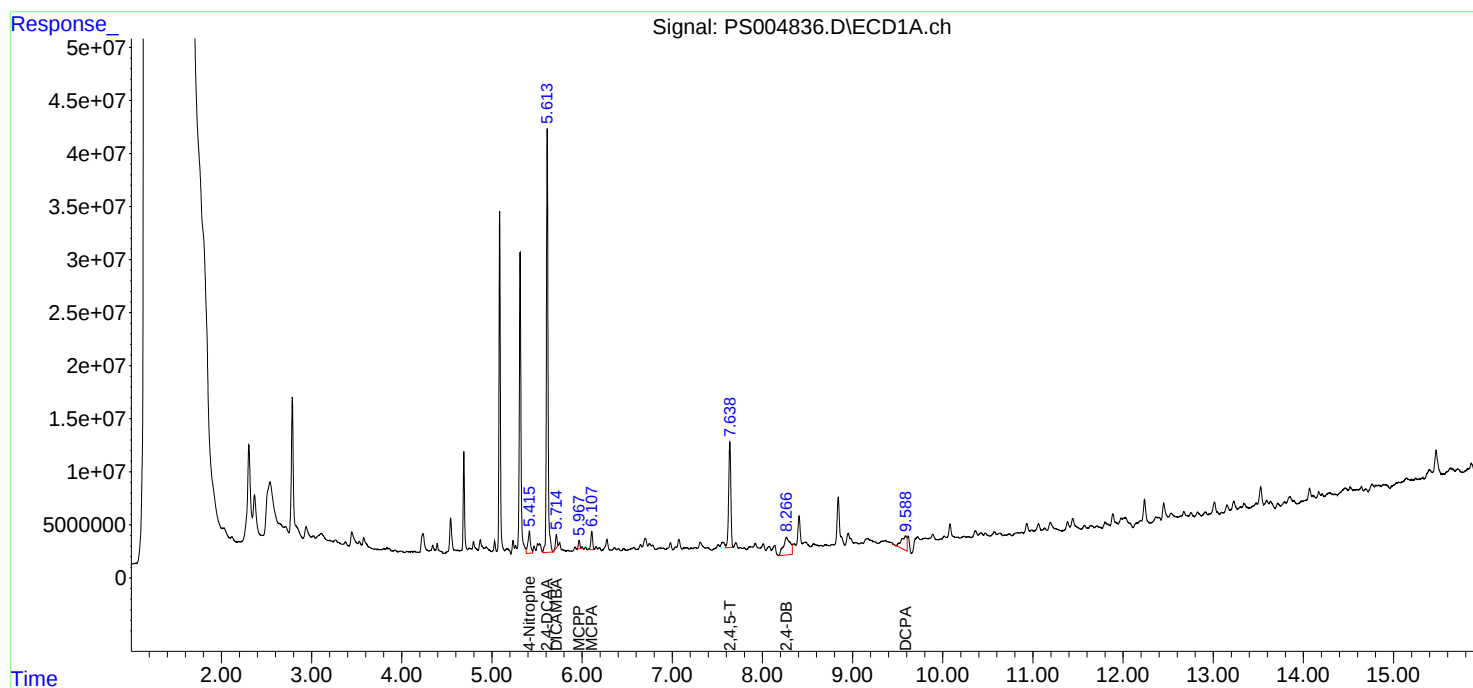


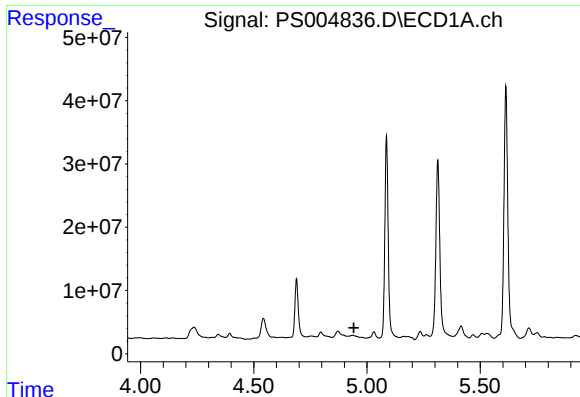

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

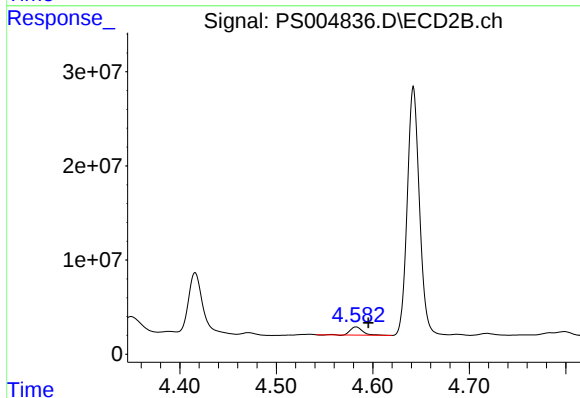


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.583 min
Delta R.T.: -0.013 min
Response: 8155797
Conc: 6.62 ng/ml

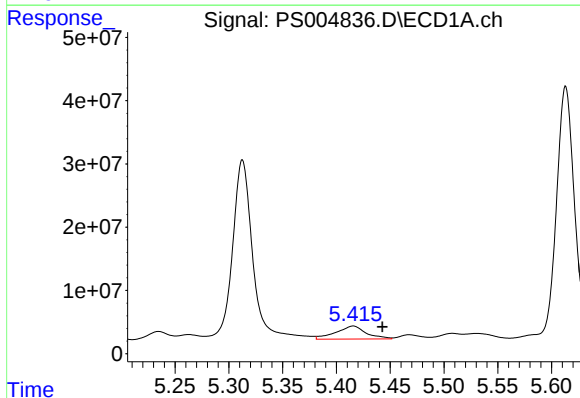


#3 4-Nitrophenol

R.T.: 5.415 min
Delta R.T.: -0.027 min
Response: 40352053
Conc: 64.72 ng/ml

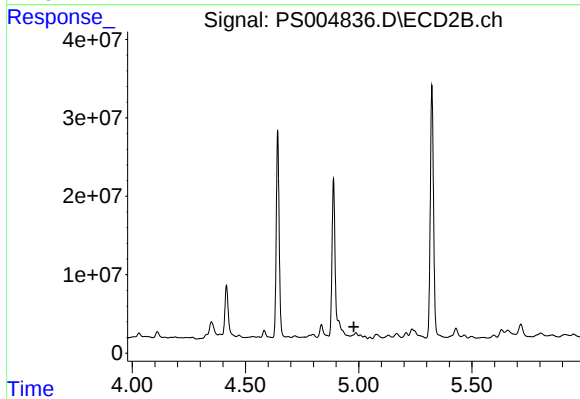

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

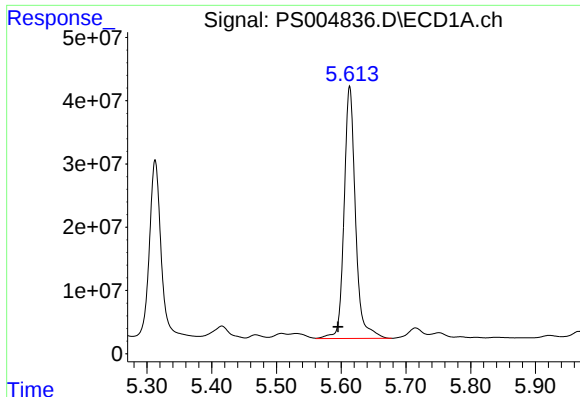

#4 2,4-DCAA


R.T.: 5.613 min
Delta R.T.: 0.018 min
Response: 489350552
Conc: 349.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

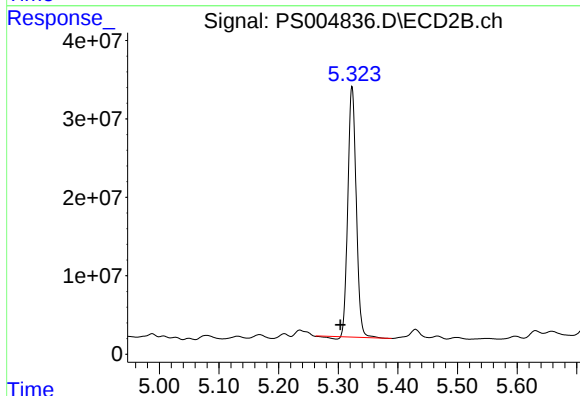


#4 2,4-DCAA

R.T.: 5.323 min
Delta R.T.: 0.020 min
Response: 309838175
Conc: 321.13 ng/ml

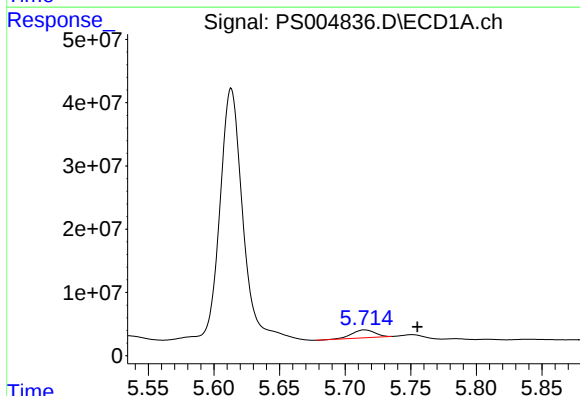


#5 DICAMBA

R.T.: 5.715 min
Delta R.T.: -0.040 min
Response: 15306901
Conc: 2.88 ng/ml

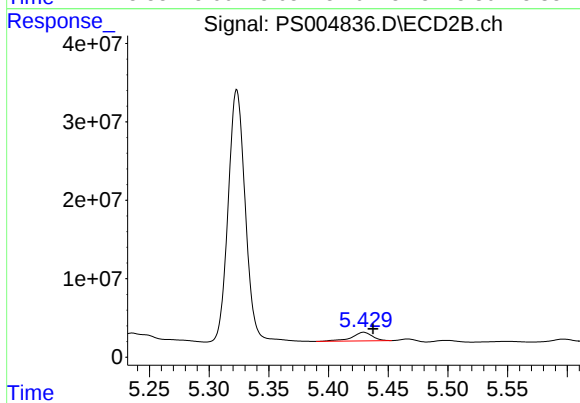

#5 DICAMBA


R.T.: 5.429 min
Delta R.T.: -0.008 min
Response: 13113658
Conc: 3.55 ng/ml

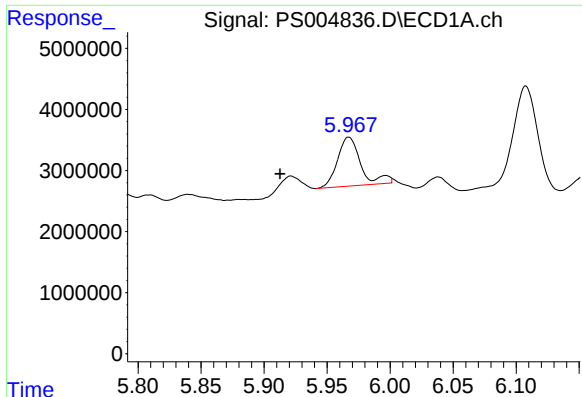

#6 MCPP


R.T.: 5.967 min
Delta R.T.: 0.055 min
Response: 10371495
Conc: 2.49 ug/ml

Instrument :
ECD_S
ClientSampleId :

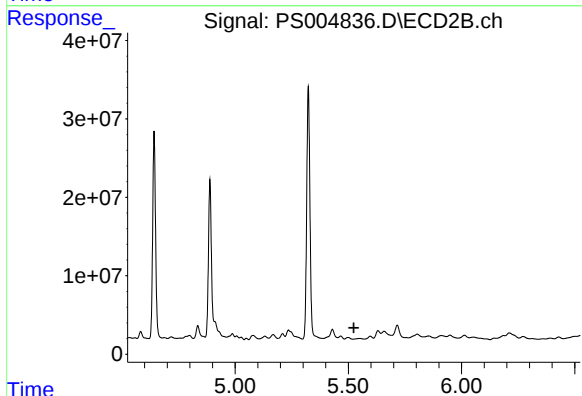


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

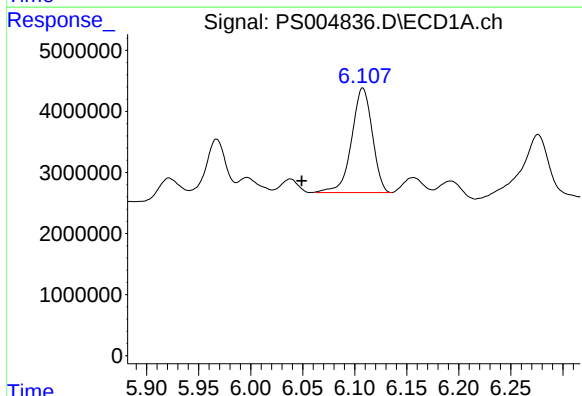


#7 MCPA

R.T.: 6.108 min
Delta R.T.: 0.059 min
Response: 23633739
Conc: 4.08 ug/ml

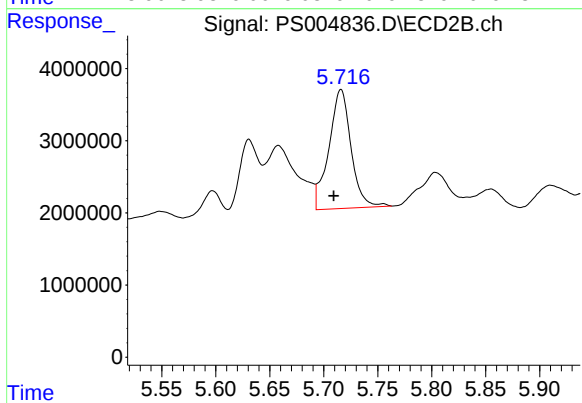

#7 MCPA


R.T.: 5.716 min
Delta R.T.: 0.007 min
Response: 23574982
Conc: 5.76 ug/ml

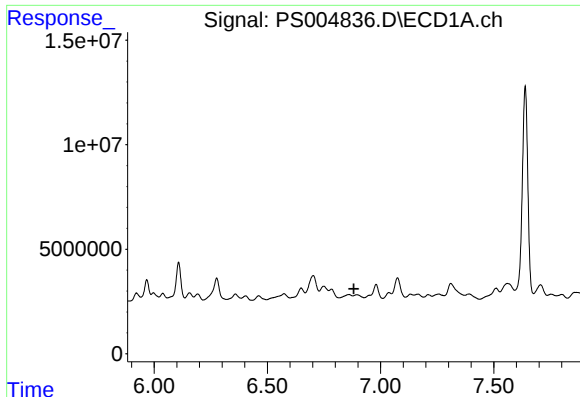

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.882 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

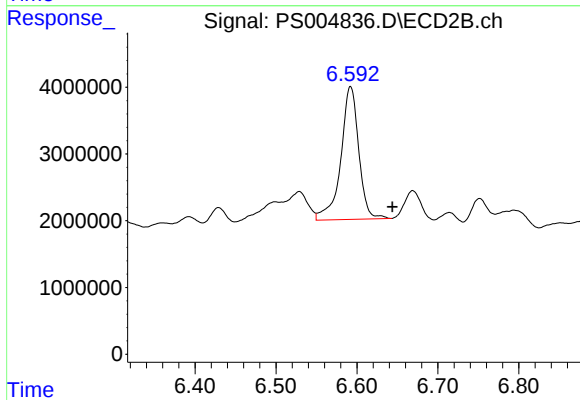


#10 Pentachlorophenol

R.T.: 6.592 min
Delta R.T.: -0.052 min
Response: 30627947
Conc: 2.49 ng/ml

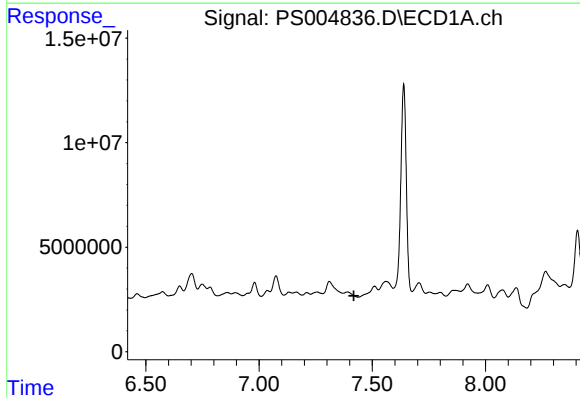


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

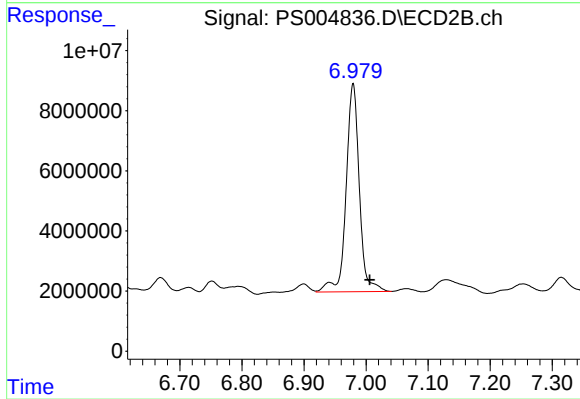

#11 2,4,5-TP (SILVEX)


R.T.: 6.979 min
Delta R.T.: -0.027 min
Response: 102623575
Conc: 19.95 ng/ml

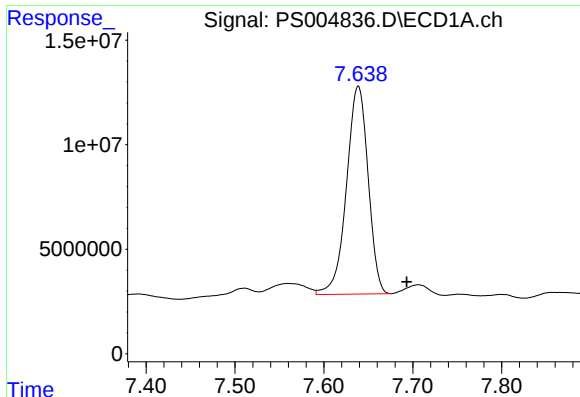

#12 2,4,5-T


R.T.: 7.639 min
Delta R.T.: -0.055 min
Response: 168282716
Conc: 22.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

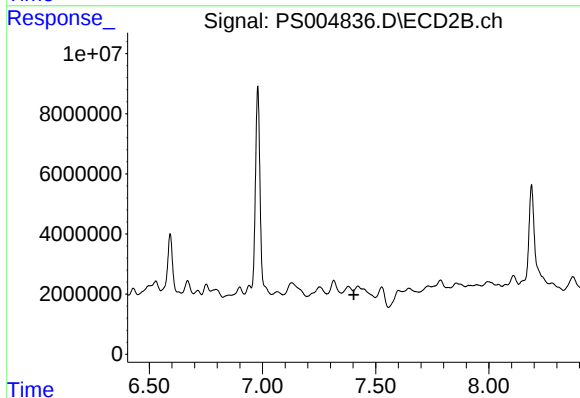


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.404 min
Response: 0
Conc: N.D.

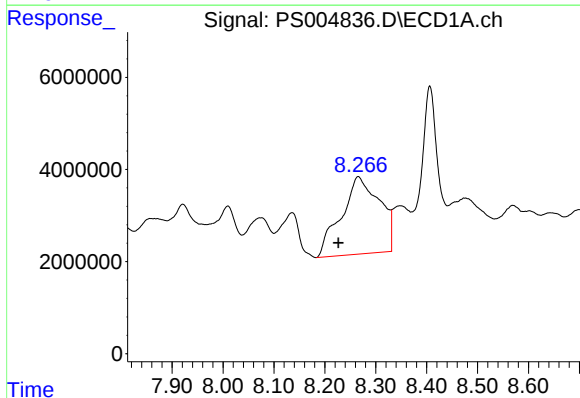


#13 2,4-DB

R.T.: 8.266 min
Delta R.T.: 0.039 min
Response: 88187813
Conc: 91.30 ng/ml

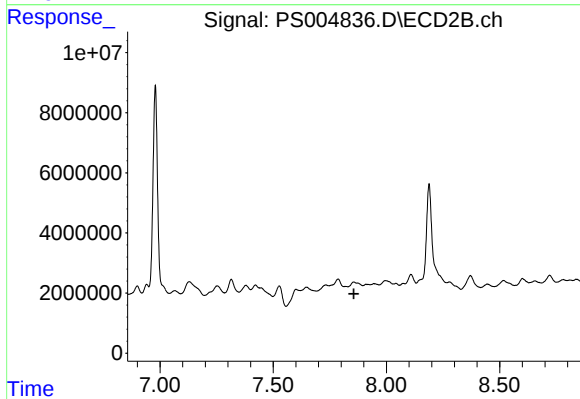

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.856 min
Response: 0
Conc: N.D.

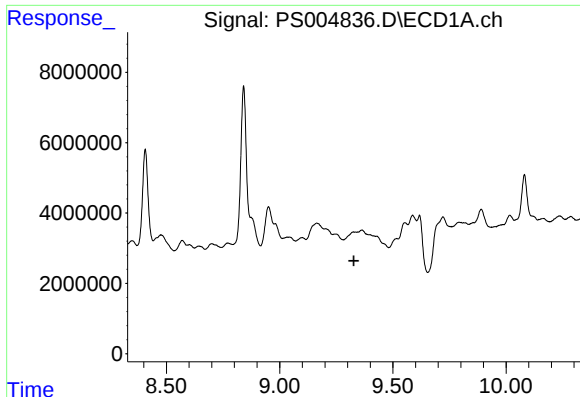

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

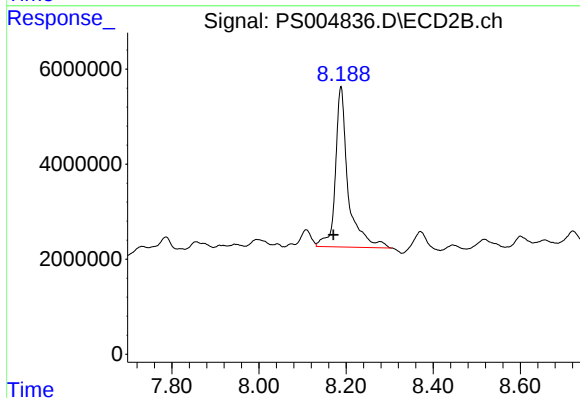


#14 DINOSEB

R.T.: 8.188 min
Delta R.T.: 0.017 min
Response: 68487226
Conc: 17.82 ng/ml

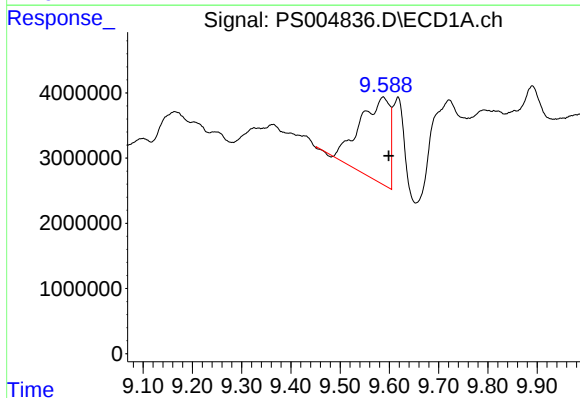

#16 DCPA

R.T.: 9.587 min
Delta R.T.: -0.012 min
Response: 54180171
Conc: 6.08 ng/ml

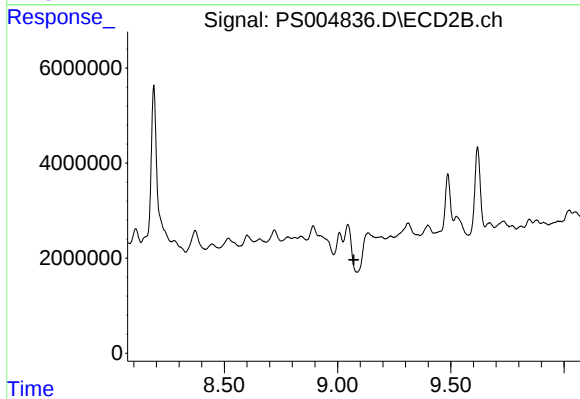

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.072 min
Response: 0
Conc: N.D.